

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100524\
 Data File : PL092225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 17:49
 Operator : AR\AJ
 Sample : P4258-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 Chamberlain Ave

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 02:54:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.781	39305469	45781255	17.668	18.254
28)	SA Decachlor...	9.058	7.921	15933357	23482824	9.726	9.386
Target Compounds							
2)	A alpha-BHC	0.000	3.282	0	1205063	N.D.	0.331 #
4)	MA Heptachlor	0.000	3.948	0	2069057	N.D.	0.600 #
5)	MB Aldrin	0.000	4.239	0	376329	N.D.	0.111 #
6)	B beta-BHC	0.000	3.915	0	440152	N.D.	0.293 #
7)	B delta-BHC	4.770	4.142	12149830	895184	4.213	0.258 #
8)	B Heptachlo...	0.000	4.736	0	406146	N.D.	0.134 #
15)	B Endosulfa...	0.000	5.936	0	43345	N.D.	0.017 #
17)	MA 4,4'-DDT	0.000	6.048	0	438555	N.D.	0.190 #
22)	Mirex	0.000	7.048f	0	555899	N.D.	0.229 #
27)	Chlordane-5	0.000	5.936	0	43345	N.D.	0.400 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100524\
Data File : PL092225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 17:49
Operator : AR\AJ
Sample : P4258-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
Chamberlain Ave

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 02:54:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

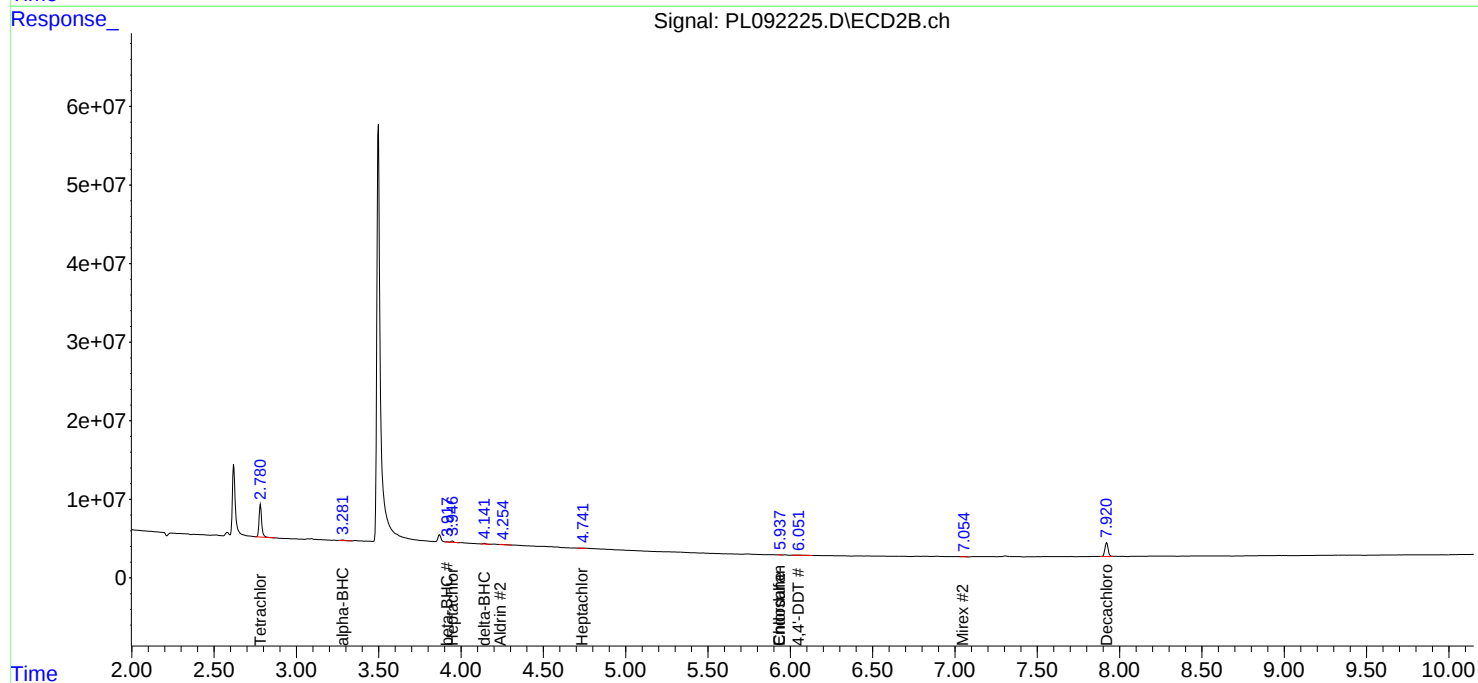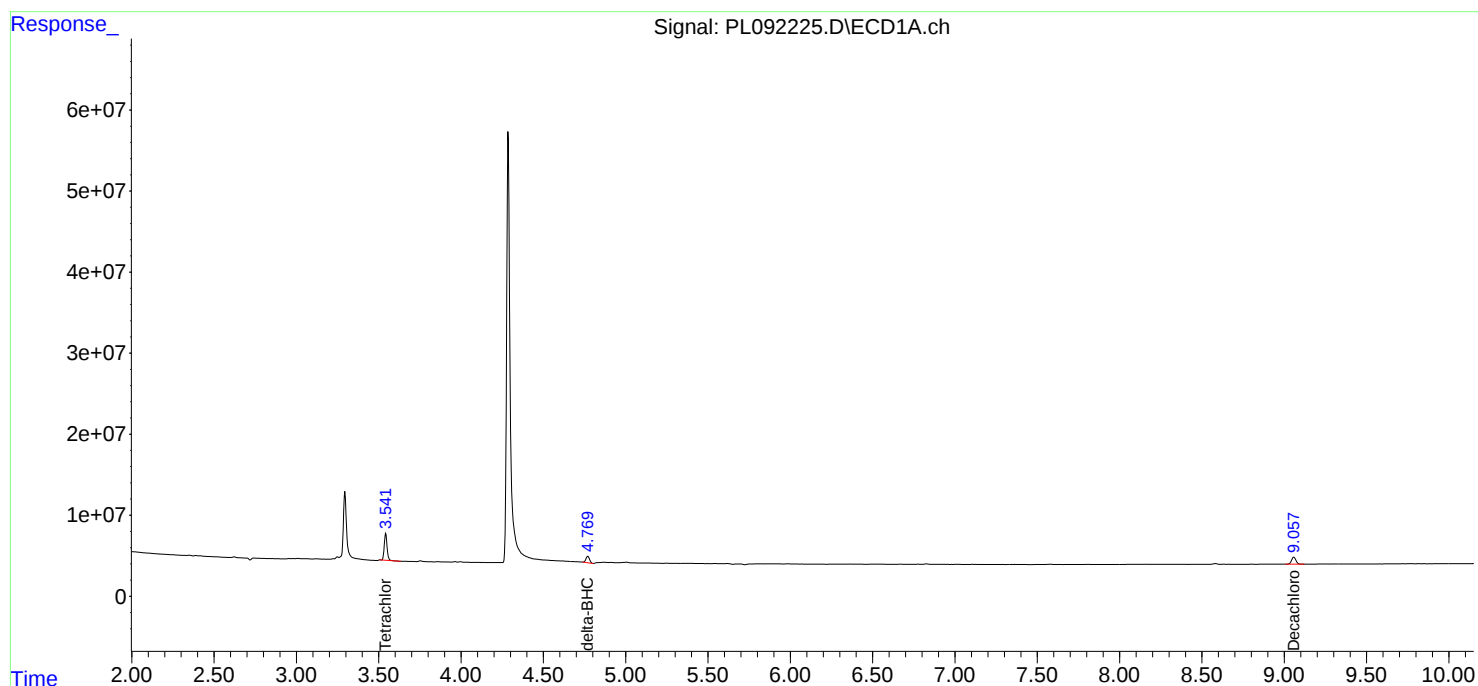


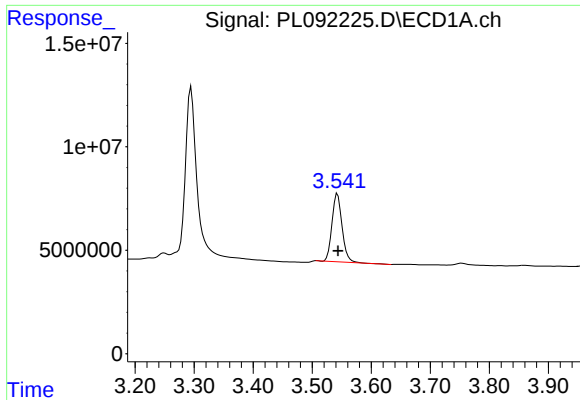

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 39305469
Conc: 17.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
Chamberlain Ave

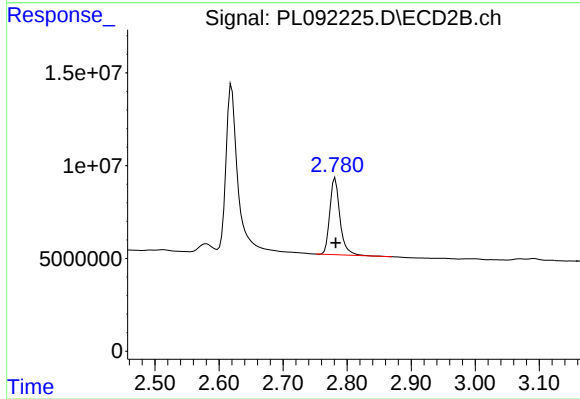


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: 0.000 min
Response: 45781255
Conc: 18.25 ng/ml

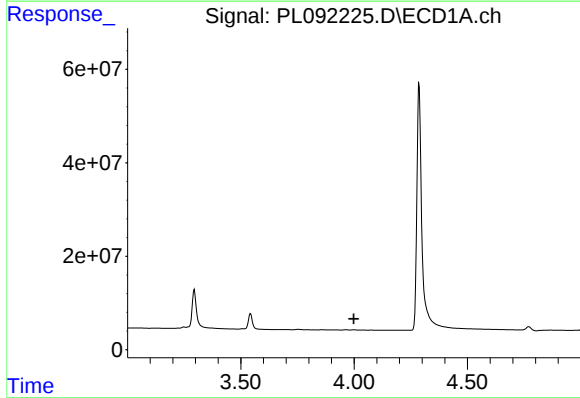


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.999 min
Response: 0
Conc: N.D.

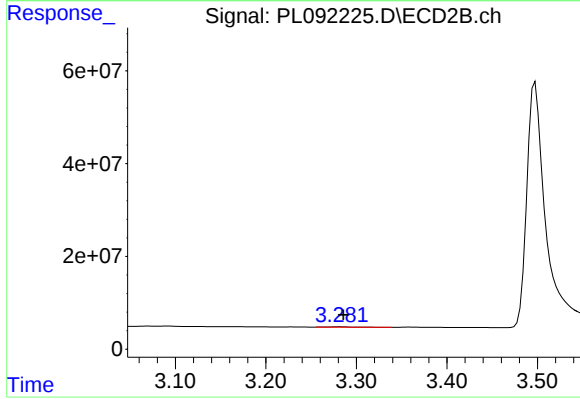

#2 alpha-BHC


R.T.: 3.282 min
Delta R.T.: -0.003 min
Response: 1205063
Conc: 0.33 ng/ml

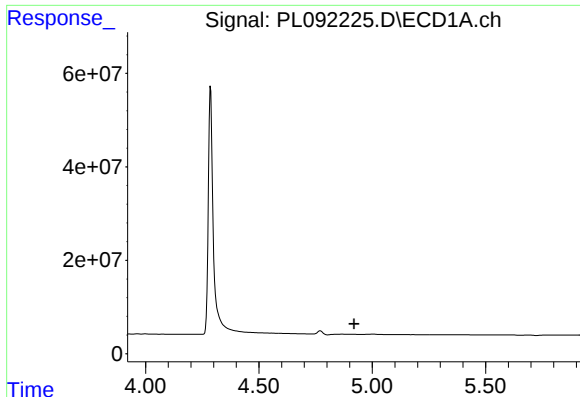

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
Chamberlain Ave

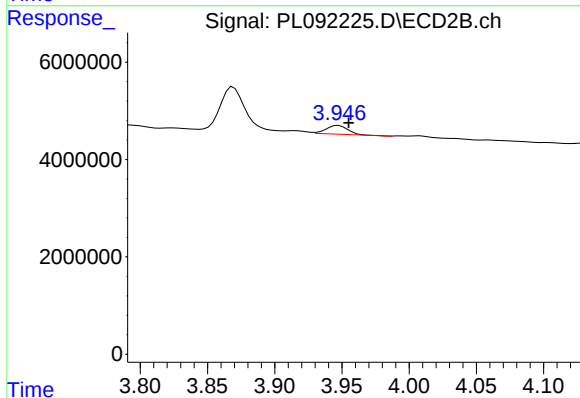


#4 Heptachlor

R.T.: 3.948 min
Delta R.T.: -0.008 min
Response: 2069057
Conc: 0.60 ng/ml

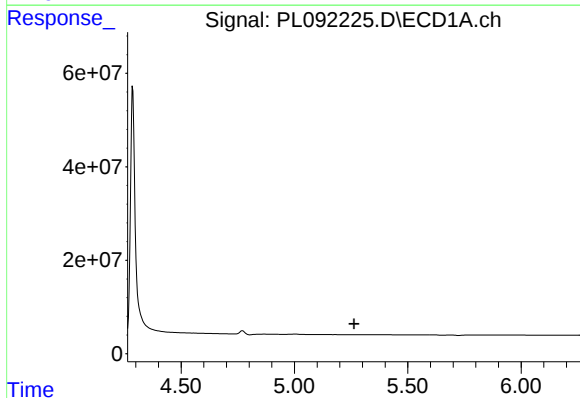


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.263 min
Response: 0
Conc: N.D.

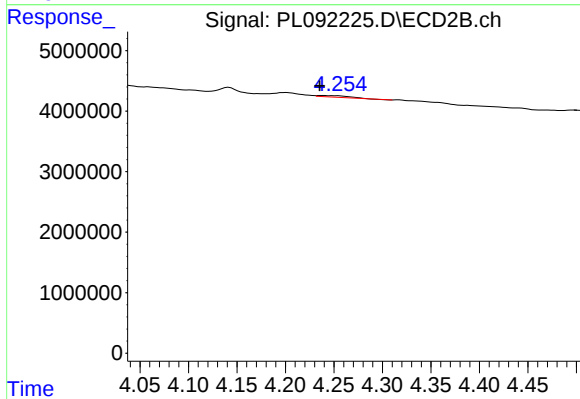

#5 Aldrin


R.T.: 4.239 min
Delta R.T.: 0.004 min
Response: 376329
Conc: 0.11 ng/ml

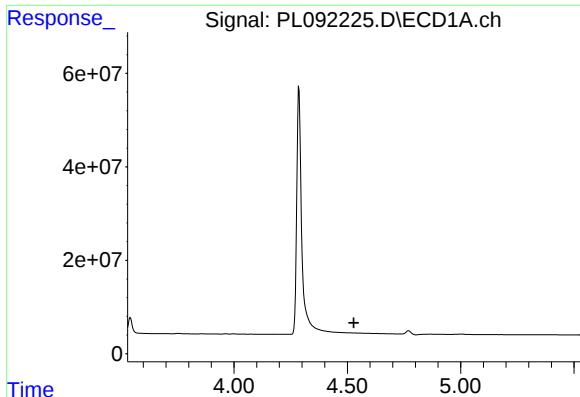

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
Chamberlain Ave

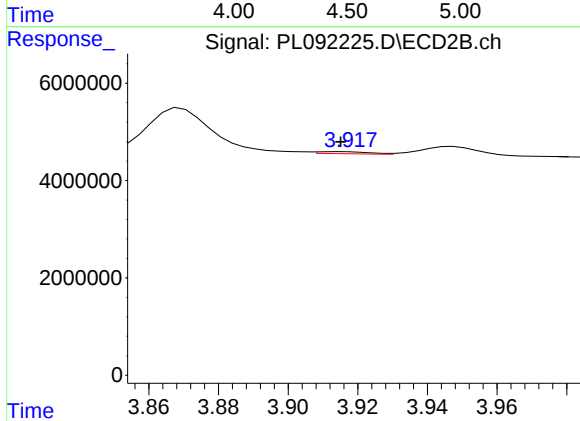


#6 beta-BHC

R.T.: 3.915 min
Delta R.T.: 0.000 min
Response: 440152
Conc: 0.29 ng/ml

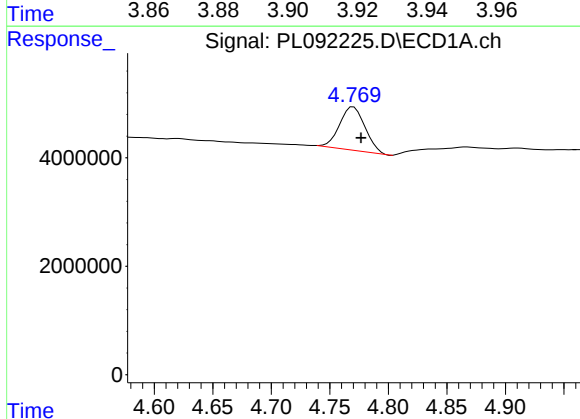


#7 delta-BHC

R.T.: 4.770 min
Delta R.T.: -0.006 min
Response: 12149830
Conc: 4.21 ng/ml

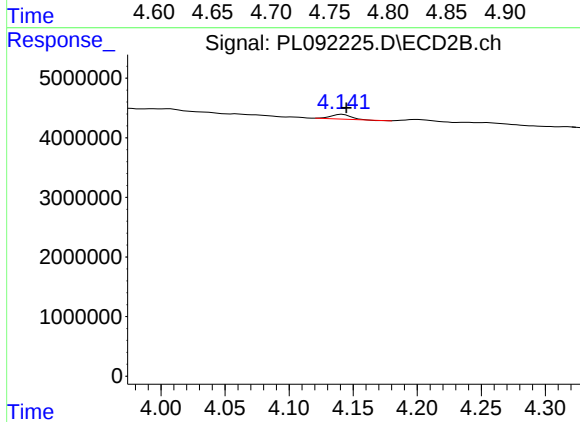

#7 delta-BHC


R.T.: 4.142 min
Delta R.T.: -0.003 min
Response: 895184
Conc: 0.26 ng/ml

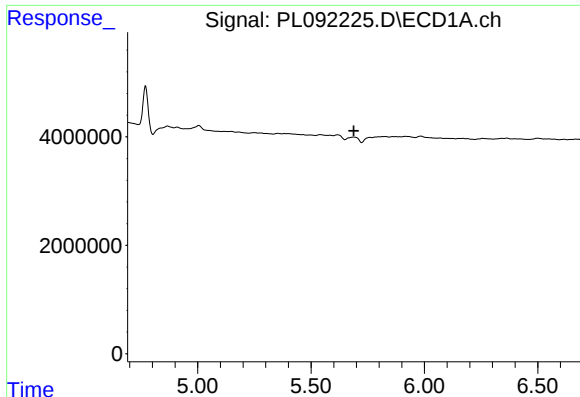

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.689 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
Chamberlain Ave

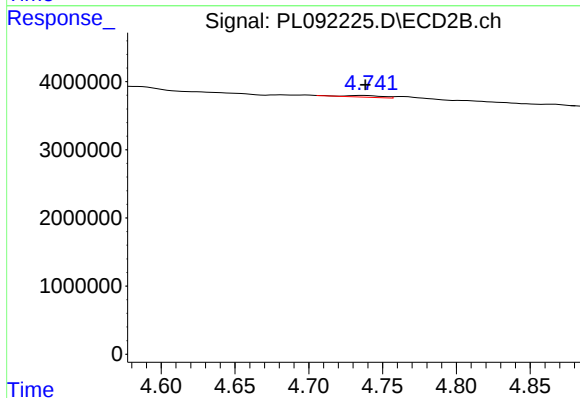


#8 Heptachlor epoxide

R.T.: 4.736 min
Delta R.T.: -0.002 min
Response: 406146
Conc: 0.13 ng/ml

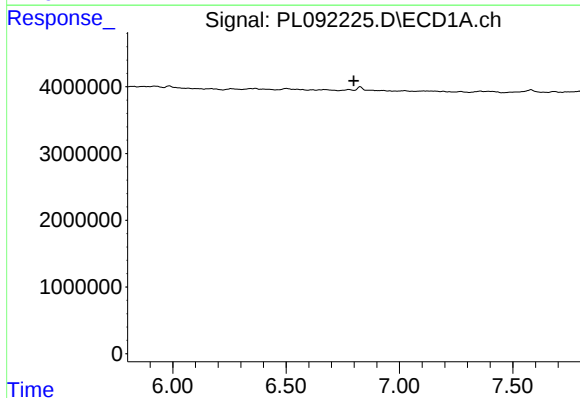


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.798 min
Response: 0
Conc: N.D.

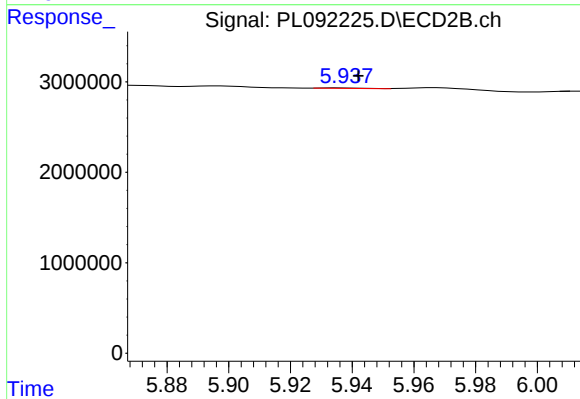

#15 Endosulfan II


R.T.: 5.936 min
Delta R.T.: -0.006 min
Response: 43345
Conc: 0.02 ng/ml

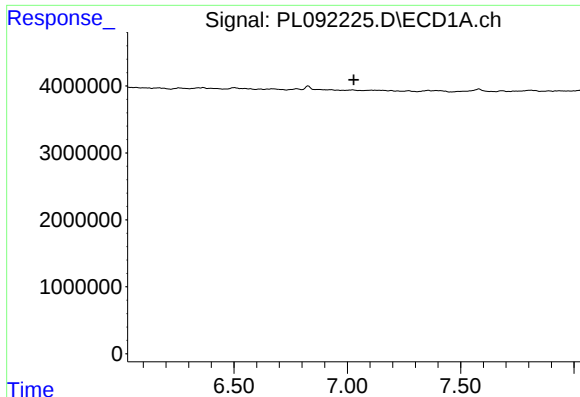

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
Chamberlain Ave

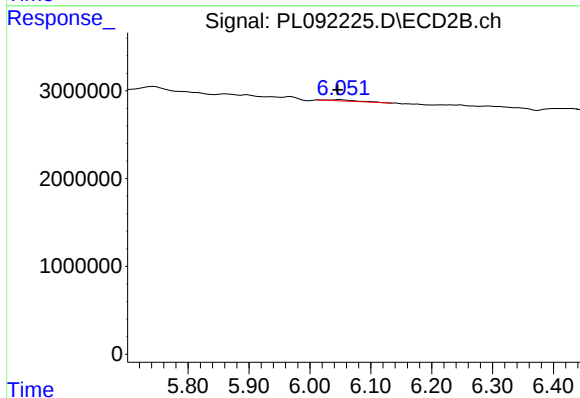


#17 4,4'-DDT

R.T.: 6.048 min
Delta R.T.: 0.003 min
Response: 438555
Conc: 0.19 ng/ml

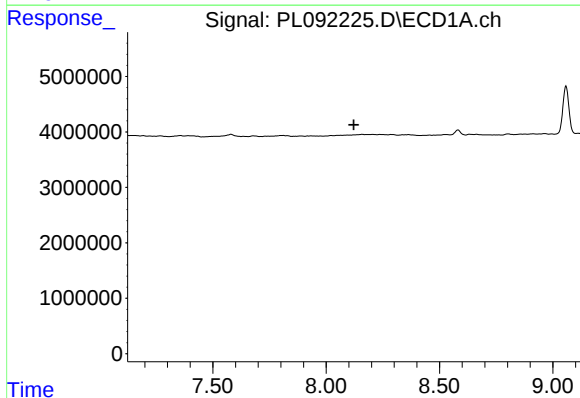


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

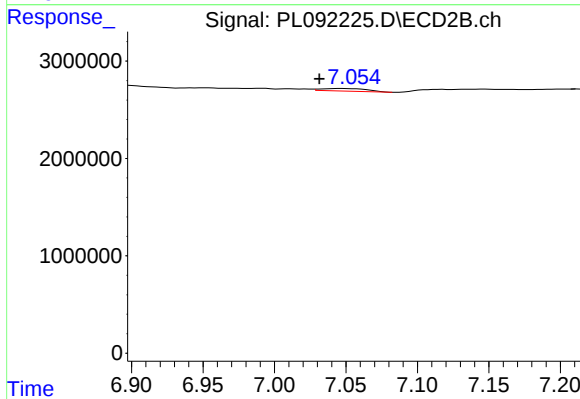

#22 Mirex


R.T.: 7.048 min
Delta R.T.: 0.016 min
Response: 555899
Conc: 0.23 ng/ml

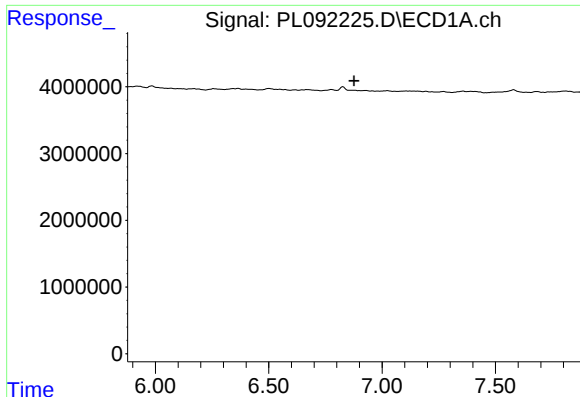

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 6.876 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
Chamberlain Ave

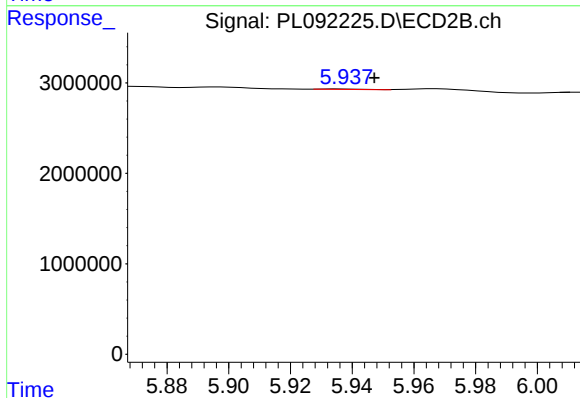


#27 Chlorine-5

R.T.: 5.936 min
Delta R.T.: -0.011 min
Response: 43345
Conc: 0.40 ng/ml

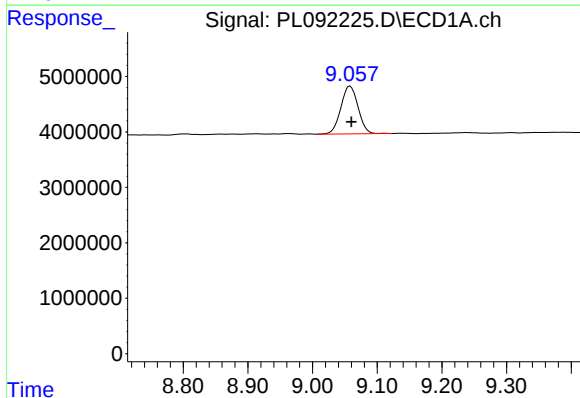

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: -0.002 min
Response: 15933357
Conc: 9.73 ng/ml

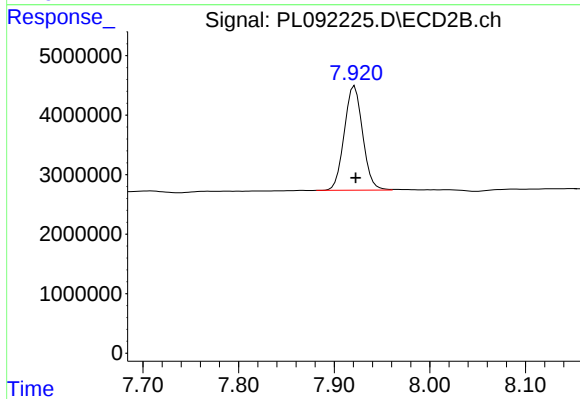

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.001 min
Response: 23482824
Conc: 9.39 ng/ml