

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101124\
 Data File : PP067767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2024 19:13
 Operator : YP\AJ
 Sample : P4385-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SP-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 01:35:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.753	4.050	18928208	20175085	20.449	19.967
2) SA Decachlor...	10.666	9.214	23901574	21628928	20.760	19.286

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101124\
Data File : PP067767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2024 19:13
Operator : YP\AJ
Sample : P4385-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SP-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 01:35:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

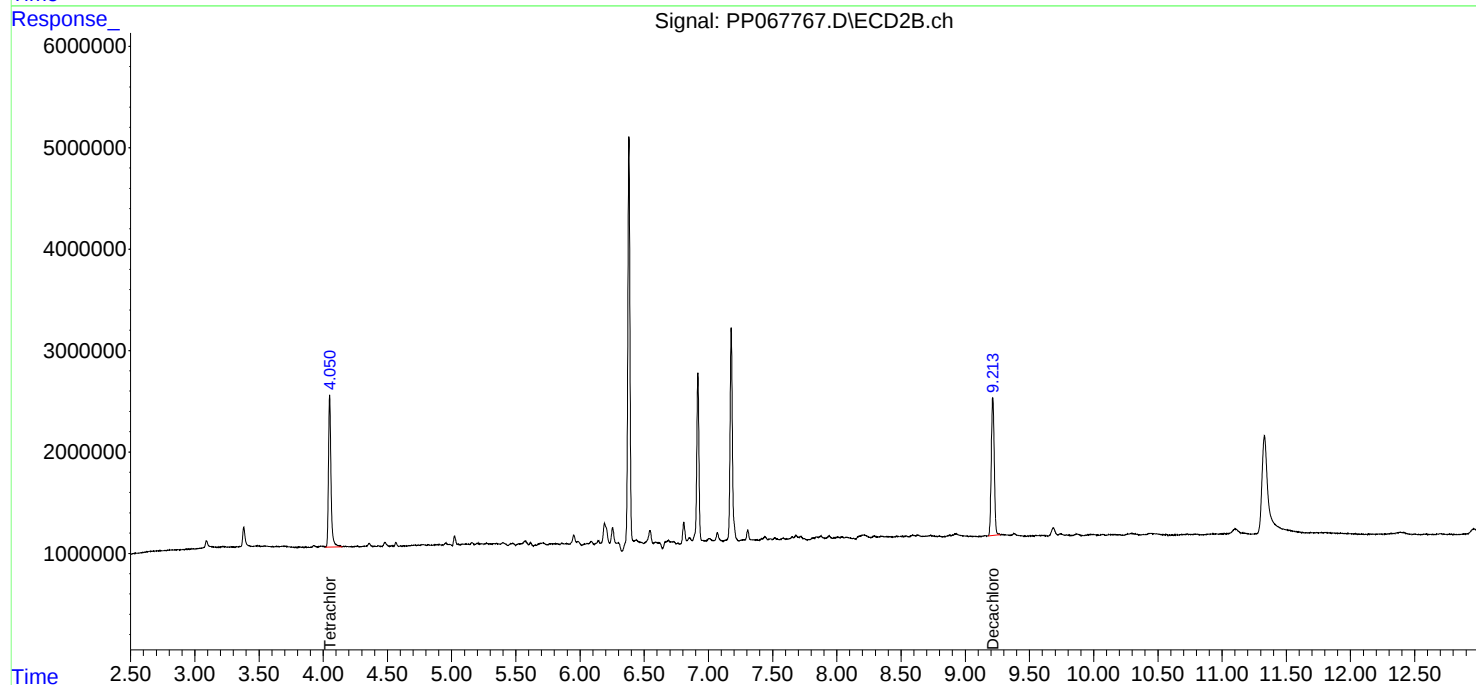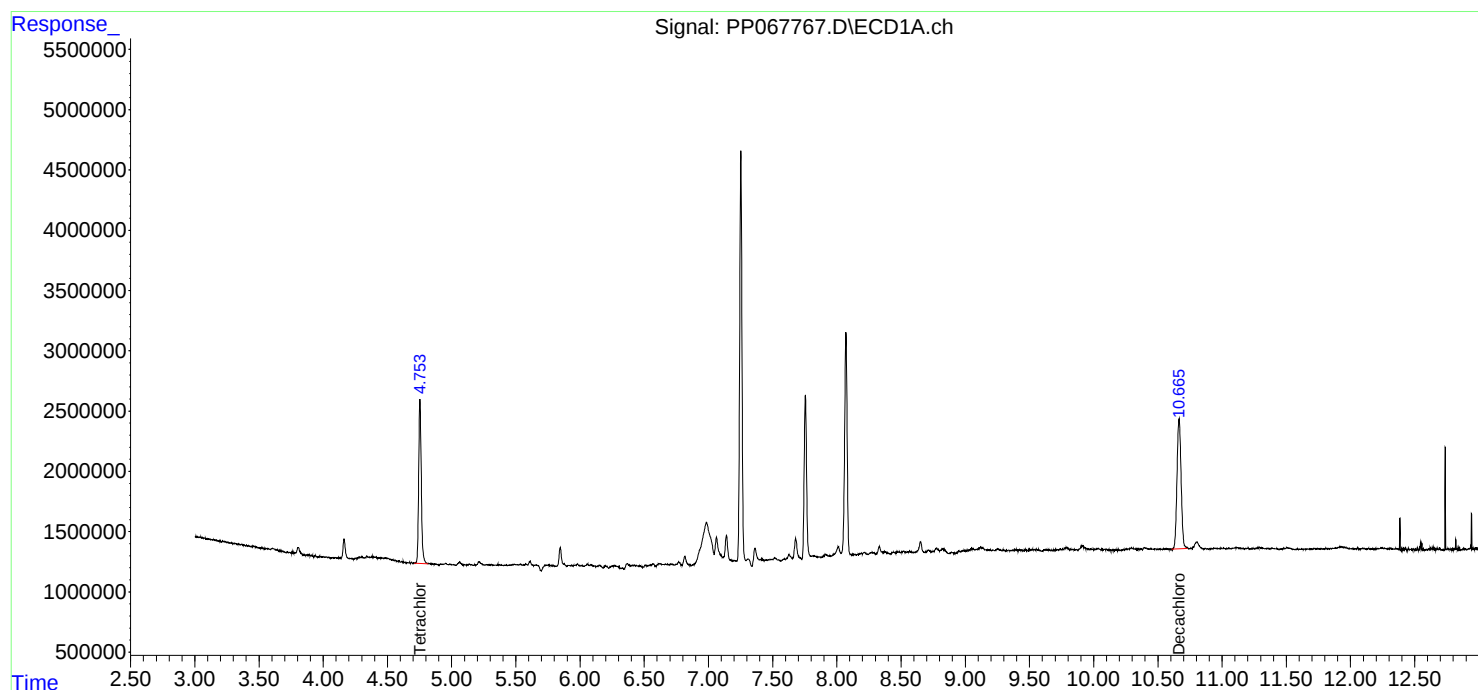


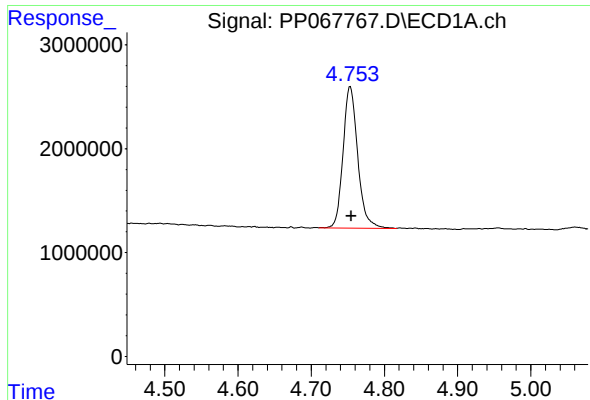

#1 Tetrachloro-m-xylene


R.T.: 4.753 min
Delta R.T.: -0.002 min
Response: 18928208
Conc: 20.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-9

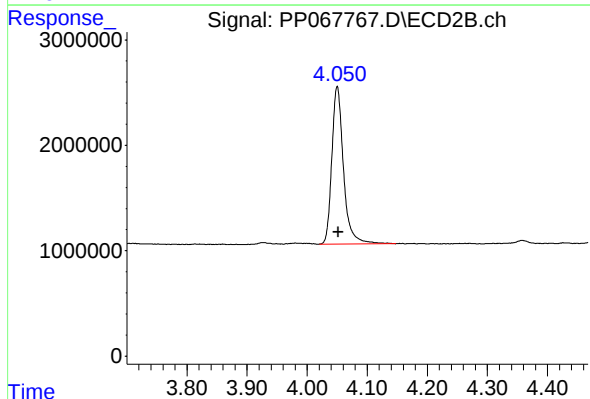


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 20175085
Conc: 19.97 ng/ml

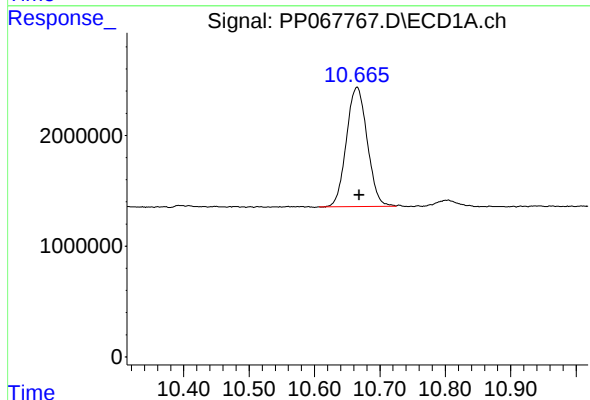

#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.003 min
Response: 23901574
Conc: 20.76 ng/ml

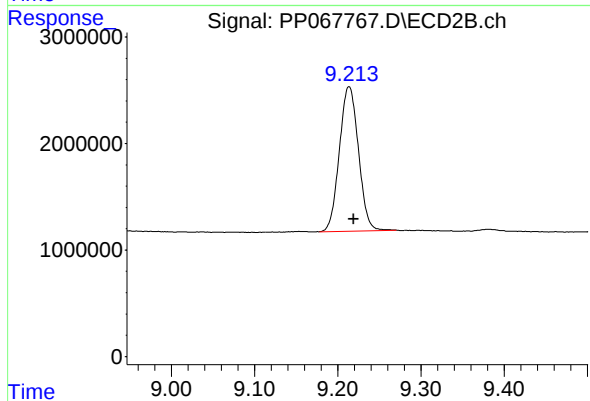

#2 Decachlorobiphenyl

R.T.: 9.214 min
Delta R.T.: -0.005 min
Response: 21628928
Conc: 19.29 ng/ml