


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102224\
Data File : BF139916.D
Acq On : 22 Oct 2024 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

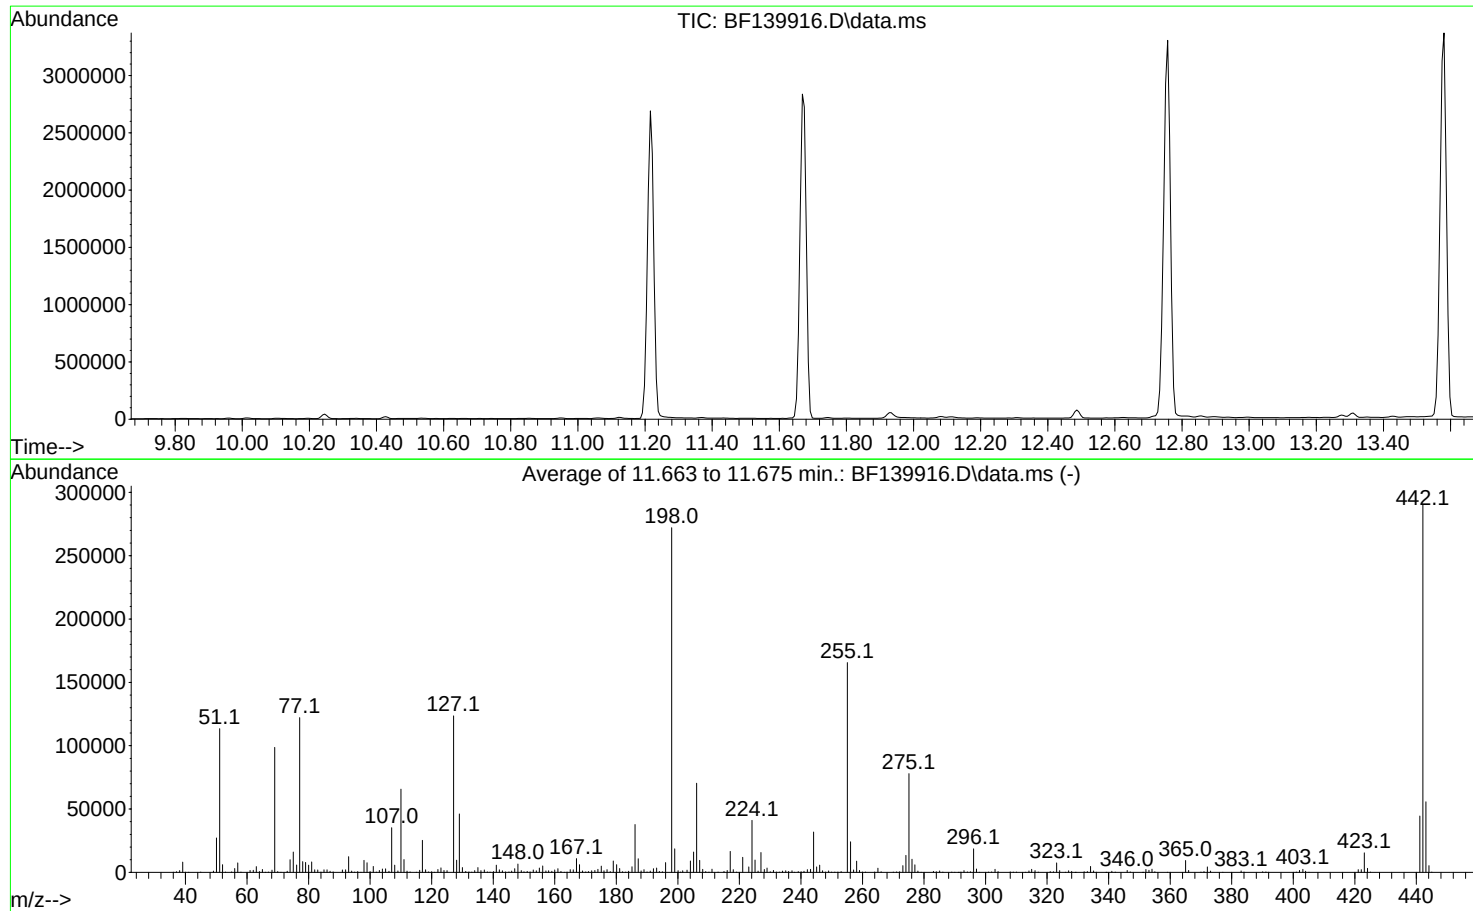




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	113501	PASS
68	69	0.00	2	1.7	1712	PASS
69	198	0.00	100	36.3	98726	PASS
70	69	0.00	2	0.7	646	PASS
127	198	10	80	45.4	123547	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	272043	PASS
199	198	5	9	6.8	18520	PASS
275	198	10	60	28.6	77909	PASS
365	198	1	100	3.5	9417	PASS
441	198	0.01	100	16.4	44501	PASS
442	442	50	100	100.0	290411	PASS
443	442	15	24	19.2	55752	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102224\
Data File : BF139916.D
Acq On : 22 Oct 2024 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 22 11:01:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

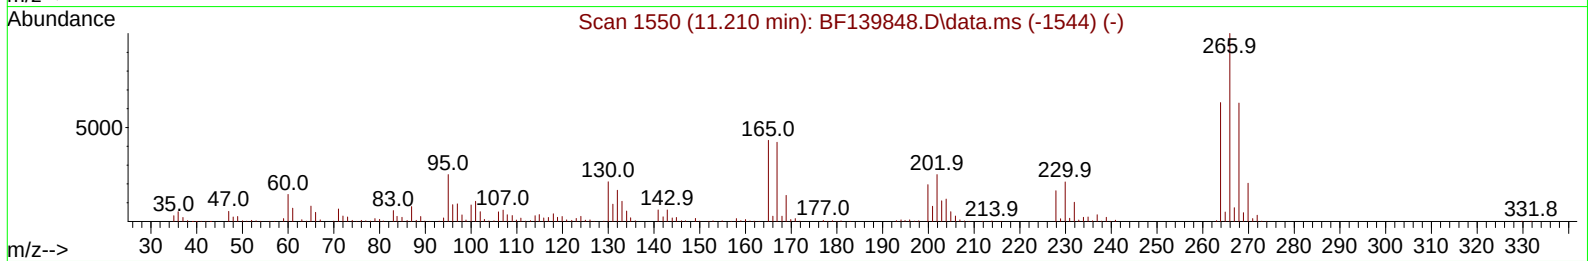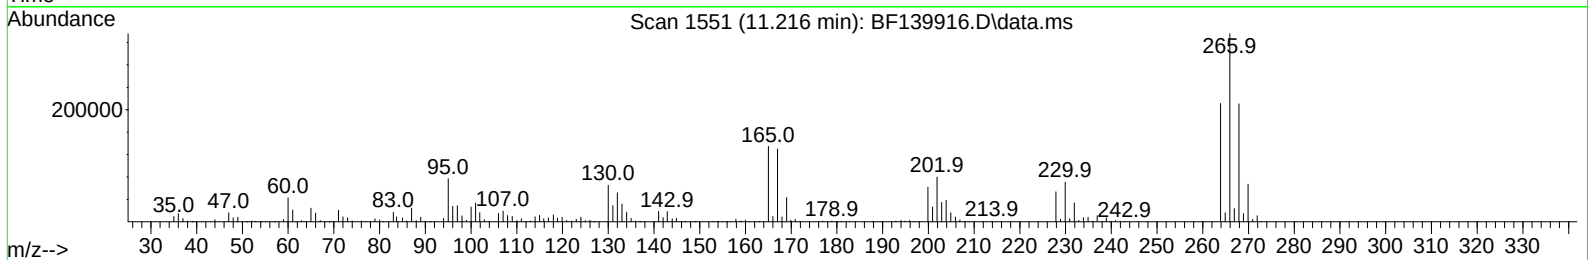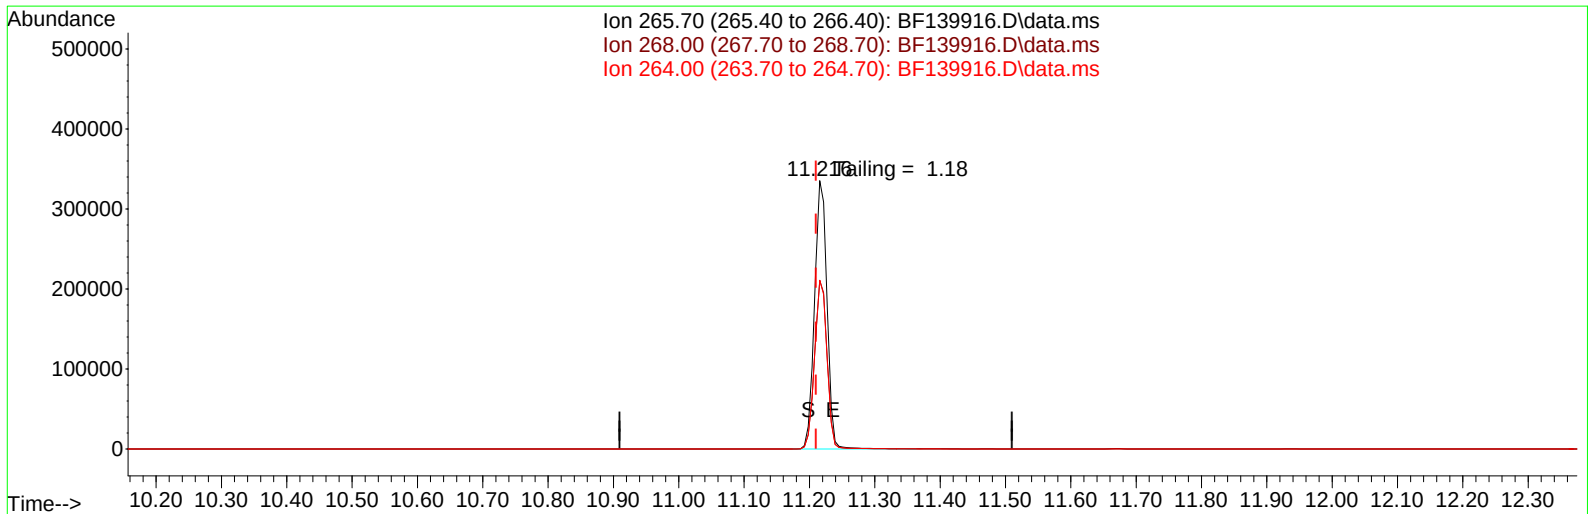

TIC: BF139916.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 57901.68 ng




response 446642

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.76
264.00	63.20	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102224\
Data File : BF139916.D
Acq On : 22 Oct 2024 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 22 11:01:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

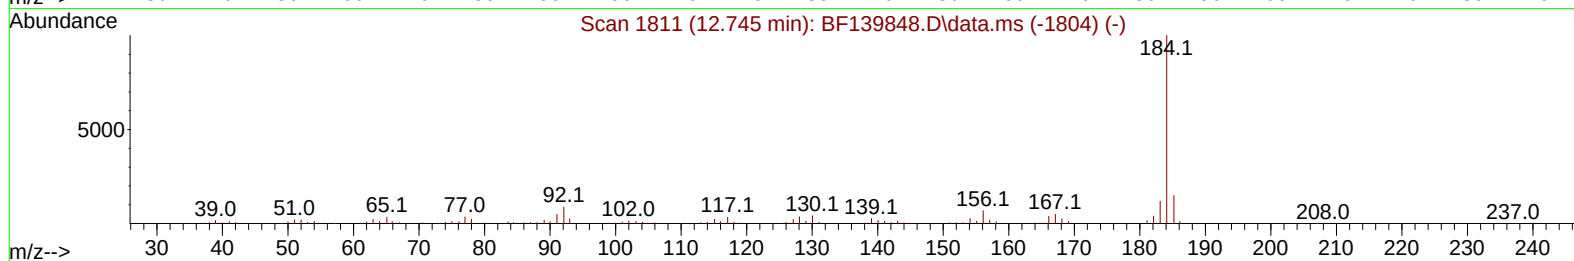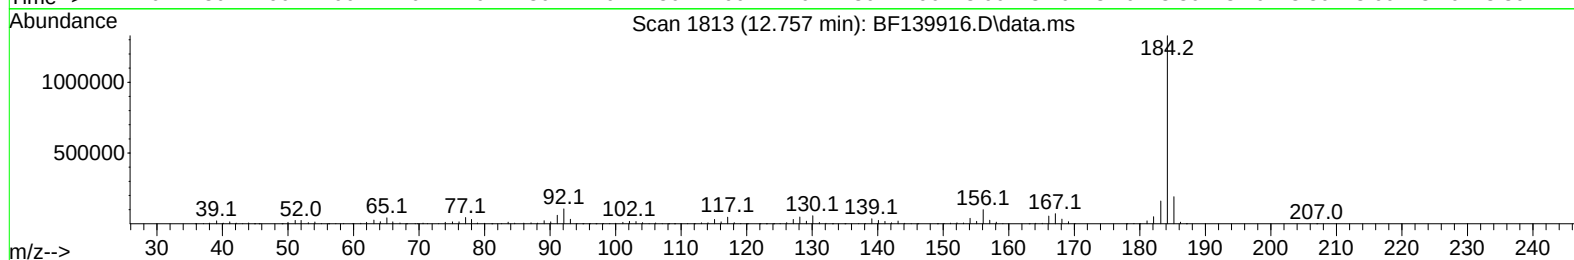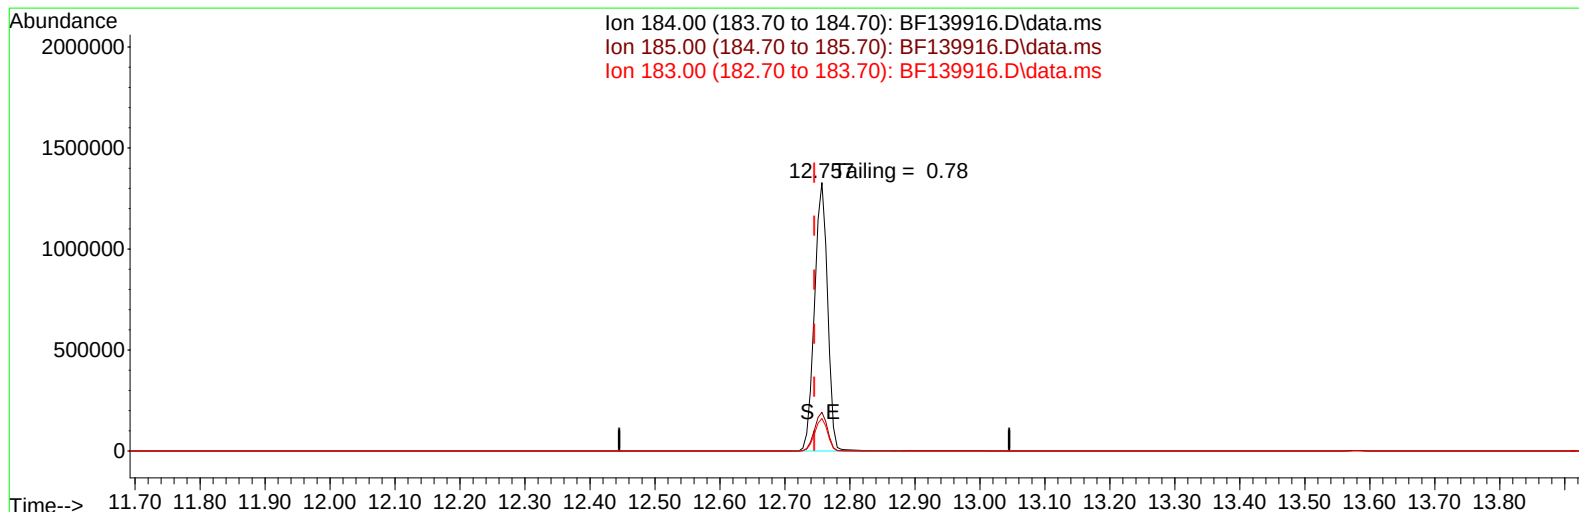

TIC: BF139916.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 72988.41 ng

response 1860275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.42
183.00	11.80	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/22/2024	BNA_F	<u>BF139916.D</u>
Compound Name	Response	Retention Time
DDT	893067	13.58
DDD	14216	13.31
DDE	862	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15078	908145	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP