
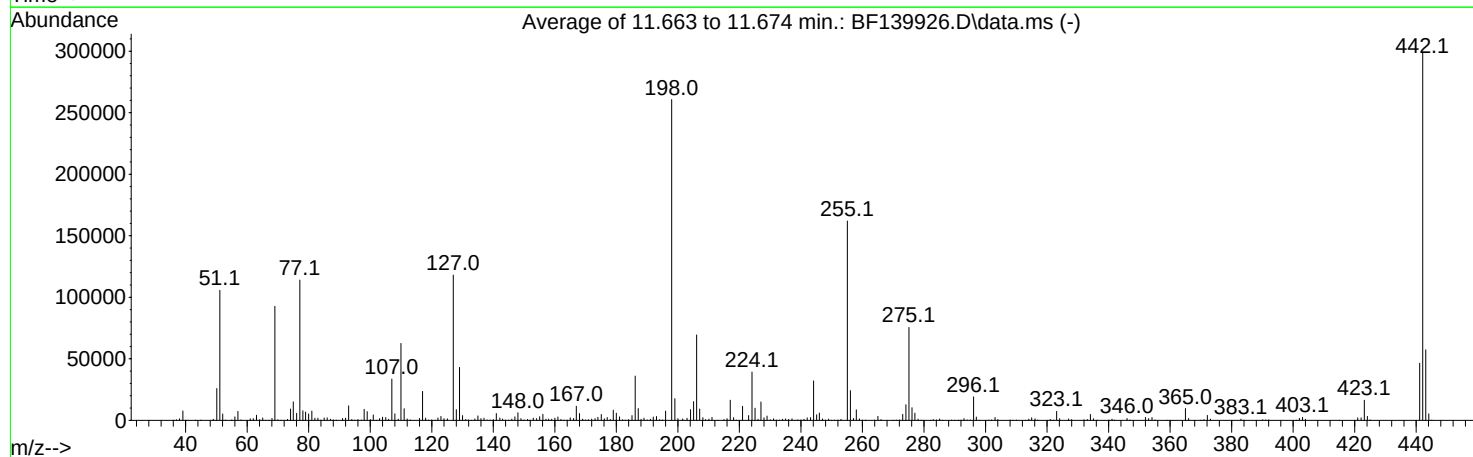


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102224\
Data File : BF139926.D
Acq On : 22 Oct 2024 14:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

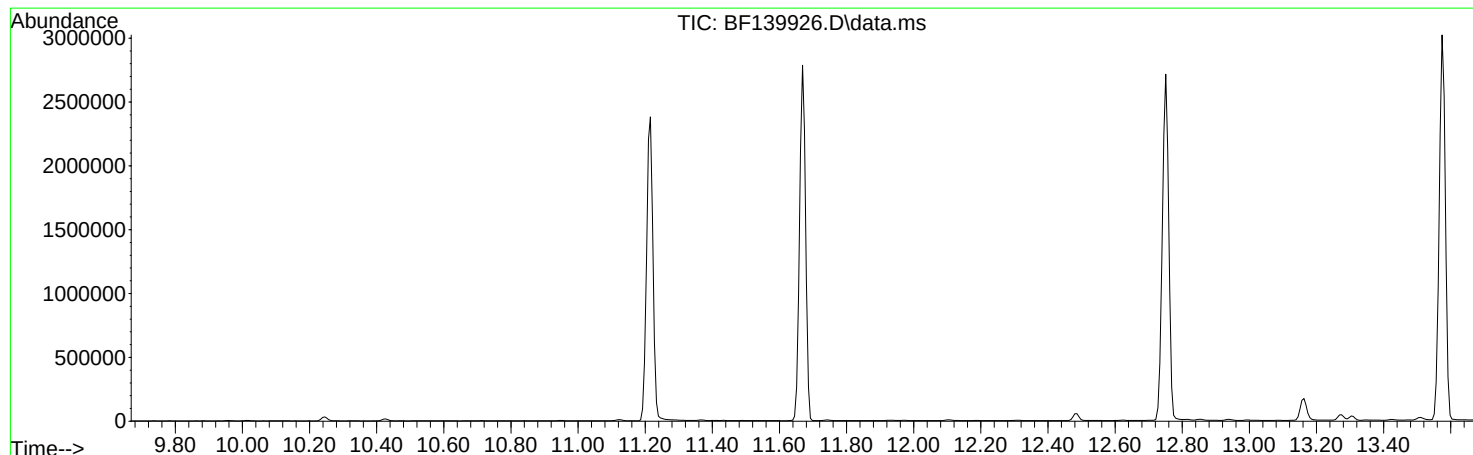




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	105765	PASS
68	69	0.00	2	1.7	1602	PASS
69	198	0.00	100	35.6	92720	PASS
70	69	0.00	2	0.6	550	PASS
127	198	10	80	45.3	118056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	260715	PASS
199	198	5	9	6.8	17717	PASS
275	198	10	60	29.0	75581	PASS
365	198	1	100	3.7	9606	PASS
441	198	0.01	100	17.8	46395	PASS
442	442	50	100	100.0	298923	PASS
443	442	15	24	19.2	57373	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102224\
Data File : BF139926.D
Acq On : 22 Oct 2024 14:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 22 14:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

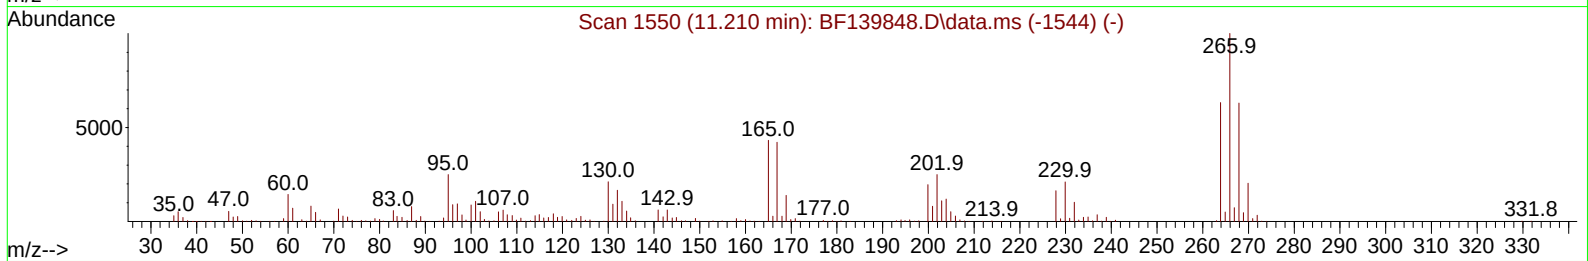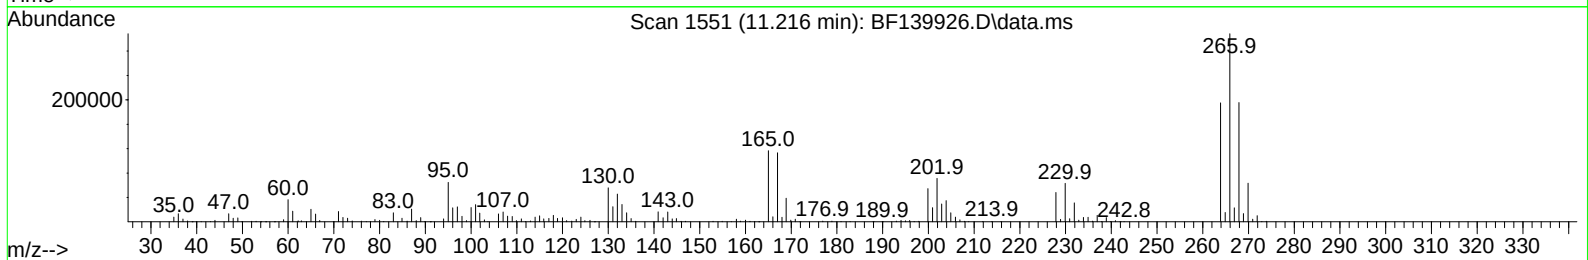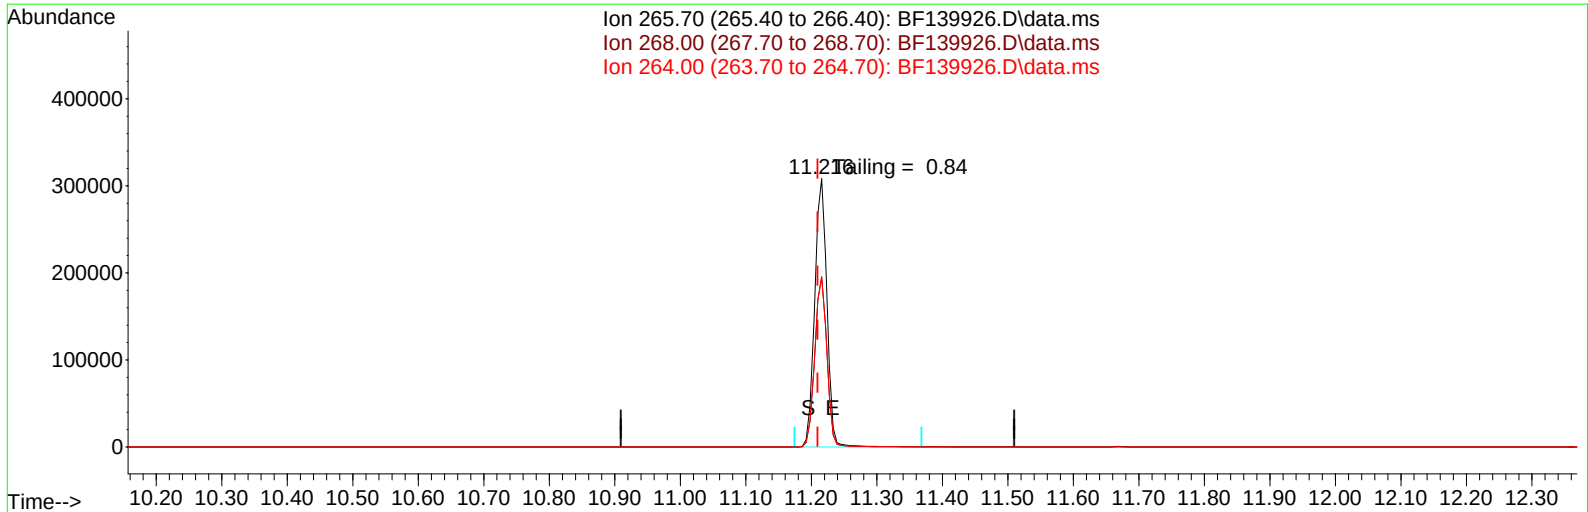

TIC: BF139926.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 57892.68 ng




response 400979

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.45
264.00	63.20	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102224\
Data File : BF139926.D
Acq On : 22 Oct 2024 14:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 22 14:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

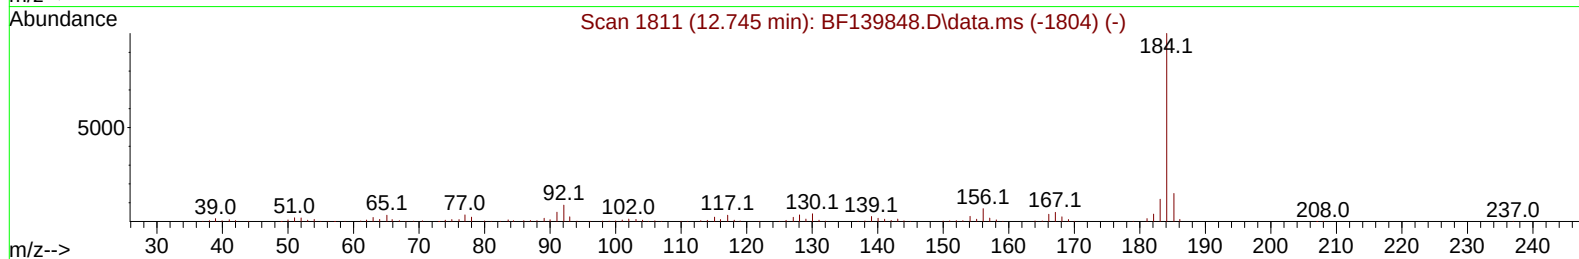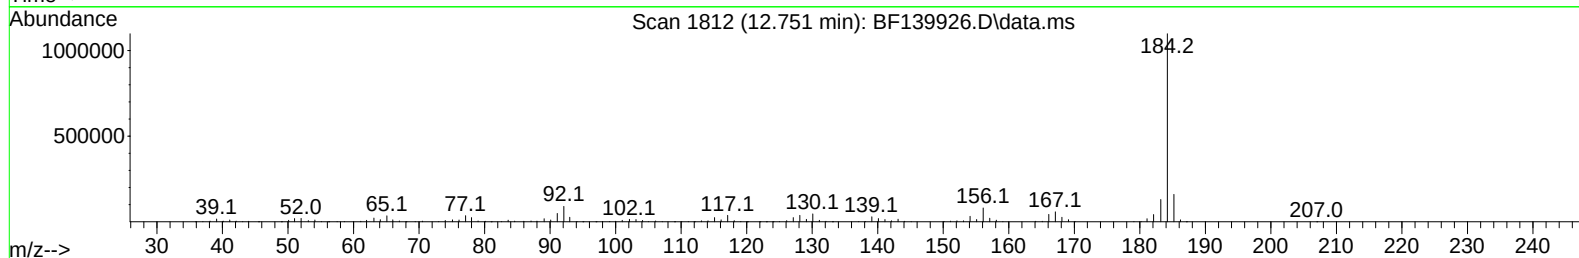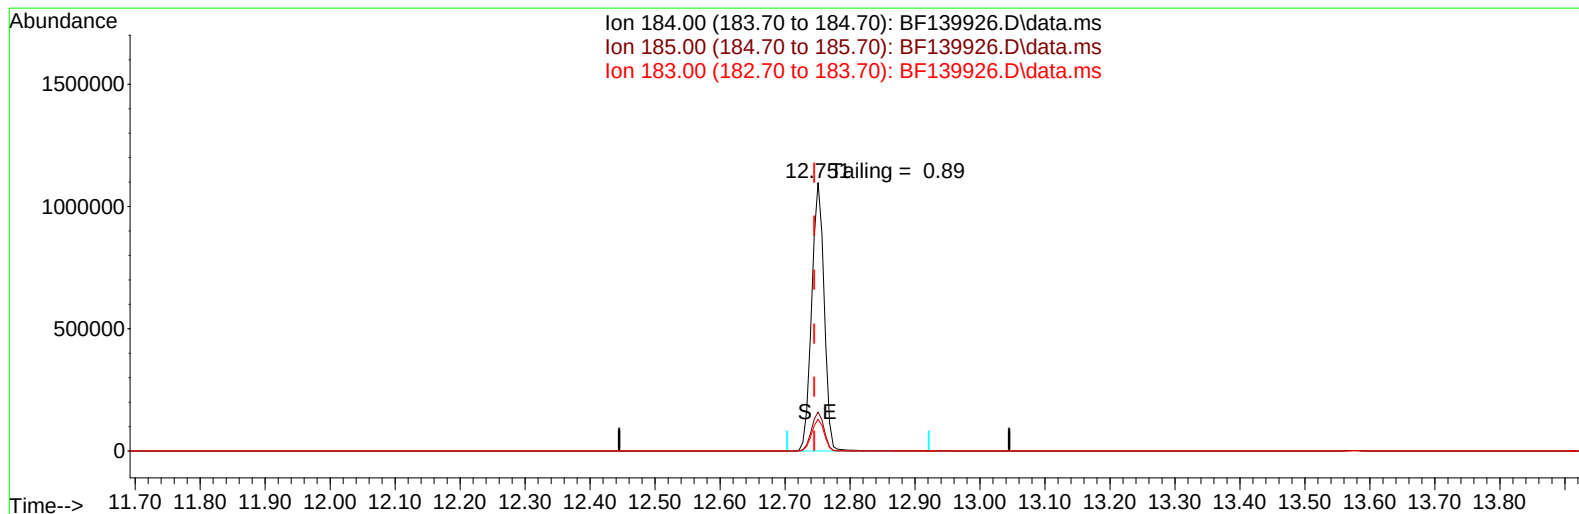

TIC: BF139926.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 78165.14 ng

response 1467813

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.58
183.00	11.80	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/22/2024	BNA_F	<u>BF139926.D</u>
Compound Name	Response	Retention Time
DDT	777904	13.574
DDD	19547	13.274
DDE	2185	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21732	799636	2.72

Instrument :
BNA_F
ClientSampleId :
DFTPP