

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
 Data File : PS028035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 11:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:40:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 23 13:25:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.091	7.613	1361.6E6	464.2E6	504.851	489.266
Target Compounds							
1) T	Dalapon	2.539	0.000	13115702	0	2.879	N.D. #
3) T	4-Nitroph...	6.880	0.000	11078898	0	5.987	N.D. #
7) T	MCPA	0.000	8.130	0	5837371	N.D.	1.268
8) T	DICHLORPROP	7.978	8.555f	-209004	3832502	N.D.	4.090
9) T	2,4-D	8.187	0.000	6674734	0	1.970	N.D. #
10) T	Pentachlo...	8.464	0.000	1858280	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.993f	0.000	3955523	0	<MDL	N.D. #
12) T	2,4,5-T	9.320	0.000	676214	0	<MDL	N.D. #
13) T	2,4-DB	9.881	0.000	298722	0	<MDL	N.D. #
14) T	DINOSEB	11.048	0.000	2919319	0	<MDL	N.D. #
15) T	Picloram	10.858	12.173	19060027	1553327	<MDL	<MDL #
16) T	DCPA	11.341	0.000	276595	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
Data File : PS028035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 11:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:40:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
Quant Title : 8080.M
QLast Update : Wed Oct 23 13:25:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

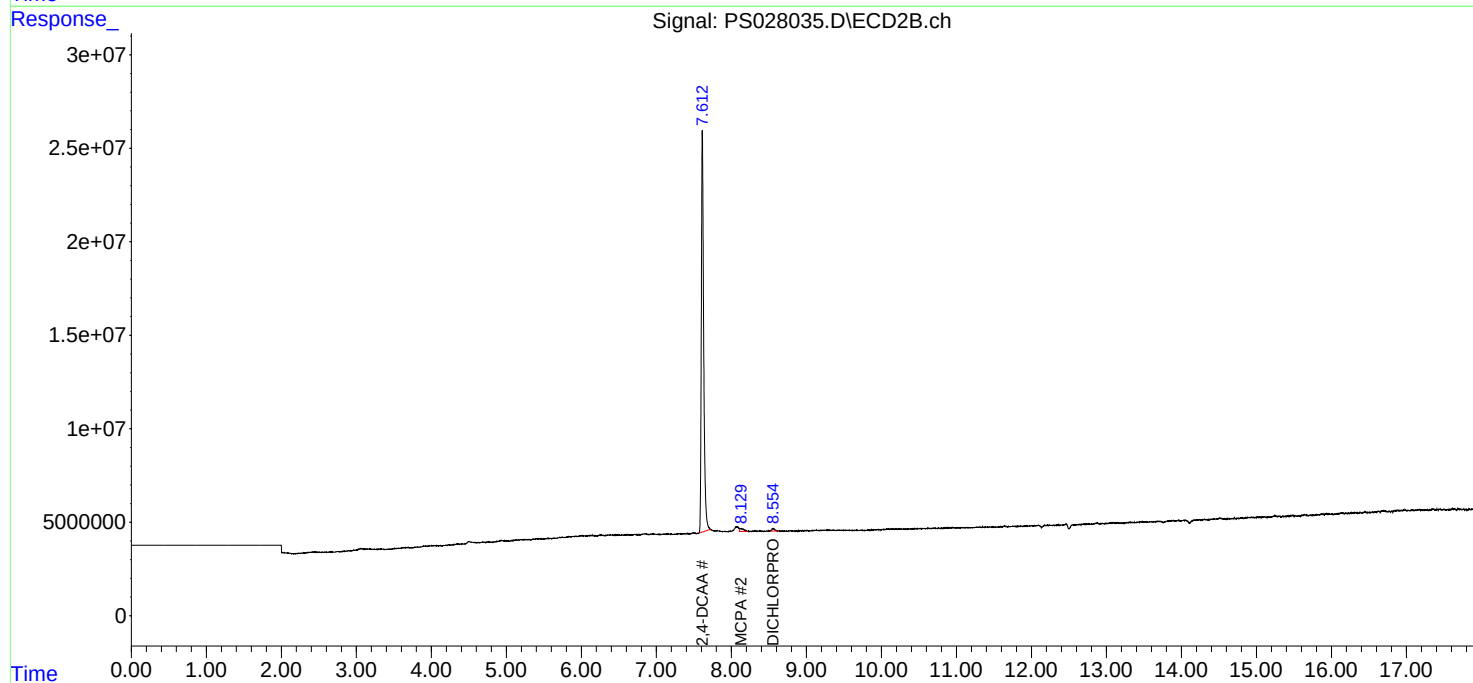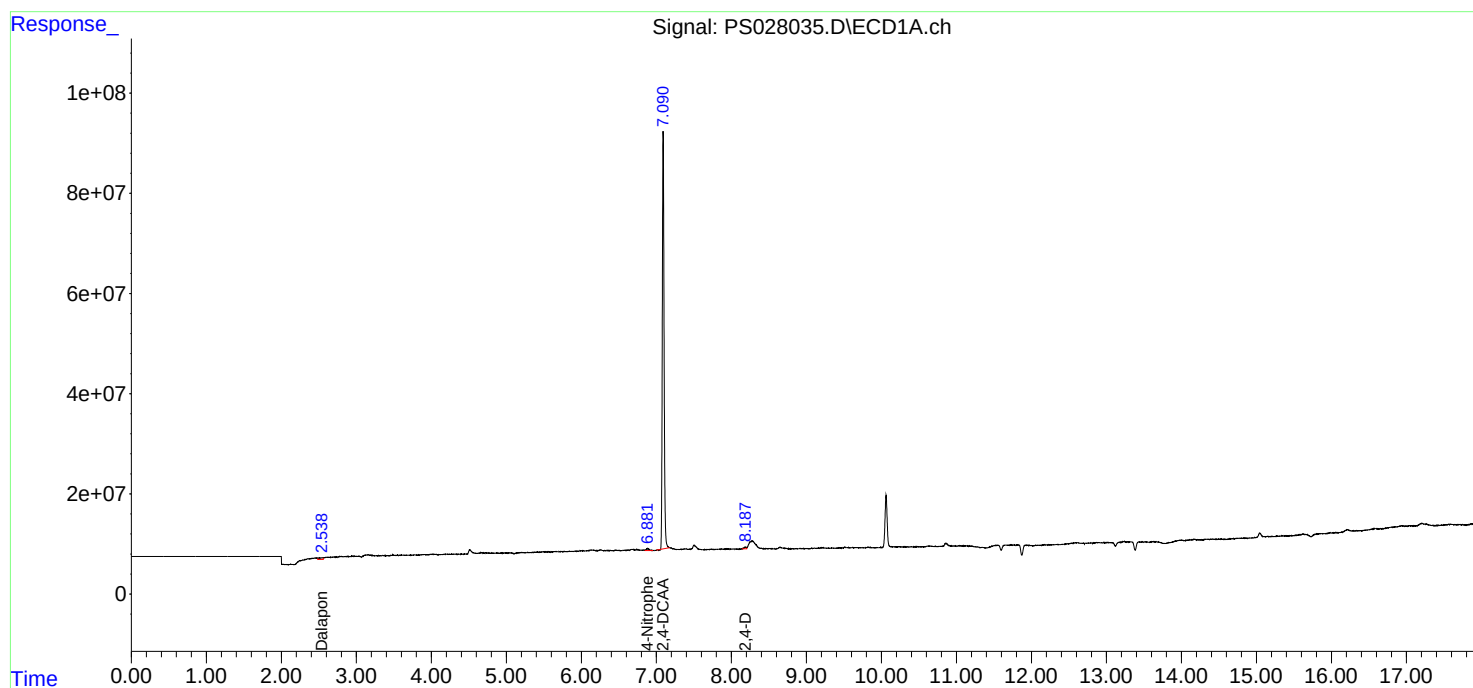


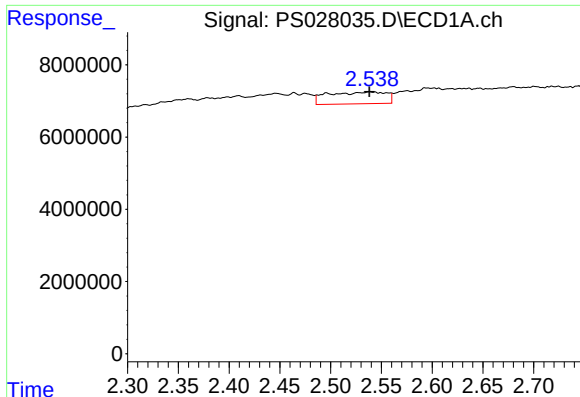

#1 Dalapon


R.T.: 2.539 min
Delta R.T.: 0.001 min
Response: 13115702
Conc: 2.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

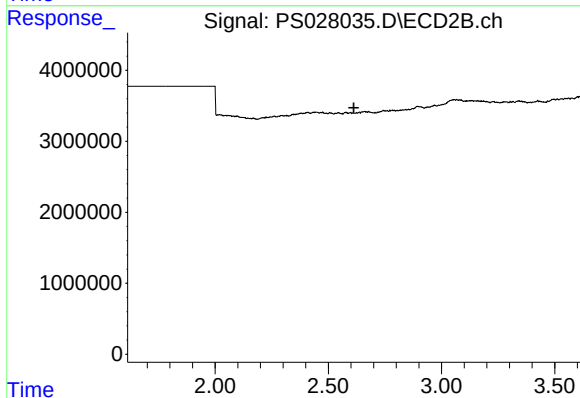


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.613 min
Response: 0
Conc: N.D.

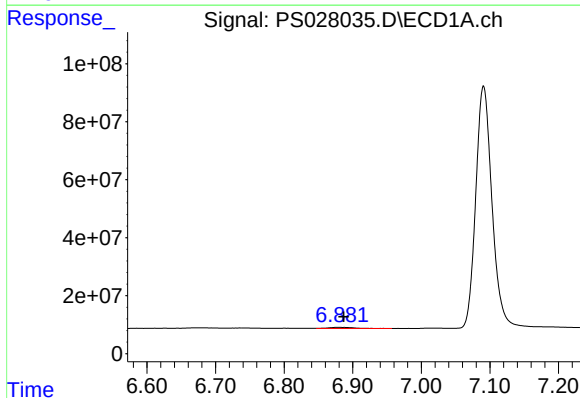


#3 4-Nitrophenol

R.T.: 6.880 min
Delta R.T.: -0.007 min
Response: 11078898
Conc: 5.99 ng/ml

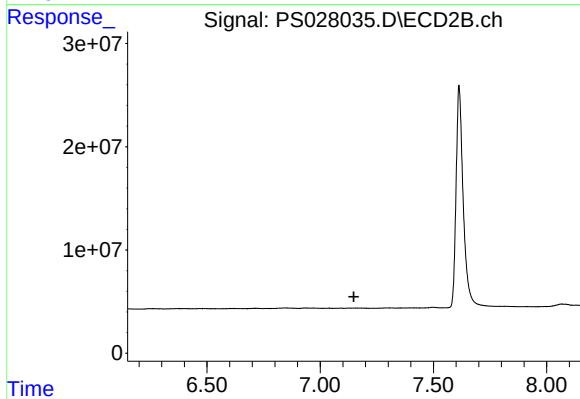

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

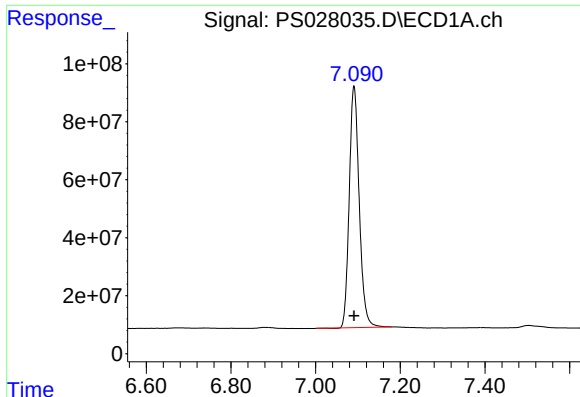

#4 2,4-DCAA


R.T.: 7.091 min
Delta R.T.: 0.000 min
Response: 1361564483
Conc: 504.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

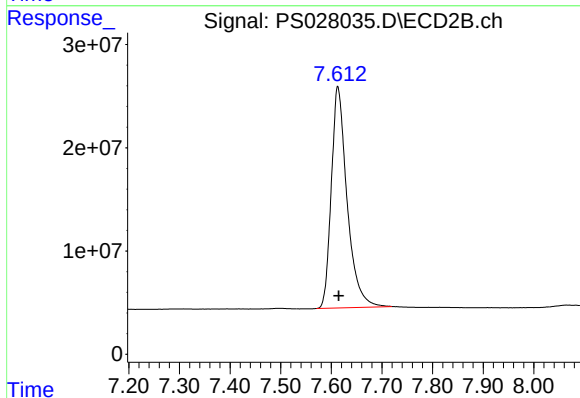


#4 2,4-DCAA

R.T.: 7.613 min
Delta R.T.: -0.002 min
Response: 464155644
Conc: 489.27 ng/ml

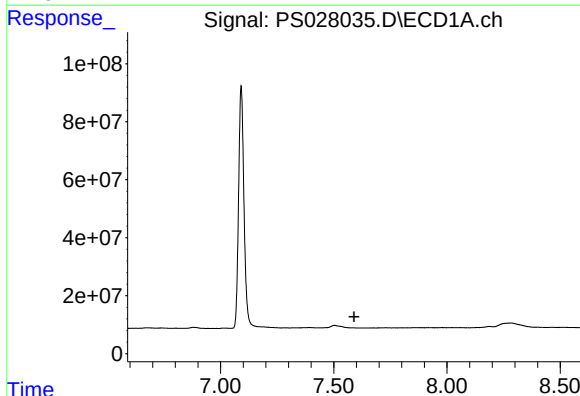


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.589 min
Response: 0
Conc: N.D.

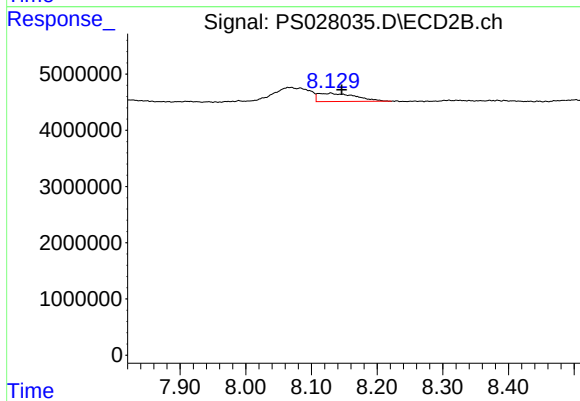

#7 MCPA


R.T.: 8.130 min
Delta R.T.: -0.017 min
Response: 5837371
Conc: 1.27 ug/ml

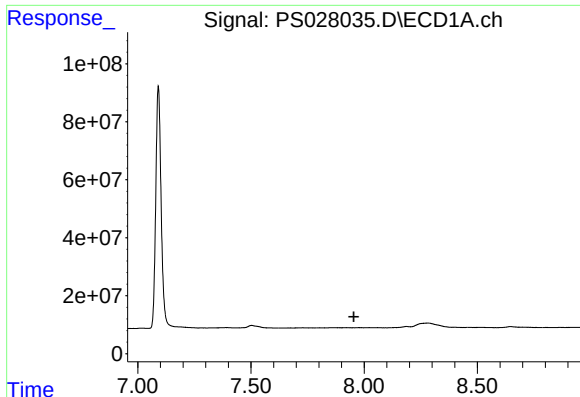

#8 DICHLORPROP


R.T.: 7.978 min
Delta R.T.: 0.023 min
Response: -209004
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

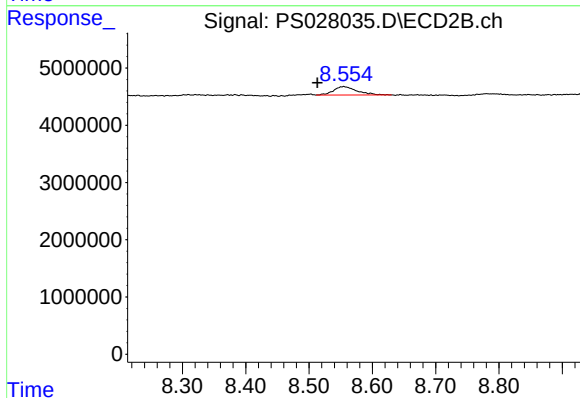


#8 DICHLORPROP

R.T.: 8.555 min
Delta R.T.: 0.042 min
Response: 3832502
Conc: 4.09 ng/ml

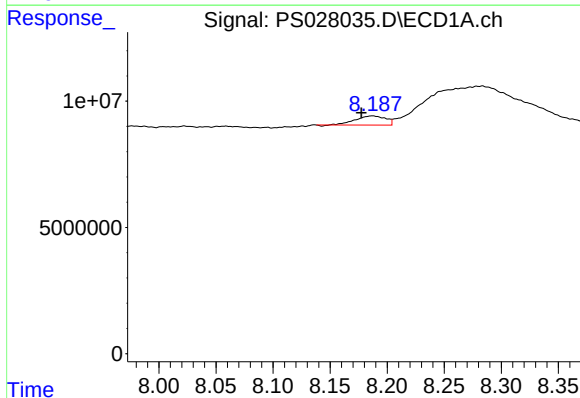

#9 2,4-D

R.T.: 8.187 min
Delta R.T.: 0.009 min
Response: 6674734
Conc: 1.97 ng/ml

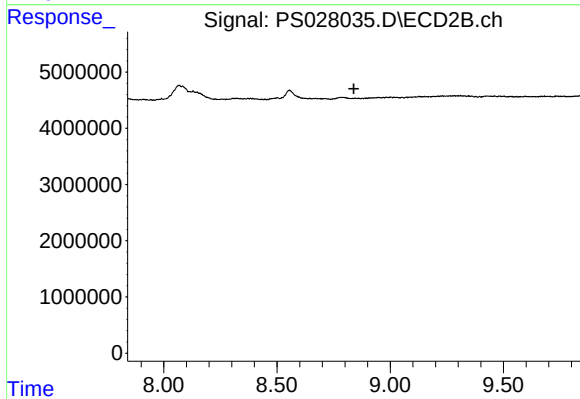

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.840 min
Response: 0
Conc: N.D.