

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
 Data File : PS028046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 20:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:49:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 23 13:25:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.091	7.612	1362.1E6	454.5E6	505.063	479.127
Target Compounds							
1) T	Dalapon	2.491f	0.000	3567174	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.326f	0.000	215163	0	<MDL	N.D. #
3) T	4-Nitroph...	6.885	0.000	9448181	0	5.106	N.D. #
6) T	MCP	7.396f	0.000	1778999	0	<MDL	N.D. #
7) T	MCPA	0.000	8.140	0	318828	N.D.	<MDL
8) T	DICHLORPROP	0.000	8.551f	0	2914520	N.D.	3.111
10) T	Pentachlo...	8.469	0.000	2737642	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.009	0.000	1041397	0	<MDL	N.D. #
12) T	2,4,5-T	9.318	0.000	1847286	0	<MDL	N.D. #
13) T	2,4-DB	9.874	0.000	1907977	0	<MDL	N.D. #
14) T	DINOSEB	11.061	0.000	1190803	0	<MDL	N.D. #
15) T	Picloram	10.857	0.000	19425838	0	<MDL	N.D. #
16) T	DCPA	11.348	0.000	3104732	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
Data File : PS028046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 20:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:49:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
Quant Title : 8080.M
QLast Update : Wed Oct 23 13:25:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

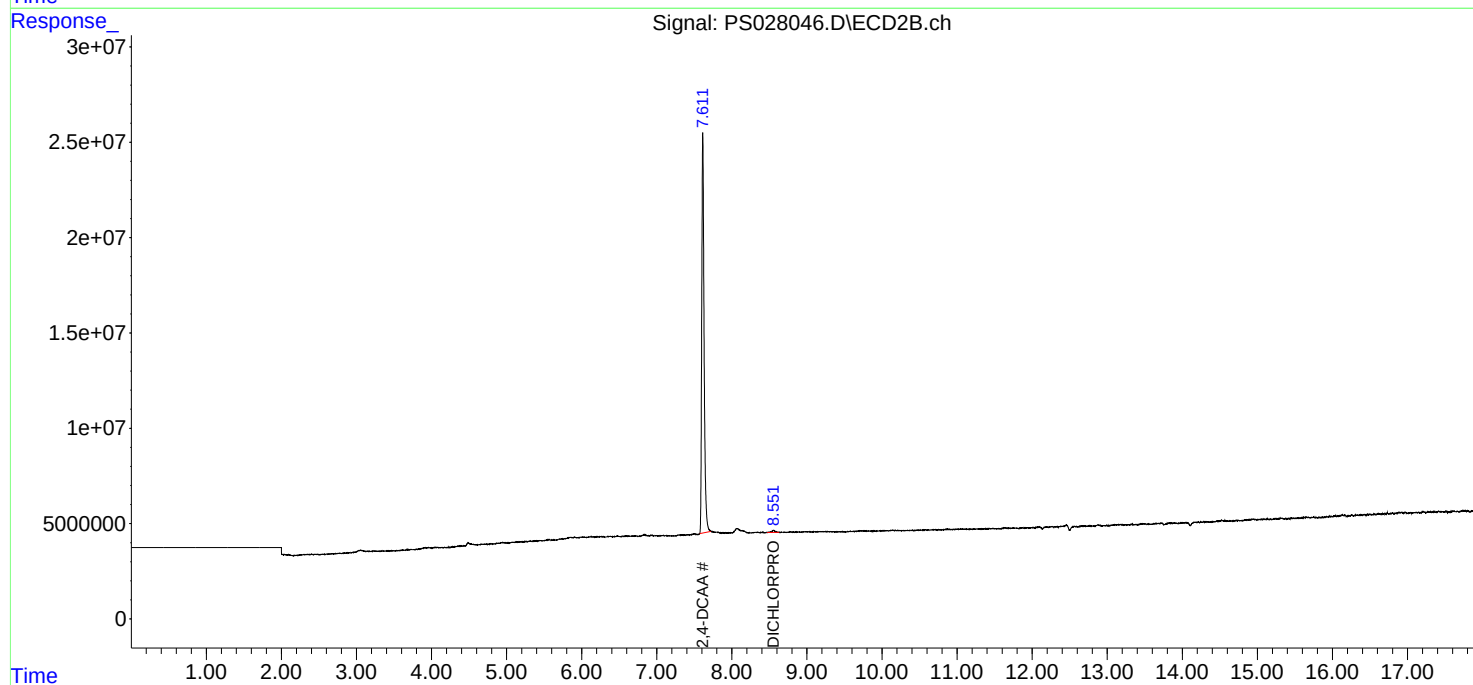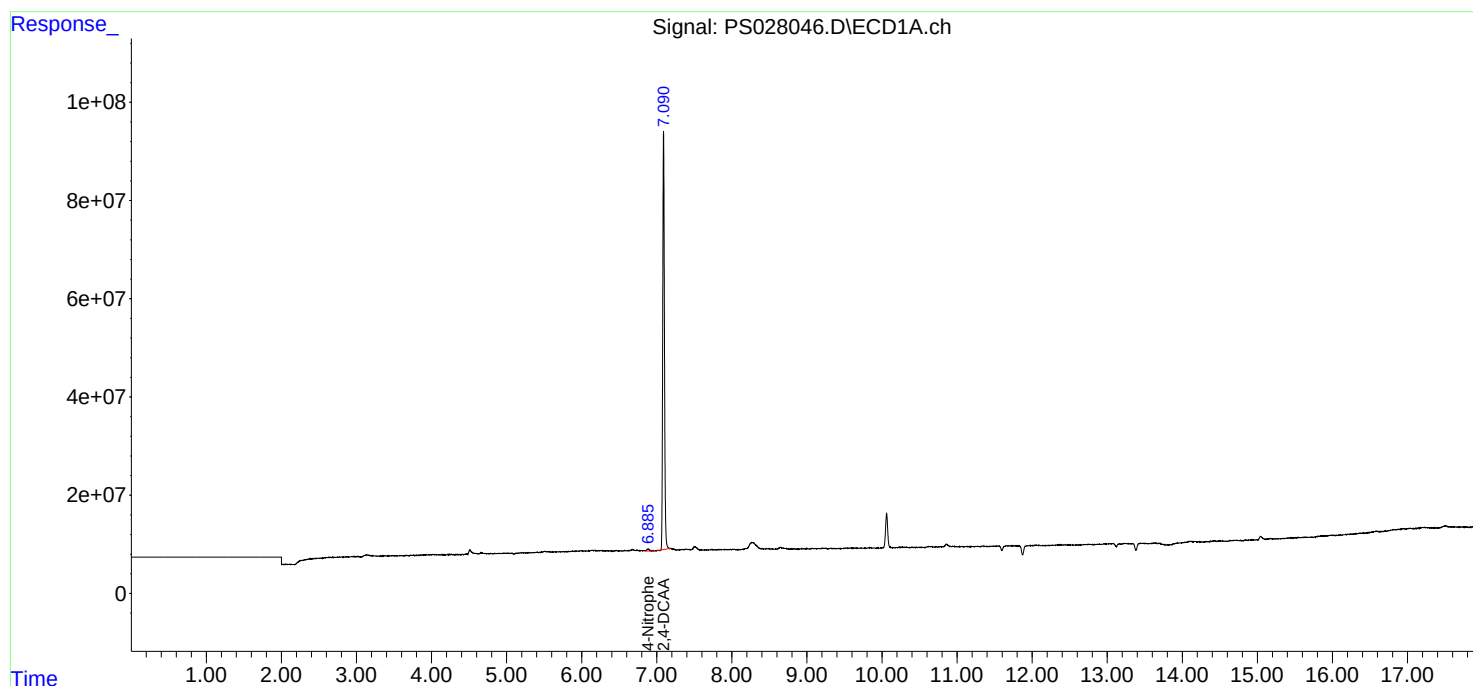


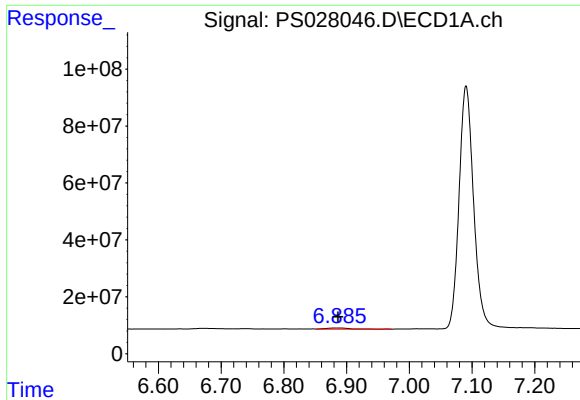

#3 4-Nitrophenol


R.T.: 6.885 min
Delta R.T.: -0.001 min
Response: 9448181
Conc: 5.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

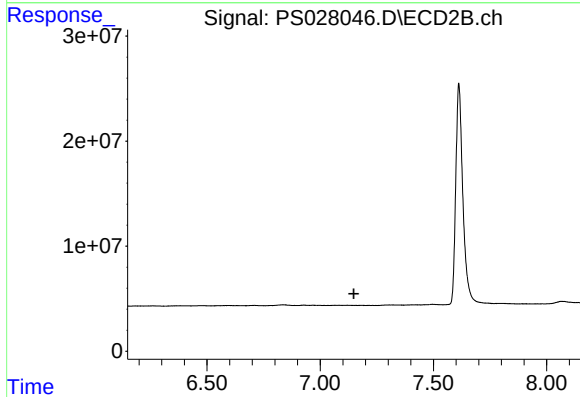


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

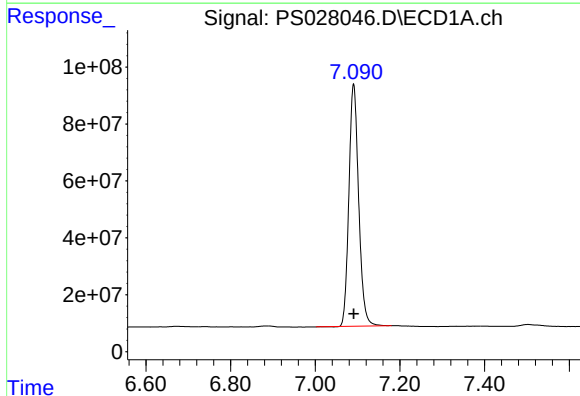


#4 2,4-DCAA

R.T.: 7.091 min
Delta R.T.: 0.000 min
Response: 1362136272
Conc: 505.06 ng/ml

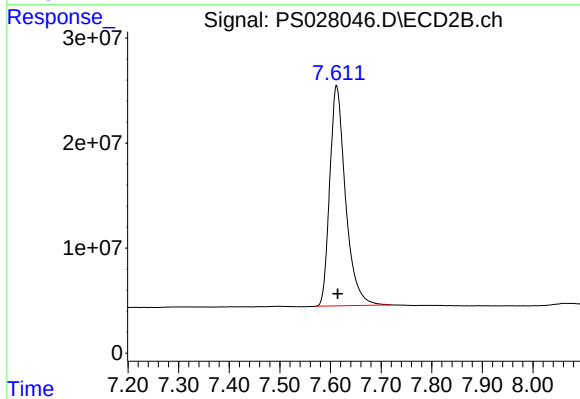

#4 2,4-DCAA


R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 454536852
Conc: 479.13 ng/ml

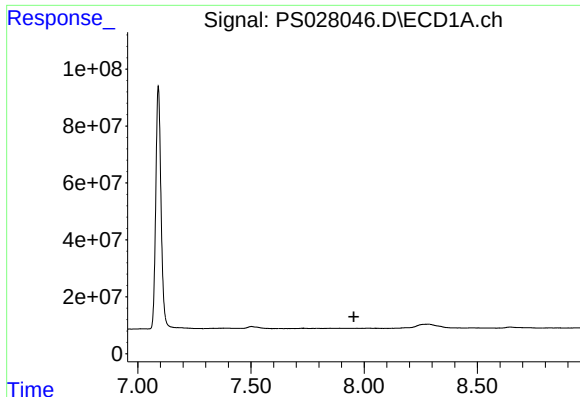

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

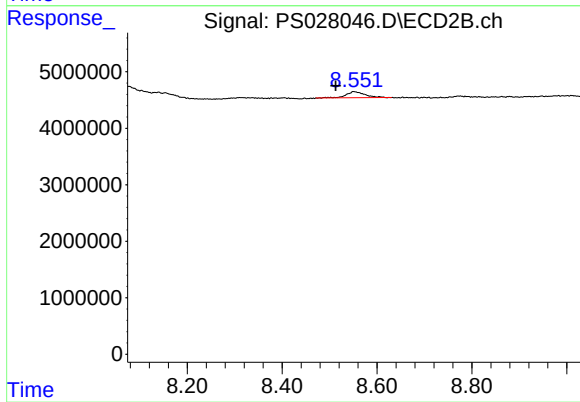

#8 DICHLORPROP

R.T.: 8.551 min
Delta R.T.: 0.037 min
Response: 2914520
Conc: 3.11 ng/ml