
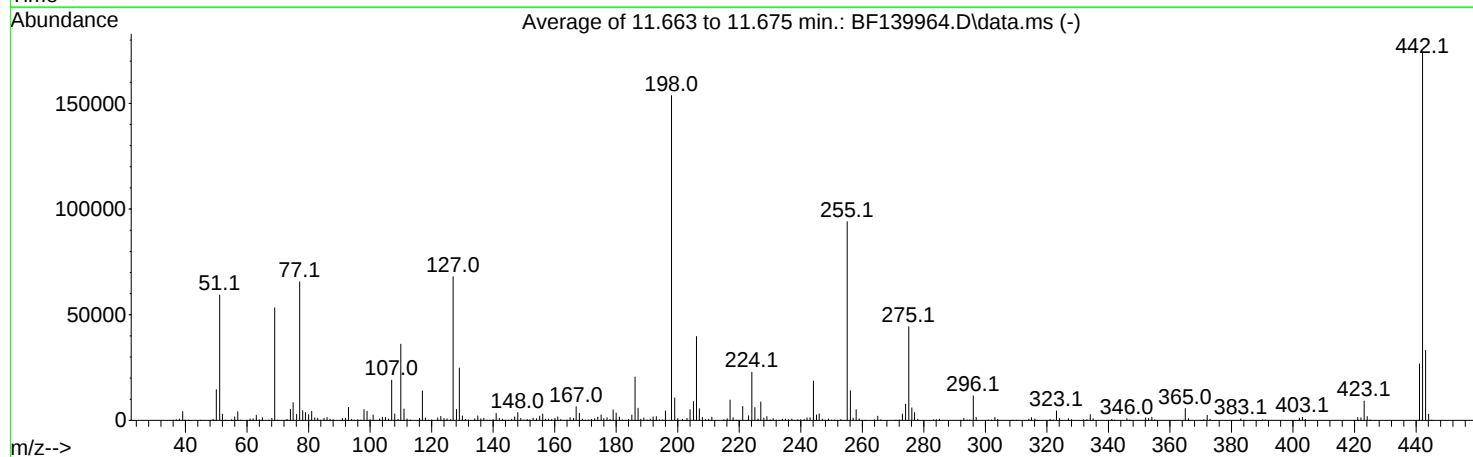


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102324\
Data File : BF139964.D
Acq On : 23 Oct 2024 15:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

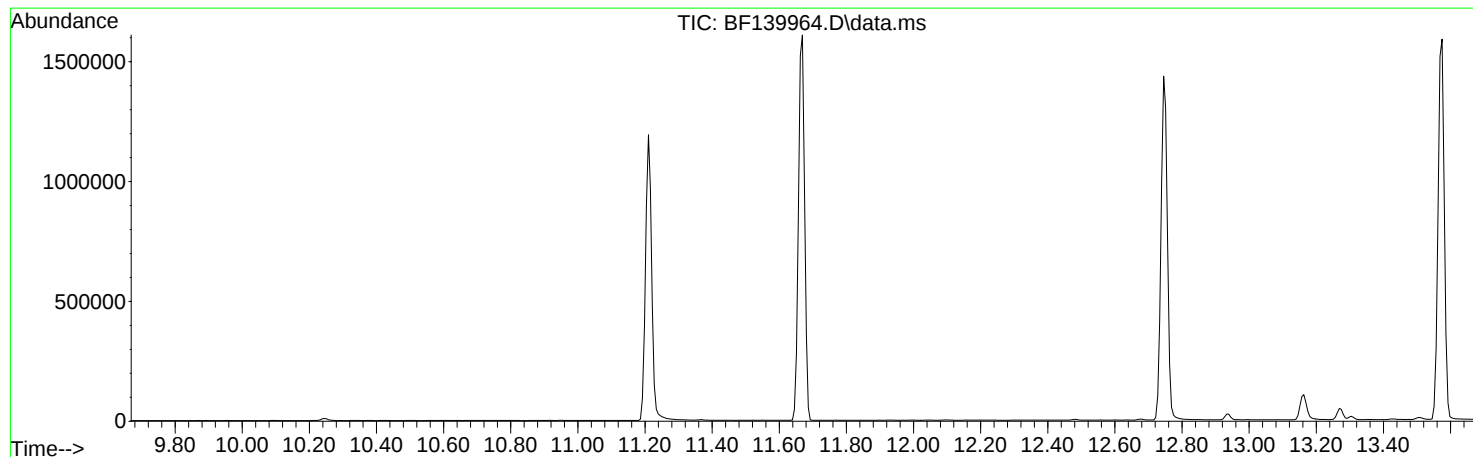

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	59323	PASS
68	69	0.00	2	1.8	983	PASS
69	198	0.00	100	34.6	53243	PASS
70	69	0.00	2	0.4	190	PASS
127	198	10	80	44.2	67984	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153731	PASS
199	198	5	9	6.9	10579	PASS
275	198	10	60	28.8	44264	PASS
365	198	1	100	3.6	5593	PASS
441	198	0.01	100	17.4	26768	PASS
442	442	50	100	100.0	174101	PASS
443	442	15	24	19.1	33184	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/23/2024	BNA_F	<u>BF139964.D</u>
Compound Name	Response	Retention Time
DDT	418094	13.575
DDD	17070	13.269
DDE	5569	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22639	440733	5.14

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102324\
Data File : BF139964.D
Acq On : 23 Oct 2024 15:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 23 15:33:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

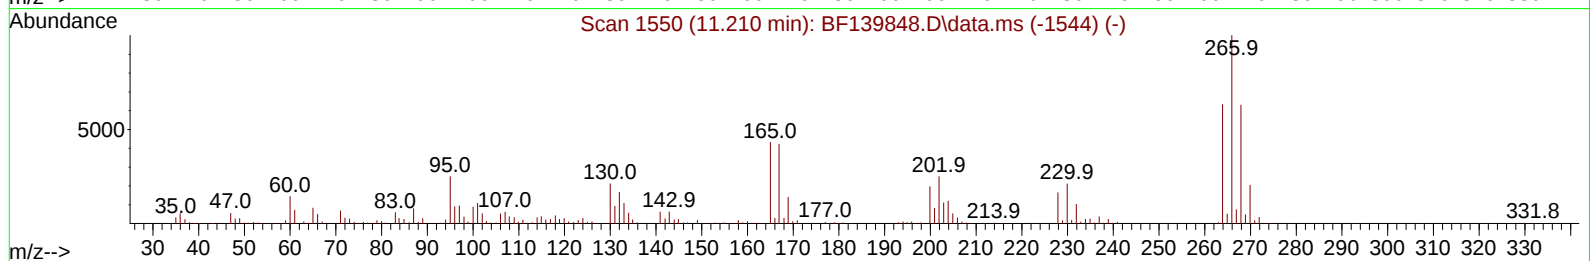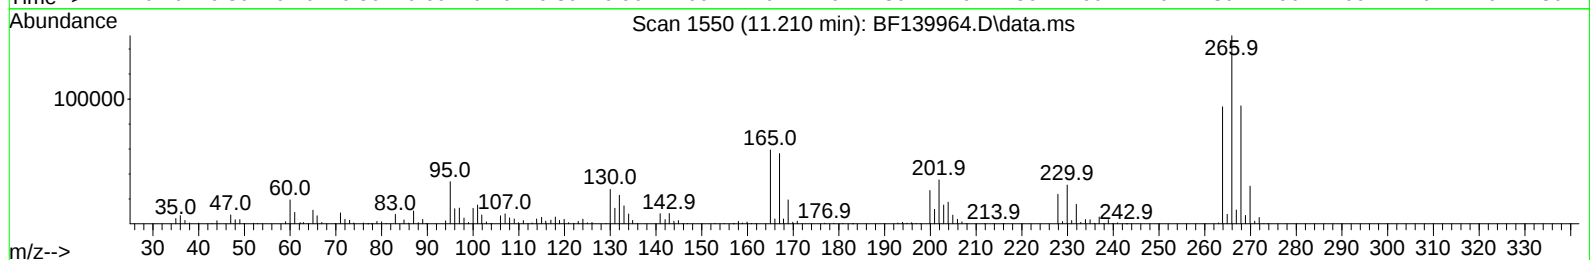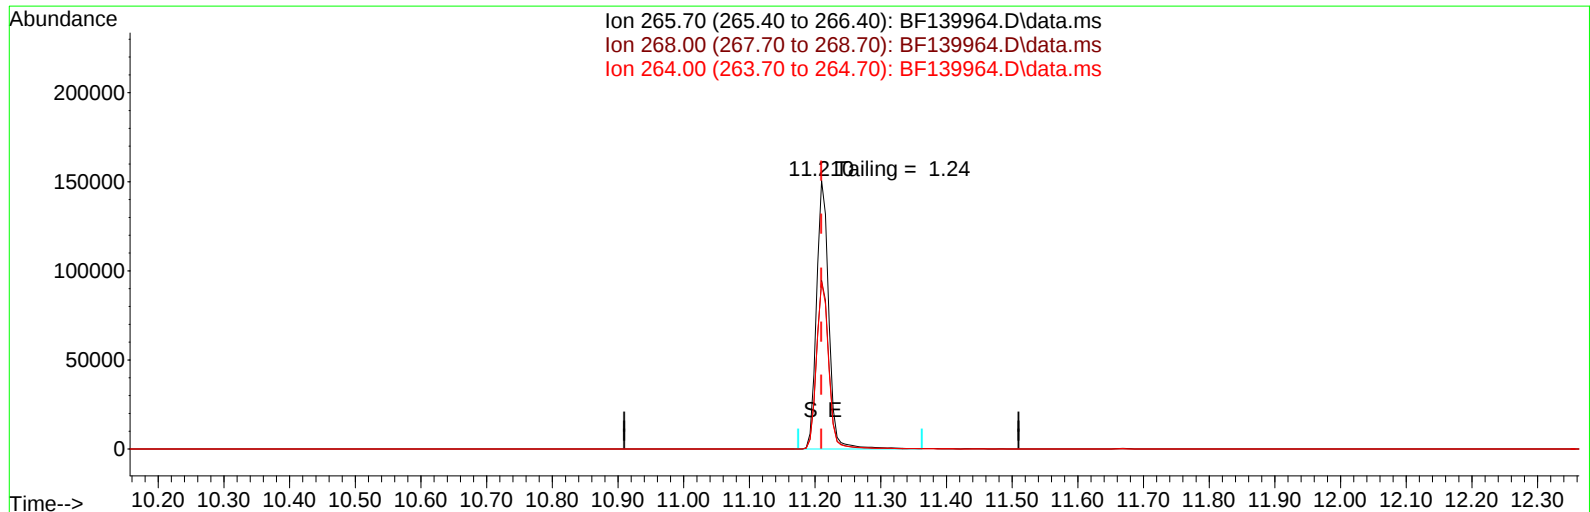

TIC: BF139964.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.000) 37980.39 ng




response 197630

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.75
264.00	63.20	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102324\
Data File : BF139964.D
Acq On : 23 Oct 2024 15:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 23 15:33:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

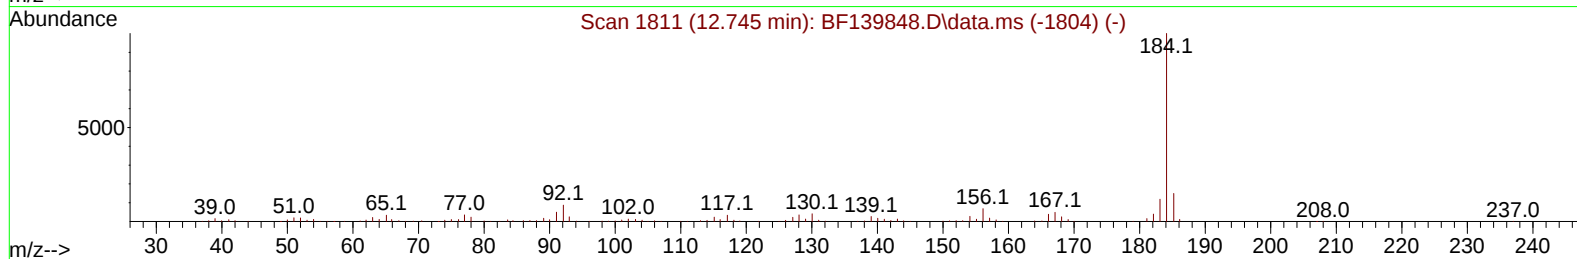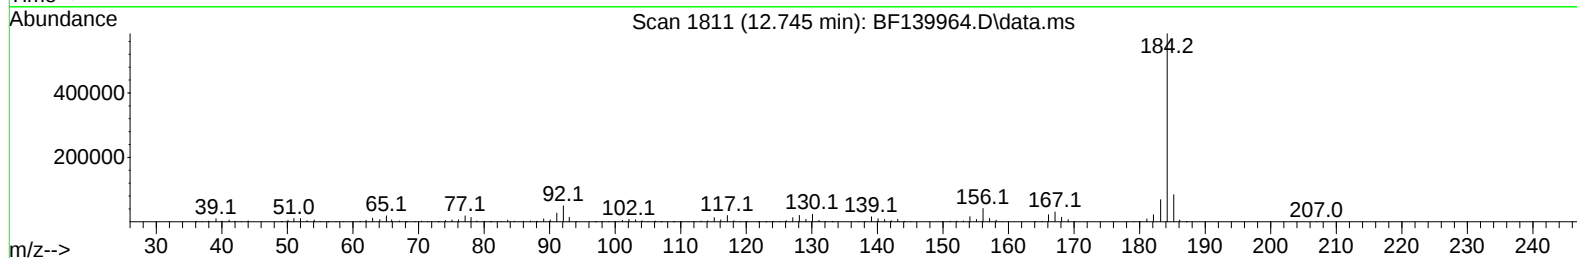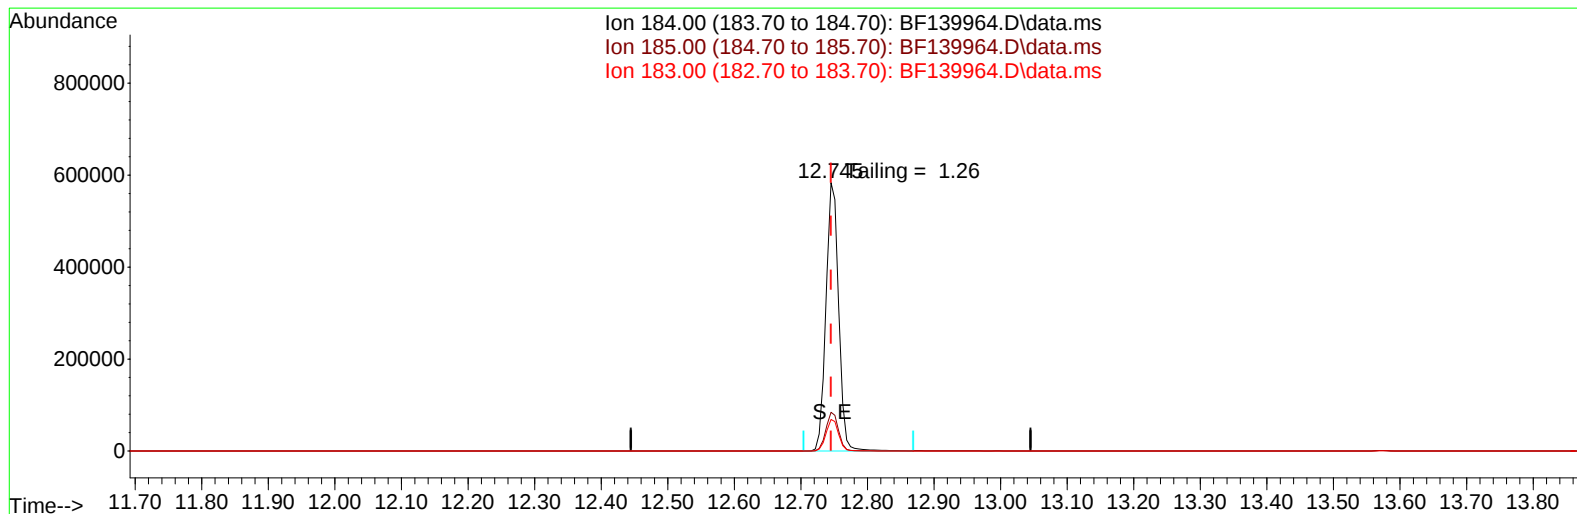

TIC: BF139964.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 775484

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.45
183.00	11.80	11.75
0.00	0.00	0.00