
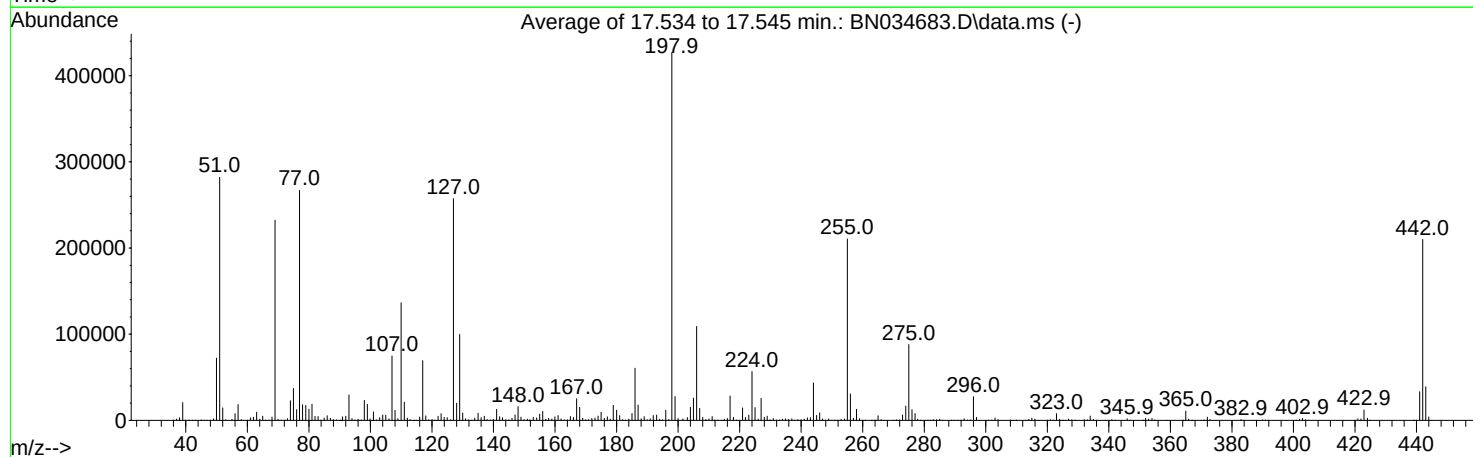


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
Data File : BN034683.D
Acq On : 24 Oct 2024 07:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 24 13:17:02 2024

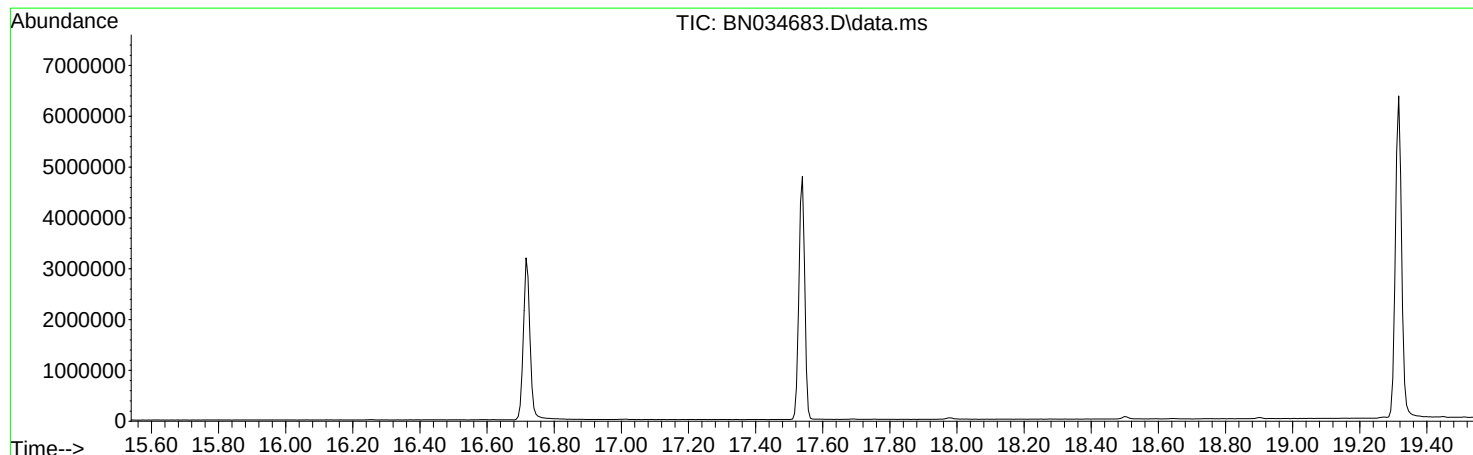

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.1	282114	PASS
68	69	0.00	2	1.7	3908	PASS
69	198	0.00	100	54.4	232312	PASS
70	69	0.00	2	0.5	1275	PASS
127	198	10	80	60.3	257365	PASS
197	198	0.00	2	0.2	1012	PASS
198	198	100	100	100.0	426901	PASS
199	198	5	9	6.5	27752	PASS
275	198	10	60	20.6	88117	PASS
365	198	1	100	2.5	10758	PASS
441	198	0.01	100	7.8	33160	PASS
442	442	50	100	100.0	210005	PASS
443	442	15	24	18.6	39008	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/24/2024	BNA_N	<u>BN034683.D</u>
Compound Name	Response	Retention Time
DDT	1329547	20.563
DDD	11879	20.175
DDE	111	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11990	1341537	0.89

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
Data File : BN034683.D
Acq On : 24 Oct 2024 07:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 24 12:50:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 02:40:52 2024
Response via : Initial Calibration

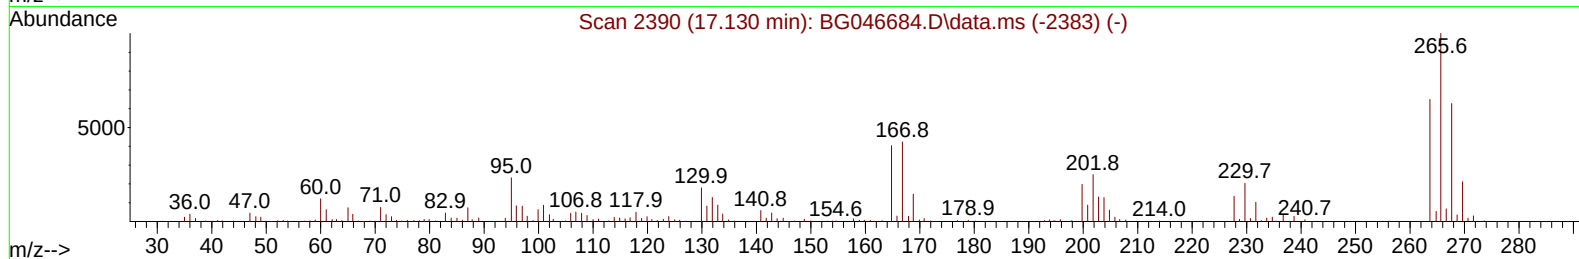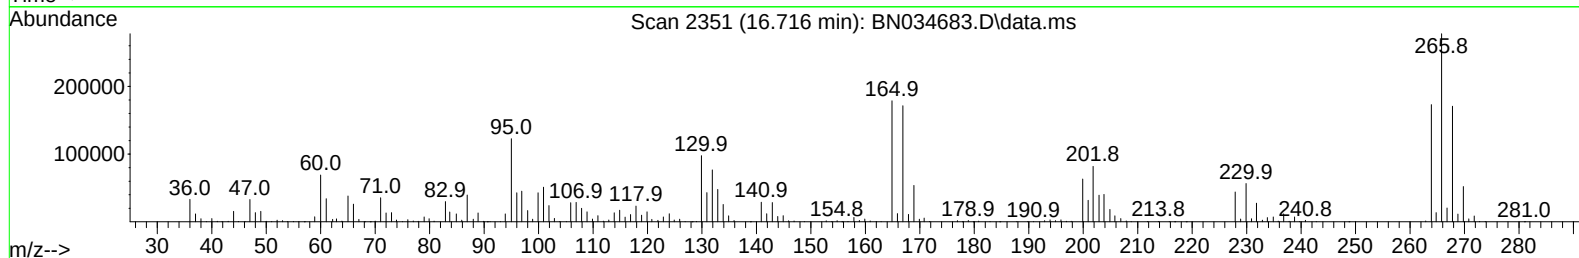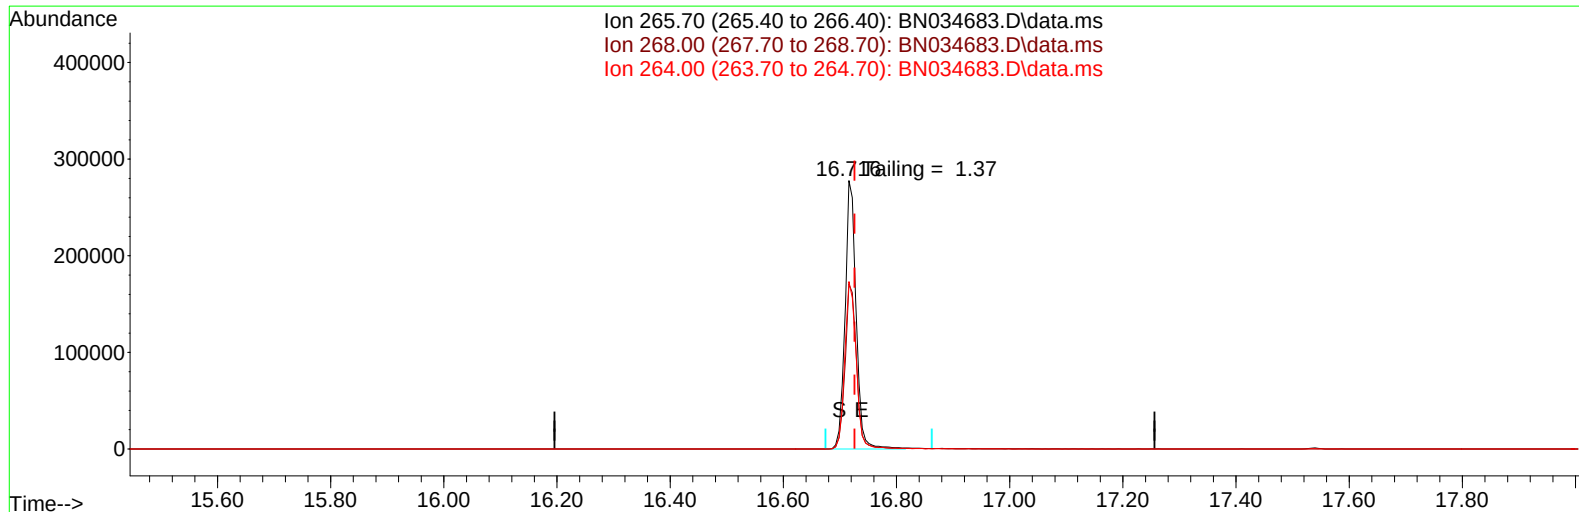

TIC: BN034683.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.010) 17805.12 ng




response 375874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.45
264.00	61.60	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
Data File : BN034683.D
Acq On : 24 Oct 2024 07:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 24 12:50:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 02:40:52 2024
Response via : Initial Calibration

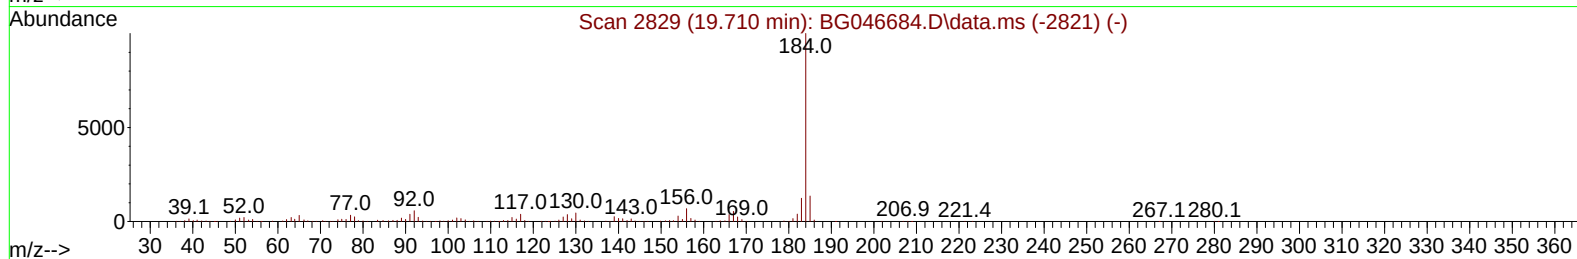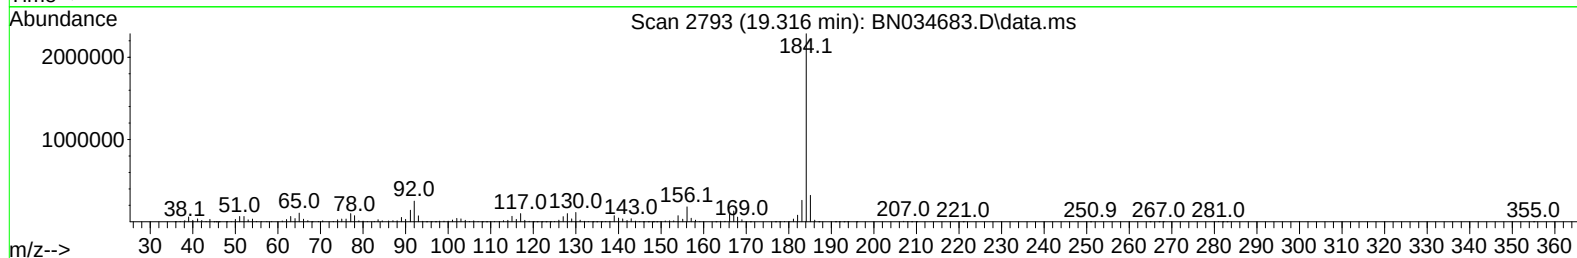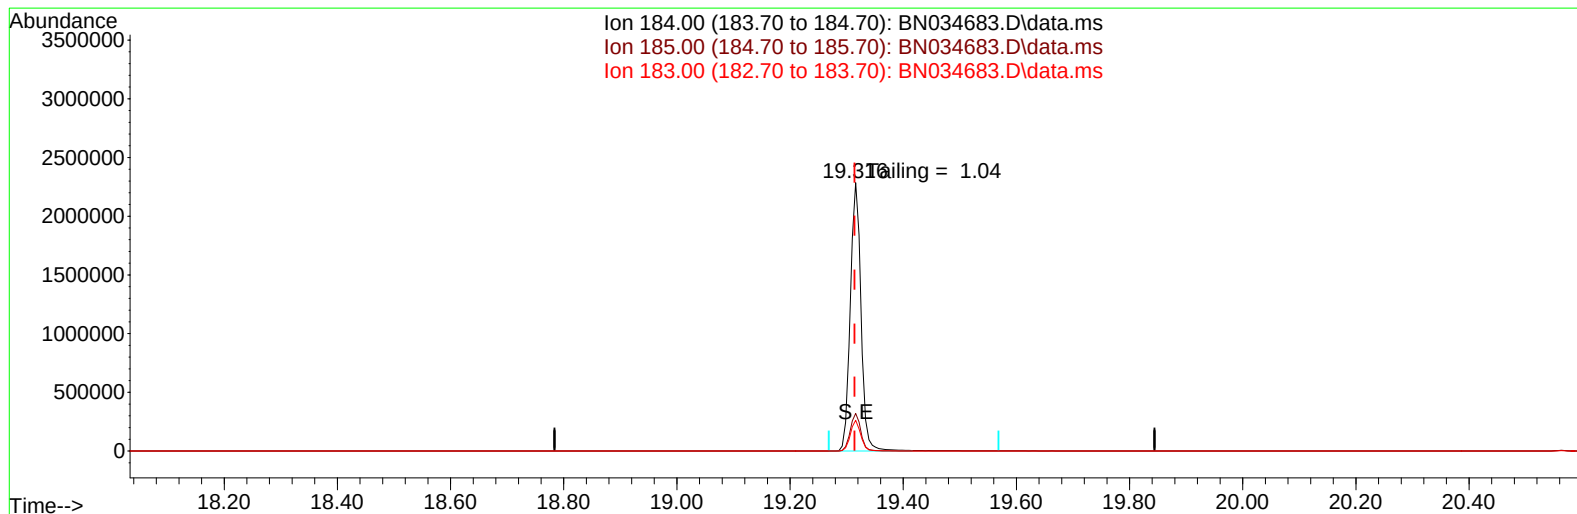

TIC: BN034683.D\data.ms

(77) Benzidine

19.316min (+ 0.002) 0.00 ng

response 3022437

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	11.45
0.00	0.00	0.00