
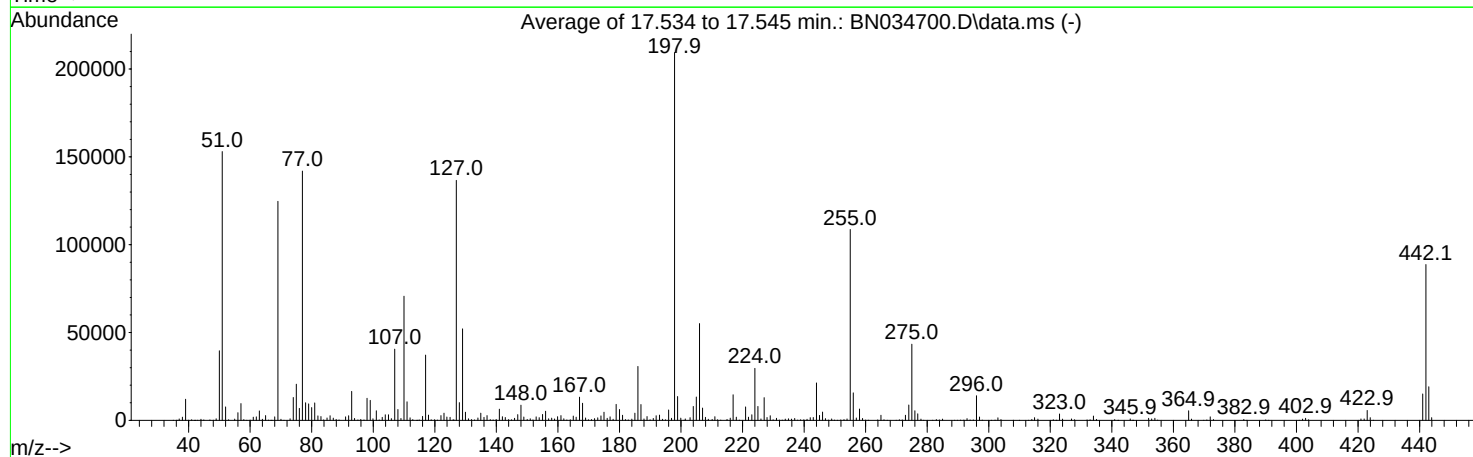


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
Data File : BN034700.D
Acq On : 24 Oct 2024 20:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 24 13:17:02 2024

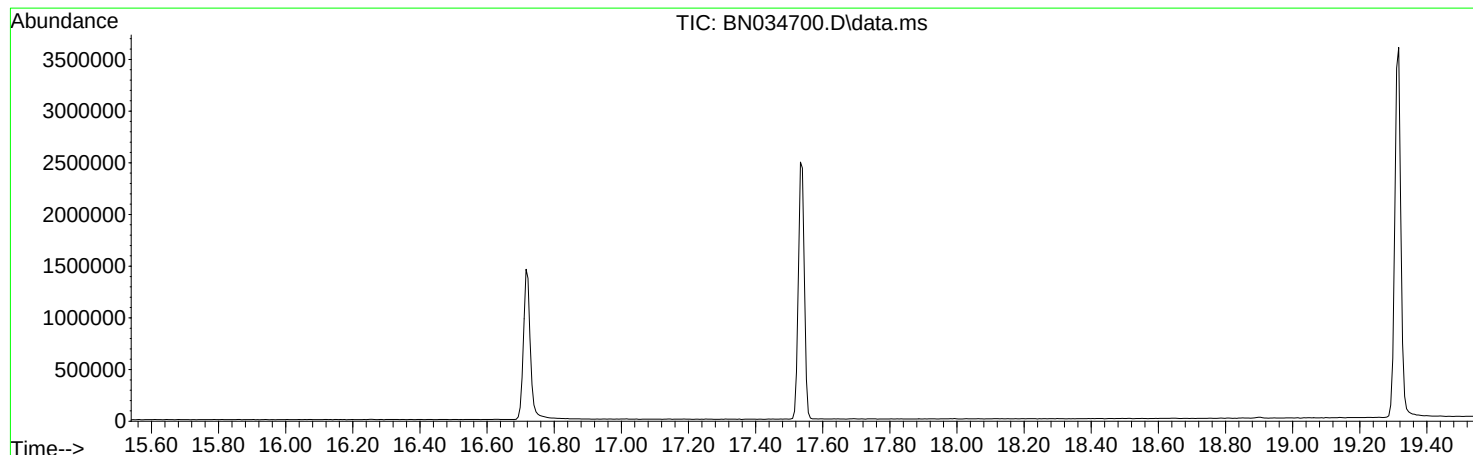

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	73.1	153072	PASS
68	69	0.00	2	1.6	1977	PASS
69	198	0.00	100	59.5	124685	PASS
70	69	0.00	2	0.5	613	PASS
127	198	10	80	65.2	136648	PASS
197	198	0.00	2	0.5	1148	PASS
198	198	100	100	100.0	209429	PASS
199	198	5	9	6.5	13571	PASS
275	198	10	60	20.7	43333	PASS
365	198	1	100	2.6	5435	PASS
441	198	0.01	100	7.2	15057	PASS
442	442	50	100	100.0	88755	PASS
443	442	15	24	21.6	19165	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/24/2024	BNA_N	<u>BN034700.D</u>
Compound Name	Response	Retention Time
DDT	622621	20.557
DDD	5755	20.169
DDE	0	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5755	628376	0.92

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
Data File : BN034700.D
Acq On : 24 Oct 2024 20:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 25 02:24:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 02:24:36 2024
Response via : Initial Calibration

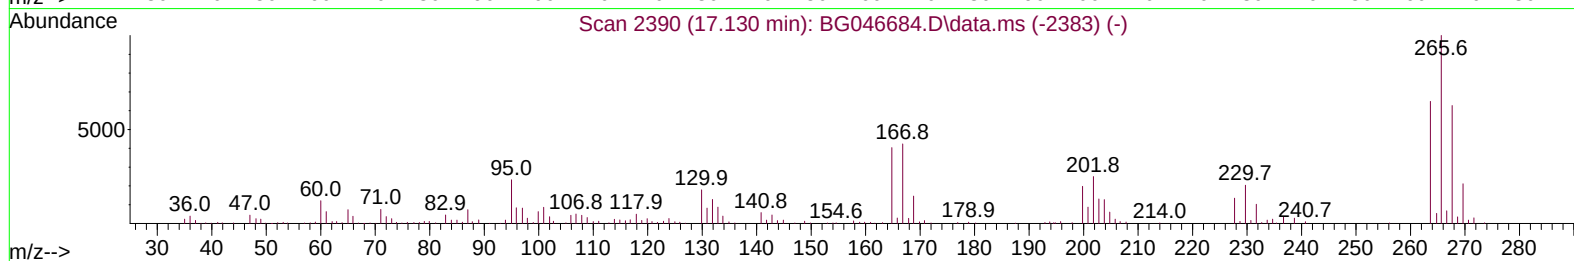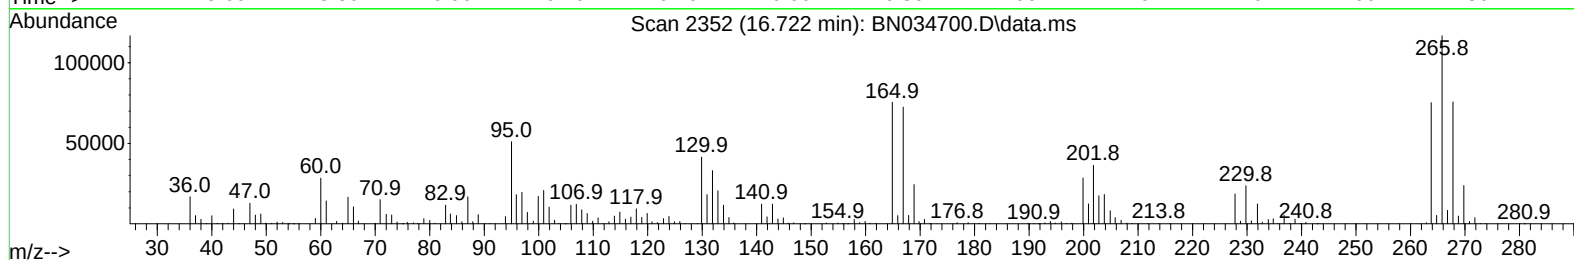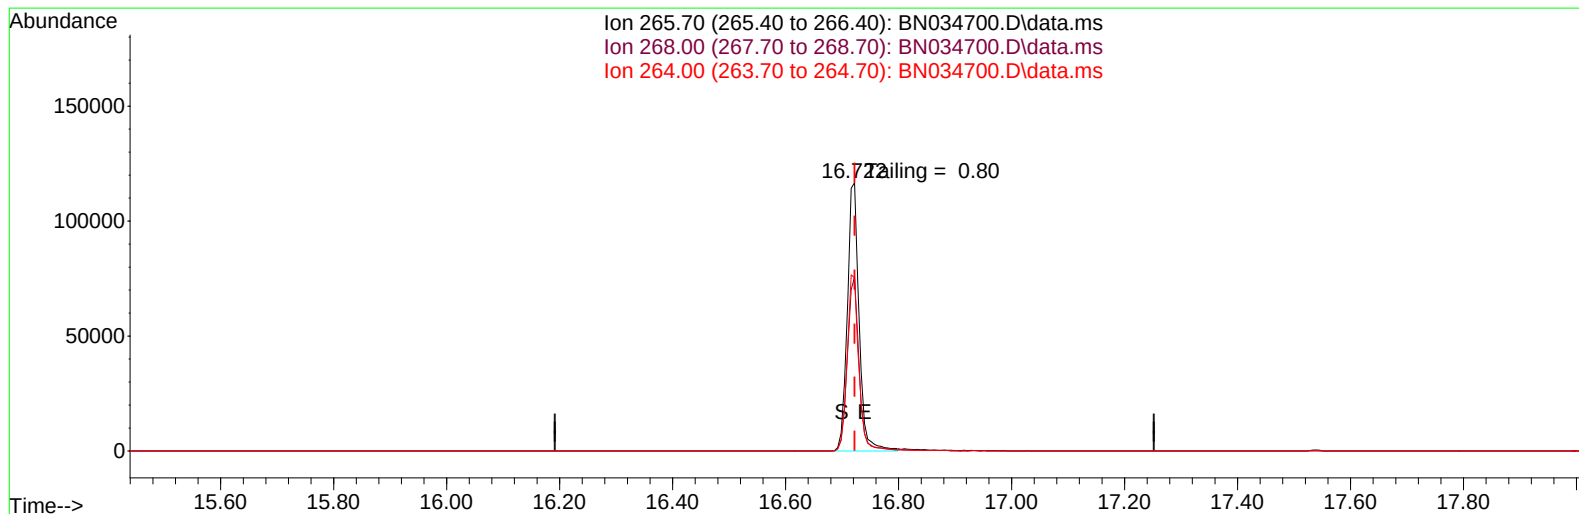

TIC: BN034700.D\data.ms

(70) Pentachlorophenol (C)

16.722min (0.000) 17028.21 ng




response 171184

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.80
264.00	61.60	64.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102424\
Data File : BN034700.D
Acq On : 24 Oct 2024 20:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 25 02:24:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 25 02:24:36 2024
Response via : Initial Calibration

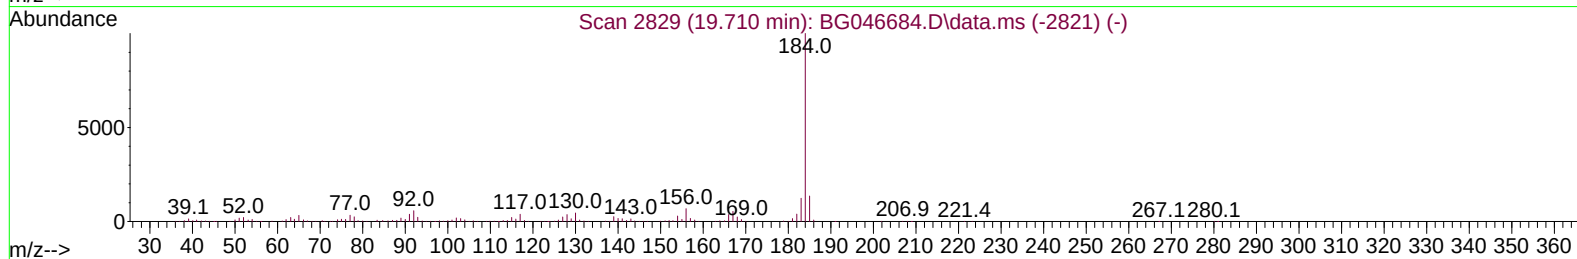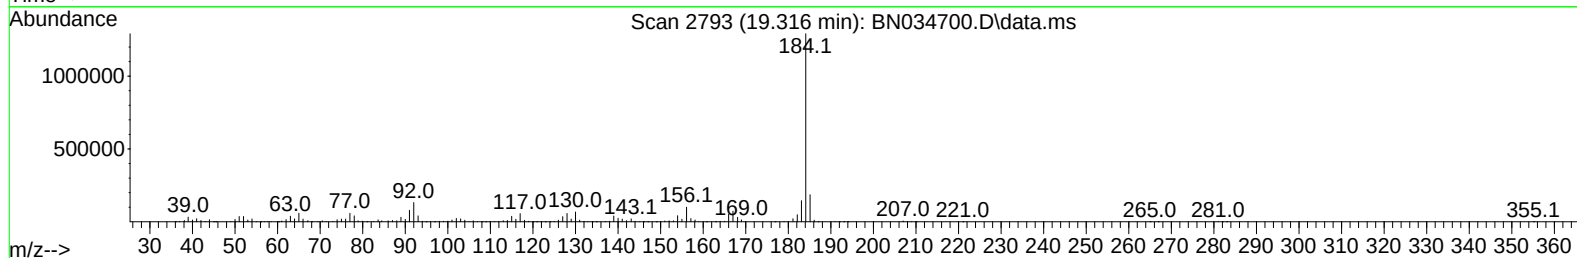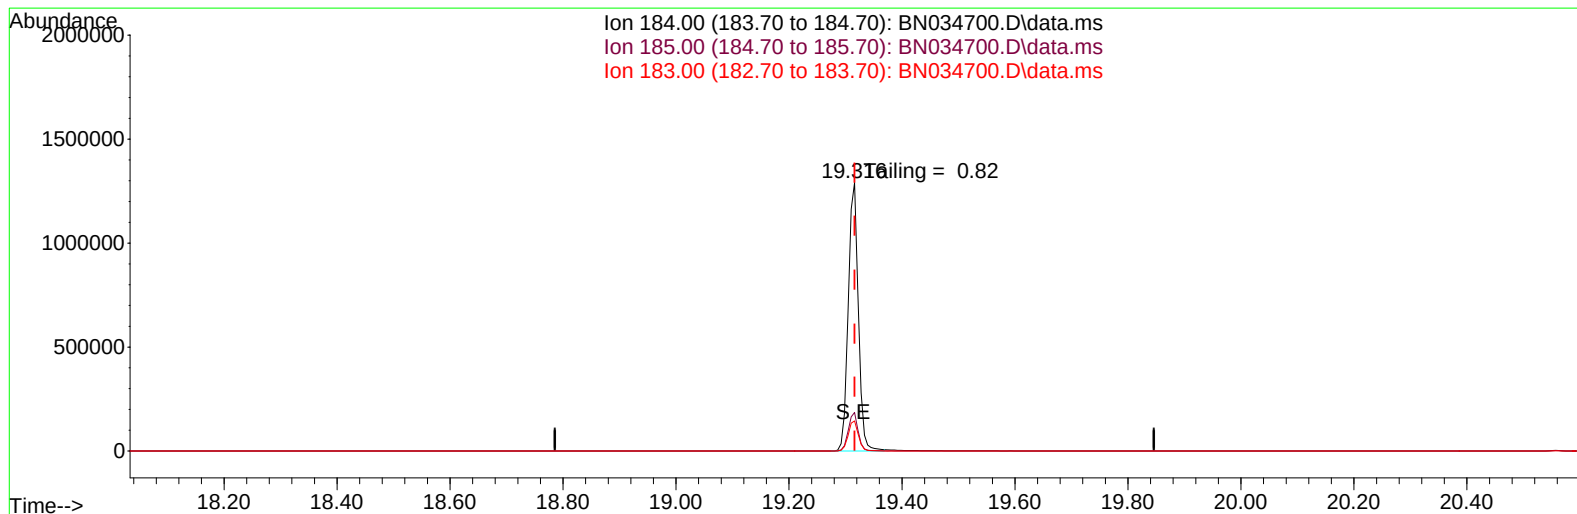

TIC: BN034700.D\data.ms

(77) Benzidine

19.316min (0.000) 0.00 ng

response 1621578

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.38
183.00	13.20	11.24
0.00	0.00	0.00