
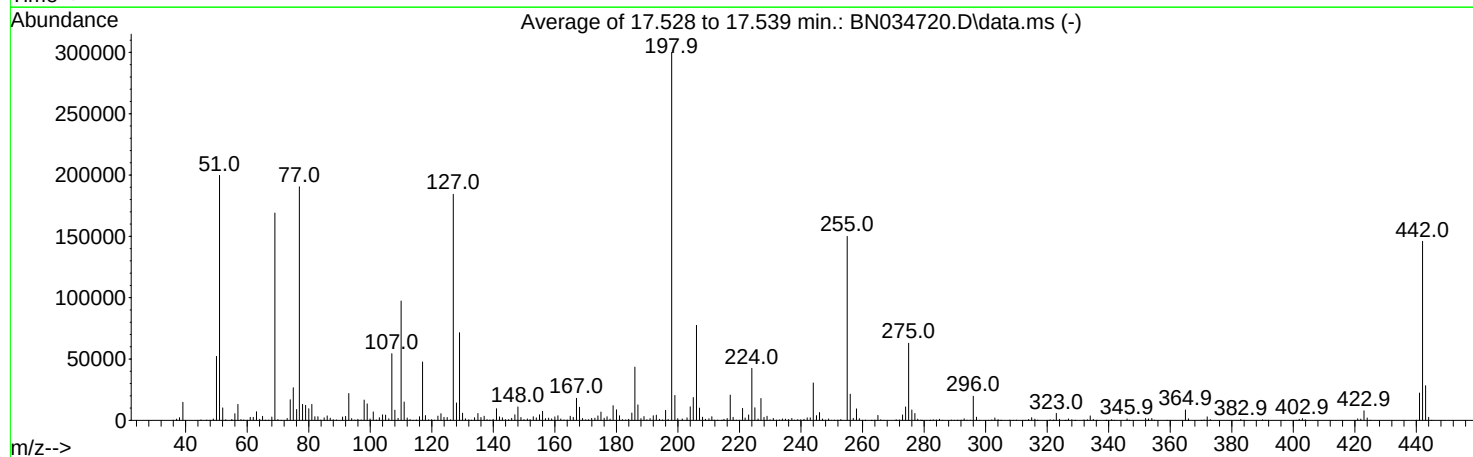


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN102524\  
Data File : BN034720.D  
Acq On : 25 Oct 2024 09:07  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN102424.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Oct 25 22:11:36 2024

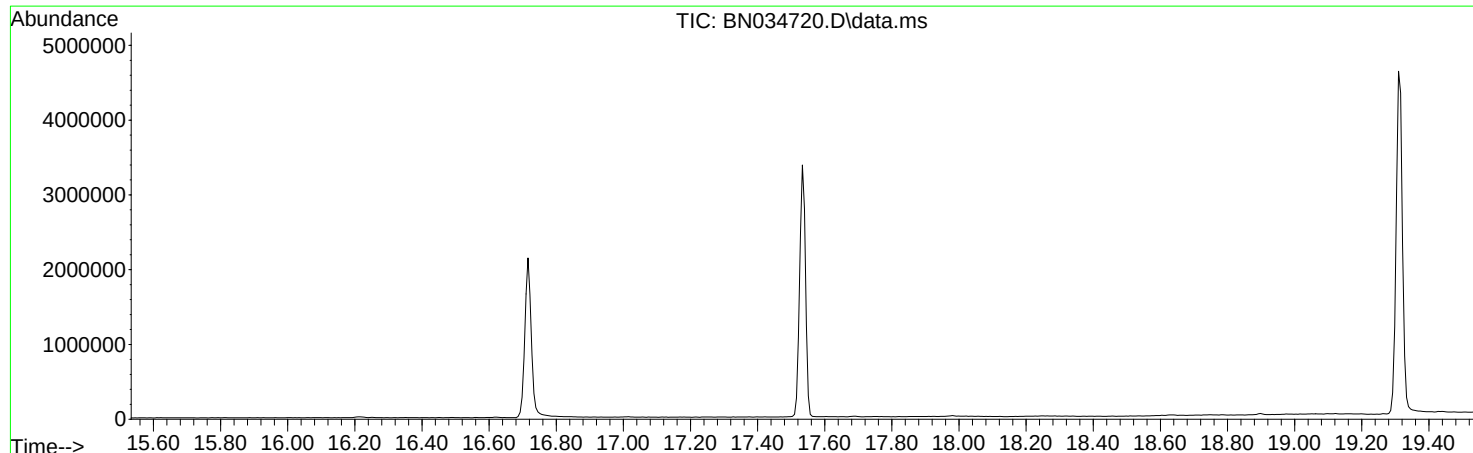

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 66.6         | 199713     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 2696       | PASS                |
| 69             | 198             | 0.00            | 100             | 56.4         | 169054     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 594        | PASS                |
| 127            | 198             | 10              | 80              | 61.5         | 184363     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 764        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 299904     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 20312      | PASS                |
| 275            | 198             | 10              | 60              | 21.0         | 62957      | PASS                |
| 365            | 198             | 1               | 100             | 2.8          | 8432       | PASS                |
| 441            | 198             | 0.01            | 100             | 7.4          | 22267      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 145949     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 28343      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/25/2024    | BNA_N            | <u>BN034720.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 888185           | 20.557             |
| DDD           | 14092            | 20.169             |
| DDE           | 315              | 19.61              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 14407         | 902592           | 1.60               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN102524\  
Data File : BN034720.D  
Acq On : 25 Oct 2024 09:07  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Oct 25 14:47:07 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 25 02:24:36 2024  
Response via : Initial Calibration

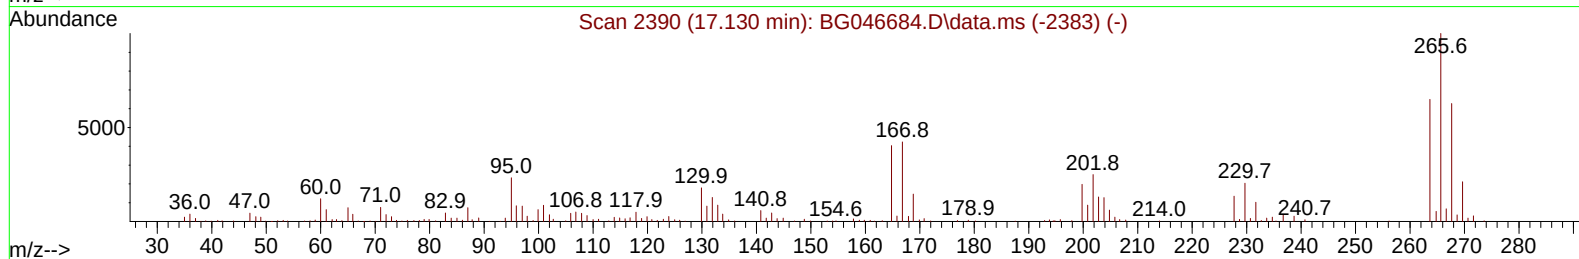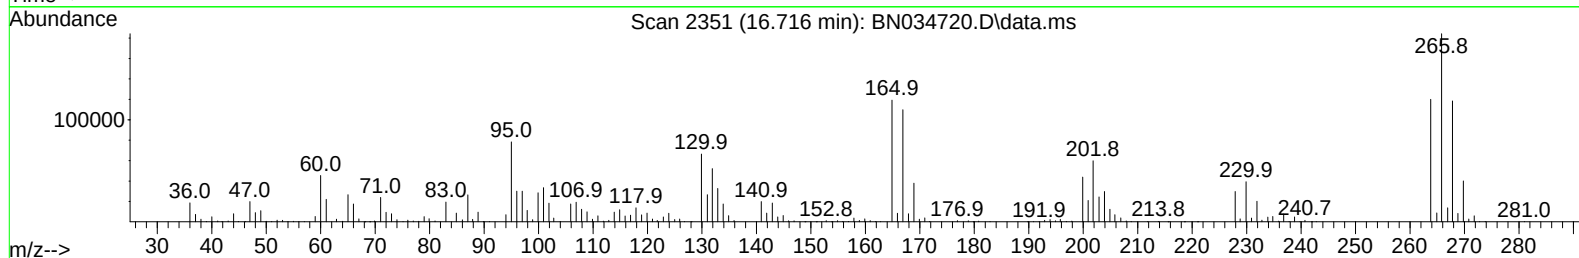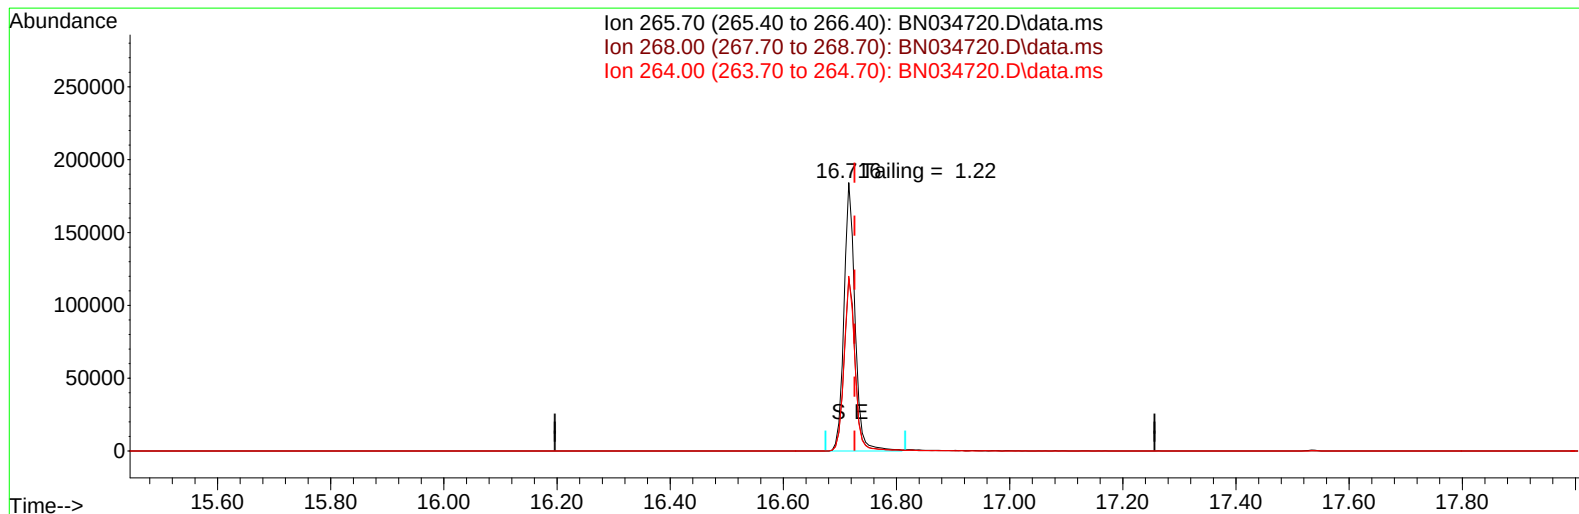

TIC: BN034720.D\data.ms

**(70) Pentachlorophenol (C)**

16.716min (-0.010) 16177.27 ng




response 249213

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.29  |
| 264.00 | 61.60  | 65.12  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN102524\  
Data File : BN034720.D  
Acq On : 25 Oct 2024 09:07  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Oct 25 14:47:07 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 25 02:24:36 2024  
Response via : Initial Calibration

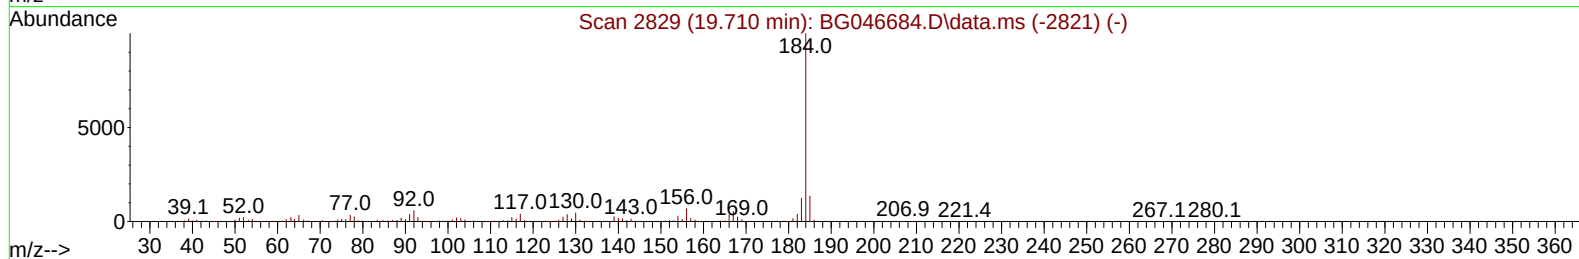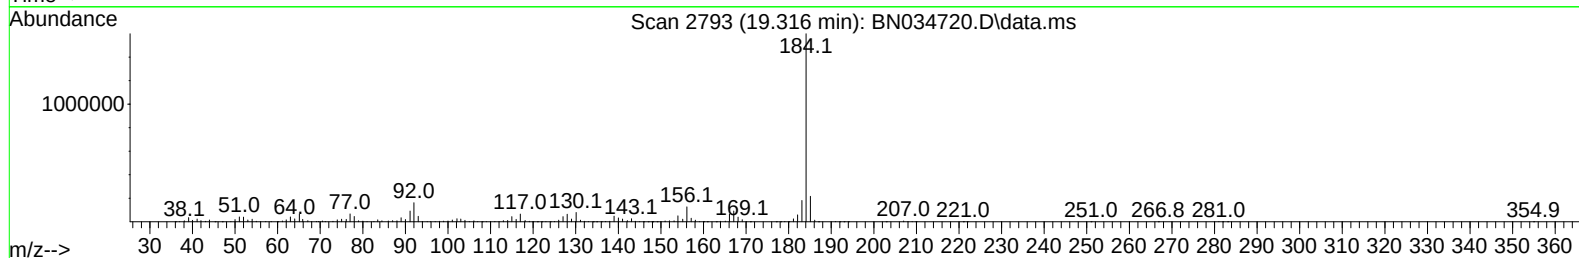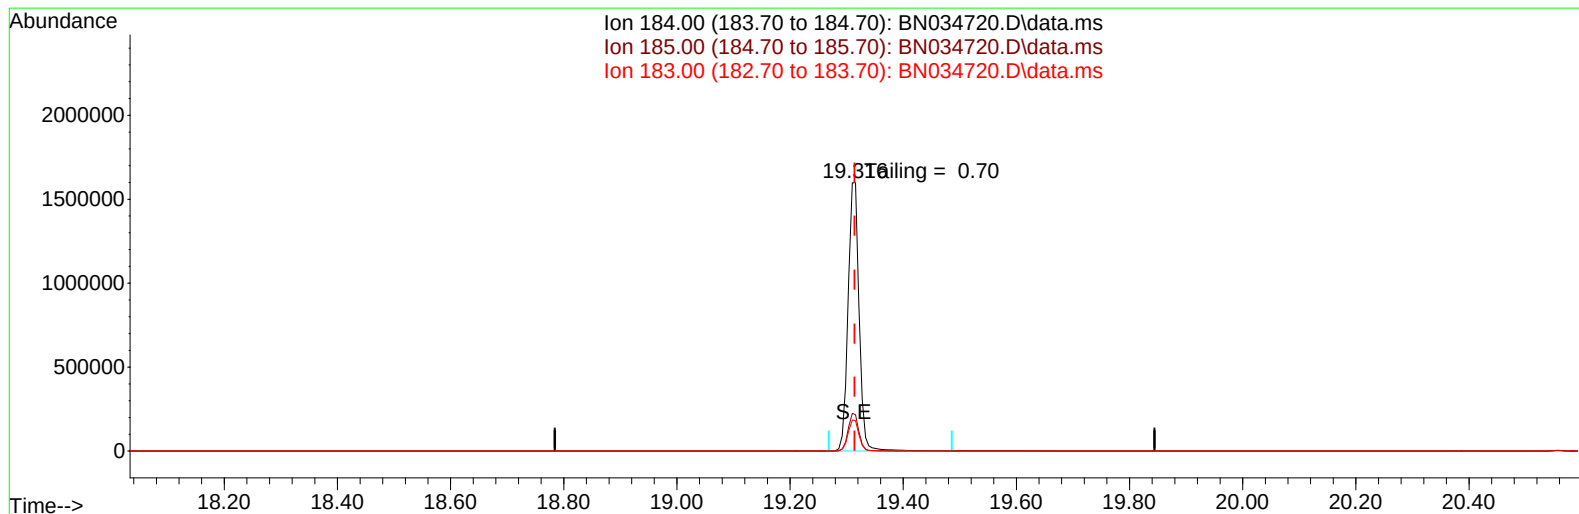

TIC: BN034720.D\data.ms

**(77) Benzidine**

**19.316min (+ 0.002) 0.00 ng**

**response 2170006**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.53  |
| 183.00 | 13.20  | 11.36  |
| 0.00   | 0.00   | 0.00   |