

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102624\
 Data File : PL092637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2024 15:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/28/2024
 Supervised By : Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 22:37:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 17:09:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.779	53746660	59899848	19.952m	21.567m
28)	SA Decachlor...	9.061	7.919	44803860	64265381	22.058	24.389

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102624\
Data File : PL092637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2024 15:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/28/2024
Supervised By : Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 22:37:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 17:09:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

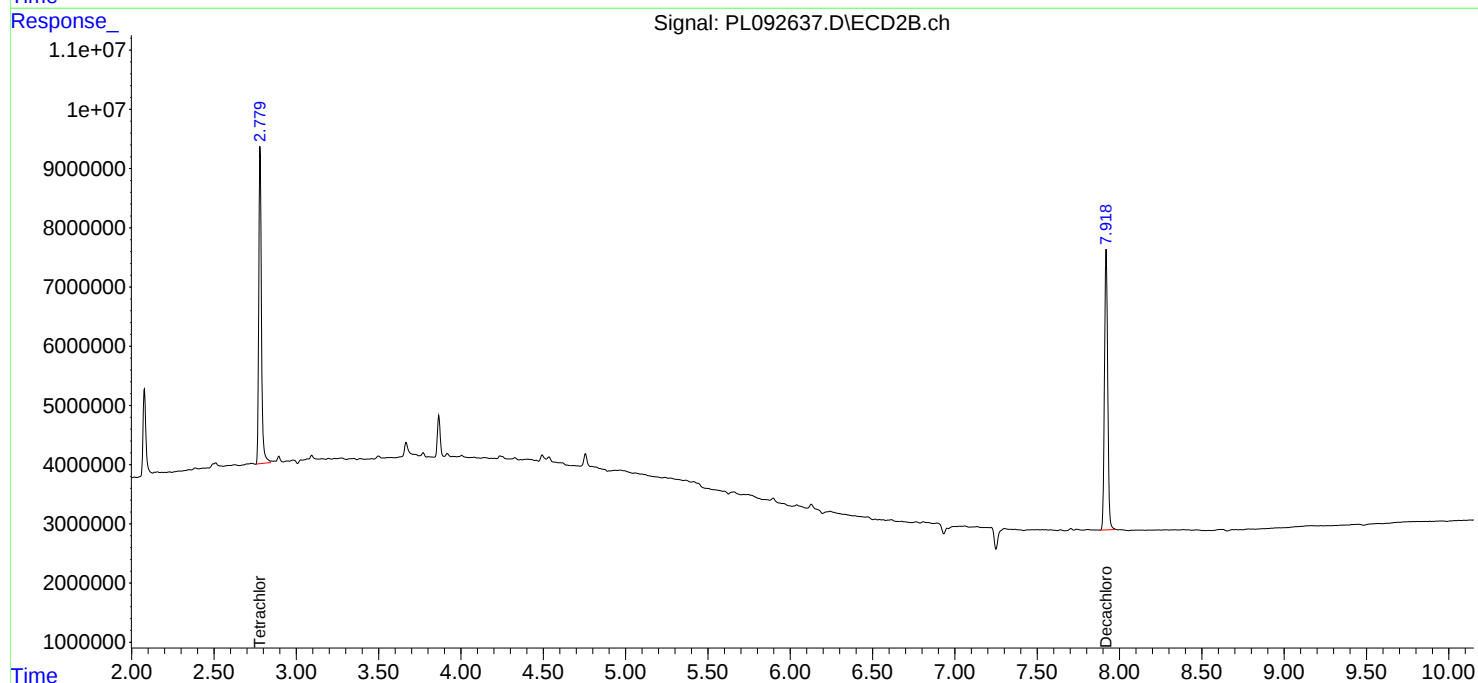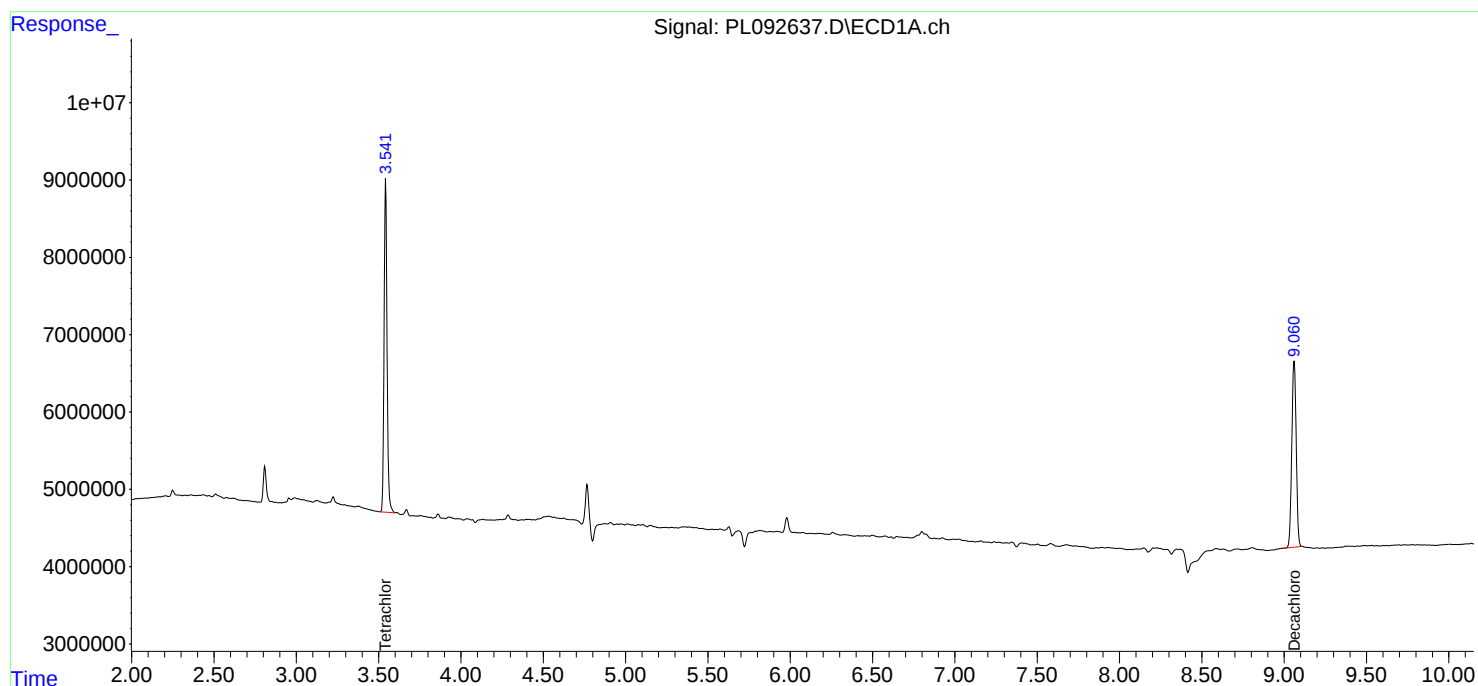

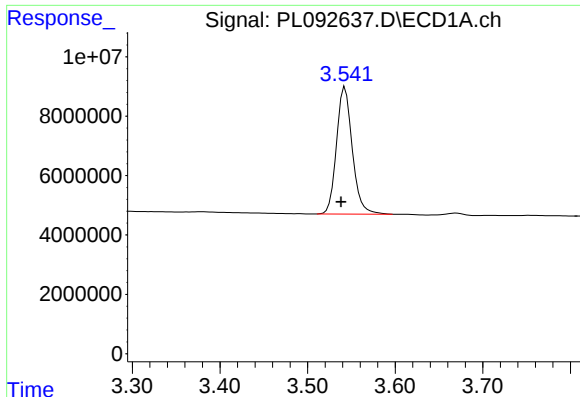


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.003 min
Response: 53746660
Conc: 19.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

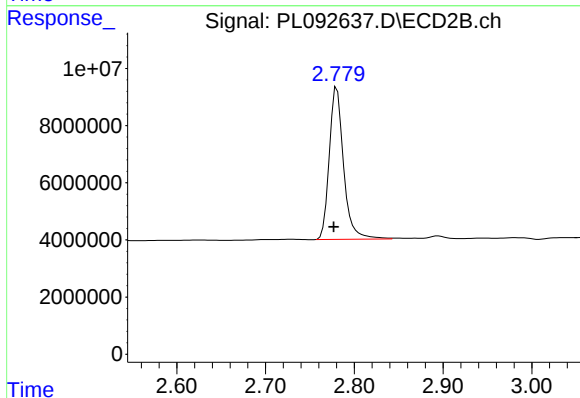


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.002 min
Response: 59899848
Conc: 21.57 ng/ml m

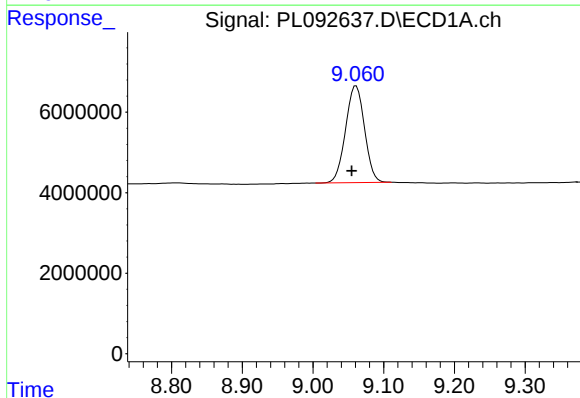

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.006 min
Response: 44803860
Conc: 22.06 ng/ml

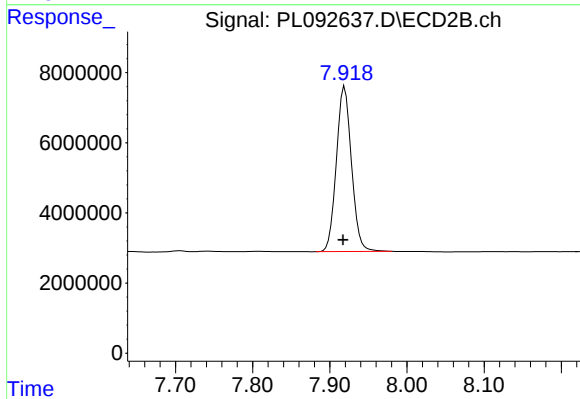

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: 0.002 min
Response: 64265381
Conc: 24.39 ng/ml