
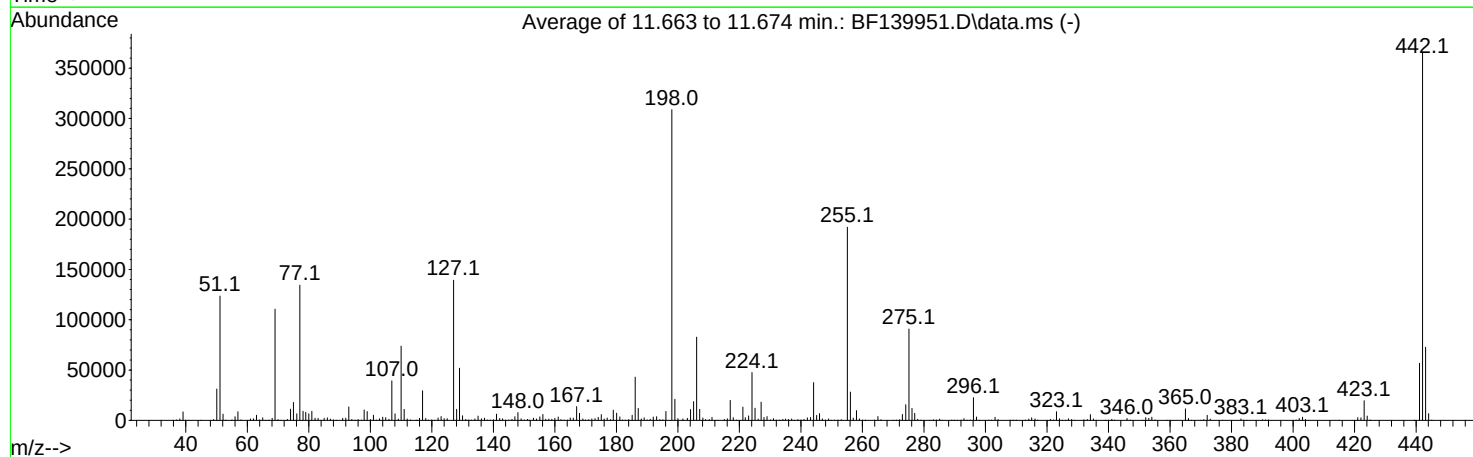


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102324\
Data File : BF139951.D
Acq On : 23 Oct 2024 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

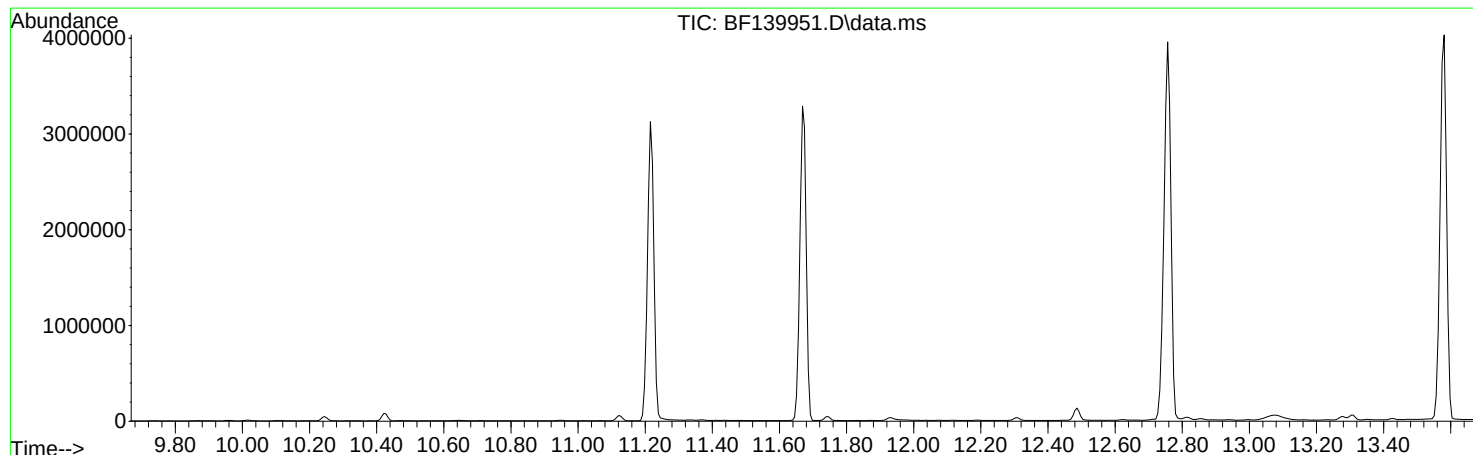

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	123525	PASS
68	69	0.00	2	1.8	2014	PASS
69	198	0.00	100	35.8	110510	PASS
70	69	0.00	2	0.7	742	PASS
127	198	10	80	45.1	139315	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	308736	PASS
199	198	5	9	6.8	21040	PASS
275	198	10	60	29.4	90893	PASS
365	198	1	100	3.7	11511	PASS
441	198	0.01	100	18.4	56747	PASS
442	442	50	100	100.0	365589	PASS
443	442	15	24	19.9	72741	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/23/2024	BNA_F	<u>BF139951.D</u>
Compound Name	Response	Retention Time
DDT	1114000	13.58
DDD	17745	13.31
DDE	1145	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18890	1132890	1.67

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102324\
Data File : BF139951.D
Acq On : 23 Oct 2024 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 23 16:03:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

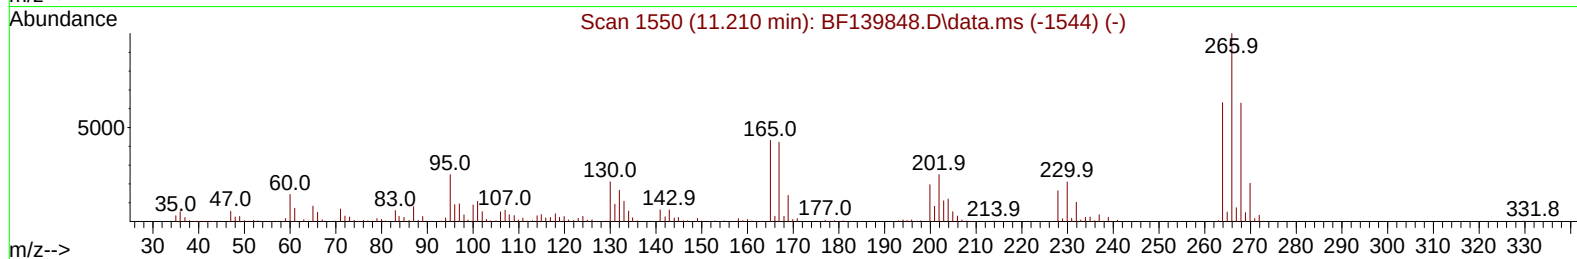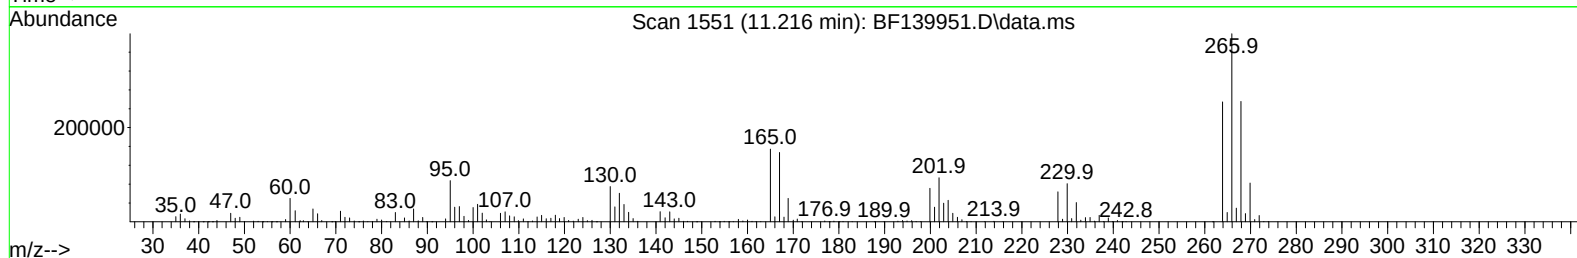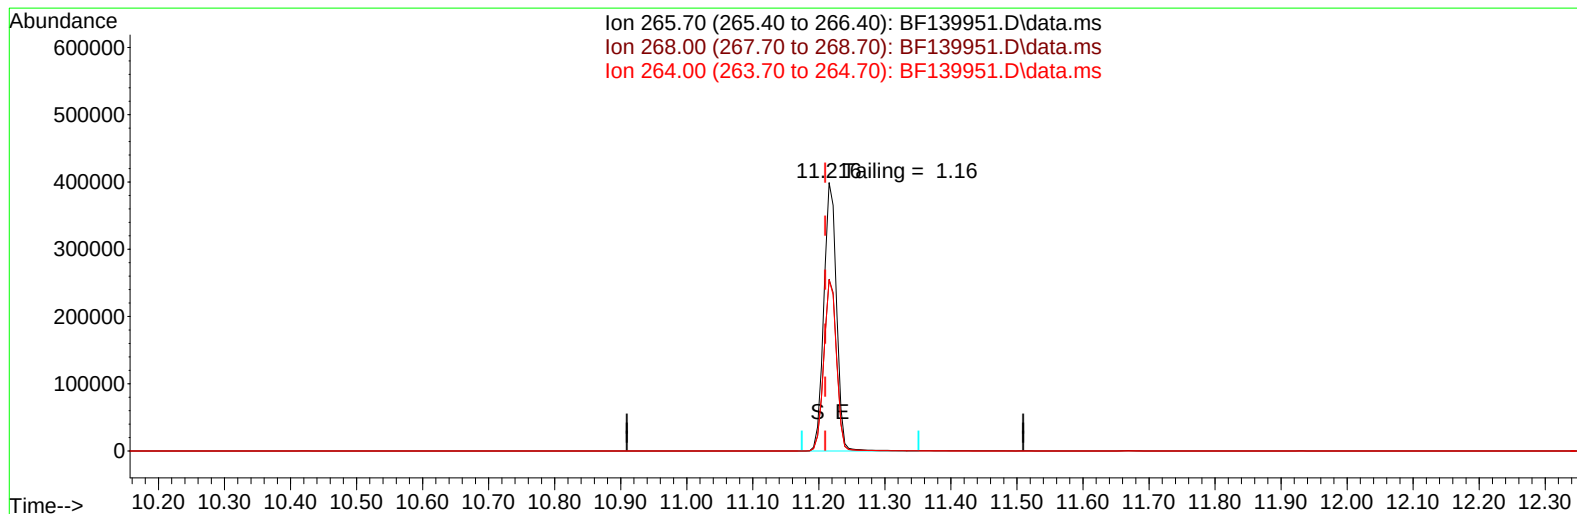

TIC: BF139951.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 71911.08 ng




response 533470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.99
264.00	63.20	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102324\
Data File : BF139951.D
Acq On : 23 Oct 2024 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 23 16:03:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

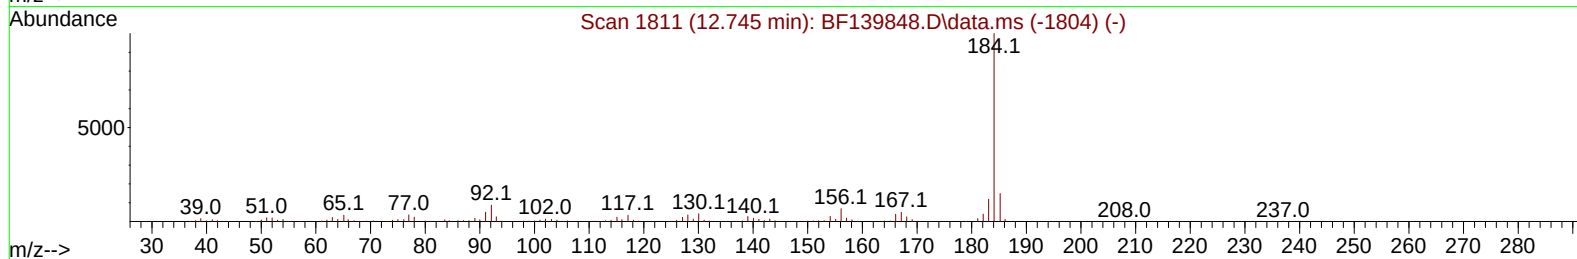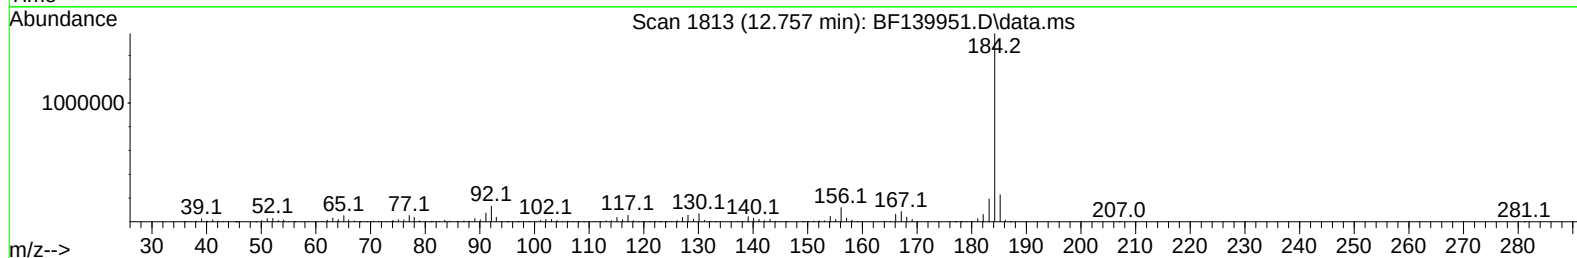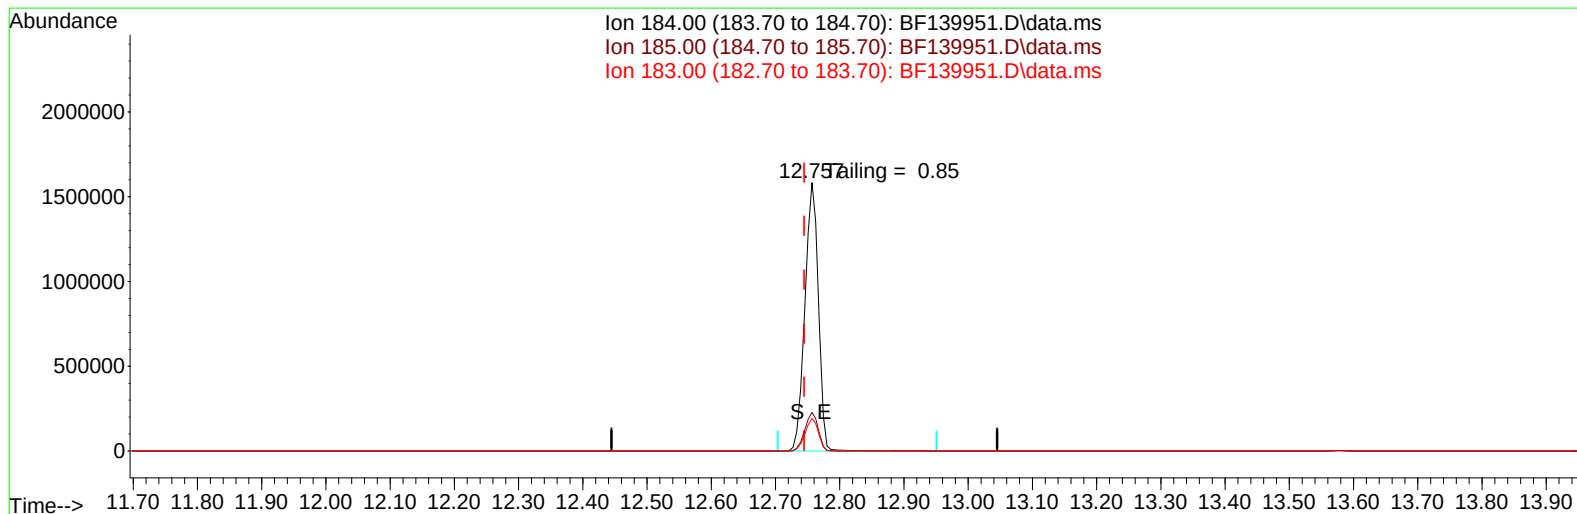

TIC: BF139951.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 73198.86 ng

response 2307374

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.40
183.00	11.80	12.12
0.00	0.00	0.00