
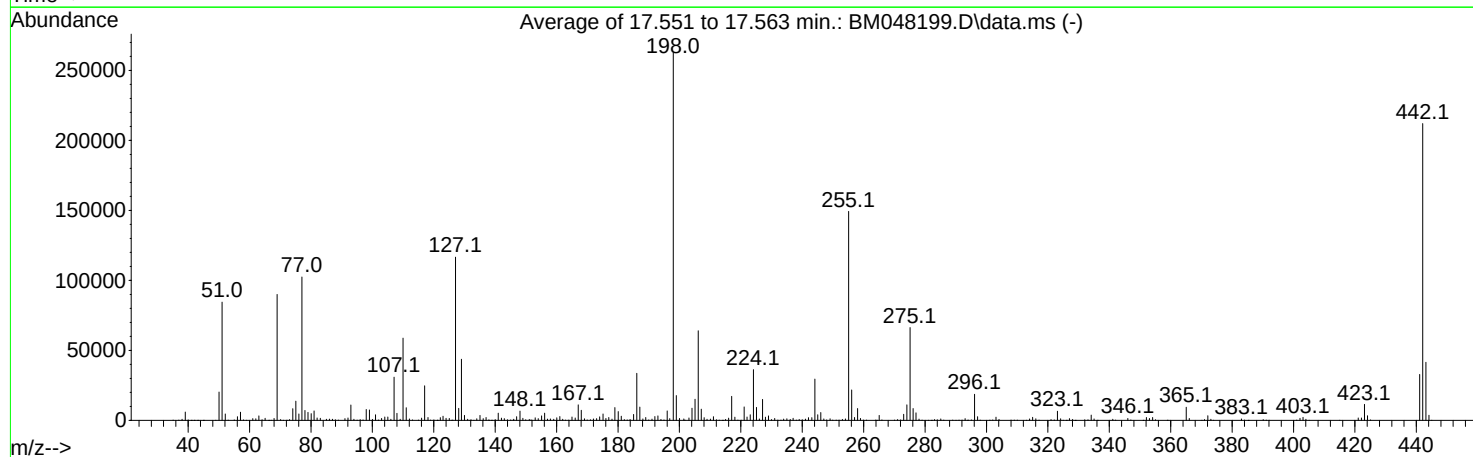


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102324\
Data File : BM048199.D
Acq On : 23 Oct 2024 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 23 18:21:59 2024

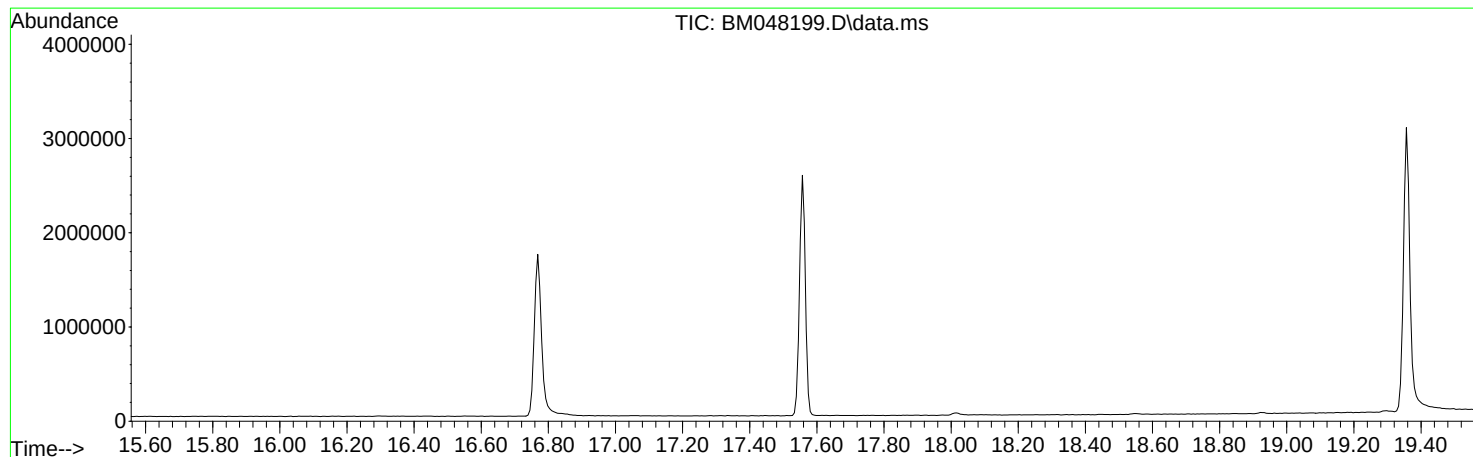


AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	84540	PASS
68	69	0.00	2	1.6	1406	PASS
69	198	0.00	100	34.2	89921	PASS
70	69	0.00	2	0.7	587	PASS
127	198	10	80	44.4	116637	PASS
197	198	0.00	2	0.5	1321	PASS
198	198	100	100	100.0	262784	PASS
199	198	5	9	6.8	17767	PASS
275	198	10	60	25.2	66333	PASS
365	198	1	100	3.6	9406	PASS
441	198	0.01	100	12.5	32765	PASS
442	442	50	100	100.0	211989	PASS
443	442	15	24	19.6	41467	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102324\
Data File : BM048199.D
Acq On : 23 Oct 2024 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 23 14:47:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 13:43:53 2024
Response via : Initial Calibration

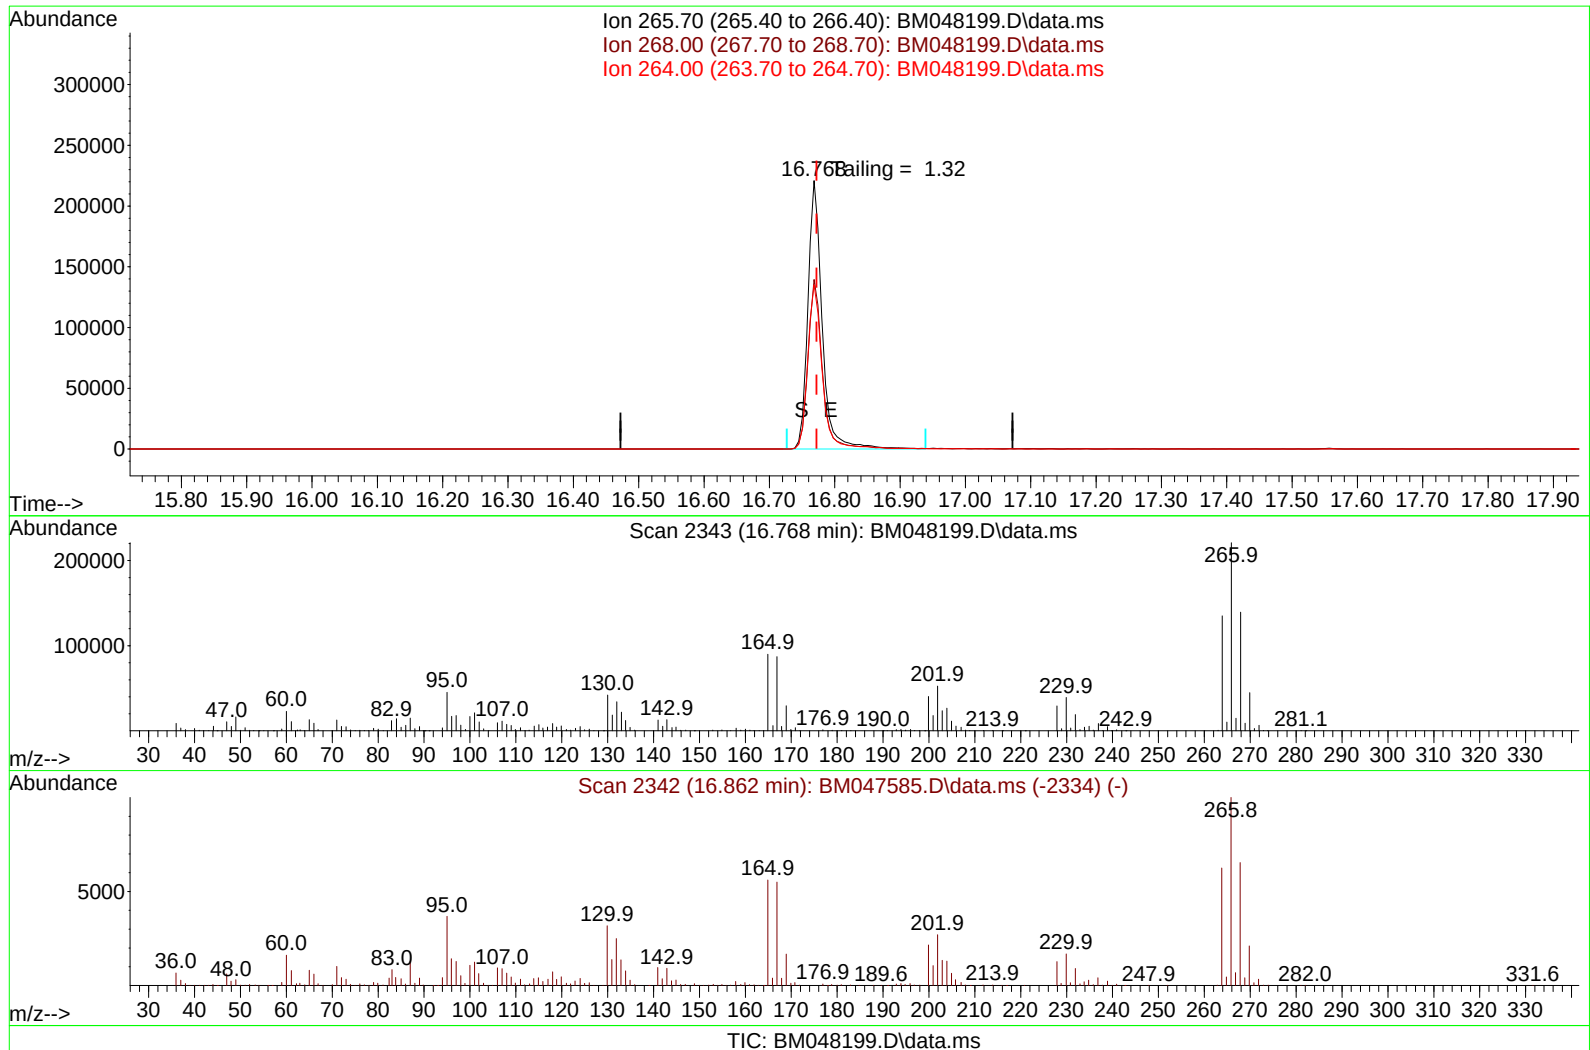

(70) Pentachlorophenol (C)

16.768min (-0.004) 0.00 ng




response 336927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.12
264.00	62.50	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102324\
Data File : BM048199.D
Acq On : 23 Oct 2024 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 23 14:47:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 13:43:53 2024
Response via : Initial Calibration

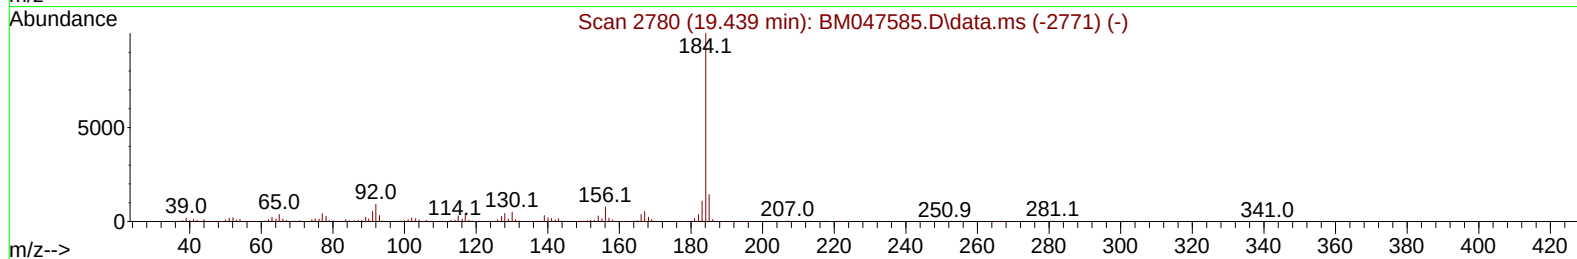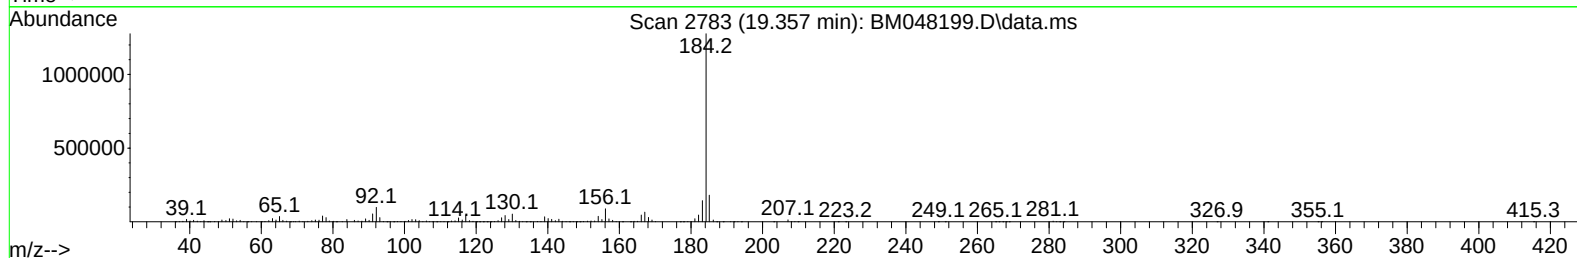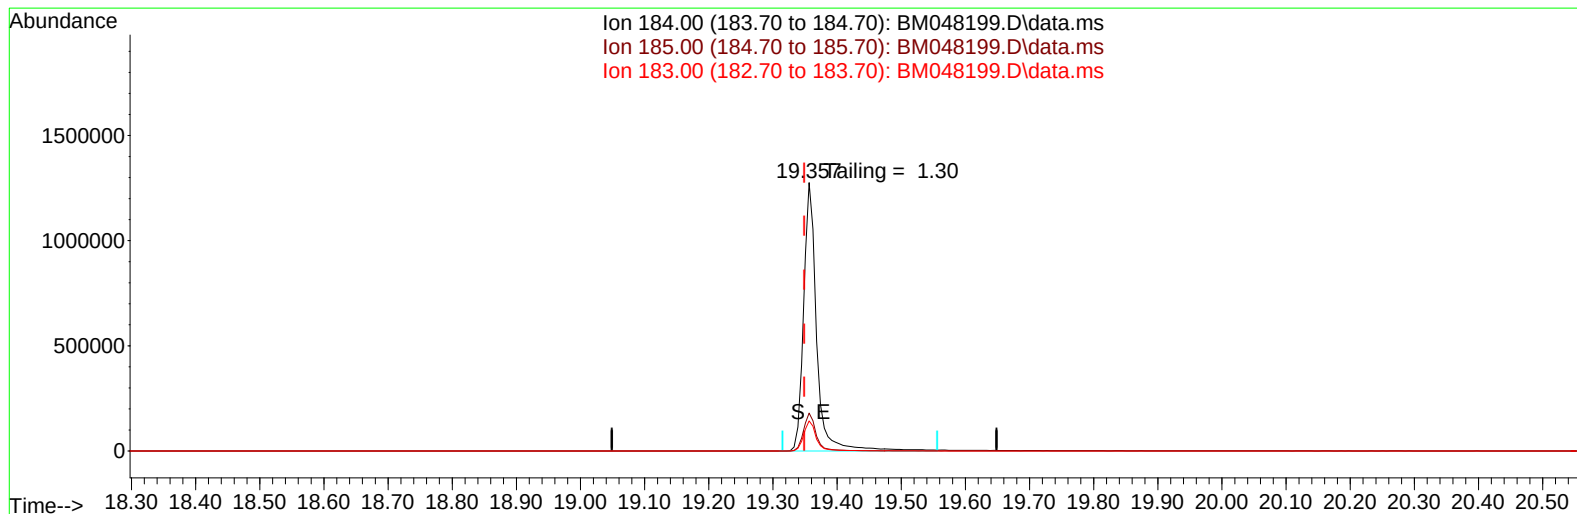

TIC: BM048199.D\data.ms

(77) Benzidine

19.357min (+ 0.008) 0.00 ng

response 1816071

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.15
183.00	10.90	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/23/2024	BNA_M	<u>BM048199.D</u>
Compound Name	Response	Retention Time
DDT	917513	20.586
DDD	9873	20.203
DDE	0	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9873	927386	1.06

Instrument :
BNA_M
ClientSampleId :
DFTPP