


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
Data File : BM048210.D
Acq On : 24 Oct 2024 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 23 18:21:59 2024

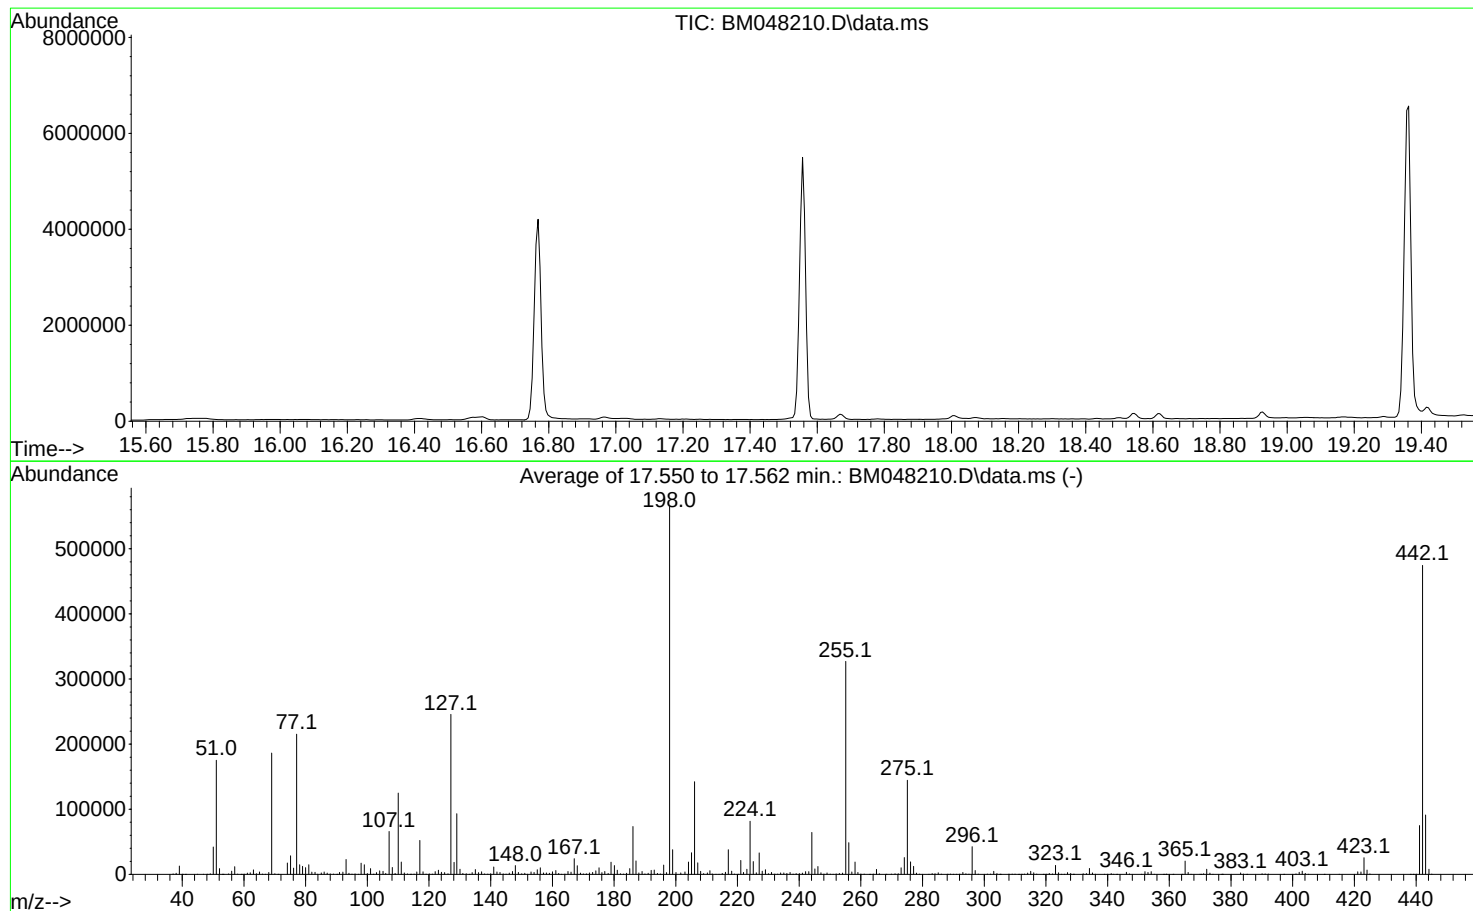




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	175247	PASS
68	69	0.00	2	1.5	2851	PASS
69	198	0.00	100	33.0	186183	PASS
70	69	0.00	2	0.6	1071	PASS
127	198	10	80	43.5	245632	PASS
197	198	0.00	2	0.5	2701	PASS
198	198	100	100	100.0	564949	PASS
199	198	5	9	6.7	37907	PASS
275	198	10	60	25.6	144432	PASS
365	198	1	100	3.6	20424	PASS
441	198	0.01	100	13.3	75067	PASS
442	442	50	100	100.0	474603	PASS
443	442	15	24	19.2	91077	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
Data File : BM048210.D
Acq On : 24 Oct 2024 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 24 12:20:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 18:21:59 2024
Response via : Initial Calibration

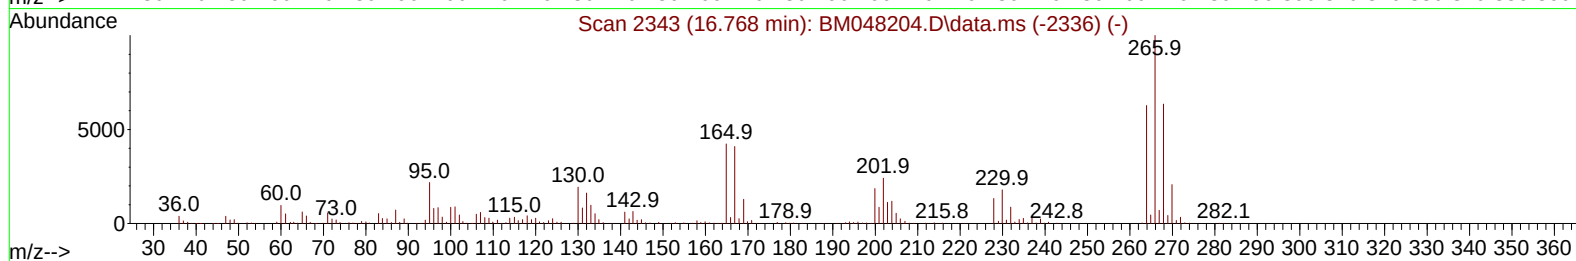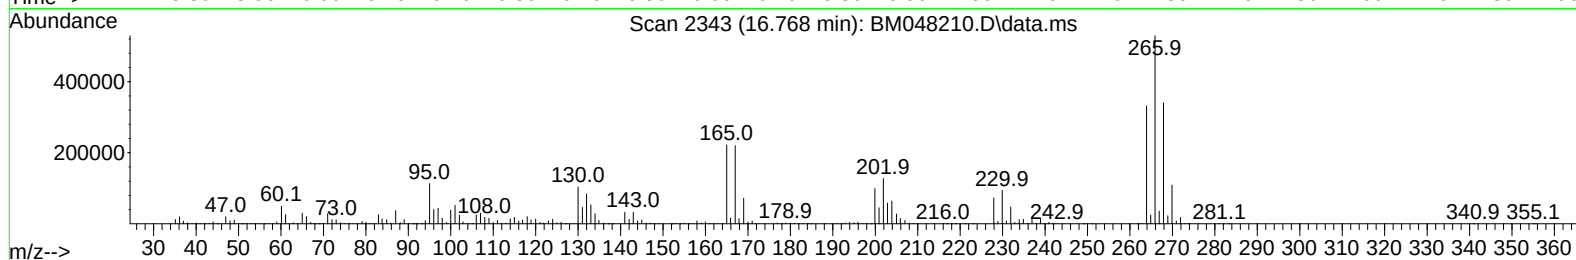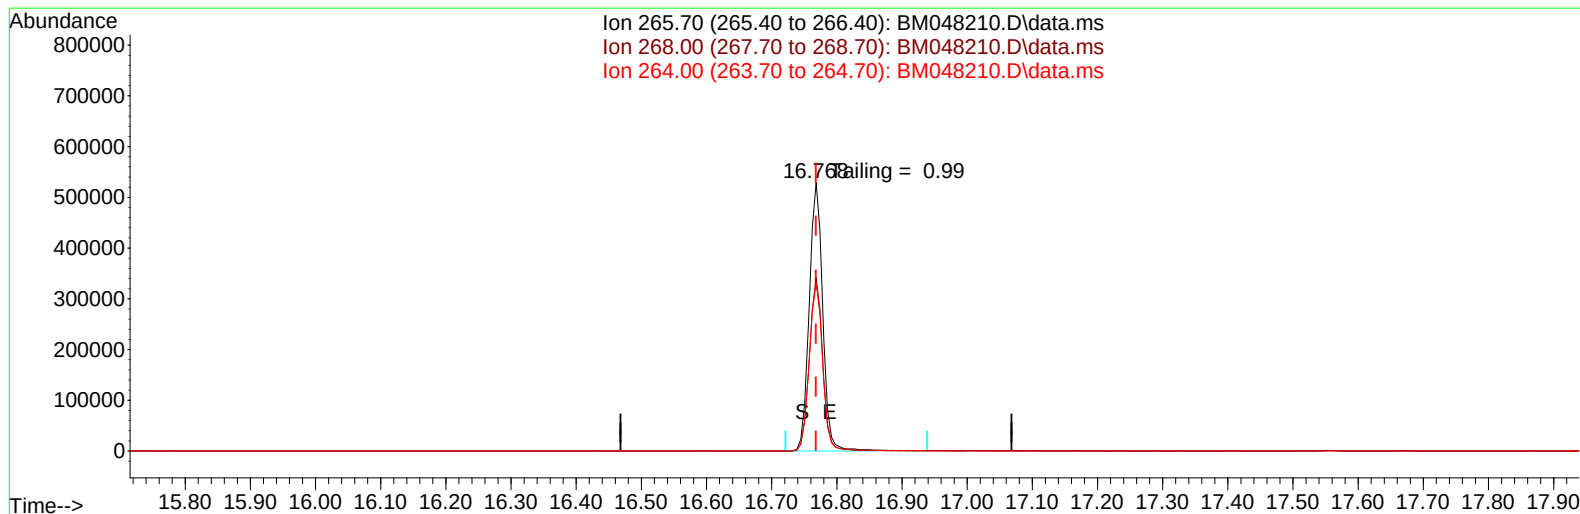

TIC: BM048210.D\data.ms

(70) Pentachlorophenol (C)

16.768min (-0.000) 92717.46 ng




response 764974

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.34
264.00	62.70	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
Data File : BM048210.D
Acq On : 24 Oct 2024 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 24 12:20:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 18:21:59 2024
Response via : Initial Calibration

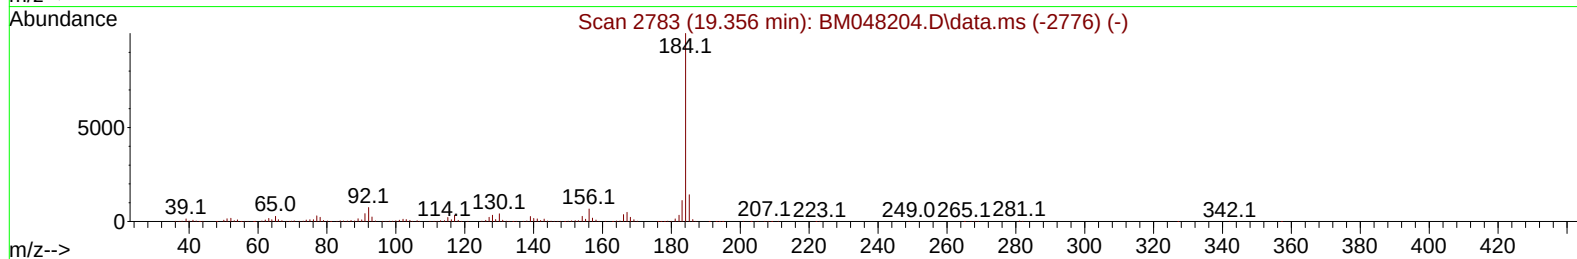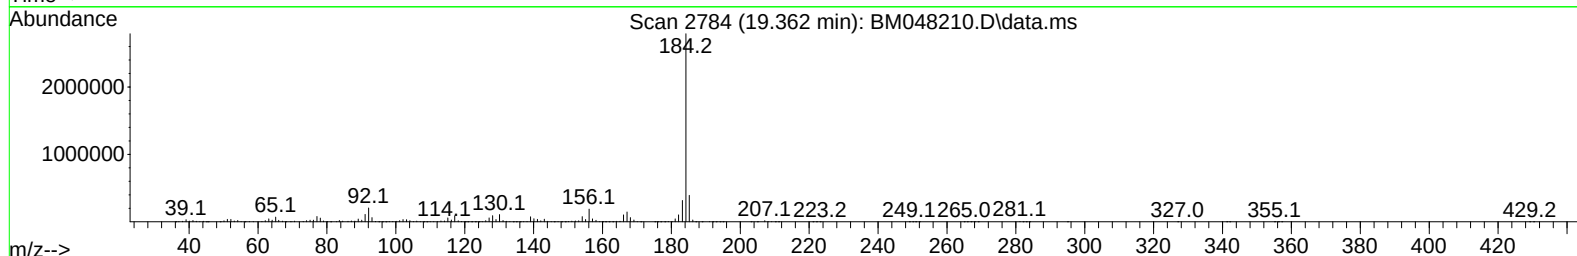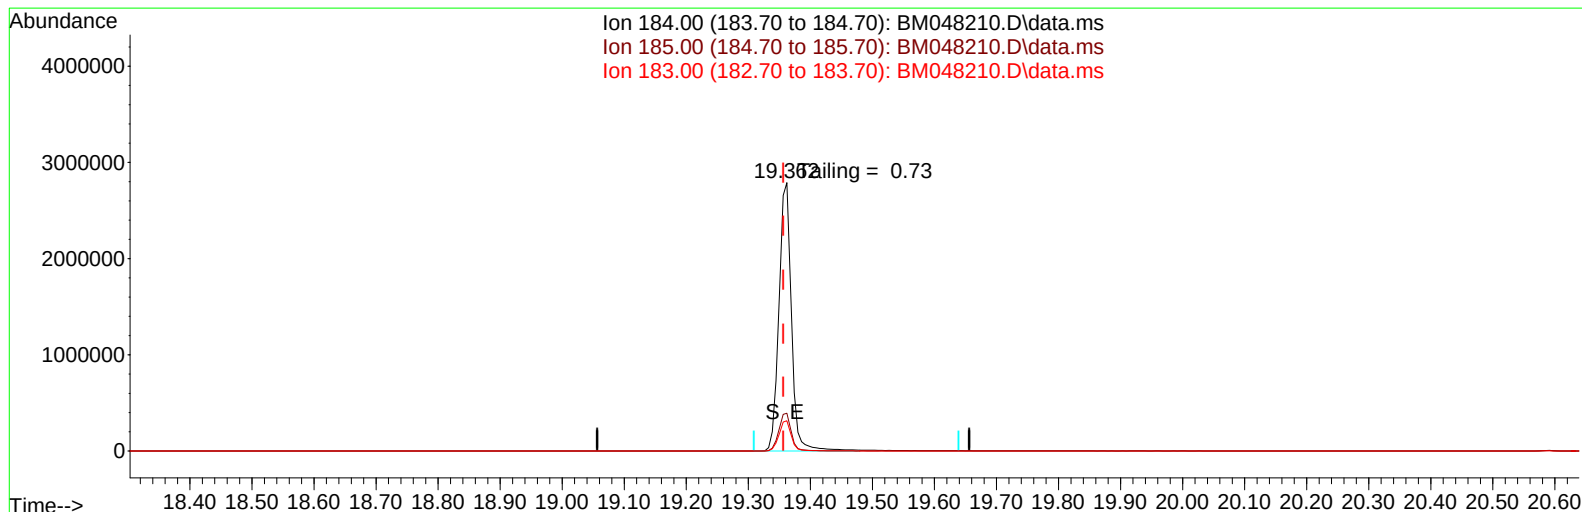

TIC: BM048210.D\data.ms

(77) Benzidine

19.362min (+ 0.006) 54520.09 ng

response 3968464

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.08
183.00	11.20	11.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/24/2024	BNA_M	<u>BM048210.D</u>
Compound Name	Response	Retention Time
DDT	2000528	20.591
DDD	38402	20.15
DDE	2130	19.644
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40532	2041060	1.99

Instrument :
BNA_M
ClientSampleId :
DFTPP