


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048227.D
Acq On : 25 Oct 2024 08:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 23 18:21:59 2024

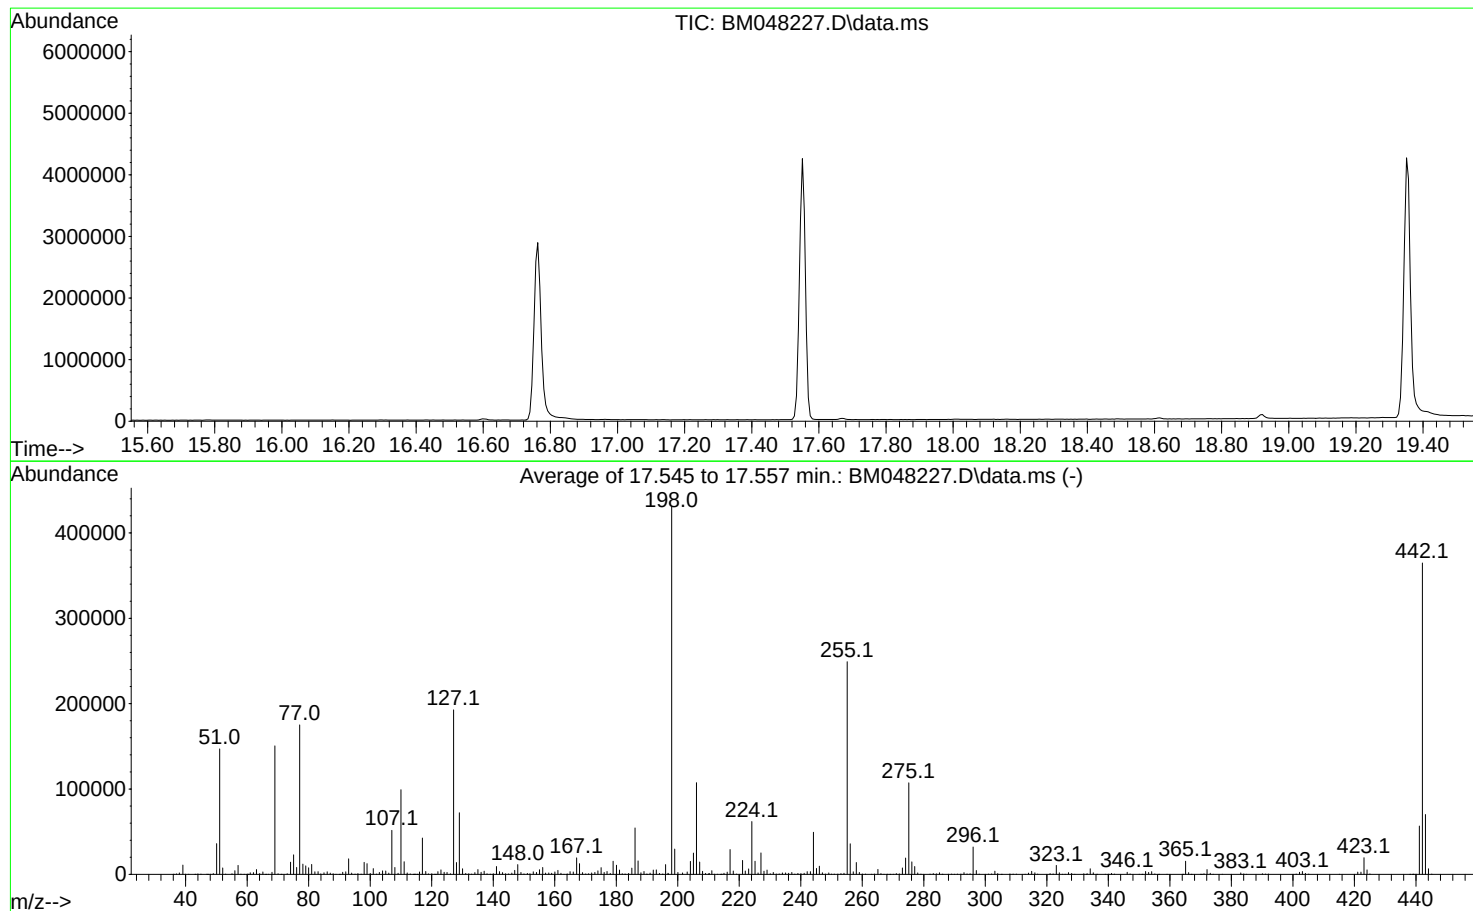

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	146931	PASS
68	69	0.00	2	1.6	2399	PASS
69	198	0.00	100	34.9	150621	PASS
70	69	0.00	2	0.5	723	PASS
127	198	10	80	44.7	192704	PASS
197	198	0.00	2	0.3	1314	PASS
198	198	100	100	100.0	430976	PASS
199	198	5	9	6.9	29624	PASS
275	198	10	60	24.9	107243	PASS
365	198	1	100	3.6	15327	PASS
441	198	0.01	100	13.1	56541	PASS
442	442	50	100	100.0	364736	PASS
443	442	15	24	19.2	70056	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/25/2024	BNA_M	<u>BM048227.D</u>
Compound Name	Response	Retention Time
DDT	1418943	20.58
DDD	28471	20.145
DDE	1742	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30213	1449156	2.08

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048227.D
Acq On : 25 Oct 2024 08:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 25 13:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 18:21:59 2024
Response via : Initial Calibration

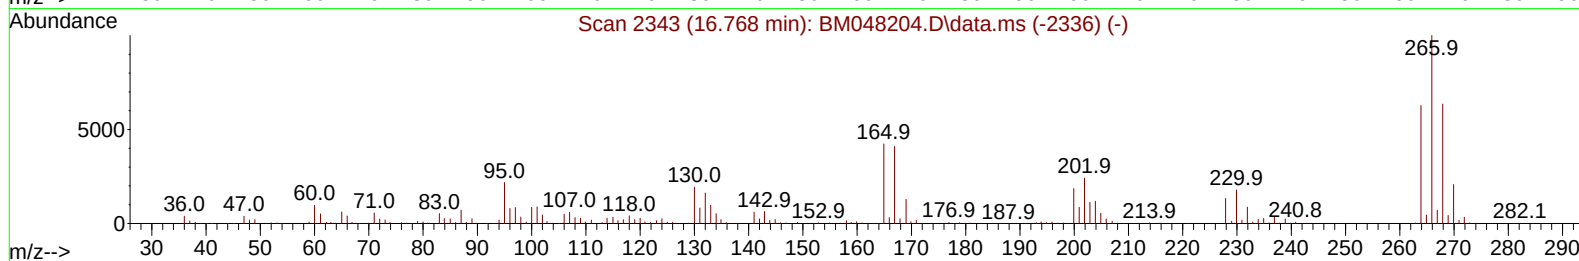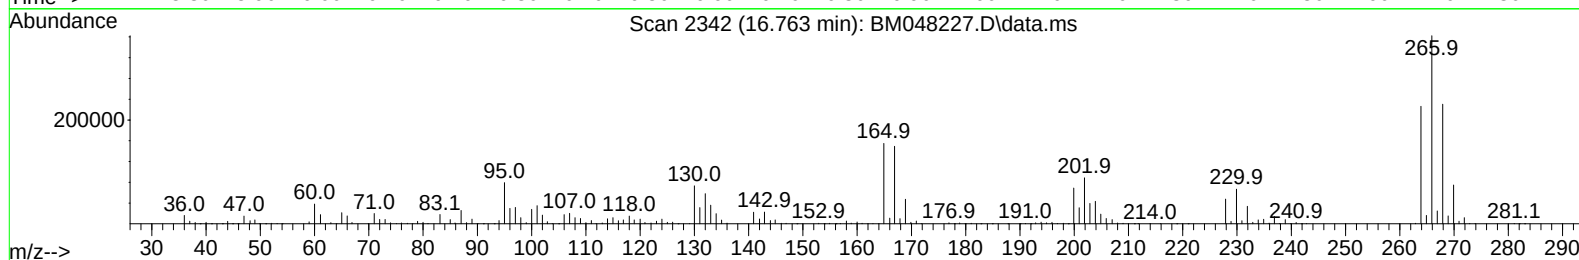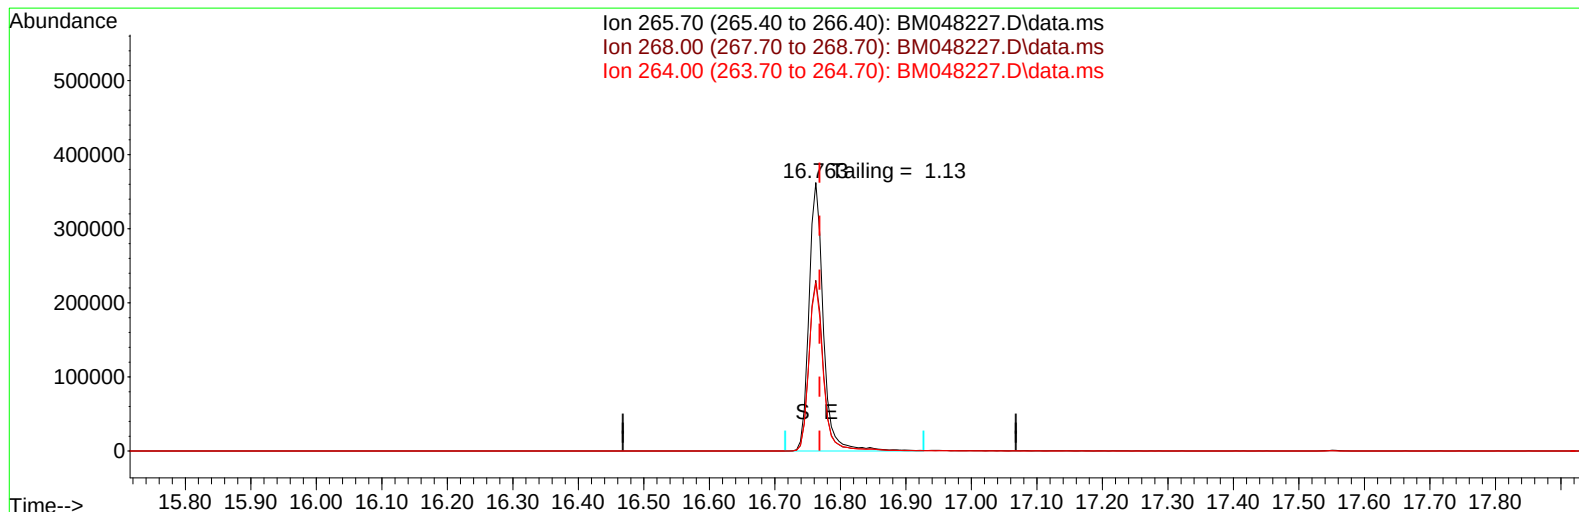

TIC: BM048227.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.006) 395736.19 ng




response 550504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.55
264.00	62.70	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048227.D
Acq On : 25 Oct 2024 08:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 25 13:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 18:21:59 2024
Response via : Initial Calibration

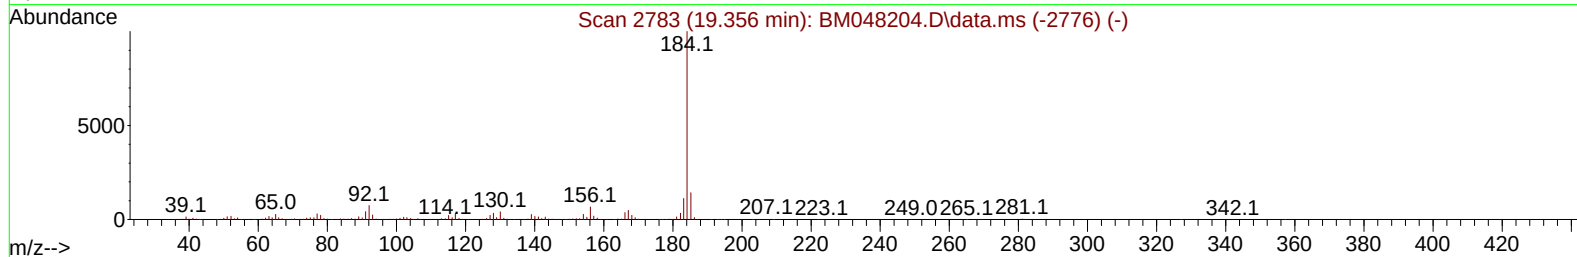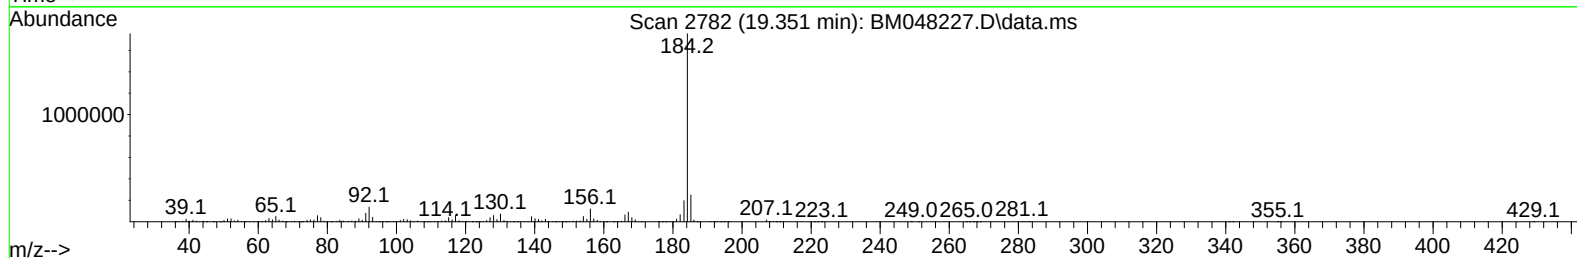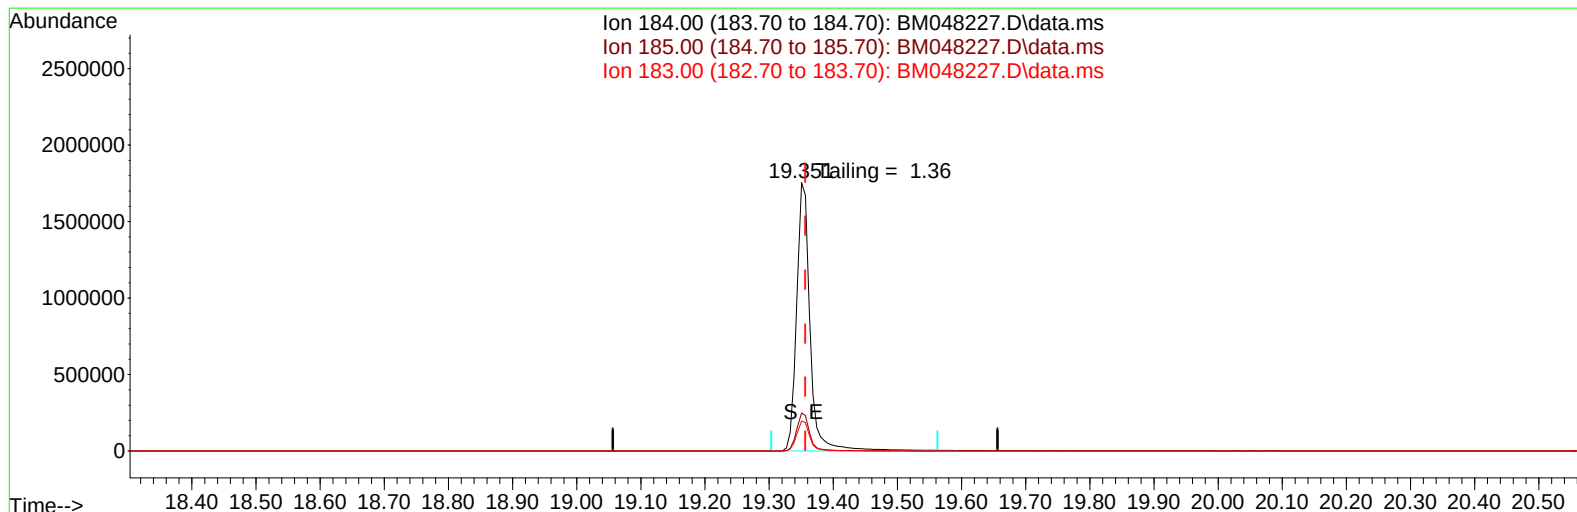

TIC: BM048227.D\data.ms

(77) Benzidine

19.351min (-0.006) 261475.58 ng

response 2555981

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.22
183.00	11.20	11.24
0.00	0.00	0.00