
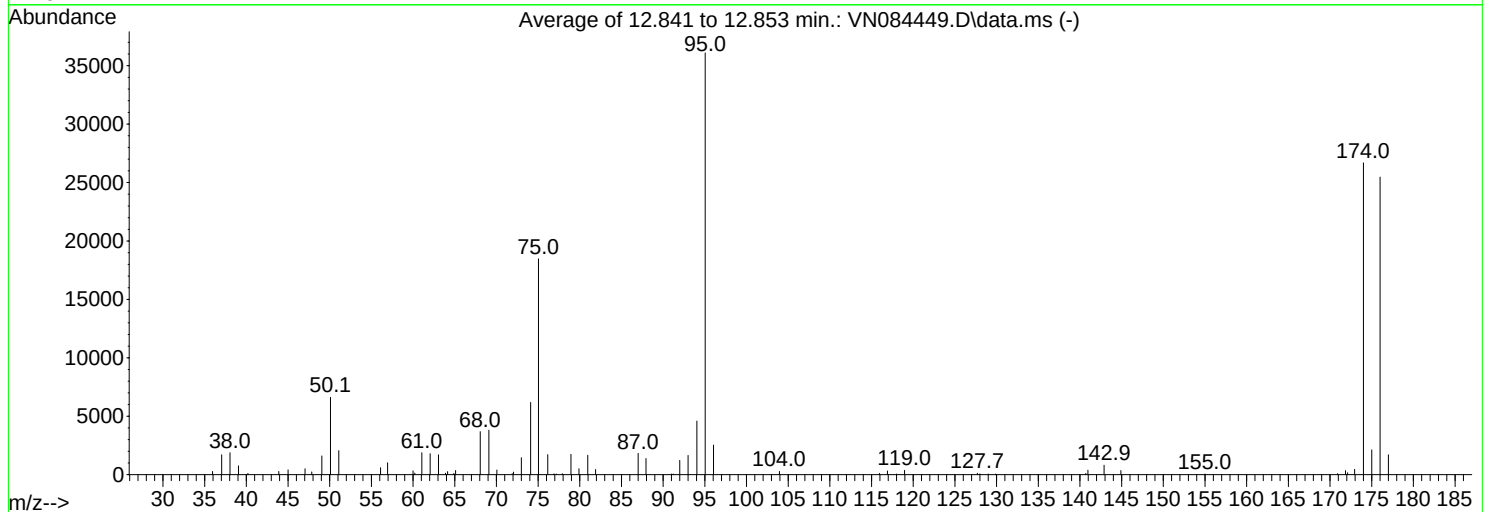


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN102224\  
Data File : VN084449.D  
Acq On : 22 Oct 2024 08:33  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N093024W.M  
Title : SW846 8260  
Last Update : Tue Oct 01 07:11:01 2024

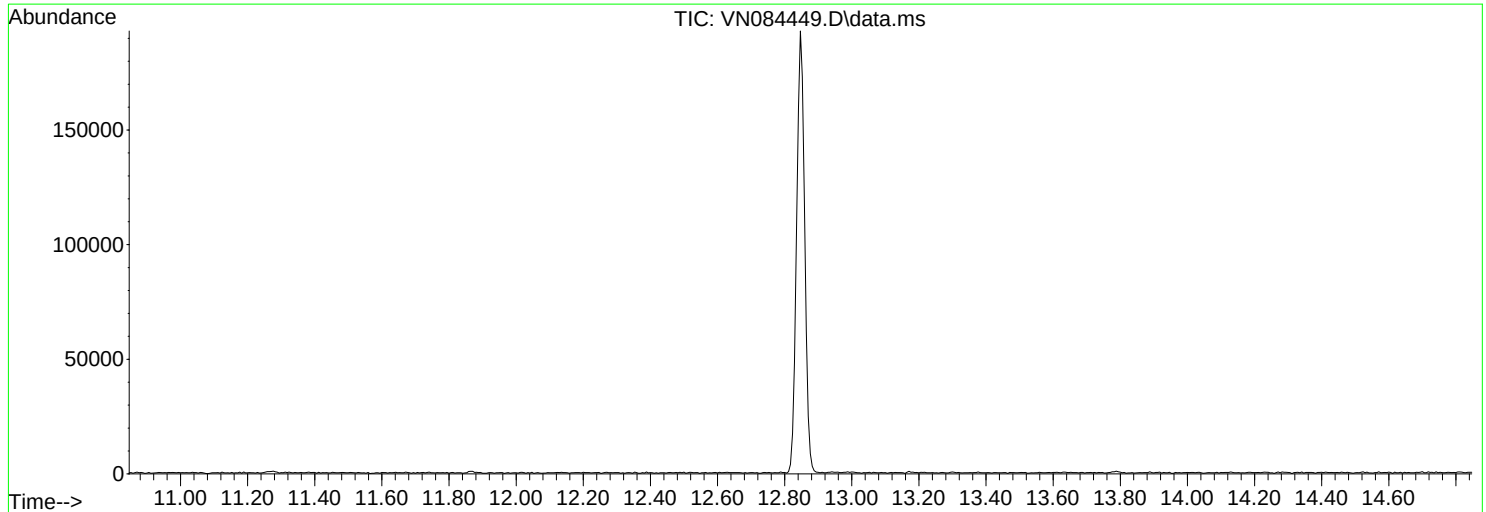

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.3         | 6621       | PASS                |
| 75             | 95              | 30              | 60              | 51.2         | 18475      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 36101      | PASS                |
| 96             | 95              | 5               | 9               | 7.0          | 2529       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.7          | 450        | PASS                |
| 174            | 95              | 50              | 100             | 73.9         | 26696      | PASS                |
| 175            | 174             | 5               | 9               | 7.9          | 2121       | PASS                |
| 176            | 174             | 95              | 101             | 95.4         | 25467      | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 1699       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.95 | 269    | 51.10 | 2048   | 65.10 | 358    | 77.20 | 61     |
| 37.05 | 1703   | 56.10 | 596    | 68.05 | 3681   | 77.90 | 81     |
| 38.05 | 1879   | 56.95 | 1016   | 69.10 | 3809   | 78.95 | 174    |
| 39.05 | 753    | 60.00 | 334    | 70.05 | 396    | 79.90 | 50     |
| 40.20 | 114    | 60.20 | 138    | 71.90 | 89     | 80.95 | 1659   |
| 43.90 | 270    | 61.05 | 1873   | 72.05 | 223    | 81.90 | 436    |
| 45.00 | 419    | 62.05 | 1793   | 73.00 | 1459   | 87.00 | 1816   |
| 47.05 | 510    | 63.05 | 1703   | 74.10 | 6180   | 87.95 | 1391   |
| 47.85 | 233    | 63.90 | 118    | 75.05 | 18475  | 91.00 | 54     |
| 49.05 | 1602   | 64.15 | 262    | 76.15 | 1707   | 91.20 | 56     |
| 50.10 | 6621   | 64.90 | 116    | 76.90 | 73     | 92.00 | 1224   |

Average of 12.841 to 12.853 min.: VN084449.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z | abund. |
|--------|--------|--------|--------|--------|--------|-----|--------|
| 93.00  | 1646   | 129.00 | 52     | 174.00 | 26696  |     |        |
| 94.05  | 4594   | 129.90 | 60     | 175.00 | 2121   |     |        |
| 95.05  | 36101  | 140.70 | 114    | 176.00 | 25467  |     |        |
| 96.05  | 2529   | 140.95 | 391    | 177.00 | 1699   |     |        |
| 103.95 | 278    | 142.90 | 812    |        |        |     |        |
| 115.95 | 112    | 144.90 | 355    |        |        |     |        |
| 116.90 | 314    | 155.00 | 51     |        |        |     |        |
| 118.00 | 63     | 170.90 | 78     |        |        |     |        |
| 118.95 | 376    | 171.85 | 349    |        |        |     |        |
| 127.70 | 122    | 172.10 | 170    |        |        |     |        |
| 128.00 | 74     | 172.95 | 450    |        |        |     |        |

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB