

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102224AL\
Data File : FC067495.D
Signal(s) : FID1A.ch
Acq On : 23 Oct 2024 07:17
Operator : YP/AJ
Sample : P4471-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
B-180-SB02

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :Ankita Jodhani 10/24/2024

Integration File: autoint1.e
Quant Time: Oct 23 11:05:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 09:13:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.934	2582219	22.812 ug/mlm
Spiked Amount	50.000	Recovery	= 45.62%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102224AL\
Data File : FC067495.D
Signal(s) : FID1A.ch
Acq On : 23 Oct 2024 07:17
Operator : YP/AJ
Sample : P4471-02
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
B-180-SB02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :Ankita Jodhani 10/24/2024

Integration File: autoint1.e
Quant Time: Oct 23 11:05:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 09:13:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

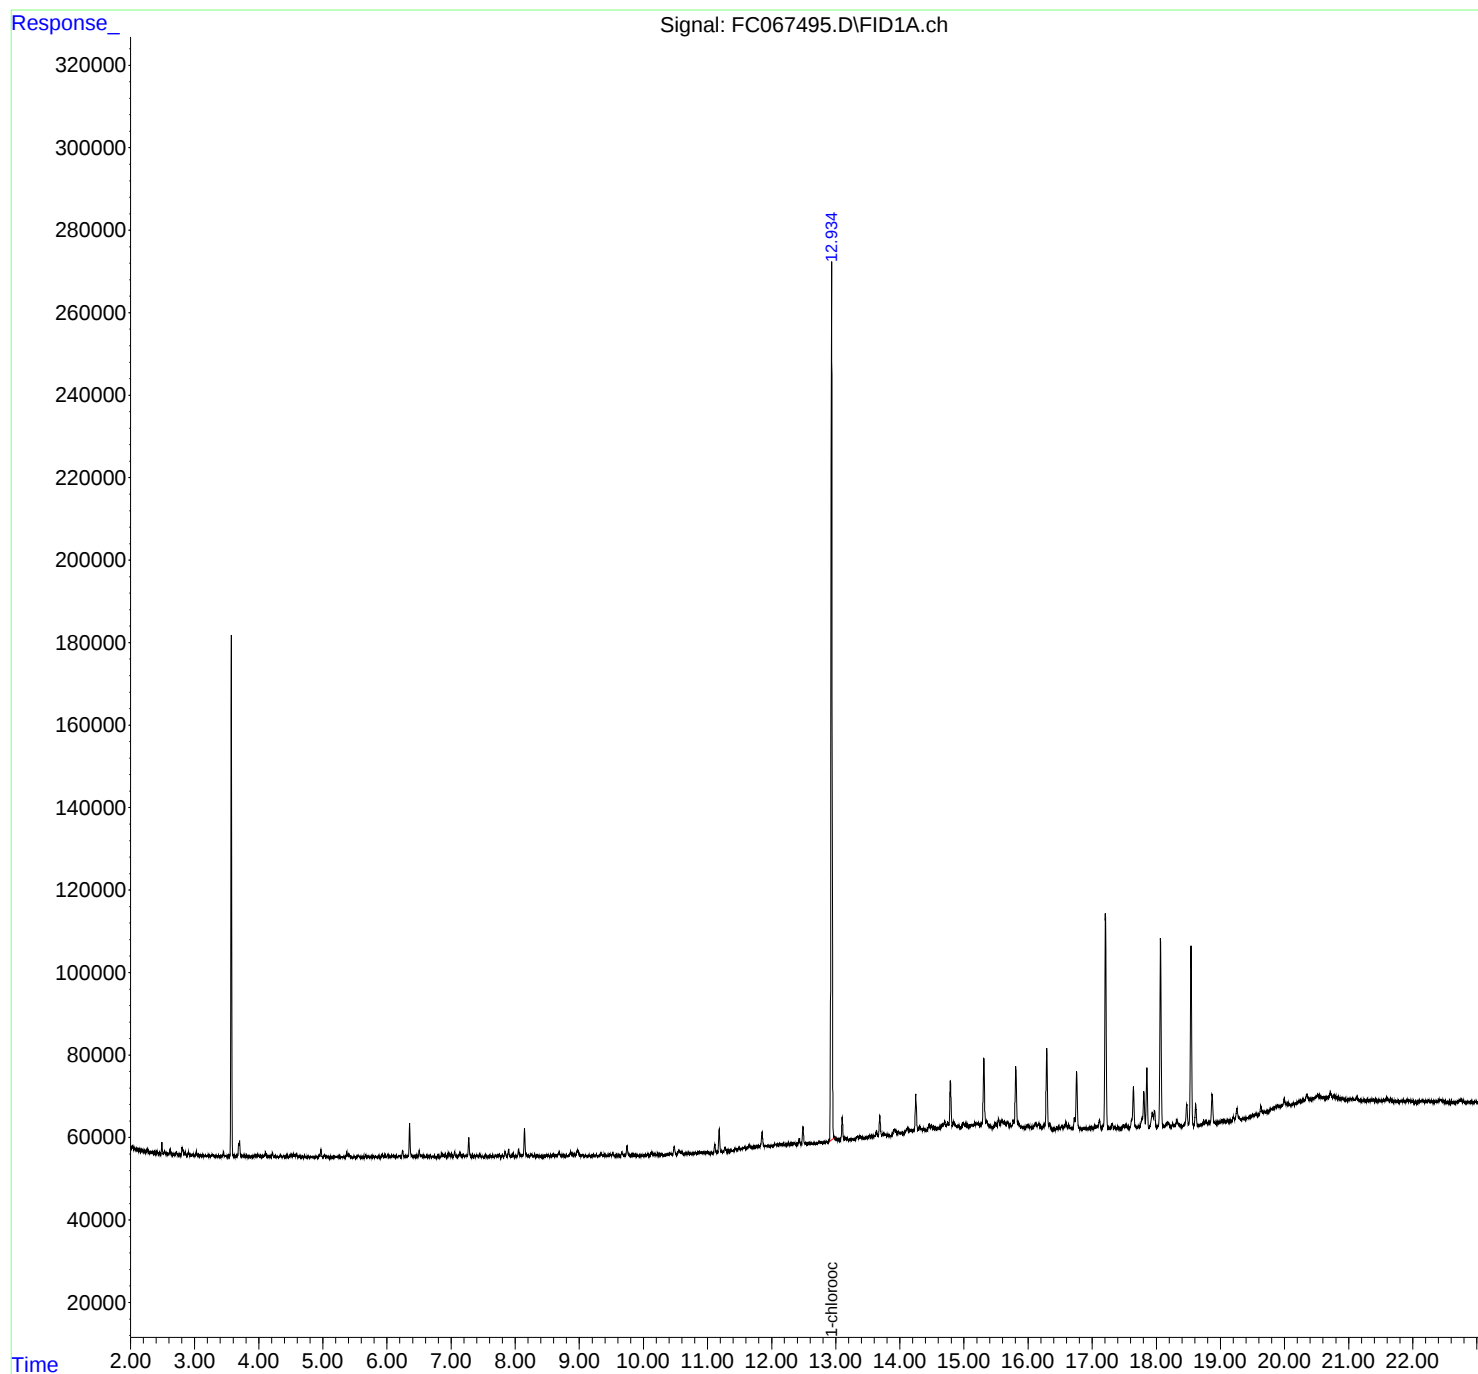

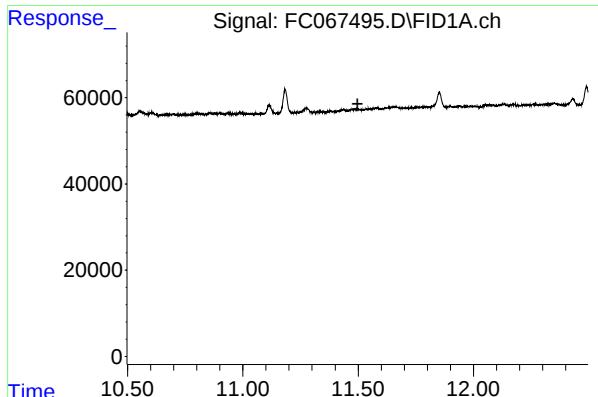


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
B-180-SB02

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :Ankita Jodhani 10/24/2024

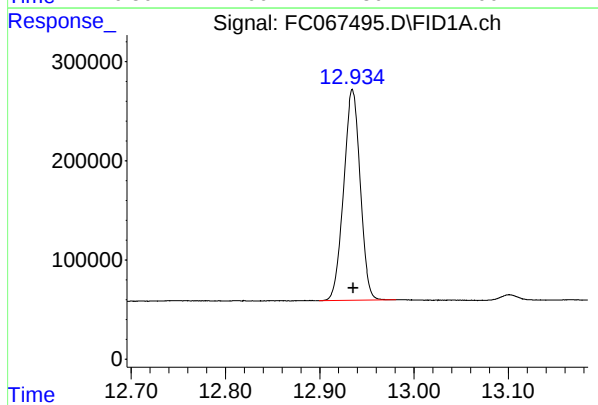

#12 1-chlorooctadecane (SURR)

R.T.: 12.934 min
Delta R.T.: -0.001 min
Response: 2582219
Conc: 22.81 ug/ml m