
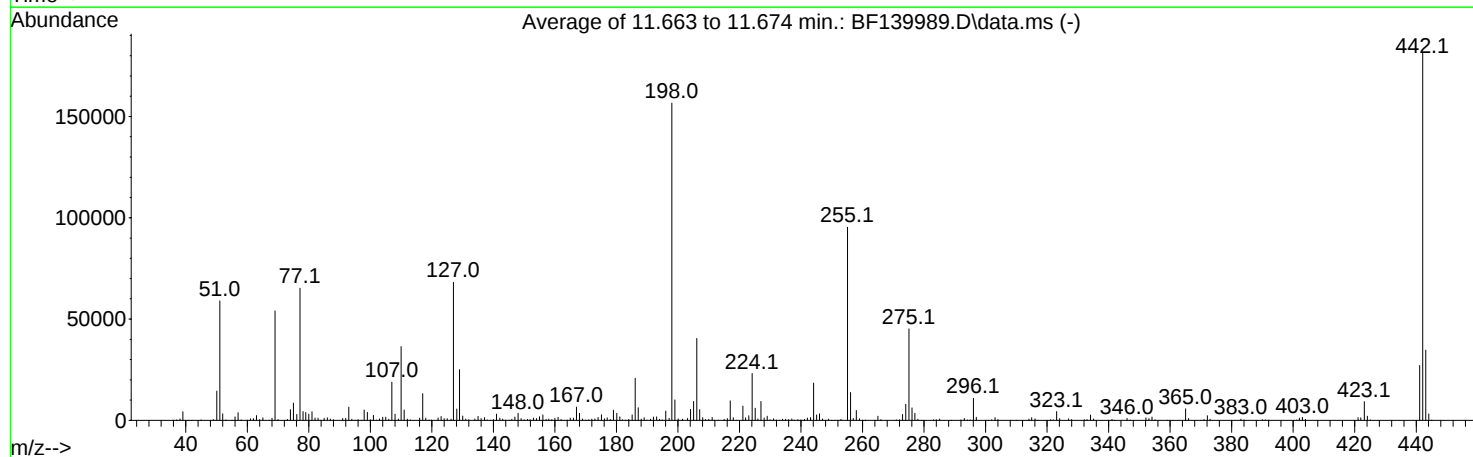


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF139989.D
Acq On : 24 Oct 2024 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

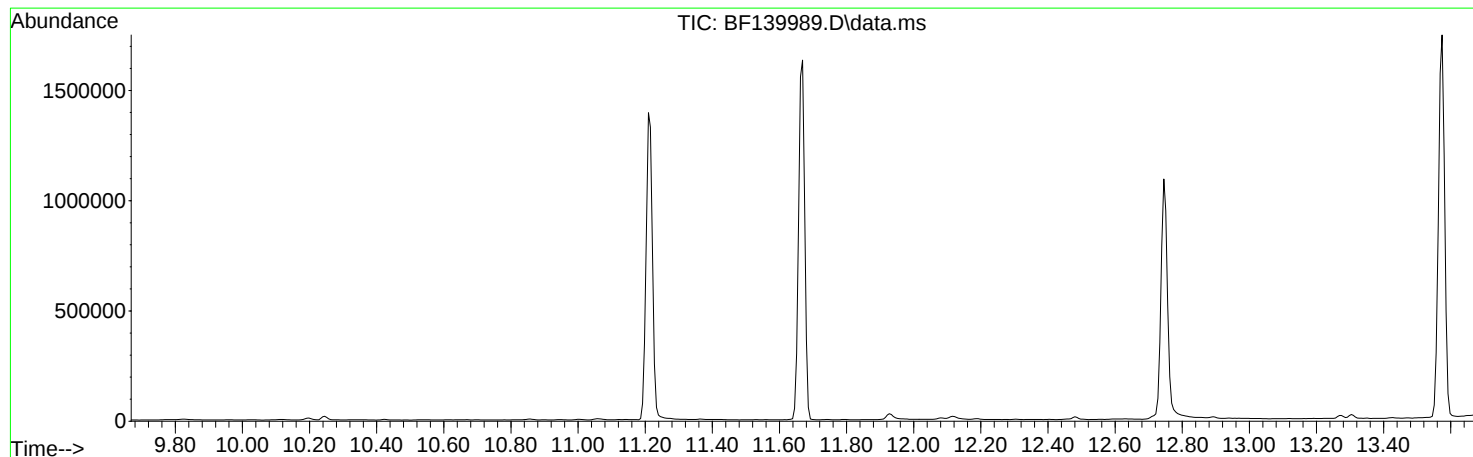

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	58978	PASS
68	69	0.00	2	1.9	1013	PASS
69	198	0.00	100	34.5	54048	PASS
70	69	0.00	2	0.7	372	PASS
127	198	10	80	43.5	68144	PASS
197	198	0.00	2	0.7	1061	PASS
198	198	100	100	100.0	156656	PASS
199	198	5	9	6.5	10146	PASS
275	198	10	60	28.9	45216	PASS
365	198	1	100	3.7	5733	PASS
441	198	0.01	100	17.3	27125	PASS
442	442	50	100	100.0	181589	PASS
443	442	15	24	19.1	34717	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/24/2024	BNA_F	<u>BF139989.D</u>
Compound Name	Response	Retention Time
DDT	459539	13.574
DDD	8411	13.304
DDE	2706	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11117	470656	2.36

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF139989.D
Acq On : 24 Oct 2024 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 24 15:15:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

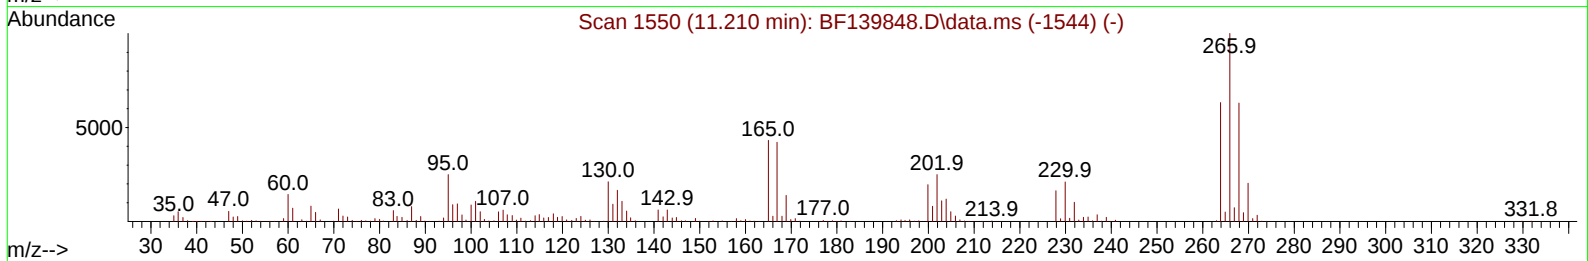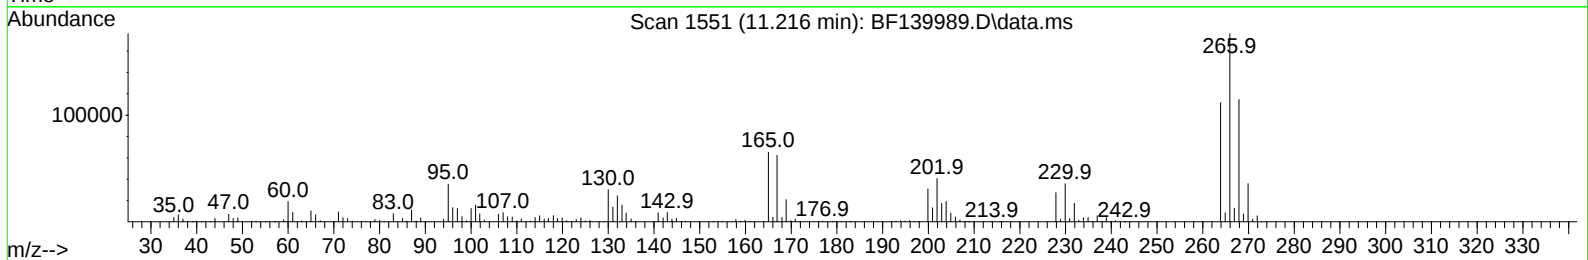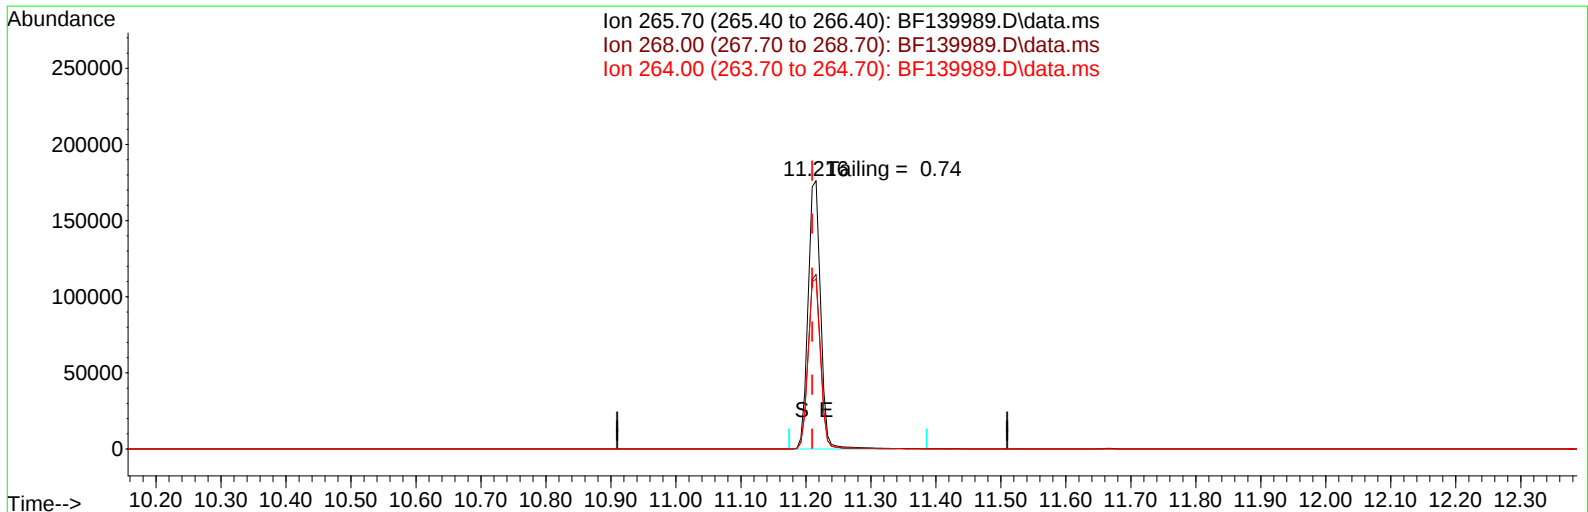

TIC: BF139989.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 53480.74 ng




response 237671

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.03
264.00	63.20	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF139989.D
Acq On : 24 Oct 2024 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 24 15:15:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

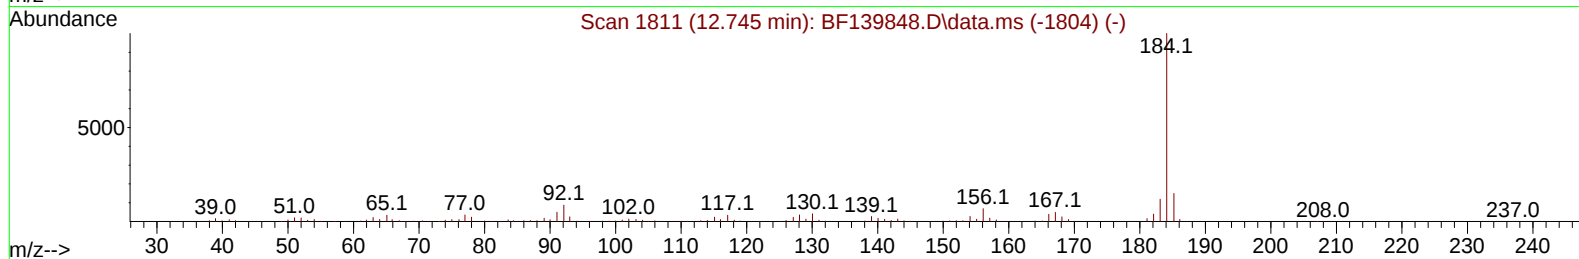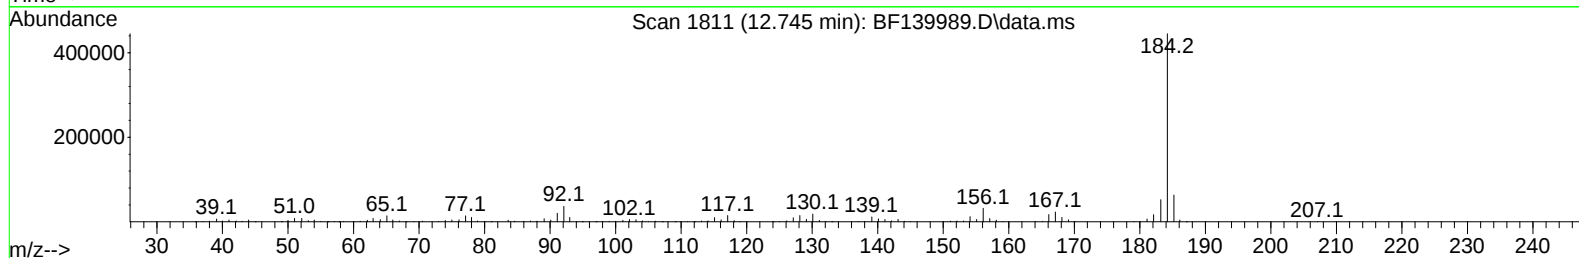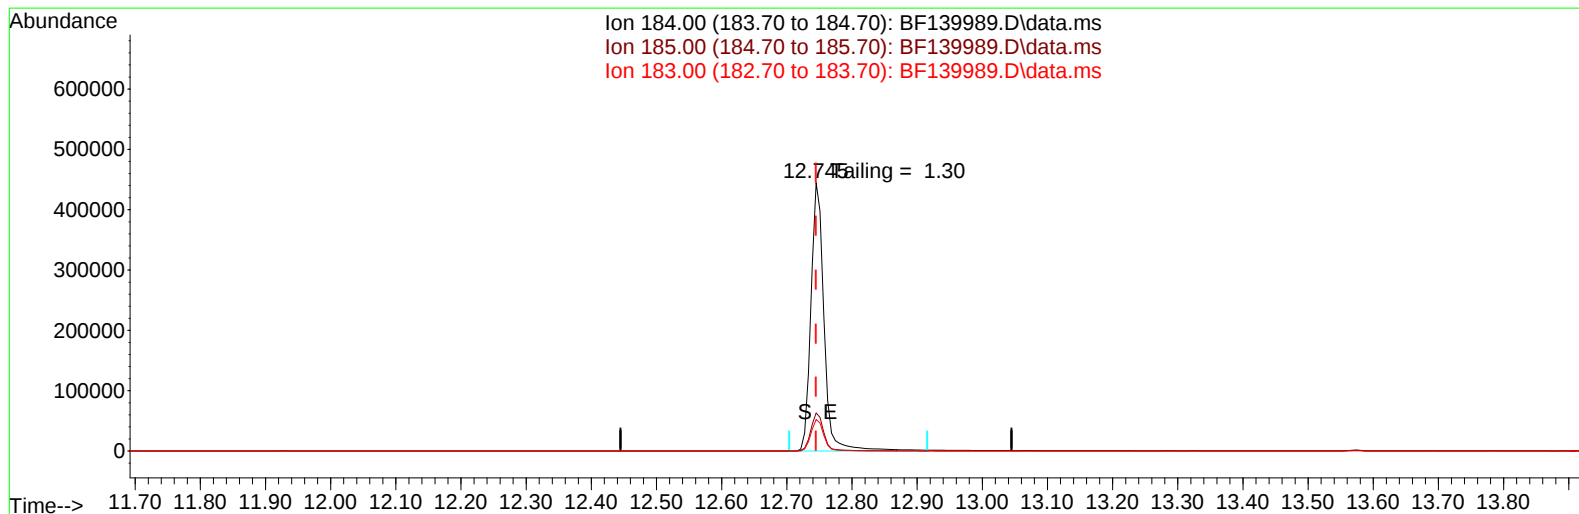

TIC: BF139989.D\data.ms

(77) Benzidine

12.745min (-0.000) 78892.96 ng

response 623986

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.22
183.00	11.80	11.75
0.00	0.00	0.00