


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF140000.D
Acq On : 24 Oct 2024 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

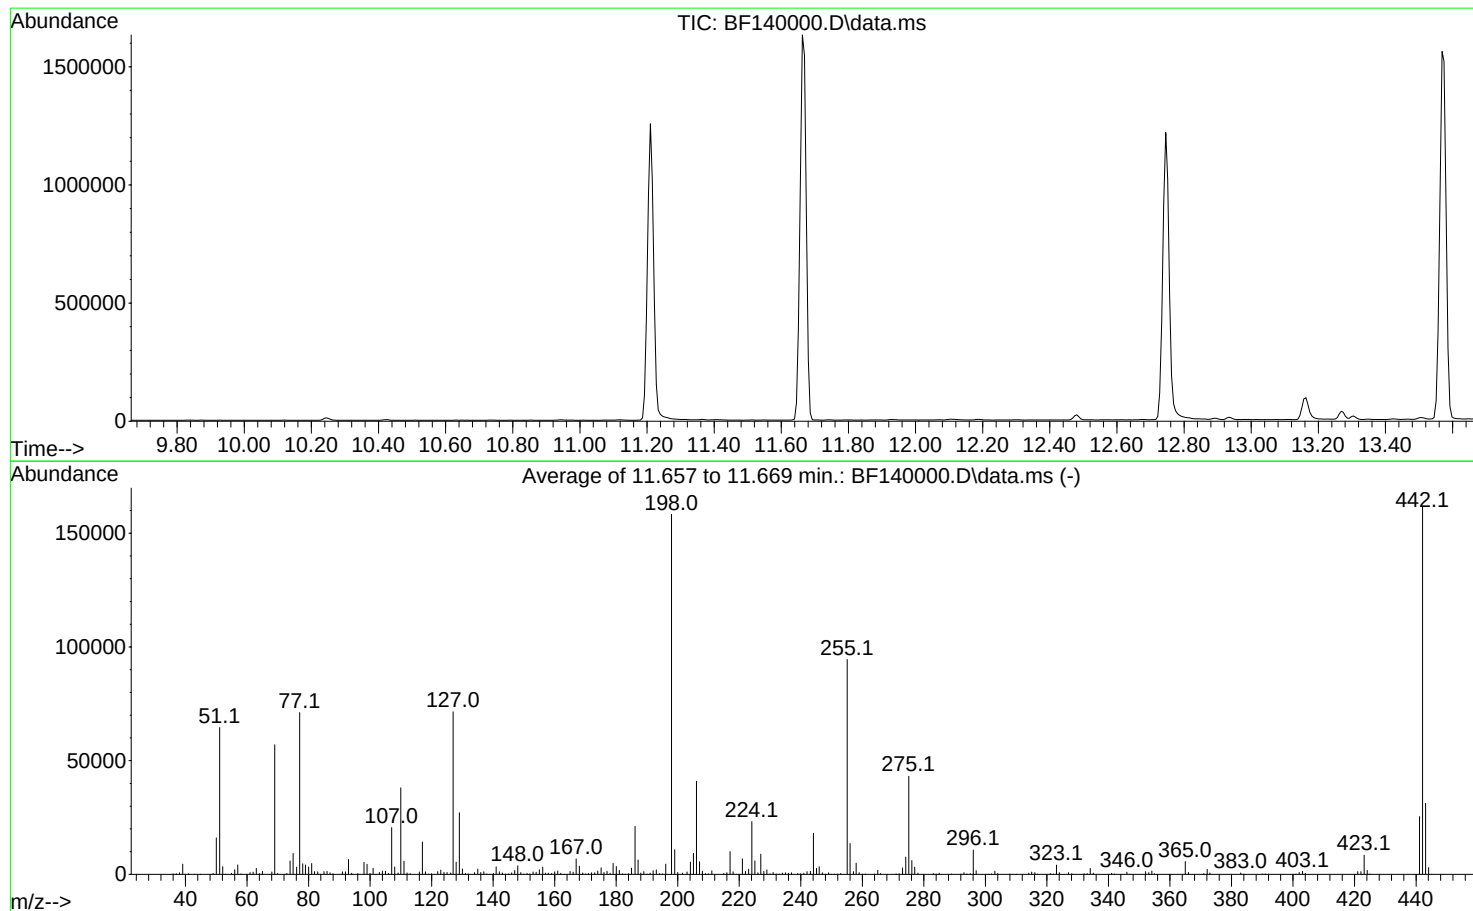

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	64629	PASS
68	69	0.00	2	1.9	1095	PASS
69	198	0.00	100	36.0	57000	PASS
70	69	0.00	2	0.7	403	PASS
127	198	10	80	45.1	71469	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	158301	PASS
199	198	5	9	6.8	10841	PASS
275	198	10	60	27.3	43141	PASS
365	198	1	100	3.6	5671	PASS
441	198	0.01	100	16.0	25384	PASS
442	442	50	100	100.0	161765	PASS
443	442	15	24	19.3	31248	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/24/2024	BNA_F	<u>BF140000.D</u>
Compound Name	Response	Retention Time
DDT	418161	13.575
DDD	12931	13.269
DDE	2295	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15226	433387	3.51

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF140000.D
Acq On : 24 Oct 2024 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 24 15:14:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

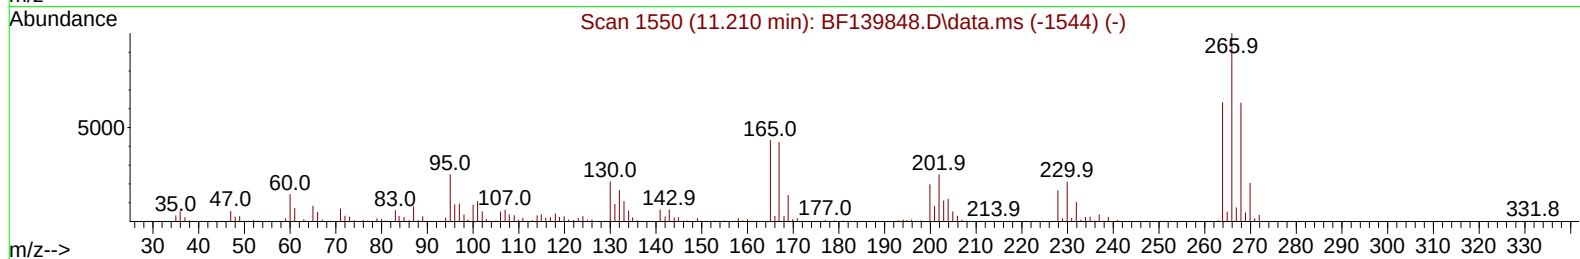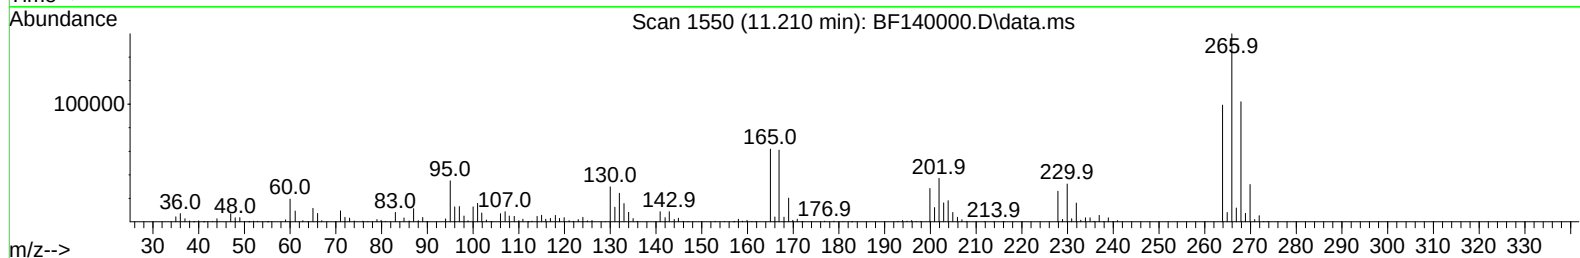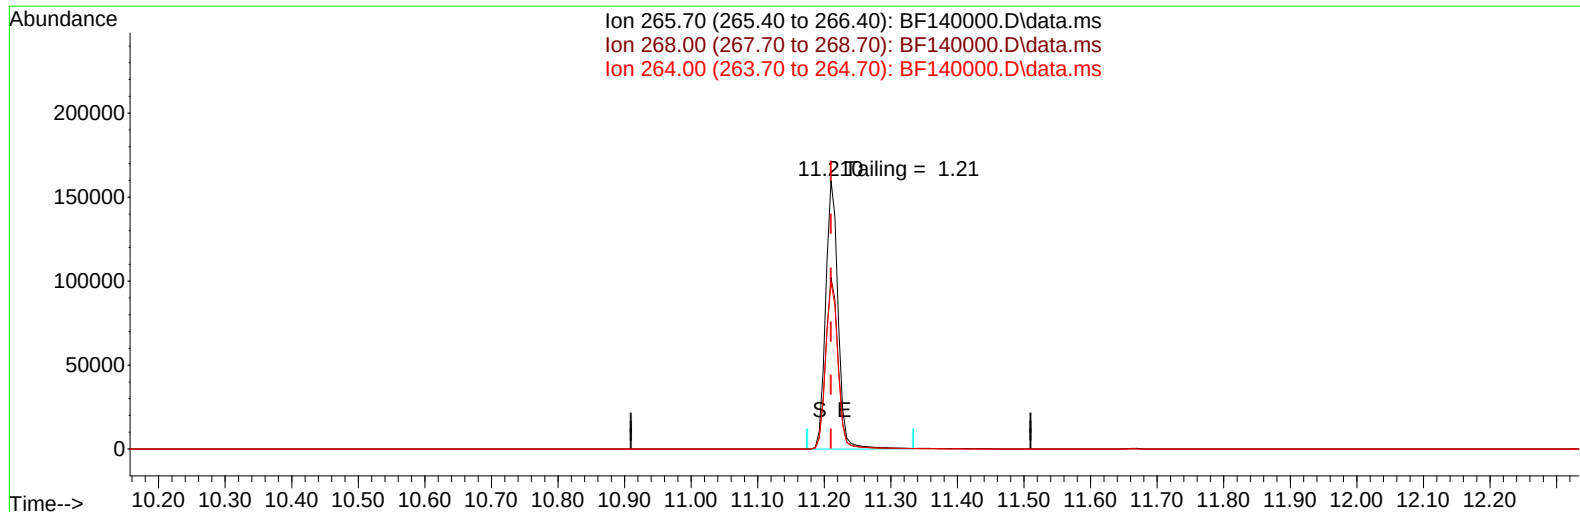

TIC: BF140000.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.000) 39709.65 ng




response 208862

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.86
264.00	63.20	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF140000.D
Acq On : 24 Oct 2024 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 24 15:14:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

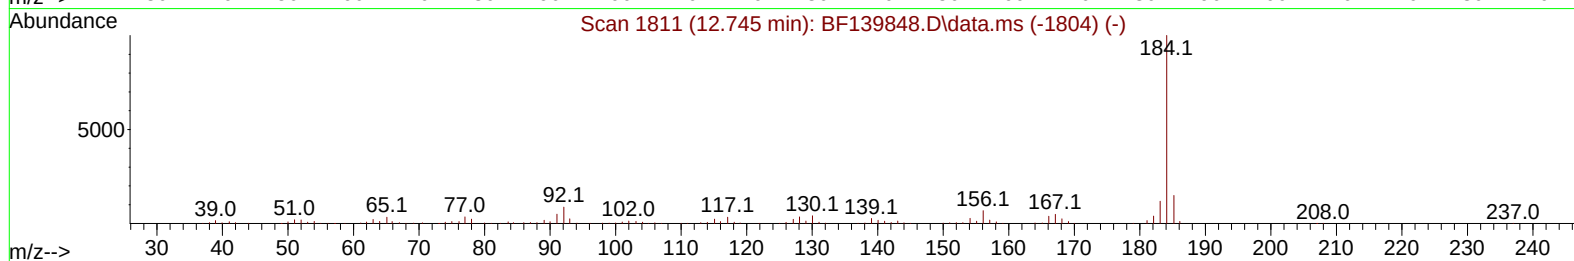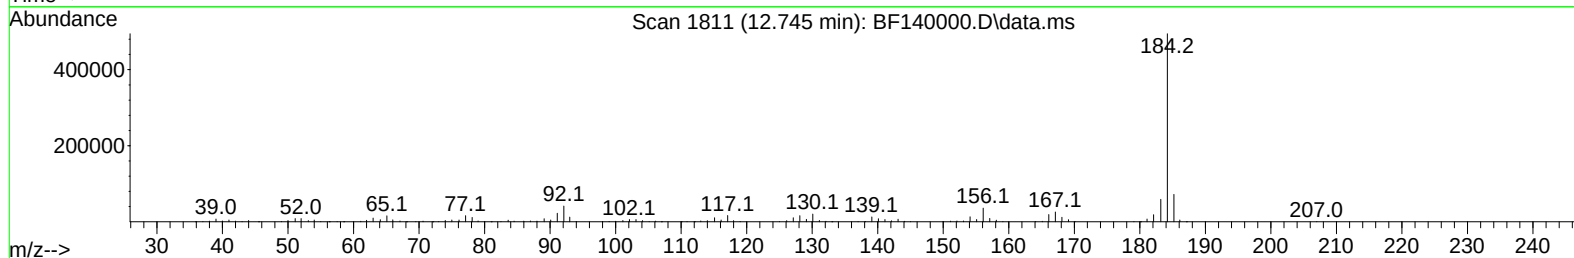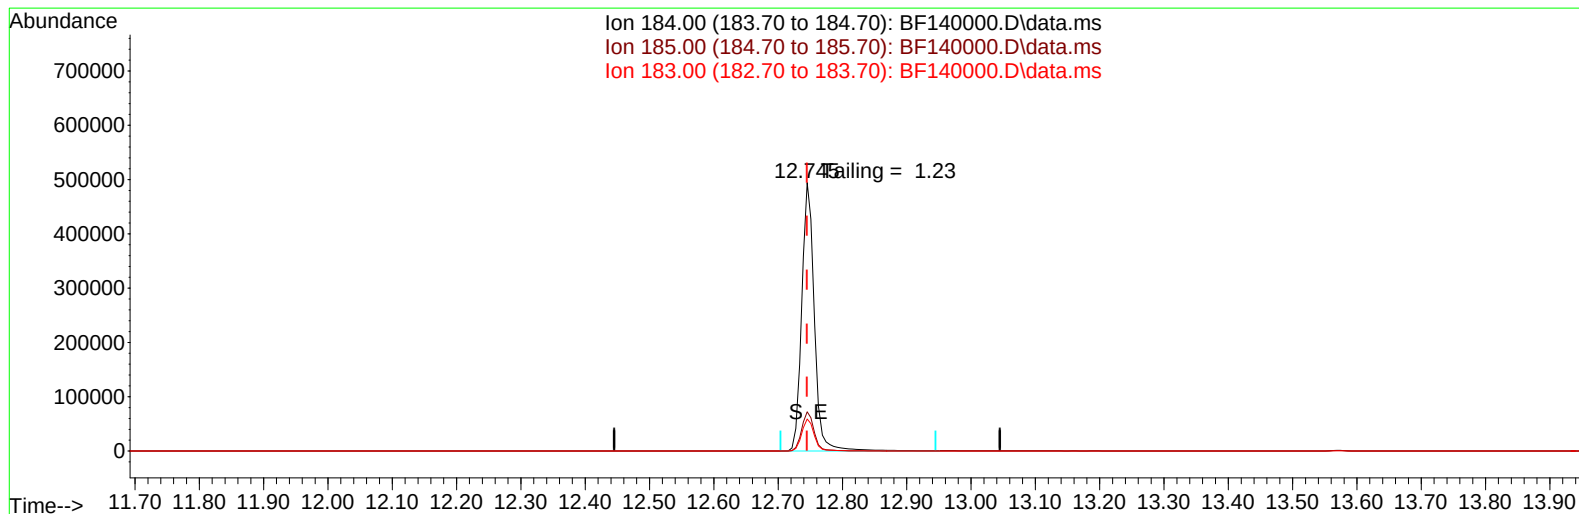

TIC: BF140000.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 156375.06 ng

response 678833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.62
183.00	11.80	11.94
0.00	0.00	0.00