

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112524\
 Data File : PS028613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 09:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 23:47:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	7.727	1411.0E6	583.0E6	552.071	451.119
Target Compounds							
2) T	3,5-DICHL...	6.415	0.000	211233	0	<MDL	N.D. #
3) T	4-Nitroph...	7.019	0.000	8270371	0	4.869	N.D. #
6) T	MCP	7.656f	0.000	6165585	0	<MDL	N.D. #
8) T	DICHLORPROP	8.187f	8.694f	4092973	4527082	1.387	3.100 #
11) T	2,4,5-TP ...	9.293f	0.000	12195661	0	<MDL	N.D. #
12) T	2,4,5-T	9.524	10.284f	833319	4504048	<MDL	<MDL #
13) T	2,4-DB	10.149f	0.000	215440	0	<MDL	N.D. #
14) T	DINOSEB	11.304f	0.000	696381	0	<MDL	N.D. #
15) T	Picloram	11.124	12.340	21716904	13002048	<MDL	1.149 #
16) T	DCPA	11.598f	12.340f	1545979	13002048	<MDL	1.341 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112524\
Data File : PS028613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 09:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 23:47:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

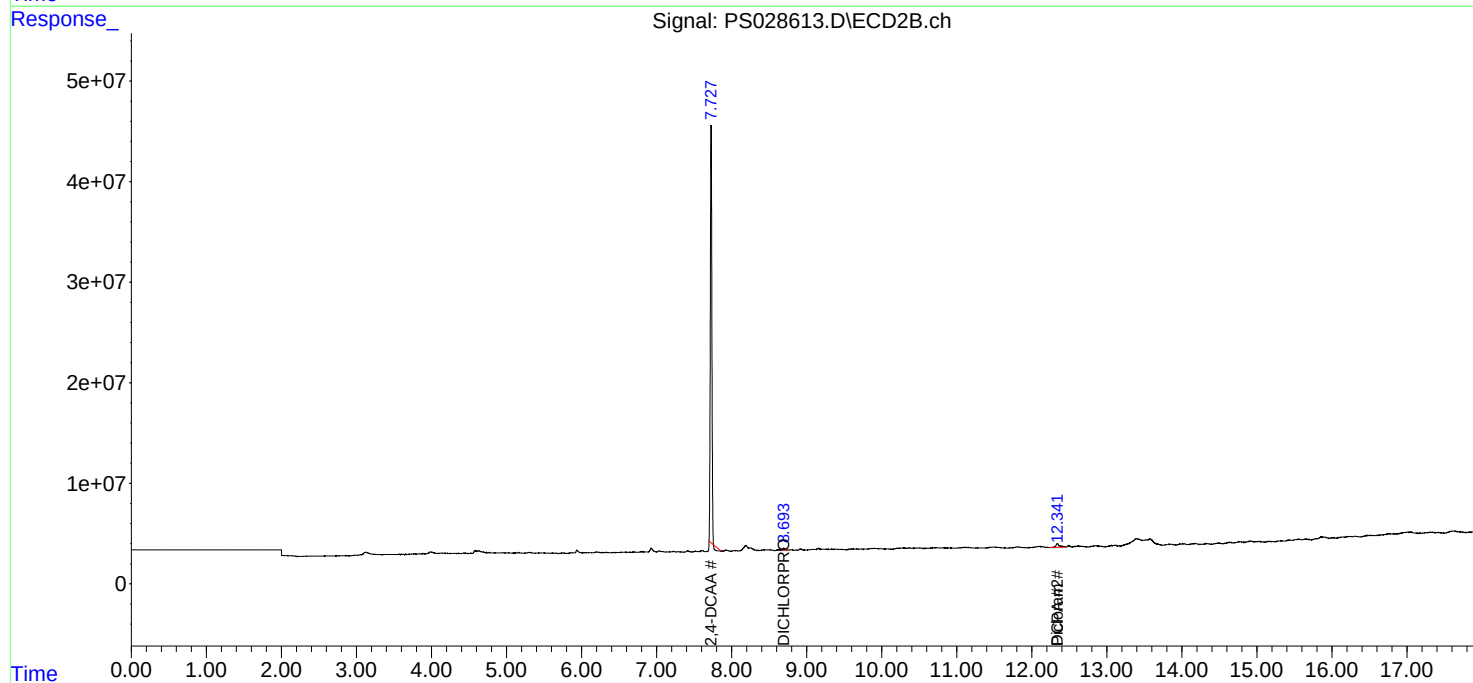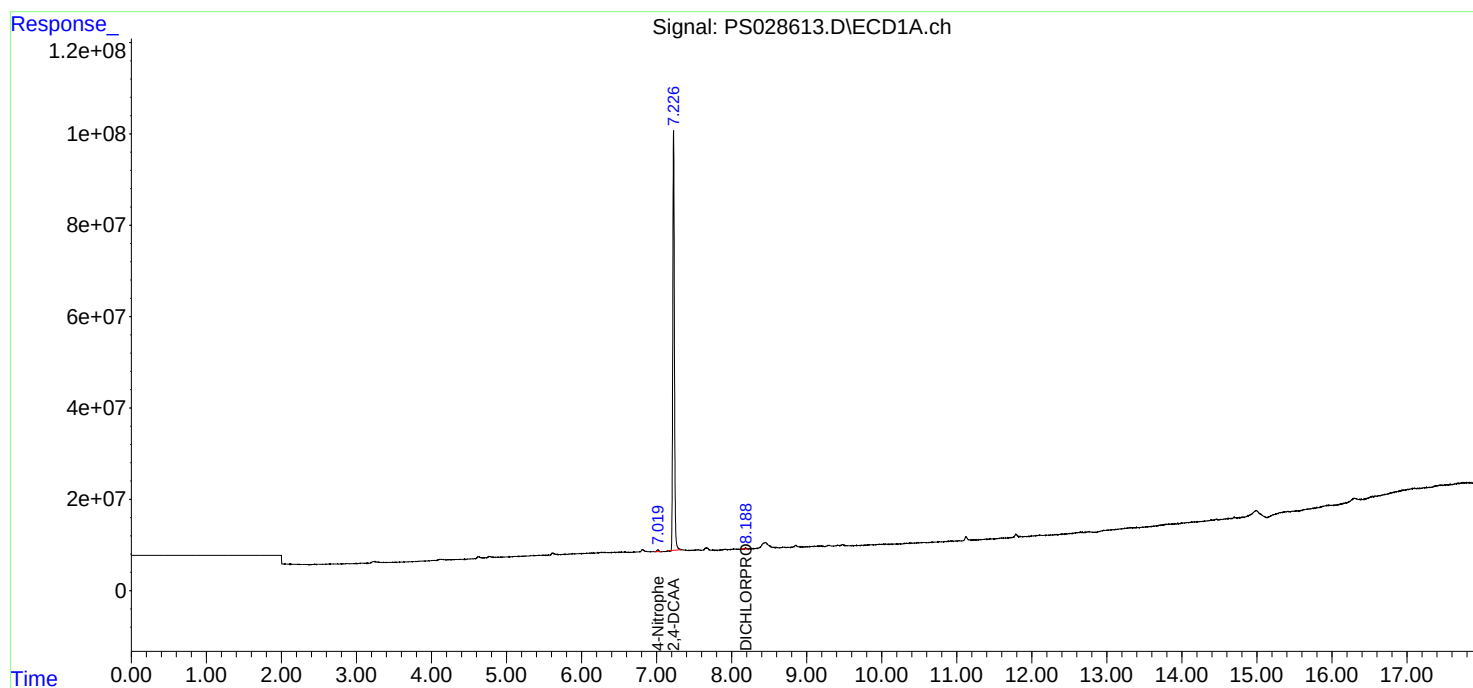


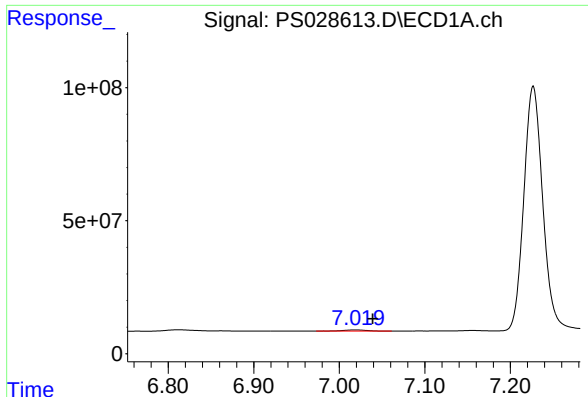

#3 4-Nitrophenol


R.T.: 7.019 min
Delta R.T.: -0.020 min
Response: 8270371
Conc: 4.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

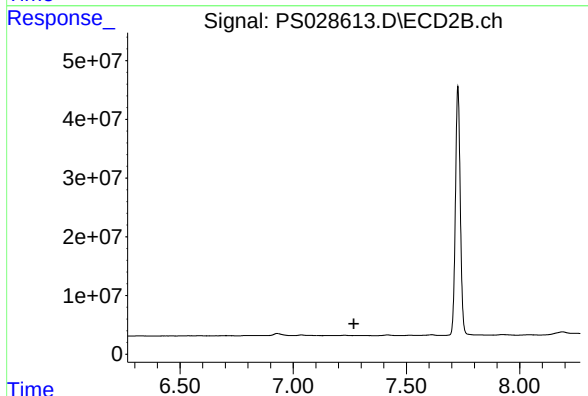


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

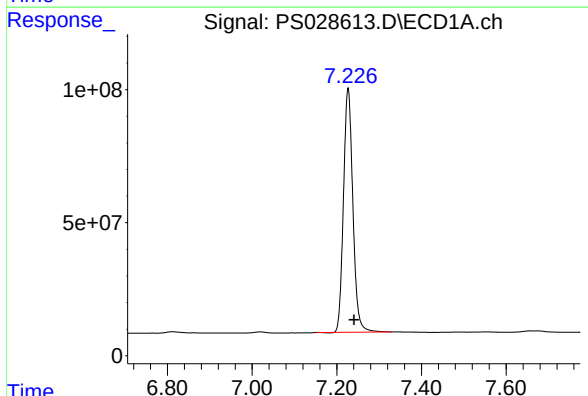


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: -0.014 min
Response: 1411029546
Conc: 552.07 ng/ml

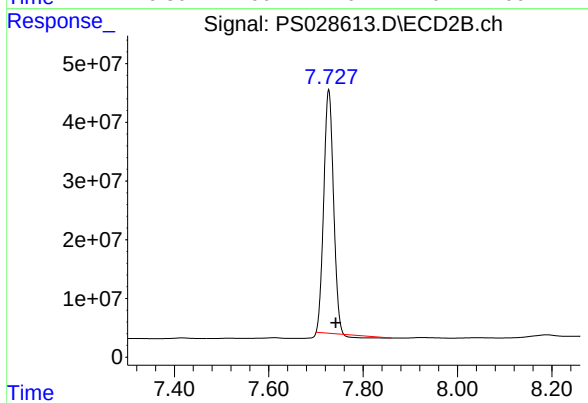

#4 2,4-DCAA


R.T.: 7.727 min
Delta R.T.: -0.015 min
Response: 582982645
Conc: 451.12 ng/ml

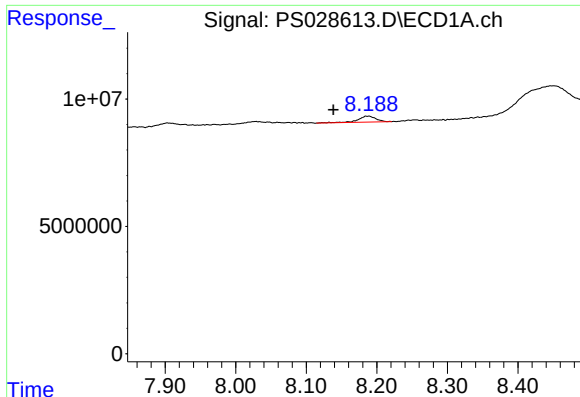

#8 DICHLORPROP


R.T.: 8.187 min
Delta R.T.: 0.049 min
Response: 4092973
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

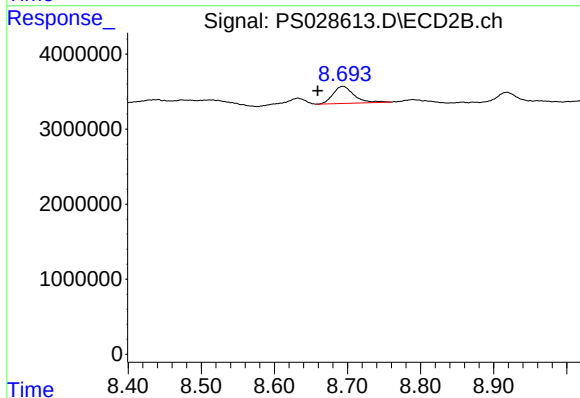


#8 DICHLORPROP

R.T.: 8.694 min
Delta R.T.: 0.034 min
Response: 4527082
Conc: 3.10 ng/ml

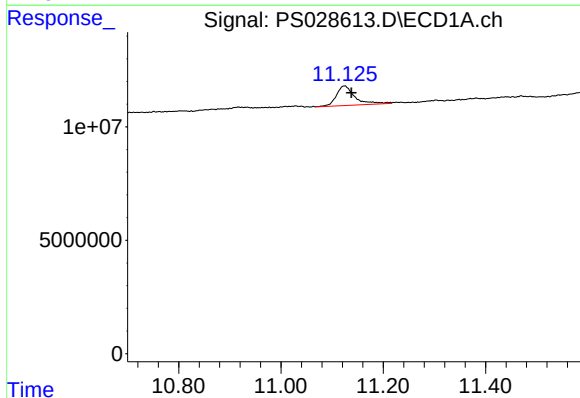


#15 Picloram

R.T.: 11.124 min
Delta R.T.: -0.014 min
Response: 21716904
Conc: N.D.

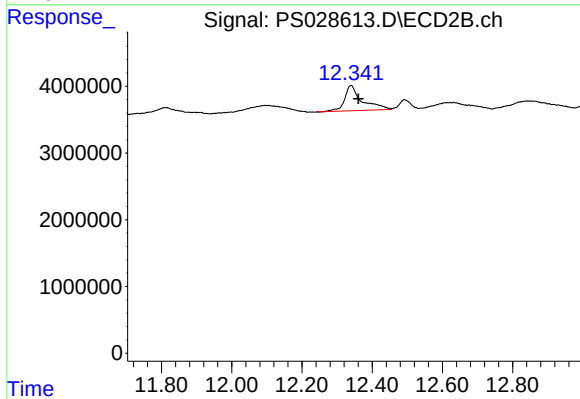

#15 Picloram


R.T.: 12.340 min
Delta R.T.: -0.020 min
Response: 13002048
Conc: 1.15 ng/ml

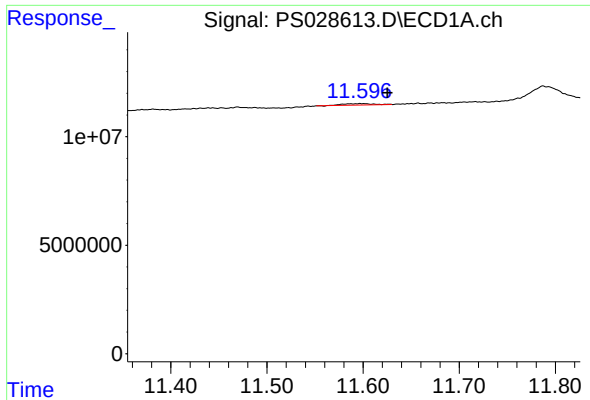

#16 DCPA

R.T.: 11.598 min
Delta R.T.: -0.027 min
Response: 1545979
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

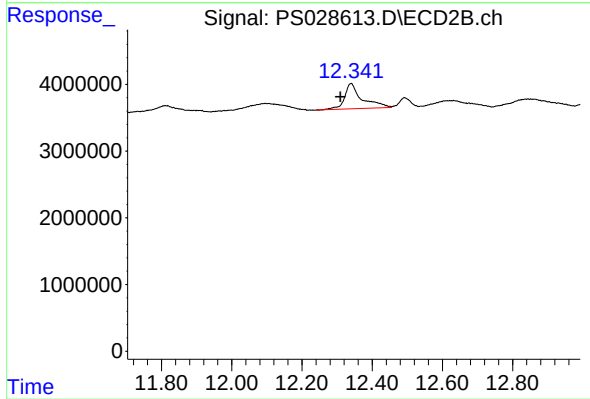

#16 DCPA

R.T.: 12.340 min
Delta R.T.: 0.031 min
Response: 13002048
Conc: 1.34 ng/ml