

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 14:29
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:21:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:19:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.778	48587926	52085719	19.830	19.141
28)	SA Decachlor...	9.054	7.916	38629596	53476121	20.072	19.594
Target Compounds							
9)	A Endosulfan I	6.070	5.102	26602716	28047383	10.635	9.186
10)	B gamma-Chl...	5.940	4.982	28607831	32626788	10.752	9.705
12)	B 4,4'-DDE	6.193	5.235	47717989	61582025	20.141	19.115
13)	MA Dieldrin	6.345	5.366	51856039	61668549	19.676	18.462
19)	B Endosulfa...	7.158	6.338	40592527	50485467	18.703	18.720
20)	A Methoxychlor	7.499	6.615	100.3E6	134.2E6	87.976	93.949
21)	B Endrin ke...	7.643	6.844	47240044	57600618	19.498	18.770



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 14:29
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:21:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:19:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

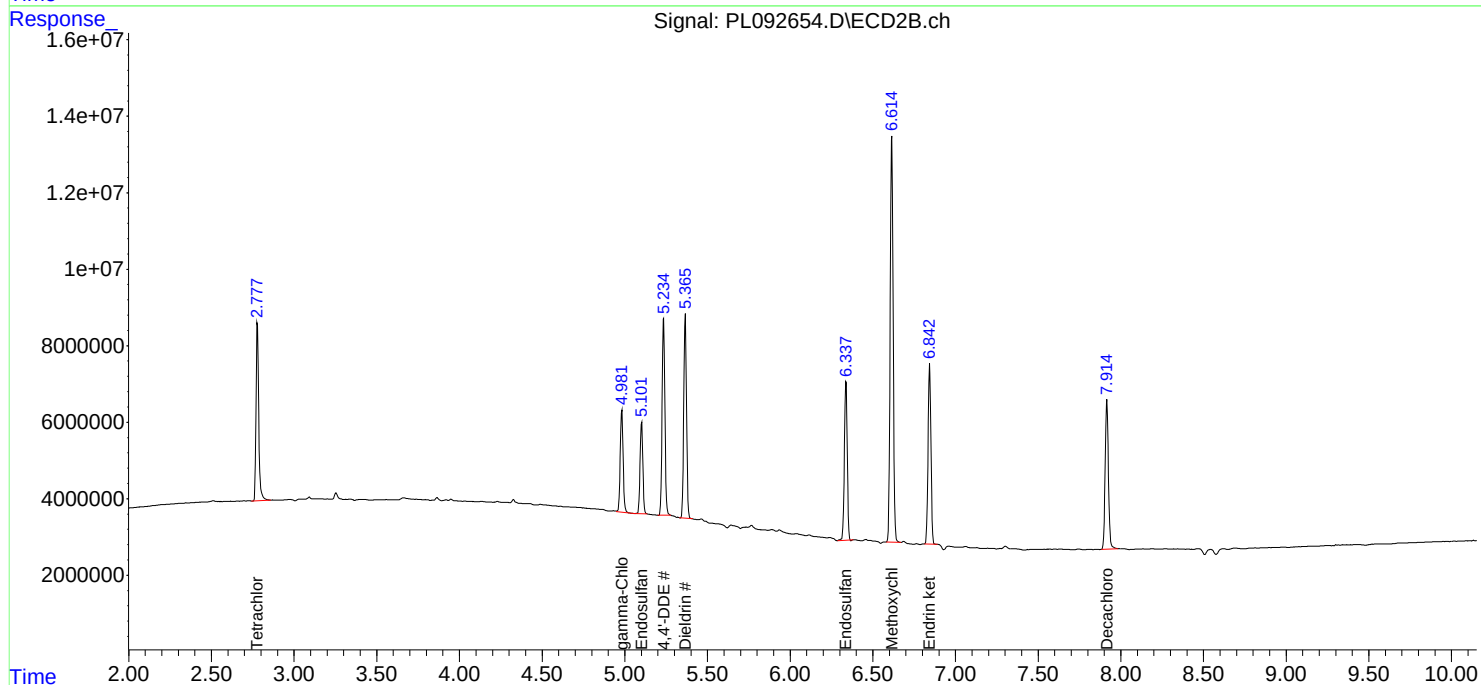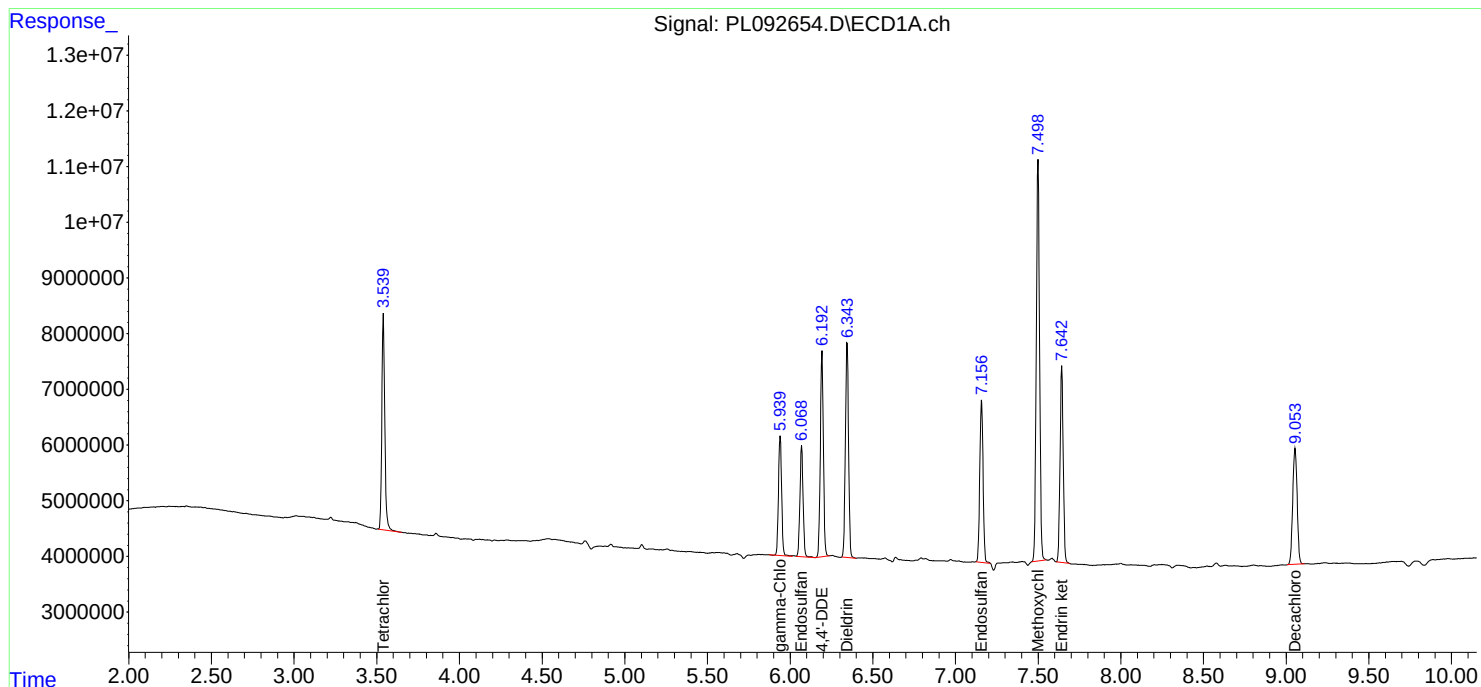


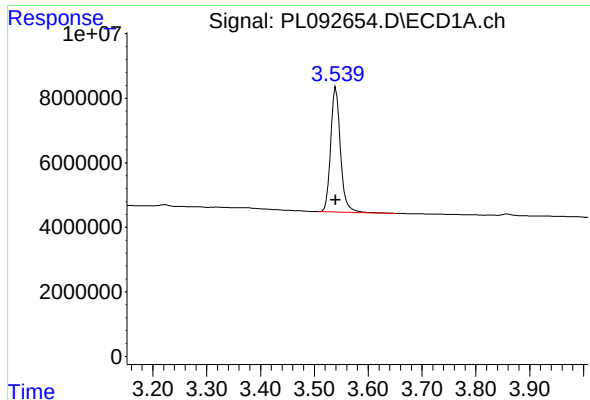

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 48587926
Conc: 19.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

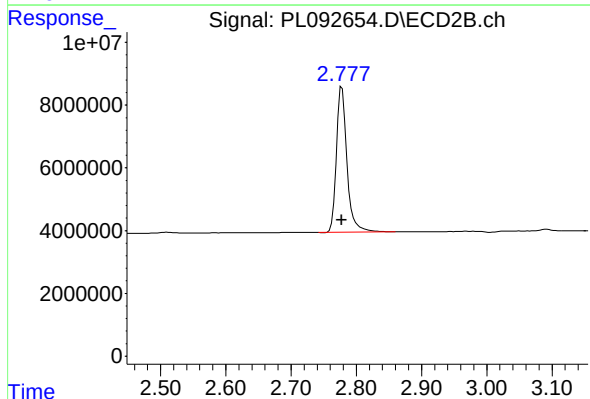


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 52085719
Conc: 19.14 ng/ml

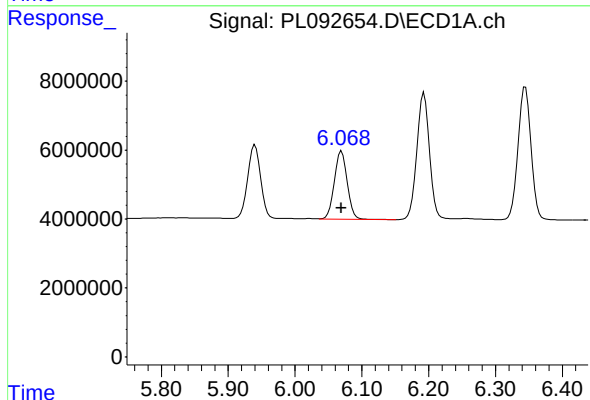


#9 Endosulfan I

R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 26602716
Conc: 10.64 ng/ml

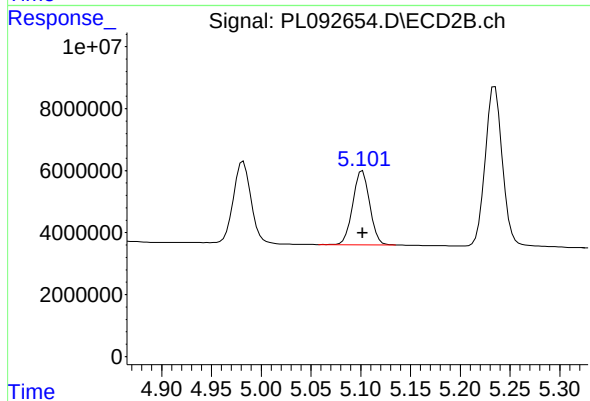

#9 Endosulfan I


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 28047383
Conc: 9.19 ng/ml

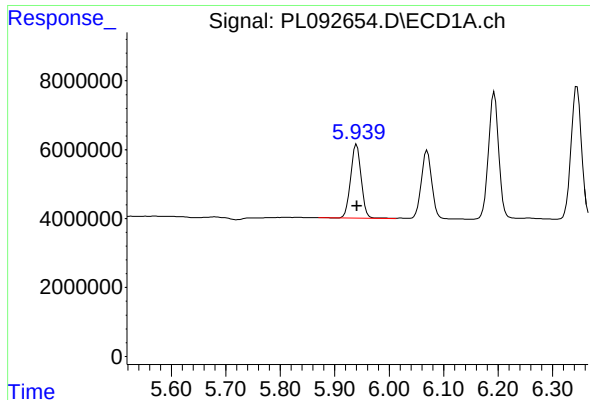

#10 gamma-Chlordane


R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 28607831
Conc: 10.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

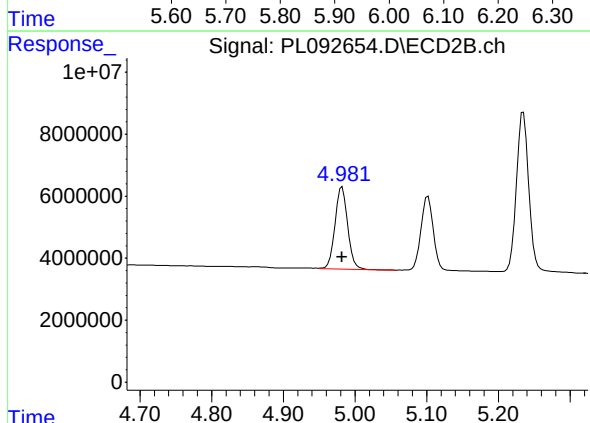


#10 gamma-Chlordane

R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 32626788
Conc: 9.71 ng/ml

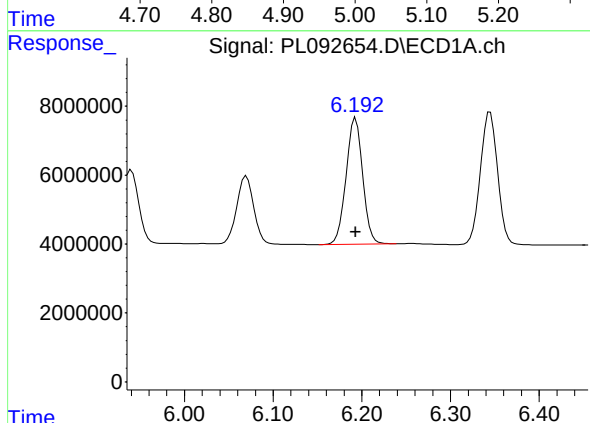


#12 4,4'-DDE

R.T.: 6.193 min
Delta R.T.: 0.000 min
Response: 47717989
Conc: 20.14 ng/ml

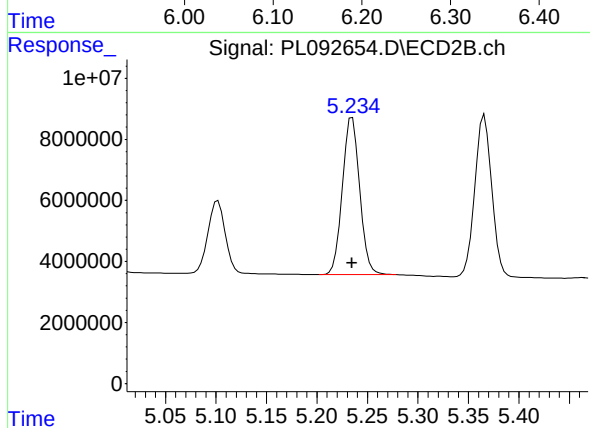

#12 4,4'-DDE


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 61582025
Conc: 19.12 ng/ml

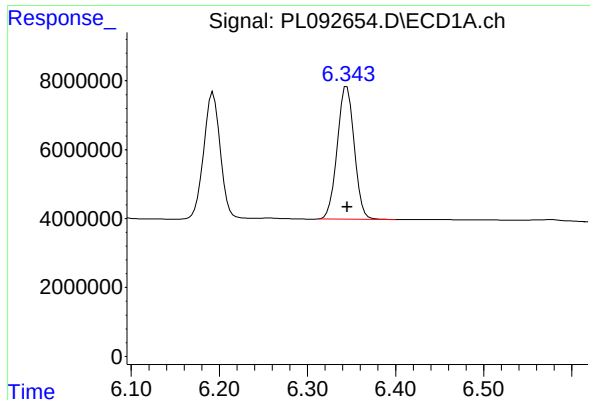

#13 Dieldrin


R.T.: 6.345 min
Delta R.T.: 0.000 min
Response: 51856039
Conc: 19.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

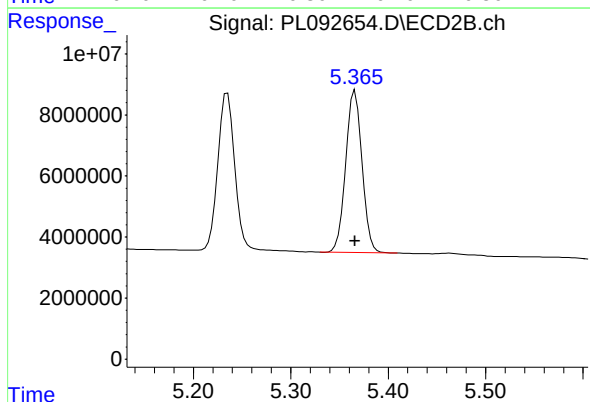


#13 Dieldrin

R.T.: 5.366 min
Delta R.T.: 0.000 min
Response: 61668549
Conc: 18.46 ng/ml

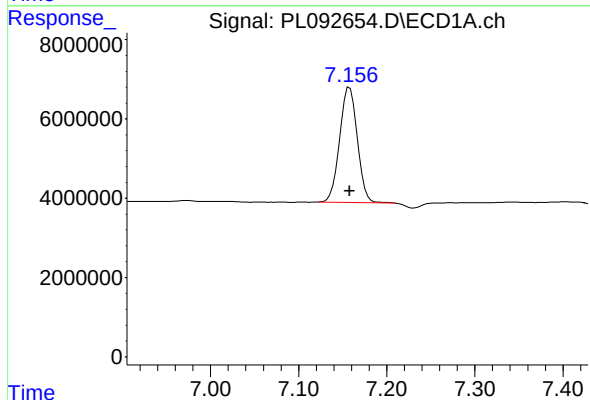


#19 Endosulfan Sulfate

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 40592527
Conc: 18.70 ng/ml

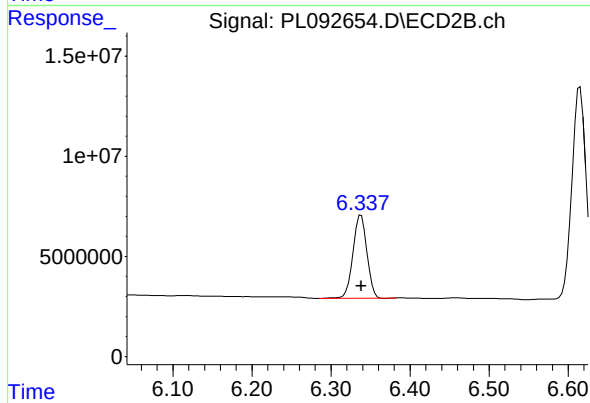

#19 Endosulfan Sulfate


R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 50485467
Conc: 18.72 ng/ml

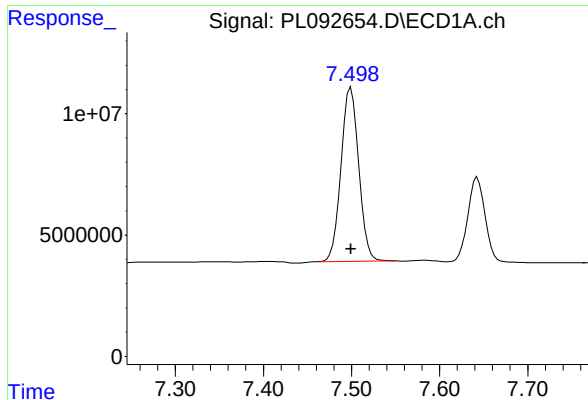

#20 Methoxychlor


R.T.: 7.499 min
Delta R.T.: 0.000 min
Response: 100292431
Conc: 87.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

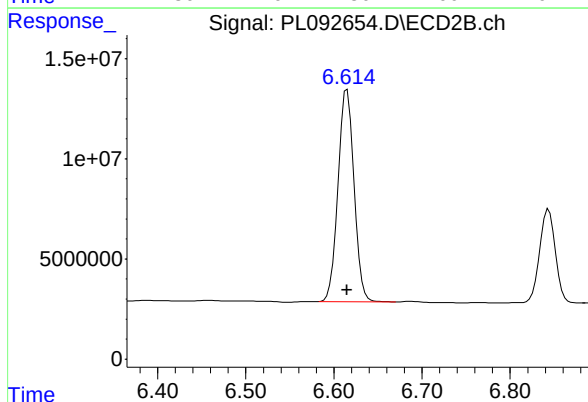


#20 Methoxychlor

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 134162458
Conc: 93.95 ng/ml

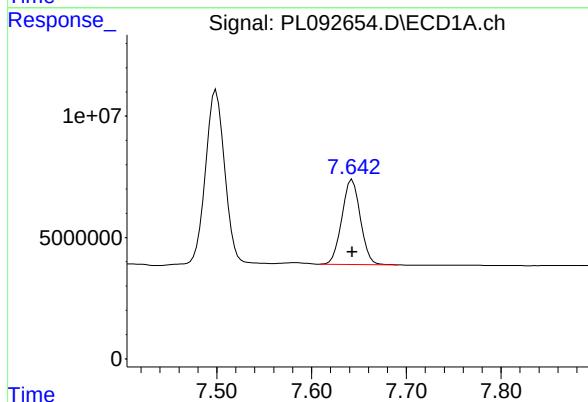


#21 Endrin ketone

R.T.: 7.643 min
Delta R.T.: 0.000 min
Response: 47240044
Conc: 19.50 ng/ml

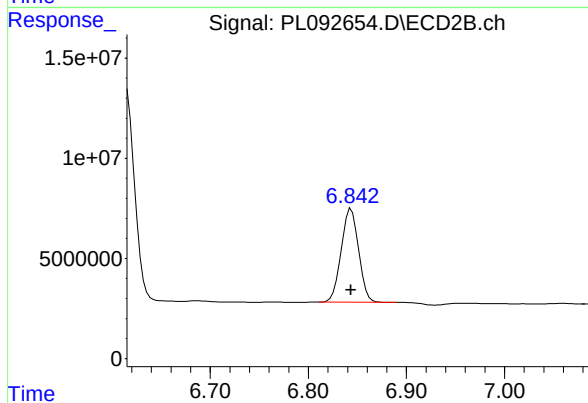

#21 Endrin ketone


R.T.: 6.844 min
Delta R.T.: 0.000 min
Response: 57600618
Conc: 18.77 ng/ml

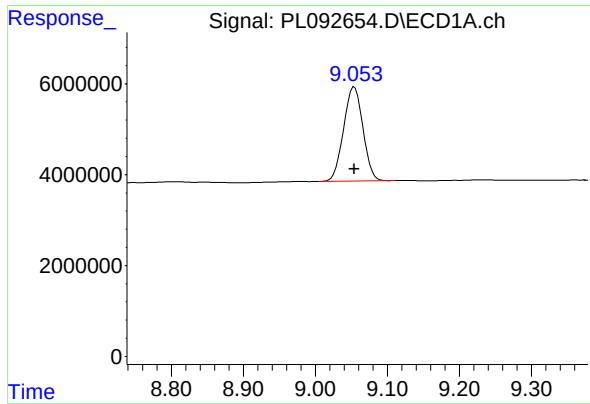

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 38629596
Conc: 20.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

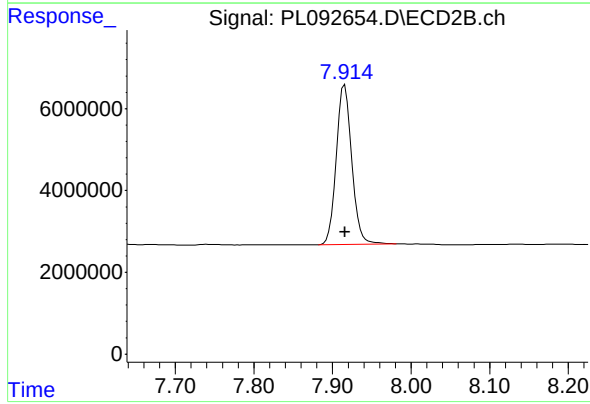

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 53476121
Conc: 19.59 ng/ml