


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101824\
Data File : BF139843.D
Acq On : 18 Oct 2024 09:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

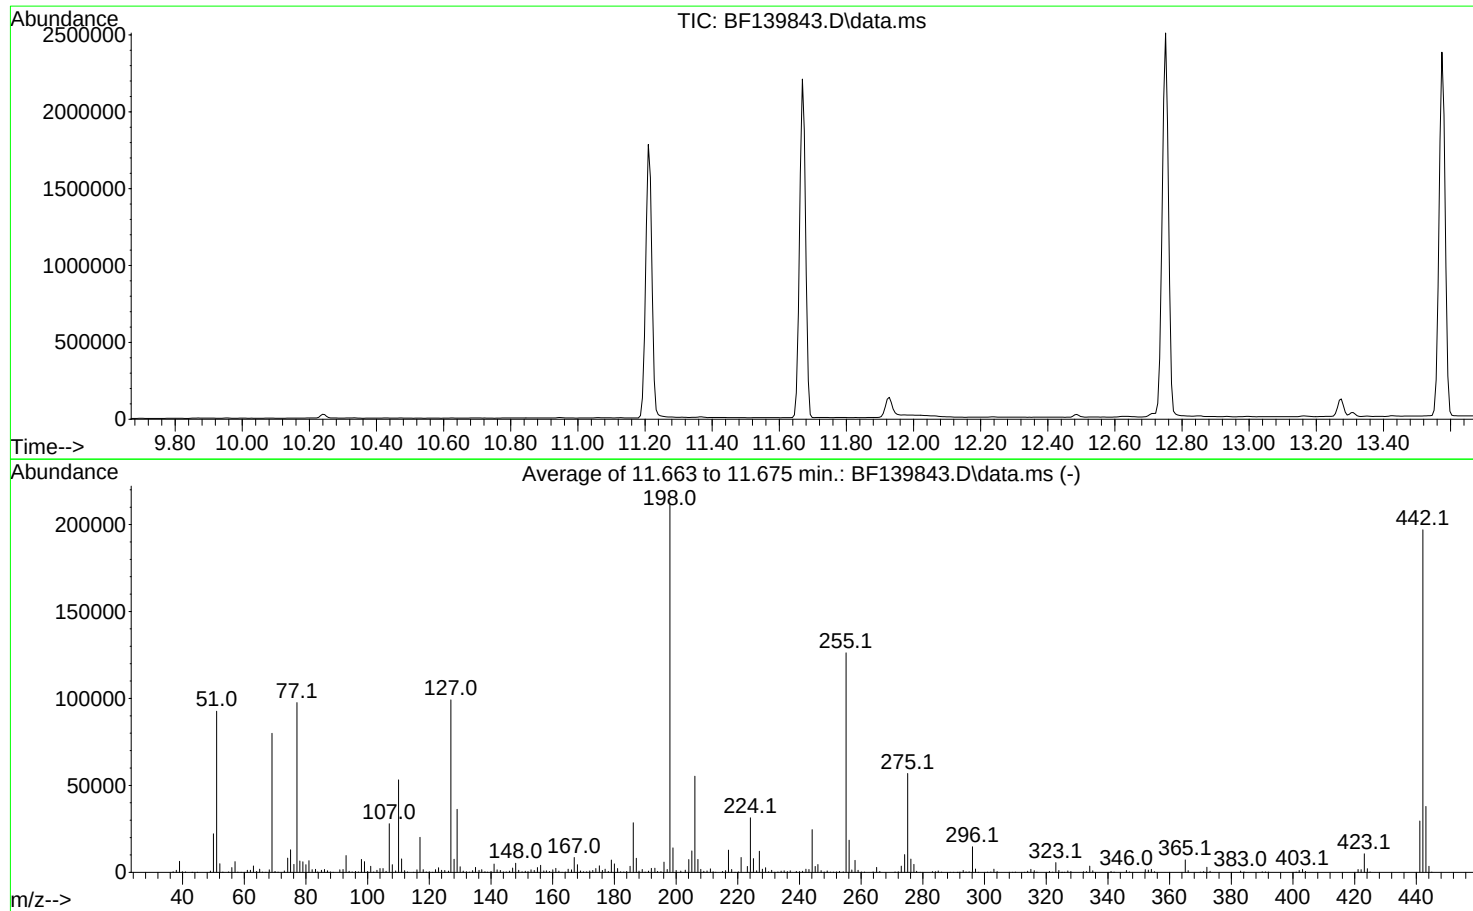

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	92701	PASS
68	69	0.00	2	1.9	1486	PASS
69	198	0.00	100	37.8	79959	PASS
70	69	0.00	2	0.7	529	PASS
127	198	10	80	46.9	99176	PASS
197	198	0.00	2	0.8	1650	PASS
198	198	100	100	100.0	211520	PASS
199	198	5	9	6.7	14078	PASS
275	198	10	60	26.9	56867	PASS
365	198	1	100	3.4	7148	PASS
441	198	0.01	100	14.0	29512	PASS
442	442	50	100	100.0	196979	PASS
443	442	15	24	19.2	37896	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/18/2024	BNA_F	<u>BF139843.D</u>
Compound Name	Response	Retention Time
DDT	585942	13.574
DDD	33558	13.274
DDE	421	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33979	619921	5.48

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101824\
Data File : BF139843.D
Acq On : 18 Oct 2024 09:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 18 11:03:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 11:03:04 2024
Response via : Initial Calibration

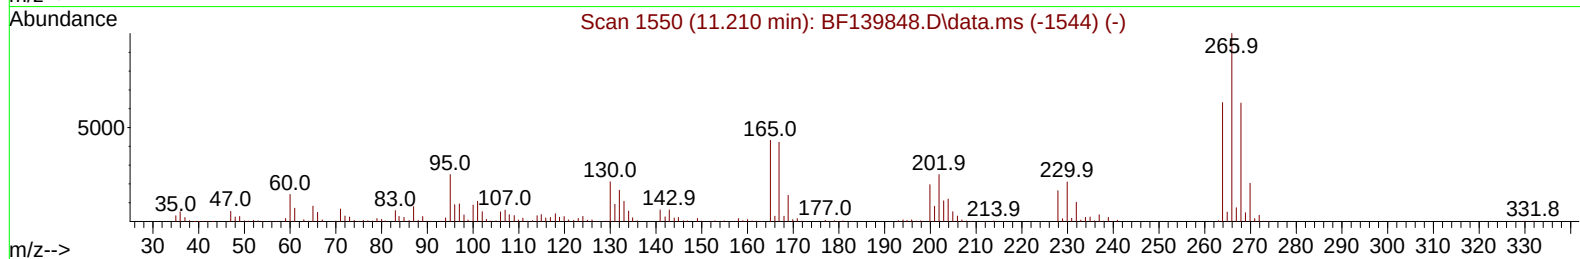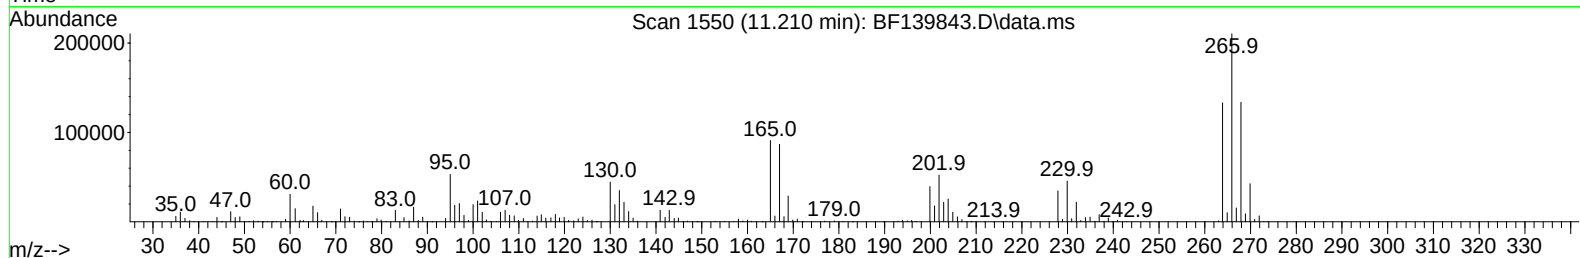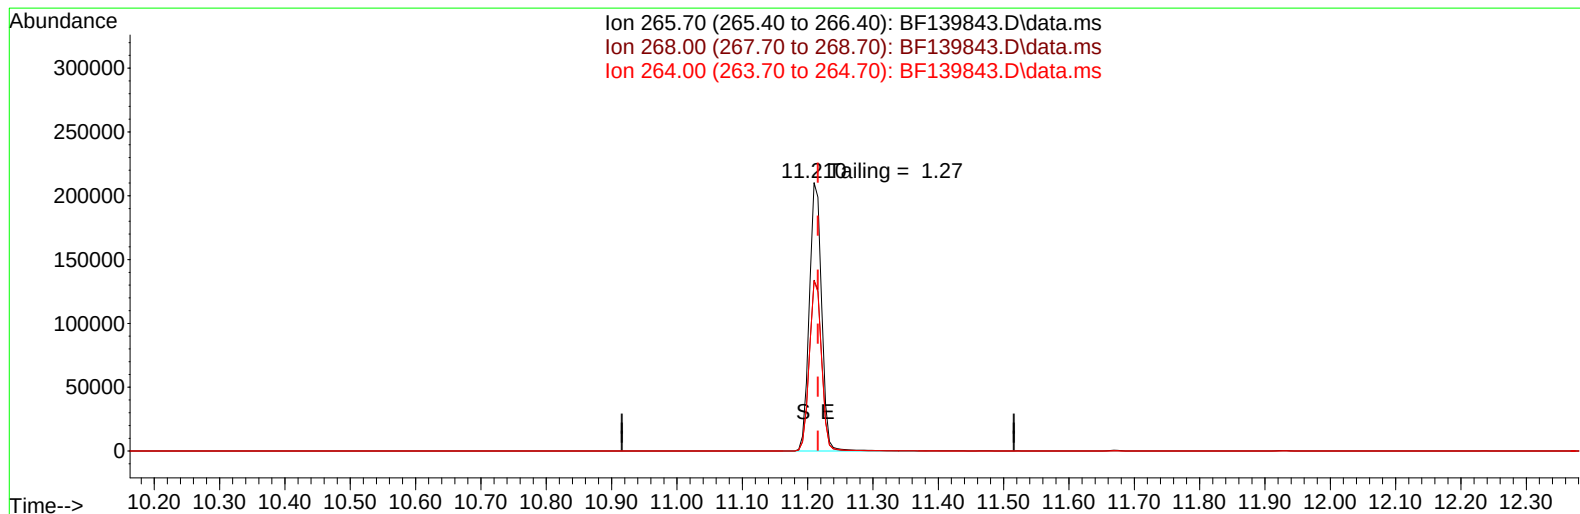

TIC: BF139843.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 60102.24 ng




response 277191

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.60
264.00	62.50	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101824\
Data File : BF139843.D
Acq On : 18 Oct 2024 09:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 18 11:03:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 11:03:04 2024
Response via : Initial Calibration

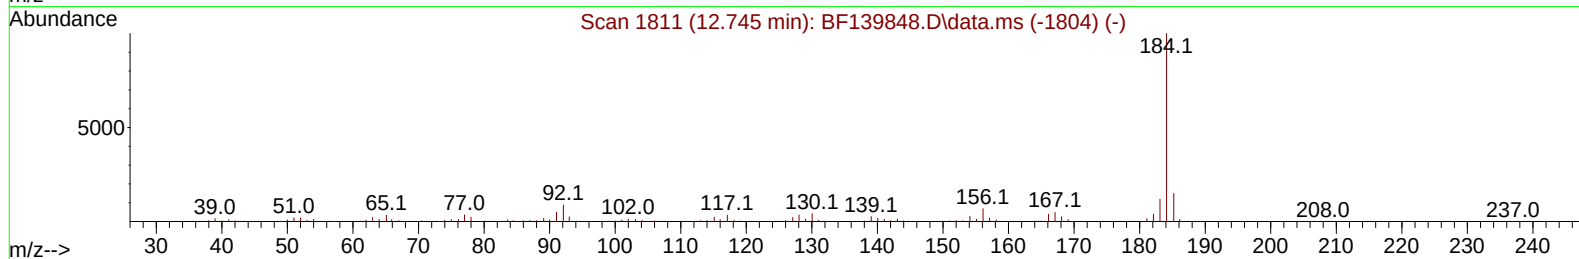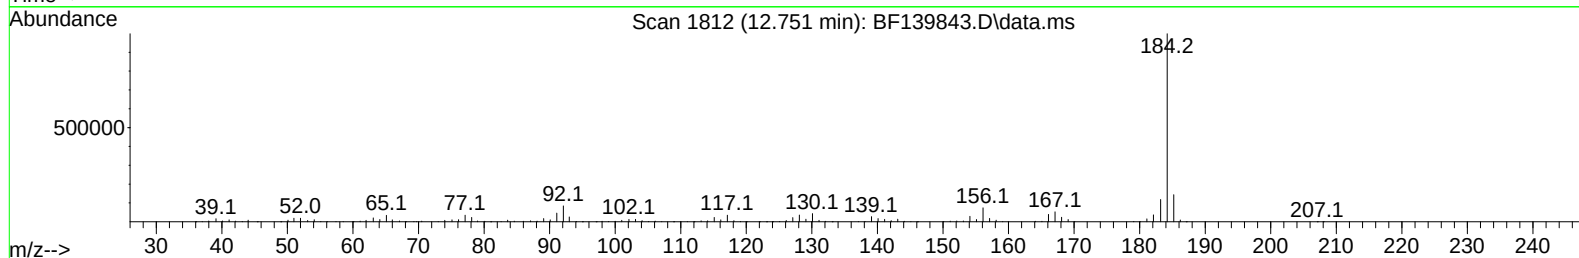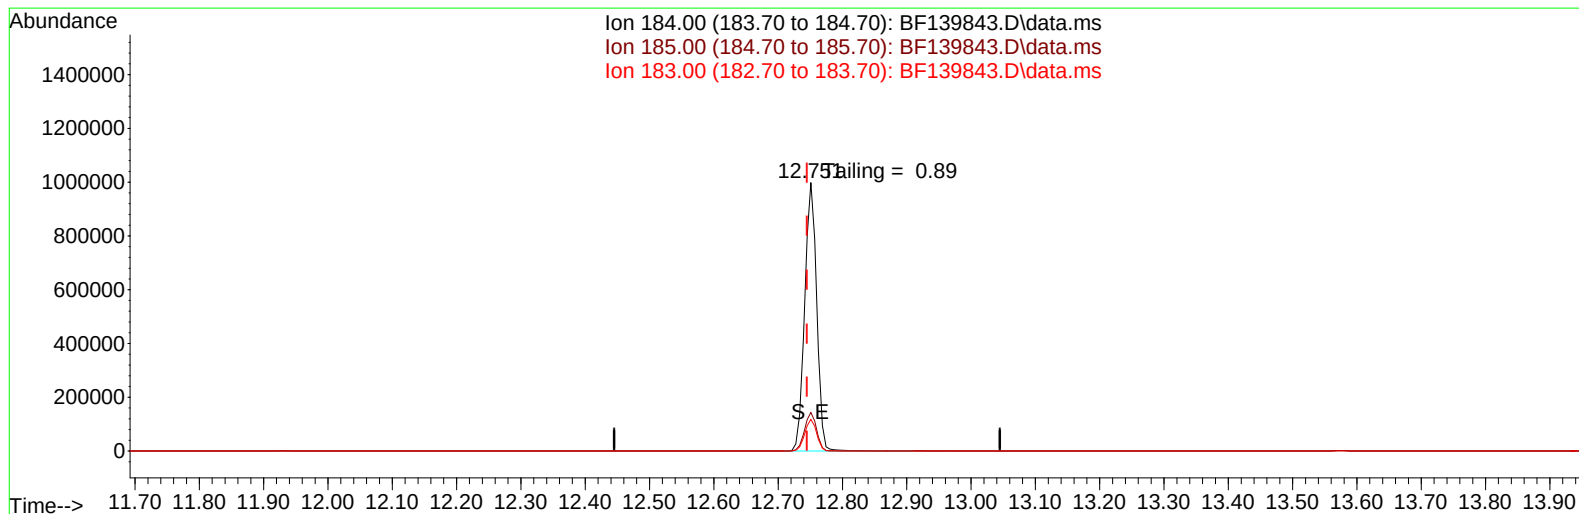

TIC: BF139843.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 86231.01 ng

response 1303015

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.39
183.00	11.70	11.82
0.00	0.00	0.00