


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111324\
Data File : BN035061.D
Acq On : 13 Nov 2024 12:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 17:18:14 2024

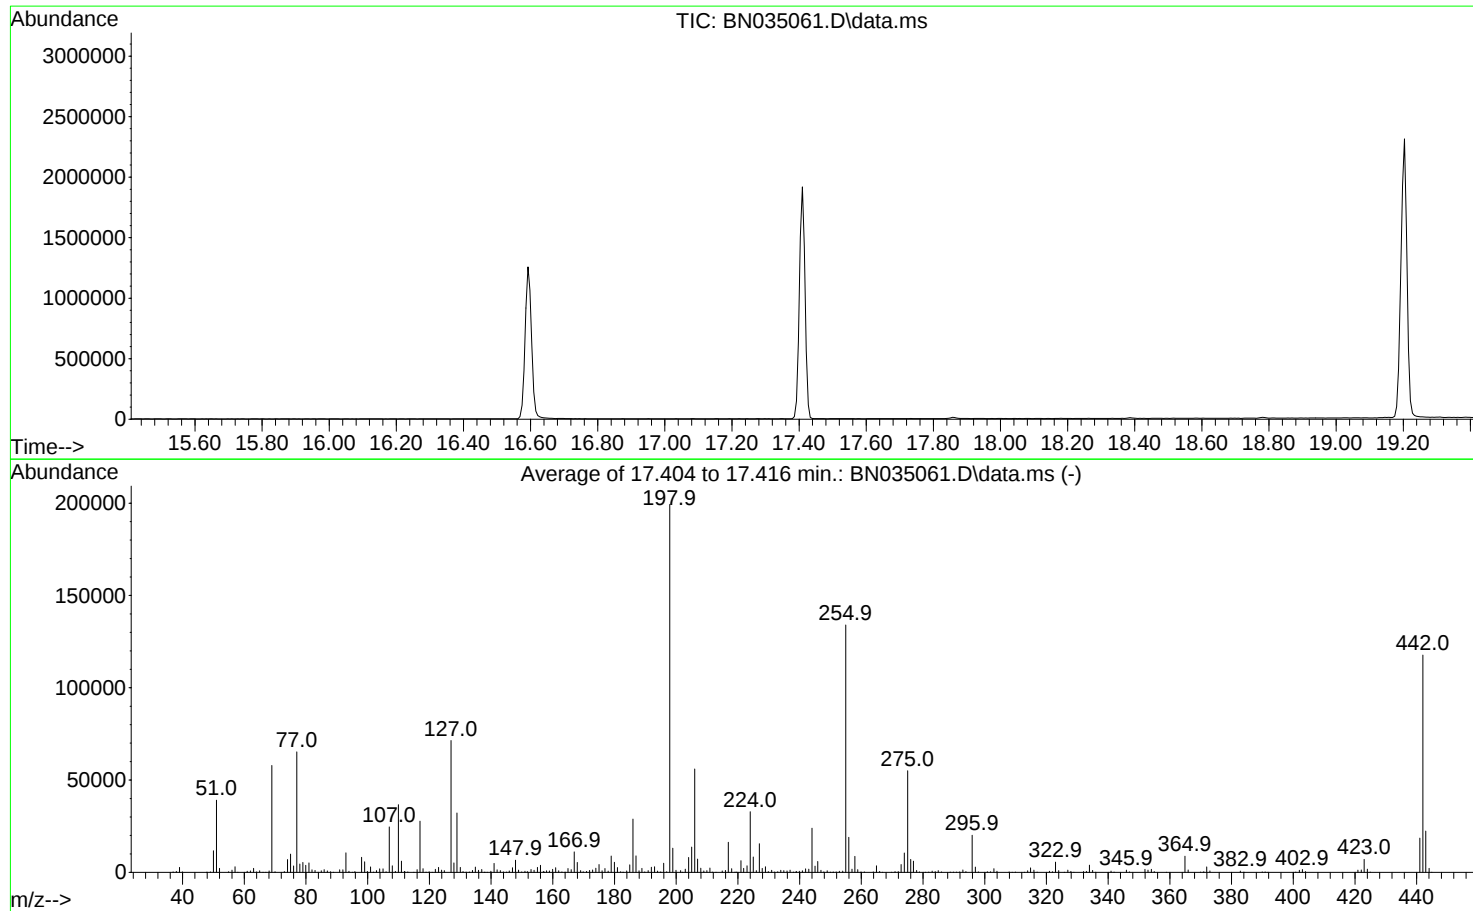




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.6	39078	PASS
68	69	0.00	2	1.4	807	PASS
69	198	0.00	100	29.1	57928	PASS
70	69	0.00	2	0.7	382	PASS
127	198	10	80	35.9	71451	PASS
197	198	0.00	2	0.2	365	PASS
198	198	100	100	100.0	199275	PASS
199	198	5	9	6.6	13094	PASS
275	198	10	60	27.6	55048	PASS
365	198	1	100	4.4	8801	PASS
441	198	0.01	100	9.3	18540	PASS
442	442	50	100	100.0	117725	PASS
443	442	15	24	19.0	22395	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111324\
Data File : BN035061.D
Acq On : 13 Nov 2024 12:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 14 15:14:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 04:05:27 2024
Response via : Initial Calibration

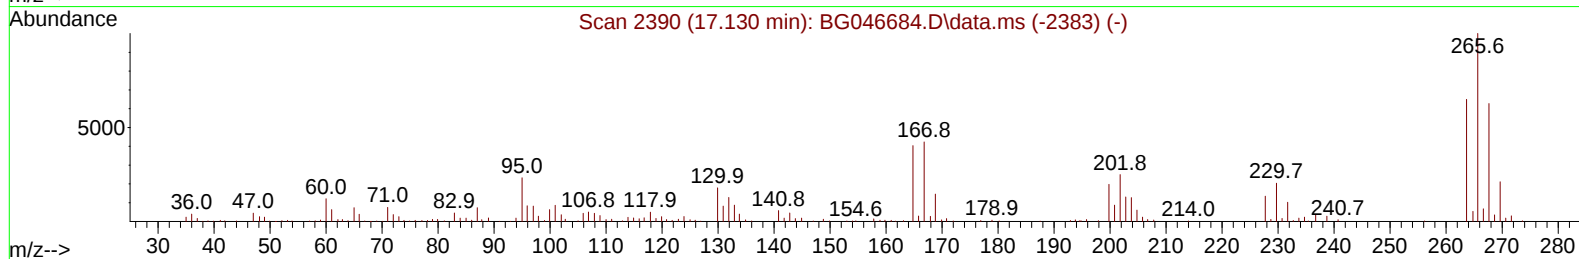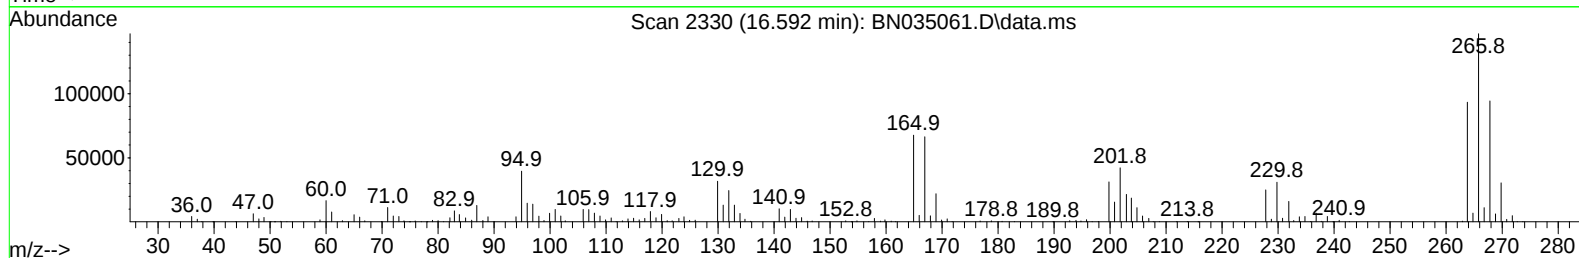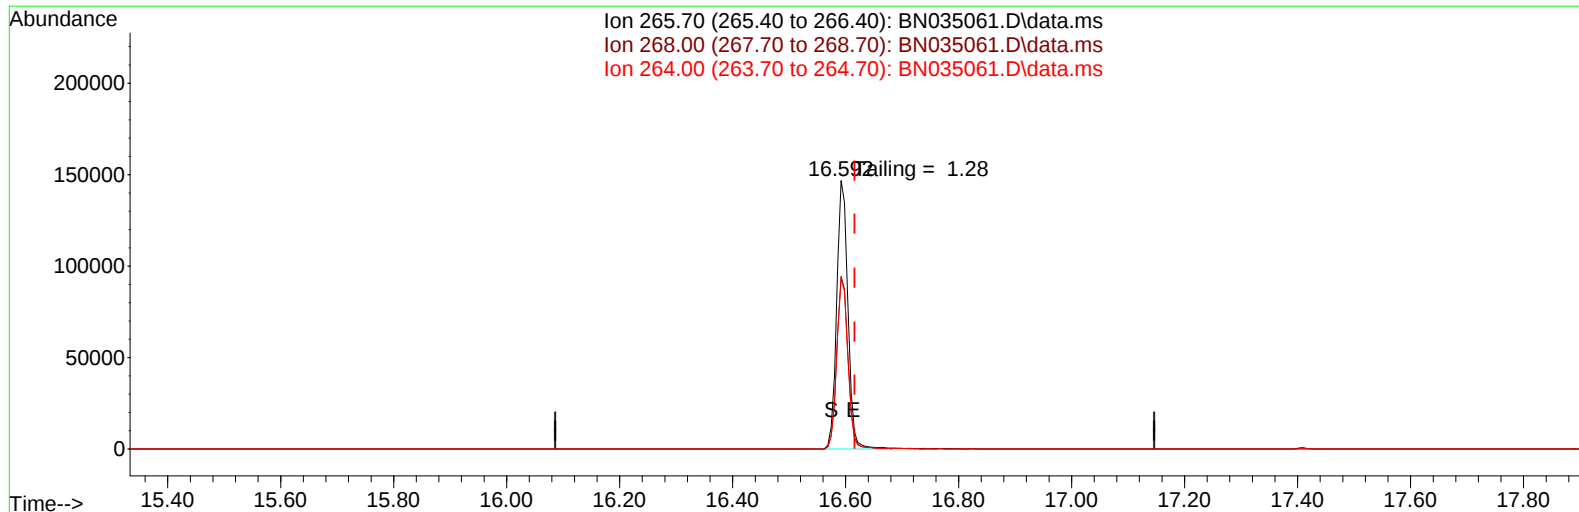

TIC: BN035061.D\data.ms

(70) Pentachlorophenol (C)

16.592min (-0.024) 20966.65 ng




response 202879

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.29
264.00	61.60	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111324\
Data File : BN035061.D
Acq On : 13 Nov 2024 12:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 14 15:14:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 04:05:27 2024
Response via : Initial Calibration

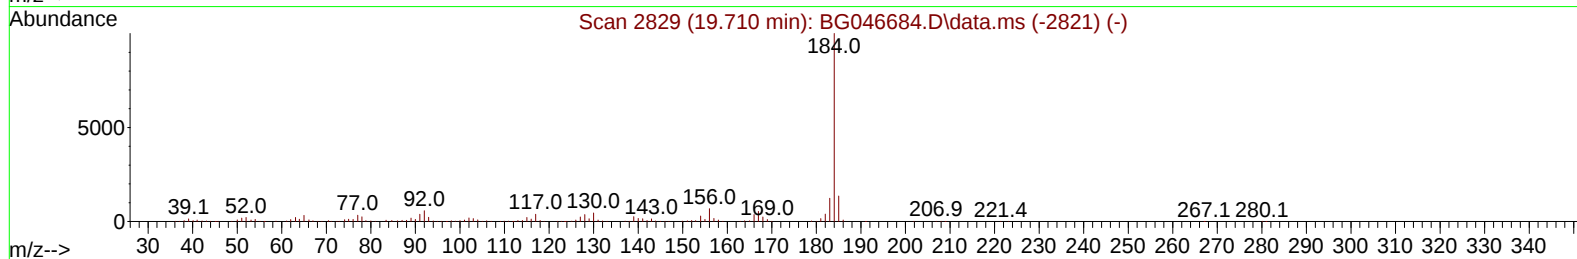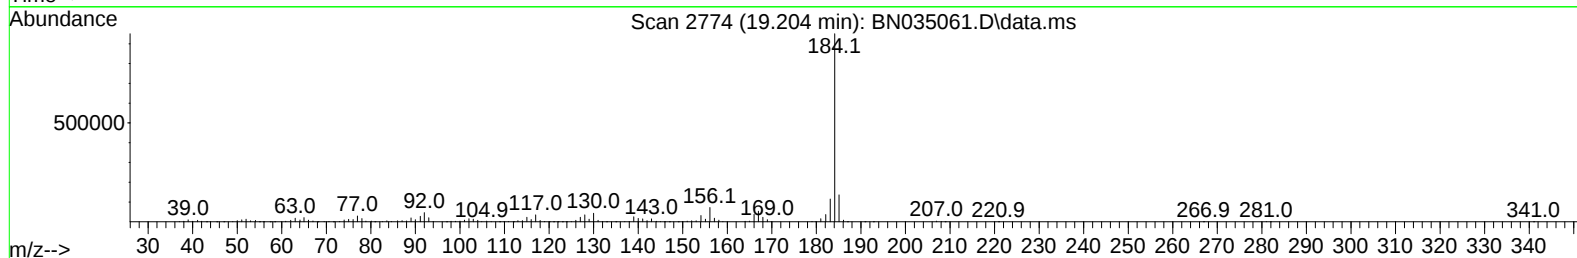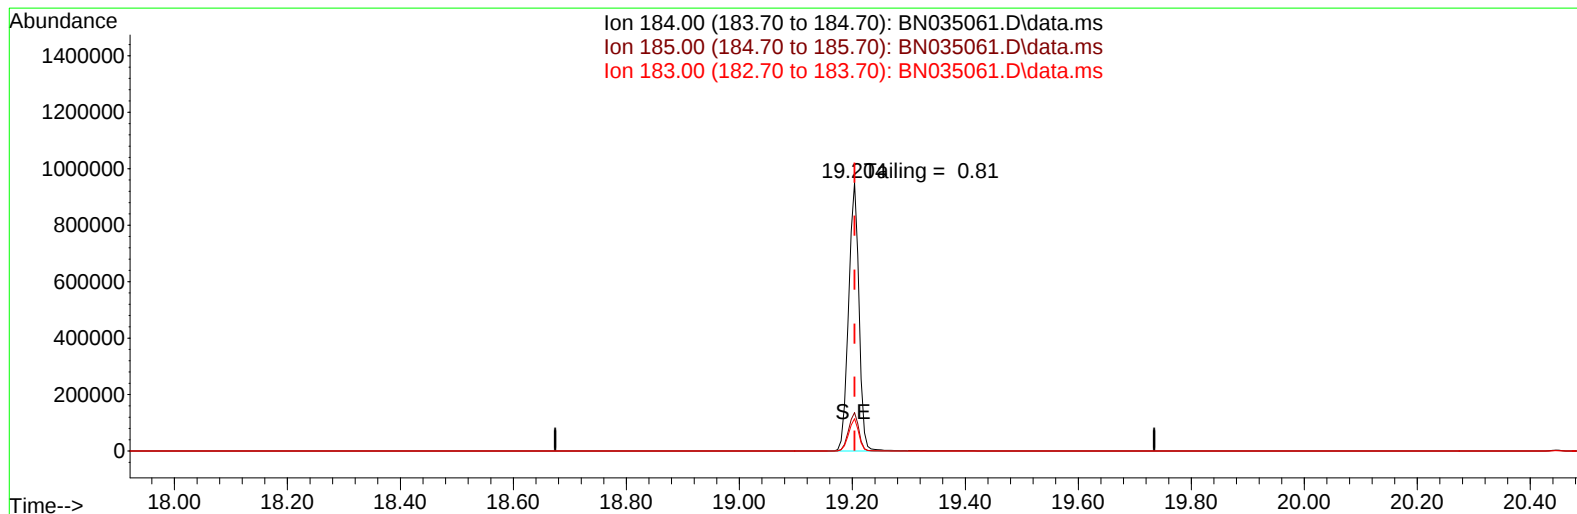

TIC: BN035061.D\data.ms

(77) Benzidine

19.204min (-0.000) 0.00 ng

response 1216684

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2024	BNA_N	<u>BN035561.D</u>
Compound Name	Response	Retention Time
DDT	699321	20.445
DDD	6440	20.057
DDE	0	19.527
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6440	705761	0.91

Instrument :
BNA_N
ClientSampleId :
DFTPP