
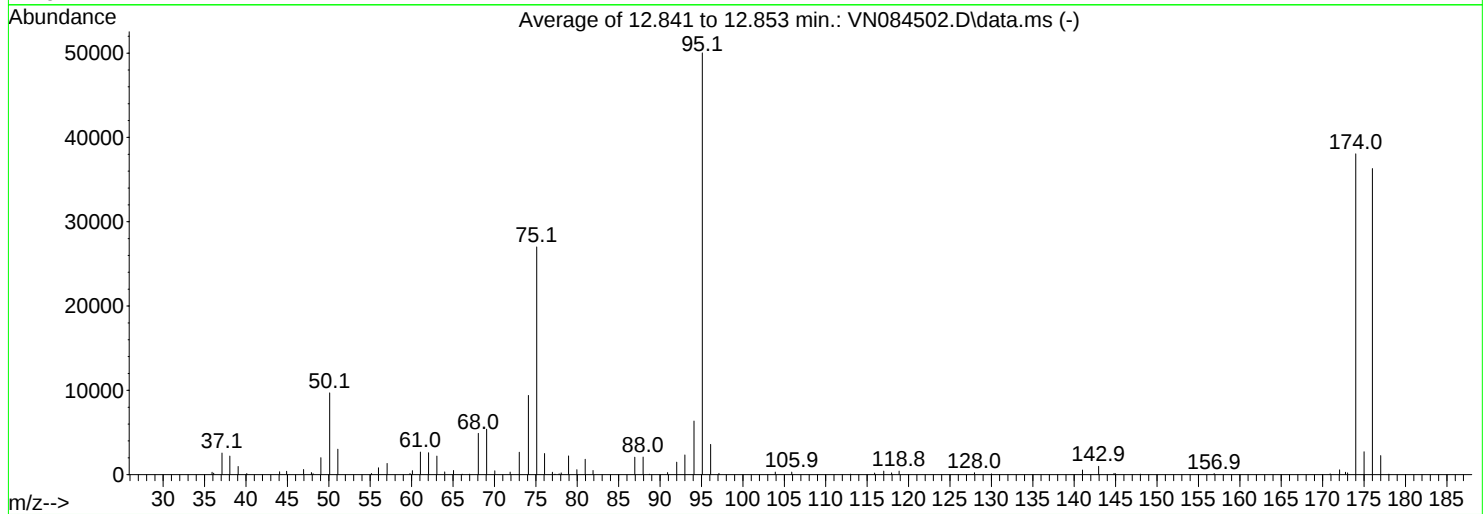


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102524\
Data File : VN084502.D
Acq On : 25 Oct 2024 08:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

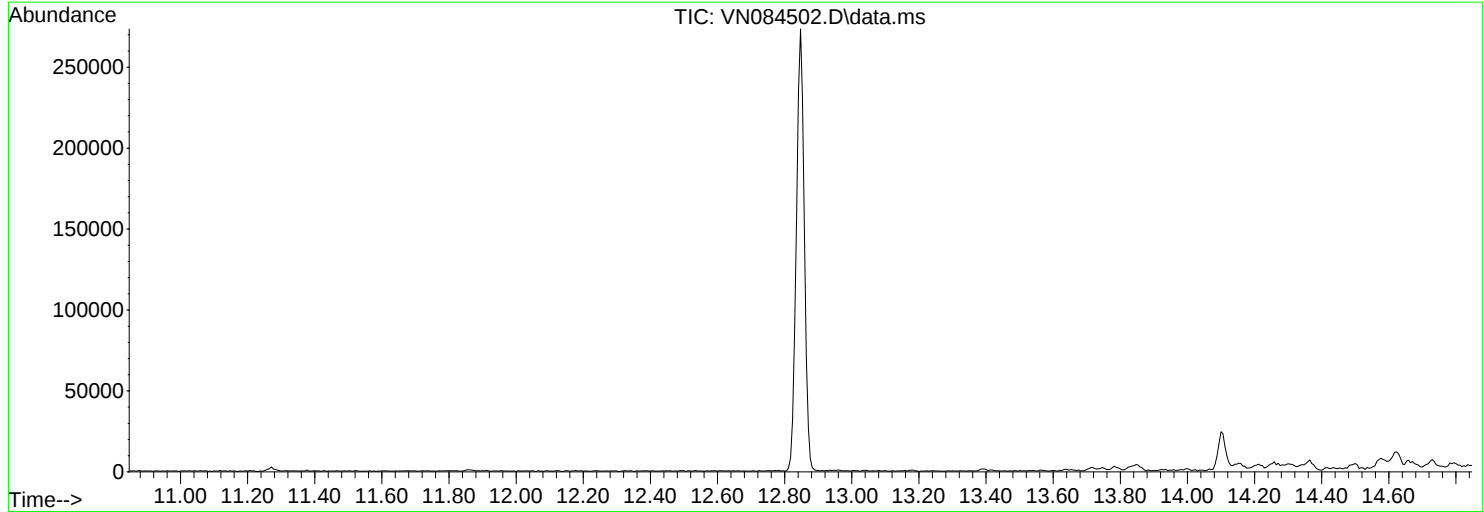

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	9707	PASS
75	95	30	60	54.0	27013	PASS
95	95	100	100	100.0	50032	PASS
96	95	5	9	7.2	3591	PASS
173	174	0.00	2	0.7	282	PASS
174	95	50	100	76.0	38048	PASS
175	174	5	9	7.1	2716	PASS
176	174	95	101	95.4	36315	PASS
177	176	5	9	6.2	2254	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	294	49.05	2007	64.00	332	76.05	2501
36.10	164	50.10	9707	65.05	491	77.00	2841
37.10	2565	51.10	3013	66.10	56	77.30	61
38.05	2205	55.15	142	67.00	56	77.80	92
39.05	964	56.00	826	68.05	4890	78.05	207
40.10	143	57.05	1321	69.05	5382	78.95	2215
44.05	345	59.80	128	70.05	462	79.95	596
44.90	395	60.10	473	71.90	311	80.95	1825
46.95	600	61.05	2683	73.00	2658	81.90	489
47.90	241	62.05	2607	74.10	9393	86.95	2073
48.10	110	63.05	2197	75.10	27013	87.95	2085

Average of 12.841 to 12.853 min.: VN084502.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.70	61	115.90	187	156.90	134		
90.90	252	117.00	415	170.90	93		
92.00	1476	117.95	206	172.05	569		
93.00	2335	118.85	420	172.75	282		
94.10	6368	127.95	234	173.00	213		
95.10	50032	130.00	105	174.00	38048		
96.10	3591	141.00	543	175.00	2716		
97.10	161	142.95	993	176.00	36315		
103.90	297	144.80	144	177.00	2254		
105.90	305	144.95	136	178.00	52		
113.00	57	148.00	58				

Instrument :

MSVOA_N

ClientSampleId :

BFB