
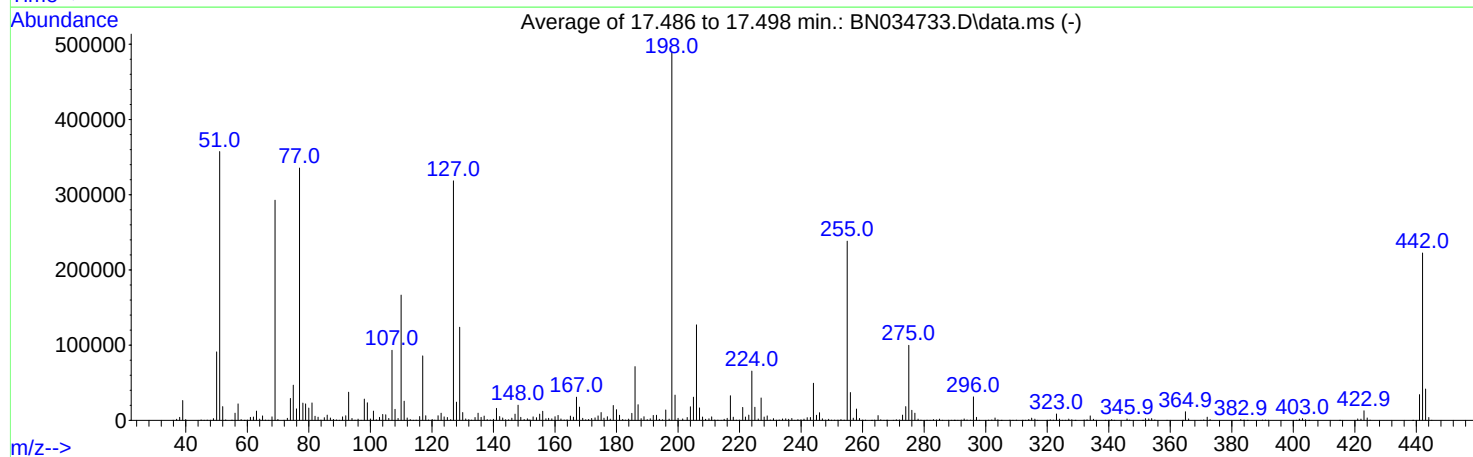


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102524\
Data File : BN034733.D
Acq On : 26 Oct 2024 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 28 00:44:15 2024

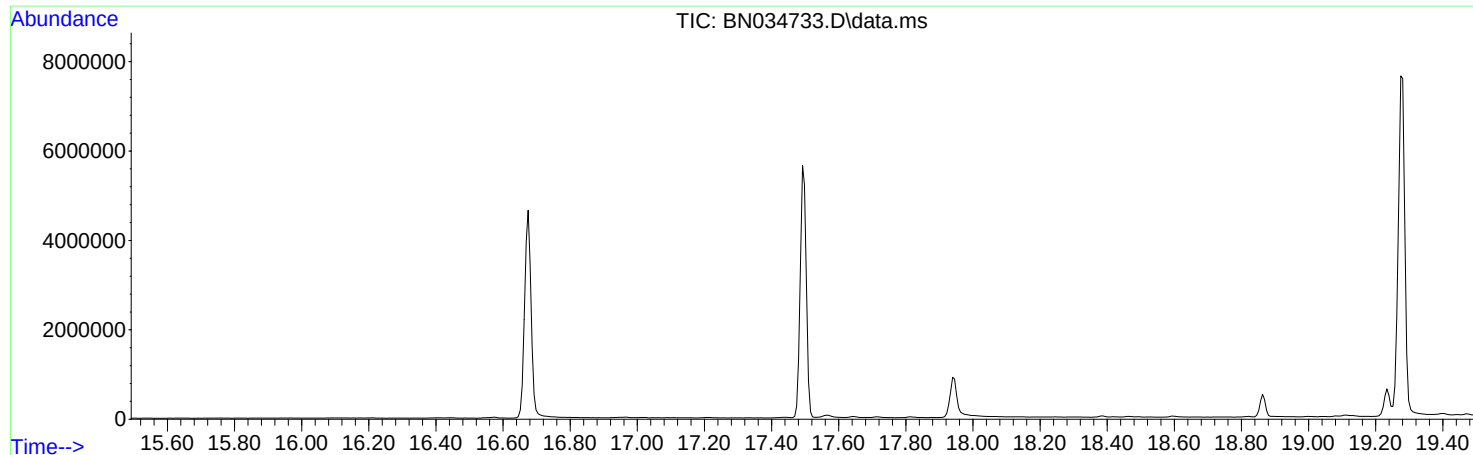




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	73.1	357461	PASS
68	69	0.00	2	1.6	4669	PASS
69	198	0.00	100	59.9	292804	PASS
70	69	0.00	2	0.4	1190	PASS
127	198	10	80	65.1	318485	PASS
197	198	0.00	2	0.4	1781	PASS
198	198	100	100	100.0	489045	PASS
199	198	5	9	6.9	33523	PASS
275	198	10	60	20.4	99795	PASS
365	198	1	100	2.4	11574	PASS
441	198	0.01	100	7.0	34328	PASS
442	442	50	100	100.0	222520	PASS
443	442	15	24	18.8	41749	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102524\
Data File : BN034733.D
Acq On : 26 Oct 2024 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 28 00:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 28 00:36:54 2024
Response via : Initial Calibration

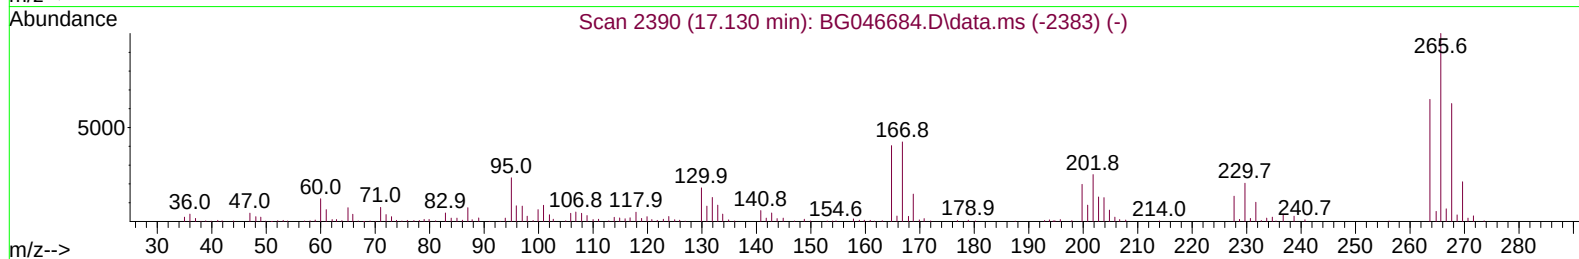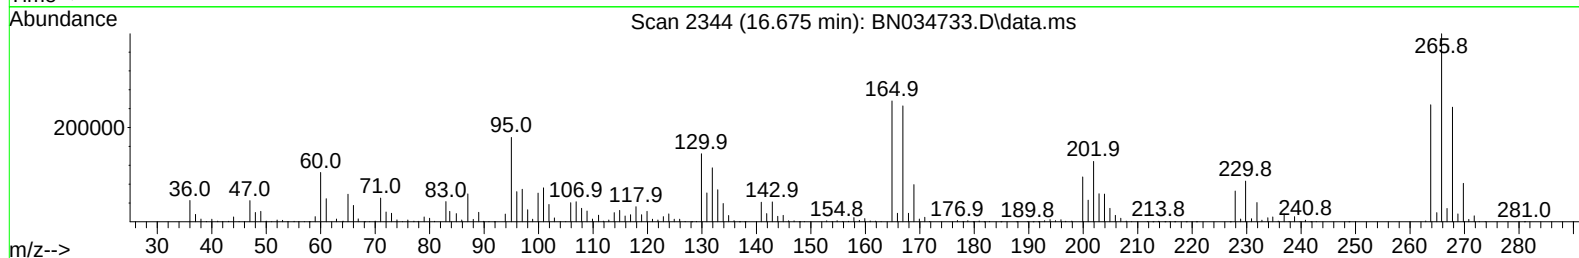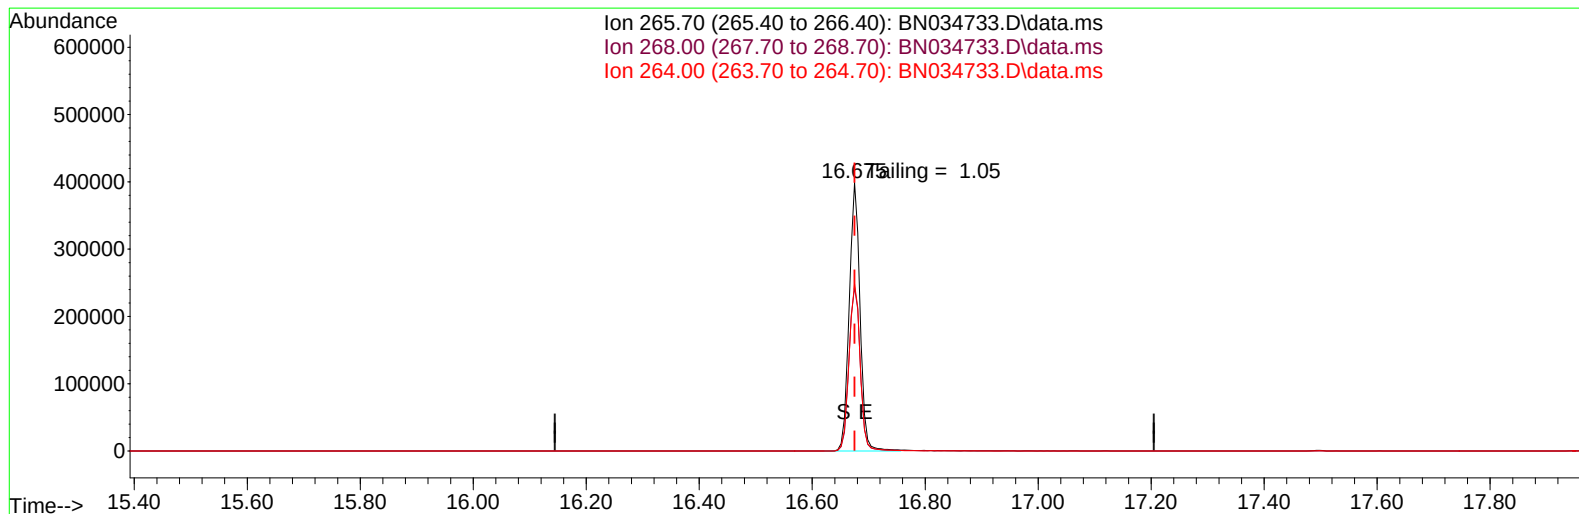

TIC: BN034733.D\data.ms

(70) Pentachlorophenol (C)

16.675min (0.000) 21413.45 ng




response 535399

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.98
264.00	61.60	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102524\
Data File : BN034733.D
Acq On : 26 Oct 2024 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 28 00:37:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 28 00:36:54 2024
Response via : Initial Calibration

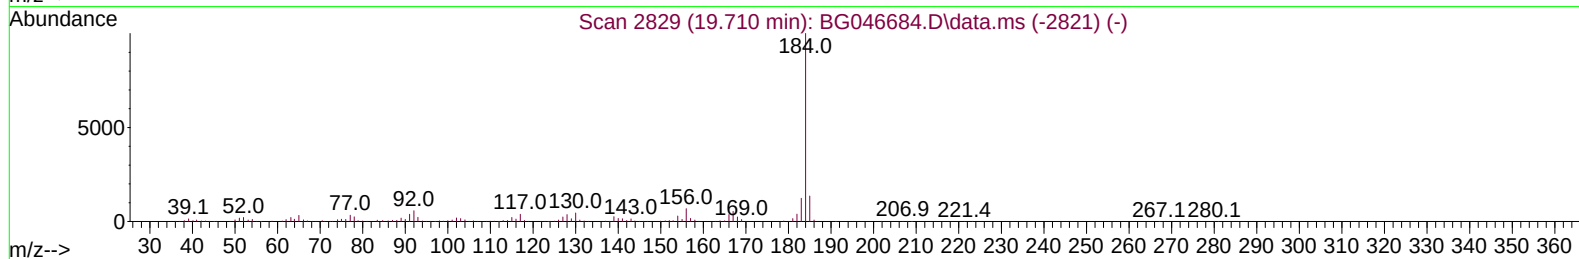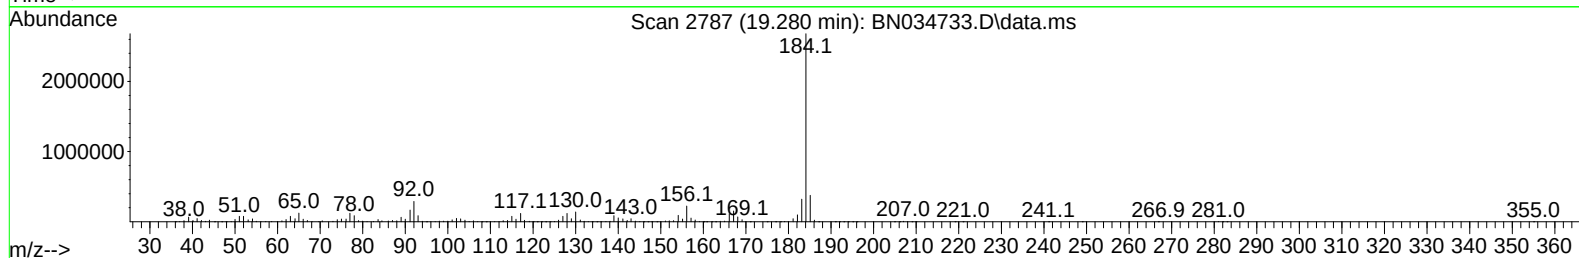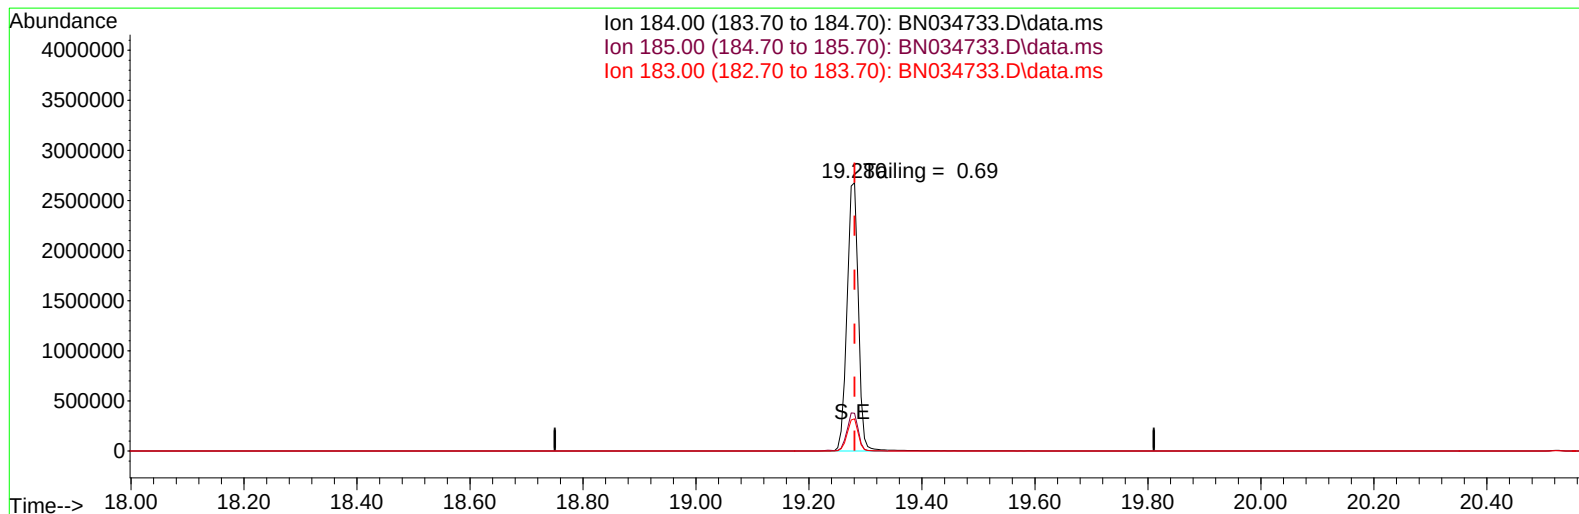

TIC: BN034733.D\data.ms

(77) Benzidine

19.280min (0.000) 0.00 ng

response 3728042

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/25/2024	BNA_N	<u>BN034733.D</u>
Compound Name	Response	Retention Time
DDT	1627373	20.527
DDD	33067	20.08
DDE	1197	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34264	1661637	2.06

Instrument :
BNA_N
ClientSampleId :
DFTPP