

Prep Standard - Chemical Standard Summary

Order ID : P4578

Test : EPH

Prepbatch ID : PB164525,PB164532,

Sequence ID/Qc Batch ID: FC103024AL,FD103024AR,FE103024AL,FE103124AL,FE110124AL,FG103024AR,FG103124AR,

Standard ID :

EP2517,EP2538,EP2546,EP2554,PP23429,PP23430,PP23519,PP23520,PP23521,PP23522,PP23523,PP23534,PP23538,PP23644,PP23645,PP23646,PP23647,PP23648,PP23649,PP23650,PP23704,PP23706,PP23712,PP23892,PP23916,

Chemical ID :

E2865,E3551,E3743,E3757,E3768,E3788,E3789,E3793,E3794,E3819,E3822,M5929,P10259,P11137,P12362,P12972,P13004,P13005,P13017,P13018,P13019,P13020,P13022,P13044,P13045,P13047,P13048,P13094,P13096,P13098,P13100,P13101,P13102,P13258,P13259,P13266,P13268,P13271,P13278,P13299,P13423,P13424,P13427,P13430,P13431,P13432,P13433,P13434,P13435,P13436,P13442,P13444,P13447,P13448,P13451,P13452,P13453,P13454,P13455,P13456,P13473,P13625,P13626,P13627,P13718,P13719,P13720,P13721,P13722,P13723,P13724,P13725,P13726,P13727,P9826,V11252,V14143,W3112,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3319	6N HCL	EP2517	07/23/2024	12/08/2024	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 07/23/2024

FROM 219.00000ml of M5929 + 781.00000ml of W3112 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3868	METHELENE CHLORIDE+ACETONE	EP2538	09/17/2024	03/11/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 09/17/2024

FROM 8000.00000ml of E3793 + 8000.00000ml of E3794 = Final Quantity: 1600.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2546	10/11/2024	01/03/2025	RUPESHKUMAR SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Rajesh Parikh 10/11/2024
<u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2554	10/26/2024	01/03/2025	RUPESHKUMAR SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Rajesh Parikh 10/26/2024
<u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
782	100 PPM Aromatic HC Working STD	PP23429	05/21/2024	11/16/2024	Yogesh Patel	None	None	Ankita Jodhani
								05/24/2024

FROM 0.25000ml of P13004 + 0.62500ml of P13259 + 1.25000ml of P10259 + 22.87500ml of E3743 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2945	100 PPM Aromatic HC Working STD (Absolute)	PP23430	05/21/2024	11/16/2024	Yogesh Patel	None	None	Ankita Jodhani
								05/24/2024

FROM 0.25000ml of P13005 + 0.62500ml of P13258 + 1.25000ml of P11137 + 22.87500ml of E3743 = Final Quantity: 25.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
787	50 PPM Aromatic HC STD	PP23519	07/15/2024	11/16/2024	Yogesh Patel	None	None	Ankita Jodhani
								07/16/2024

FROM 0.50000ml of E3768 + 0.50000ml of PP23429 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
788	20 PPM Aromatic HC STD	PP23520	07/15/2024	11/16/2024	Yogesh Patel	None	None	Ankita Jodhani
								07/16/2024

FROM 0.80000ml of E3768 + 0.20000ml of PP23429 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
789	10 PPM Aromatic HC STD	PP23521	07/15/2024	11/16/2024	Yogesh Patel	None	None	Ankita Jodhani
								07/16/2024

FROM 0.90000ml of E3768 + 0.10000ml of PP23429 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
790	5 PPM Aromatic HC STD	PP23522	07/15/2024	11/16/2024	Yogesh Patel	None	None	Ankita Jodhani
								07/16/2024

FROM 0.90000ml of E3768 + 0.10000ml of PP23519 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2946	20 PPM Aromatic HC STD ICV (Absolute)	PP23523	07/15/2024	11/16/2024	Yogesh Patel	None	None	Ankita Jodhani
								07/16/2024

FROM 0.80000ml of E3768 + 0.20000ml of PP23430 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
231	10 PPM GRO STD 1ST SOURCE	PP23534	07/29/2024	01/22/2025	Yogesh Patel	None	None	Ankita Jodhani
								07/30/2024

FROM 0.11100ml of P9826 + 9.89000ml of V14143 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3619	25 PPM AAA-TFT Surg	PP23538	07/29/2024	01/22/2025	Yogesh Patel	None	None	Ankita Jodhani
								07/30/2024

FROM 0.10000ml of V11252 + 9.90000ml of V14143 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
781	100 PPM Aliphatic HC Working STD (Restek)	PP23644	09/09/2024	02/13/2025	Yogesh Patel	None	None	Ankita Jodhani
								09/10/2024

FROM 0.25000ml of P12972 + 0.25000ml of P13017 + 1.25000ml of P12362 + 23.25000ml of E3789 = Final Quantity: 25.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2900	100 PPM Aliphatic HC STD (Absolute)	PP23645	09/09/2024	02/13/2025	Yogesh Patel	None	None	Ankita Jodhani
09/10/2024								

FROM 0.25000ml of P12972 + 0.25000ml of P13017 + 2.50000ml of P13278 + 22.00000ml of E3789 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
783	50 PPM Aliphatic HC STD	PP23646	09/09/2024	02/13/2025	Yogesh Patel	None	None	Ankita Jodhani
09/10/2024								

FROM 0.50000ml of E3789 + 0.50000ml of PP23644 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
784	20 PPM Aliphatic HC STD	PP23647	09/09/2024	02/13/2025	Yogesh Patel	None	None	Ankita Jodhani
								09/10/2024

FROM 0.80000ml of E3789 + 0.20000ml of PP23644 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
785	10 PPM Aliphatic HC STD	PP23648	09/09/2024	02/13/2025	Yogesh Patel	None	None	Ankita Jodhani
								09/10/2024

FROM 0.90000ml of E3789 + 0.10000ml of PP23644 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
786	5 PPM Aliphatic HC STD	PP23649	09/09/2024	02/13/2025	Yogesh Patel	None	None	Ankita Jodhani
09/10/2024								

FROM 0.90000ml of E3789 + 0.10000ml of PP23646 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2901	20 PPM Aliphatic HC STD ICV (Absolute)	PP23650	09/09/2024	02/13/2025	Yogesh Patel	None	None	Ankita Jodhani
09/10/2024								

FROM 0.80000ml of E3789 + 0.20000ml of PP23645 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
234	100 PPB ICC GRO STD	PP23704	09/24/2024	01/22/2025	Yogesh Patel	None	None	Ankita Jodhani
								10/01/2024

FROM 5.00000ml of W3112 + 0.02000ml of PP23538 + 0.05000ml of PP23534 = Final Quantity: 5.070 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1339	100 PPM NJEPH Surrogate Spike	PP23706	09/26/2024	02/13/2025	Yogesh Patel	None	None	Ankita Jodhani
								10/01/2024

FROM 1.25000ml of P13018 + 1.25000ml of P13019 + 1.25000ml of P13020 + 1.25000ml of P13022 + 1.25000ml of P13044 +
1.25000ml of P13045 + 1.25000ml of P13047 + 1.25000ml of P13048 + 490.00000ml of E3788 = Final Quantity: 500.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1330	100 PPM NJEPH Spike Solution	PP23712	09/30/2024	03/30/2025	Yogesh Patel	None	None	Ankita Jodhani 10/01/2024
<u>FROM</u>	5.00000ml of P13094 + 5.00000ml of P13096 + 5.00000ml of P13424 + 5.00000ml of P13430 + 5.00000ml of P13431 + 5.00000ml of P13432 + 5.00000ml of P13433 + 5.00000ml of P13434 + 5.00000ml of P13435 + 5.00000ml of P13436 + 5.00000ml of P13442 + 5.00000ml of P13444 + 5.00000ml of P13447 + 5.00000ml of P13448 + 5.00000ml of P13451 + 5.00000ml of P13452 + 5.00000ml of P13453 + 5.00000ml of P13454 + 5.00000ml of P13455 + 5.00000ml of P13456 = Final Quantity: 100.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1331	100 PPM NJEPH Fractionating Surrogate	PP23892	10/17/2024	04/15/2025	Yogesh Patel	None	None	Ankita Jodhani 10/18/2024
<u>FROM</u>	1.25000ml of P13266 + 1.25000ml of P13268 + 1.25000ml of P13271 + 1.25000ml of P13473 + 195.00000ml of E3819 = Final Quantity: 200.000 ml							



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1330	100 PPM NJEPH Spike Solution	PP23916	10/25/2024	04/25/2025	Yogesh Patel	None	None	Ankita Jodhani 10/28/2024
<p><u>FROM</u> 5.00000ml of P13098 + 5.00000ml of P13100 + 5.00000ml of P13101 + 5.00000ml of P13102 + 5.00000ml of P13299 + 5.00000ml of P13423 + 5.00000ml of P13427 + 5.00000ml of P13625 + 5.00000ml of P13626 + 5.00000ml of P13627 + 5.00000ml of P13718 + 5.00000ml of P13719 + 5.00000ml of P13720 + 5.00000ml of P13721 + 5.00000ml of P13722 + 5.00000ml of P13723 + 5.00000ml of P13724 + 5.00000ml of P13725 + 5.00000ml of P13726 + 5.00000ml of P13727 = Final Quantity: 100.000 ml</p>								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	01/03/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24C0162011	11/16/2024	05/16/2024 / Rajesh	04/26/2024 / Rajesh	E3743

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
phenomenex	SI500025-30 / Cleanert SPE Silica, 5000 mg/25 ml	Z0513CK1	03/04/2025	09/04/2024 / Rajesh	04/03/2024 / Rajesh	E3757

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24E2462004	01/08/2025	07/08/2024 / Rajesh	06/21/2024 / Rajesh	E3768

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	23H1462005	04/23/2025	08/13/2024 / Rajesh	08/13/2024 / Rajesh	E3788

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	02/13/2025	08/13/2024 / Rajesh	08/13/2024 / Rajesh	E3789

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	03/11/2025	09/12/2024 / Rajesh	09/11/2024 / Rajesh	E3793

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24G2362009	03/17/2025	09/17/2024 / Rajesh	09/03/2024 / Rajesh	E3794

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	04/15/2025	10/15/2024 / Rajesh	10/09/2024 / Rajesh	E3819

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24I2662006	04/23/2025	10/24/2024 / Rajesh	10/24/2024 / Rajesh	E3822

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	22G2862015	12/08/2024	06/24/2024 / Al-Terek	06/07/2024 / Al-Terek	M5929

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30541 / Custom NJEPH Aromatics Calibration Standard	A0165529	11/21/2024	05/21/2024 / yogesh	01/26/2021 / dhaval	P10259

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95709 / NJ EPH Aromatic Hydrocarbons, 2000 PPM	060420	07/08/2024	01/08/2024 / yogesh	10/29/2021 / Abdul	P11137

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30540 / Custom NJEPH Aliphatics Calibration Standard	A0190424	03/09/2025	09/09/2024 / yogesh	03/16/2023 / Yogesh	P12362

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0204989	03/09/2025	09/09/2024 / yogesh	12/20/2023 / Yogesh	P12972

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0204177	11/21/2024	05/21/2024 / yogesh	12/21/2023 / Yogesh	P13004

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0204177	11/21/2024	05/21/2024 / yogesh	12/21/2023 / Yogesh	P13005

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0204177	03/09/2025	09/09/2024 / yogesh	12/21/2023 / Yogesh	P13017

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0204177	03/26/2025	09/26/2024 / yogesh	12/21/2023 / Yogesh	P13018

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0204177	03/26/2025	09/26/2024 / yogesh	12/21/2023 / Yogesh	P13019

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0204177	03/26/2025	09/26/2024 / yogesh	12/21/2023 / Yogesh	P13020

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0204177	03/26/2025	09/26/2024 / yogesh	12/21/2023 / Yogesh	P13022

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0200707	03/26/2025	09/26/2024 / yogesh	12/26/2023 / Yogesh	P13044

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0200707	03/26/2025	09/26/2024 / yogesh	12/26/2023 / Yogesh	P13045

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0200707	03/26/2025	09/26/2024 / yogesh	12/26/2023 / Yogesh	P13047

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0200707	03/26/2025	09/26/2024 / yogesh	12/26/2023 / Yogesh	P13048

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0203911	03/30/2025	09/30/2024 / yogesh	01/12/2024 / Yogesh	P13094

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0203911	03/30/2025	09/30/2024 / yogesh	01/12/2024 / Yogesh	P13096

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0203911	04/25/2025	10/25/2024 / yogesh	01/12/2024 / Yogesh	P13098

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0200008	04/25/2025	10/25/2024 / yogesh	01/12/2024 / Yogesh	P13100

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0200008	04/25/2025	10/25/2024 / yogesh	01/12/2024 / Yogesh	P13101

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0200008	04/25/2025	10/25/2024 / yogesh	01/12/2024 / Yogesh	P13102

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0206496	11/21/2024	05/21/2024 / yogesh	02/20/2024 / yogesh	P13258

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0206496	11/21/2024	05/21/2024 / yogesh	02/20/2024 / yogesh	P13259

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0206496	04/17/2025	10/17/2024 / yogesh	02/20/2024 / yogesh	P13266

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0206496	04/17/2025	10/17/2024 / yogesh	02/20/2024 / yogesh	P13268

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0206496	04/17/2025	10/17/2024 / yogesh	02/20/2024 / yogesh	P13271

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95899 / NJ EPH Aliphatic n-Hydrocarbons-Revised, 1000 PPM	040524	03/09/2025	09/09/2024 / yogesh	04/11/2024 / yogesh	P13278

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0207239	04/25/2025	10/25/2024 / yogesh	04/23/2024 / yogesh	P13299

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0207239	04/25/2025	10/25/2024 / yogesh	07/16/2024 / Yogesh	P13423

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0207239	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13424

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0207239	04/25/2025	10/25/2024 / yogesh	07/16/2024 / Yogesh	P13427

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13430

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13431

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13432

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13433

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13434

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13435

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13436

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13442

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13444

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13447

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13448

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13451

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13452

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0207019	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13453

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0207019	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13454

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0207019	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13455

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0207019	03/30/2025	09/30/2024 / yogesh	07/16/2024 / Yogesh	P13456

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0210831	04/17/2025	10/17/2024 / yogesh	07/23/2024 / yogesh	P13473

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	04/25/2025	10/25/2024 / yogesh	10/16/2024 / yogesh	P13625

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	04/25/2025	10/25/2024 / yogesh	10/16/2024 / yogesh	P13626

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0211112	04/25/2025	10/25/2024 / yogesh	10/16/2024 / yogesh	P13627

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13718

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13719

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13720

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13721

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13722

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13723

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13724

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13725

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13726

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0217838	04/25/2025	10/25/2024 / yogesh	10/24/2024 / yogesh	P13727

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30065 / GRO Mix (EPA)	A0155991	01/25/2025	07/25/2024 / yogesh	09/11/2020 / DHAVAL	P9826

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30068 / VOA Mix, a, a, a-trifluorotoluene 2500ug/ml, P&T methanol, 1ml	A0158026	05/31/2028	11/27/2023 / yogesh	09/11/2020 / DHAVAL	V11252

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	01/22/2025	07/22/2024 / SAM	02/06/2024 / SAM	V14143

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

DD
06/17/2021

Catalog No. : 30541 **Lot No.:** A0172403

Description : NJEPH Aromatics Calibration Standard

NJEPH Aromatics Calibration Standard 2,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2027 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P10758
TO
P10762
(S)

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene CAS # 526-73-8 (Lot 8776.10-36) Purity 98%	2,010.0 µg/mL	+/- 11.7957 µg/mL Gravimetric +/- 90.5449 µg/mL Unstressed +/- 100.4678 µg/mL Stressed
2	Naphthalene CAS # 91-20-3 (Lot MKBZ8680V) Purity 99%	2,006.0 µg/mL	+/- 11.7723 µg/mL Gravimetric +/- 90.3656 µg/mL Unstressed +/- 100.2689 µg/mL Stressed
3	2-Methylnaphthalene CAS # 91-57-6 (Lot STBG8884) Purity 99%	2,008.0 µg/mL	+/- 11.7841 µg/mL Gravimetric +/- 90.4557 µg/mL Unstressed +/- 100.3688 µg/mL Stressed
4	Acenaphthylene CAS # 208-96-8 (Lot N19U) Purity 95%	2,002.6 µg/mL	+/- 11.7524 µg/mL Gravimetric +/- 90.2125 µg/mL Unstressed +/- 100.0989 µg/mL Stressed
5	Acenaphthene CAS # 83-32-9 (Lot MKCN0610) Purity 99%	2,000.0 µg/mL	+/- 11.7371 µg/mL Gravimetric +/- 90.0953 µg/mL Unstressed +/- 99.9689 µg/mL Stressed
6	Fluorene CAS # 86-73-7 (Lot 10217947) Purity 99%	2,016.0 µg/mL	+/- 11.8310 µg/mL Gravimetric +/- 90.8161 µg/mL Unstressed +/- 100.7687 µg/mL Stressed
7	Phenanthrene CAS # 85-01-8 (Lot MKCL7390) Purity 99%	2,012.0 µg/mL	+/- 11.8075 µg/mL Gravimetric +/- 90.6359 µg/mL Unstressed +/- 100.5688 µg/mL Stressed

8	Anthracene			2,002.0	µg/mL	+/-	11.7489	µg/mL	Gravimetric
	CAS #	120-12-7	(Lot MKCM0015)			+/-	90.1854	µg/mL	Unstressed
	Purity	99%				+/-	100.0689	µg/mL	Stressed
9	Fluoranthene			2,003.0	µg/mL	+/-	11.7547	µg/mL	Gravimetric
	CAS #	206-44-0	(Lot MKCF7378)			+/-	90.2305	µg/mL	Unstressed
	Purity	99%				+/-	100.1189	µg/mL	Stressed
10	Pyrene			2,011.0	µg/mL	+/-	11.8017	µg/mL	Gravimetric
	CAS #	129-00-0	(Lot BCCB9880)			+/-	90.5909	µg/mL	Unstressed
	Purity	99%				+/-	100.5188	µg/mL	Stressed
11	Benz(a)anthracene			2,011.0	µg/mL	+/-	11.8014	µg/mL	Gravimetric
	CAS #	56-55-3	(Lot P0022018-0505)			+/-	90.5890	µg/mL	Unstressed
	Purity	98%				+/-	100.5168	µg/mL	Stressed
12	Chrysene			2,000.0	µg/mL	+/-	11.7371	µg/mL	Gravimetric
	CAS #	218-01-9	(Lot STBJ8094)			+/-	90.0953	µg/mL	Unstressed
	Purity	99%				+/-	99.9689	µg/mL	Stressed
13	Benzo(b)fluoranthene			2,006.0	µg/mL	+/-	11.7721	µg/mL	Gravimetric
	CAS #	205-99-2	(Lot 012012B)			+/-	90.3638	µg/mL	Unstressed
	Purity	97%				+/-	100.2669	µg/mL	Stressed
14	Benzo(k)fluoranthene			2,010.0	µg/mL	+/-	11.7958	µg/mL	Gravimetric
	CAS #	207-08-9	(Lot 012019K)			+/-	90.5458	µg/mL	Unstressed
	Purity	99%				+/-	100.4688	µg/mL	Stressed
15	Benzo(a)pyrene			2,004.0	µg/mL	+/-	11.7606	µg/mL	Gravimetric
	CAS #	50-32-8	(Lot RP210113)			+/-	90.2755	µg/mL	Unstressed
	Purity	99%				+/-	100.1689	µg/mL	Stressed
16	Indeno(1,2,3-cd)pyrene			2,010.0	µg/mL	+/-	11.7958	µg/mL	Gravimetric
	CAS #	193-39-5	(Lot 1-RAK-33-4)			+/-	90.5458	µg/mL	Unstressed
	Purity	99%				+/-	100.4688	µg/mL	Stressed
17	Dibenz(a,h)anthracene			2,017.0	µg/mL	+/-	11.8369	µg/mL	Gravimetric
	CAS #	53-70-3	(Lot ER032211-01)			+/-	90.8611	µg/mL	Unstressed
	Purity	99%				+/-	100.8187	µg/mL	Stressed
18	Benzo(g,h,i)perylene			2,003.0	µg/mL	+/-	11.7547	µg/mL	Gravimetric
	CAS #	191-24-2	(Lot 8GFYJ)			+/-	90.2305	µg/mL	Unstressed
	Purity	99%				+/-	100.1189	µg/mL	Stressed
<hr/>									
Solvent:	Methylene chloride								
	CAS #	75-09-2							
	Purity	99%							

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)


Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

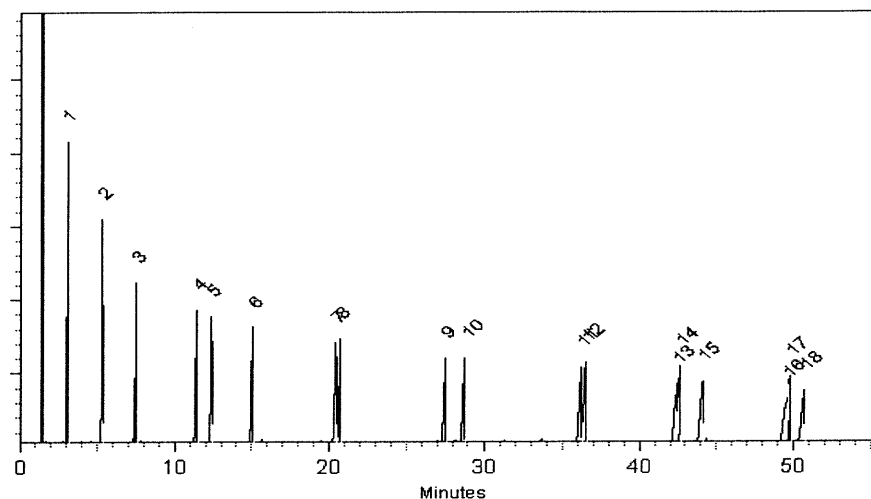

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Lane Kibe - Mix Technician

Date Mixed: 14-May-2021 Balance: B345965662


Alexis Shelow - Operations Tech I

Date Passed: 18-May-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1

Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Material No.: 92E
Batch No.: 24C016
Manufactured Date: 2024-C
Expiration Date: 2025-C
Revision I

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	10
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC
Manufacturer source batch: MG24A04224

E 3743


Ken Koehnlein
Sr. Manager, Quality Assurance

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700
Page 1 of 1

Cleanert EPH

5g/25ml 15/pkg

固相萃取产品

LOT#:Z0513CK1



MFG#:F04005



Made in China



CAT# SI500025-30

Agela Technologies

E 3757



Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 24E2462004
Manufactured Date: 2024-04-10
Expiration Date: 2025-07-10
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	3
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.1 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC
Manufacturer source batch: MG24D10725

E 3768

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03
Batch No.: 23H1462005
Manufactured Date: 2023-07-26
Expiration Date: 2026-07-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 8/13/24

E 3788

Ken Koehnlein
Sr. Manager, Quality Assurance

Material No.: 926
Batch No.: 24C186
Manufactured Date: 2024-0
Expiration Date: 2025-0
Revision N

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 8/13/24

E 3789



Jamie Croak
Director Quality Operations, Bioscience Products

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Acetone
CMOS

avantor™



Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

>>> Continued on page 2 >>>

Recd. by RP on 9/11/24

E3793

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use
Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC

Michelle Bales
Sr. Manager, Quality Assurance

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 10/09/24

E 3819

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700
Page 1 of 1

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4

Batch No.: 24I2662006

Manufactured Date: 2024-08-29

Expiration Date: 2025-11-28

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	3
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	99.9 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	$< 5 \text{ ppm}$
Water (by KF, coulometric)	$\leq 0.02 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3822

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



Material No.: 9077-02
Batch No.: 22L0562016
Manufactured Date: 2022-10-26
Expiration Date: 2025-10-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid (μeq/g)	≤ 0.3	0.2
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis - Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier
Vice President Global Quality



CERTIFIED WEIGHT REPORT

Part Number: 95709
Lot Number: 060420
Description: NJ EPH Aromatic Hydrocarbons
18 components
Expiration Date: 06/4/25
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 2000
NIST Test ID#: 23060
Weight(s) shown below were combined and diluted to (mL): 500.0
Balance Uncertainty: 5E-05
Flask Uncertainty: 0.058

Solvent(s): Methylene chloride
Lot# 104923

Formulated By:	<i>Benson Chan</i>	060420
Reviewed By:	<i>Pedro L. Renteria</i>	060420
		DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	SDS Information	
											(Solvent Safety Info. On Attached pg.)	LD50
1. Acenaphthene	1	MKB14871V	2000	99	0.2	1.01003	1.01010	2000.1	8.1	83-32-9	N/A	ip-ral 600mg/kg
2. Acenaphthylene	3	012014	2000	98	0.2	1.02033	1.02053	2000.4	8.2	208-96-6	N/A	N/A
3. Anthracene	13	A0210580	2000	99	0.2	1.01003	1.01009	2000.1	8.1	120-12-7	0.2mg/m3 (8h)	ip-trus 430mg/kg
4. Benz(a)anthracene	28	JY2TD-JT	2000	98	0.2	1.02033	1.02051	2000.3	8.2	56-55-3	N/A	N/A
5. Benz(a)pyrene	30	012012	2000	99.5	0.2	1.00495	1.00511	2000.3	8.1	50-32-8	0.2mg/m3 (8h)	scu-ral 50mg/kg
6. Benz(b)fluoranthene	31	012012b	2000	99	0.2	1.01003	1.01012	2000.2	8.1	205-99-2	N/A	N/A
7. Benz(k)fluoranthene	33	012012k	2000	99	0.2	1.01003	1.01018	2000.3	8.1	207-08-9	N/A	N/A
8. Benz(g,h,i)perylene	32	012018	2000	99	0.2	1.01003	1.01019	2000.3	8.1	191-24-2	N/A	N/A
9. Chrysene	91	012015	2000	98	0.2	1.02033	1.02040	2000.1	8.2	218-01-9	0.2mg/m3	N/A
10. Dibenzo(a,h)anthracene	112	012011	2000	98	0.2	1.02033	1.02050	2000.3	8.2	53-70-3	0.2mg/m3	N/A
11. Fluoranthene	183	04221PV	2000	98	0.2	1.02033	1.02050	2000.3	8.2	206-44-0	N/A	of-ral 2000mg/kg
12. Fluorene	184	07211MV	2000	98	0.2	1.02033	1.02047	2000.3	8.2	86-73-7	N/A	ip-trus 2 g/kg
13. Indeno(1,2,3-cd)pyrene	202	012014	2000	99.9	0.2	1.00093	1.00119	2000.5	8.0	193-39-5	N/A	N/A
14. 2-Methylnaphthalene	214	MKB13783V	2000	97	0.2	1.03085	1.03090	2000.1	8.3	91-57-6	N/A	of-ral 1630mg/kg
15. Naphthalene	222	MKB26890V	2000	100	0.2	0.99993	0.99999	2000.1	8.0	91-20-3	10 ppm (50mg/m3/8h)	of-ral 490mg/kg
16. Phenanthrene	248	03410PV	2000	99	0.2	1.01003	1.01030	2000.5	8.1	85-01-8	0.2mg/m3/8h	of-trus 700mg/kg
17. Pyrene	259	010197	2000	98	0.2	1.02033	1.02042	2000.2	8.2	129-00-0	0.2mg/m3/8h	of-ral 2700mg/kg
18. 1,2,3-Trimethylbenzene	944	031097	2000	99	0.2	1.01003	1.01025	2000.4	8.1	526-73-8	N/A	N/A

• The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
• Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
• Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
• All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
• Uncertainty Reference: Taylor, B.N., and Kuyat, C.F., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).


P11137

P11131

11/10/21



Method GC8MSD-2.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (14min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Melissa Stonier.

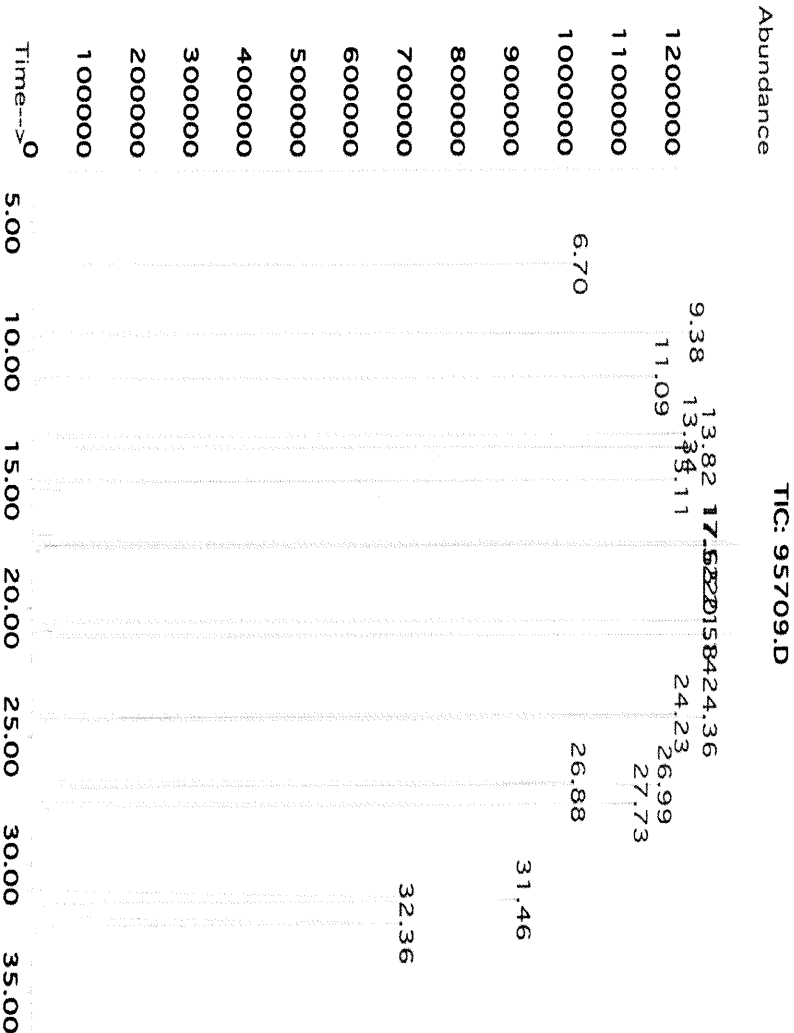

Peak No.	Name	MSD RT (min.)
1	1,2,3-Trimethylbenzene	6.70
2	Naphthalene	9.38
3	2-Methylnaphthalene	11.09
4	Acenaphthylene	13.34
5	Acenaphthene	13.82
6	Fluorene	15.11
7	Phenanthrene	17.52
8	Anthracene	17.65
9	Fluoranthene	20.58
10	Pyrene	21.14
11	Chrysene	24.23
12	Benzo(a)anthracene	24.36
13	Benzo(b)fluoranthene/Benzo(k)fluoranthene	26.98
14	Benzo(a)pyrene	27.73
15	Indeno(1,2,3-cd)pyrene/Dibenzo(a,h)anthracene	31.46
16	Benzo(g,h,i)perylene	32.36



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30540 **Lot No.:** A0190424

Description : NJEPH Aliphatics Calibration Standard

Aliphatics Calibration Standard 2000µg/mL, Hexane/Carbon Disulfide (80:20), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2029 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P12361
↓
P12370 } Y.P.
031/6/23

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)			
1	n-Nonane (C9) CAS # 111-84-2 Purity 99% (Lot SHBN5361)	2,014.0 µg/mL	+/- 11.8193	µg/mL	Gravimetric	
			+/- 50.0027	µg/mL	Unstressed	
			+/- 59.9491	µg/mL	Stressed	
2	n-Decane (C10) CAS # 124-18-5 Purity 99% (Lot SHBN8619)	2,014.7 µg/mL	+/- 11.8232	µg/mL	Gravimetric	
			+/- 50.0193	µg/mL	Unstressed	
			+/- 59.9689	µg/mL	Stressed	
3	Naphthalene CAS # 91-20-3 Purity 99% (Lot MKCH0219)	2,015.3 µg/mL	+/- 11.8271	µg/mL	Gravimetric	
			+/- 50.0358	µg/mL	Unstressed	
			+/- 59.9888	µg/mL	Stressed	
4	n-Dodecane (C12) CAS # 112-40-3 Purity 99% (Lot SHBN7174)	2,008.0 µg/mL	+/- 11.7841	µg/mL	Gravimetric	
			+/- 49.8538	µg/mL	Unstressed	
			+/- 59.7705	µg/mL	Stressed	
5	2-Methylnaphthalene CAS # 91-57-6 Purity 96% (Lot STBK0259)	2,007.0 µg/mL	+/- 11.7784	µg/mL	Gravimetric	
			+/- 49.8299	µg/mL	Unstressed	
			+/- 59.7419	µg/mL	Stressed	
6	n-Tetradecane (C14) CAS # 629-59-4 Purity 99% (Lot STBK2282)	2,016.7 µg/mL	+/- 11.8349	µg/mL	Gravimetric	
			+/- 50.0689	µg/mL	Unstressed	
			+/- 60.0284	µg/mL	Stressed	
7	n-Hexadecane (C16) CAS # 544-76-3 Purity 98% (Lot SHBM4146)	2,014.9 µg/mL	+/- 11.8244	µg/mL	Gravimetric	
			+/- 50.0246	µg/mL	Unstressed	
			+/- 59.9753	µg/mL	Stressed	

8	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	(Lot VZKOJ)	2,004.7 µg/mL	+/-	11.7645	µg/mL	Gravimetric
				+/-	49.7710	µg/mL	Unstressed
				+/-	59.6712	µg/mL	Stressed
9	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	(Lot MKCF7888)	2,018.0 µg/mL	+/-	11.8428	µg/mL	Gravimetric
				+/-	50.1020	µg/mL	Unstressed
				+/-	60.0681	µg/mL	Stressed
10	n-Heneicosane (C21) CAS # 629-94-7 Purity 99%	(Lot MKCL3226)	2,000.7 µg/mL	+/-	11.7410	µg/mL	Gravimetric
				+/-	49.6717	µg/mL	Unstressed
				+/-	59.5522	µg/mL	Stressed
11	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	2,005.3 µg/mL	+/-	11.7684	µg/mL	Gravimetric
				+/-	49.7876	µg/mL	Unstressed
				+/-	59.6911	µg/mL	Stressed
12	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	2,018.0 µg/mL	+/-	11.8428	µg/mL	Gravimetric
				+/-	50.1020	µg/mL	Unstressed
				+/-	60.0681	µg/mL	Stressed
13	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	2,014.0 µg/mL	+/-	11.8193	µg/mL	Gravimetric
				+/-	50.0027	µg/mL	Unstressed
				+/-	59.9491	µg/mL	Stressed
14	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	2,002.0 µg/mL	+/-	11.7489	µg/mL	Gravimetric
				+/-	49.7048	µg/mL	Unstressed
				+/-	59.5919	µg/mL	Stressed
15	n-Triacontane (C30) CAS # 638-68-6 Purity 97%	(Lot MKCQ9436)	2,011.1 µg/mL	+/-	11.8025	µg/mL	Gravimetric
				+/-	49.9316	µg/mL	Unstressed
				+/-	59.8637	µg/mL	Stressed
16	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	2,012.0 µg/mL	+/-	11.8075	µg/mL	Gravimetric
				+/-	49.9531	µg/mL	Unstressed
				+/-	59.8895	µg/mL	Stressed
17	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	2,006.7 µg/mL	+/-	11.7762	µg/mL	Gravimetric
				+/-	49.8207	µg/mL	Unstressed
				+/-	59.7308	µg/mL	Stressed
18	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot Z27H018)	2,017.3 µg/mL	+/-	11.8388	µg/mL	Gravimetric
				+/-	50.0855	µg/mL	Unstressed
				+/-	60.0483	µg/mL	Stressed
19	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 96%	(Lot 0000145137)	2,017.3 µg/mL	+/-	11.8385	µg/mL	Gravimetric
				+/-	50.0842	µg/mL	Unstressed
				+/-	60.0467	µg/mL	Stressed
20	n-Tetracontane (C40) CAS # 4181-95-7 Purity 99%	(Lot BSBME)	2,008.7 µg/mL	+/-	11.7880	µg/mL	Gravimetric
				+/-	49.8703	µg/mL	Unstressed
				+/-	59.7903	µg/mL	Stressed
Solvent: Hexane/Carbon disulfide (80:20)							
	CAS # 110-54-3/75-15-0						
	Purity 99%						

Column:
30m x 0.25mm x 0.25µm
Pxx-5 (cat.#10223)


Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

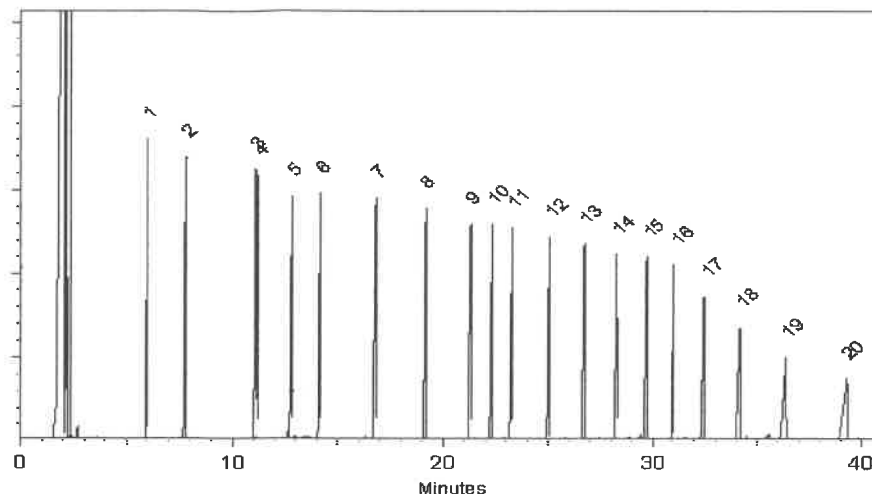

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Morgan Craighead - Mix Technician

Date Mixed: 10-Oct-2022 Balance: 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Oct-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31098 **Lot No.:** A0204989

Description: 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2031 **Storage:** 10°C or colder

Ship: Ambient

P12960
↓
P12991 } Y.P.
12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	14738400	99%	10,097.3 µg/mL	+/- 567.2675

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:

FID

Split Vent:

10 ml/min.

Inj. Vol

1µl



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31097 **Lot No.:** A0204177

Description: o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: June 30, 2027 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P12992 } Y.P.
↓
P13031 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,000.5 µg/mL	+/- 450.4278

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
10 ml/min.

Inj. Vol
1µl

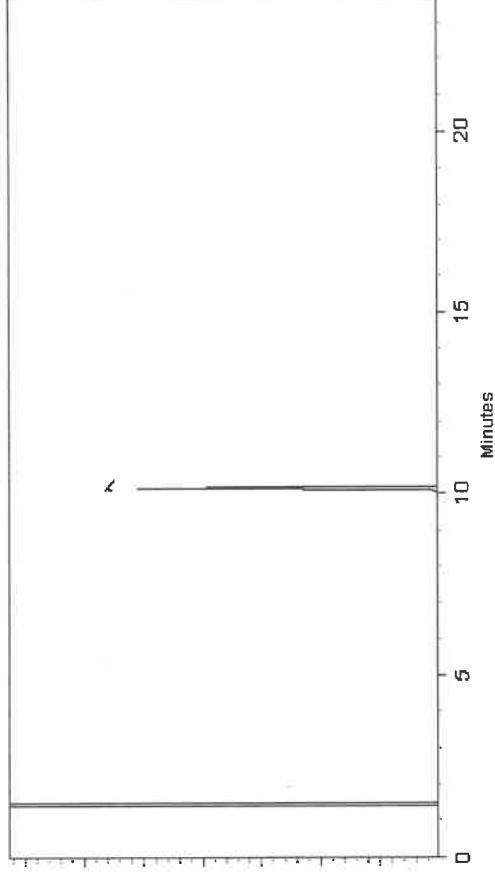

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-Nov-2023 **Balance Serial #** 1128360905


Dillian Murphy - Operations Technician I

Date Passed: 09-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31097 **Lot No.:** A0204177

Description: o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: June 30, 2027 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P12992 } Y.P.
↓
P13031 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,000.5 µg/mL	+/- 450.4278

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
10 ml/min.

Inj. Vol
1µl

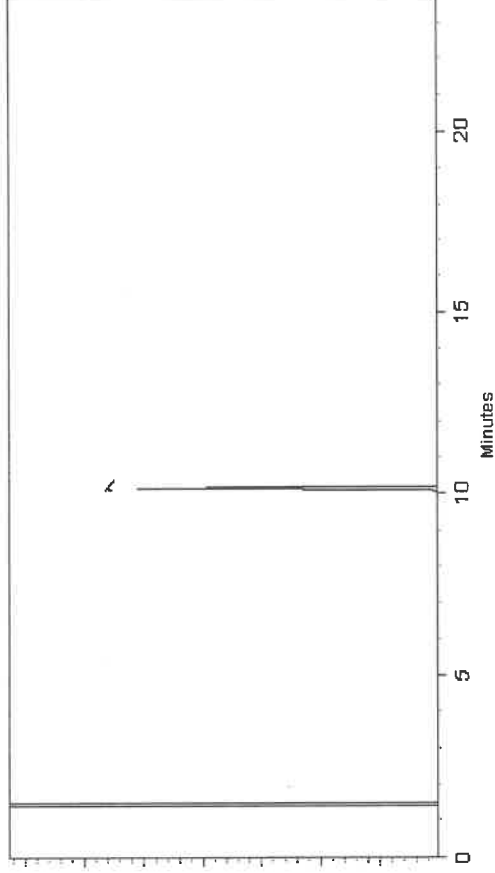

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.



Laith Clemente - Operations Technician I

Date Mixed: 07-Nov-2023 **Balance Serial #** 1128360905



Dillian Murphy - Operations Technician I

Date Passed: 09-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31097 **Lot No.:** A0204177

Description: o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: June 30, 2027 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P12992 } Y.P.
↓
P13031 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,000.5 µg/mL	+/- 450.4278

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
10 ml/min.

Inj. Vol
1µl

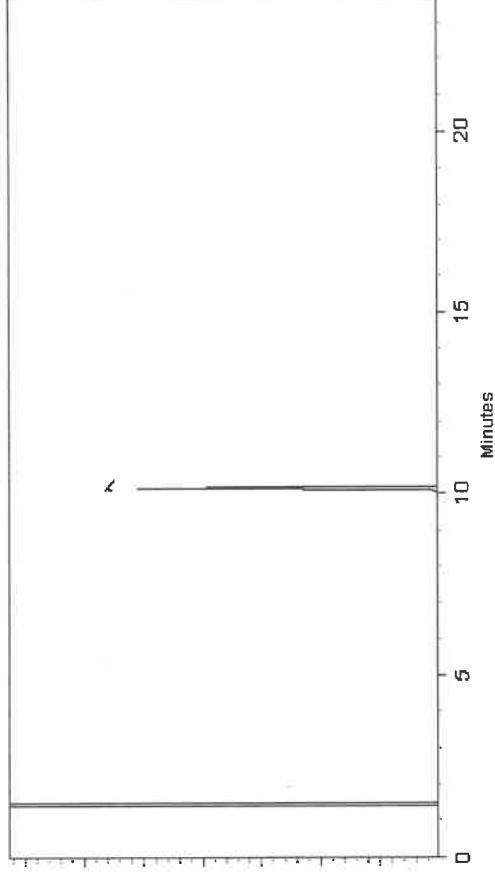

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-Nov-2023 **Balance Serial #** 1128360905


Dillian Murphy - Operations Technician I

Date Passed: 09-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31097 Lot No.: A0204177

Description: o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: June 30, 2027 Storage: 10°C or colder

Handling: Sonicate prior to use. Ship: Ambient

P12992 } Y.P.
↓
P13031 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,000.5 µg/mL	+/- 450.4278

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
10 ml/min.

Inj. Vol
1µl

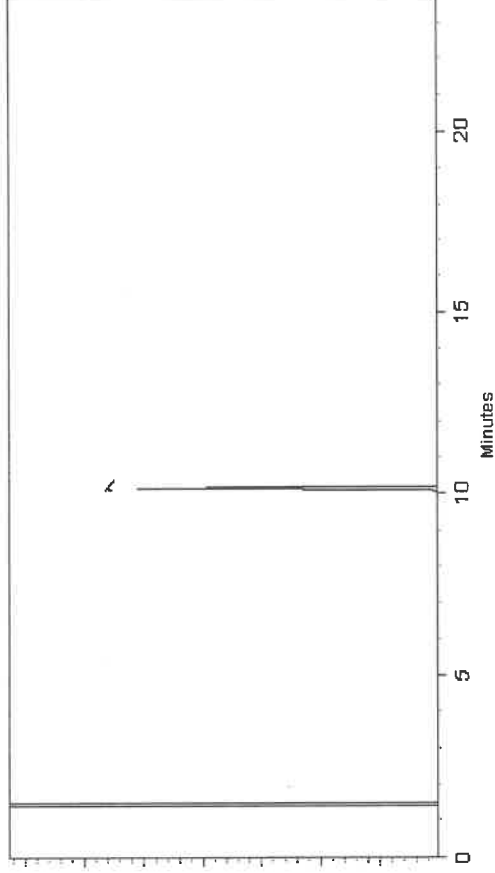

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.



Laith Clemente - Operations Technician I

Date Mixed: 07-Nov-2023 **Balance Serial #** 1128360905



Dillian Murphy - Operations Technician I

Date Passed: 09-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31097 **Lot No.:** A0204177

Description: o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: June 30, 2027 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P12992 } Y.P.
↓
P13031 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,000.5 µg/mL	+/- 450.4278

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
10 ml/min.

Inj. Vol
1µl

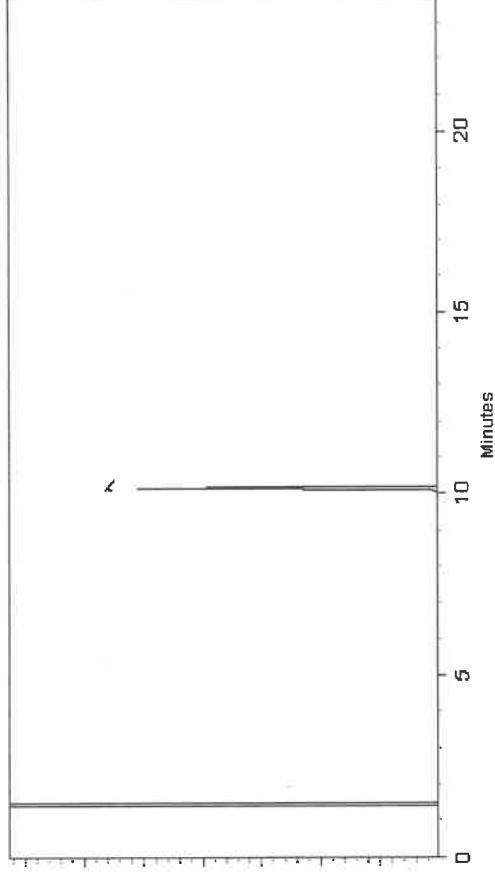

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.



Laith Clemente - Operations Technician I

Date Mixed: 07-Nov-2023 **Balance Serial #** 1128360905



Dillian Murphy - Operations Technician I

Date Passed: 09-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31097 **Lot No.:** A0204177

Description: o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: June 30, 2027 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P12992 } Y.P.
↓
P13031 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,000.5 µg/mL	+/- 450.4278

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
10 ml/min.

Inj. Vol
1µl

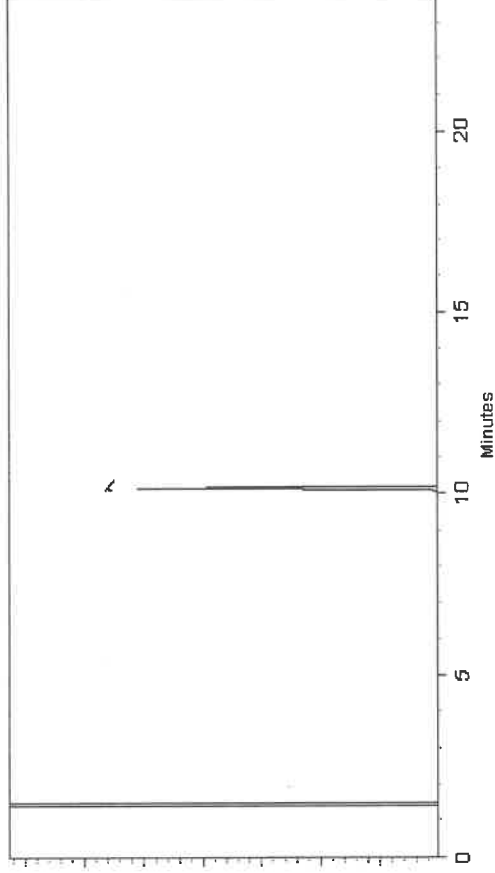

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-Nov-2023 **Balance Serial #** 1128360905


Dillian Murphy - Operations Technician I

Date Passed: 09-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 31097 **Lot No.:** A0204177

Description: o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: June 30, 2027 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P12992 } Y.P.
↓
P13031 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,000.5 µg/mL	+/- 450.4278

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
10 ml/min.

Inj. Vol
1µl

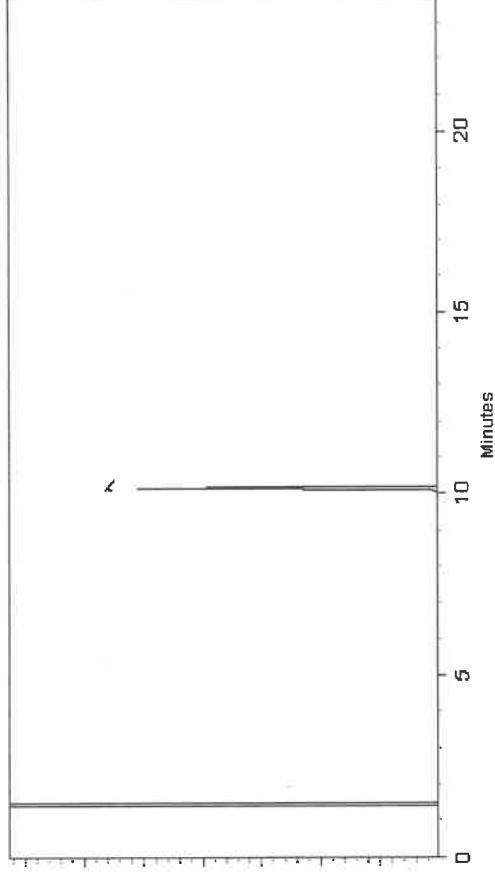

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-Nov-2023 **Balance Serial #** 1128360905


Dillian Murphy - Operations Technician I

Date Passed: 09-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0200707

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : September 30, 2030 **Storage:** 10°C or colder

Ship: Ambient

P130hh
2
P13051 } Y.B.
12/26/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	E230426RSRB	99%	10,018.0 µg/mL	+/- 562.8106

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

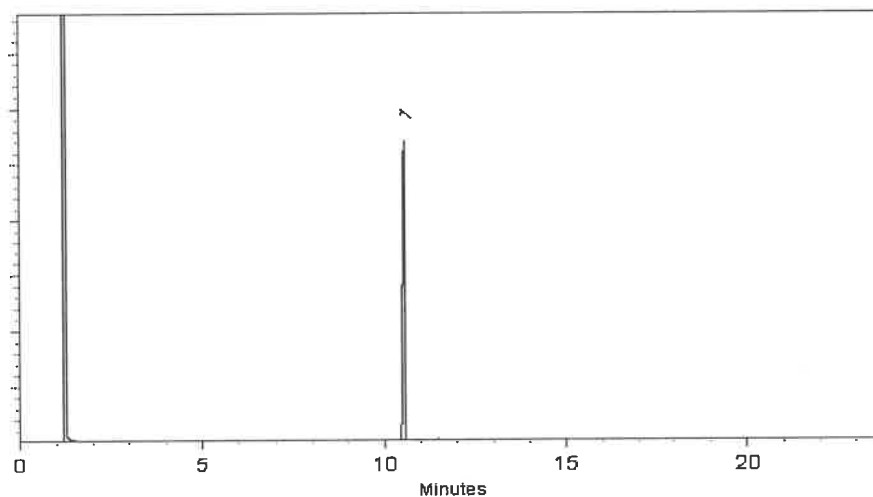

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Ashley Frantz - Quoting Technician

Date Mixed: 07-Aug-2023

Balance Serial # 1128360905


Dillan Murphy - Operations Technician I

Date Passed: 10-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0200707

Description : 1-Chlorooctadecane Standard
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,
1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : September 30, 2030 **Storage:** 10°C or colder
Ship: Ambient

P130hh
2
P13051 } Y.B.
12/26/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	E230426RSRB	99%	10,018.0 µg/mL	+/- 562.8106

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

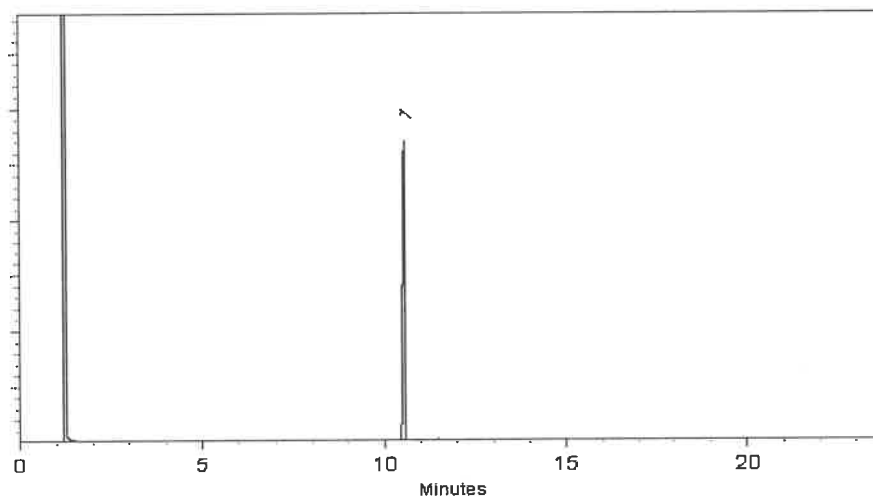

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Ashley Frantz - Quoting Technician

Date Mixed: 07-Aug-2023

Balance Serial # 1128360905


Dillan Murphy - Operations Technician I

Date Passed: 10-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0200707

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : September 30, 2030 **Storage:** 10°C or colder

Ship: Ambient

P130hh
↓
P13051 } Y.B.
12/26/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	E230426RSRB	99%	10,018.0 µg/mL	+/- 562.8106

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

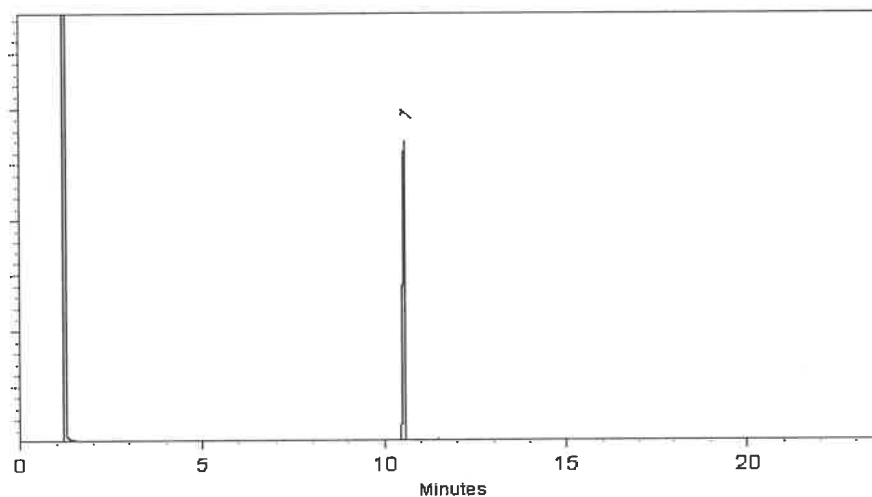

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Ashley Frantz - Quoting Technician

Date Mixed: 07-Aug-2023

Balance Serial # 1128360905


Dillan Murphy - Operations Technician I

Date Passed: 10-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31098 **Lot No.:** A0200707

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : September 30, 2030 **Storage:** 10°C or colder

Ship: Ambient

P130hh
2
P13051 } Y.B.
12/26/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	E230426RSRB	99%	10,018.0 µg/mL	+/- 562.8106

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

10 ml/min.

Inj. Vol

1µl

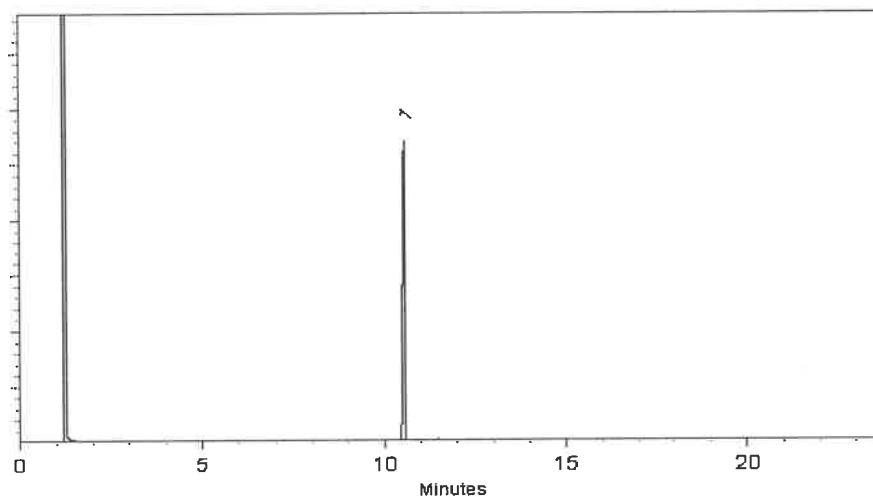

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Ashley Frantz - Quoting Technician

Date Mixed: 07-Aug-2023

Balance Serial # 1128360905


Dillan Murphy - Operations Technician I

Date Passed: 10-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0203911

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : November 30, 2030 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13053 } Y.P.
↓
P13099 } 01/12/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.0 µg/mL	+/- 5.1667
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.0 µg/mL	+/- 5.1667
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.6 µg/mL	+/- 5.1815
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCL8682	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	200.3 µg/mL	+/- 5.1753
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.5 µg/mL	+/- 5.1788
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

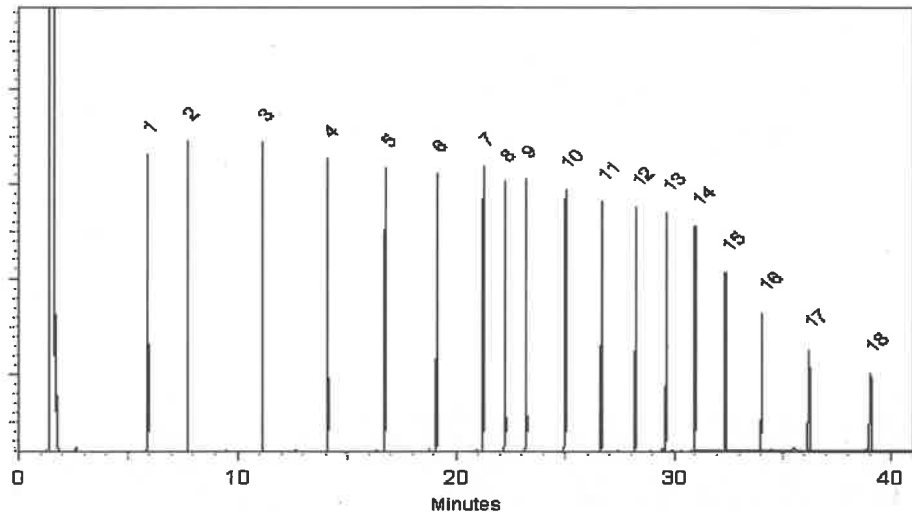

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 31-Oct-2023

Balance Serial # B345965662


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0203911

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : November 30, 2030 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13053 } Y.P.
↓
P13099 } 01/12/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.0 µg/mL	+/- 5.1667
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.0 µg/mL	+/- 5.1667
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.6 µg/mL	+/- 5.1815
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCL8682	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	200.3 µg/mL	+/- 5.1753
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.5 µg/mL	+/- 5.1788
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

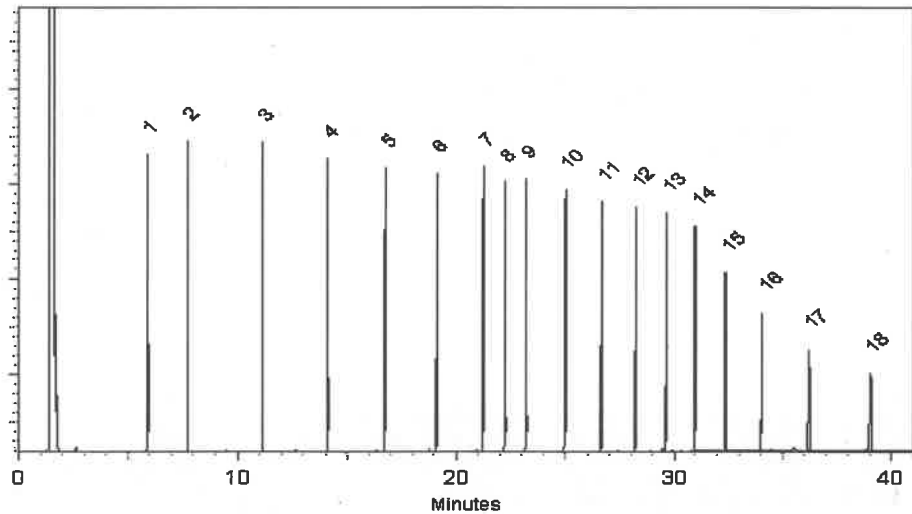

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 31-Oct-2023

Balance Serial # B345965662


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0203911

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : November 30, 2030 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13053 } Y.P.
↓
P13099 } 01/12/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.0 µg/mL	+/- 5.1667
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.0 µg/mL	+/- 5.1667
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.6 µg/mL	+/- 5.1815
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCL8682	99%	200.3 µg/mL	+/- 5.1753
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	200.3 µg/mL	+/- 5.1753
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.0 µg/mL	+/- 5.1667
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.5 µg/mL	+/- 5.1788
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.0 µg/mL	+/- 5.1667
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.0 µg/mL	+/- 5.1667
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.0 µg/mL	+/- 5.1667

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

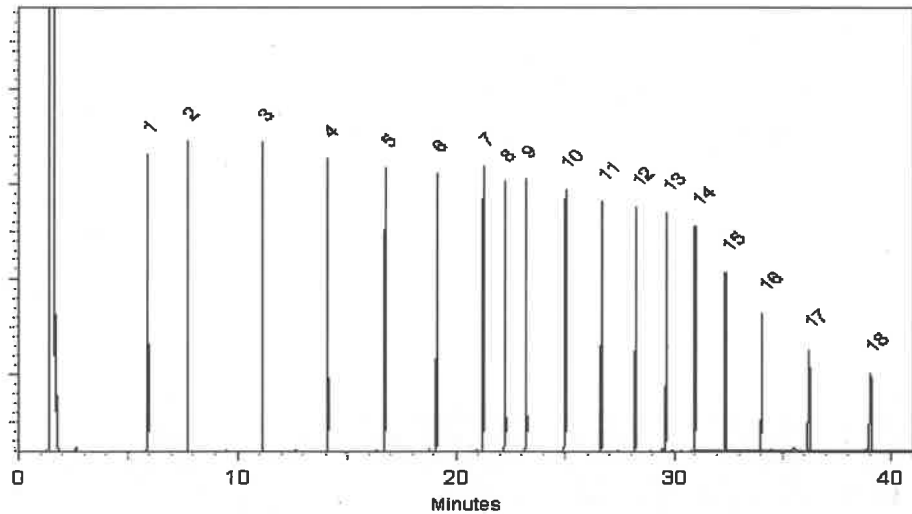

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 31-Oct-2023

Balance Serial # B345965662


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0200008

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : August 31, 2030 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13100 } Y.P.
2/
P13102 } 01/12/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.7 µg/mL	+/- 5.2098
2	n-Decane (C10)	124-18-5	SHBP4427	99%	201.3 µg/mL	+/- 5.2012
3	n-Dodecane (C12)	112-40-3	SHBN7174	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	201.0 µg/mL	+/- 5.1926
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	201.7 µg/mL	+/- 5.2098
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	201.2 µg/mL	+/- 5.1984
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	201.4 µg/mL	+/- 5.2038
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	201.3 µg/mL	+/- 5.2012
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	201.3 µg/mL	+/- 5.2012
10	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.7 µg/mL	+/- 5.2098
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	201.0 µg/mL	+/- 5.1926
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.5 µg/mL	+/- 5.1788
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.3 µg/mL	+/- 5.2012
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.7 µg/mL	+/- 5.1839
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.0 µg/mL	+/- 5.1926
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	201.3 µg/mL	+/- 5.1998

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C


Det. Type:
FID

Split Vent:
2 ml/min.


Inj. Vol
1µl

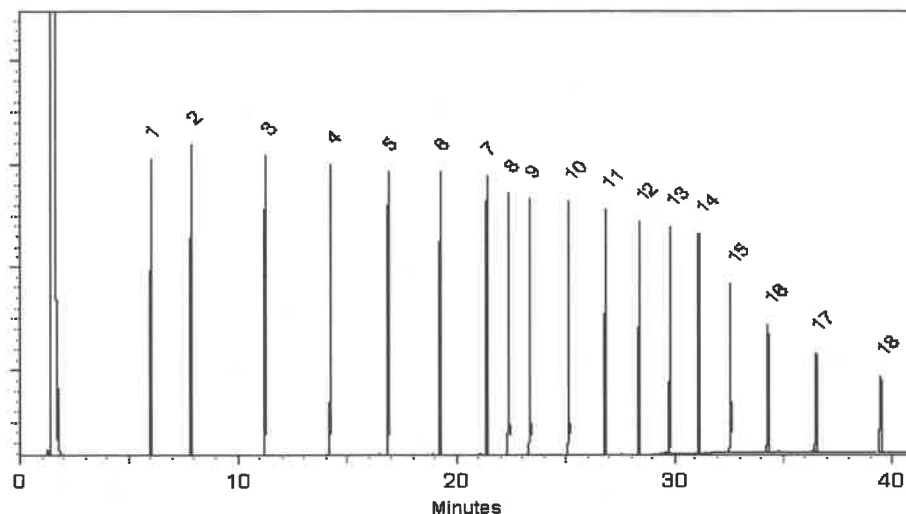

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


John Friedline - Operations Technician I

Date Mixed: 18-Jul-2023 **Balance Serial #** 1127510105


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Jul-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0200008

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : August 31, 2030 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13100 } Y.P.
2/ }
P13102 } 01/12/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.7 µg/mL	+/- 5.2098
2	n-Decane (C10)	124-18-5	SHBP4427	99%	201.3 µg/mL	+/- 5.2012
3	n-Dodecane (C12)	112-40-3	SHBN7174	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	201.0 µg/mL	+/- 5.1926
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	201.7 µg/mL	+/- 5.2098
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	201.2 µg/mL	+/- 5.1984
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	201.4 µg/mL	+/- 5.2038
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	201.3 µg/mL	+/- 5.2012
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	201.3 µg/mL	+/- 5.2012
10	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.7 µg/mL	+/- 5.2098
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	201.0 µg/mL	+/- 5.1926
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.5 µg/mL	+/- 5.1788
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.3 µg/mL	+/- 5.2012
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.7 µg/mL	+/- 5.1839
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.0 µg/mL	+/- 5.1926
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	201.3 µg/mL	+/- 5.1998

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C


Det. Type:
FID

Split Vent:
2 ml/min.


Inj. Vol
1µl

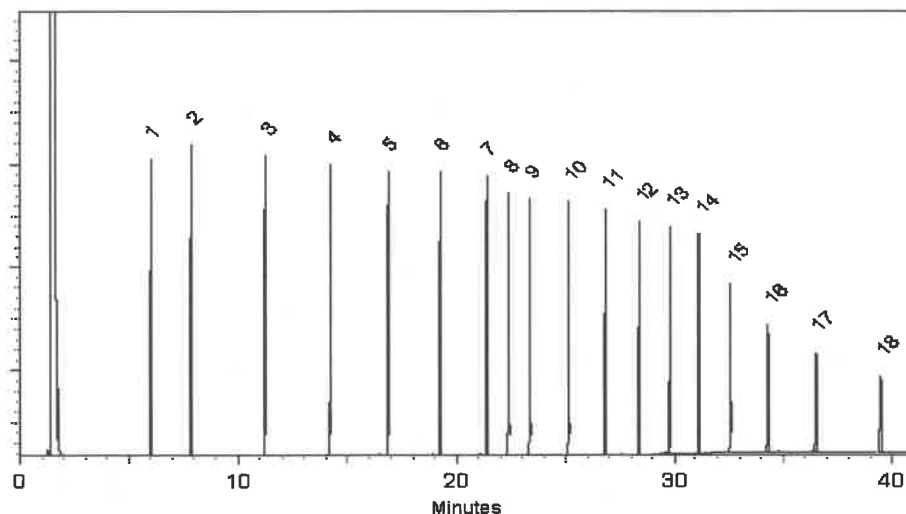

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


John Friedline - Operations Technician I

Date Mixed: 18-Jul-2023 **Balance Serial #** 1127510105


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Jul-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0200008

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : August 31, 2030 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13100 } Y.P.
2/ }
P13102 } 01/12/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.7 µg/mL	+/- 5.2098
2	n-Decane (C10)	124-18-5	SHBP4427	99%	201.3 µg/mL	+/- 5.2012
3	n-Dodecane (C12)	112-40-3	SHBN7174	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	201.0 µg/mL	+/- 5.1926
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	201.7 µg/mL	+/- 5.2098
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	201.2 µg/mL	+/- 5.1984
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	201.4 µg/mL	+/- 5.2038
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	201.3 µg/mL	+/- 5.2012
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	201.3 µg/mL	+/- 5.2012
10	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.7 µg/mL	+/- 5.2098
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	201.0 µg/mL	+/- 5.1926
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.5 µg/mL	+/- 5.1788
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.3 µg/mL	+/- 5.2012
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.7 µg/mL	+/- 5.1839
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.0 µg/mL	+/- 5.1926
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	201.3 µg/mL	+/- 5.1998

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C


Det. Type:
FID

Split Vent:
2 ml/min.


Inj. Vol
1µl

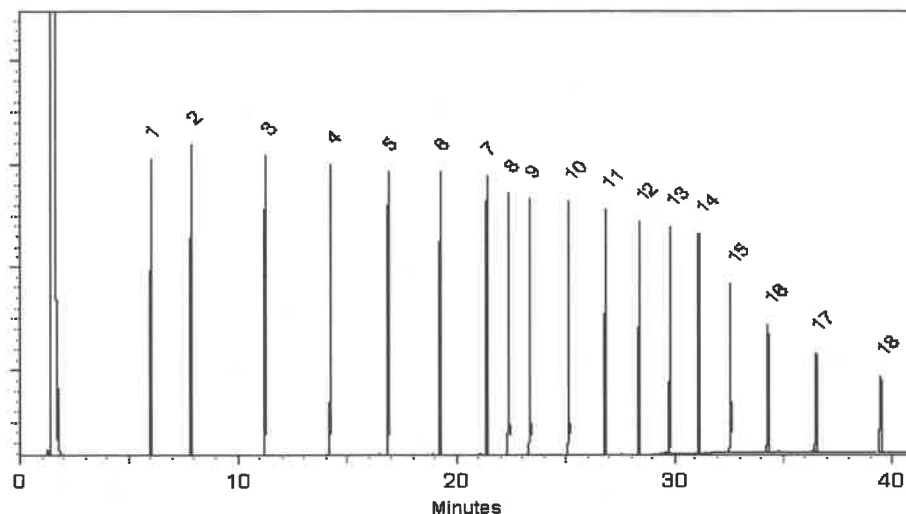

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


John Friedline - Operations Technician I

Date Mixed: 18-Jul-2023 **Balance Serial #** 1127510105


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Jul-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0206496

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13258 } 7-P.
↓
P13277 } 02/20/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,008.5 µg/mL	+/- 180.5736
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,001.5 µg/mL	+/- 180.2582

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

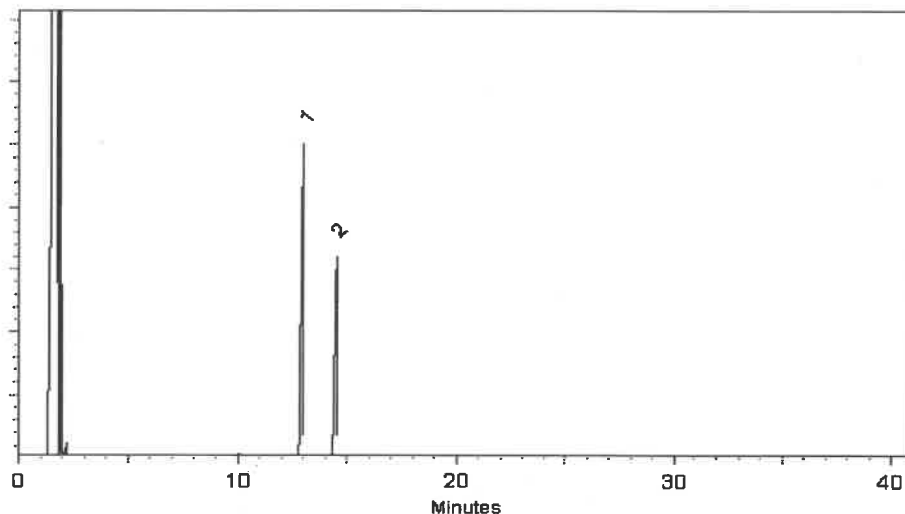

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich

Rebecca Gingerich - Operations Tech II

Date Mixed: 11-Jan-2024

Balance Serial # B345965662

Dylan Murphy

Dylan Murphy - Operations Technician I

Date Passed: 15-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0206496

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13258 } 7-P.
↓
P13277 } 02/20/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,008.5 µg/mL	+/- 180.5736
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,001.5 µg/mL	+/- 180.2582

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

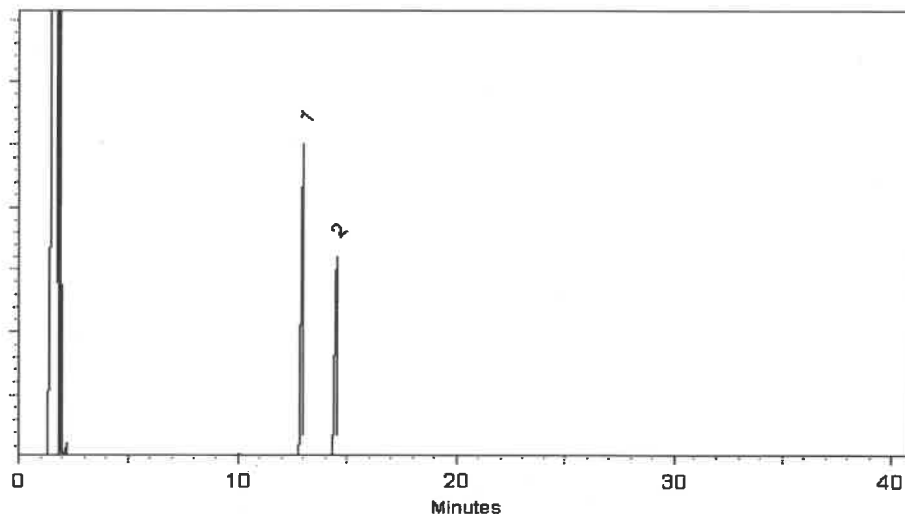

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich

Rebecca Gingerich - Operations Tech II

Date Mixed: 11-Jan-2024

Balance Serial # B345965662

Dylan Murphy

Dylan Murphy - Operations Technician I

Date Passed: 15-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0206496

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13258 } 7-P.
↓
P13277 } 02/20/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,008.5 µg/mL	+/- 180.5736
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,001.5 µg/mL	+/- 180.2582

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

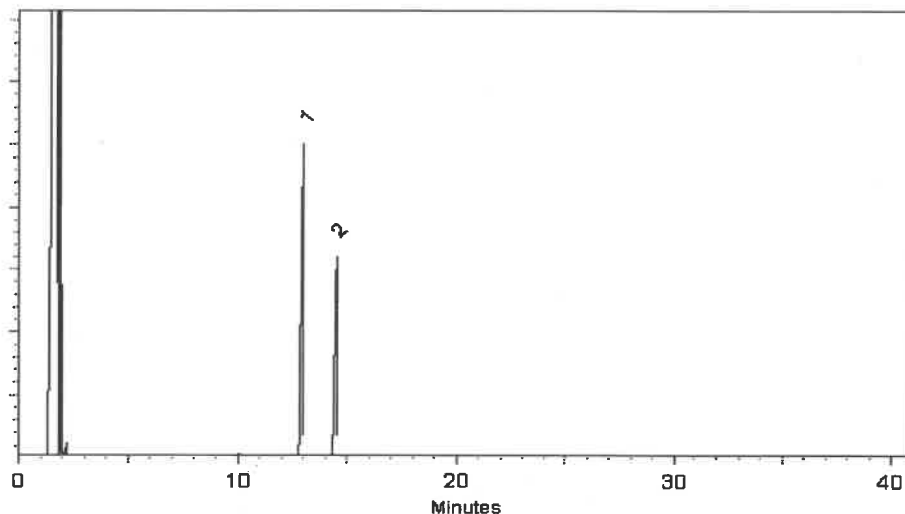

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich

Rebecca Gingerich - Operations Tech II

Date Mixed: 11-Jan-2024

Balance Serial # B345965662

Dylan Murphy

Dylan Murphy - Operations Technician I

Date Passed: 15-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0206496

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13258 } 7-P.
↓
P13277 } 02/20/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,008.5 µg/mL	+/- 180.5736
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,001.5 µg/mL	+/- 180.2582

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

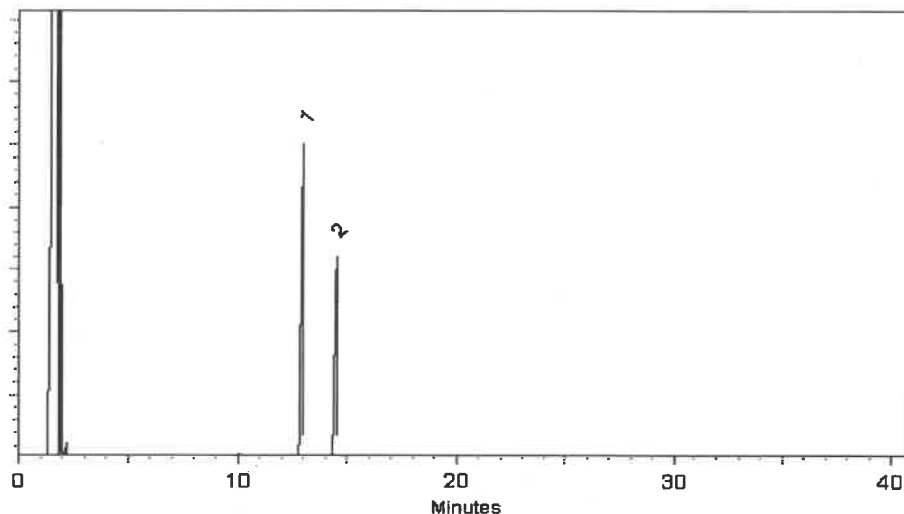

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich

Rebecca Gingerich - Operations Tech II

Date Mixed: 11-Jan-2024

Balance Serial # B345965662

Dylan Murphy

Dylan Murphy - Operations Technician I

Date Passed: 15-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0206496

Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13258 } 7-P.
↓
P13277 } 02/20/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,008.5 µg/mL	+/- 180.5736
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,001.5 µg/mL	+/- 180.2582

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

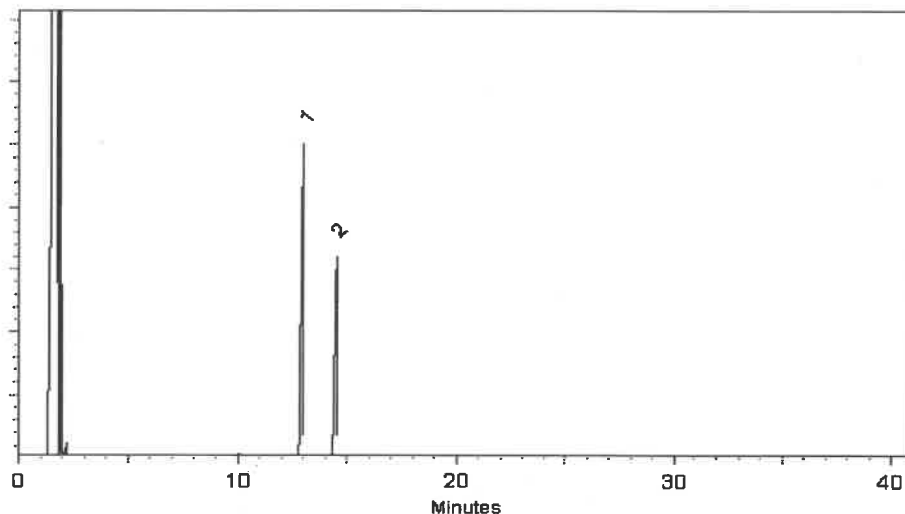

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich

Rebecca Gingerich - Operations Tech II

Date Mixed: 11-Jan-2024

Balance Serial # B345965662

Dylan Murphy

Dylan Murphy - Operations Technician I

Date Passed: 15-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.


- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



CERTIFIED WEIGHT REPORT

Part Number: 95999

Lot Number: 040524

Description: NJ EPH Aliphatic n-Hydrocarbons - Revised
20 components

Expiration Date: 040534

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test ID#: 6UTB

Weight(s) shown below were combined and diluted to (mL):

CAUTION: Sonicate Before Use

Solvent(s):
Cyclohexane

Lot#
28930

Formulated By:	Anthony Mahoney	040524	DATE
Reviewed By:	Pedro L. Rentas	040524	DATE

P13278
Y.P.
P13287
04/11/24

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

CAUTION: Sonicate Before Use

Compound															SDS Information		
(RM#)	Lot	Dil.	Initial	Initial	Nominal	Purity	Purity	Uncertainty	Target	Actual	Expanded	(Solvent Safety Info. On Attached pg.)					
Part Number	Number	Factor	Vol. (mL)	Conc.(µg/mL)	Conc (µg/mL)	(%)	Uncertainty	Pipette	Weight(g)	Conc (µg/mL)	(+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50			
1. 2-Methylnaphthalene	(0214)	MKBF3783V	NA	NA	NA	1000	97	0.2	NA	0.02579	0.02594	1005.7	91-57-6	N/A			
2. Naphthalene	(0222)	MKBZ9680V	NA	NA	NA	1000	100	0.2	NA	0.02502	0.02511	1003.7	91-20-3	10 ppm (50mg/m3/8H)			
3. n-Nonane	95708	120222	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	NA	1000.0	4.2	111-84-2			
4. n-Decane	95708	120222	1.00	25.00	1000.9	1000	NA	0.013	NA	NA	NA	1000.2	4.2	124-18-5			
5. n-Dodecane	95708	120222	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	NA	1000.0	4.2	112-40-3			
6. n-Tetradecane	95708	120222	1.00	25.00	1002.1	1000	NA	0.013	NA	NA	NA	1001.3	4.2	629-59-4			
7. n-Hexadecane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.7	4.2	544-76-3			
8. n-Octadecane	95708	120222	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	NA	1000.3	4.1	593-45-3			
9. n-Eicosane	95708	120222	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	NA	1000.3	4.2	112-95-8			
10. n-Henelcosane	95708	120222	1.00	25.00	1002.4	1000	NA	0.013	NA	NA	NA	1001.6	4.2	628-94-7			
11. n-Docosane	95708	120222	1.00	25.00	1001.9	1000	NA	0.013	NA	NA	NA	1001.2	4.2	629-97-0			
12. n-Tetracosane	95708	120222	1.00	25.00	1000.8	1000	NA	0.013	NA	NA	NA	1000.1	4.2	646-31-1			
13. n-Hexacosane	95708	120222	1.00	25.00	1001.2	1000	NA	0.013	NA	NA	NA	1000.4	4.2	630-01-3			
14. n-Octacosane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.2	630-02-4			
15. n-Triacontane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.2	638-68-6			
16. n-Dotriacontane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.3	544-85-4			
17. n-Tetraacontane	95708	120222	1.00	25.00	1000.4	1000	NA	0.013	NA	NA	NA	999.7	4.2	14167-59-0			
18. n-Hexatriacontane	95708	120222	1.00	25.00	1000.3	1000	NA	0.013	NA	NA	NA	1000.8	4.2	630-08-8			
19. n-Octatriacontane	95708	120222	1.00	25.00	1001.5	1000	NA	0.013	NA	NA	NA	999.6	4.3	7194-85-6			
20. n-Tetracontane	95708	120222	1.00	25.00	1000.6	1000	NA	0.013	NA	NA	NA	999.9	4.3	4181-95-7			

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0207239

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : February 28, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13288 } Y.P.
↓
P13317 } 06/28/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.0 µg/mL	+/- 5.1926
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1839
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBM4146	98%	200.6 µg/mL	+/- 5.1815
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	199.9 µg/mL	+/- 5.1647
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	199.8 µg/mL	+/- 5.1621
8	n-Heneicosane (C21)	629-94-7	MKCL8682	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.7 µg/mL	+/- 5.1839
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.3 µg/mL	+/- 5.1753
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	199.8 µg/mL	+/- 5.1621
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.0 µg/mL	+/- 5.1926
15	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	200.7 µg/mL	+/- 5.1839
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	201.0 µg/mL	+/- 5.1915

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

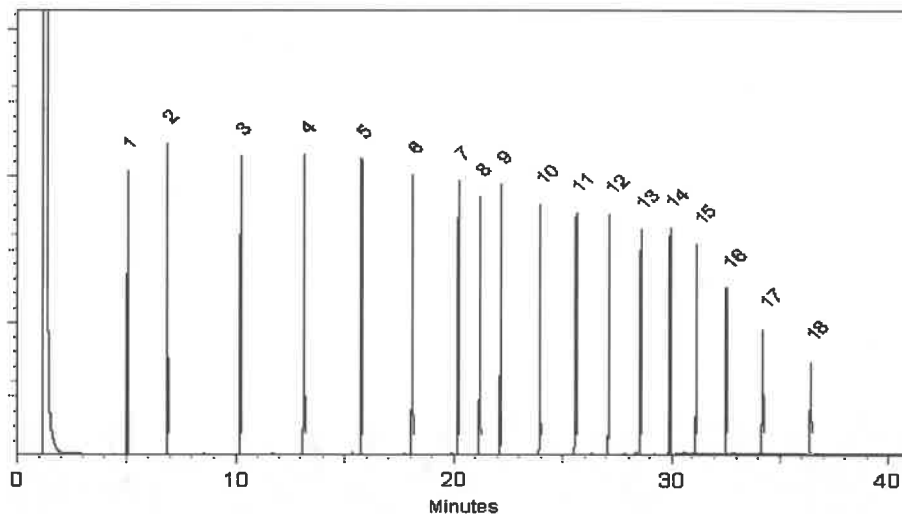

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Matt Fragassi - Mix Technician

Date Mixed: 31-Jan-2024 **Balance Serial #** 1128353505


Dillan Murphy - Operations Technician I

Date Passed: 02-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0207239

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : February 28, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13417 } Y-P.
2 }
P13429 } 07/11/24.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.0 µg/mL	+/- 5.1926
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1839
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBM4146	98%	200.6 µg/mL	+/- 5.1815
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	199.9 µg/mL	+/- 5.1647
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	199.8 µg/mL	+/- 5.1621
8	n-Heneicosane (C21)	629-94-7	MKCL8682	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKQC3882	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.7 µg/mL	+/- 5.1839
11	n-Hexacosane (C26)	630-01-3	MKQC4814	99%	200.3 µg/mL	+/- 5.1753
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKQC9436	97%	199.8 µg/mL	+/- 5.1621
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.0 µg/mL	+/- 5.1926
15	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	200.7 µg/mL	+/- 5.1839
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	201.0 µg/mL	+/- 5.1915

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.3 µg/mL	+/- 5.1753
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

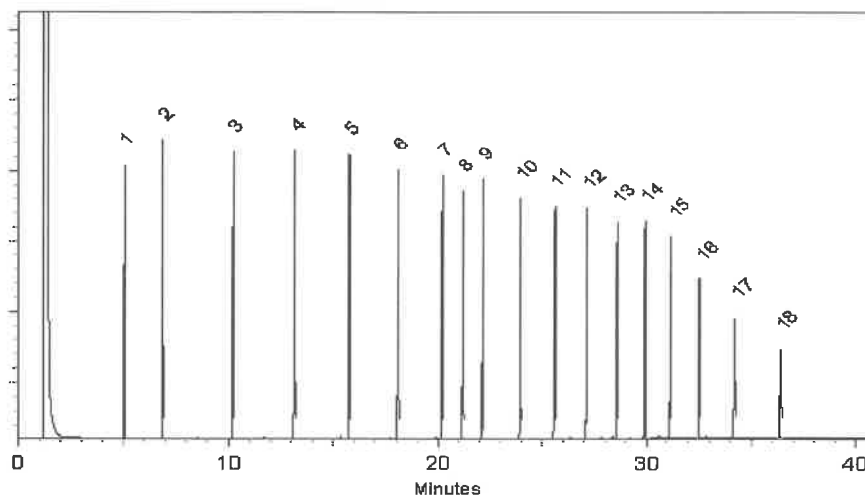

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Matt Fraga
Matt Fraga - Mix Technician

Date Mixed: 31-Jan-2024 **Balance Serial #** 1128353505

Dylan Murphy
Dylan Murphy - Operations Technician I

Date Passed: 02-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0207239

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : February 28, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13417 } Y-P.
2 }
P13429 } 07/11/24.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.0 µg/mL	+/- 5.1926
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1839
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBM4146	98%	200.6 µg/mL	+/- 5.1815
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	199.9 µg/mL	+/- 5.1647
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	199.8 µg/mL	+/- 5.1621
8	n-Heneicosane (C21)	629-94-7	MKCL8682	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKQC3882	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.7 µg/mL	+/- 5.1839
11	n-Hexacosane (C26)	630-01-3	MKQC4814	99%	200.3 µg/mL	+/- 5.1753
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKQC9436	97%	199.8 µg/mL	+/- 5.1621
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.0 µg/mL	+/- 5.1926
15	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	200.7 µg/mL	+/- 5.1839
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	201.0 µg/mL	+/- 5.1915

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.3 µg/mL	+/- 5.1753
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

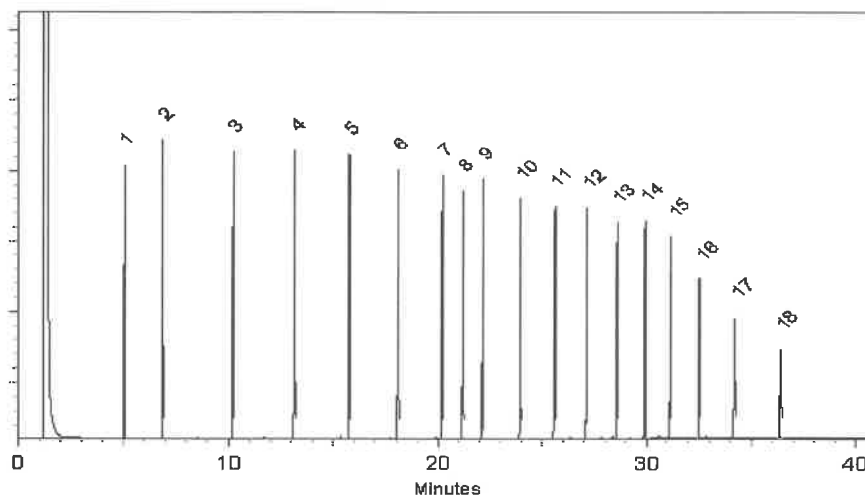

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Matt Fragaesi - Mix Technician

Date Mixed: 31-Jan-2024 **Balance Serial #** 1128353505


Dillan Murphy - Operations Technician I

Date Passed: 02-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0207239

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : February 28, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13h17 } Y-P.
2 }
P13h29 } 07/11/24.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.0 µg/mL	+/- 5.1926
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1839
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.7 µg/mL	+/- 5.1839
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBM4146	98%	200.6 µg/mL	+/- 5.1815
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	199.9 µg/mL	+/- 5.1647
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	199.8 µg/mL	+/- 5.1621
8	n-Heneicosane (C21)	629-94-7	MKCL8682	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKCCQ3882	99%	200.0 µg/mL	+/- 5.1667
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.7 µg/mL	+/- 5.1839
11	n-Hexacosane (C26)	630-01-3	MKCCQ4814	99%	200.3 µg/mL	+/- 5.1753
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCCQ9436	97%	199.8 µg/mL	+/- 5.1621
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.0 µg/mL	+/- 5.1926
15	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	200.7 µg/mL	+/- 5.1839
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.0 µg/mL	+/- 5.1667
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	201.0 µg/mL	+/- 5.1915

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.3 µg/mL	+/- 5.1753
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

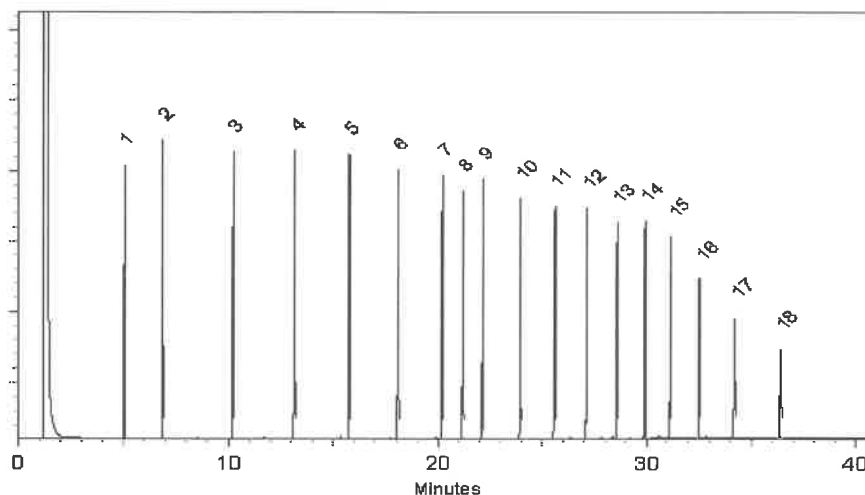

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Matt Fraga
Matt Fragaesi - Mix Technician

Date Mixed: 31-Jan-2024 **Balance Serial #** 1128353505

Dylan Murphy
Dylan Murphy - Operations Technician I

Date Passed: 02-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13430 } Y-8.
↓
P13436 } 67116124

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.5 µg/mL	+/- 5.1805
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

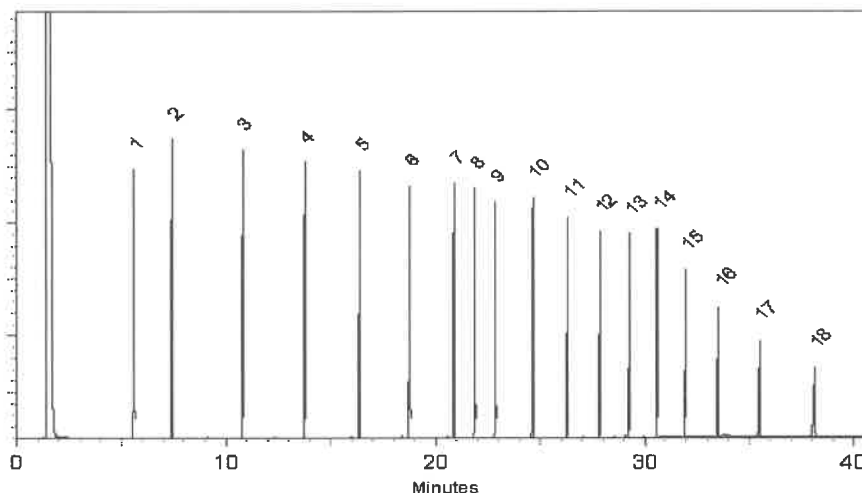

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 07-May-2024 **Balance Serial #** 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13430 } Y-8.
↓
P13436 } 67116124

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.5 µg/mL	+/- 5.1805
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

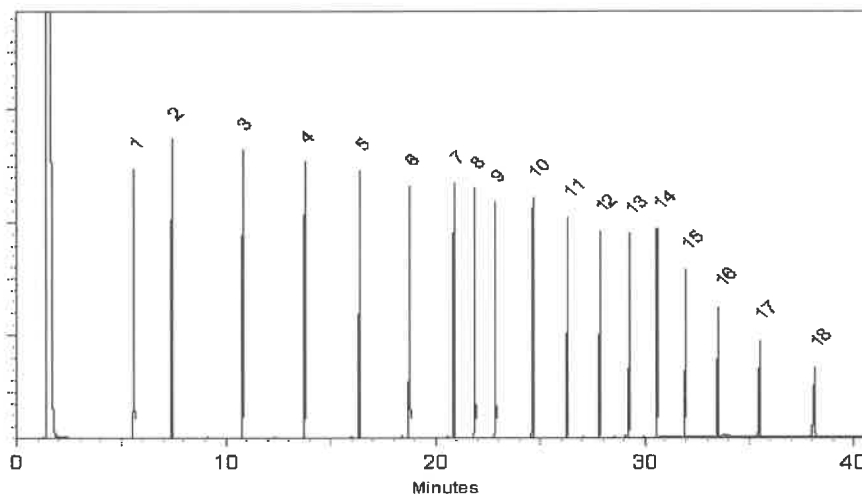

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 07-May-2024 **Balance Serial #** 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13430 } Y-8.
↓
P13436 } 67116124

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.5 µg/mL	+/- 5.1805
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

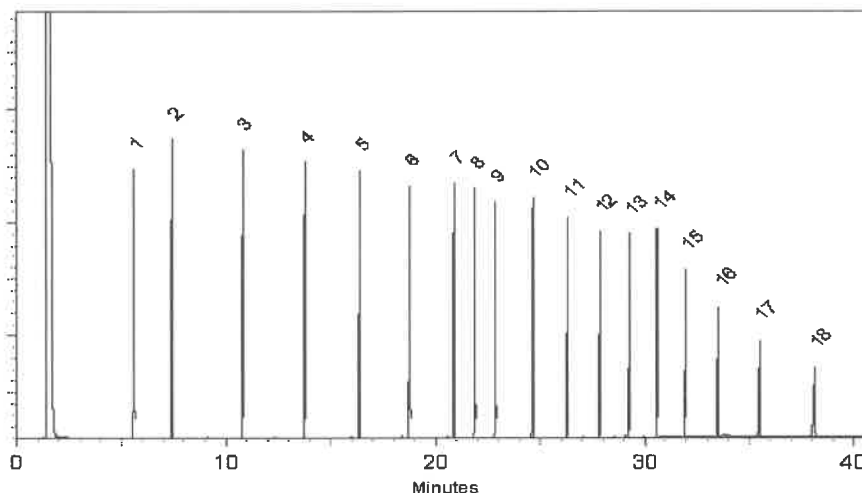

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-May-2024 **Balance Serial #** 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13430 } Y-8.
↓
P13436 } 67116124

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.5 µg/mL	+/- 5.1805
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

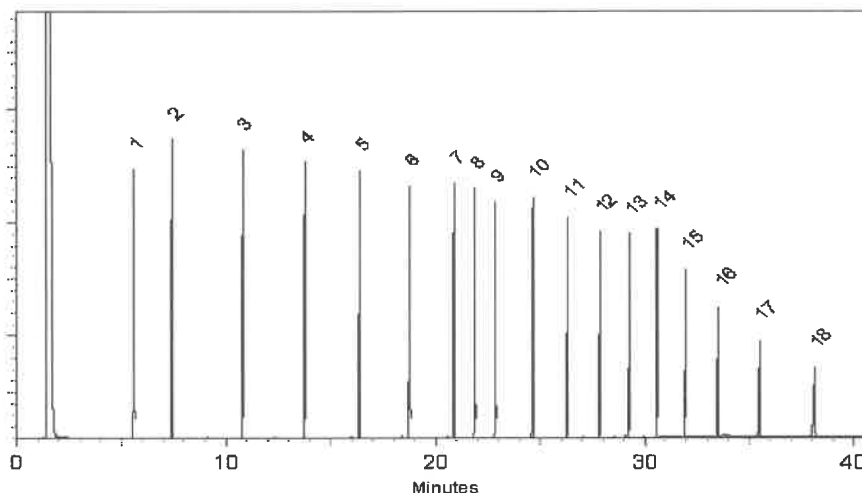

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-May-2024 **Balance Serial #** 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13430 } Y-8.
↓
P13436 } 67116124

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.5 µg/mL	+/- 5.1805
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

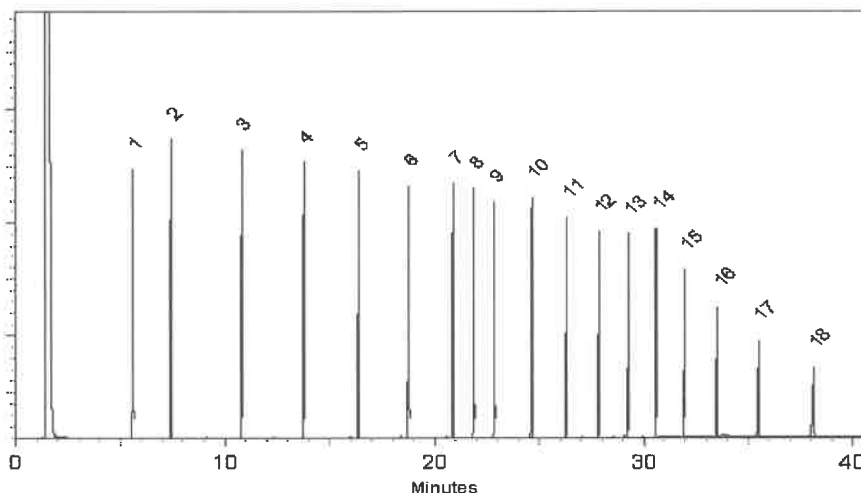

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-May-2024 **Balance Serial #** 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13430 } Y-8.
↓
P13436 } 67116124

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.5 µg/mL	+/- 5.1805
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

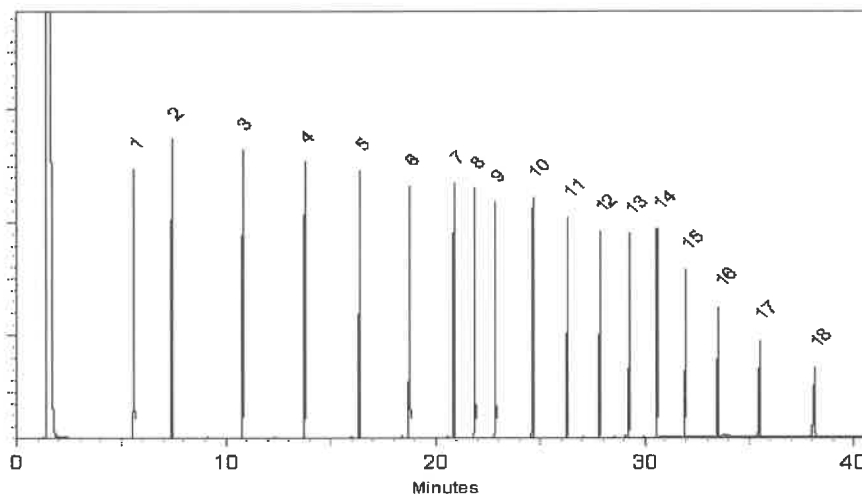

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-May-2024 **Balance Serial #** 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13430 } Y-8.
↓
P13436 } 67116124

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

18	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	200.5 µg/mL	+/- 5.1805
----	----------------------	-----------	-------	-----	-------------	------------

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-S (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

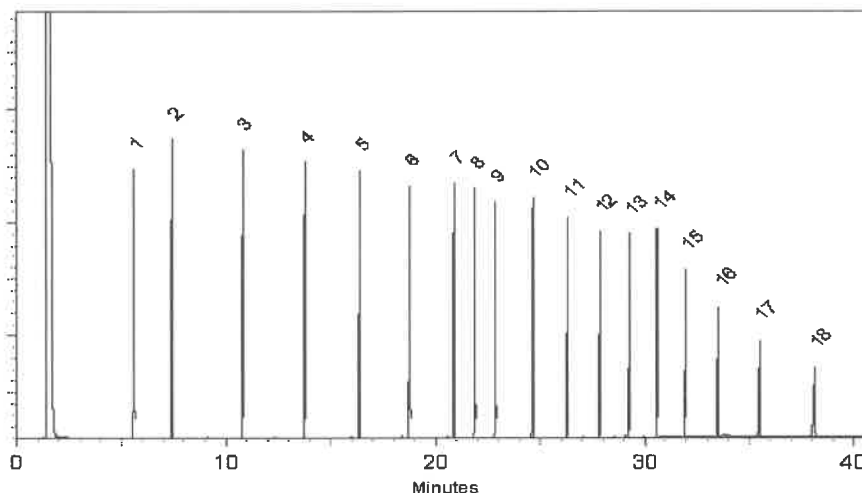

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 07-May-2024 **Balance Serial #** 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0211254

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13437
↓
P13452 } 7-P.
07/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

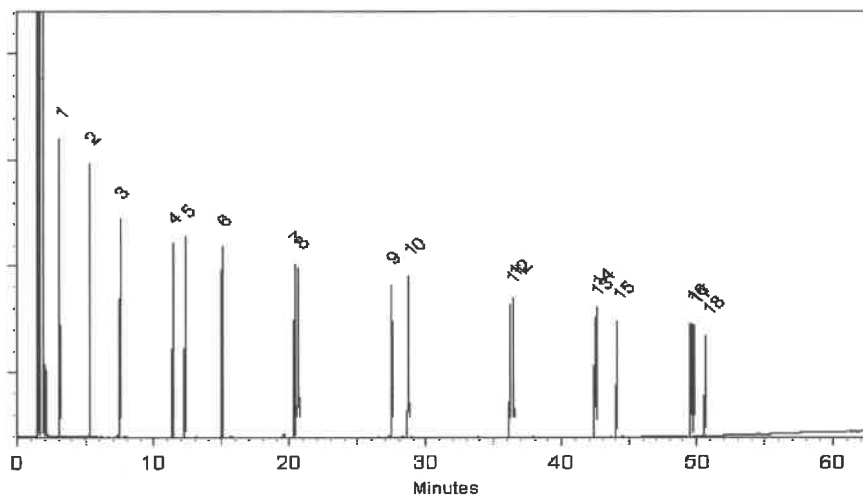

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 09-May-2024 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0211254

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13437
↓
P13452 } Y-P.
07/16/24.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

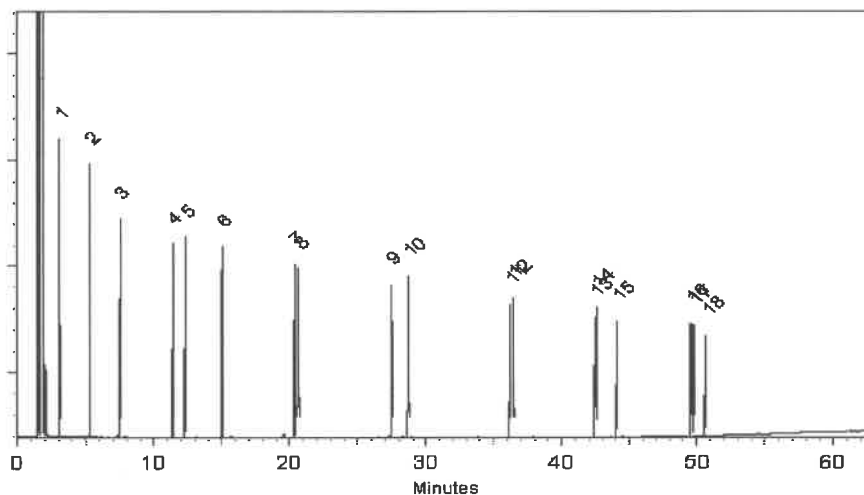

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 09-May-2024 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0211254

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13437
↓
P13452 } Y-P.
07/16/24.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

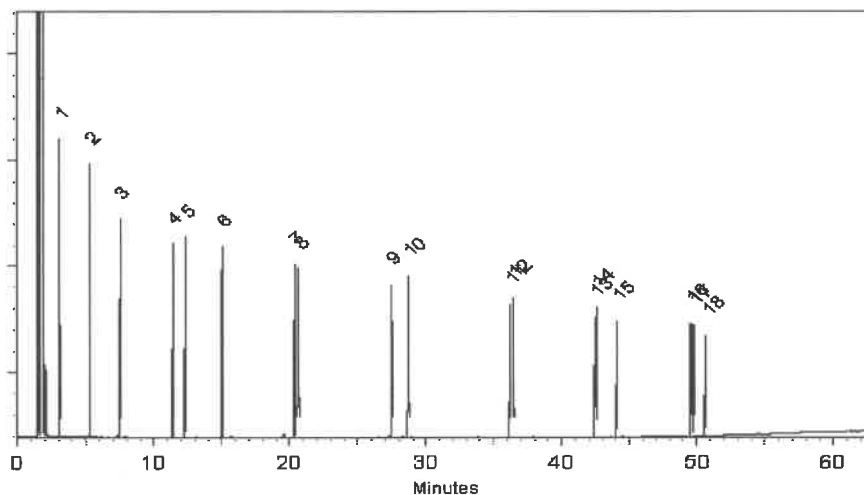

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 09-May-2024 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0211254

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13437
↓
P13452 } Y-P.
07/16/24.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

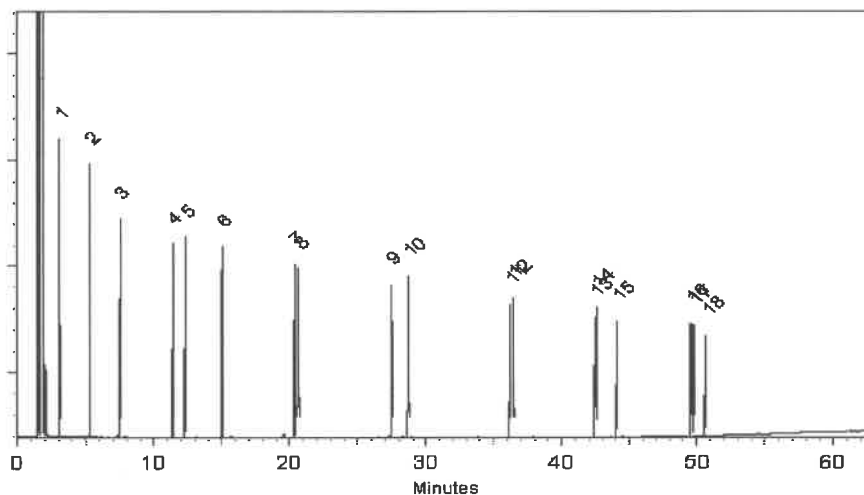

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 09-May-2024 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0211254

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13437
↓
P13452 } Y-P.
07/16/24.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

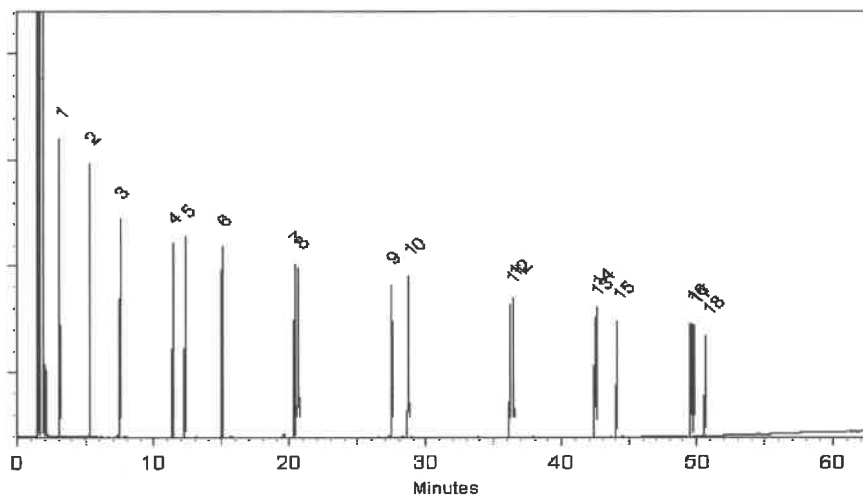

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 09-May-2024 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0211254

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13437
↓
P13452 } 7-P.
07/16/24.

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

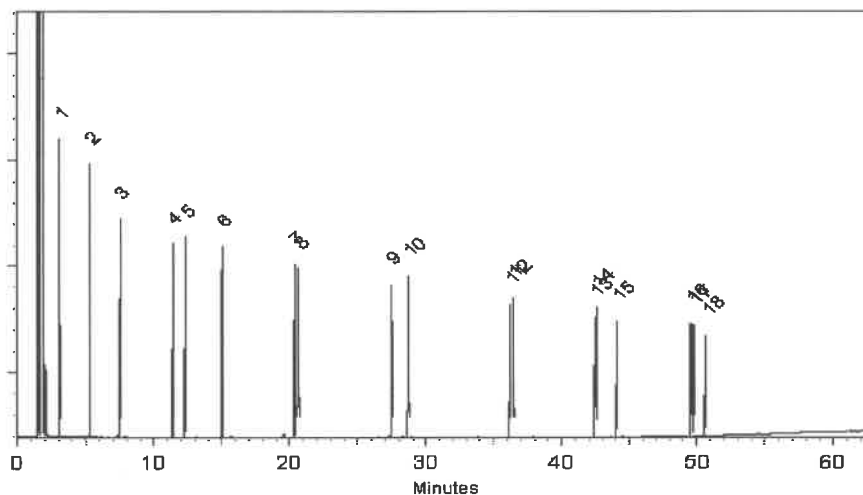

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 09-May-2024 **Balance Serial #** 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0207019

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13h53
↓
P13h56 } 7-P.
07/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.6 µg/mL	+/- 9.0384
2	Naphthalene	91-20-3	STBL1057	99%	200.6 µg/mL	+/- 9.0384
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0299
4	Acenaphthylene	208-96-8	L10L	95%	200.7 µg/mL	+/- 9.0437
5	Acenaphthene	83-32-9	MKCR7169	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10241100	99%	200.4 µg/mL	+/- 9.0294
7	Phenanthrene	85-01-8	MKCQ2033	99%	200.5 µg/mL	+/- 9.0330
8	Anthracene	120-12-7	MKCR0570	99%	200.7 µg/mL	+/- 9.0438
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.6 µg/mL	+/- 9.0366
10	Pyrene	129-00-0	BCCG8479	98%	200.7 µg/mL	+/- 9.0449
11	Benz(a)anthracene	56-55-3	I20012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP230601	99%	200.5 µg/mL	+/- 9.0330
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.6 µg/mL	+/- 9.0384
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.8 µg/mL	+/- 9.0456
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.6 µg/mL	+/- 9.0378
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0400

17	Dibenz(a,h)anthracene	53-70-3	ER032211-01	99%	200.4 µg/mL	+/- 9.0276
18	Benzo(g,h,i)perylene	191-24-2	RP231003RSR	99%	200.5 µg/mL	+/- 9.0330

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

20 ml/min.

Inj. Vol

1µl

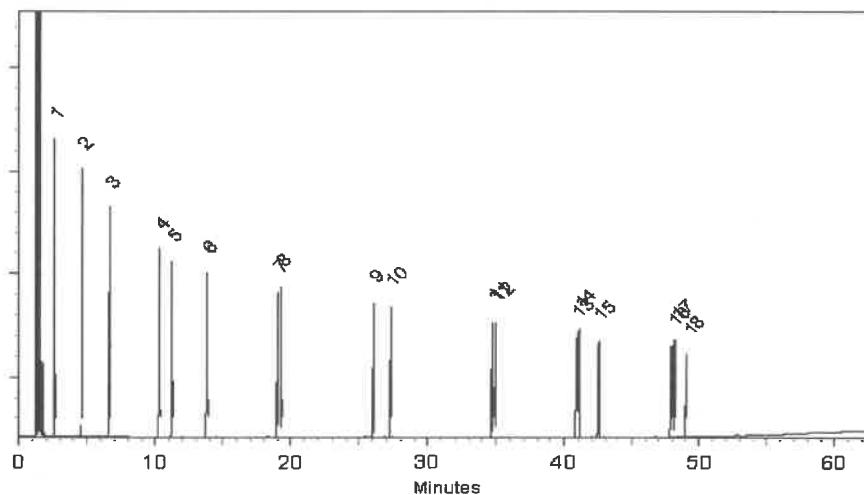

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Laith Clemente
Laith Clemente - Operations Technician I

Date Mixed: 25-Jan-2024

Balance Serial # 1128360905

Dillon Murphy
Dillon Murphy - Operations Technician I

Date Passed: 29-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0207019

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13h53
↓
P13h56 } 7-P.
07/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.6 µg/mL	+/- 9.0384
2	Naphthalene	91-20-3	STBL1057	99%	200.6 µg/mL	+/- 9.0384
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0299
4	Acenaphthylene	208-96-8	L10L	95%	200.7 µg/mL	+/- 9.0437
5	Acenaphthene	83-32-9	MKCR7169	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10241100	99%	200.4 µg/mL	+/- 9.0294
7	Phenanthrene	85-01-8	MKCQ2033	99%	200.5 µg/mL	+/- 9.0330
8	Anthracene	120-12-7	MKCR0570	99%	200.7 µg/mL	+/- 9.0438
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.6 µg/mL	+/- 9.0366
10	Pyrene	129-00-0	BCCG8479	98%	200.7 µg/mL	+/- 9.0449
11	Benz(a)anthracene	56-55-3	I20012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP230601	99%	200.5 µg/mL	+/- 9.0330
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.6 µg/mL	+/- 9.0384
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.8 µg/mL	+/- 9.0456
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.6 µg/mL	+/- 9.0378
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0400

17	Dibenz(a,h)anthracene	53-70-3	ER032211-01	99%	200.4 µg/mL	+/- 9.0276
18	Benzo(g,h,i)perylene	191-24-2	RP231003RSR	99%	200.5 µg/mL	+/- 9.0330

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
 Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

100°C (hold 1 min.) to 330°C
 @ 4°C/min. (hold 5 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

20 ml/min.

Inj. Vol

1µl

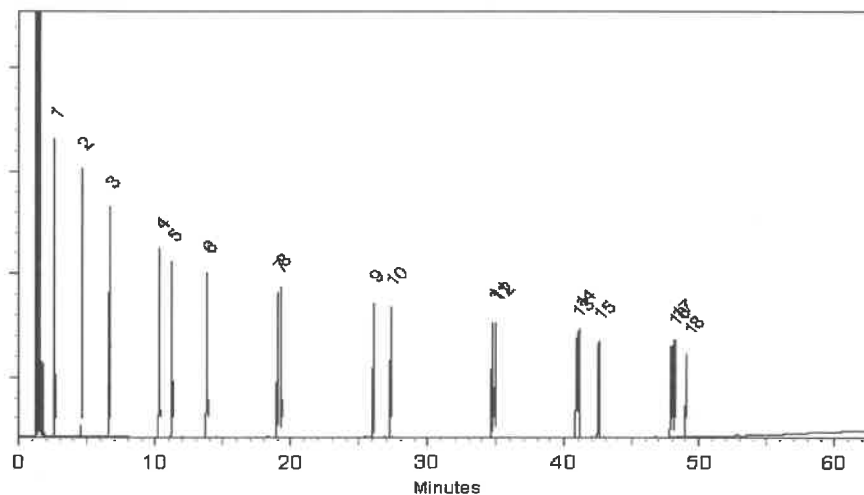

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


 Laith Clemente - Operations Technician I

Date Mixed: 25-Jan-2024

Balance Serial # 1128360905


 Dillan Murphy - Operations Technician I

Date Passed: 29-Jan-2024

Manufactured under Restek's ISO 9001:2015
 Registered Quality System
 Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0207019

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13h53
↓
P13h56 } 7-P.
07/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.6 µg/mL	+/- 9.0384
2	Naphthalene	91-20-3	STBL1057	99%	200.6 µg/mL	+/- 9.0384
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0299
4	Acenaphthylene	208-96-8	L10L	95%	200.7 µg/mL	+/- 9.0437
5	Acenaphthene	83-32-9	MKCR7169	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10241100	99%	200.4 µg/mL	+/- 9.0294
7	Phenanthrene	85-01-8	MKCQ2033	99%	200.5 µg/mL	+/- 9.0330
8	Anthracene	120-12-7	MKCR0570	99%	200.7 µg/mL	+/- 9.0438
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.6 µg/mL	+/- 9.0366
10	Pyrene	129-00-0	BCCG8479	98%	200.7 µg/mL	+/- 9.0449
11	Benz(a)anthracene	56-55-3	I20012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP230601	99%	200.5 µg/mL	+/- 9.0330
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.6 µg/mL	+/- 9.0384
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.8 µg/mL	+/- 9.0456
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.6 µg/mL	+/- 9.0378
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0400

17	Dibenz(a,h)anthracene	53-70-3	ER032211-01	99%	200.4 µg/mL	+/- 9.0276
18	Benzo(g,h,i)perylene	191-24-2	RP231003RSR	99%	200.5 µg/mL	+/- 9.0330

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
 Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

100°C (hold 1 min.) to 330°C
 @ 4°C/min. (hold 5 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

20 ml/min.

Inj. Vol

1µl

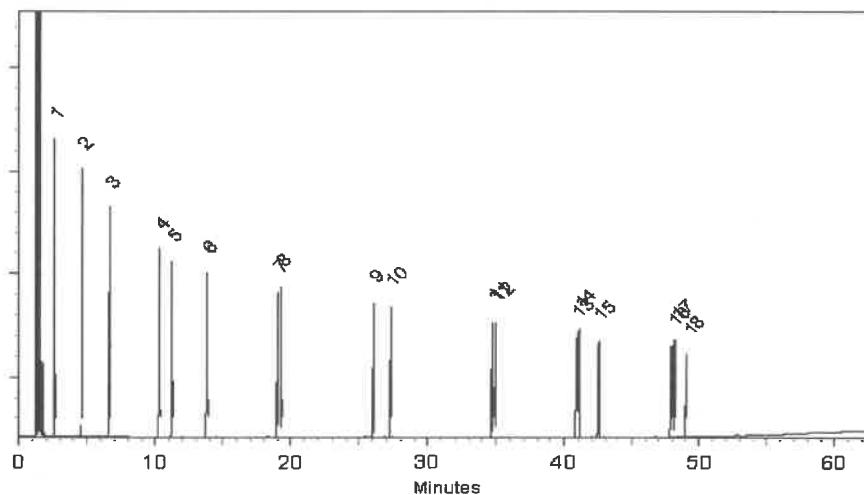

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
 Laith Clemente - Operations Technician I

Date Mixed: 25-Jan-2024

Balance Serial # 1128360905

[Signature]
 Dillan Murphy - Operations Technician I

Date Passed: 29-Jan-2024

Manufactured under Restek's ISO 9001:2015
 Registered Quality System
 Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543 **Lot No.:** A0207019

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : December 31, 2029 **Storage:** 10°C or colder

Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13h53
↓
P13h56 } 7-P.
07/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.6 µg/mL	+/- 9.0384
2	Naphthalene	91-20-3	STBL1057	99%	200.6 µg/mL	+/- 9.0384
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0299
4	Acenaphthylene	208-96-8	L10L	95%	200.7 µg/mL	+/- 9.0437
5	Acenaphthene	83-32-9	MKCR7169	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10241100	99%	200.4 µg/mL	+/- 9.0294
7	Phenanthrene	85-01-8	MKCQ2033	99%	200.5 µg/mL	+/- 9.0330
8	Anthracene	120-12-7	MKCR0570	99%	200.7 µg/mL	+/- 9.0438
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.6 µg/mL	+/- 9.0366
10	Pyrene	129-00-0	BCCG8479	98%	200.7 µg/mL	+/- 9.0449
11	Benz(a)anthracene	56-55-3	I20012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP230601	99%	200.5 µg/mL	+/- 9.0330
13	Benzo(b)fluoranthene	205-99-2	022013B	99%	200.6 µg/mL	+/- 9.0384
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.8 µg/mL	+/- 9.0456
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.6 µg/mL	+/- 9.0378
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0400

17	Dibenz(a,h)anthracene	53-70-3	ER032211-01	99%	200.4 µg/mL	+/- 9.0276
18	Benzo(g,h,i)perylene	191-24-2	RP231003RSR	99%	200.5 µg/mL	+/- 9.0330

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

20 ml/min.

Inj. Vol

1µl

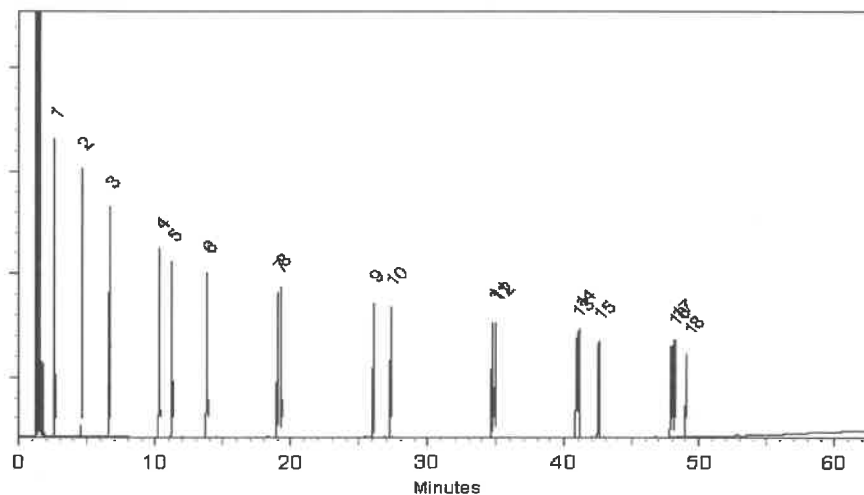

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Laith Clemente
Laith Clemente - Operations Technician I

Date Mixed: 25-Jan-2024

Balance Serial # 1128360905

Dillon Murphy
Dillon Murphy - Operations Technician I

Date Passed: 29-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31480 **Lot No.:** A0210831
Description : MA Fractionation Surrogate Spike Mix
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : March 31, 2030 **Storage:** 10°C or colder
Handling: Sonication required. Mix is photosensitive. **Ship:** Ambient

P13h57
↓
P13h78 } Y.P.
67/23/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,031.0 µg/mL	+/- 181.5871
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,037.5 µg/mL	+/- 181.8799

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

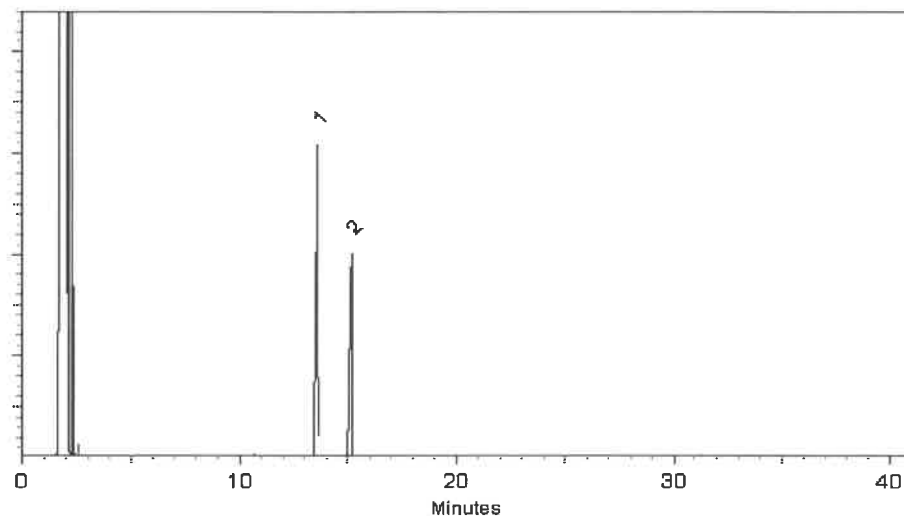

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 29-Apr-2024

Balance Serial #

B345965662

Dillan Murphy - Operations Technician I

Date Passed: 30-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13625
↓
P13644 } Y.P.
10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane**CAS #** 109-66-0**Purity** 99%

Quality Confirmation Test

Column:30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

Temp. Program:40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

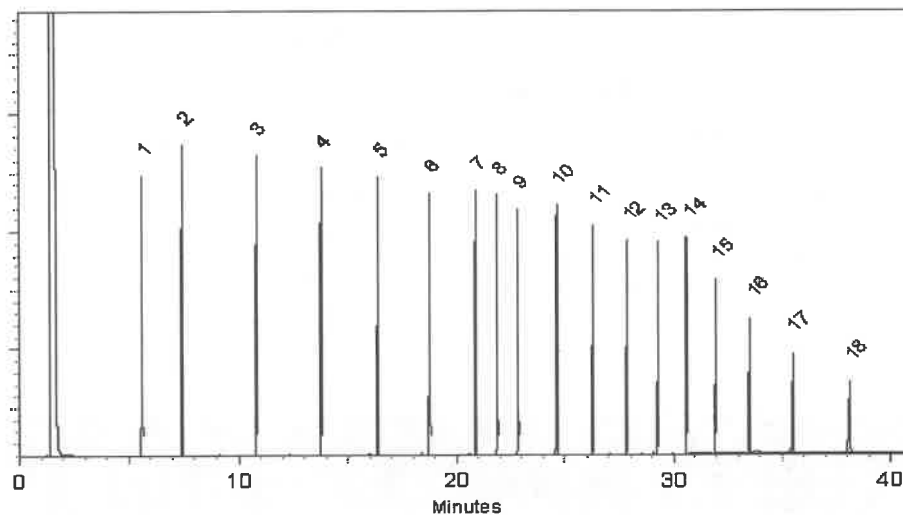

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I**Date Mixed:** 07-May-2024**Balance Serial #** 1128360905
Jennifer Pollino - Operations Tech III - ARM QC**Date Passed:** 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13625
↓
P13644 } Y.P.
10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane**CAS #** 109-66-0**Purity** 99%

Quality Confirmation Test

Column:30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

Temp. Program:40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

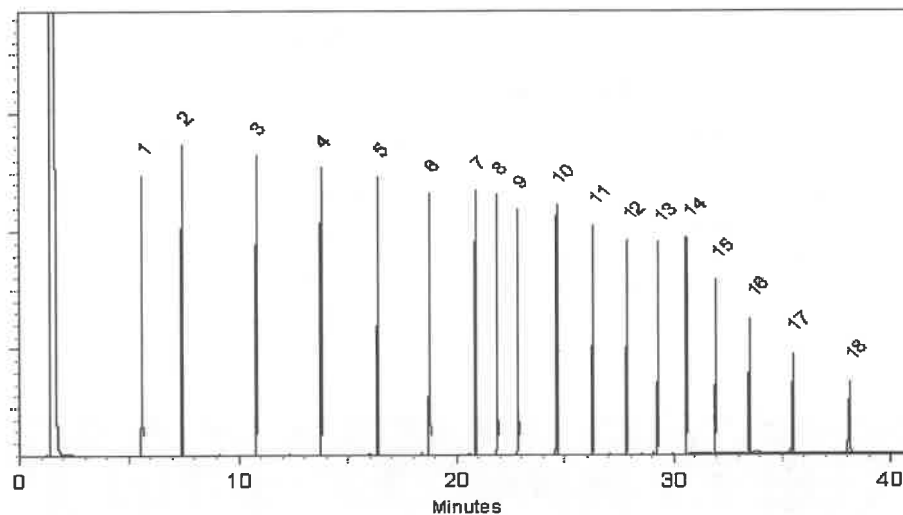

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I**Date Mixed:** 07-May-2024**Balance Serial #** 1128360905
Jennifer Pollino - Operations Tech III - ARM QC**Date Passed:** 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30542 **Lot No.:** A0211112

Description : NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : June 30, 2031 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

P13625
↓
P13644 } Y.P.
10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.9 µg/mL	+/- 5.1891
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	200.7 µg/mL	+/- 5.1857
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.4 µg/mL	+/- 5.1771
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.6 µg/mL	+/- 5.1822
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	200.4 µg/mL	+/- 5.1782
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.4 µg/mL	+/- 5.1771
8	n-Heneicosane (C21)	629-94-7	MKCL3226	99%	200.5 µg/mL	+/- 5.1796
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.6 µg/mL	+/- 5.1814
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.5 µg/mL	+/- 5.1805
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCG0084	99%	200.5 µg/mL	+/- 5.1796
13	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	200.4 µg/mL	+/- 5.1763
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.4 µg/mL	+/- 5.1779
15	n-Tetratriacontane (C34)	14167-59-0	D3MZN	99%	200.5 µg/mL	+/- 5.1805
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	200.5 µg/mL	+/- 5.1808

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane
CAS # 109-66-0
Purity 99%

Quality Confirmation Test

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

330°C

Det. Type:


FID

Split Vent:

2 ml/min.

Inj. Vol

1µl

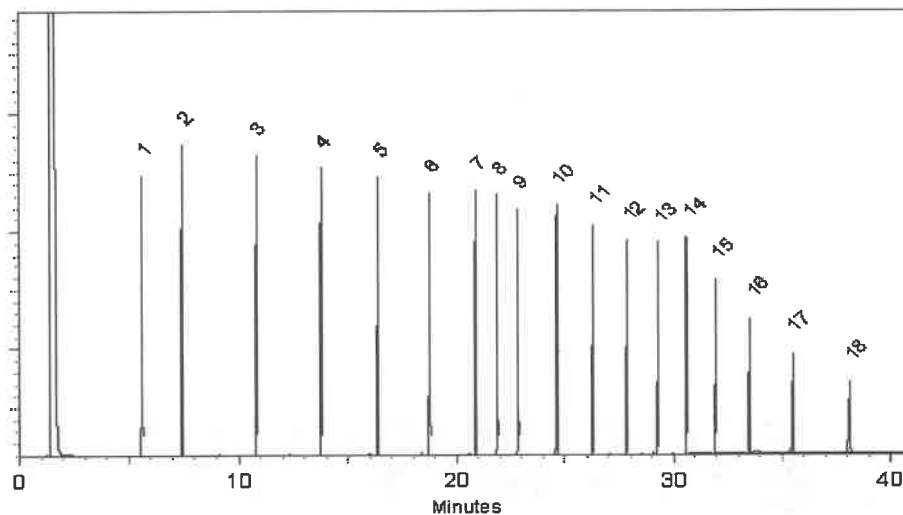

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 07-May-2024

Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-May-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A } 7.P
↓
p13727 } 10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

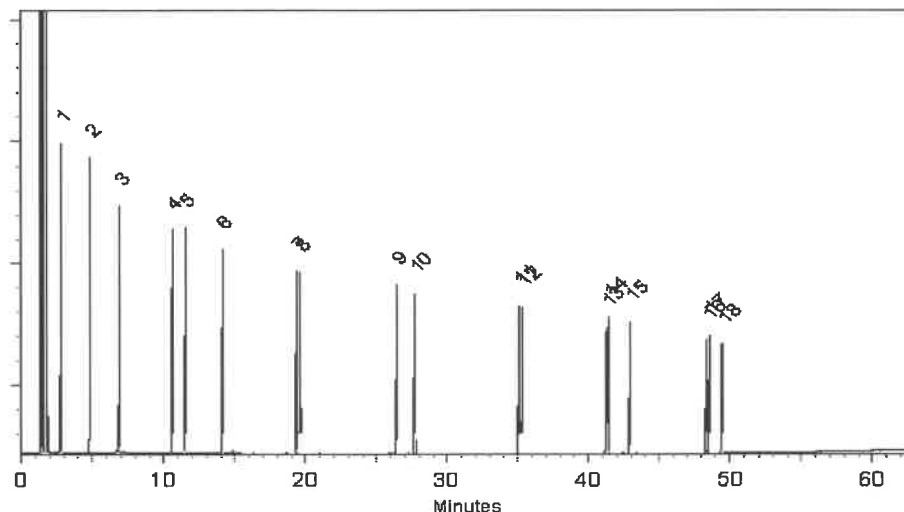

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A
↓
p13727
7.P
10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKQC4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

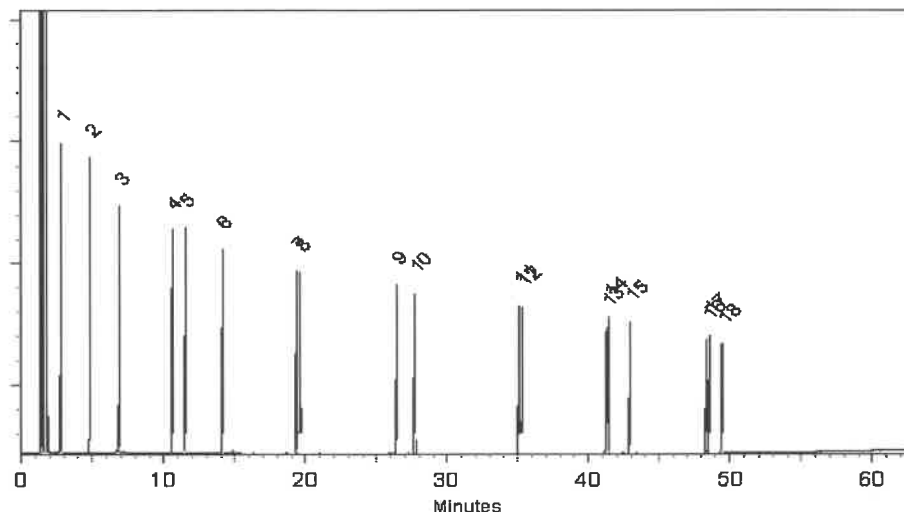

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A
↓
p13727
7.P
10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKQCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

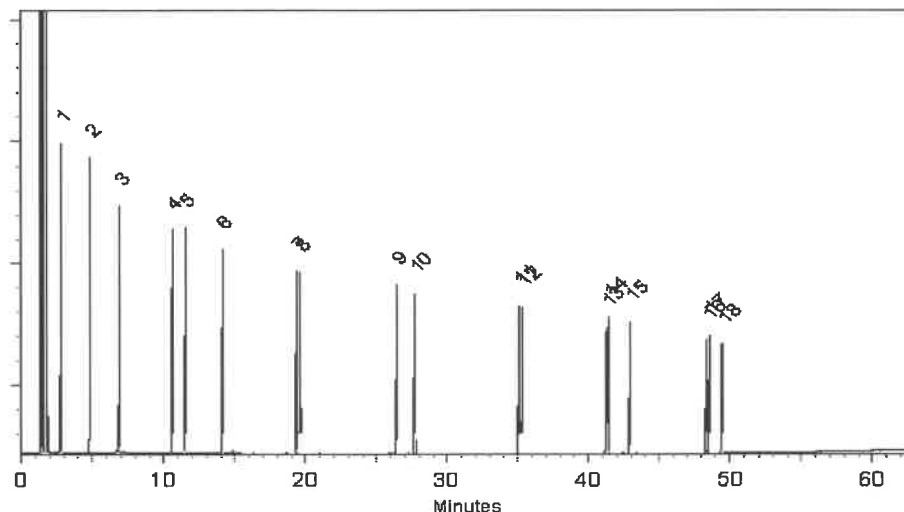

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A } 7.P
↓
p13727 } 10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKQC4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

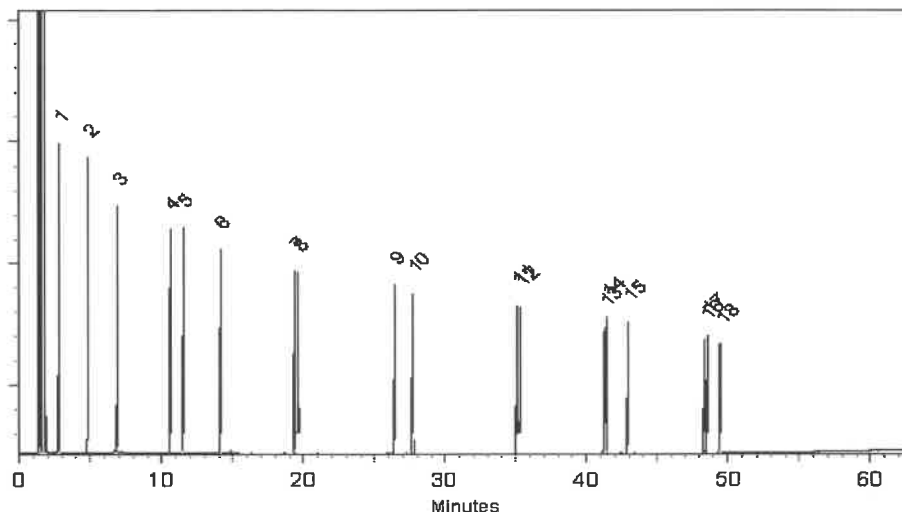

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024

Balance Serial # 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A
↓
p13727
7.P
10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKQC4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

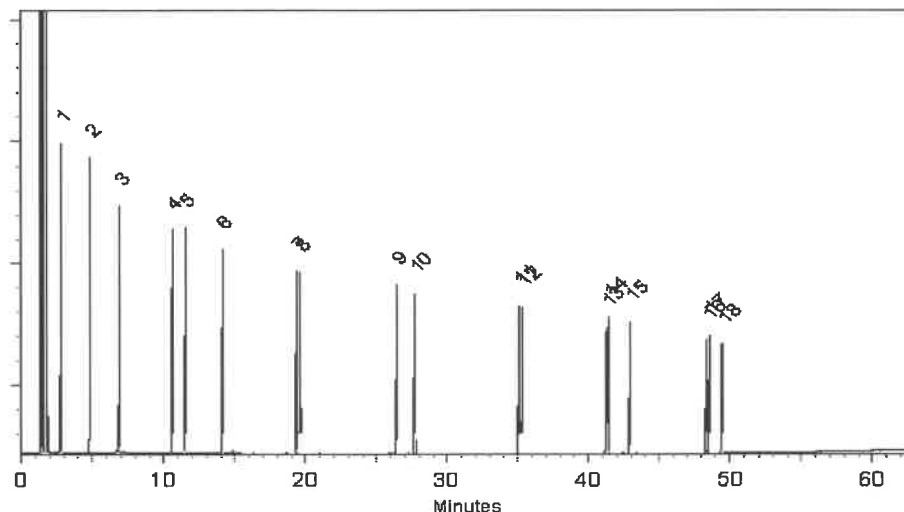

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A
↓
p13727
7.P
10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKQC4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

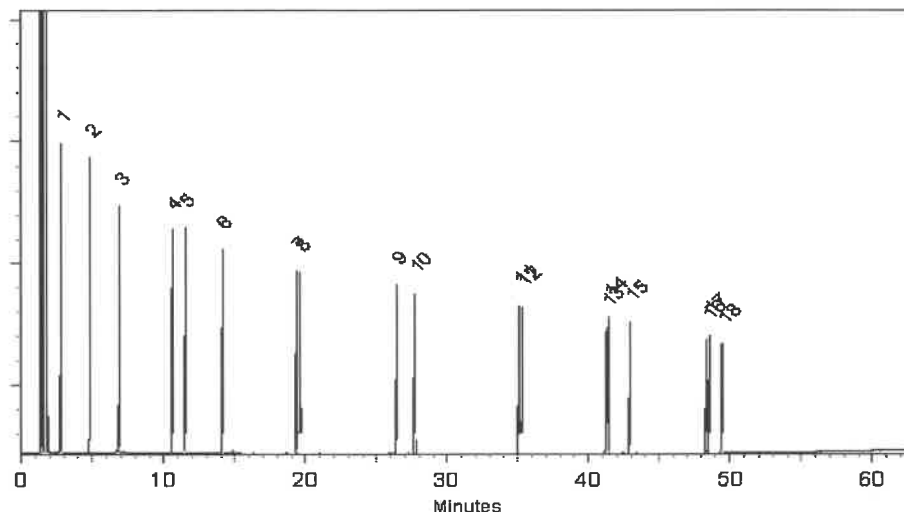

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50),
5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is
photosensitive.

Ship: Ambient

p137A } 7.P
↓
p13727 } 10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKQC4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683


17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)
Carrier Gas:
hydrogen-constant pressure 10 psi.
Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)
Inj. Temp:
250°C
Det. Temp:
330°C
Det. Type:
FID
Split Vent:
20 ml/min.
Inj. Vol
1µl

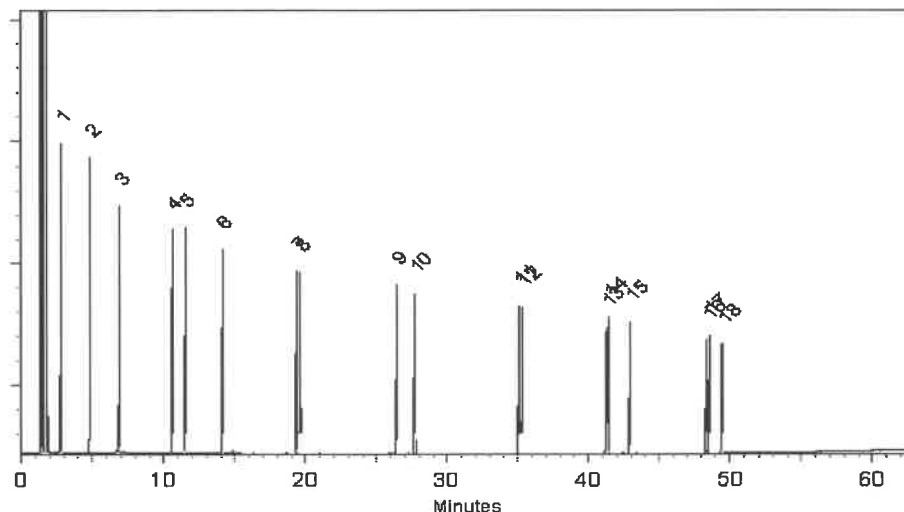

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A } 7.P
↓
p13727 } 10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

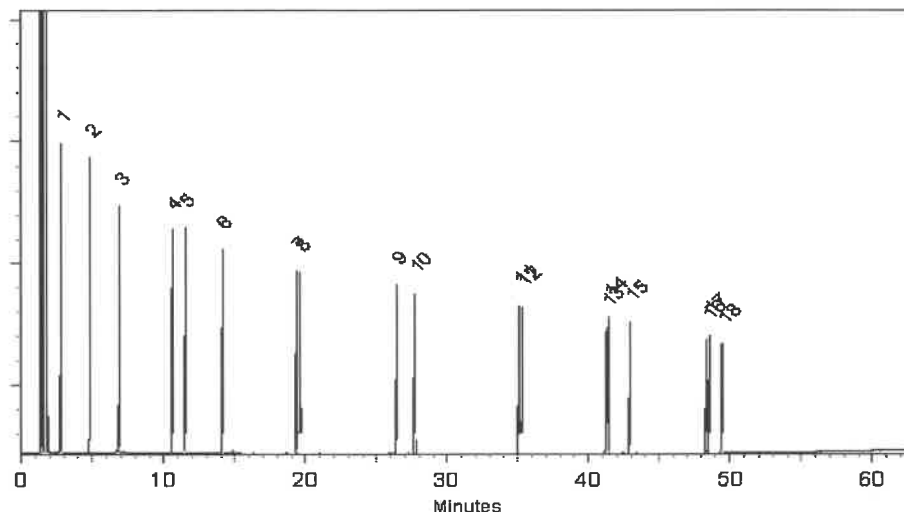

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A
↓
p13727
7.P
10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKQC4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

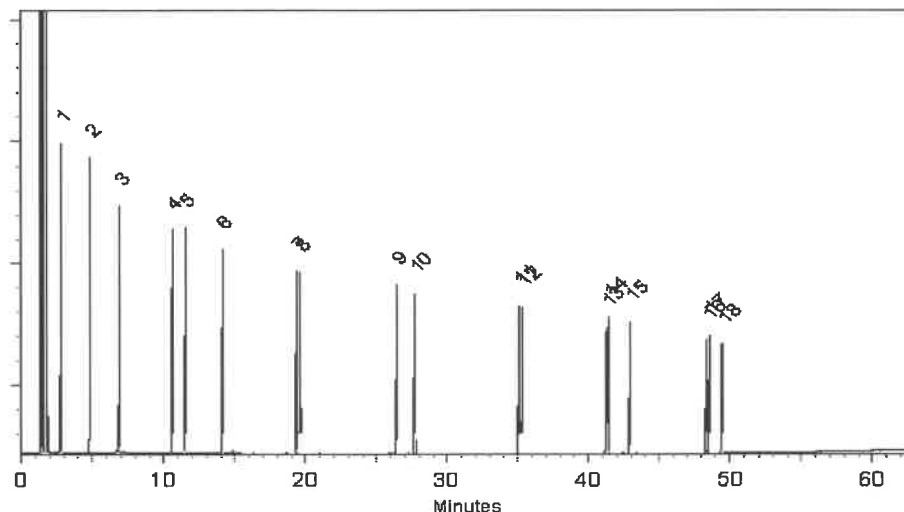

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30543

Lot No.: A0217838

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : September 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

p137A
↓
p13727 } 7.P
10/24/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	201.6 µg/mL	+/- 9.0835
2	Naphthalene	91-20-3	STBL1057	99%	200.0 µg/mL	+/- 9.0114
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	214935V18H	95%	199.1 µg/mL	+/- 8.9717
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.5 µg/mL	+/- 9.0784
7	Phenanthrene	85-01-8	MKCT3391	99%	201.2 µg/mL	+/- 9.0655
8	Anthracene	120-12-7	101492T18R	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKQC4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCK2592	99%	200.0 µg/mL	+/- 9.0114
11	Benz(a)anthracene	56-55-3	I60012022BAA	99%	200.0 µg/mL	+/- 9.0114
12	Chrysene	218-01-9	RP240627ECS	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	052013B	99%	201.2 µg/mL	+/- 9.0655
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	201.6 µg/mL	+/- 9.0835
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	199.9 µg/mL	+/- 9.0078
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.0 µg/mL	+/- 8.9683

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240625RSR	97%	199.0 µg/mL	+/- 8.9683

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone/Toluene (50:50)
CAS # 67-64-1/108-88-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
100°C (hold 1 min.) to 330°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
20 ml/min.

Inj. Vol
1µl

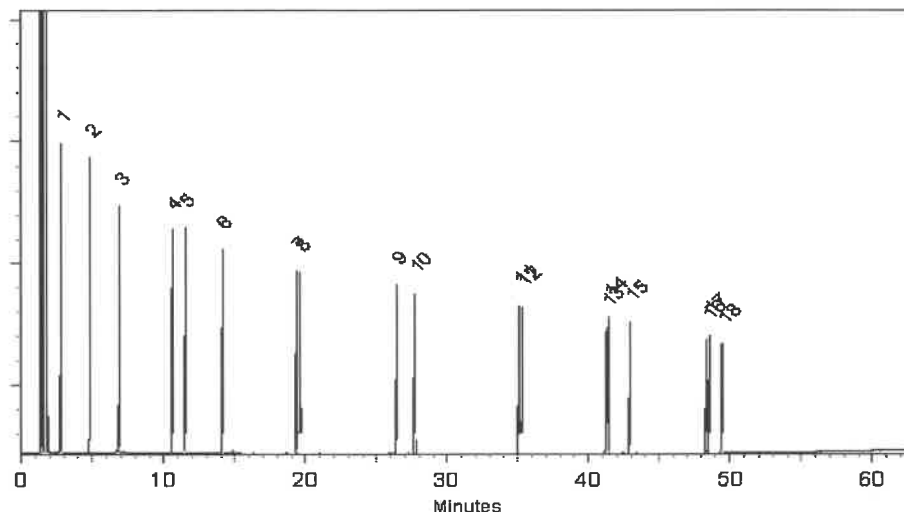

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Rebecca Gingerich
Rebecca Gingerich - Operations Tech II

Date Mixed: 14-Oct-2024 **Balance Serial #** 1128360905

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 21-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

