

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102824\
 Data File : P0107460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 00:09
 Operator : YP/AJ
 Sample : P4578-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WB-305-TOP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/29/2024
 Supervised By :Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:56:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.370	3.643	147.6E6	64601581	16.191m	20.072m
2) SA Decachlor...	10.054	8.633	40999655	40497778	16.712	14.772

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102824\
Data File : PO107460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 00:09
Operator : YP/AJ
Sample : P4578-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WB-305-TOP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2024
Supervised By :Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:56:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

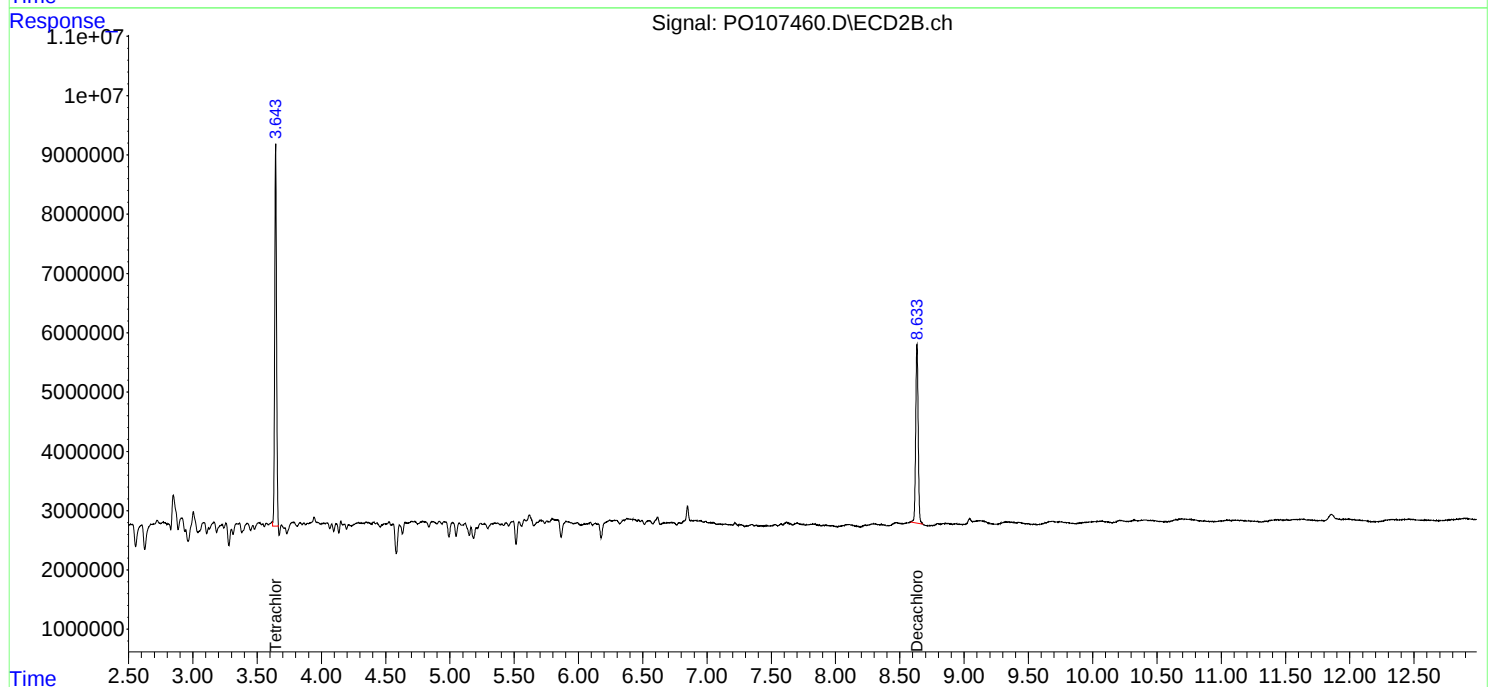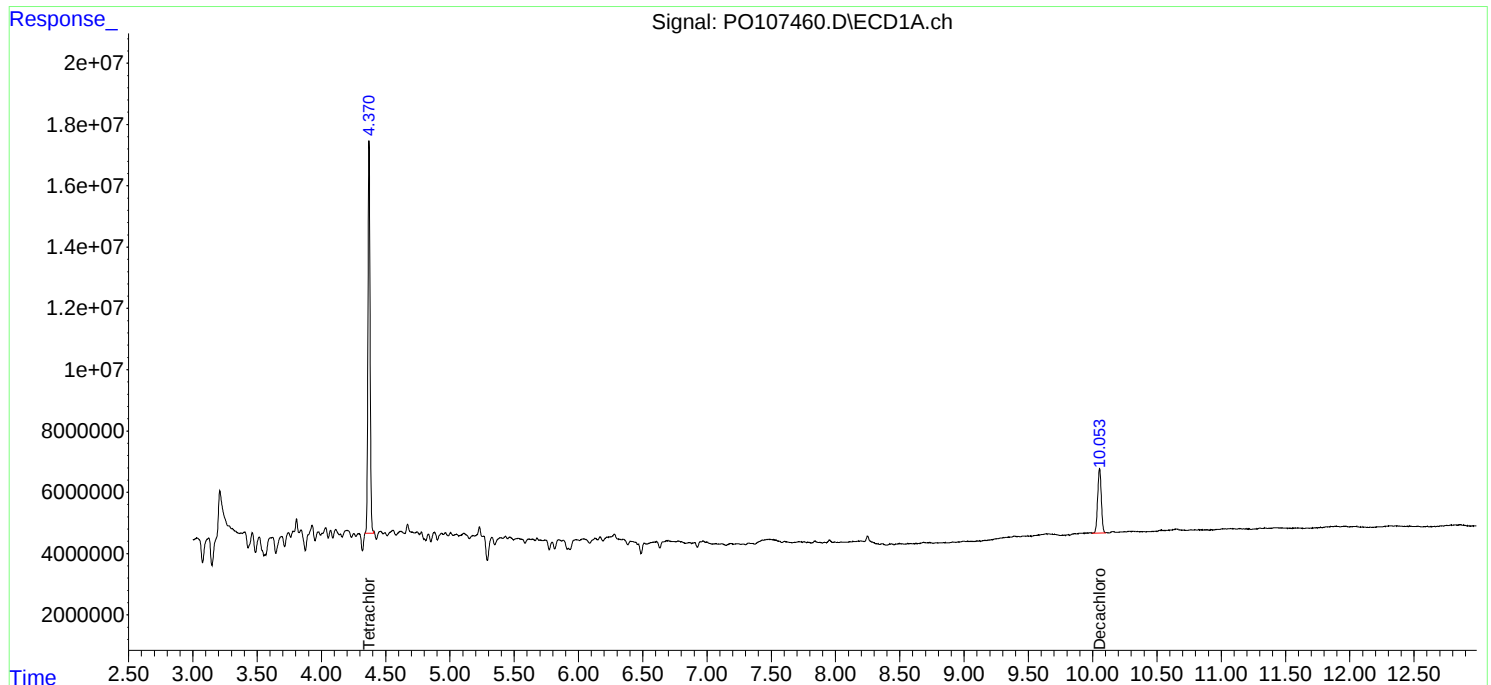

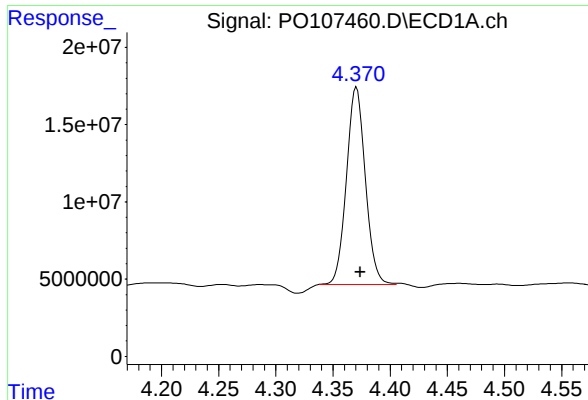


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: -0.004 min
Response: 147562908
Conc: 16.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
WB-305-TOP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2024
Supervised By :Ankita Jodhani 10/29/2024

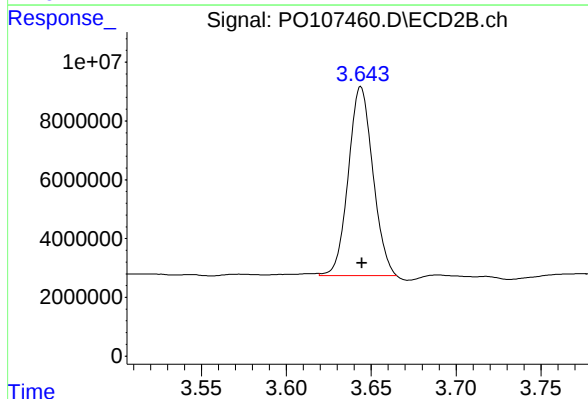


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.001 min
Response: 64601581
Conc: 20.07 ng/ml

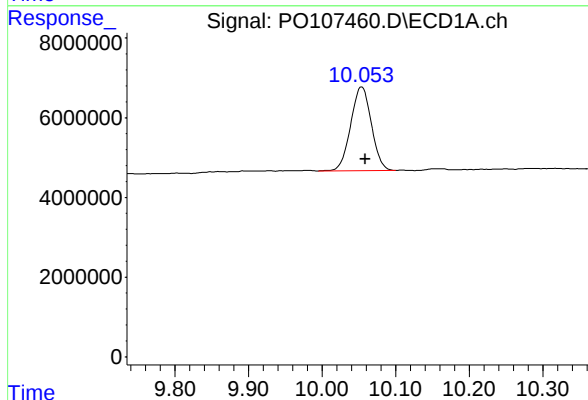

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: -0.005 min
Response: 40999655
Conc: 16.71 ng/ml

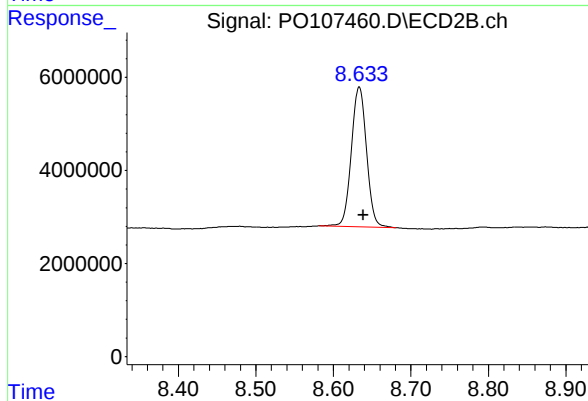

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.005 min
Response: 40497778
Conc: 14.77 ng/ml