

Cover Page

Order ID : P4578

Project ID : Amtrak Sawtooth Bridges 2024

Client : Portal Partners Tri-Venture

Lab Sample Number

P4578-01
P4578-02
P4578-03
P4578-04
P4578-05
P4578-06
P4578-07
P4578-08
P4578-09

Client Sample Number

WB-305-SW
WB-305-SW-1
WB-305-TOP
WB-305-TOP-1
WB-305-BOT
WB-305-BOT
WB-305-BOT-1
WB-305-BOT-1
TB-10252024

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 11/6/2024

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following "Results Qualifiers" are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as "12 B".
E	Indicates the analyte 's concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: P4578

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Custody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: KETAN PATEL

Date: 11/06/2024

LAB CHRONICLE

OrderID:	P4578	OrderDate:	10/25/2024 3:58:00 PM
Client:	Portal Partners Tri-Venture	Project:	Amtrak Sawtooth Bridges 2024
Contact:	Joseph Krupansky	Location:	K63,VOA Ref. #2 Soil,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
P4578-01	WB-305-SW	WATER	PCB	8082A	10/25/24	10/29/24	10/29/24	10/25/24
P4578-02	WB-305-SW-1	WATER	PCB	8082A	10/25/24	10/29/24	10/29/24	10/25/24
P4578-03	WB-305-TOP	SOIL	PCB	8082A	10/25/24	10/28/24	10/29/24	10/25/24
P4578-04	WB-305-TOP-1	SOIL	PCB	8082A	10/25/24	10/28/24	10/29/24	10/25/24
P4578-05	WB-305-BOT	SOIL	PCB	8082A	10/25/24	10/28/24	10/29/24	10/25/24
P4578-06	WB-305-BOT	TCLP	TCLP Pesticide	8081B	10/25/24	10/26/24	10/29/24	10/25/24
P4578-07	WB-305-BOT-1	SOIL	PCB	8082A	10/25/24	10/28/24	10/29/24	10/25/24
P4578-08	WB-305-BOT-1	TCLP	TCLP Pesticide	8081B	10/25/24	10/26/24	10/29/24	10/25/24



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: P4578

Order ID: P4578

Client: Portal Partners Tri-Venture

Project ID: Amtrak Sawtooth Bridges 2024

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: **P4578**

Client: **Portal Partners Tri-Venture**

Analytical Method: **8081B**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PL092652.D	PIBLK-PL092652.D	Decachlorobiphenyl	1	20	22.7	114		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	21.6	108		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	21.7	109		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	20.4	102		30 (77)	150 (126)
I.BLK-PL092693.D	PIBLK-PL092693.D	Decachlorobiphenyl	1	20	23.1	115		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	22.4	112		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	23.5	118		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	21.5	107		30 (77)	150 (126)
PB164445BL	PB164445BL	Decachlorobiphenyl	1	20	19.2	96		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	18.3	91		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	18.5	92		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	17.8	89		30 (77)	150 (126)
PB164445BS	PB164445BS	Decachlorobiphenyl	1	20	19.5	98		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	18.1	91		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	18.4	92		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	17.0	85		30 (77)	150 (126)
PB164393TB	PB164393TB	Decachlorobiphenyl	1	20	19.7	98		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	18.3	92		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	18.9	94		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	17.5	87		30 (77)	150 (126)
P4578-06	WB-305-BOT	Decachlorobiphenyl	1	20	13.7	68		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	18.1	91		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	13.2	66		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	18.0	90		30 (77)	150 (126)
P4578-06MS	WB-305-BOTMS	Decachlorobiphenyl	1	20	15.9	80		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	18.1	91		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	15.5	78		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	18.4	92		30 (77)	150 (126)
P4578-06MSD	WB-305-BOTMSD	Decachlorobiphenyl	1	20	15.8	79		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	18.0	90		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	15.8	79		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	18.4	92		30 (77)	150 (126)
P4578-08	WB-305-BOT-1	Decachlorobiphenyl	1	20	16.5	83		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	17.7	89		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	16.7	83		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	17.3	86		30 (77)	150 (126)
I.BLK-PL092710.D	PIBLK-PL092710.D	Decachlorobiphenyl	1	20	23.8	119		30 (43)	150 (140)
		Tetrachloro-m-xylene	1	20	23.1	115		30 (77)	150 (126)
		Decachlorobiphenyl	2	20	24.7	124		30 (43)	150 (140)
		Tetrachloro-m-xylene	2	20	22.5	113		30 (77)	150 (126)

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P4578

Client: Portal Partners Tri-Venture

Analytical Method: 8081B

DataFile : PL092701.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	WB-305-BOTMS											
P4578-06MS	gamma-BHC (Lindane)	0.5	0	0.46	ug/L	92				30 (60)	150 (152)	
	Heptachlor	0.5	0	0.47	ug/L	94				30 (56)	150 (147)	
	Heptachlor epoxide	0.5	0	0.46	ug/L	93				30 (77)	150 (143)	
	Endrin	0.5	0	0.47	ug/L	94				30 (76)	150 (144)	
	Methoxychlor	0.5	0	0.46	ug/L	91				30 (70)	150 (142)	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P4578

Client: Portal Partners Tri-Venture

Analytical Method: 8081B

DataFile : PL092702.D

Lab Sample ID:	Parameter	Spike	Sample		Units	Rec	Rec	RPD		Limits		
			Qual	RPD			Qual	Low	High	RPD		
Client Sample ID:	WB-305-BOTMSD											
P4578-06MSD	gamma-BHC (Lindane)	0.5	0	0.46	ug/L	92		0		30 (60)	150 (152)	20 (20)
	Heptachlor	0.5	0	0.47	ug/L	94		0		30 (56)	150 (147)	20 (20)
	Heptachlor epoxide	0.5	0	0.46	ug/L	93		0		30 (77)	150 (143)	20 (20)
	Endrin	0.5	0	0.47	ug/L	93		1		30 (76)	150 (144)	20 (20)
	Methoxychlor	0.5	0	0.46	ug/L	91		0		30 (70)	150 (142)	20 (20)

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: P4578

Client: Portal Partners Tri-Venture

Analytical Method: **8081B** Datafile : PL092698.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB164445BS	gamma-BHC (Lindane)	0.05	0.048	ug/L	96				40 (82)	140 (129)	
	Heptachlor	0.05	0.050	ug/L	99				40 (79)	140 (127)	
	Heptachlor epoxide	0.05	0.049	ug/L	98				40 (81)	140 (124)	
	Endrin	0.05	0.045	ug/L	91				40 (81)	140 (128)	
	Methoxychlor	0.05	0.045	ug/L	90				40 (78)	140 (108)	

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB164445BL

Lab Name: CHEMTECH

Contract: PORT06

Lab Code: CHEM Case No.: P4578

SAS No.: P4578 SDG NO.: P4578

Lab Sample ID: PB164445BL

Lab File ID: PL092697.D

Matrix: (soil/water) water

Extraction: (Type) _____

Sulfur Cleanup: (Y/N) N

Date Extracted: 10/26/2024

Date Analyzed (1): 10/29/2024

Date Analyzed (2): 10/29/2024

Time Analyzed (1): 10:43

Time Analyzed (2): 10:43

Instrument ID (1): ECD_L

Instrument ID (2): ECD_L

GC Column (1): ZB-MR2 ID: 0.32 (mm)

GC Column (2): ZB-MR1 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB164445BS	PB164445BS	PL092698.D	10/29/2024	10/29/2024
PB164393TB	PB164393TB	PL092699.D	10/29/2024	10/29/2024
WB-305-BOT	P4578-06	PL092700.D	10/29/2024	10/29/2024
WB-305-BOTMS	P4578-06MS	PL092701.D	10/29/2024	10/29/2024
WB-305-BOTMSD	P4578-06MSD	PL092702.D	10/29/2024	10/29/2024
WB-305-BOT-1	P4578-08	PL092703.D	10/29/2024	10/29/2024

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	10/25/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	10/25/24
Client Sample ID:	WB-305-BOT	SDG No.:	P4578
Lab Sample ID:	P4578-06	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0
Sample Wt/Vol:	100	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	TCLP Pesticide
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Decanted:	
		Final Vol:	1000
		Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092700.D	1	10/26/24 12:50	10/29/24 11:23	PB164445

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.0049	U	0.0049	0.050	ug/L
76-44-8	Heptachlor	0.0054	U	0.0054	0.050	ug/L
1024-57-3	Heptachlor epoxide	0.0090	U	0.0090	0.050	ug/L
72-20-8	Endrin	0.0043	U	0.0043	0.050	ug/L
72-43-5	Methoxychlor	0.011	U	0.011	0.050	ug/L
8001-35-2	Toxaphene	0.15	U	0.15	1.00	ug/L
57-74-9	Chlordane	0.082	U	0.082	0.50	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	13.7		30 (43) - 150 (140)	68%	SPK: 20
877-09-8	Tetrachloro-m-xylene	18.1		30 (77) - 150 (126)	91%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 11:23
 Operator : AR\AJ
 Sample : P4578-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WB-305-BOT

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/30/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 05:12:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.779	44417090	48927074	18.128	17.980
28) SA Decachlor...	9.052	7.915	26283055	35975975	13.657	13.182
Target Compounds						
2) A alpha-BHC	3.995	3.282	1097432	1528799	0.324m	0.383

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 11:23
Operator : AR\AJ
Sample : P4578-06
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WB-305-BOT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/30/2024
Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 05:12:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

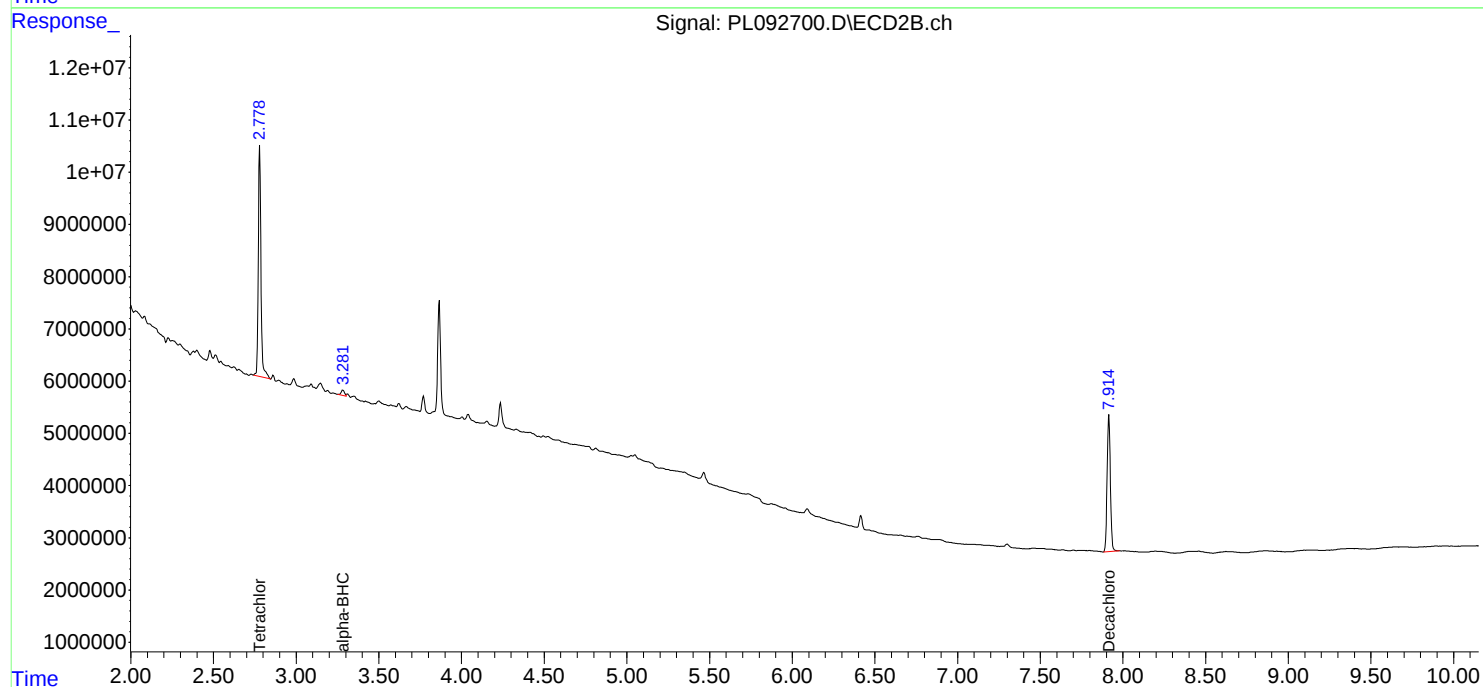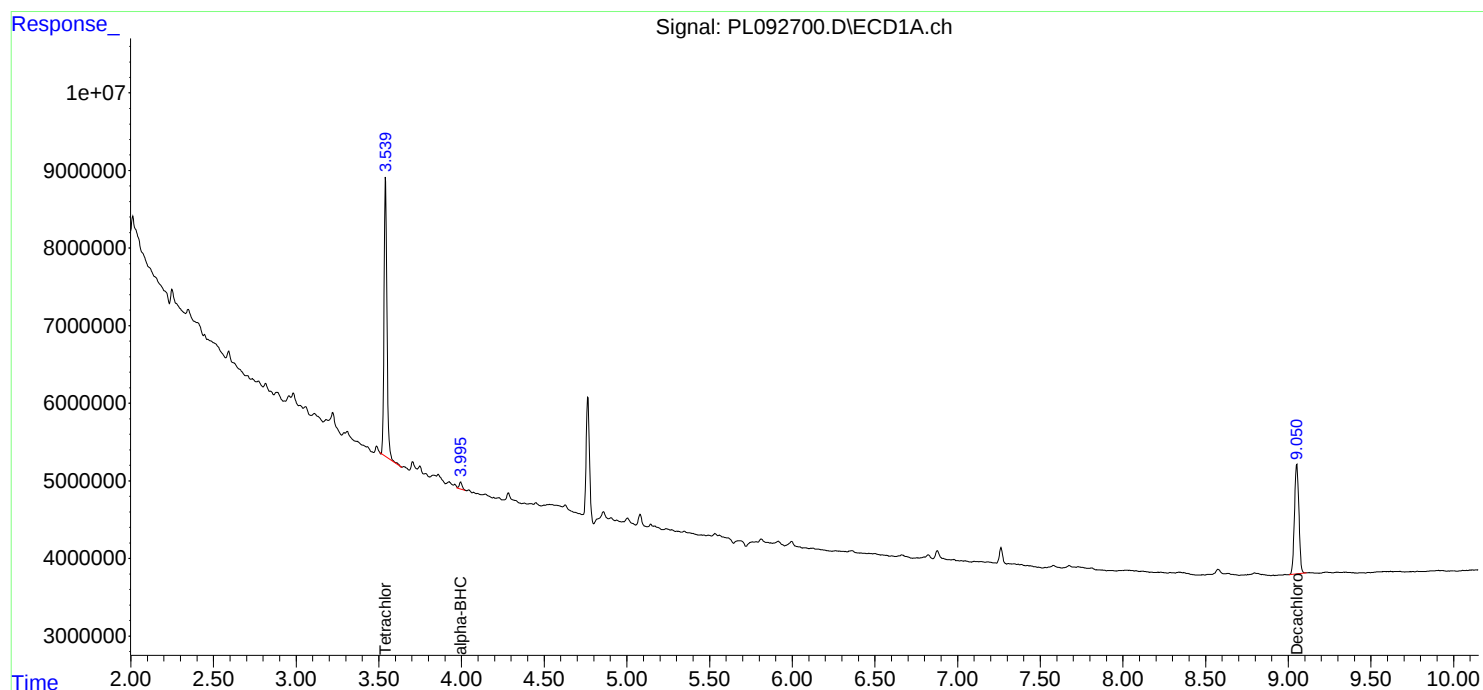

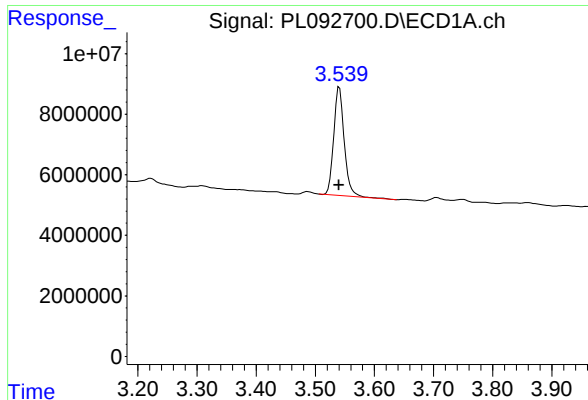


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 44417090
Conc: 18.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
WB-305-BOT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/30/2024
Supervised By :Ankita Jodhani 11/04/2024

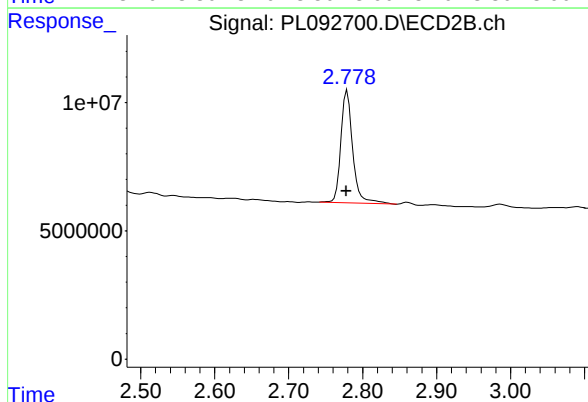


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.001 min
Response: 48927074
Conc: 17.98 ng/ml

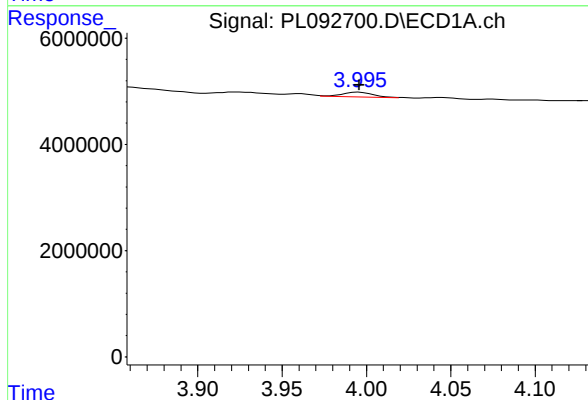


#2 alpha-BHC

R.T.: 3.995 min
Delta R.T.: -0.001 min
Response: 1097432
Conc: 0.32 ng/ml m

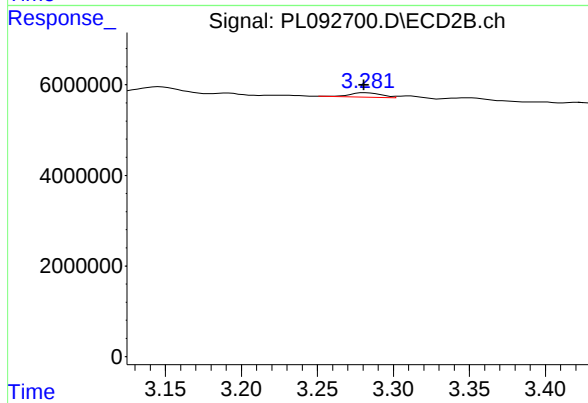

#2 alpha-BHC

R.T.: 3.282 min
Delta R.T.: 0.001 min
Response: 1528799
Conc: 0.38 ng/ml

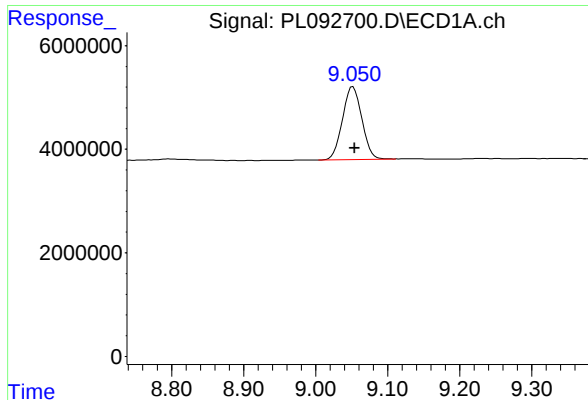


#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: -0.002 min
Response: 26283055
Conc: 13.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
WB-305-BOT

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/30/2024
Supervised By :Ankita Jodhani 11/04/2024

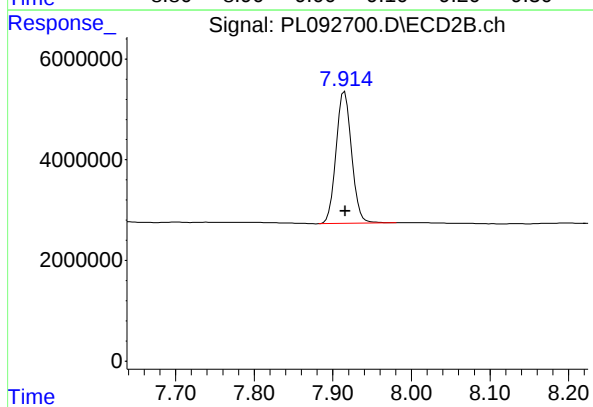

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 35975975
Conc: 13.18 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	10/25/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	10/25/24
Client Sample ID:	WB-305-BOT-1	SDG No.:	P4578
Lab Sample ID:	P4578-08	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0
Sample Wt/Vol:	100	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	TCLP Pesticide
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Decanted:	
		Final Vol:	1000
		Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092703.D	1	10/26/24 12:50	10/29/24 12:04	PB164445

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.0049	U	0.0049	0.050	ug/L
76-44-8	Heptachlor	0.0054	U	0.0054	0.050	ug/L
1024-57-3	Heptachlor epoxide	0.0090	U	0.0090	0.050	ug/L
72-20-8	Endrin	0.0043	U	0.0043	0.050	ug/L
72-43-5	Methoxychlor	0.011	U	0.011	0.050	ug/L
8001-35-2	Toxaphene	0.15	U	0.15	1.00	ug/L
57-74-9	Chlordane	0.082	U	0.082	0.50	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	16.7		30 (43) - 150 (140)	83%	SPK: 20
877-09-8	Tetrachloro-m-xylene	17.7		30 (77) - 150 (126)	89%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 12:04
 Operator : AR\AJ
 Sample : P4578-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WB-305-BOT-1

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/30/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:13:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.779	43357398	46969618	17.695m	17.261
28) SA Decachlor...	9.051	7.915	31815674	45553727	16.531	16.691

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 12:04
Operator : AR\AJ
Sample : P4578-08
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WB-305-BOT-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/30/2024
Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:13:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

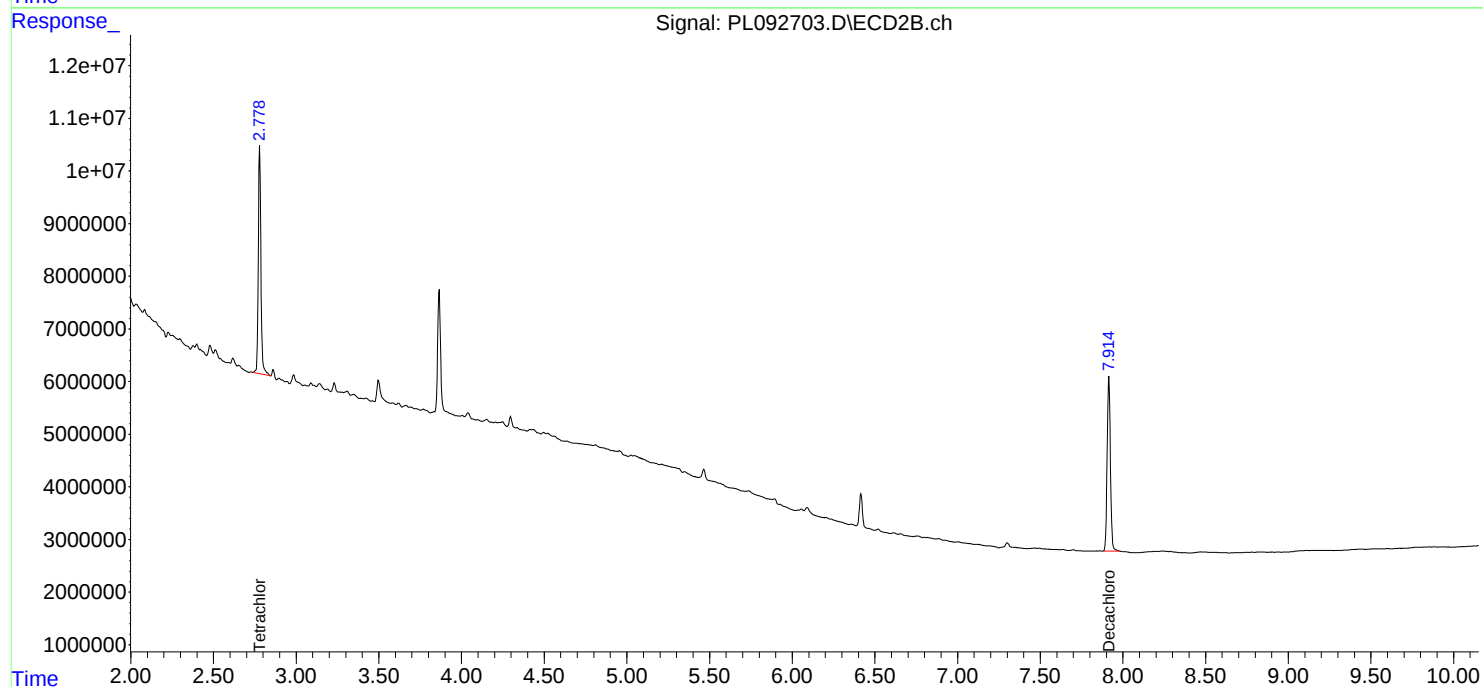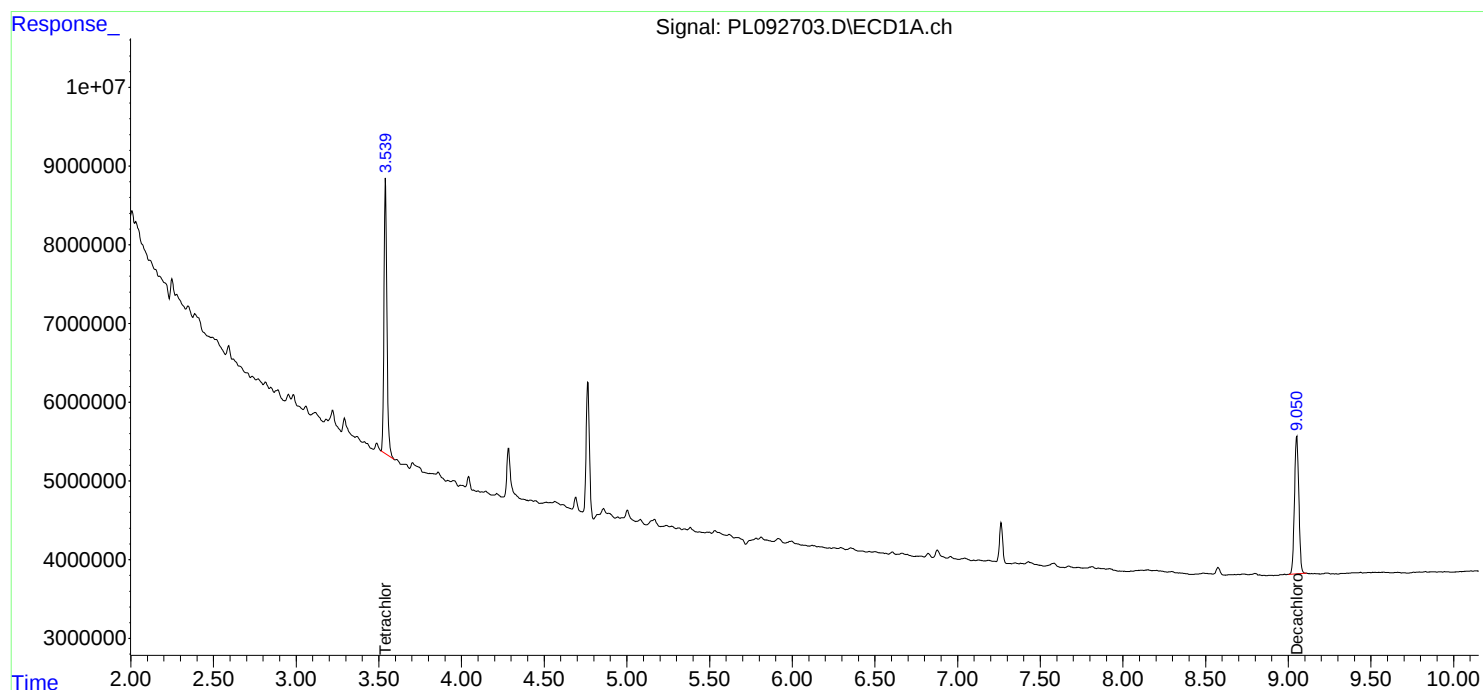

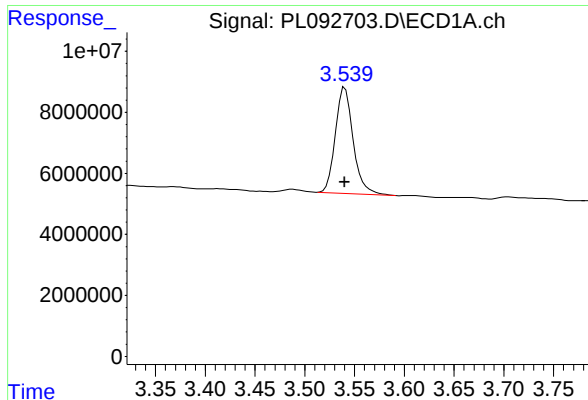


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 43357398
Conc: 17.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
WB-305-BOT-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/30/2024
Supervised By :Ankita Jodhani 11/04/2024

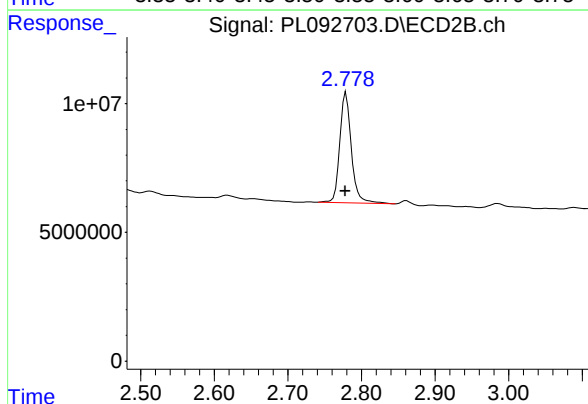


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.001 min
Response: 46969618
Conc: 17.26 ng/ml

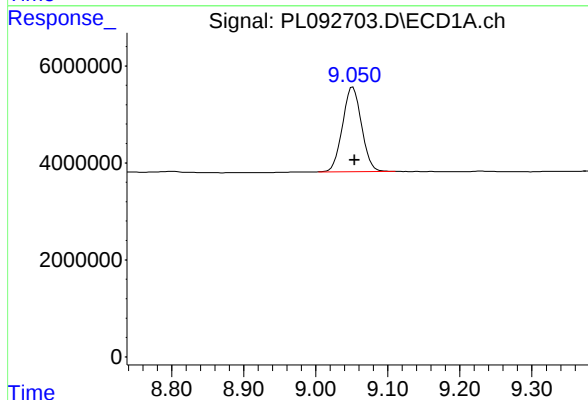

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.003 min
Response: 31815674
Conc: 16.53 ng/ml

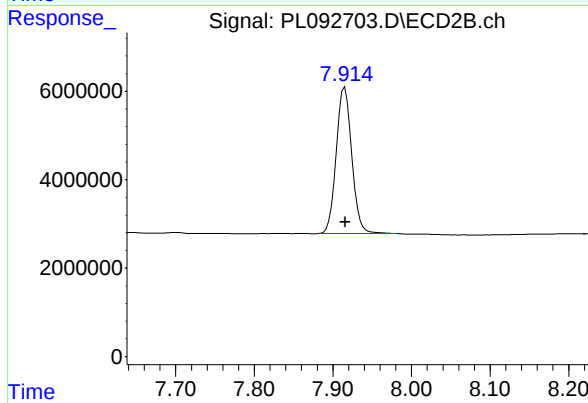

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 45553727
Conc: 16.69 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	10/26/24
Client Sample ID:	PB164393TB	SDG No.:	P4578
Lab Sample ID:	PB164393TB	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0 Decanted:
Sample Wt/Vol:	100 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	TCLP Pesticide
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092699.D	1	10/26/24 12:50	10/29/24 11:10	PB164445

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.0049	U	0.0049	0.050	ug/L
76-44-8	Heptachlor	0.0054	U	0.0054	0.050	ug/L
1024-57-3	Heptachlor epoxide	0.0090	U	0.0090	0.050	ug/L
72-20-8	Endrin	0.0043	U	0.0043	0.050	ug/L
72-43-5	Methoxychlor	0.011	U	0.011	0.050	ug/L
8001-35-2	Toxaphene	0.15	U	0.15	1.00	ug/L
57-74-9	Chlordane	0.082	U	0.082	0.50	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	19.7		30 (43) - 150 (140)	98%	SPK: 20
877-09-8	Tetrachloro-m-xylene	18.3		30 (77) - 150 (126)	92%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092699.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 11:10
 Operator : AR\AJ
 Sample : PB164393TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164393TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:10:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.779	44873551	47553325	18.314	17.475
28) SA Decachlor...	9.052	7.915	37864442	51503356	19.674	18.871

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 11:10
Operator : AR\AJ
Sample : PB164393TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB164393TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:10:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

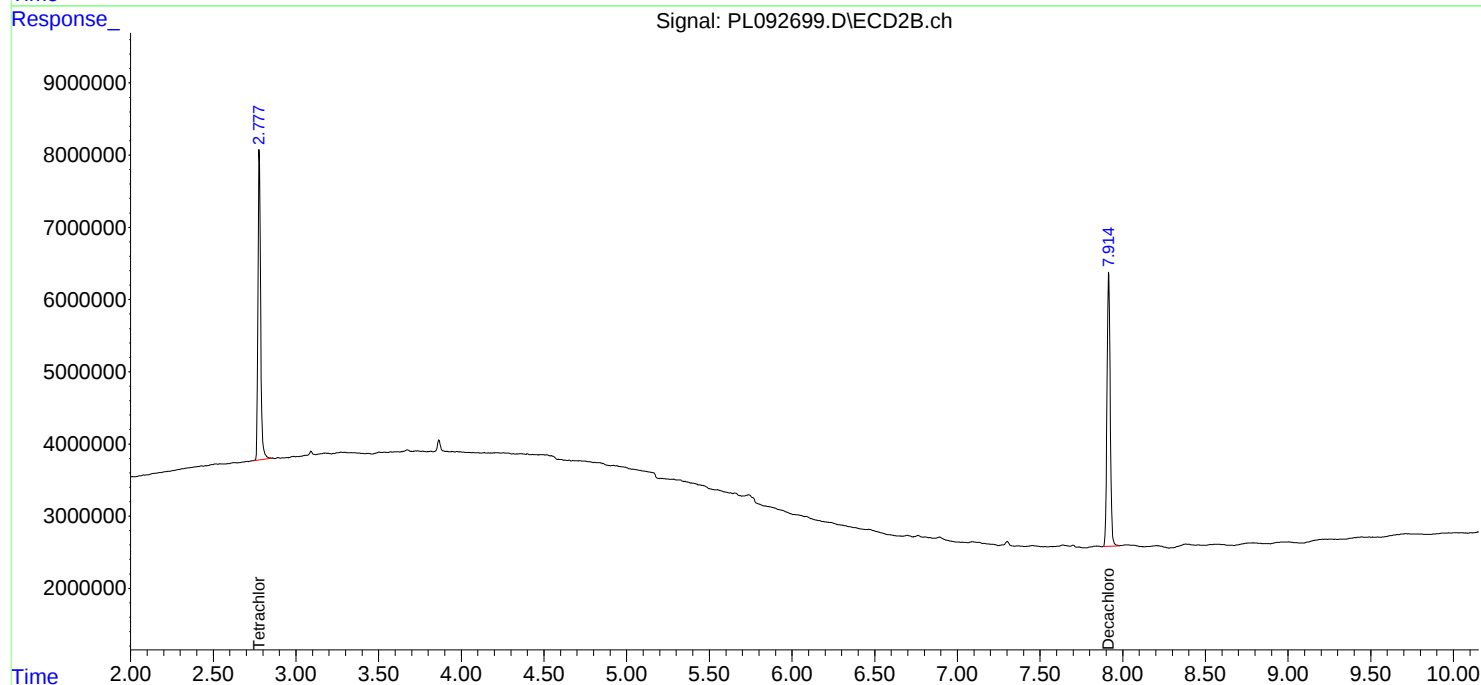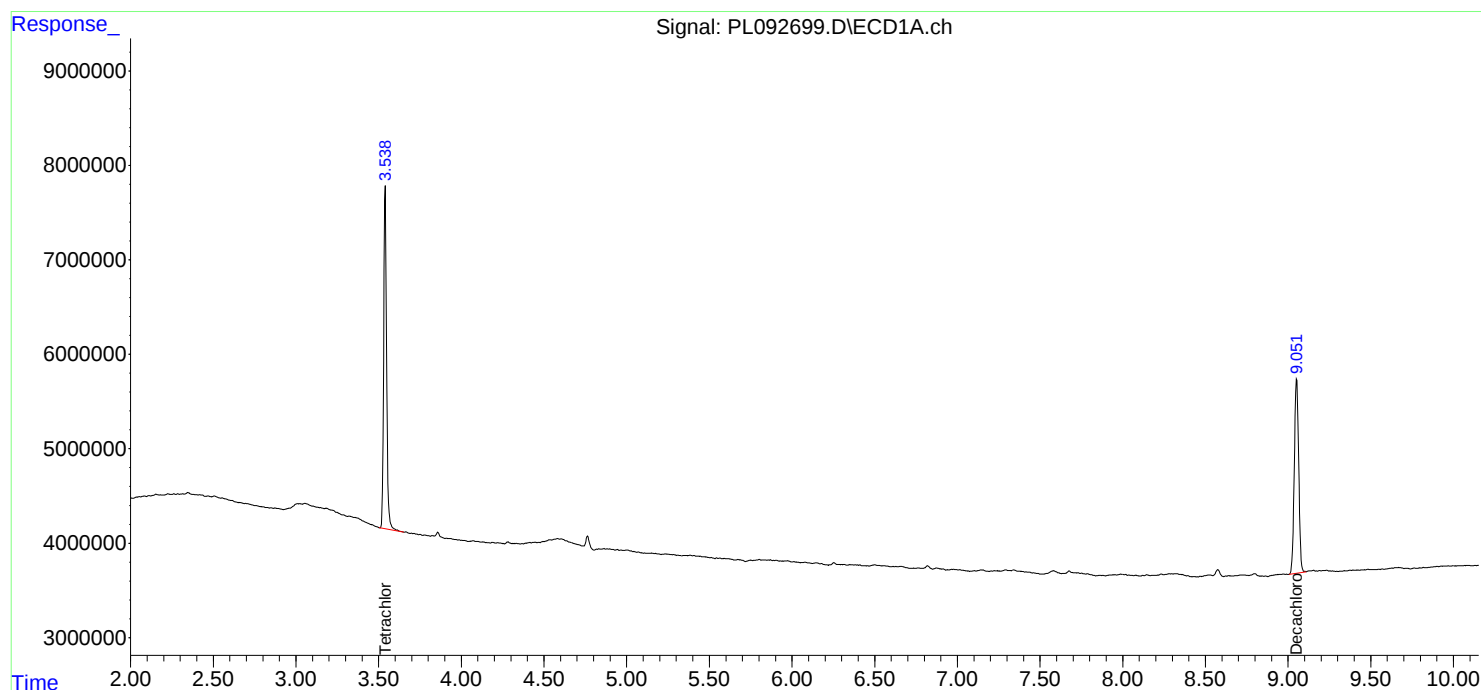


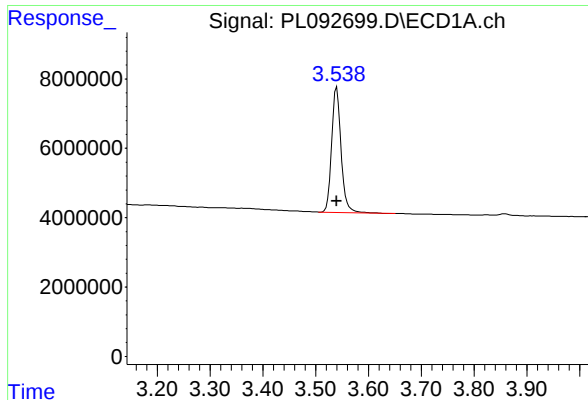

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 44873551
Conc: 18.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164393TB

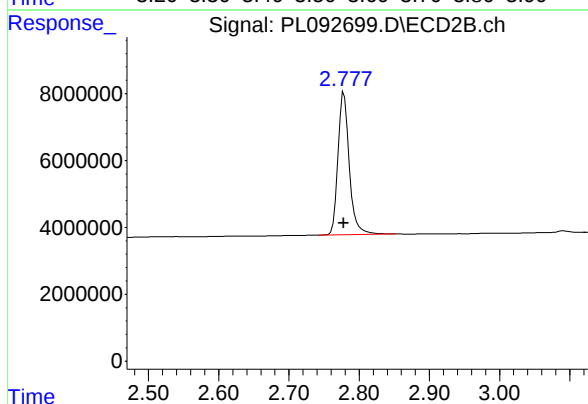


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.000 min
Response: 47553325
Conc: 17.48 ng/ml

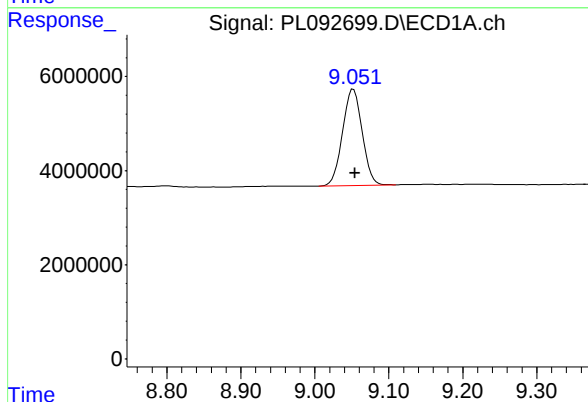

#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: -0.002 min
Response: 37864442
Conc: 19.67 ng/ml

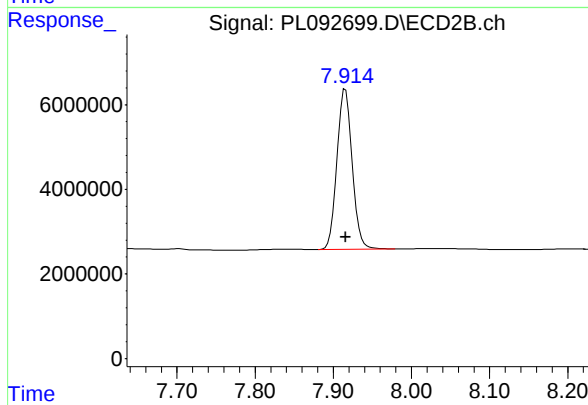

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 51503356
Conc: 18.87 ng/ml



CALIBRATION SUMMARY

GC Column: ZB-MR2 ID: 0.32 (mm)

[illegible]

RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>PORT06</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>P4578</u>	SAS No.:	<u>P4578</u>	SDG NO.:	<u>P4578</u>
Instrument ID:	<u>ECD_L</u>	Calibration Date(s):		<u>10/28/2024</u>	<u>10/28/2024</u>		
		Calibration Times:		<u>14:43</u>	<u>15:36</u>		

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 100 =	<u>PL092655.D</u>	RT 075 =	<u>PL092656.D</u>
	RT 050 =	PL092657.D	RT 025 =	PL092658.D
			RT 005 =	PL092659.D

[illegible]



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

Instrument ID: ECD_L

Calibration Date(s): 10/28/2024 10/28/2024

Calibration Times: 14:43 15:36

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		CF 100 =	<u>PL092655.D</u>	CF 075 =	<u>PL092656.D</u>		
CF 050 =	<u>PL092657.D</u>	CF 025 =	<u>PL092658.D</u>	CF 005 =	<u>PL092659.D</u>		
COMPOUND	CF 100	CF 075	CF 050	CF 025	CF 005	CF	% RSD
Decachlorobiphenyl	1738840000	1756630000	1819720000	1998760000	2308800000	1924550000	12
Endrin	2111540000	2103000000	2121260000	2324460000	2723040000	2276660000	12
gamma-BHC (Lindane)	3198960000	3133030000	3104430000	3278360000	3583040000	3259560000	6
Heptachlor	2817300000	2795570000	2829220000	3064000000	3509480000	3003110000	10
Heptachlor epoxide	2536240000	2521530000	2566410000	2821600000	3361270000	2761410000	13
Methoxychlor	1040530000	1050870000	1078280000	1189160000	1341160000	1140000000	11
Tetrachloro-m-xylene	2319350000	2304070000	2328420000	2512350000	2786990000	2450240000	8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

Instrument ID: ECD_L

Calibration Date(s): 10/28/2024 10/28/2024

Calibration Times: 14:43 15:36

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:		CF 100 =	<u>PL092655.D</u>	CF 075 =	<u>PL092656.D</u>		
CF 050 =		<u>PL092657.D</u>	CF 025 =	<u>PL092658.D</u>	CF 005 =	<u>PL092659.D</u>	
COMPOUND	CF 100	CF 075	CF 050	CF 025	CF 005	CF	% RSD
Decachlorobiphenyl	2606810000	2575500000	2605540000	2793460000	3064890000	2729240000	8
Endrin	2969490000	2878380000	2828080000	2876210000	2912860000	2893010000	2
gamma-BHC (Lindane)	4083950000	3934430000	3833920000	3828430000	3616530000	3859450000	4
Heptachlor	3876200000	3766580000	3709120000	3779090000	3738650000	3773930000	2
Heptachlor epoxide	3405420000	3318630000	3272090000	3352830000	3358060000	3341410000	1
Methoxychlor	1400820000	1385450000	1393920000	1470360000	1489590000	1428030000	3
Tetrachloro-m-xylene	2724750000	2661560000	2643180000	2728430000	2847900000	2721160000	3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

Instrument ID: ECD_L Date(s) Analyzed: 10/28/2024 10/28/2024

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Chlordane	500	1	4.70	4.60	4.80	106996000
		2	5.23	5.13	5.33	110397000
		3	5.94	5.84	6.04	372388000
		4	6.02	5.92	6.12	458405000
		5	6.87	6.77	6.97	92161100
Toxaphene	500	1	6.24	6.14	6.34	23962400
		2	6.44	6.34	6.54	13823600
		3	7.06	6.96	7.16	79159800
		4	7.15	7.05	7.25	59803700
		5	7.93	7.83	8.03	45329200



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

Instrument ID: ECD_L Date(s) Analyzed: 10/28/2024 10/28/2024

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Chlordane	500	1	3.78	3.68	3.88	105092000
		2	4.35	4.25	4.45	120641000
		3	4.98	4.88	5.08	361048000
		4	5.05	4.95	5.15	346821000
		5	5.94	5.84	6.04	124060000
Toxaphene	500	1	5.01	4.91	5.11	19952700
		2	5.33	5.23	5.43	19749600
		3	6.61	6.51	6.71	70222500
		4	6.73	6.63	6.83	98337700
		5	7.05	6.95	7.15	65479700

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 14:43
 Operator : AR\AJ
 Sample : PSTDICC100
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC100

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:08:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:06:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.778	231.9E6	272.5E6	99.805	101.520
28)	SA Decachlor...	9.054	7.915	173.9E6	260.7E6	97.727	100.024
Target Compounds							
2)	A alpha-BHC	3.996	3.281	335.7E6	428.2E6	101.915	103.738
3)	MA gamma-BHC...	4.328	3.611	319.9E6	408.4E6	101.500	103.158
4)	MA Heptachlor	4.917	3.950	281.7E6	387.6E6	99.789	102.203
5)	MB Aldrin	5.258	4.230	284.7E6	384.1E6	100.711	102.971
6)	B beta-BHC	4.525	3.910	134.3E6	162.5E6	99.068	101.057
7)	B delta-BHC	4.773	4.139	306.8E6	408.8E6	101.972	103.616
8)	B Heptachlo...	5.685	4.732	253.6E6	340.5E6	99.409	101.997
9)	A Endosulfan I	6.070	5.102	232.1E6	311.1E6	99.407	101.931
10)	B gamma-Chl...	5.940	4.982	249.7E6	347.0E6	100.095	102.605
11)	B alpha-Chl...	6.019	5.046	248.7E6	340.9E6	99.933	102.323
12)	B 4,4'-DDE	6.193	5.235	225.4E6	333.5E6	100.536	102.774
13)	MA Dieldrin	6.345	5.366	248.7E6	348.3E6	100.220	102.853
14)	MA Endrin	6.575	5.641	211.2E6	296.9E6	99.771	102.439
15)	B Endosulfa...	6.794	5.936	216.0E6	288.2E6	98.961	101.794
16)	A 4,4'-DDD	6.710	5.789	181.0E6	261.5E6	99.788	103.390
17)	MA 4,4'-DDT	7.024	6.039	194.9E6	279.7E6	100.211	102.948
18)	B Endrin al...	6.924	6.115	171.2E6	227.4E6	98.679	100.967
19)	B Endosulfa...	7.158	6.338	197.4E6	270.8E6	98.735	101.573
20)	A Methoxychlor	7.500	6.614	104.1E6	140.1E6	98.219	100.247
21)	B Endrin ke...	7.643	6.843	225.4E6	309.0E6	99.557	101.257
22)	Mirex	8.117	7.024	176.1E6	246.6E6	97.640	99.464



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 14:43
Operator : AR\AJ
Sample : PSTDICC100
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDICC100

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:08:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:06:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

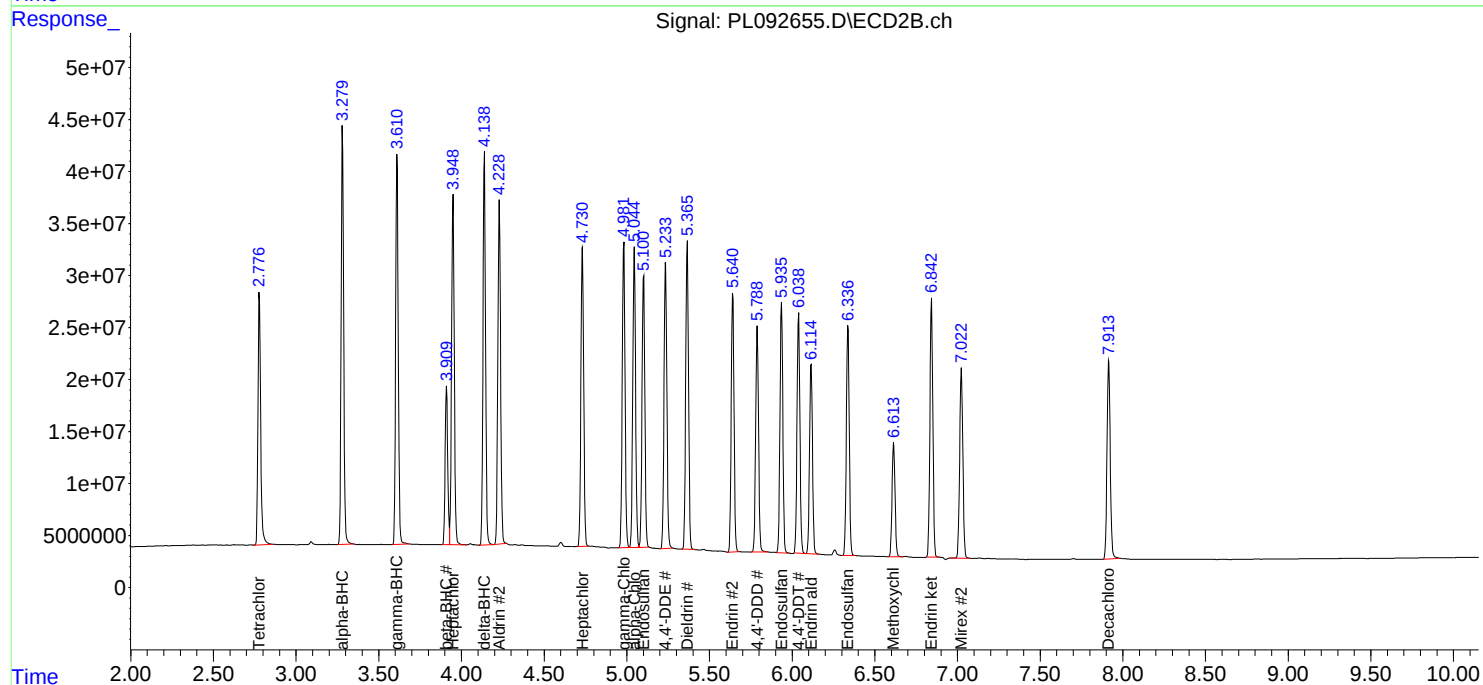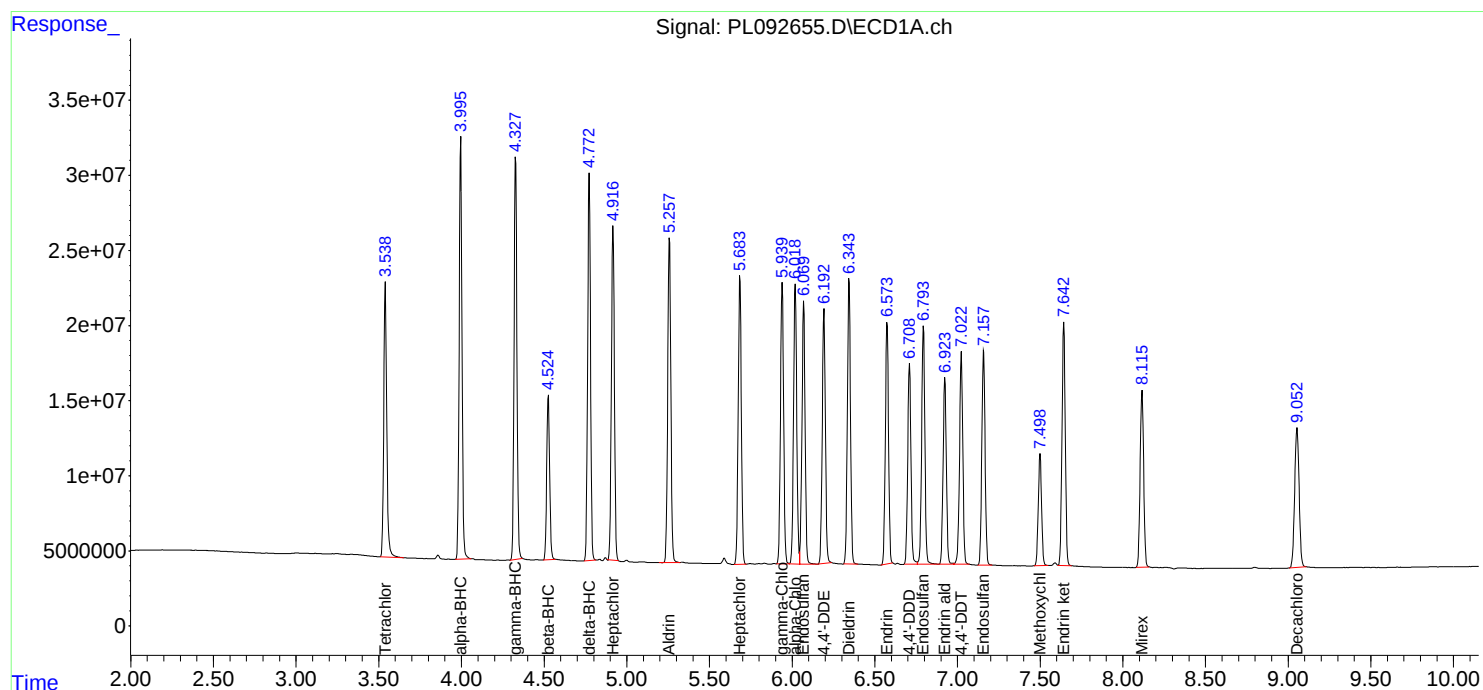

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 14:56
 Operator : AR\AJ
 Sample : PSTDICC075
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC075

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:11:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:10:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.778	172.8E6	199.6E6	74.573	74.581
28)	SA Decachlor...	9.054	7.916	131.7E6	193.2E6	74.361	74.409
Target Compounds							
2)	A alpha-BHC	3.996	3.281	245.4E6	306.7E6	74.672	74.526
3)	MA gamma-BHC...	4.328	3.611	235.0E6	295.1E6	74.703	74.690
4)	MA Heptachlor	4.917	3.950	209.7E6	282.5E6	74.508	74.655
5)	MB Aldrin	5.259	4.230	210.2E6	277.9E6	74.567	74.665
6)	B beta-BHC	4.526	3.911	100.4E6	119.6E6	74.376	74.585
7)	B delta-BHC	4.773	4.140	223.5E6	294.4E6	74.528	74.738
8)	B Heptachlo...	5.685	4.733	189.1E6	248.9E6	74.414	74.698
9)	A Endosulfan I	6.070	5.103	173.5E6	227.5E6	74.558	74.676
10)	B gamma-Chl...	5.941	4.982	185.8E6	251.7E6	74.671	74.608
11)	B alpha-Chl...	6.019	5.047	185.2E6	247.8E6	74.613	74.571
12)	B 4,4'-DDE	6.193	5.235	167.0E6	241.9E6	74.650	74.705
13)	MA Dieldrin	6.345	5.366	184.3E6	252.3E6	74.504	74.669
14)	MA Endrin	6.575	5.642	157.7E6	215.9E6	74.683	74.647
15)	B Endosulfa...	6.794	5.937	162.1E6	211.0E6	74.503	74.700
16)	A 4,4'-DDD	6.710	5.790	135.1E6	188.0E6	74.665	74.546
17)	MA 4,4'-DDT	7.024	6.040	145.0E6	203.5E6	74.705	74.920
18)	B Endrin al...	6.924	6.116	128.9E6	168.3E6	74.510	74.830
19)	B Endosulfa...	7.159	6.339	148.5E6	198.5E6	74.498	74.635
20)	A Methoxychlor	7.500	6.615	78815004	103.9E6	74.596	74.572
21)	B Endrin ke...	7.643	6.844	168.5E6	226.7E6	74.619	74.533
22)	Mirex	8.117	7.024	133.9E6	183.5E6	74.491	74.331



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 14:56
Operator : AR\AJ
Sample : PSTDICC075
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDICC075

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:11:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:10:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

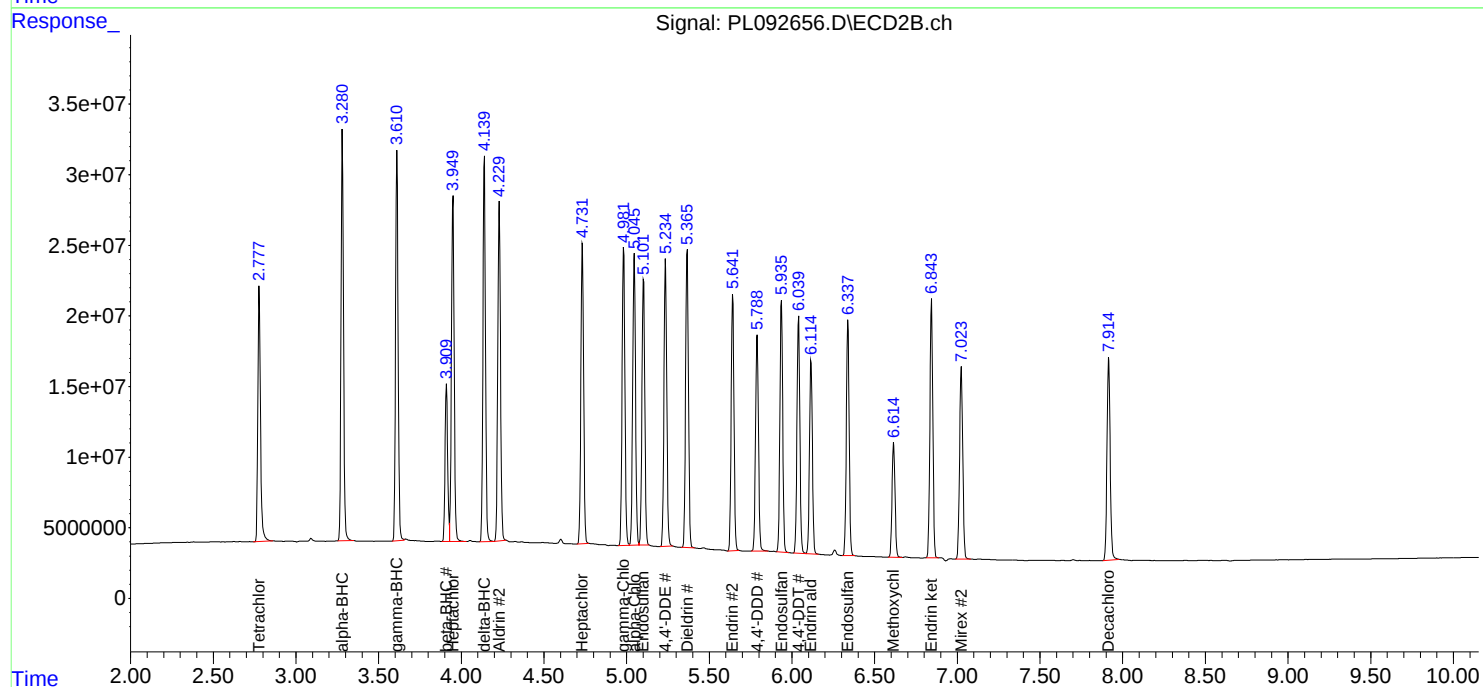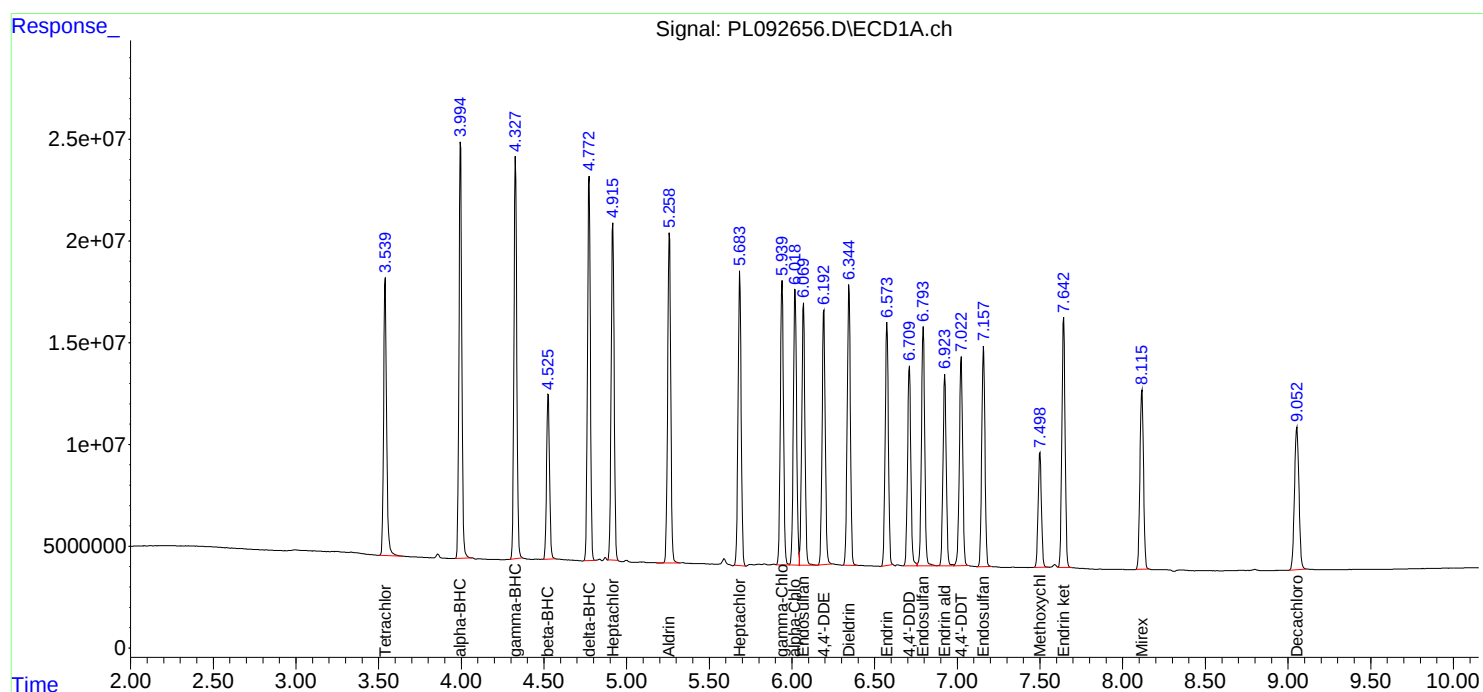

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 15:09
 Operator : AR\AJ
 Sample : PSTDICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:06:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:06:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.778	116.4E6	132.2E6	50.000	50.000
28)	SA Decachlor...	9.054	7.916	90985898	130.3E6	50.000	50.000
Target Compounds							
2)	A alpha-BHC	3.996	3.281	161.5E6	198.7E6	50.000	50.000
3)	MA gamma-BHC...	4.328	3.611	155.2E6	191.7E6	50.000	50.000
4)	MA Heptachlor	4.917	3.949	141.5E6	185.5E6	50.000	50.000
5)	MB Aldrin	5.258	4.229	140.4E6	181.0E6	50.000	50.000
6)	B beta-BHC	4.525	3.910	68426712	79558092	50.000	50.000
7)	B delta-BHC	4.772	4.139	147.5E6	190.1E6	50.000	50.000
8)	B Heptachlo...	5.684	4.732	128.3E6	163.6E6	50.000	50.000
9)	A Endosulfan I	6.070	5.102	117.4E6	149.7E6	50.000	50.000
10)	B gamma-Chl...	5.941	4.982	124.6E6	164.7E6	50.000	50.000
11)	B alpha-Chl...	6.019	5.045	124.5E6	162.7E6	50.000	50.000
12)	B 4,4'-DDE	6.193	5.235	111.5E6	157.7E6	50.000	50.000
13)	MA Dieldrin	6.345	5.366	123.8E6	164.5E6	50.000	50.000
14)	MA Endrin	6.574	5.641	106.1E6	141.4E6	50.000	50.000
15)	B Endosulfa...	6.794	5.936	110.3E6	139.0E6	50.000	50.000
16)	A 4,4'-DDD	6.710	5.789	90898841	122.2E6	50.000	50.000
17)	MA 4,4'-DDT	7.023	6.040	97035972	131.9E6	50.000	50.000
18)	B Endrin al...	6.924	6.115	87908093	111.5E6	50.000	50.000
19)	B Endosulfa...	7.158	6.338	101.2E6	131.2E6	50.000	50.000
20)	A Methoxychlor	7.499	6.615	53913903	69696231	50.000	50.000
21)	B Endrin ke...	7.643	6.843	113.7E6	150.7E6	50.000	50.000
22)	Mirex	8.116	7.024	92300183	124.6E6	50.000	50.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 15:09
Operator : AR\AJ
Sample : PSTDICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:06:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:06:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

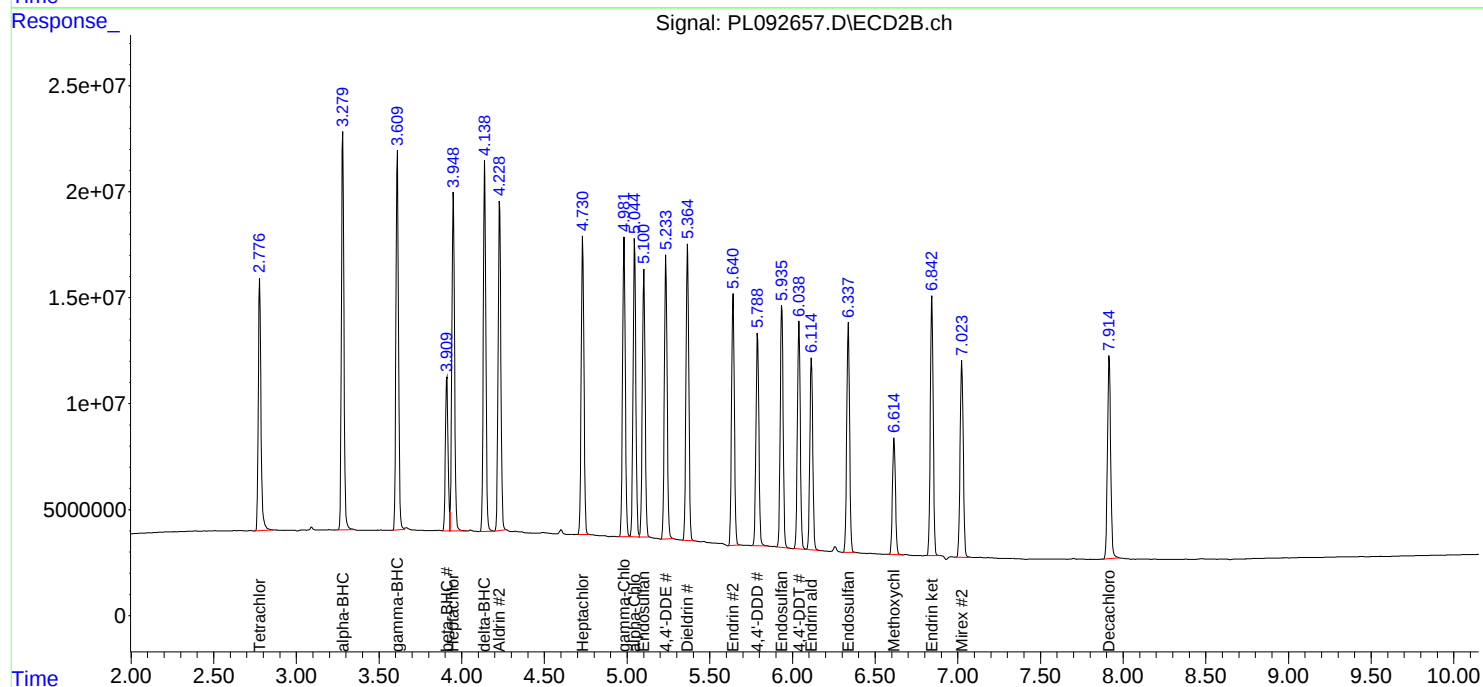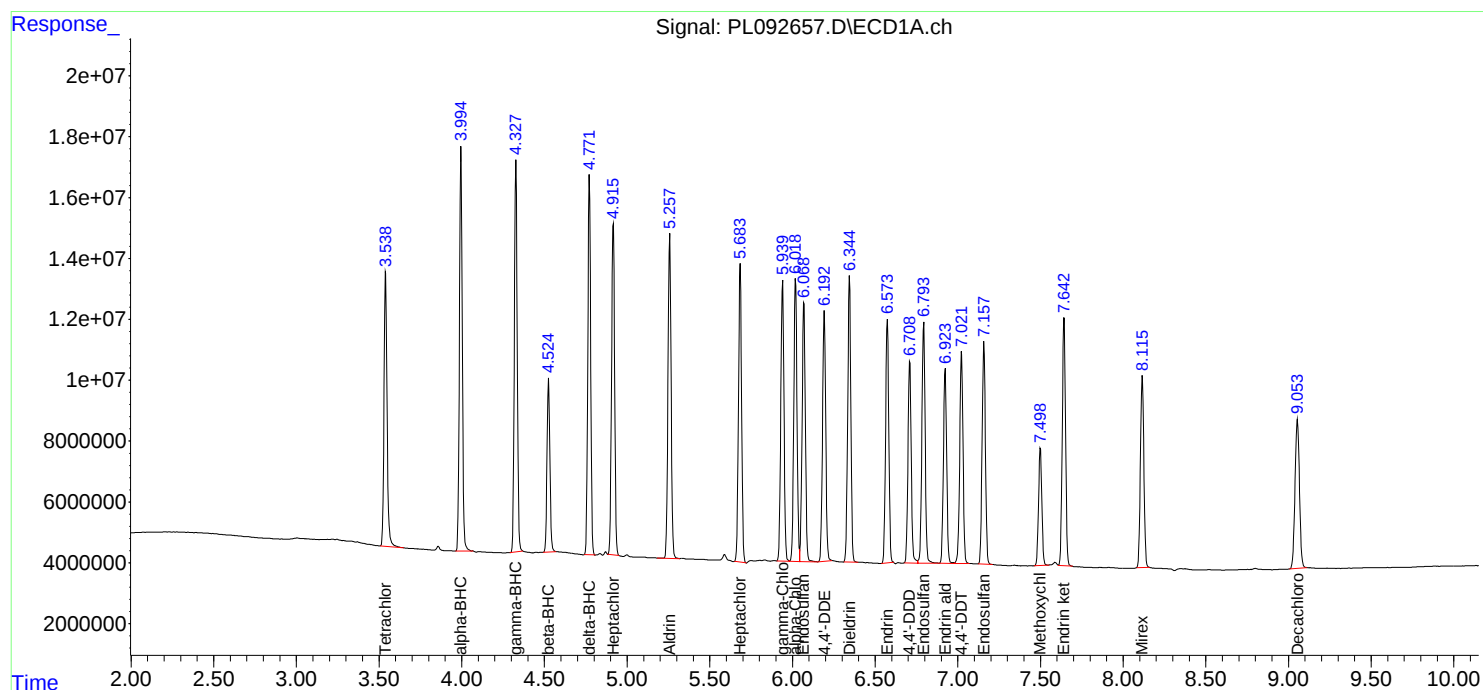

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 15:23
 Operator : AR\AJ
 Sample : PSTDICC025
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:13:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:10:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.778	62808688	68210857	26.546	25.362
28)	SA Decachlor...	9.054	7.916	49968947	69836578	27.328	26.400
Target Compounds							
2)	A alpha-BHC	3.996	3.281	84927238	98362013	25.627	24.168
3)	MA gamma-BHC...	4.328	3.611	81958950	95710712	25.784	24.415
4)	MA Heptachlor	4.917	3.950	76599935	94477178	26.629	24.976
5)	MB Aldrin	5.259	4.230	76180853	90483526	26.486	24.481
6)	B beta-BHC	4.526	3.911	37295050	41549746	26.915	25.675
7)	B delta-BHC	4.773	4.140	77991786	94555626	25.748	24.249
8)	B Heptachlo...	5.685	4.732	70540111	83820686	27.012	25.117
9)	A Endosulfan I	6.070	5.102	63654358	76808476	26.720	25.162
10)	B gamma-Chl...	5.941	4.982	67586796	83550406	26.583	24.826
11)	B alpha-Chl...	6.019	5.046	67542919	83232660	26.625	25.039
12)	B 4,4'-DDE	6.193	5.235	60061765	80248978	26.363	24.834
13)	MA Dieldrin	6.345	5.366	66985225	82586412	26.531	24.577
14)	MA Endrin	6.574	5.642	58111422	71905340	26.841	24.898
15)	B Endosulfa...	6.793	5.937	61248899	71530905	27.295	25.239
16)	A 4,4'-DDD	6.710	5.790	49194300	62230288	26.599	24.759
17)	MA 4,4'-DDT	7.023	6.040	52836397	66342279	26.630	24.568
18)	B Endrin al...	6.923	6.116	48897872	58336435	27.376	25.694
19)	B Endosulfa...	7.158	6.339	55996056	67808739	27.255	25.373
20)	A Methoxychlor	7.499	6.615	29728906	36759011	27.282	26.022
21)	B Endrin ke...	7.643	6.844	61777342	77430982	26.728	25.339
22)	Mirex	8.116	7.025	51864163	67137696	27.785	26.612



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 15:23
Operator : AR\AJ
Sample : PSTDICC025
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDICC025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:13:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:10:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

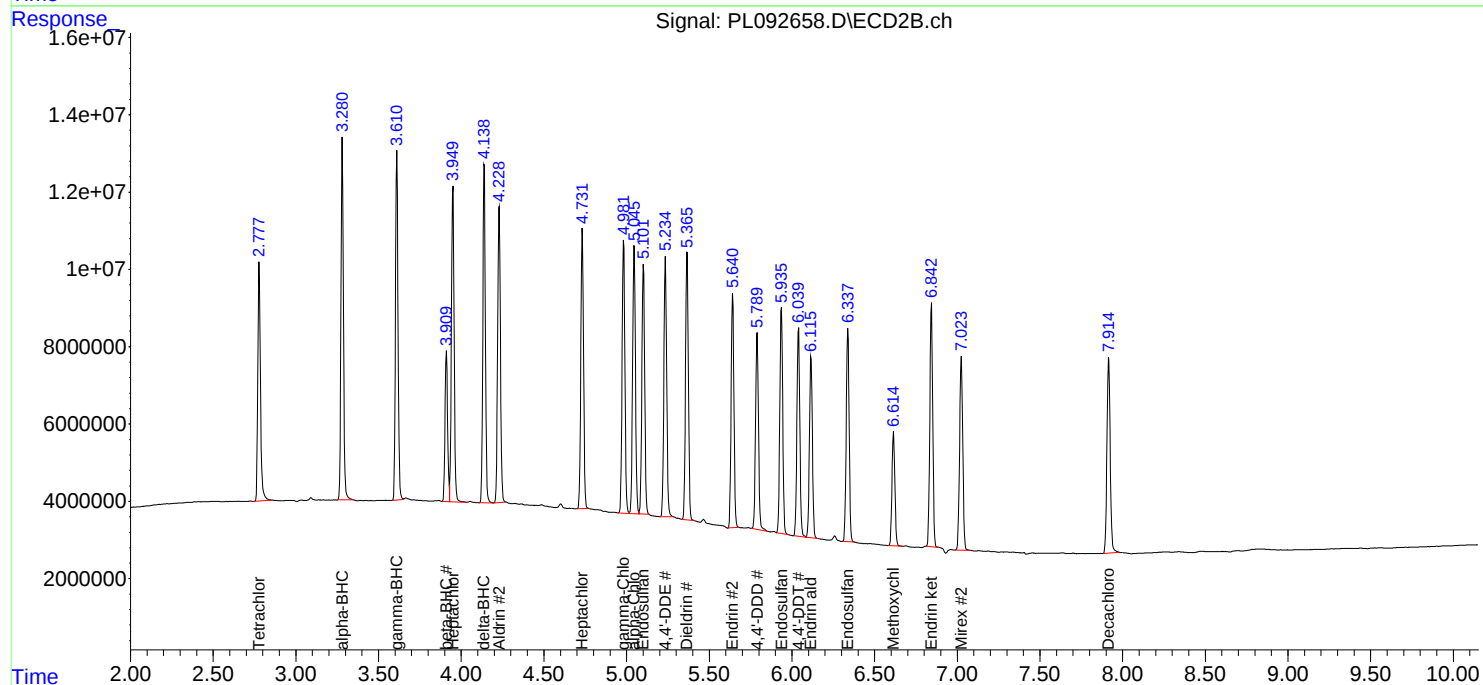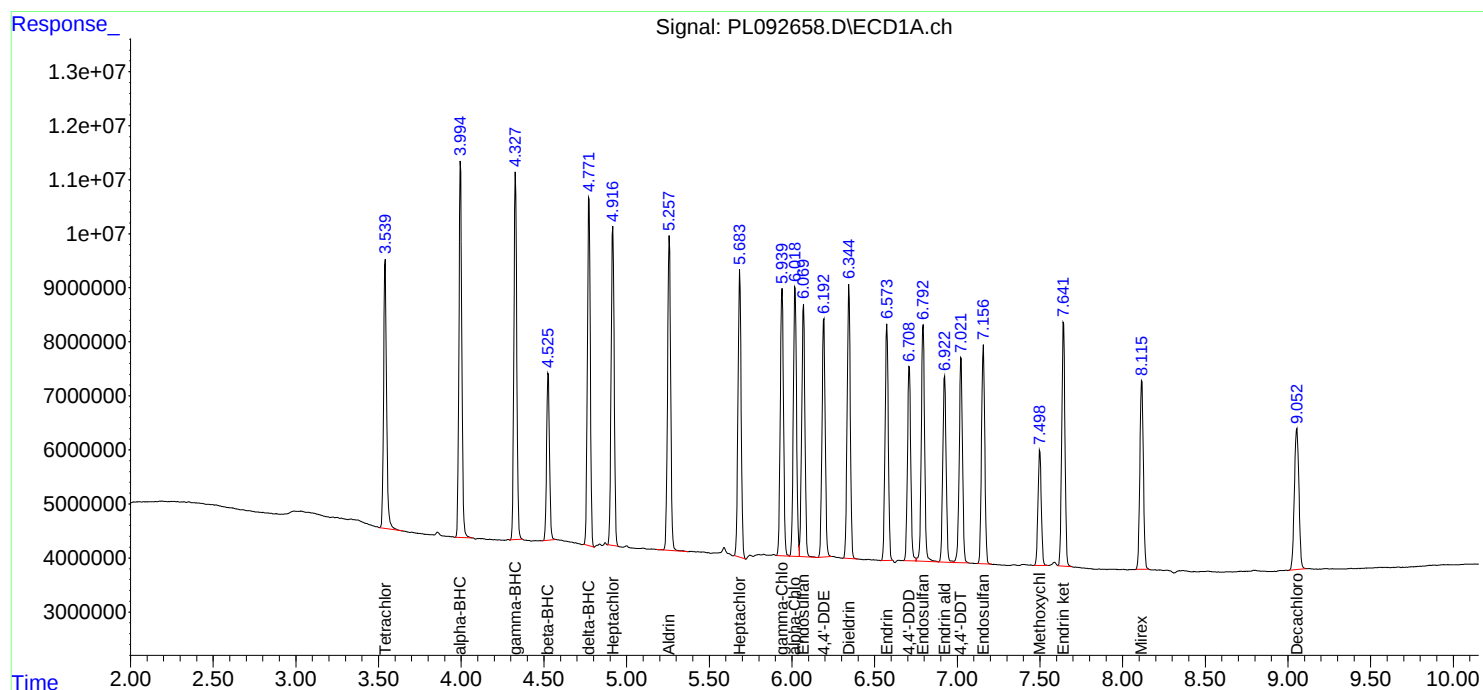

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 15:36
 Operator : AR\AJ
 Sample : PSTDICC005
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

PSTDICC005

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 10/29/2024

Supervised By :Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:16:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:10:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.778	13934946	14239511	5.687	5.233
28) SA Decachlor...	9.053	7.915	11544004	15324471	5.998	5.615
Target Compounds						
2) A alpha-BHC	3.995	3.280	18509728	18354234	5.458	4.600
3) MA gamma-BHC...	4.328	3.611	17915176	18082634	5.496	4.685
4) MA Heptachlor	4.916	3.950	17547418	18693239	5.843	4.953
5) MB Aldrin	5.258	4.229	17512022	17582981	5.834	4.804
6) B beta-BHC	4.526	3.910	8423294	8790546	5.827	5.340
7) B delta-BHC	4.771	4.139	17664985	18090728	5.611m	4.707
8) B Heptachlo...	5.682	4.732	16806367	16790300	6.074m	5.025
9) A Endosulfan I	6.069	5.102	14888105	15277635	5.952	5.004
10) B gamma-Chl...	5.940	4.982	15665588	16732339	5.888	4.977
11) B alpha-Chl...	6.019	5.046	15466528	16668126	5.841	5.011
12) B 4,4'-DDE	6.192	5.235	13664798	15911321	5.768	4.939
13) MA Dieldrin	6.344	5.366	15390264	16300991	5.840	4.880
14) MA Endrin	6.573	5.641	13615222	14564290	5.980	5.034
15) B Endosulfa...	6.793	5.936	14715849	14149758	6.173	4.994
16) A 4,4'-DDD	6.709	5.789	10998106	11982712	5.730	4.812
17) MA 4,4'-DDT	7.023	6.039	12061270	13048754	5.827	4.865
18) B Endrin al...	6.923	6.115	11226054	12274278	5.978	5.320
19) B Endosulfa...	7.157	6.338	13167738	13973088	6.067	5.181
20) A Methoxychlor	7.499	6.614	6705797	7447941	5.882	5.216
21) B Endrin ke...	7.643	6.843	14342863	15604260	5.920	5.085
22) Mirex	8.116	7.024	12209643	14769955	6.161	5.661

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 15:36
Operator : AR\AJ
Sample : PSTDICC005
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

PSTDICC005



Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 10/29/2024
Supervised By :Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:16:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:10:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

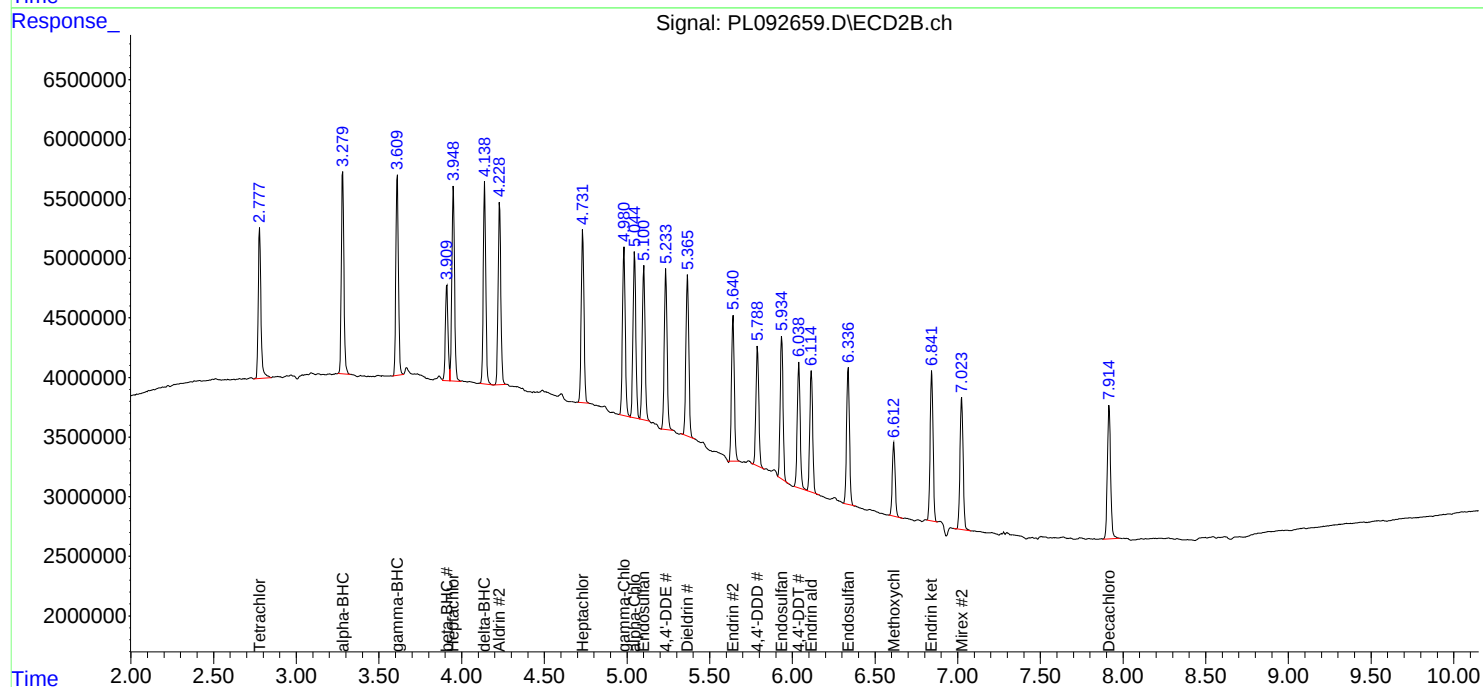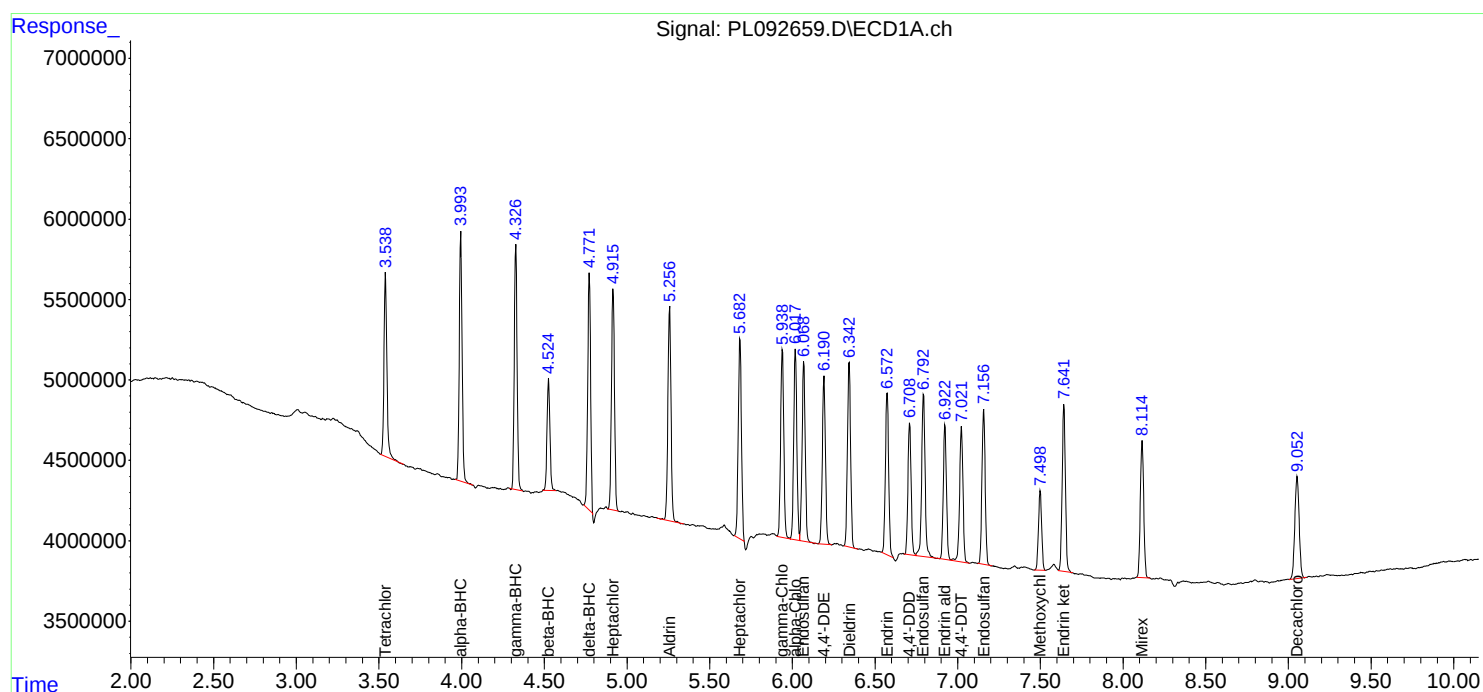

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 16:16
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 16:53:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 16:53:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.777	115.3E6	161.4E6	50.000	50.000
28)	SA Decachlor...	9.055	7.916	90689456	133.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.702	3.776	53498186	52546046	500.000	500.000
24)	Chlordane-2	5.231	4.352	55198384	60320369	500.000	500.000
25)	Chlordane-3	5.941	4.982	186.2E6	180.5E6	500.000	500.000
26)	Chlordane-4	6.023	5.045	229.2E6	173.4E6	500.000	500.000
27)	Chlordane-5	6.872	5.941	46080525	62029874	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 16:16
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 16:53:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 16:53:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

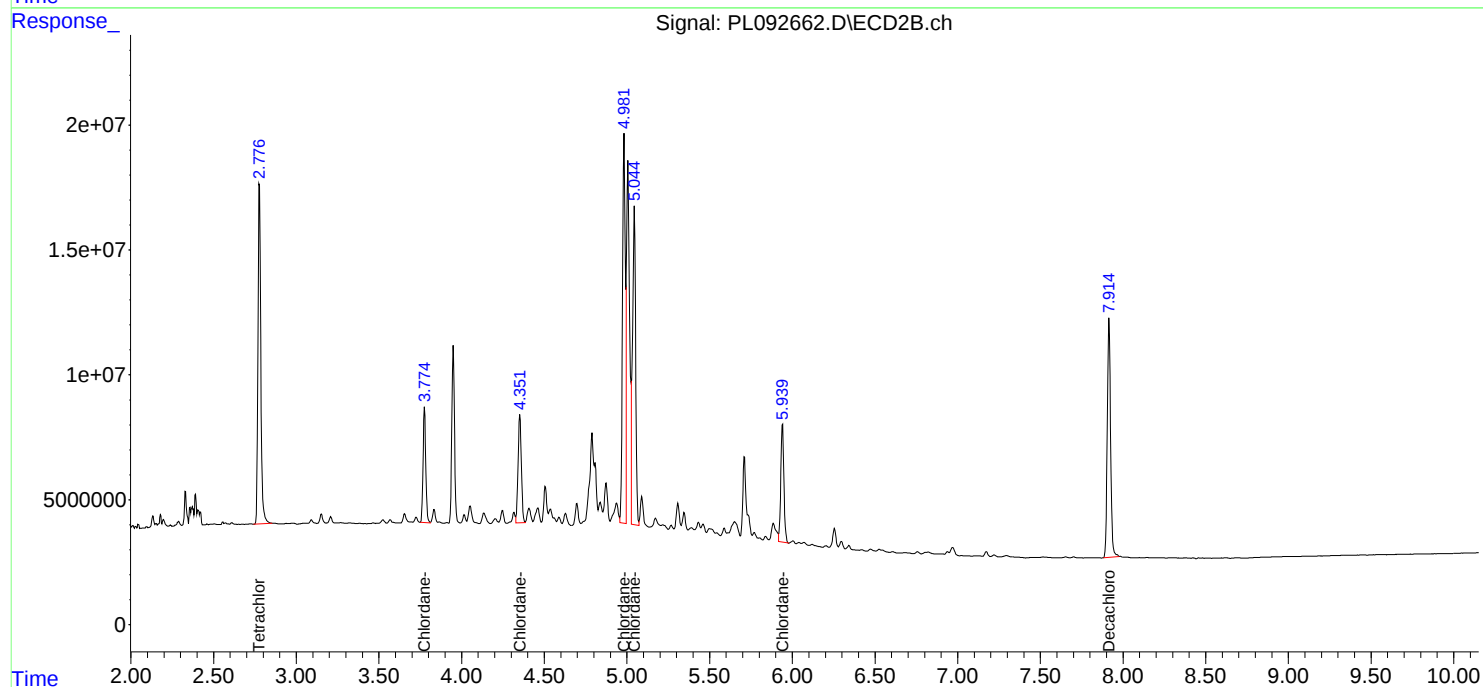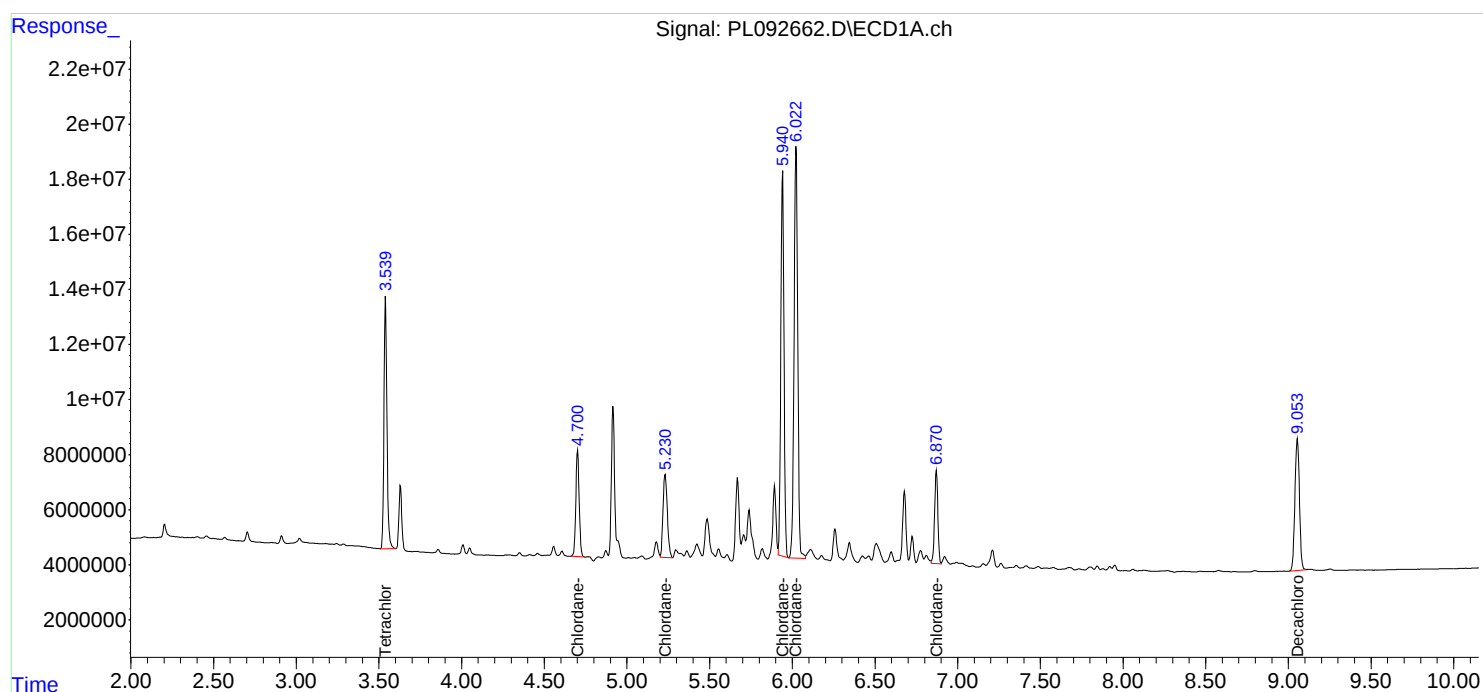

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 17:23
 Operator : AR\AJ
 Sample : PTOXICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PTOXICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:35:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\LTX102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:35:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticide 1 Signal #2 Phase: Rtx-CLPesticide 1
 Signal #1 Info : 30M x 0.32mm x0.3 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.778	120.2E6	137.2E6	50.000	50.000
7) SA Decachlor...	9.054	7.916	94872630	139.2E6	50.000	50.000
Target Compounds						
2) Toxaphene-1	6.237	5.007	11981208	9976373	500.000	500.000
3) Toxaphene-2	6.441	5.332	6911814	9874812	500.000	500.000
4) Toxaphene-3	7.058	6.605	39579915	35111261	500.000	500.000
5) Toxaphene-4	7.149	6.733	29901849	49168858	500.000	500.000
6) Toxaphene-5	7.934	7.045	22664593	32739853	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 17:23
Operator : AR\AJ
Sample : PTOXICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PTOXICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:35:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\LTX102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:35:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticide 1 Signal #2 Phase: Rtx-CLPesticide 1
Signal #1 Info : 30M x 0.32mm x 0.3 Signal #2 Info : 30M x 0.32mm x 0.25µm

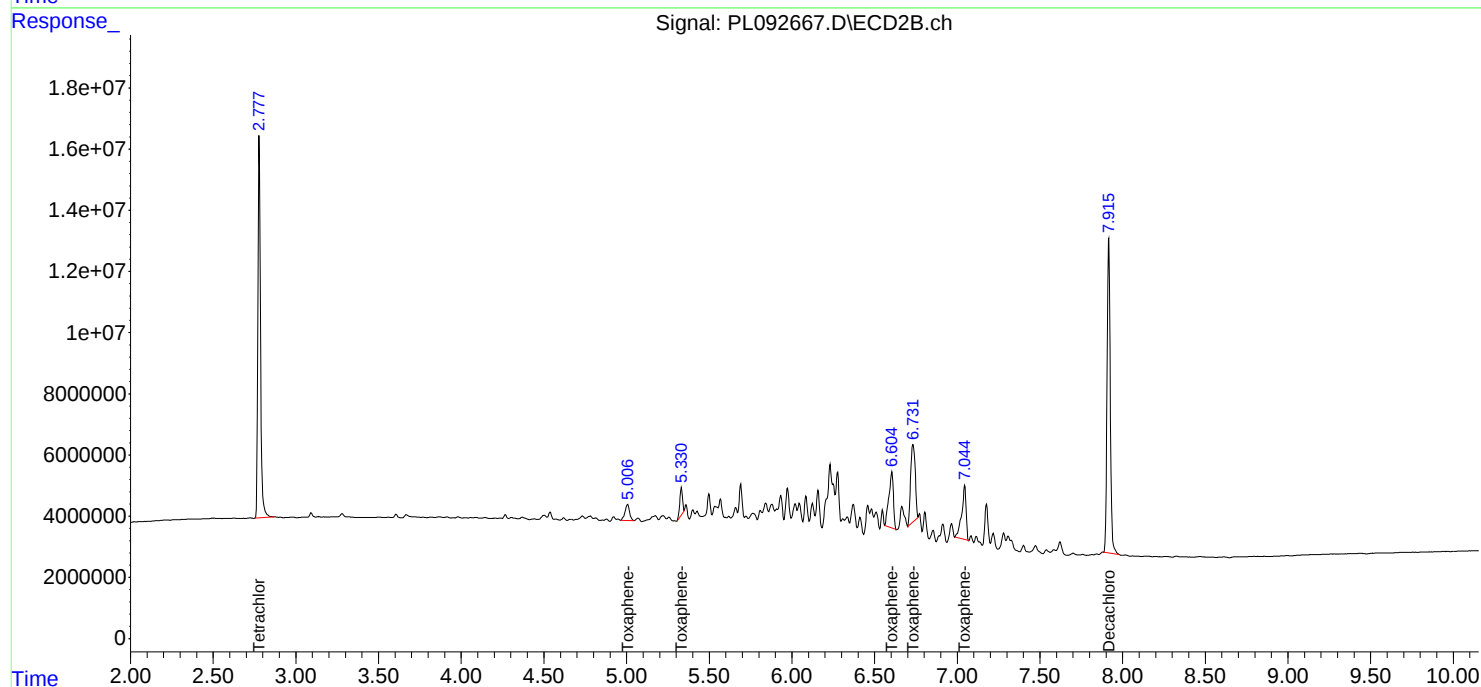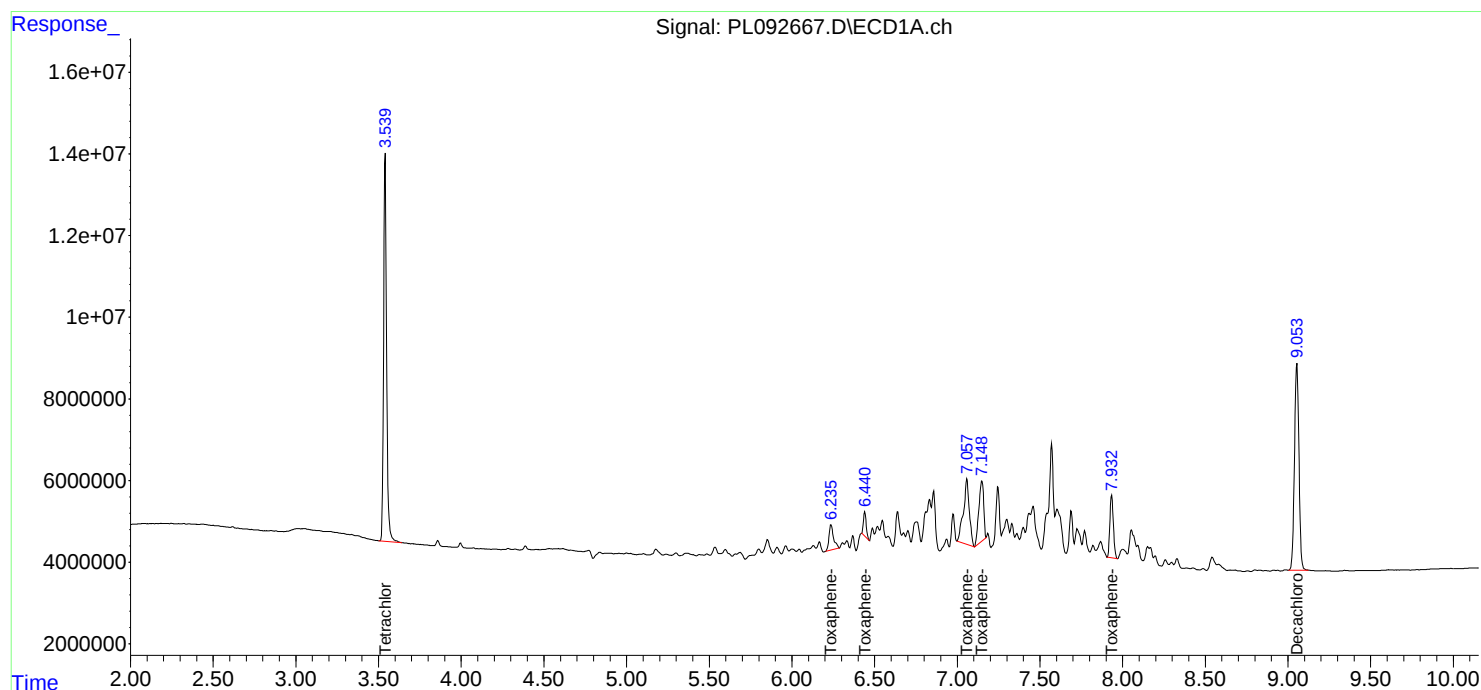

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 18:03
 Operator : AR\AJ
 Sample : PSTDICV050
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL102824

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 18:20:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:19:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.778	119.9E6	136.6E6	48.932	50.204
28)	SA Decachlor...	9.054	7.916	94182239	139.9E6	48.937	51.259
Target Compounds							
2)	A alpha-BHC	3.996	3.281	167.5E6	204.0E6	49.379	51.127
3)	MA gamma-BHC...	4.328	3.611	160.1E6	197.4E6	49.125	51.136
4)	MA Heptachlor	4.916	3.950	147.0E6	192.1E6	48.942	50.906
5)	MB Aldrin	5.258	4.230	145.8E6	187.4E6	48.580	51.194
6)	B beta-BHC	4.526	3.911	70600682	82244973	48.843	49.959
7)	B delta-BHC	4.773	4.140	153.4E6	196.7E6	49.025	51.190
8)	B Heptachlo...	5.684	4.732	133.1E6	169.7E6	48.213	50.772
9)	A Endosulfan I	6.069	5.102	121.8E6	154.2E6	48.702	50.518
10)	B gamma-Chl...	5.941	4.982	129.8E6	169.3E6	48.769	50.359
11)	B alpha-Chl...	6.019	5.046	129.4E6	167.6E6	48.847	50.380
12)	B 4,4'-DDE	6.193	5.235	116.5E6	164.4E6	49.166	51.019
13)	MA Dieldrin	6.345	5.366	129.0E6	171.0E6	48.947	51.185
14)	MA Endrin	6.575	5.642	110.2E6	147.7E6	48.393	51.063
15)	B Endosulfa...	6.794	5.937	115.4E6	145.0E6	48.417	51.175
16)	A 4,4'-DDD	6.710	5.790	95447383	127.7E6	49.724	51.292
17)	MA 4,4'-DDT	7.024	6.040	102.8E6	137.5E6	49.676	51.253
18)	B Endrin al...	6.924	6.116	91870810	116.2E6	48.920	50.348
19)	B Endosulfa...	7.159	6.339	106.0E6	136.5E6	48.859	50.601
20)	A Methoxychlor	7.500	6.615	57010538	73335025	50.009	51.354
21)	B Endrin ke...	7.644	6.844	118.9E6	157.6E6	49.074	51.358
22)	Mirex	8.117	7.025	96541027	131.1E6	48.716	50.260



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 18:03
Operator : AR\AJ
Sample : PSTDICV050
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL102824

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 18:20:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:19:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

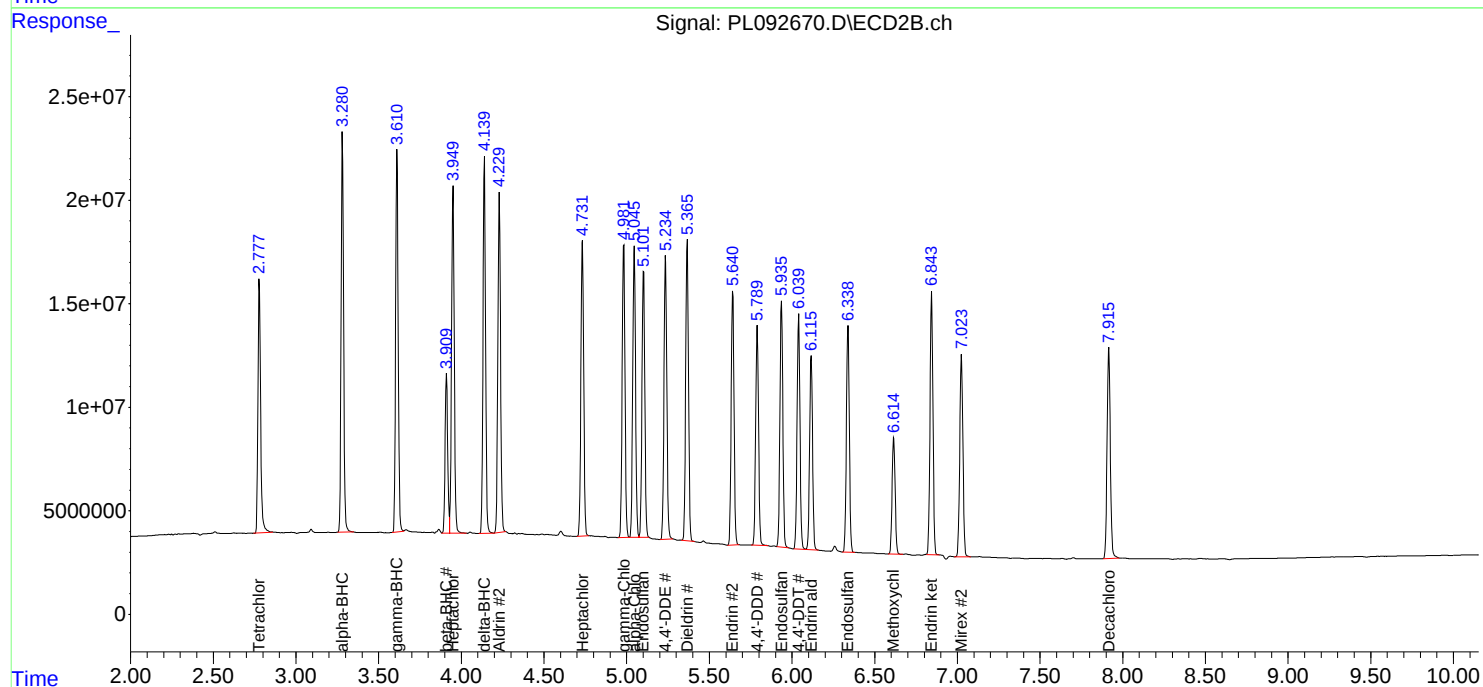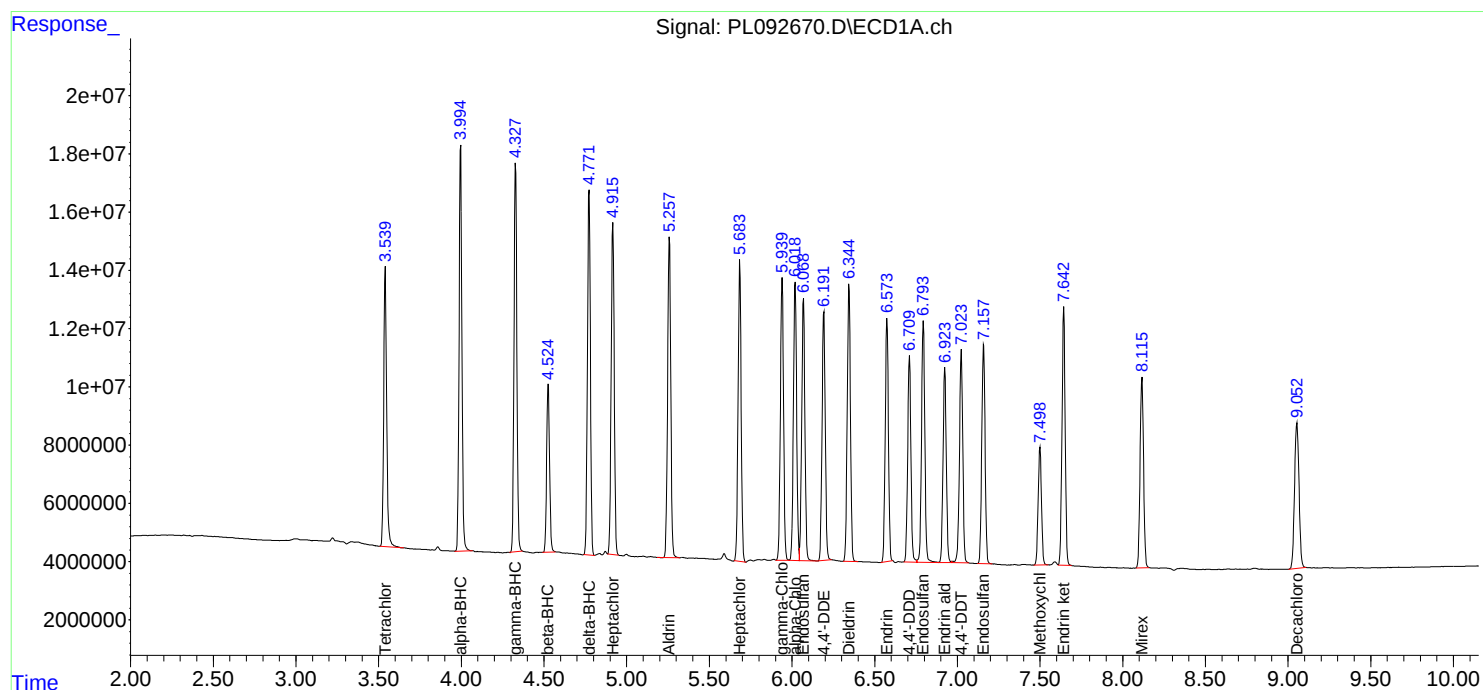

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 18:30
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL102824CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 18:55:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:55:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.777	116.2E6	162.6E6	48.370	49.862
28) SA Decachlor...	9.053	7.915	91212958	135.8E6	48.151	49.359
Target Compounds						
23) Chlordane-1	4.701	3.775	53586597	53029458	487.196	499.551
24) Chlordane-2	5.231	4.352	54950332	60704270	479.439	490.132
25) Chlordane-3	5.941	4.982	186.4E6	180.0E6	477.568	496.319
26) Chlordane-4	6.022	5.045	229.4E6	173.9E6	479.933	497.043
27) Chlordane-5	6.872	5.940	46544927	61748302	491.706	486.943



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 18:30
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL102824CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 18:55:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:55:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

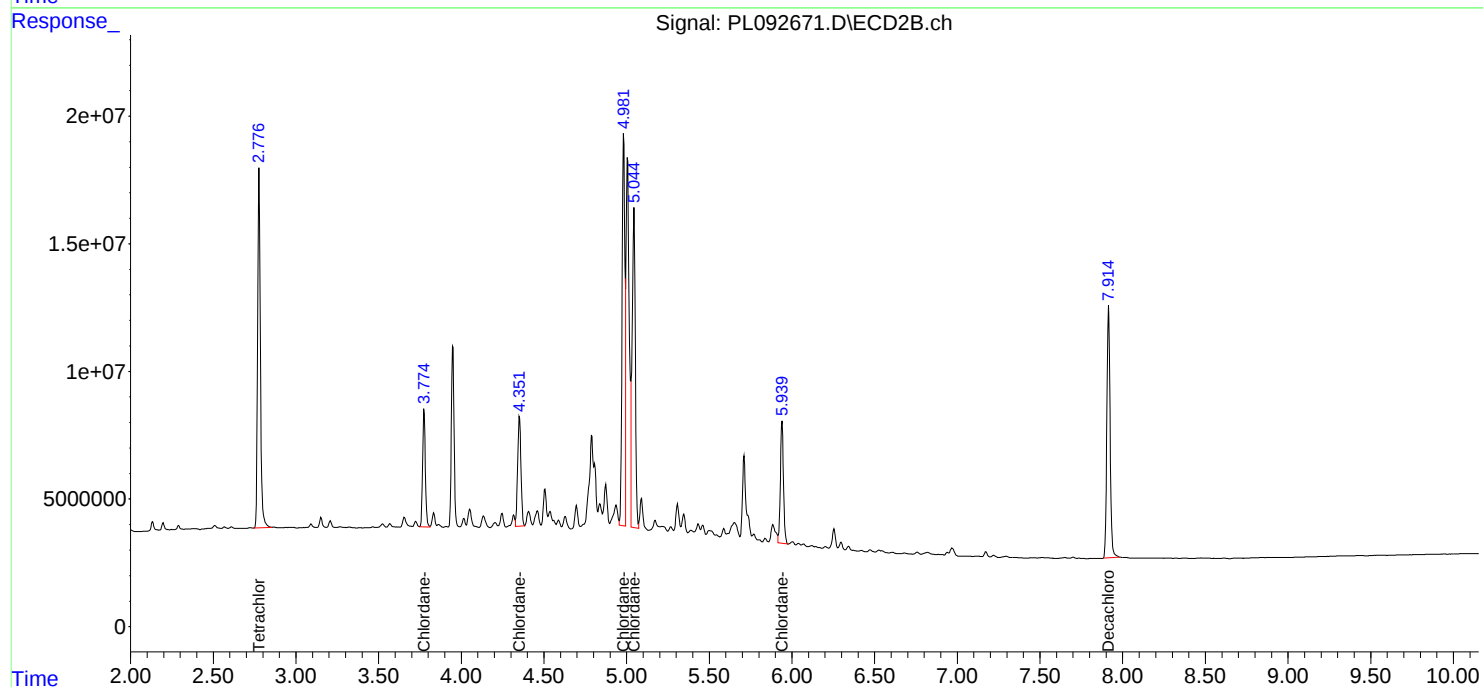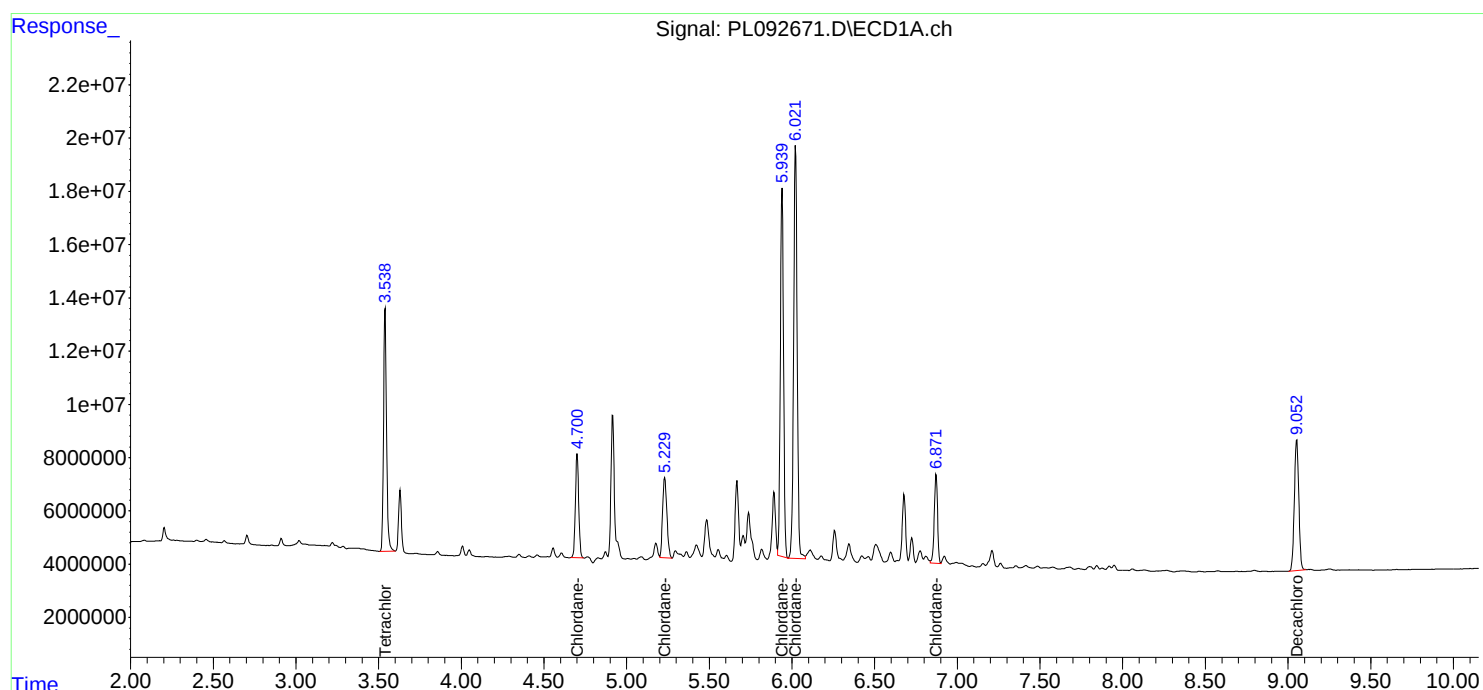

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 18:57
 Operator : AR\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL102824TOX

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 19:11:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\LTX102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:04:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticide 1 Signal #2 Phase: Rtx-CLPesticide 1
 Signal #1 Info : 30M x 0.32mm x0.3 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.778	120.8E6	137.1E6	50.385	51.035
7) SA Decachlor...	9.053	7.916	95483844	139.1E6	50.356	50.519
Target Compounds						
2) Toxaphene-1	6.237	5.006	12257412	10058947	555.039	528.973
3) Toxaphene-2	6.441	5.331	6863785	9788249	506.186	497.458
4) Toxaphene-3	7.058	6.604	39909041	34565997	513.663	508.031
5) Toxaphene-4	7.149	6.732	29767251	48553437	501.141	526.978
6) Toxaphene-5	7.933	7.046	22590334	32781409	503.299	499.967



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 18:57
Operator : AR\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL102824TOX

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 19:11:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\LTX102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:04:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticide 1 Signal #2 Phase: Rtx-CLPesticide 1
Signal #1 Info : 30M x 0.32mm x 0.3 Signal #2 Info : 30M x 0.32mm x 0.25µm

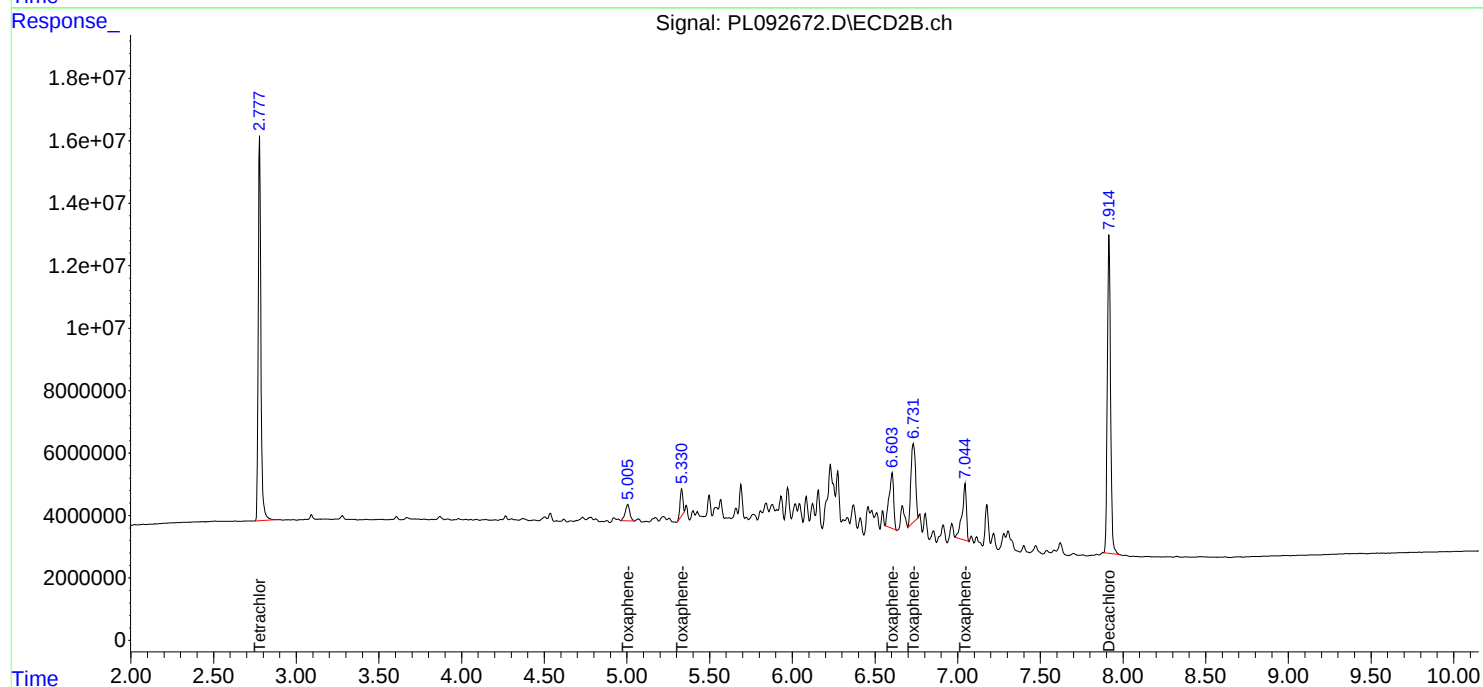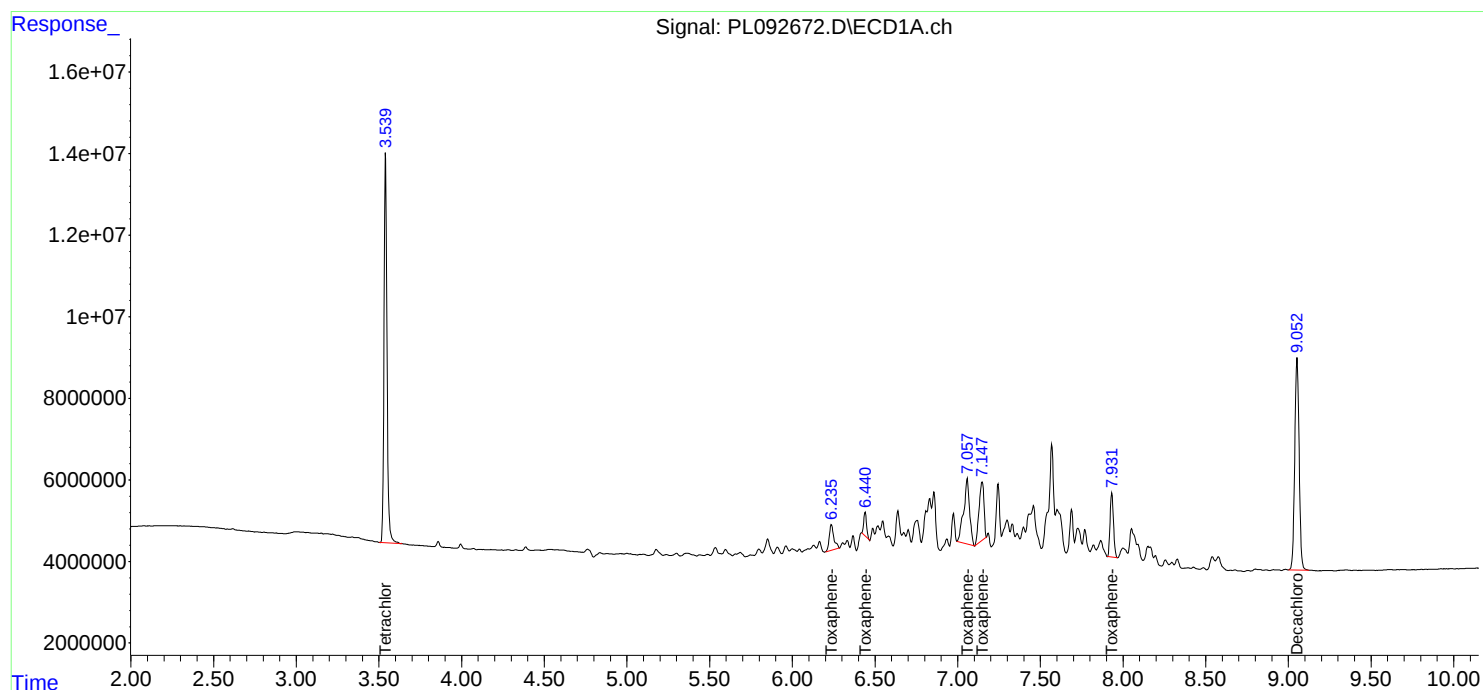



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

Continuing Calib Date: 10/29/2024 Initial Calibration Date(s): 10/28/2024 10/28/2024

Continuing Calib Time: 10:15 Initial Calibration Time(s): 14:43 15:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Decachlorobiphenyl	9.05	9.05	8.95	9.15	0.00
Tetrachloro-m-xylene	3.54	3.54	3.44	3.64	0.00
gamma-BHC (Lindane)	4.33	4.33	4.23	4.43	0.00
Heptachlor	4.92	4.92	4.82	5.02	0.00
Heptachlor epoxide	5.68	5.68	5.58	5.78	0.00
Endrin	6.58	6.57	6.47	6.67	0.00
Methoxychlor	7.50	7.50	7.40	7.60	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

Continuing Calib Date: 10/29/2024 Initial Calibration Date(s): 10/28/2024 10/28/2024

Continuing Calib Time: 10:15 Initial Calibration Time(s): 14:43 15:36

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW		DIFF RT
			FROM	TO	
Decachlorobiphenyl	7.92	7.92	7.82	8.02	0.01
Tetrachloro-m-xylene	2.78	2.78	2.68	2.88	0.00
gamma-BHC (Lindane)	3.61	3.61	3.51	3.71	0.00
Heptachlor	3.95	3.95	3.85	4.05	0.00
Heptachlor epoxide	4.73	4.73	4.63	4.83	0.00
Endrin	5.64	5.64	5.54	5.74	0.00
Methoxychlor	6.61	6.62	6.52	6.72	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY
Contract: PORT06
Lab Code: CHEM **Case No.:** P4578 **SAS No.:** P4578 **SDG NO.:** P4578
GC Column: ZB-MR2 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 10/28/2024 10/28/2024
Client Sample No.: CCAL01 **Date Analyzed:** 10/29/2024
Lab Sample No.: PSTDCCC050 **Data File :** PL092695.D **Time Analyzed:** 10:15

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Decachlorobiphenyl	9.053	8.954	9.154	49.010	50.000	-2.0
Endrin	6.575	6.474	6.674	47.250	50.000	-5.5
gamma-BHC (Lindane)	4.328	4.228	4.428	49.670	50.000	-0.7
Heptachlor	4.916	4.817	5.017	48.700	50.000	-2.6
Heptachlor epoxide	5.684	5.584	5.784	50.730	50.000	1.5
Methoxychlor	7.498	7.399	7.599	48.570	50.000	-2.9
Tetrachloro-m-xylene	3.540	3.440	3.640	49.870	50.000	-0.3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 10/28/2024 10/28/2024

Client Sample No.: CCAL01 Date Analyzed: 10/29/2024

Lab Sample No.: PSTDCCC050 Data File : PL092695.D Time Analyzed: 10:15

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Decachlorobiphenyl	7.915	7.816	8.016	51.500	50.000	3.0
Endrin	5.641	5.541	5.741	51.690	50.000	3.4
gamma-BHC (Lindane)	3.611	3.511	3.711	51.790	50.000	3.6
Heptachlor	3.950	3.849	4.049	50.790	50.000	1.6
Heptachlor epoxide	4.732	4.632	4.832	51.090	50.000	2.2
Methoxychlor	6.614	6.515	6.715	49.430	50.000	-1.1
Tetrachloro-m-xylene	2.779	2.678	2.878	50.880	50.000	1.8

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 10:15
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 12:30:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.779	122.2E6	138.5E6	49.867	50.880
28)	SA Decachlor...	9.053	7.915	94316934	140.6E6	49.007	51.502
Target Compounds							
2)	A alpha-BHC	3.996	3.281	169.9E6	206.4E6	50.093	51.736
3)	MA gamma-BHC...	4.328	3.611	161.9E6	199.9E6	49.670	51.789
4)	MA Heptachlor	4.916	3.950	146.2E6	191.7E6	48.696	50.785
5)	MB Aldrin	5.258	4.229	145.8E6	188.4E6	48.562	51.486
6)	B beta-BHC	4.526	3.911	70587805	83164682	48.834	50.518
7)	B delta-BHC	4.772	4.139	154.8E6	199.1E6	49.465	51.819
8)	B Heptachlo...	5.684	4.732	140.1E6	170.7E6	50.727	51.093
9)	A Endosulfan I	6.069	5.102	121.8E6	153.8E6	48.676	50.373
10)	B gamma-Chl...	5.940	4.982	128.8E6	170.9E6	48.413	50.834
11)	B alpha-Chl...	6.019	5.045	128.9E6	168.4E6	48.672	50.620
12)	B 4,4'-DDE	6.192	5.234	115.5E6	166.8E6	48.766	51.760
13)	MA Dieldrin	6.345	5.366	127.8E6	172.0E6	48.481	51.477
14)	MA Endrin	6.575	5.641	107.6E6	149.5E6	47.249	51.690
15)	B Endosulfa...	6.794	5.936	113.1E6	147.3E6	47.428	51.976
16)	A 4,4'-DDD	6.710	5.789	96577737	131.4E6	50.313	52.768
17)	MA 4,4'-DDT	7.023	6.039	99801551	133.9E6	48.219	49.916
18)	B Endrin al...	6.924	6.115	90822683	116.9E6	48.362	50.678
19)	B Endosulfa...	7.158	6.338	105.0E6	137.6E6	48.392	51.017
20)	A Methoxychlor	7.498	6.614	55366658	70584471	48.567	49.428
21)	B Endrin ke...	7.643	6.843	119.3E6	157.9E6	49.234	51.468
22)	Mirex	8.116	7.024	95870127	131.0E6	48.378	50.217



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 10:15
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 12:30:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

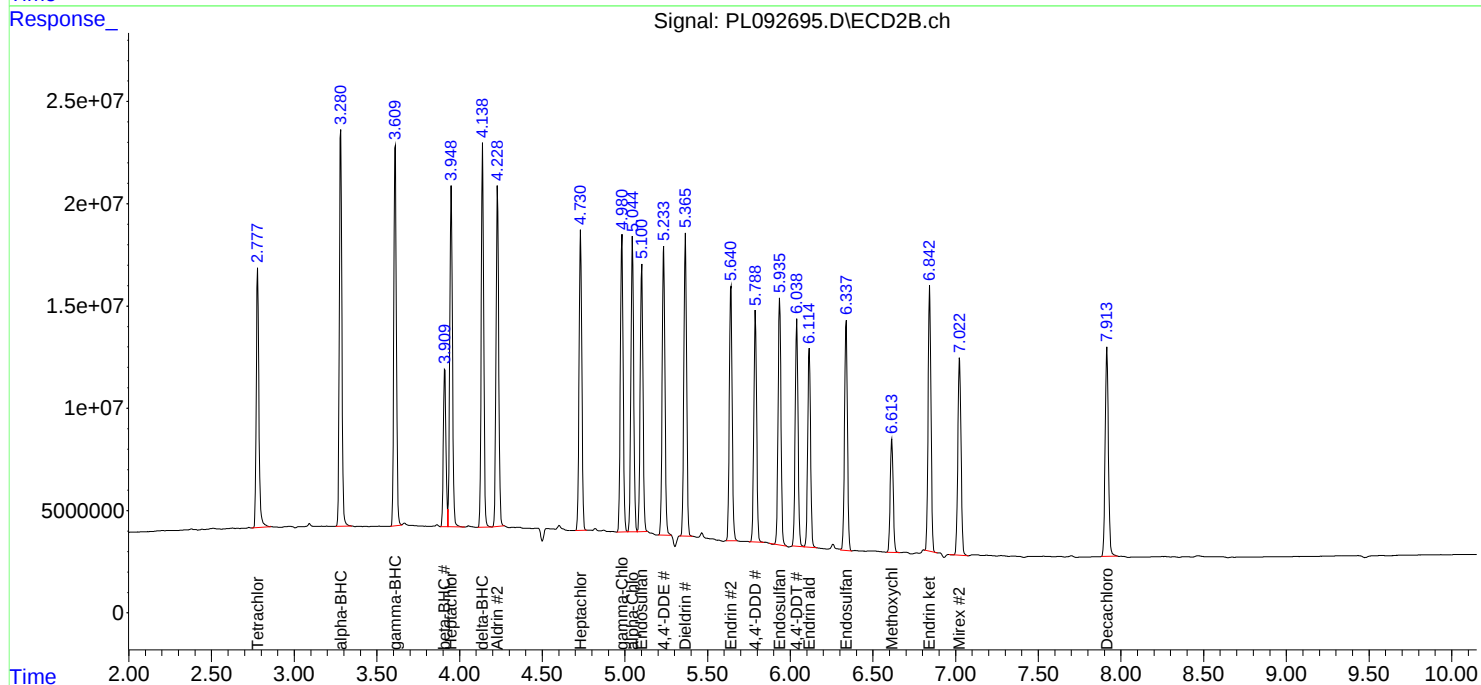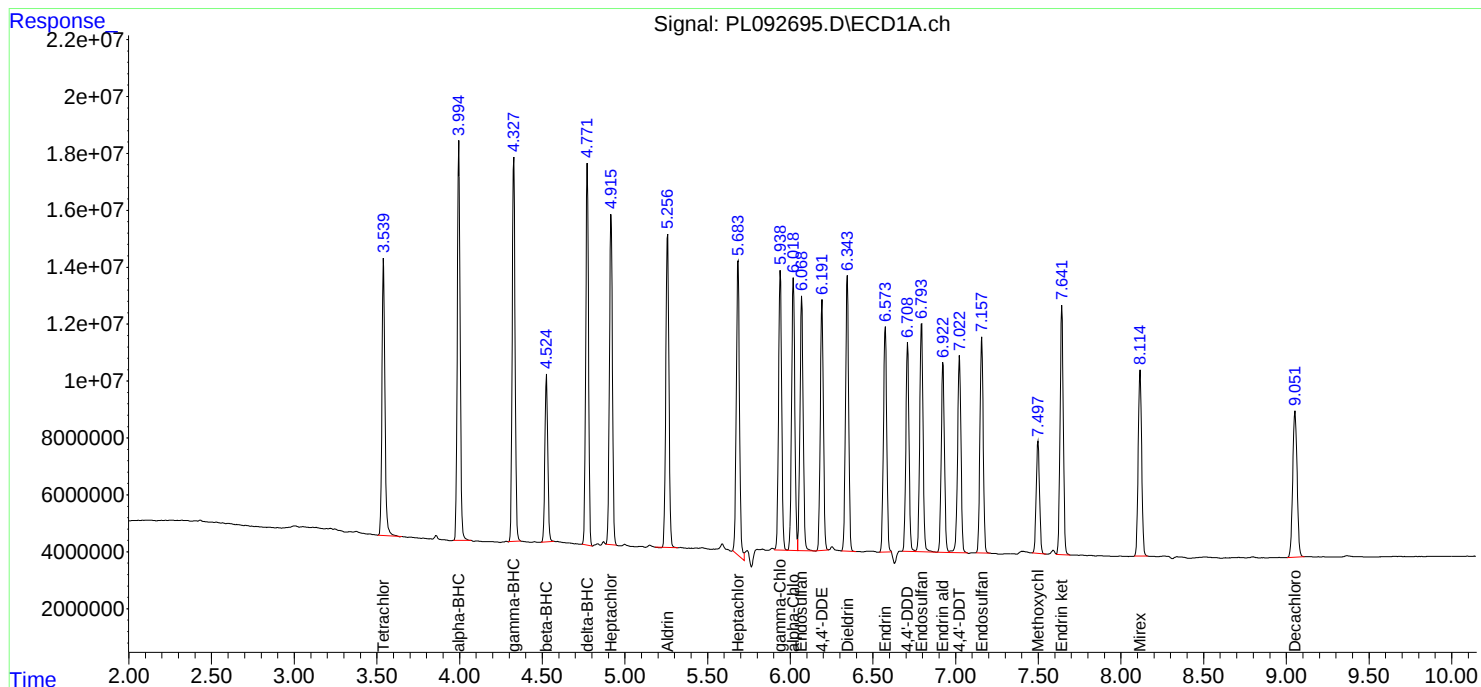



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

Continuing Calib Date: 10/29/2024 Initial Calibration Date(s): 10/28/2024 10/28/2024

Continuing Calib Time: 14:07 Initial Calibration Time(s): 14:43 15:36

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW		DIFF RT
			FROM	TO	
Decachlorobiphenyl	9.05	9.05	8.95	9.15	0.00
Tetrachloro-m-xylene	3.54	3.54	3.44	3.64	0.00
gamma-BHC (Lindane)	4.33	4.33	4.23	4.43	0.00
Heptachlor	4.92	4.92	4.82	5.02	0.00
Heptachlor epoxide	5.69	5.68	5.58	5.78	0.00
Endrin	6.58	6.57	6.47	6.67	0.00
Methoxychlor	7.50	7.50	7.40	7.60	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM **Case No.:** P4578 **SAS No.:** P4578 **SDG NO.:** P4578

Continuing Calib Date: 10/29/2024 **Initial Calibration Date(s):** 10/28/2024 10/28/2024

Continuing Calib Time: 14:07 **Initial Calibration Time(s):** 14:43 15:36

GC Column: ZB-MR1 **ID:** 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW		DIFF RT
			FROM	TO	
Decachlorobiphenyl	7.92	7.92	7.82	8.02	0.00
Tetrachloro-m-xylene	2.78	2.78	2.68	2.88	0.00
gamma-BHC (Lindane)	3.61	3.61	3.51	3.71	0.00
Heptachlor	3.95	3.95	3.85	4.05	0.00
Heptachlor epoxide	4.73	4.73	4.63	4.83	0.00
Endrin	5.64	5.64	5.54	5.74	0.00
Methoxychlor	6.61	6.62	6.52	6.72	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PORT06

Lab Code: CHEM Case No.: P4578 SAS No.: P4578 SDG NO.: P4578

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 10/28/2024 10/28/2024

Client Sample No.: CCAL02 Date Analyzed: 10/29/2024

Lab Sample No.: PSTDCCC050 Data File : PL092711.D Time Analyzed: 14:07

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Decachlorobiphenyl	9.054	8.954	9.154	50.330	50.000	0.7
Endrin	6.575	6.474	6.674	46.800	50.000	-6.4
gamma-BHC (Lindane)	4.329	4.228	4.428	51.390	50.000	2.8
Heptachlor	4.917	4.817	5.017	49.780	50.000	-0.4
Heptachlor epoxide	5.685	5.584	5.784	50.060	50.000	0.1
Methoxychlor	7.500	7.399	7.599	46.810	50.000	-6.4
Tetrachloro-m-xylene	3.541	3.440	3.640	51.450	50.000	2.9



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY
Contract: PORT06
Lab Code: CHEM **Case No.:** P4578 **SAS No.:** P4578 **SDG NO.:** P4578
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 10/28/2024 10/28/2024
Client Sample No.: CCAL02 **Date Analyzed:** 10/29/2024
Lab Sample No.: PSTDCCC050 **Data File :** PL092711.D **Time Analyzed:** 14:07

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Decachlorobiphenyl	7.916	7.816	8.016	53.470	50.000	6.9
Endrin	5.641	5.541	5.741	52.150	50.000	4.3
gamma-BHC (Lindane)	3.610	3.511	3.711	53.770	50.000	7.5
Heptachlor	3.949	3.849	4.049	52.090	50.000	4.2
Heptachlor epoxide	4.732	4.632	4.832	53.380	50.000	6.8
Methoxychlor	6.614	6.515	6.715	49.000	50.000	-2.0
Tetrachloro-m-xylene	2.778	2.678	2.878	52.950	50.000	5.9

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 14:07
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

PSTDCCC050

Manual Integrations**APPROVED**

Reviewed By :Abdul Mirza 10/30/2024

Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 00:51:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.778	126.1E6	144.1E6	51.450	52.945
28)	SA Decachlor...	9.054	7.916	96870332	145.9E6	50.334	53.468
Target Compounds							
2)	A alpha-BHC	3.996	3.280	175.2E6	215.4E6	51.670	53.986
3)	MA gamma-BHC...	4.329	3.610	167.5E6	207.5E6	51.385	53.771
4)	MA Heptachlor	4.917	3.949	149.5E6	196.6E6	49.783	52.091
5)	MB Aldrin	5.258	4.229	150.6E6	196.8E6	50.184m	53.760
6)	B beta-BHC	4.527	3.910	73253824	86231673	50.679	52.381
7)	B delta-BHC	4.773	4.139	160.4E6	206.3E6	51.247	53.679
8)	B Heptachlo...	5.685	4.732	138.2E6	178.4E6	50.056	53.377
9)	A Endosulfan I	6.070	5.101	125.1E6	161.2E6	50.005	52.800
10)	B gamma-Chl...	5.941	4.982	134.0E6	178.7E6	50.347	53.144
11)	B alpha-Chl...	6.020	5.045	133.0E6	176.3E6	50.234	52.998
12)	B 4,4'-DDE	6.193	5.234	119.9E6	172.8E6	50.594	53.648
13)	MA Dieldrin	6.345	5.366	131.8E6	178.8E6	50.014	53.536
14)	MA Endrin	6.575	5.641	106.5E6	150.9E6	46.799	52.154
15)	B Endosulfa...	6.795	5.934	117.4E6	152.0E6	49.234	53.648m
16)	A 4,4'-DDD	6.711	5.789	102.2E6	141.1E6	53.243	56.657
17)	MA 4,4'-DDT	7.023	6.040	97499557	131.2E6	47.107	48.922
18)	B Endrin al...	6.925	6.115	95349863	120.6E6	50.773	52.264
19)	B Endosulfa...	7.159	6.338	107.0E6	142.3E6	49.283	52.747
20)	A Methoxychlor	7.500	6.614	53358109	69970481	46.805	48.998
21)	B Endrin ke...	7.643	6.843	122.4E6	166.3E6	50.519	54.205
22)	Mirex	8.117	7.022	96842515	134.4E6	48.868	51.526m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 14:07
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

PSTDCCC050

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 10/30/2024

Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 00:51:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

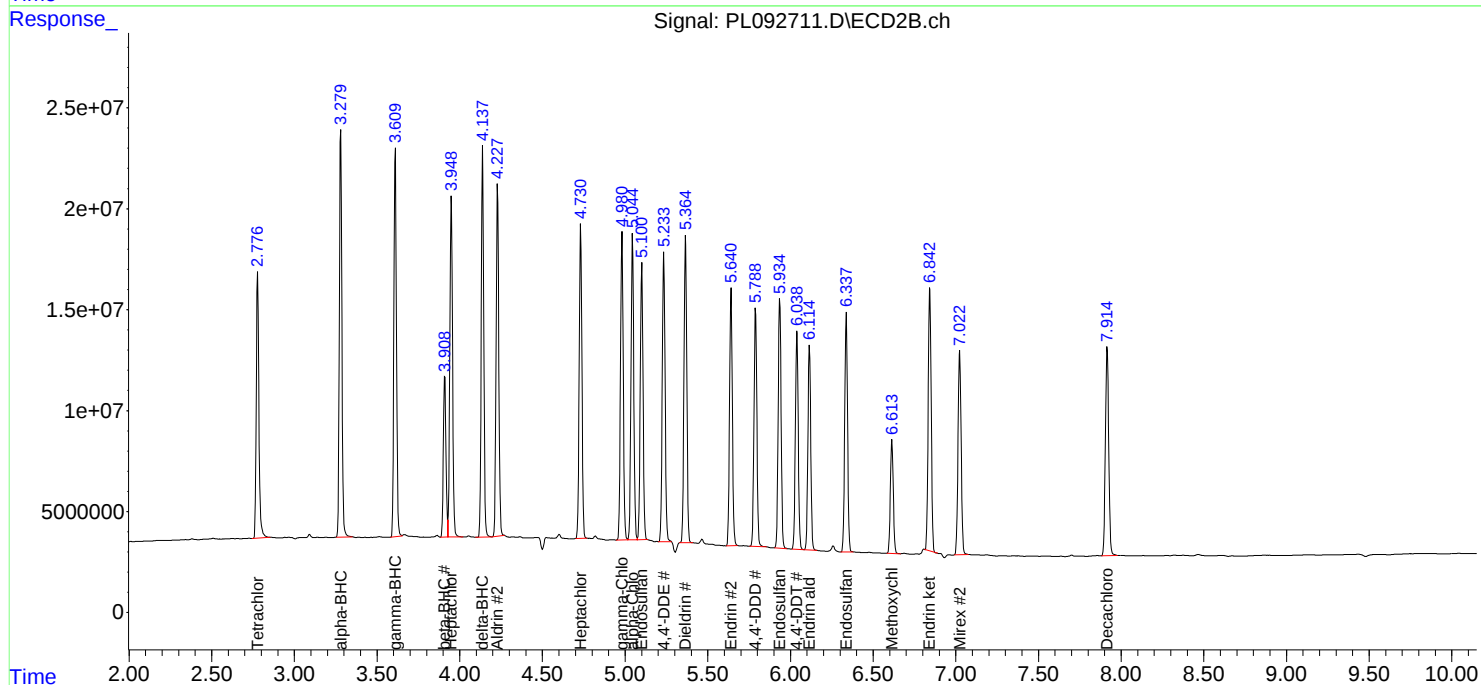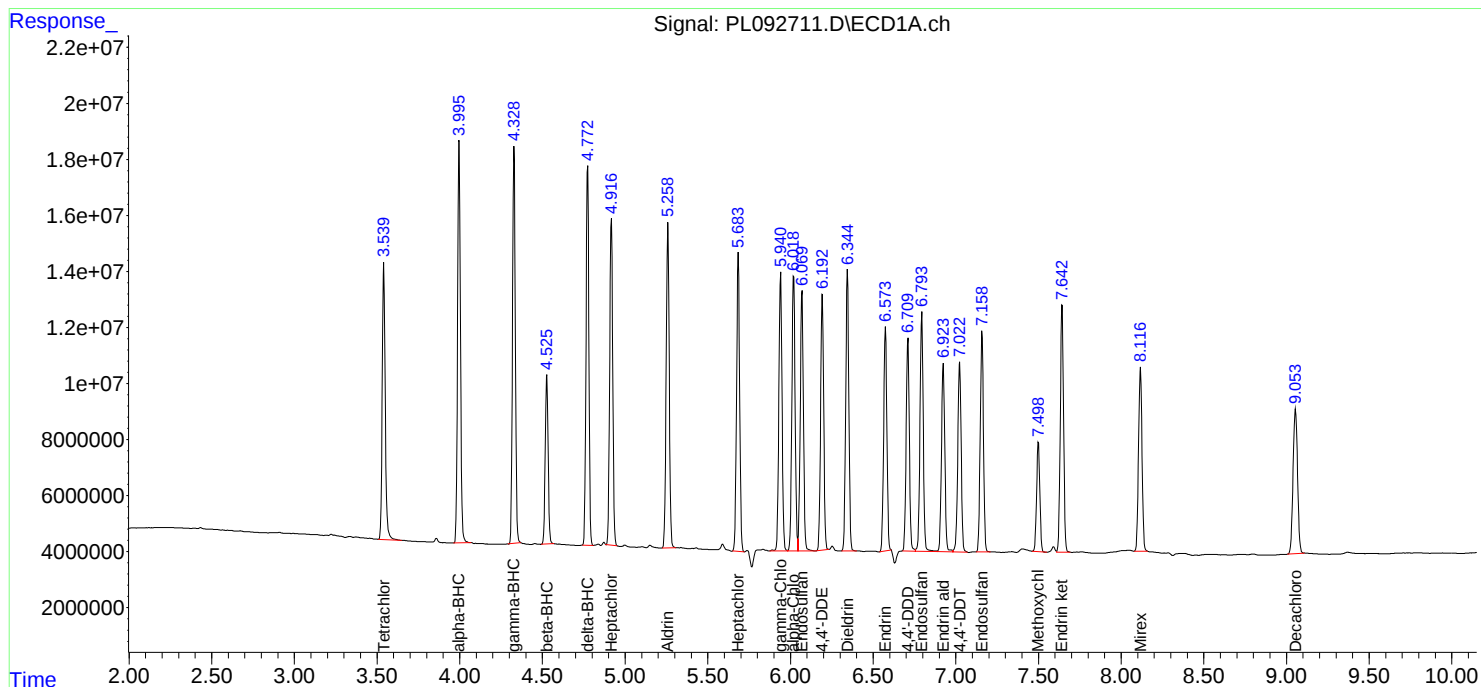

PESTICIDE CALIBRATION VERIFICATION SUMMARY

Contract: **PORT06**

Lab Code: **CHEM** Case No.: **P4578** SAS No.: **P4578** SDG NO.: **P4578**

GC Column: **ZB-MR2** ID: **0.32** (mm) Initi. Calib. Date(s): **10/28/2024** **10/28/2024**

Client Sample No. (PEM): **PEM - PL092653.D** Date Analyzed: **10/28/2024**

Lab Sample No.(PEM): **PEM** Time Analyzed: **14:16**

PEM COMPOUND	RT	RT WINDOW		CALC	NOM	%D
		FROM	TO	AMOUNT(ng)	AMOUNT(ng)	
Decachlorobiphenyl	9.059	8.960	9.160	19.970	20.000	-0.2
Tetrachloro-m-xylene	3.546	3.500	3.600	19.290	20.000	-3.6
alpha-BHC	4.001	3.950	4.050	9.920	10.000	-0.8
beta-BHC	4.531	4.480	4.580	10.060	10.000	0.6
gamma-BHC (Lindane)	4.334	4.280	4.380	9.660	10.000	-3.4
Endrin	6.580	6.510	6.650	41.060	50.000	-17.9
4,4'-DDT	7.030	6.960	7.100	88.060	100.000	-11.9
Methoxychlor	7.505	7.430	7.580	204.090	250.000	-18.4

GC Column: **ZB-MR1** ID: **0.32** (mm) Initi. Calib. Date(s): **10/28/2024** **10/28/2024**

Client Sample No. (PEM): **PEM - PL092653.D** Date Analyzed: **10/28/2024**

Lab Sample No.(PEM): **PEM** Time Analyzed: **14:16**

PEM COMPOUND	RT	RT WINDOW		CALC	NOM	%D
		FROM	TO	AMOUNT(ng)	AMOUNT(ng)	
Decachlorobiphenyl	7.918	7.820	8.020	19.080	20.000	-4.6
Tetrachloro-m-xylene	2.778	2.730	2.830	18.500	20.000	-7.5
alpha-BHC	3.281	3.230	3.330	8.630	10.000	-13.7
beta-BHC	3.911	3.860	3.960	9.760	10.000	-2.4
gamma-BHC (Lindane)	3.611	3.560	3.660	8.390	10.000	-16.1
Endrin	5.643	5.570	5.710	44.130	50.000	-11.7
4,4'-DDT	6.042	5.970	6.110	98.070	100.000	-1.9
Methoxychlor	6.616	6.550	6.690	225.800	250.000	-9.7

PEM
Data File: PL092653.D Date Acquired 10/28/2024 14:16
Operator: AR\AJ

ENDRIN BREAK DOWN

Column #1

Name	RT	Response	Response [E+EA+EK]	Response [EA+EK]	% Break Down
Endrin	6.58	93472858.4	100627495.1	7154636.74	7.11
Endrin aldehyde	6.93	2255618.869			
Endrin ketone	7.65	4899017.868			

Column #2

Name	RT	Response	Response [E+EA+EK]	Response [EA+EK]	% Break Down
Endrin #2	5.64	127670048.1	136276212.4	8606164.28	6.32
Endrin aldehyde #2	6.12	3697589.438			
Endrin ketone #2	6.84	4908574.846			

DDT BREAK DOWN

Column #1

Name	RT	Response	Response [DDT+DDE+DDD]	Response [DDE+DDD]	% Break Down
4,4'-DDT	7.03	182263263.3	183689930.4	1426667.08	0.78
4,4'-DDE	0.00	0			
4,4'-DDD	6.72	1426667.076			

Column #2

Name	RT	Response	Response [DDT+DDE+DDD]	Response [DDE+DDD]	% Break Down
4,4'-DDT #2	6.04	263061944.1	264286032.2	1224088.02	0.46
4,4'-DDE #2	0.00	0			
4,4'-DDD #2	5.79	1224088.016			

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092653.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 14:16
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PEM

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/29/2024
 Supervised By : Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:21:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:19:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.778	47253047	50346316	19.285	18.502
28)	SA Decachlor...	9.059	7.918	38436874	52072459	19.972	19.079
Target Compounds							
2)	A alpha-BHC	4.001	3.281	33636067	34444224	9.918	8.632
3)	MA gamma-BHC...	4.334	3.611	31492360	32364466	9.662	8.386
6)	B beta-BHC	4.531	3.911	14540729	16063325	10.060	9.758
14)	MA Endrin	6.580	5.643	93472858	127.7E6	41.057	44.131
16)	A 4,4'-DDD	6.718	5.791	1426667	1224088	0.743m	0.492m#
17)	MA 4,4'-DDT	7.030	6.042	182.3E6	263.1E6	88.060	98.075
18)	B Endrin al...	6.930	6.117	2255619	3697589	1.201	1.603 #
20)	A Methoxychlor	7.505	6.616	232.7E6	322.5E6	204.088	225.801
21)	B Endrin ke...	7.648	6.845	4899018	4908575	2.022	1.600

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092653.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 14:16
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PEM

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/29/2024
Supervised By : Ankita Jodhani 10/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:21:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:19:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

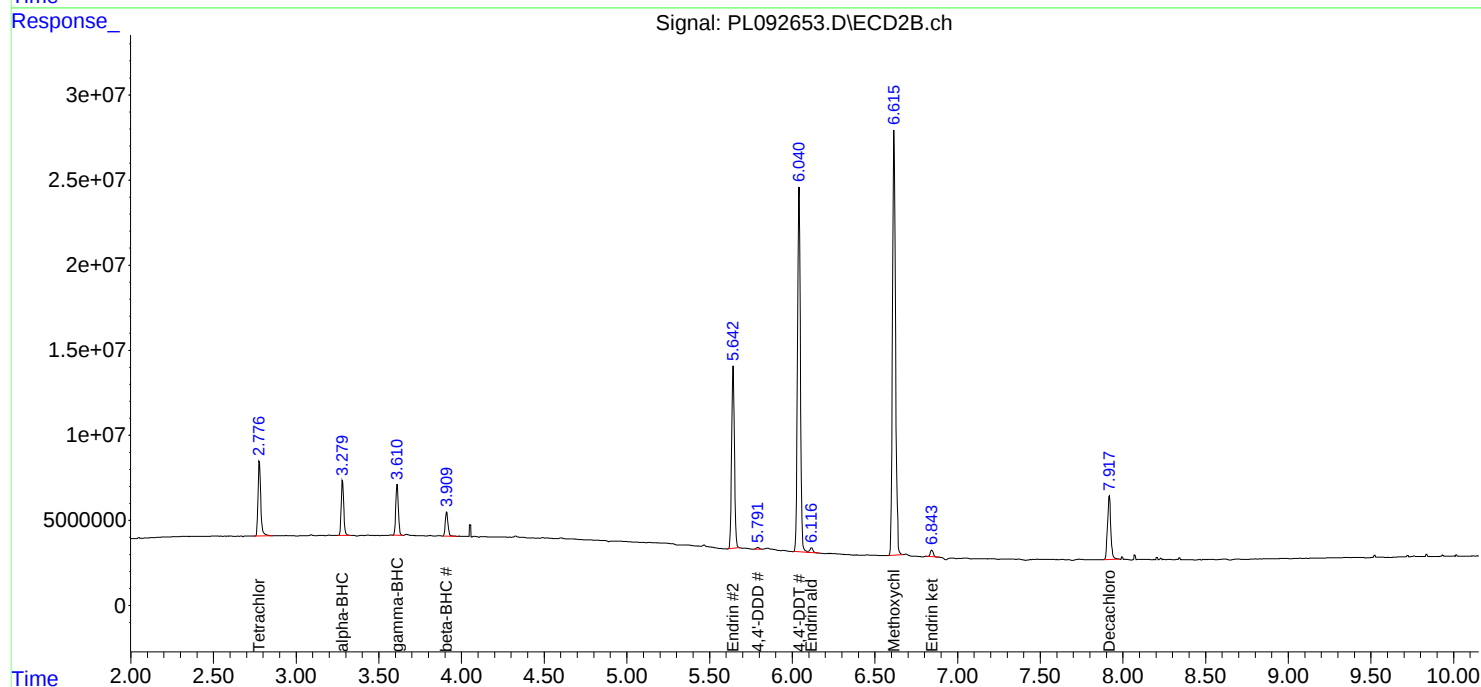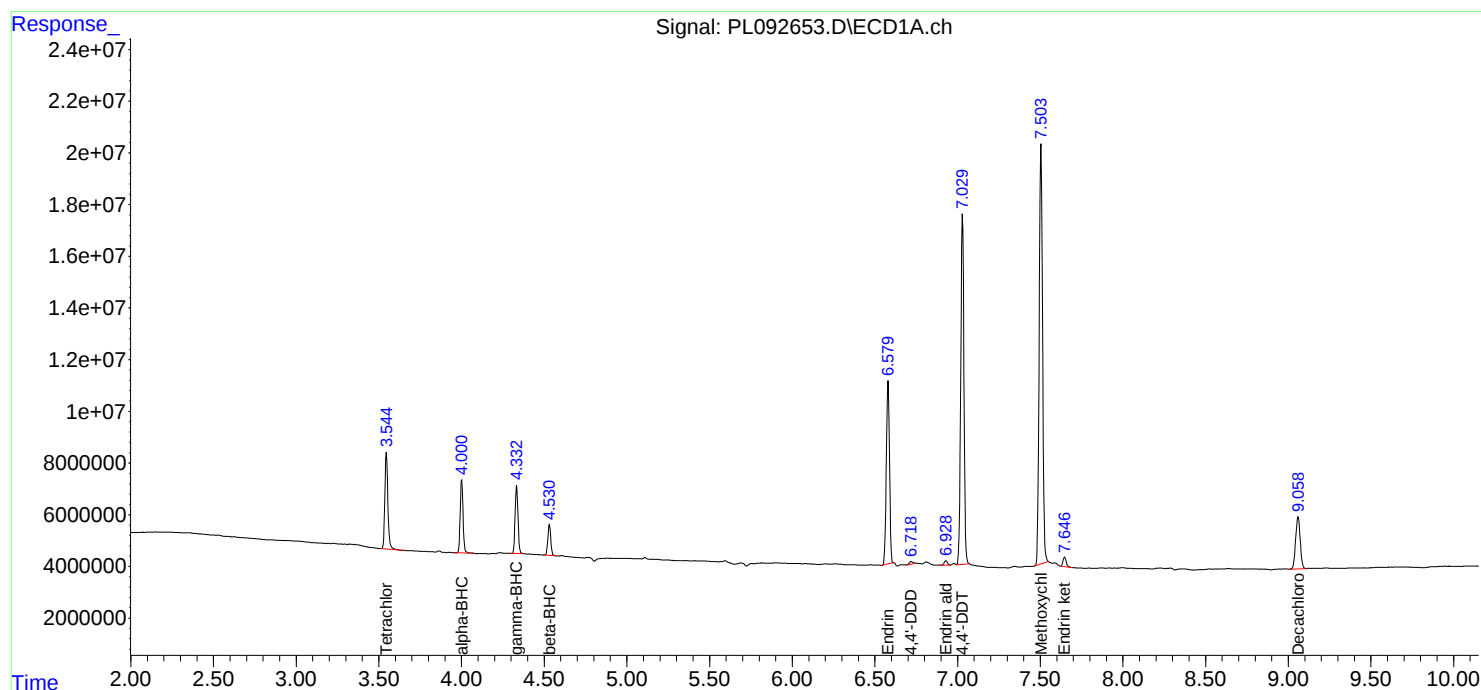

PESTICIDE CALIBRATION VERIFICATION SUMMARY

Contract: **PORT06**

Lab Code: **CHEM** Case No.: **P4578** SAS No.: **P4578** SDG NO.: **P4578**

GC Column: **ZB-MR2** ID: **0.32** (mm) Initi. Calib. Date(s): **10/28/2024** **10/28/2024**

Client Sample No. (PEM): **PEM - PL092694.D** Date Analyzed: **10/29/2024**

Lab Sample No.(PEM): **PEM** Time Analyzed: **10:02**

PEM COMPOUND	RT	RT WINDOW		CALC	NOM	%D
		FROM	TO	AMOUNT(ng)	AMOUNT(ng)	
Decachlorobiphenyl	9.054	8.950	9.150	20.630	20.000	3.2
Tetrachloro-m-xylene	3.541	3.490	3.590	20.180	20.000	0.9
alpha-BHC	3.996	3.950	4.050	10.410	10.000	4.1
beta-BHC	4.526	4.480	4.580	10.930	10.000	9.3
gamma-BHC (Lindane)	4.329	4.280	4.380	10.230	10.000	2.3
Endrin	6.575	6.500	6.650	42.430	50.000	-15.1
4,4'-DDT	7.024	6.950	7.090	89.050	100.000	-11.0
Methoxychlor	7.500	7.430	7.570	209.100	250.000	-16.4

GC Column: **ZB-MR1** ID: **0.32** (mm) Initi. Calib. Date(s): **10/28/2024** **10/28/2024**

Client Sample No. (PEM): **PEM - PL092694.D** Date Analyzed: **10/29/2024**

Lab Sample No.(PEM): **PEM** Time Analyzed: **10:02**

PEM COMPOUND	RT	RT WINDOW		CALC	NOM	%D
		FROM	TO	AMOUNT(ng)	AMOUNT(ng)	
Decachlorobiphenyl	7.916	7.820	8.020	20.450	20.000	2.3
Tetrachloro-m-xylene	2.779	2.730	2.830	19.400	20.000	-3.0
alpha-BHC	3.281	3.230	3.330	9.150	10.000	-8.5
beta-BHC	3.911	3.860	3.960	10.440	10.000	4.4
gamma-BHC (Lindane)	3.611	3.560	3.660	8.940	10.000	-10.6
Endrin	5.642	5.570	5.710	47.400	50.000	-5.2
4,4'-DDT	6.040	5.970	6.110	102.500	100.000	2.5
Methoxychlor	6.615	6.540	6.690	231.820	250.000	-7.3

PEM
Data File: PL092694.D Date Acquired 10/29/2024 10:02
Operator: AR\AJ

ENDRIN BREAK DOWN

Column #1

Name	RT	Response	Response [E+EA+EK]	Response [EA+EK]	% Break Down
Endrin	6.57	96595273.88	105834673.6	9239399.72	8.73
Endrin aldehyde	6.92	3058703.633			
Endrin ketone	7.64	6180696.091			

Column #2

Name	RT	Response	Response [E+EA+EK]	Response [EA+EK]	% Break Down
Endrin #2	5.64	137137485.5	147577853.2	10440367.7	7.07
Endrin aldehyde #2	6.12	3670909.484			
Endrin ketone #2	6.84	6769458.17			

DDT BREAK DOWN

Column #1

Name	RT	Response	Response [DDT+DDE+DDD]	Response [DDE+DDD]	% Break Down
4,4'-DDT	7.02	184305539.5	188154047.8	3848508.32	2.05
4,4'-DDE	0.00	0			
4,4'-DDD	6.71	3848508.32			

Column #2

Name	RT	Response	Response [DDT+DDE+DDD]	Response [DDE+DDD]	% Break Down
4,4'-DDT #2	6.04	274931323.4	278437313.2	3505989.73	1.26
4,4'-DDE #2	0.00	0			
4,4'-DDD #2	5.79	3505989.731			

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092694.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 10:02
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PEM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 12:30:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.779	49453430	52803176	20.183	19.405
28) SA Decachlor...	9.054	7.916	39703848	55817184	20.630	20.452
Target Compounds						
2) A alpha-BHC	3.996	3.281	35290534	36492710	10.405	9.146
3) MA gamma-BHC...	4.329	3.611	33338334	34494865	10.228	8.938
6) B beta-BHC	4.526	3.911	15793927	17190837	10.927	10.442
14) MA Endrin	6.575	5.642	96595274	137.1E6	42.429	47.403
16) A 4,4'-DDD	6.710	5.789	3848508	3505990	2.005	1.408 #
17) MA 4,4'-DDT	7.024	6.040	184.3E6	274.9E6	89.047	102.500
18) B Endrin al...	6.924	6.116	3058704	3670909	1.629	1.591
20) A Methoxychlor	7.500	6.615	238.4E6	331.0E6	209.097	231.819
21) B Endrin ke...	7.643	6.843	6180696	6769458	2.551	2.206



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092694.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 10:02
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PEM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 12:30:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

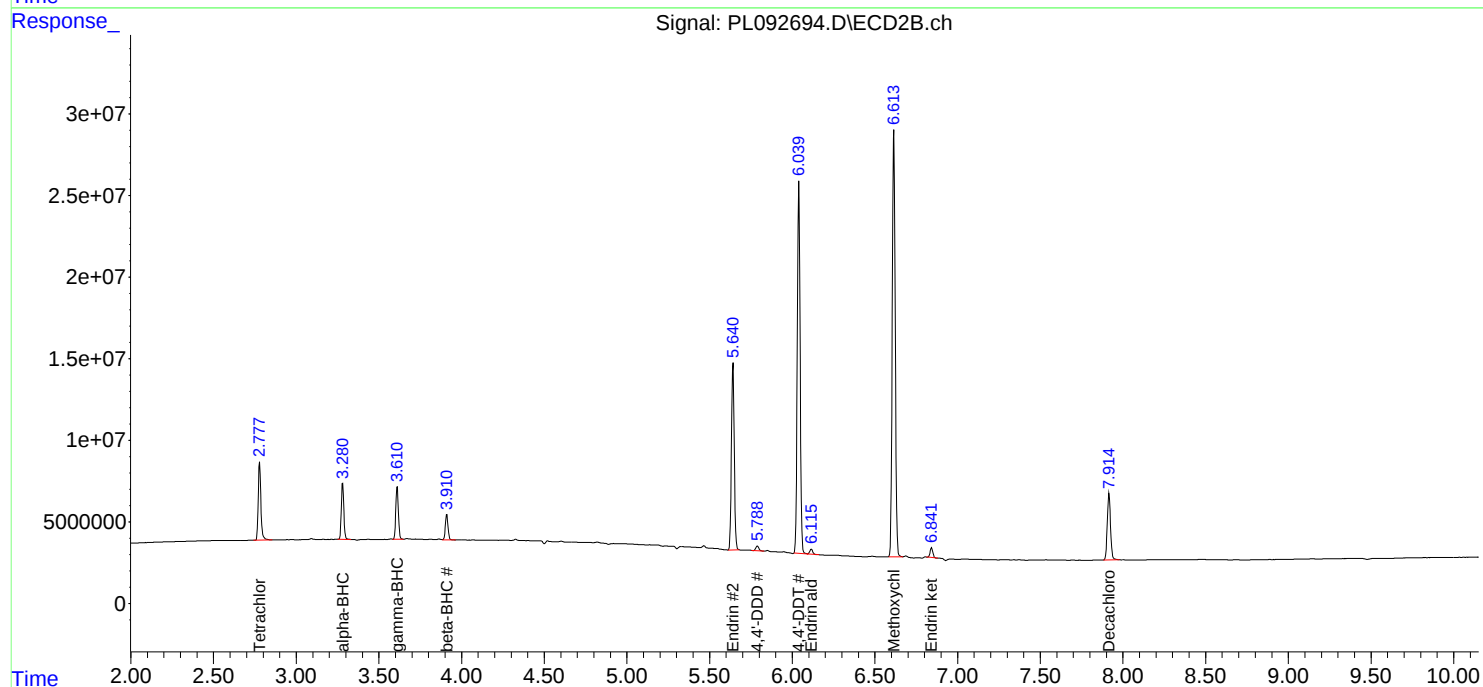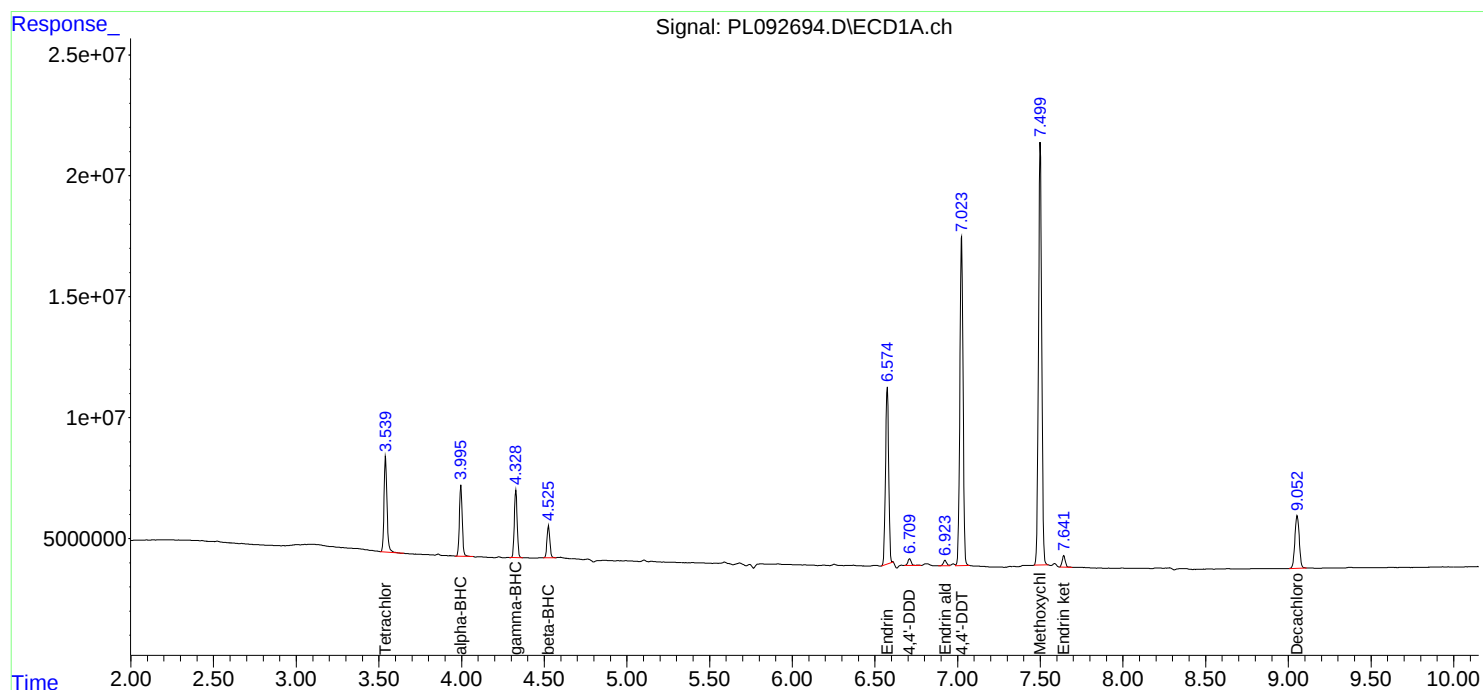

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092654.D
Acq On : 28 Oct 2024 14:29
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Title : GC Extractables
Last Update : Mon Oct 28 18:58:23 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.540	5.940	100.00%
5.940	6.070	100.00%
6.070	6.193	100.00%
6.193	6.345	100.00%
6.345	7.158	100.00%
7.158	7.499	100.00%
7.499	7.643	100.00%
7.643	9.054	100.00%

Signal #2

2.778	4.982	100.00%
4.982	5.102	100.00%
5.102	5.235	100.00%
5.235	5.366	100.00%
5.366	6.338	100.00%
6.338	6.615	100.00%
6.615	6.844	100.00%
6.844	7.916	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 14:29
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:21:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:19:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.778	48587926	52085719	19.830	19.141
28)	SA Decachlor...	9.054	7.916	38629596	53476121	20.072	19.594
Target Compounds							
9)	A Endosulfan I	6.070	5.102	26602716	28047383	10.635	9.186
10)	B gamma-Chl...	5.940	4.982	28607831	32626788	10.752	9.705
12)	B 4,4'-DDE	6.193	5.235	47717989	61582025	20.141	19.115
13)	MA Dieldrin	6.345	5.366	51856039	61668549	19.676	18.462
19)	B Endosulfa...	7.158	6.338	40592527	50485467	18.703	18.720
20)	A Methoxychlor	7.499	6.615	100.3E6	134.2E6	87.976	93.949
21)	B Endrin ke...	7.643	6.844	47240044	57600618	19.498	18.770



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 14:29
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:21:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:19:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

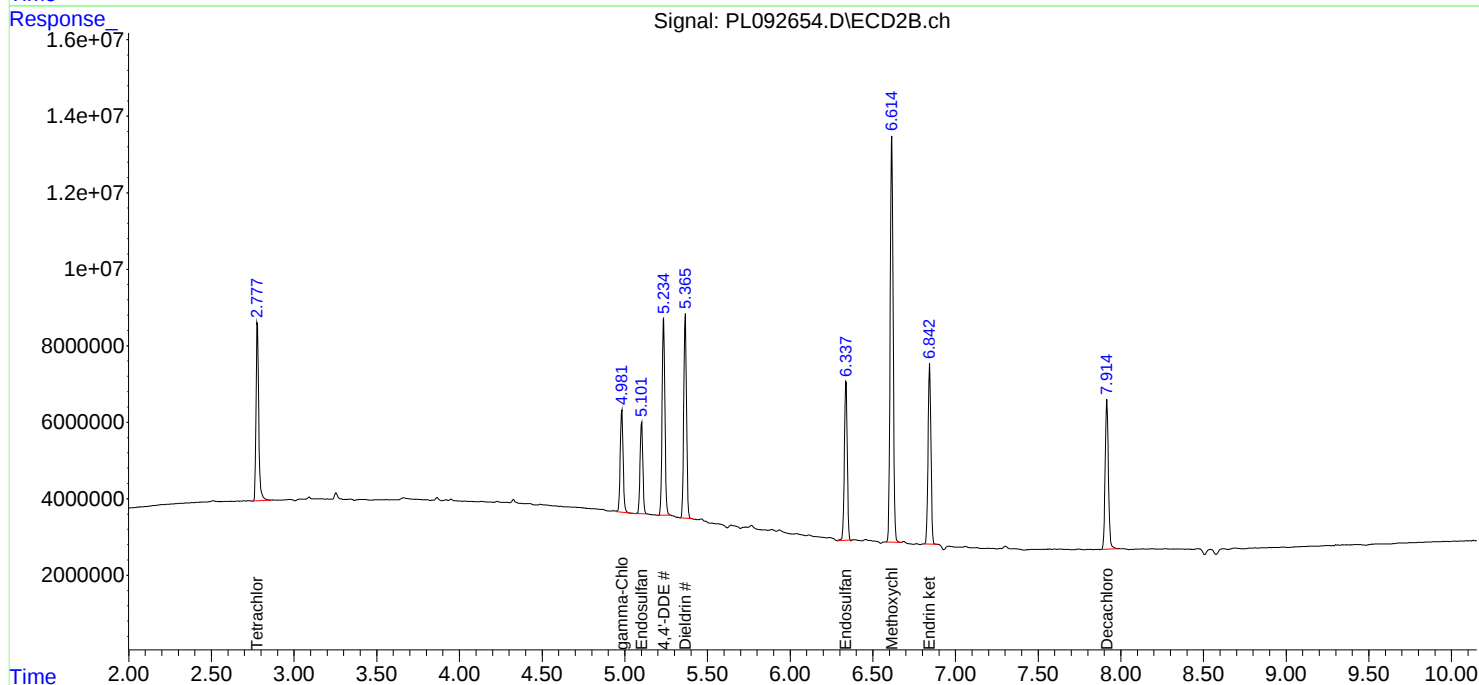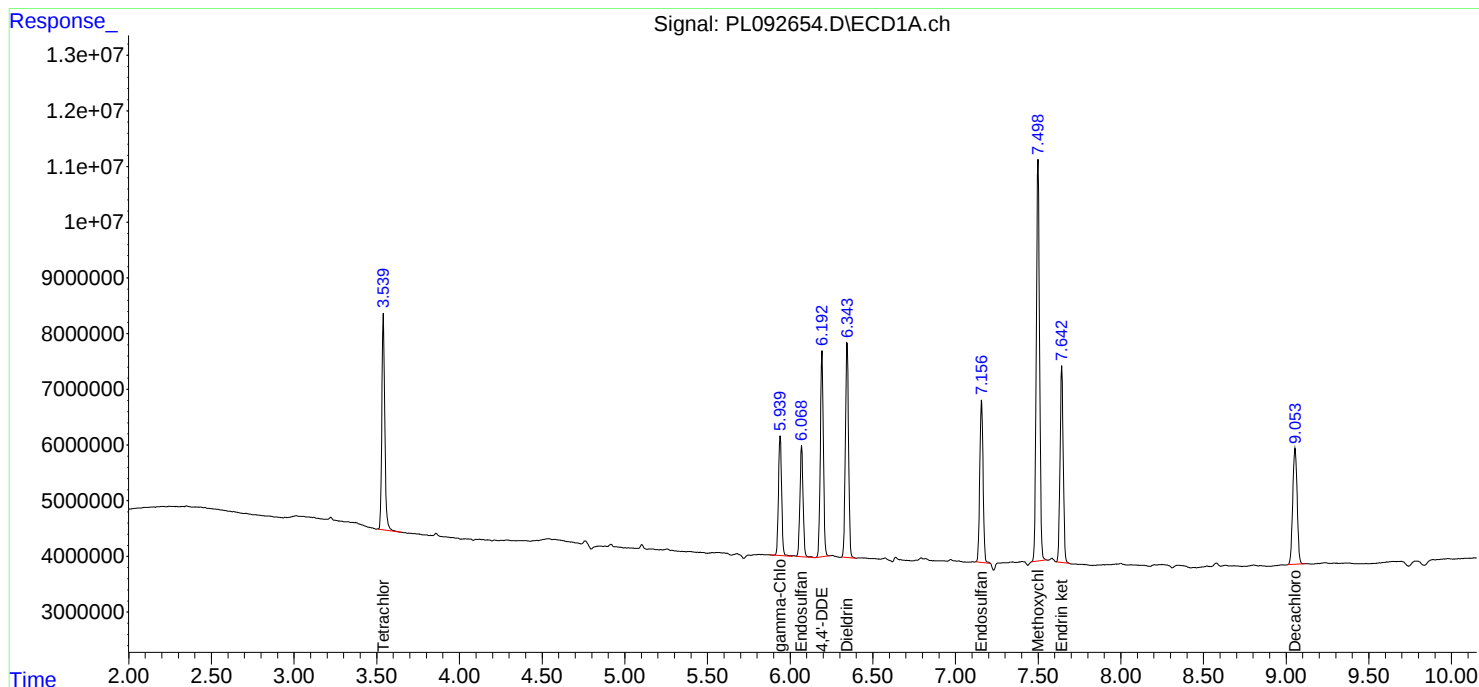

Analytical Sequence

Client: Portal Partners Tri-Venture	SDG No.: P4578
Project: Amtrak Sawtooth Bridges 2024	Instrument ID: ECD_L
GC Column: ZB-MR2	ID: 0.32 (mm) Inst. Calib. Date(s): 10/28/2024 10/28/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
LBLK	LBLK	10/28/2024	13:55	PL092652.D	9.05	3.54
PEM	PEM	10/28/2024	14:16	PL092653.D	9.06	3.55
RESCHK	RESCHK	10/28/2024	14:29	PL092654.D	9.05	3.54
PSTDICCC100	PSTDICCC100	10/28/2024	14:43	PL092655.D	9.05	3.54
PSTDICCC075	PSTDICCC075	10/28/2024	14:56	PL092656.D	9.05	3.54
PSTDICCC050	PSTDICCC050	10/28/2024	15:09	PL092657.D	9.05	3.54
PSTDICCC025	PSTDICCC025	10/28/2024	15:23	PL092658.D	9.05	3.54
PSTDICCC005	PSTDICCC005	10/28/2024	15:36	PL092659.D	9.05	3.54
PCHLORICC500	PCHLORICC500	10/28/2024	16:16	PL092662.D	9.06	3.54
PTOXICC500	PTOXICC500	10/28/2024	17:23	PL092667.D	9.05	3.54
LBLK	LBLK	10/29/2024	09:48	PL092693.D	9.06	3.54
PEM	PEM	10/29/2024	10:02	PL092694.D	9.05	3.54
PSTDCCC050	PSTDCCC050	10/29/2024	10:15	PL092695.D	9.05	3.54
PB164445BL	PB164445BL	10/29/2024	10:43	PL092697.D	9.05	3.54
PB164445BS	PB164445BS	10/29/2024	10:57	PL092698.D	9.05	3.54
PB164393TB	PB164393TB	10/29/2024	11:10	PL092699.D	9.05	3.54
WB-305-BOT	P4578-06	10/29/2024	11:23	PL092700.D	9.05	3.54
WB-305-BOTMS	P4578-06MS	10/29/2024	11:37	PL092701.D	9.05	3.54
WB-305-BOTMSD	P4578-06MSD	10/29/2024	11:50	PL092702.D	9.05	3.54
WB-305-BOT-1	P4578-08	10/29/2024	12:04	PL092703.D	9.05	3.54
LBLK	LBLK	10/29/2024	13:53	PL092710.D	9.05	3.54
PSTDCCC050	PSTDCCC050	10/29/2024	14:07	PL092711.D	9.05	3.54

Analytical Sequence

Client: Portal Partners Tri-Venture	SDG No.: P4578
Project: Amtrak Sawtooth Bridges 2024	Instrument ID: ECD_L
GC Column: ZB-MR1	ID: 0.32 (mm) Inst. Calib. Date(s): 10/28/2024 10/28/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	10/28/2024	13:55	PL092652.D	7.92	2.78
PEM	PEM	10/28/2024	14:16	PL092653.D	7.92	2.78
RESCHK	RESCHK	10/28/2024	14:29	PL092654.D	7.92	2.78
PSTDICC100	PSTDICC100	10/28/2024	14:43	PL092655.D	7.92	2.78
PSTDICC075	PSTDICC075	10/28/2024	14:56	PL092656.D	7.92	2.78
PSTDICC050	PSTDICC050	10/28/2024	15:09	PL092657.D	7.92	2.78
PSTDICC025	PSTDICC025	10/28/2024	15:23	PL092658.D	7.92	2.78
PSTDICC005	PSTDICC005	10/28/2024	15:36	PL092659.D	7.92	2.78
PCHLORICC500	PCHLORICC500	10/28/2024	16:16	PL092662.D	7.92	2.78
PTOXICC500	PTOXICC500	10/28/2024	17:23	PL092667.D	7.92	2.78
IBLK	IBLK	10/29/2024	09:48	PL092693.D	7.92	2.78
PEM	PEM	10/29/2024	10:02	PL092694.D	7.92	2.78
PSTDCCC050	PSTDCCC050	10/29/2024	10:15	PL092695.D	7.92	2.78
PB164445BL	PB164445BL	10/29/2024	10:43	PL092697.D	7.92	2.78
PB164445BS	PB164445BS	10/29/2024	10:57	PL092698.D	7.92	2.78
PB164393TB	PB164393TB	10/29/2024	11:10	PL092699.D	7.92	2.78
WB-305-BOT	P4578-06	10/29/2024	11:23	PL092700.D	7.92	2.78
WB-305-BOTMS	P4578-06MS	10/29/2024	11:37	PL092701.D	7.91	2.78
WB-305-BOTMSD	P4578-06MSD	10/29/2024	11:50	PL092702.D	7.92	2.78
WB-305-BOT-1	P4578-08	10/29/2024	12:04	PL092703.D	7.92	2.78
IBLK	IBLK	10/29/2024	13:53	PL092710.D	7.92	2.78
PSTDCCC050	PSTDCCC050	10/29/2024	14:07	PL092711.D	7.92	2.78

COMPOUND DETECTION SUMMARY

CLIENT SAMPLE NO.

PB164445BS

Contract: PORT06

Lab Code: CHEM

Case No.: P4578

SAS No.: P4578

SDG NO.: P4578

Lab Sample ID: PB164445BS

Date(s) Analyzed: 10/29/2024

10/29/2024

Instrument ID (1): ECD_L

Instrument ID (2): ECD_L

GC Column: (1): ZB-MR2

ID: 0.32 (mm)

GC Column: (2): ZB-MR1

ID: 0.32 (mm)

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
gamma-BHC (Lindane)	1	4.33	4.28	4.38	0.046	4.2
	2	3.61	3.56	3.66	0.048	
Endrin	1	6.57	6.52	6.62	0.043	6.6
	2	5.64	5.59	5.69	0.045	
Methoxychlor	1	7.50	7.45	7.55	0.045	0.2
	2	6.61	6.56	6.66	0.045	
Heptachlor	1	4.92	4.87	4.97	0.048	4.1
	2	3.95	3.90	4.00	0.050	
Heptachlor epoxide	1	5.68	5.63	5.73	0.046	6.1
	2	4.73	4.68	4.78	0.049	

COMPOUND DETECTION SUMMARY

CLIENT SAMPLE NO.

WB-305-BOTMS

Contract: PORT06

Lab Code: CHEM

Case No.: P4578

SAS No.: P4578

SDG NO.: P4578

Lab Sample ID: P4578-06MS

Date(s) Analyzed: 10/29/2024

10/29/2024

Instrument ID (1): ECD_L

Instrument ID (2): ECD_L

GC Column: (1): ZB-MR2

ID: 0.32 (mm)

GC Column: (2): ZB-MR1

ID: 0.32 (mm)

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
Methoxychlor	1	7.50	7.45	7.55	0.44	3.8
	2	6.62	6.57	6.67	0.46	
gamma-BHC (Lindane)	1	4.33	4.28	4.38	0.44	5.8
	2	3.61	3.56	3.66	0.46	
Heptachlor	1	4.92	4.87	4.97	0.45	4
	2	3.95	3.90	4.00	0.47	
Heptachlor epoxide	1	5.68	5.63	5.73	0.44	5.4
	2	4.73	4.68	4.78	0.46	
Endrin	1	6.57	6.52	6.62	0.43	8.6
	2	5.64	5.59	5.69	0.47	

COMPOUND DETECTION SUMMARY

CLIENT SAMPLE NO.

WB-305-BOTMSD

Contract: PORT06

Lab Code: CHEM

Case No.: P4578

SAS No.: P4578

SDG NO.: P4578

Lab Sample ID: P4578-06MSD

Date(s) Analyzed: 10/29/2024

10/29/2024

Instrument ID (1): ECD_L

Instrument ID (2): ECD_L

GC Column: (1): ZB-MR2

ID: 0.32 (mm)

GC Column: (2): ZB-MR1

ID: 0.32 (mm)

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
Methoxychlor	1	7.50	7.45	7.55	0.44	4.2
	2	6.61	6.56	6.66	0.46	
gamma-BHC (Lindane)	1	4.33	4.28	4.38	0.43	5.8
	2	3.61	3.56	3.66	0.46	
Heptachlor	1	4.92	4.87	4.97	0.45	4
	2	3.95	3.90	4.00	0.47	
Heptachlor epoxide	1	5.68	5.63	5.73	0.44	6.1
	2	4.73	4.68	4.78	0.46	
Endrin	1	6.57	6.52	6.62	0.43	7.6
	2	5.64	5.59	5.69	0.47	



QC SAMPLE DATA

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	
Client Sample ID:	PB164445BL	SDG No.:	P4578
Lab Sample ID:	PB164445BL	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	TCLP Pesticide
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092697.D	1	10/26/24 12:50	10/29/24 10:43	PB164445

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.00050	U	0.00050	0.0050	ug/L
76-44-8	Heptachlor	0.00050	U	0.00050	0.0050	ug/L
1024-57-3	Heptachlor epoxide	0.00090	U	0.00090	0.0050	ug/L
72-20-8	Endrin	0.00040	U	0.00040	0.0050	ug/L
72-43-5	Methoxychlor	0.0011	U	0.0011	0.0050	ug/L
8001-35-2	Toxaphene	0.015	U	0.015	0.10	ug/L
57-74-9	Chlordane	0.0082	U	0.0082	0.050	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	19.2		30 (43) - 150 (140)	96%	SPK: 20
877-09-8	Tetrachloro-m-xylene	18.3		30 (77) - 150 (126)	91%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 10:43
 Operator : AR\AJ
 Sample : PB164445BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164445BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:09:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.778	44714826	48353246	18.249	17.769
28) SA Decachlor...	9.053	7.915	36975516	50429295	19.213	18.477

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 10:43
Operator : AR\AJ
Sample : PB164445BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB164445BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:09:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

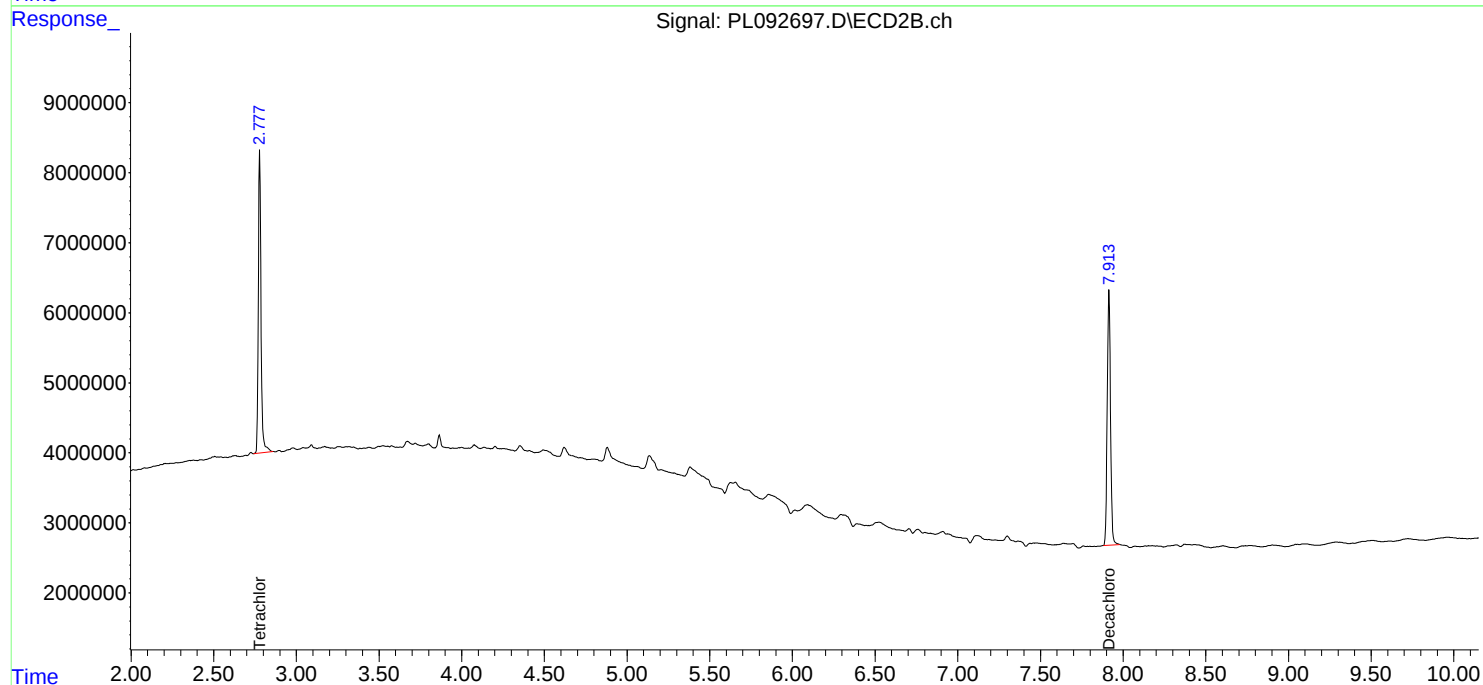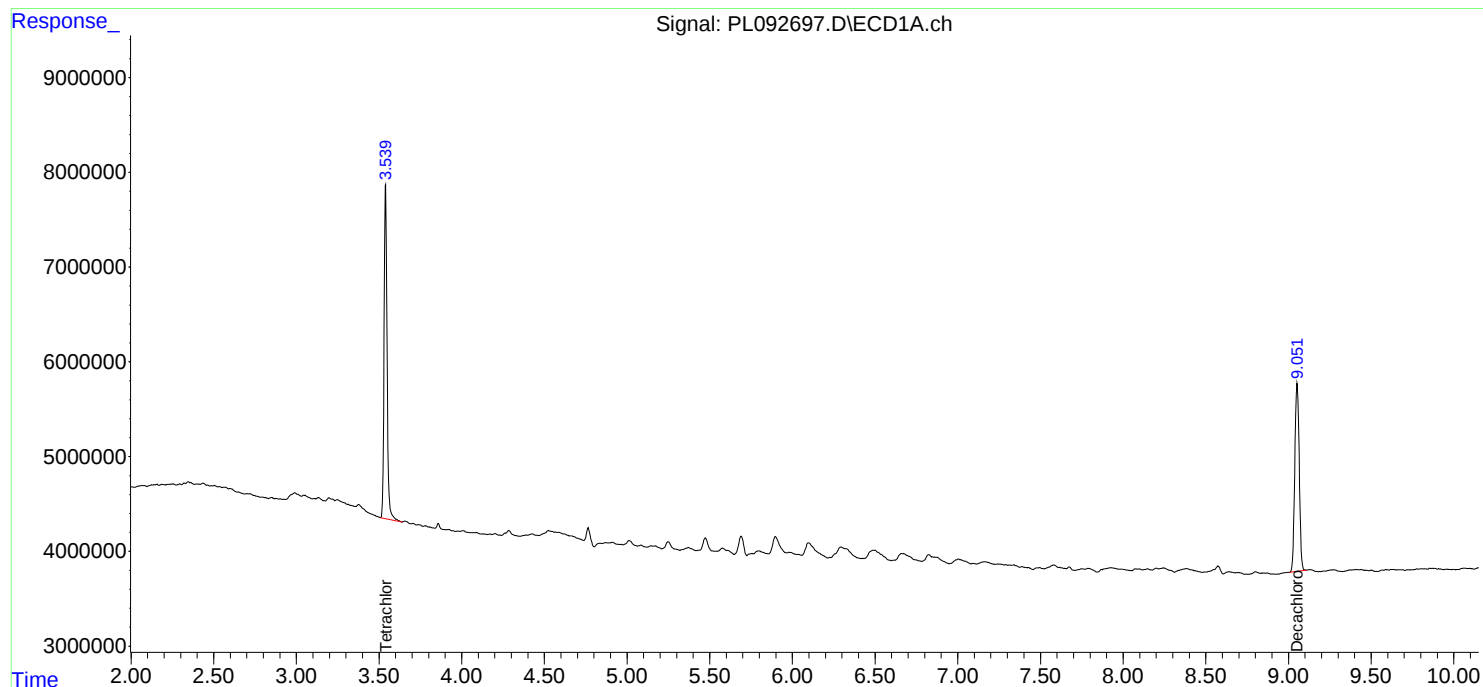


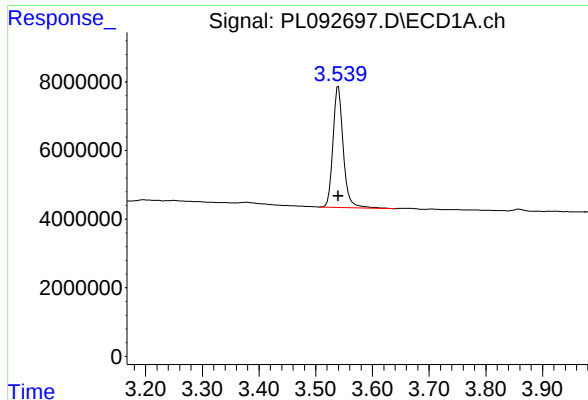

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 44714826
Conc: 18.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164445BL

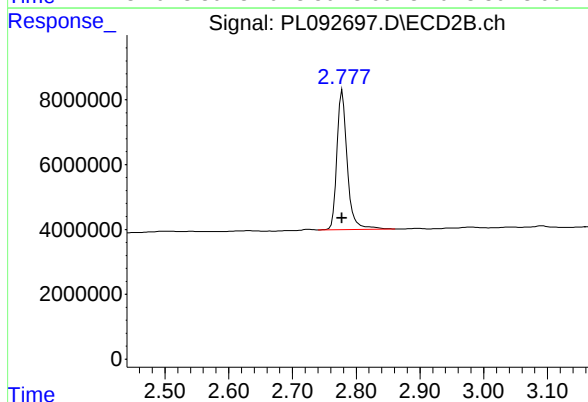


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 48353246
Conc: 17.77 ng/ml

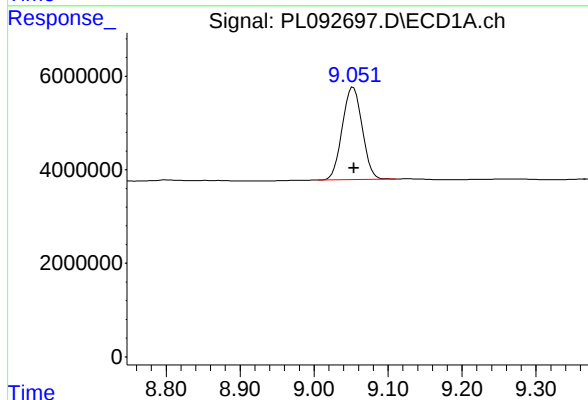

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.001 min
Response: 36975516
Conc: 19.21 ng/ml

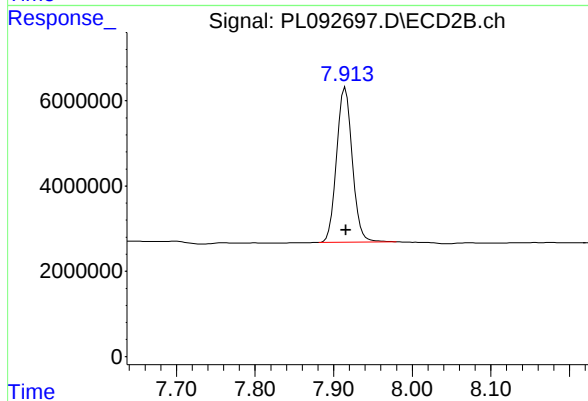

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 50429295
Conc: 18.48 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	10/28/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	10/28/24
Client Sample ID:	PIBLK-PL092652.D	SDG No.:	P4578
Lab Sample ID:	I.BLK-PL092652.D	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Decanted:	
GPC Factor :	1.0	Final Vol:	10000
PH :		Test:	TCLP Pesticide
Prep Method :	3510C	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092652.D	1		10/28/24	PL102824

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.0049	U	0.0049	0.050	ug/L
76-44-8	Heptachlor	0.0054	U	0.0054	0.050	ug/L
1024-57-3	Heptachlor epoxide	0.0090	U	0.0090	0.050	ug/L
72-20-8	Endrin	0.0043	U	0.0043	0.050	ug/L
72-43-5	Methoxychlor	0.011	U	0.011	0.050	ug/L
8001-35-2	Toxaphene	0.15	U	0.15	1.00	ug/L
57-74-9	Chlordane	0.082	U	0.082	0.50	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	22.7		30 (43) - 150 (140)	114%	SPK: 20
877-09-8	Tetrachloro-m-xylene	21.6		30 (77) - 150 (126)	108%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
 Data File : PL092652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 13:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 17:20:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 17:19:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.777	52846066	55504223	21.568	20.397
28) SA Decachlor...	9.052	7.915	43705517	59287776	22.709	21.723

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102824\
Data File : PL092652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 13:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 17:20:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 17:19:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

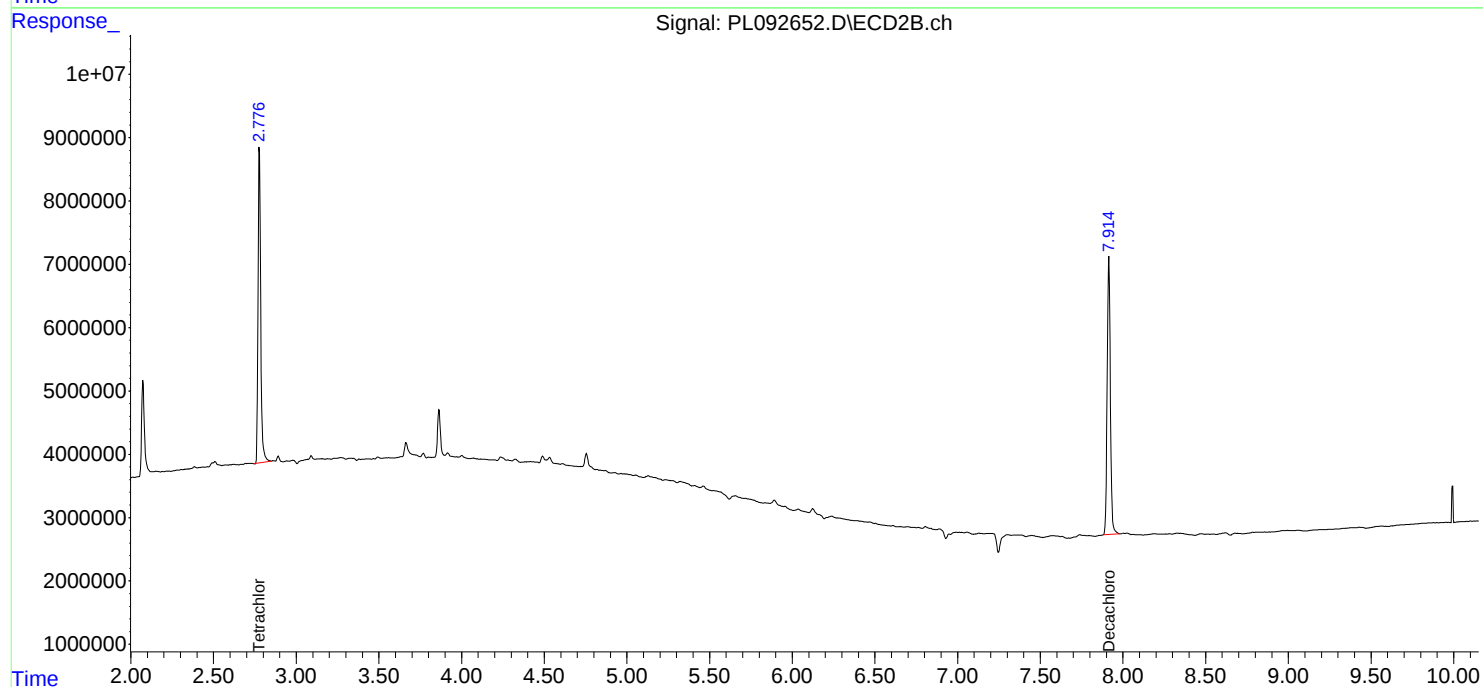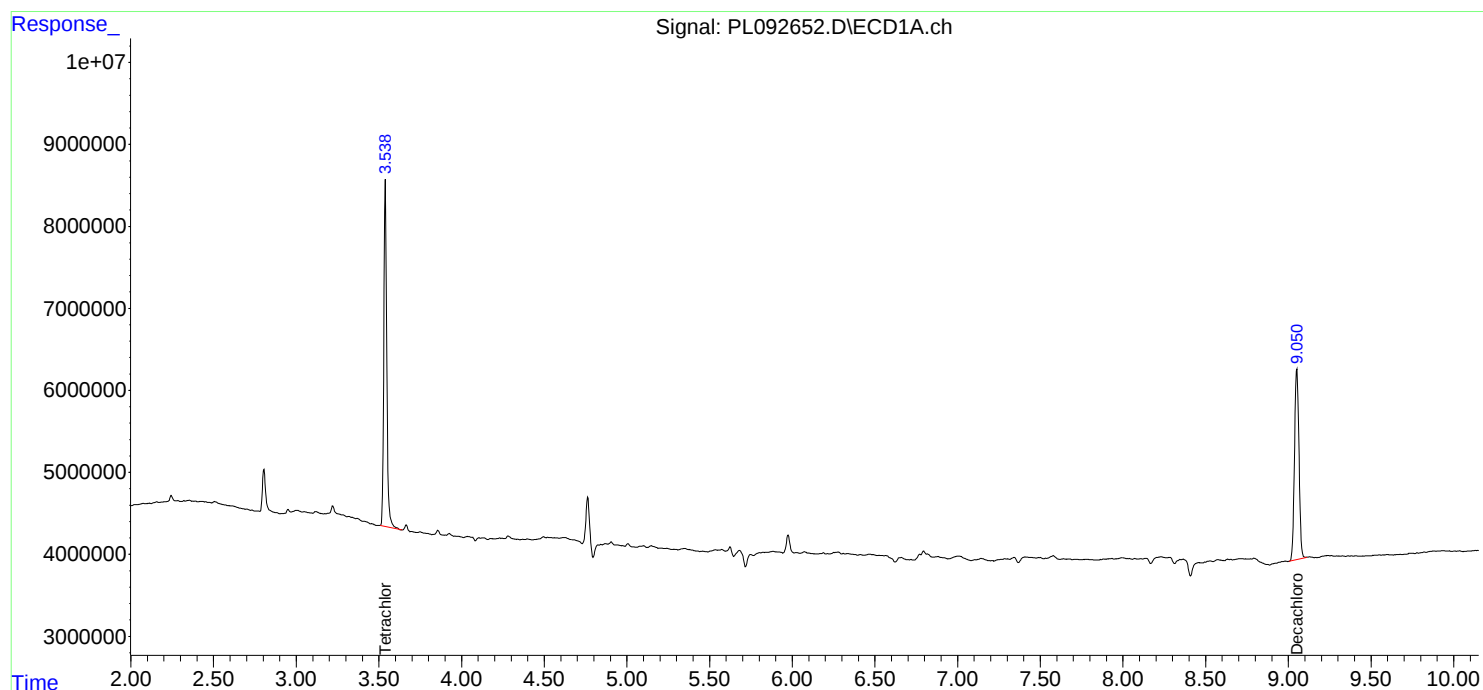


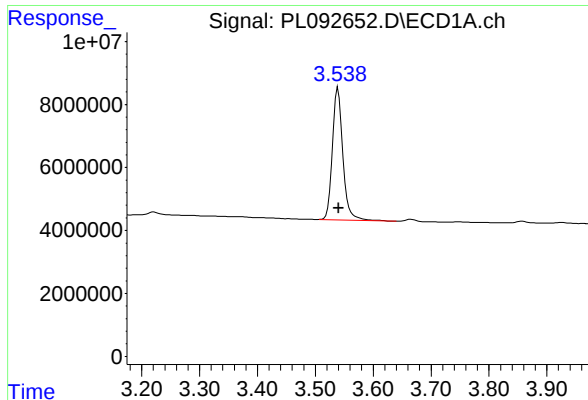

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 52846066
Conc: 21.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

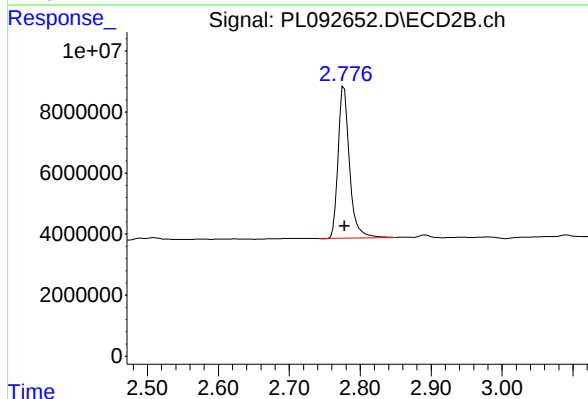


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 55504223
Conc: 20.40 ng/ml

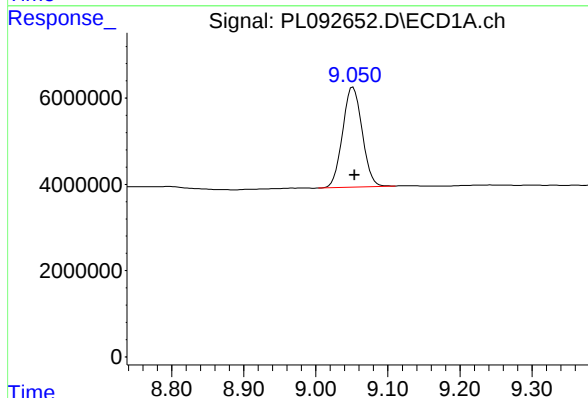

#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: -0.002 min
Response: 43705517
Conc: 22.71 ng/ml

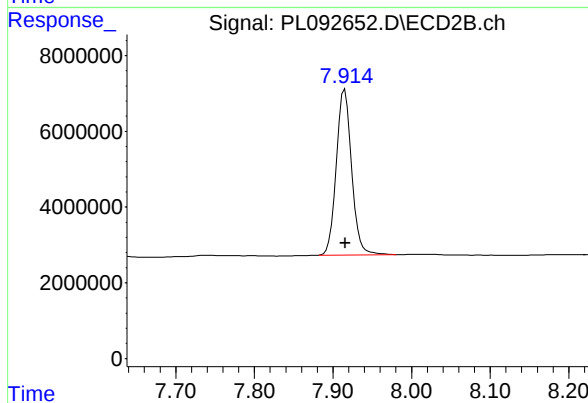

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 59287776
Conc: 21.72 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	10/29/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	10/29/24
Client Sample ID:	PIBLK-PL092693.D	SDG No.:	P4578
Lab Sample ID:	I.BLK-PL092693.D	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	TCLP Pesticide
GPC Factor :	1.0	PH :	
Prep Method :	3510C	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092693.D	1		10/29/24	PL102924

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.0049	U	0.0049	0.050	ug/L
76-44-8	Heptachlor	0.0054	U	0.0054	0.050	ug/L
1024-57-3	Heptachlor epoxide	0.0090	U	0.0090	0.050	ug/L
72-20-8	Endrin	0.0043	U	0.0043	0.050	ug/L
72-43-5	Methoxychlor	0.011	U	0.011	0.050	ug/L
8001-35-2	Toxaphene	0.15	U	0.15	1.00	ug/L
57-74-9	Chlordane	0.082	U	0.082	0.50	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	23.5		30 (43) - 150 (140)	118%	SPK: 20
877-09-8	Tetrachloro-m-xylene	22.4		30 (77) - 150 (126)	112%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 09:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 12:30:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.778	54928771	58388607	22.418	21.457
28) SA Decachlor...	9.055	7.915	44375064	64240872	23.057	23.538

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 09:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 12:30:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

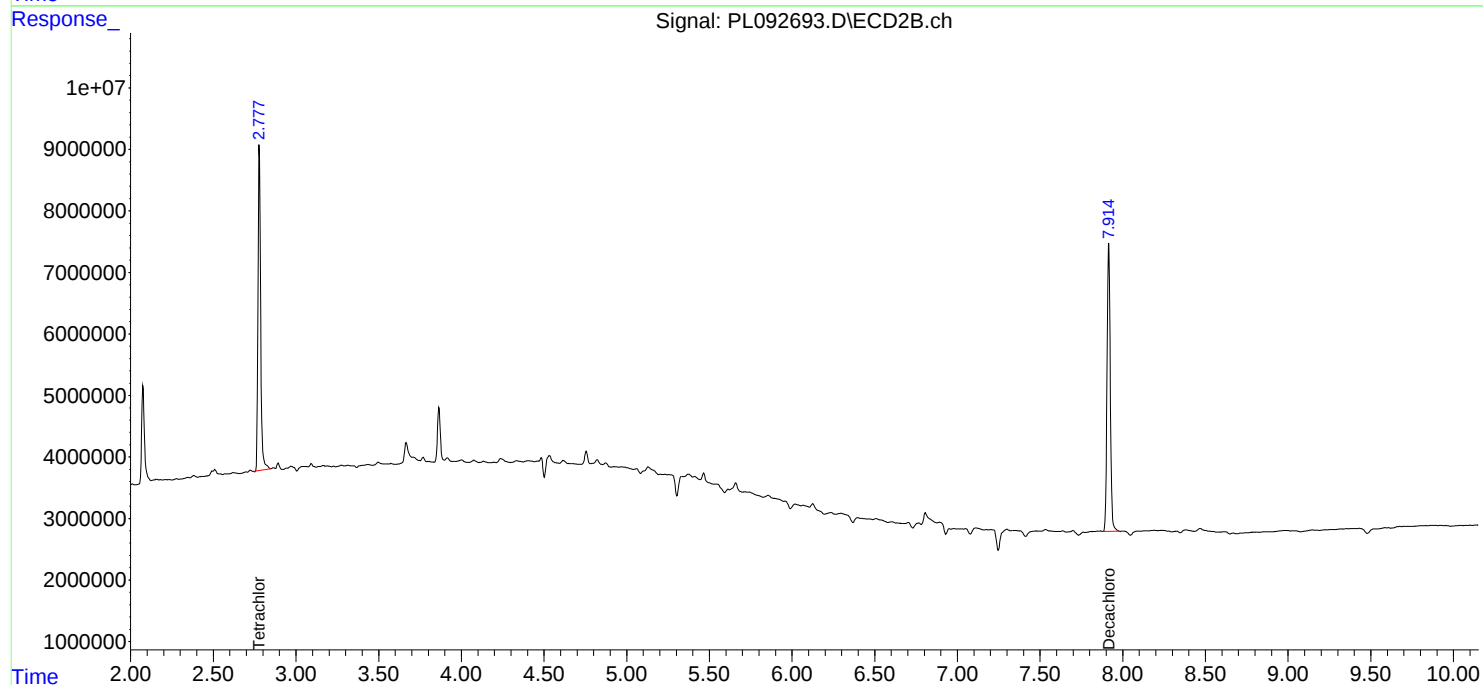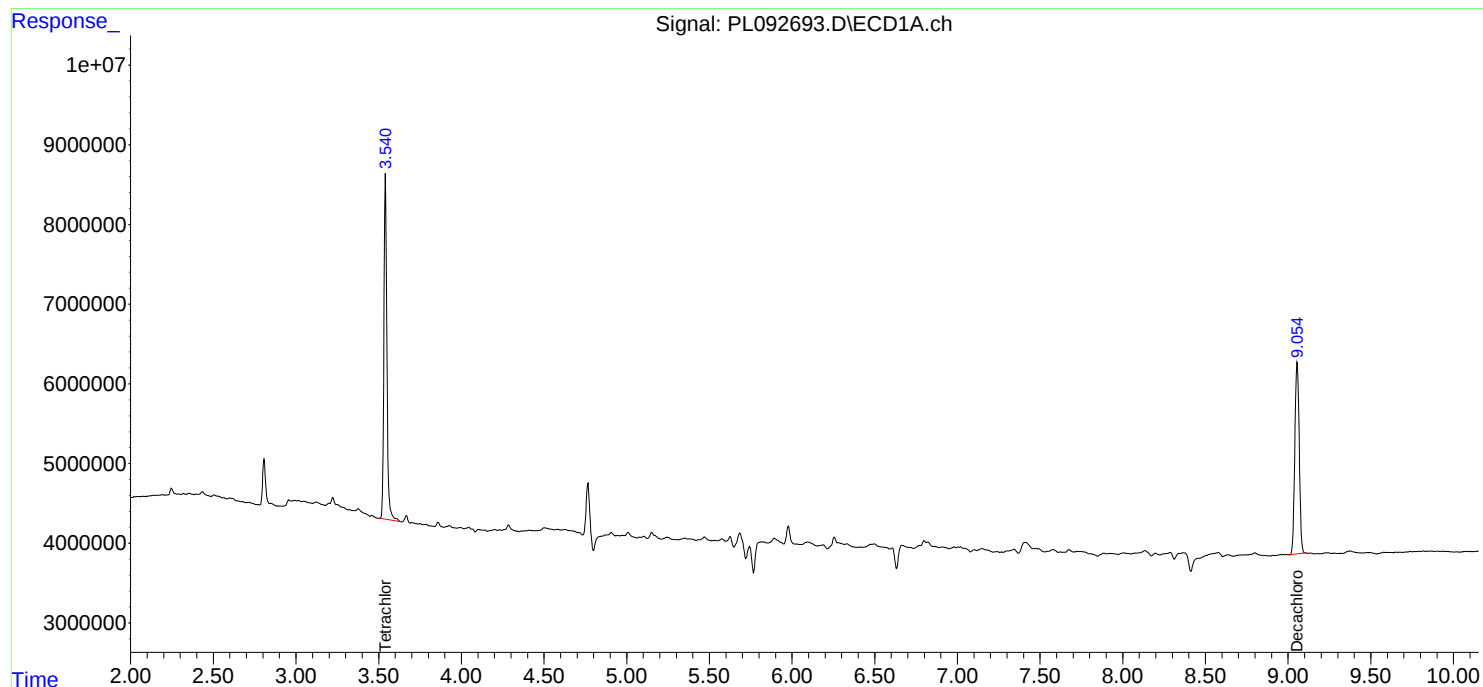


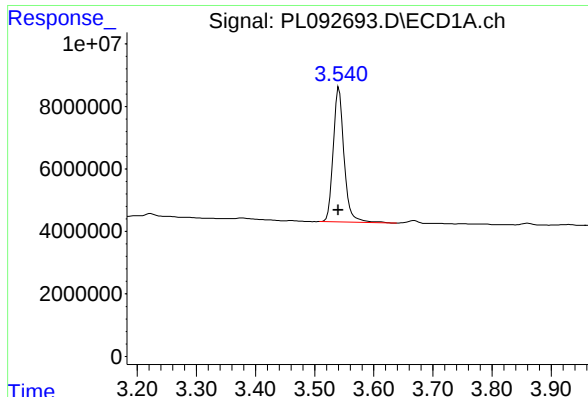

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.001 min
Response: 54928771
Conc: 22.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

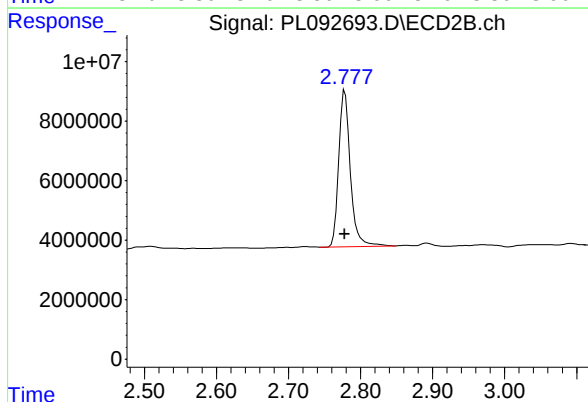


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 58388607
Conc: 21.46 ng/ml

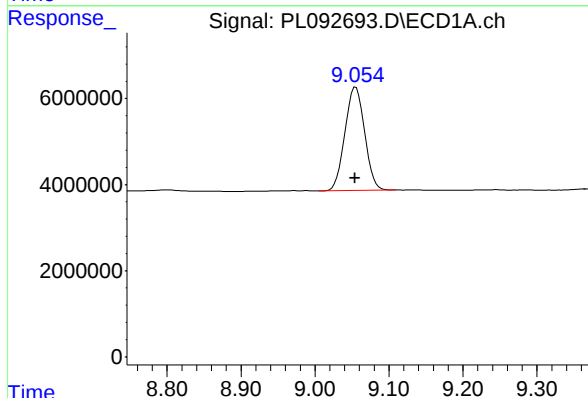

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.001 min
Response: 44375064
Conc: 23.06 ng/ml

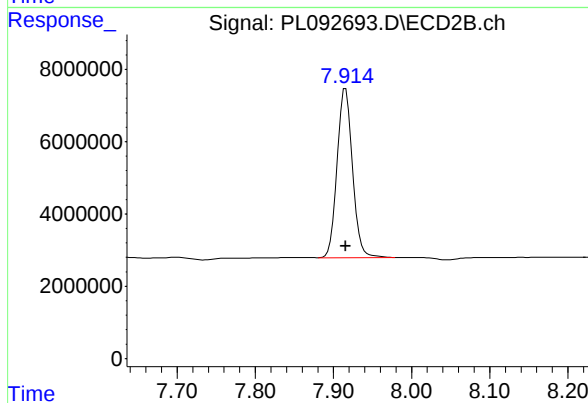

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.000 min
Response: 64240872
Conc: 23.54 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	10/29/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	10/29/24
Client Sample ID:	PIBLK-PL092710.D	SDG No.:	P4578
Lab Sample ID:	I.BLK-PL092710.D	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	TCLP Pesticide
GPC Factor :	1.0	PH :	
Prep Method :	3510C	Decanted:	
		Final Vol:	10000
		Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092710.D	1		10/29/24	PL102924

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.0049	U	0.0049	0.050	ug/L
76-44-8	Heptachlor	0.0054	U	0.0054	0.050	ug/L
1024-57-3	Heptachlor epoxide	0.0090	U	0.0090	0.050	ug/L
72-20-8	Endrin	0.0043	U	0.0043	0.050	ug/L
72-43-5	Methoxychlor	0.011	U	0.011	0.050	ug/L
8001-35-2	Toxaphene	0.15	U	0.15	1.00	ug/L
57-74-9	Chlordane	0.082	U	0.082	0.50	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	24.7		30 (43) - 150 (140)	124%	SPK: 20
877-09-8	Tetrachloro-m-xylene	23.1		30 (77) - 150 (126)	115%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 13:53
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/30/2024
 Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 00:50:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.776	56488345	61266481	23.054	22.515m
28) SA Decachlor...	9.054	7.916	45846928	67411967	23.822	24.700

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 13:53
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/30/2024
Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 00:50:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

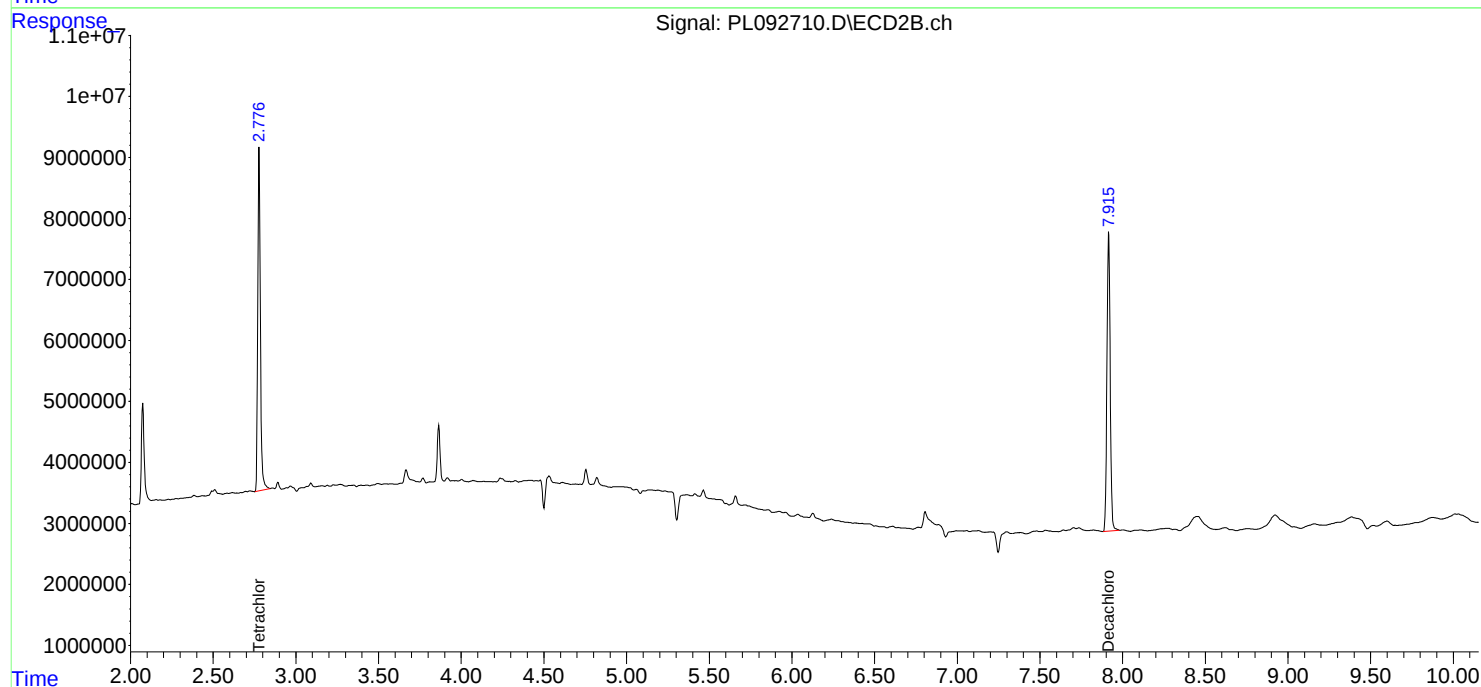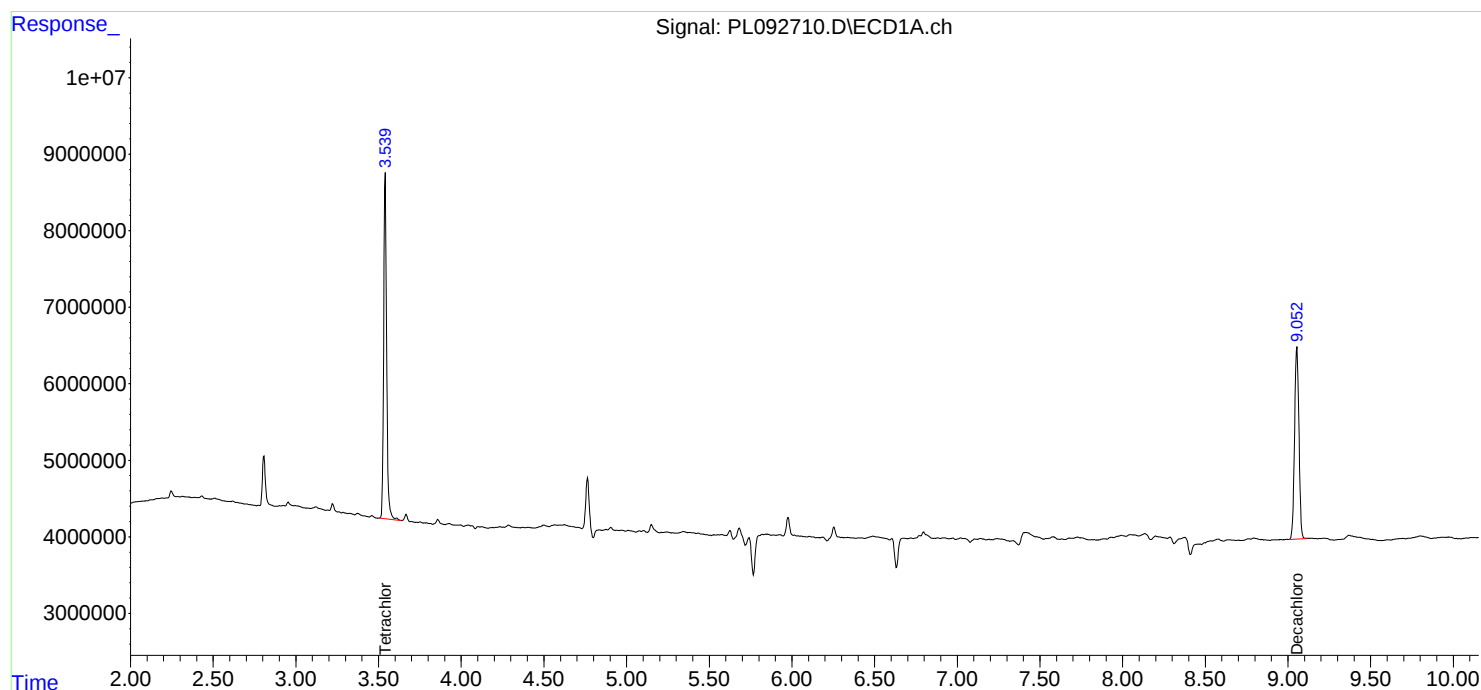

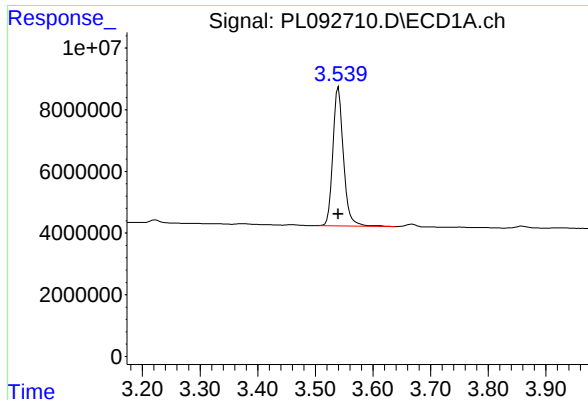


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 56488345
Conc: 23.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/30/2024
Supervised By :Ankita Jodhani 11/04/2024

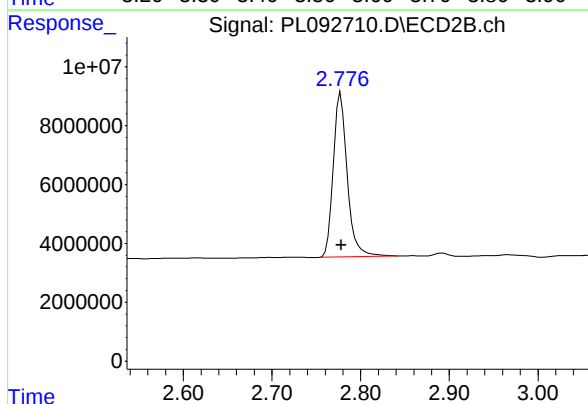


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: -0.002 min
Response: 61266481
Conc: 22.51 ng/ml m

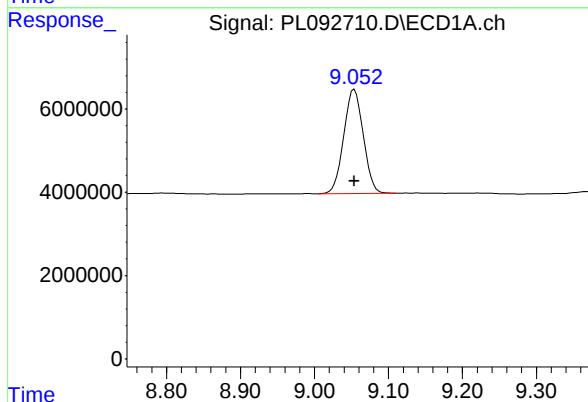

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 45846928
Conc: 23.82 ng/ml

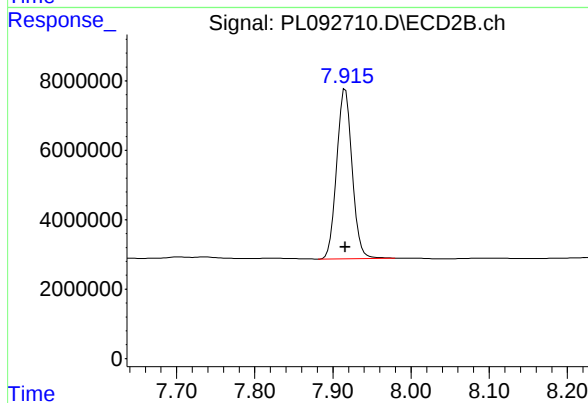

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 67411967
Conc: 24.70 ng/ml

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	
Client Sample ID:	PB164445BS	SDG No.:	P4578
Lab Sample ID:	PB164445BS	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	1000 uL
Soil Aliquot Vol:	uL	Test:	TCLP Pesticide
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092698.D	1	10/26/24 12:50	10/29/24 10:57	PB164445

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.048		0.00050	0.0050	ug/L
76-44-8	Heptachlor	0.050		0.00050	0.0050	ug/L
1024-57-3	Heptachlor epoxide	0.049		0.00090	0.0050	ug/L
72-20-8	Endrin	0.045		0.00040	0.0050	ug/L
72-43-5	Methoxychlor	0.045		0.0011	0.0050	ug/L
8001-35-2	Toxaphene	0.015	U	0.015	0.10	ug/L
57-74-9	Chlordane	0.0082	U	0.0082	0.050	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	19.5		30 (43) - 150 (140)	98%	SPK: 20
877-09-8	Tetrachloro-m-xylene	18.1		30 (77) - 150 (126)	91%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 10:57
 Operator : AR\AJ
 Sample : PB164445BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

PB164445BS

Manual Integrations**APPROVED**

Reviewed By :Abdul Mirza 10/30/2024

Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:10:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.779	44398574	46338942	18.120	17.029
28) SA Decachlor...	9.052	7.915	37613979	50150936	19.544	18.375
Target Compounds						
2) A alpha-BHC	3.996	3.281	158.7E6	194.5E6	46.784	48.740
3) MA gamma-BHC...	4.328	3.611	150.2E6	185.7E6	46.083	48.121
4) MA Heptachlor	4.917	3.950	142.6E6	186.7E6	47.468	49.469
5) MB Aldrin	5.258	4.230	136.4E6	176.7E6	45.446	48.269
6) B beta-BHC	4.526	3.911	69281571	81270375	47.930	49.367
7) B delta-BHC	4.772	4.140	130.4E6	163.0E6	41.673	42.424
8) B Heptachlo...	5.684	4.732	127.5E6	164.2E6	46.174	49.139
9) A Endosulfan I	6.069	5.101	118.0E6	154.4E6	47.176	50.581
10) B gamma-Chl...	5.940	4.982	127.9E6	170.1E6	48.086	50.595
11) B alpha-Chl...	6.019	5.045	126.6E6	167.4E6	47.824	50.332
12) B 4,4'-DDE	6.192	5.234	113.6E6	163.0E6	47.934	50.592
13) MA Dieldrin	6.344	5.366	124.6E6	166.8E6	47.265	49.938
14) MA Endrin	6.572	5.641	96671615	131.3E6	42.462m	45.370
15) B Endosulfa...	6.793	5.935	111.8E6	143.4E6	46.920	50.600
16) A 4,4'-DDD	6.709	5.789	95685802	129.8E6	49.849	52.139
17) MA 4,4'-DDT	7.023	6.039	97808774	124.6E6	47.256	46.449
18) B Endrin al...	6.924	6.115	90272597	113.7E6	48.069	49.263
19) B Endosulfa...	7.157	6.337	102.2E6	131.8E6	47.107	48.858
20) A Methoxychlor	7.498	6.614	51144756	64247709	44.864	44.990
21) B Endrin ke...	7.642	6.843	119.6E6	156.3E6	49.371	50.924
22) Mirex	8.116	7.023	82686920	107.6E6	41.725	41.256

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 10:57
Operator : AR\AJ
Sample : PB164445BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

PB164445BS

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 10/30/2024

Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:10:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

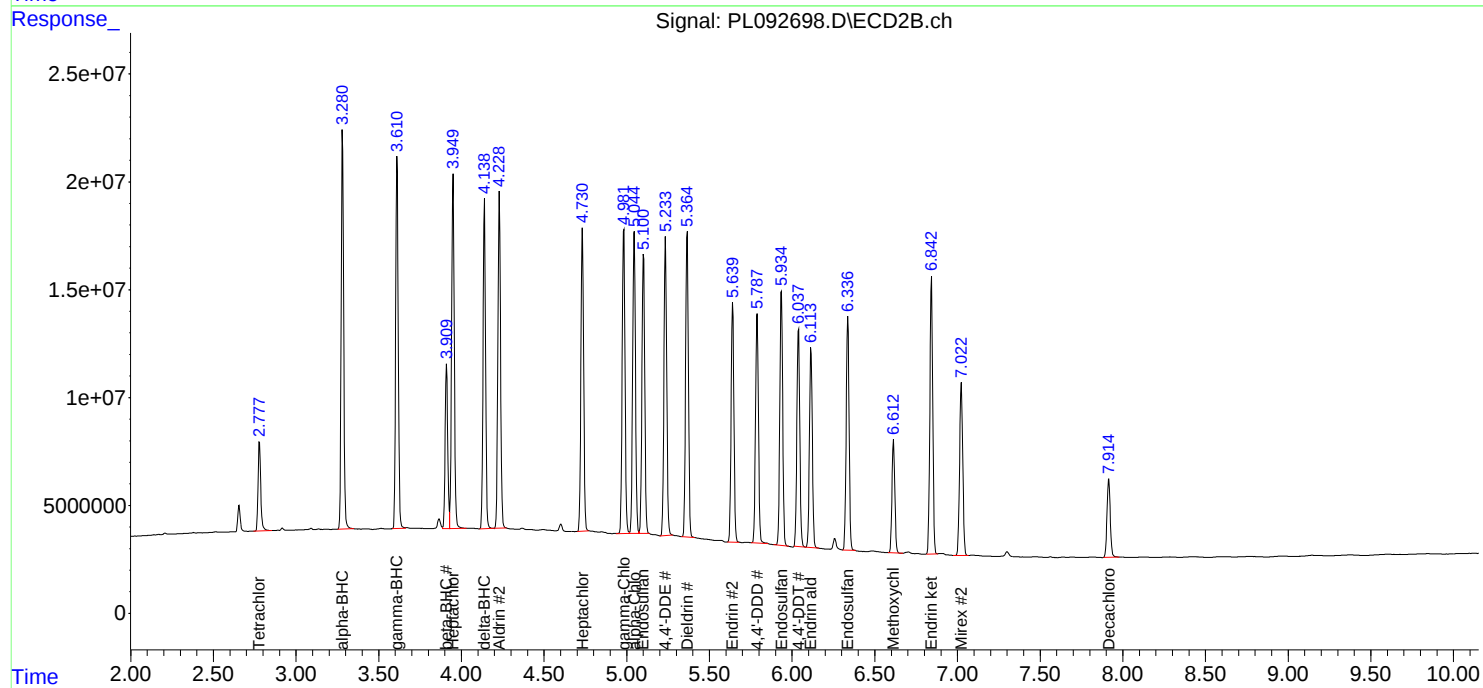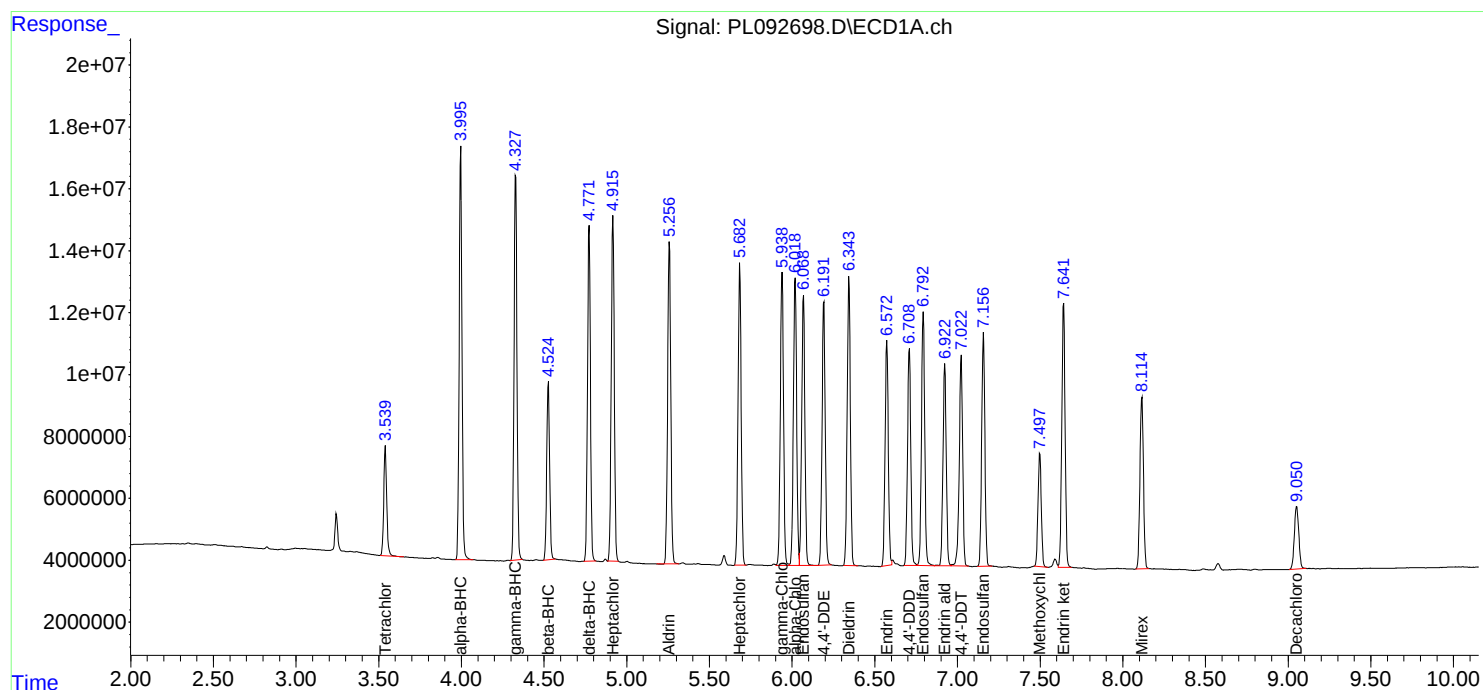

Report of Analysis

Client:	Portal Partners Tri-Venture		Date Collected:	10/25/24	
Project:	Amtrak Sawtooth Bridges 2024		Date Received:	10/25/24	
Client Sample ID:	WB-305-BOTMS		SDG No.:	P4578	
Lab Sample ID:	P4578-06MS		Matrix:	TCLP	
Analytical Method:	SW8081		% Solid:	0	Decanted:
Sample Wt/Vol:	100	Units: mL	Final Vol:	1000	uL
Soil Aliquot Vol:		uL	Test:	TCLP Pesticide	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092701.D	1	10/26/24 12:50	10/29/24 11:37	PB164445

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.46		0.0049	0.050	ug/L
76-44-8	Heptachlor	0.47		0.0054	0.050	ug/L
1024-57-3	Heptachlor epoxide	0.46		0.0090	0.050	ug/L
72-20-8	Endrin	0.47		0.0043	0.050	ug/L
72-43-5	Methoxychlor	0.46		0.011	0.050	ug/L
8001-35-2	Toxaphene	0.15	U	0.15	1.00	ug/L
57-74-9	Chlordane	0.082	U	0.082	0.50	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	15.9		30 (43) - 150 (140)	80%	SPK: 20
877-09-8	Tetrachloro-m-xylene	18.4		30 (77) - 150 (126)	92%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 11:37
 Operator : AR\AJ
 Sample : P4578-06MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

WB-305-BOTMS

Manual Integrations**APPROVED**

Reviewed By :Abdul Mirza 10/30/2024

Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:11:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.779	44424037	49979551	18.131m	18.367
28)	SA Decachlor...	9.051	7.914	30628503	42301014	15.915	15.499
Target Compounds							
2)	A alpha-BHC	3.996	3.281	153.9E6	186.8E6	45.382	46.808
3)	MA gamma-BHC...	4.327	3.611	142.0E6	178.1E6	43.574m	46.146
4)	MA Heptachlor	4.917	3.950	136.4E6	178.3E6	45.412	47.240
5)	MB Aldrin	5.257	4.230	127.5E6	170.2E6	42.472m	46.493
6)	B beta-BHC	4.526	3.910	65695763	77348574	45.450	46.985
7)	B delta-BHC	4.772	4.138	149.3E6	176.3E6	47.689	45.875m
8)	B Heptachlo...	5.684	4.732	121.3E6	155.0E6	43.929	46.395
9)	A Endosulfan I	6.070	5.101	111.9E6	145.0E6	44.740	47.499
10)	B gamma-Chl...	5.939	4.982	121.4E6	160.6E6	45.615m	47.784
11)	B alpha-Chl...	6.019	5.046	121.1E6	159.5E6	45.742	47.960
12)	B 4,4'-DDE	6.193	5.234	107.4E6	153.9E6	45.323	47.778
13)	MA Dieldrin	6.344	5.366	118.7E6	158.7E6	45.034	47.501
14)	MA Endrin	6.573	5.641	98574086	136.5E6	43.298m	47.200
15)	B Endosulfa...	6.794	5.935	105.7E6	136.5E6	44.354	48.170
16)	A 4,4'-DDD	6.709	5.789	89225698	121.2E6	46.483	48.663
17)	MA 4,4'-DDT	7.023	6.040	96273805	124.3E6	46.515	46.353
18)	B Endrin al...	6.923	6.115	79903787	102.0E6	42.548	44.206
19)	B Endosulfa...	7.158	6.338	97317956	128.2E6	44.840	47.535
20)	A Methoxychlor	7.497	6.615	50054958	65162857	43.908m	45.631
21)	B Endrin ke...	7.642	6.843	109.9E6	145.6E6	45.376	47.439
22)	Mirex	8.116	7.022	85813250	116.3E6	43.303	44.575m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 11:37
Operator : AR\AJ
Sample : P4578-06MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

WB-305-BOTMS

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 10/30/2024

Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:11:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

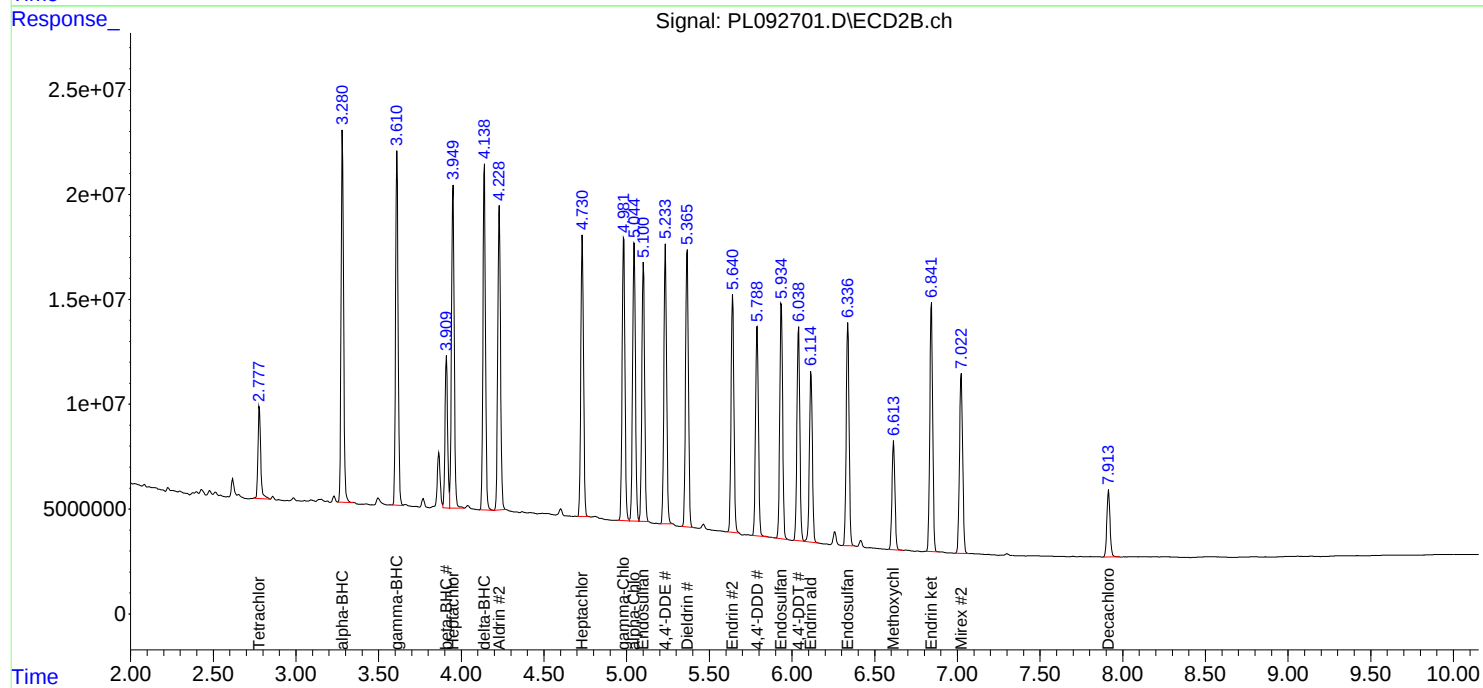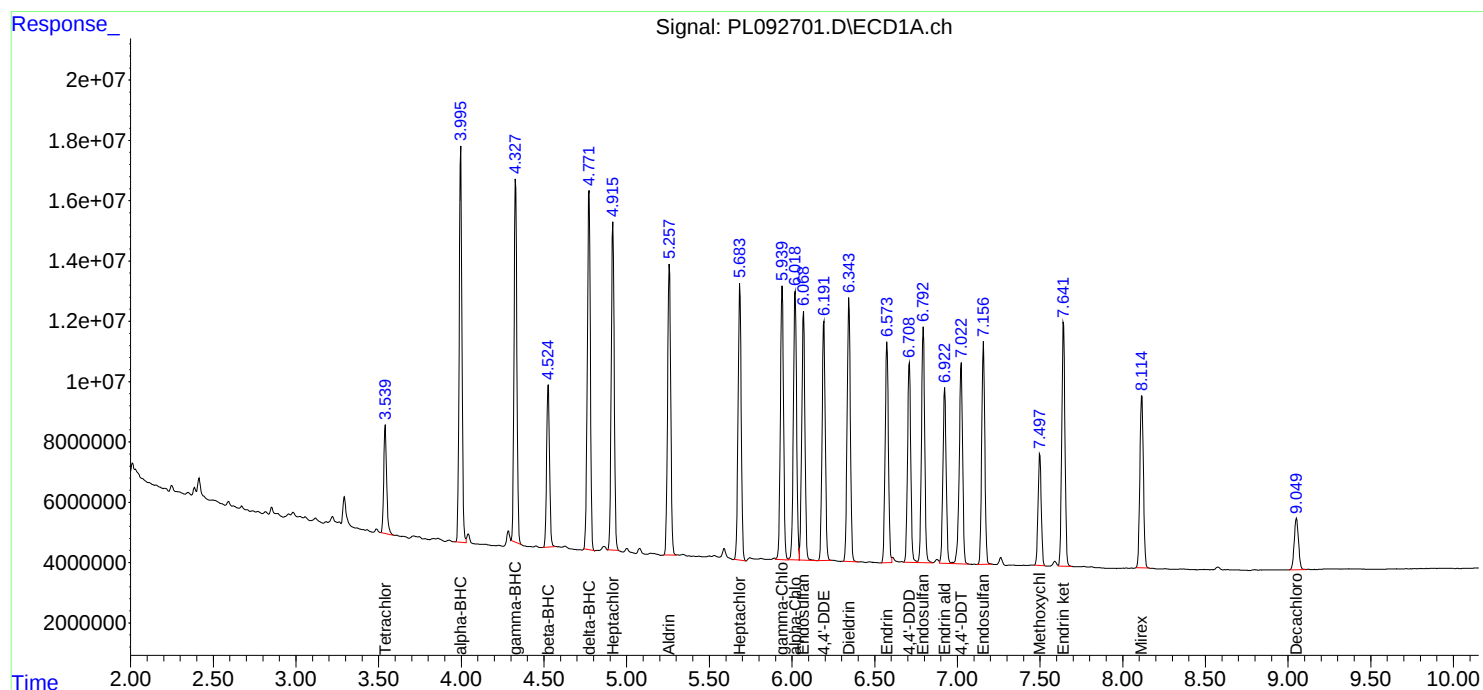

Report of Analysis

Client:	Portal Partners Tri-Venture	Date Collected:	10/25/24
Project:	Amtrak Sawtooth Bridges 2024	Date Received:	10/25/24
Client Sample ID:	WB-305-BOTMSD	SDG No.:	P4578
Lab Sample ID:	P4578-06MSD	Matrix:	TCLP
Analytical Method:	SW8081	% Solid:	0
Sample Wt/Vol:	100	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	TCLP Pesticide
GPC Factor :	1.0	PH :	
Prep Method :	3510C	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PL092702.D	1	10/26/24 12:50	10/29/24 11:50	PB164445

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
58-89-9	gamma-BHC (Lindane)	0.46		0.0049	0.050	ug/L
76-44-8	Heptachlor	0.47		0.0054	0.050	ug/L
1024-57-3	Heptachlor epoxide	0.46		0.0090	0.050	ug/L
72-20-8	Endrin	0.47		0.0043	0.050	ug/L
72-43-5	Methoxychlor	0.46		0.011	0.050	ug/L
8001-35-2	Toxaphene	0.15	U	0.15	1.00	ug/L
57-74-9	Chlordane	0.082	U	0.082	0.50	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	15.8		30 (43) - 150 (140)	79%	SPK: 20
877-09-8	Tetrachloro-m-xylene	18.4		30 (77) - 150 (126)	92%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
 Data File : PL092702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2024 11:50
 Operator : AR\AJ
 Sample : P4578-06MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WB-305-BOTMSD

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/30/2024
 Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 01:12:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.779	44037963	49951186	17.973m	18.357
28) SA Decachlor...	9.053	7.915	30303124	43134949	15.746	15.805
Target Compounds						
2) A alpha-BHC	3.996	3.281	152.8E6	187.0E6	45.060	46.869
3) MA gamma-BHC...	4.327	3.611	141.6E6	177.7E6	43.429m	46.043
4) MA Heptachlor	4.917	3.950	135.5E6	177.1E6	45.112	46.931
5) MB Aldrin	5.257	4.230	127.1E6	169.7E6	42.358m	46.357
6) B beta-BHC	4.526	3.910	65623061	77148090	45.399	46.863
7) B delta-BHC	4.773	4.139	149.3E6	175.2E6	47.698	45.591
8) B Heptachlo...	5.684	4.732	120.2E6	154.6E6	43.524	46.268
9) A Endosulfan I	6.070	5.102	111.4E6	143.2E6	44.545	46.892
10) B gamma-Chl...	5.939	4.982	120.6E6	160.3E6	45.329m	47.681
11) B alpha-Chl...	6.019	5.046	120.8E6	158.9E6	45.603	47.767
12) B 4,4'-DDE	6.192	5.235	106.5E6	152.4E6	44.940	47.297
13) MA Dieldrin	6.345	5.366	118.1E6	157.9E6	44.806	47.278
14) MA Endrin	6.573	5.641	98565833	135.1E6	43.294m	46.697
15) B Endosulfa...	6.794	5.936	104.7E6	136.5E6	43.938	48.185
16) A 4,4'-DDD	6.709	5.789	88486220	120.3E6	46.098	48.304
17) MA 4,4'-DDT	7.023	6.039	95657230	124.0E6	46.217	46.226
18) B Endrin al...	6.924	6.115	79416139	102.2E6	42.288	44.305
19) B Endosulfa...	7.158	6.338	96867761	127.3E6	44.632	47.208
20) A Methoxychlor	7.498	6.614	49721767	64973570	43.616	45.499
21) B Endrin ke...	7.643	6.843	109.8E6	146.8E6	45.304	47.848
22) Mirex	8.116	7.022	85444548	115.0E6	43.117	44.062m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102924\
Data File : PL092702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2024 11:50
Operator : AR\AJ
Sample : P4578-06MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

WB-305-BOTMSD



Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 10/30/2024
Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 01:12:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

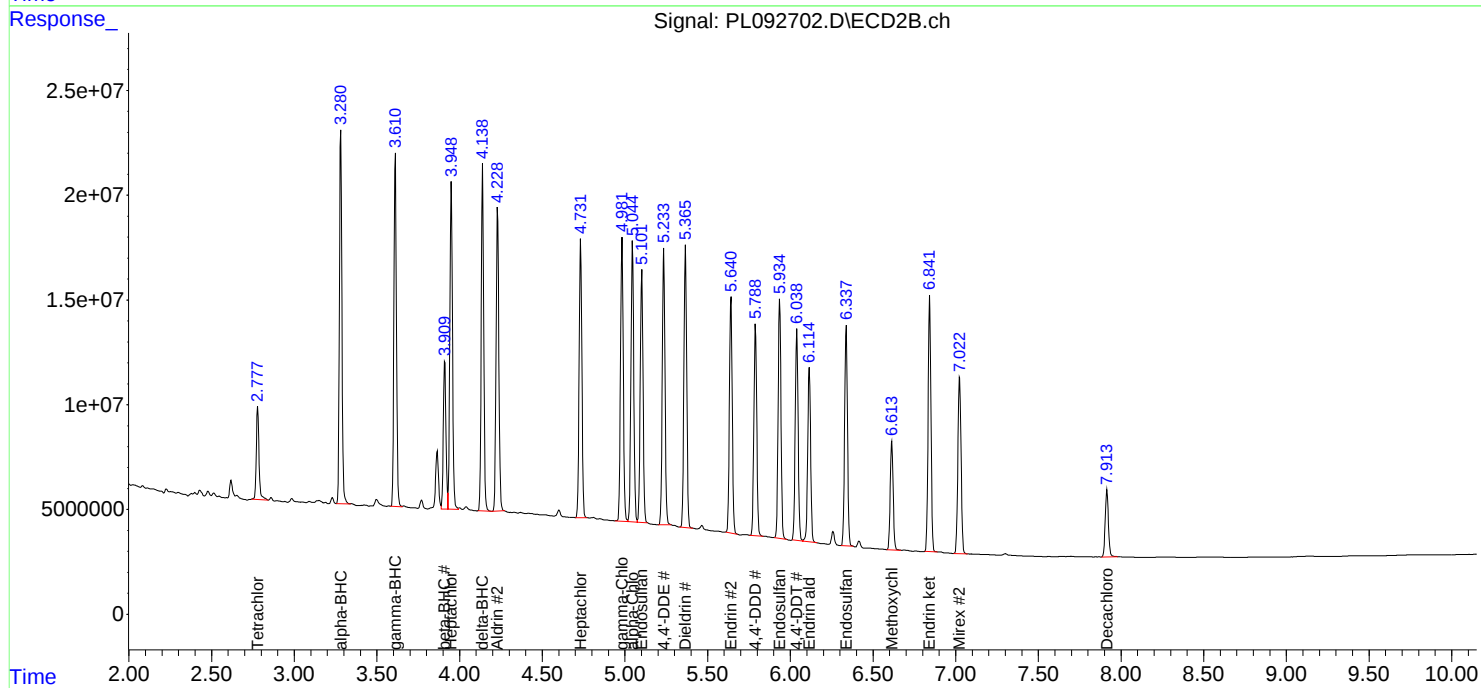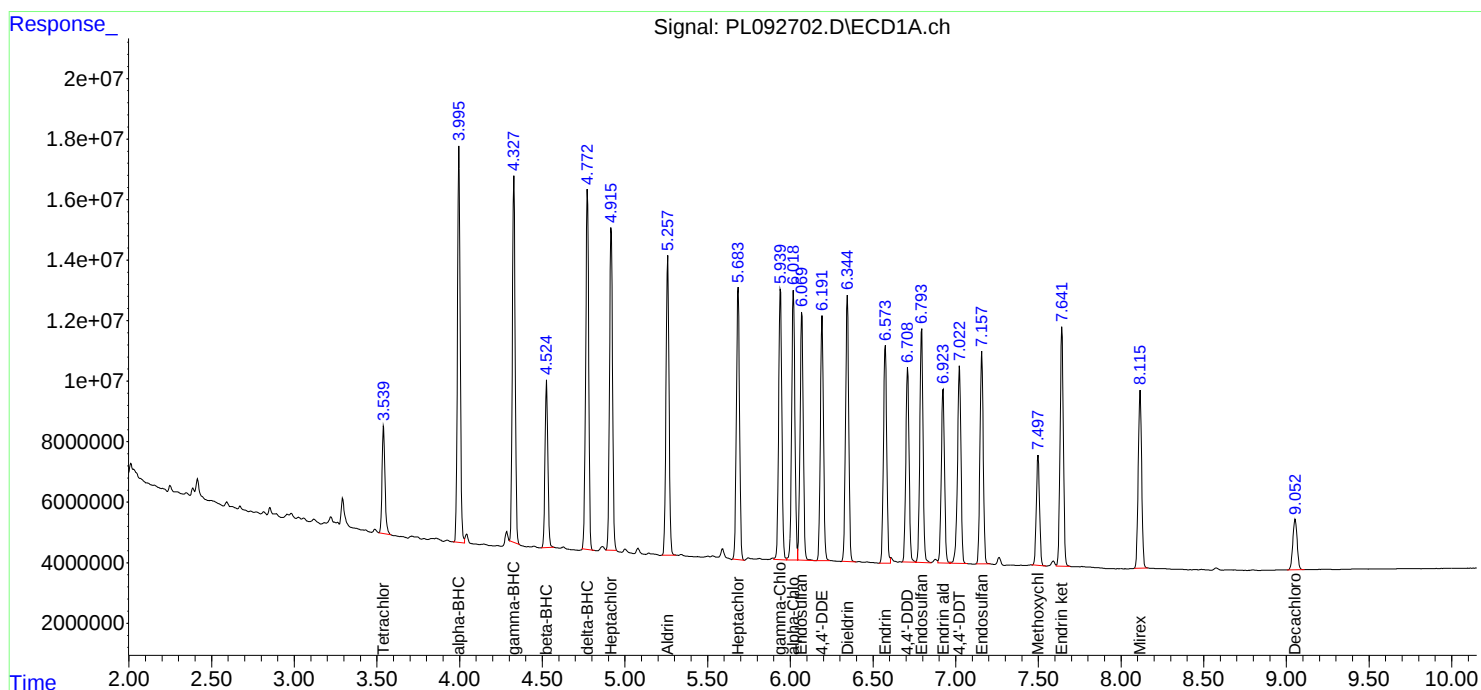

Manual Integration Report

Sequence:	PL102824	Instrument	ECD_I
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
PEM	PL092653.D	4,4"-DDD	Abdul	10/29/2024 9:08:09 AM	Ankita	10/29/2024 10:01:26	Peak Integrated by Software
PEM	PL092653.D	4,4"-DDD #2	Abdul	10/29/2024 9:08:09 AM	Ankita	10/29/2024 10:01:26	Peak Integrated by Software
PSTDICC005	PL092659.D	delta-BHC	Abdul	10/29/2024 9:08:13 AM	Ankita	10/29/2024 10:01:28	Peak Integrated by Software
PSTDICC005	PL092659.D	Heptachlor epoxide	Abdul	10/29/2024 9:08:13 AM	Ankita	10/29/2024 10:01:28	Peak Integrated by Software
PEM	PL092674.D	4,4"-DDD #2	Abdul	10/29/2024 9:08:21 AM	Ankita	10/29/2024 10:01:31	Peak Integrated by Software
PEM	PL092674.D	4,4"-DDE	Abdul	10/29/2024 9:08:21 AM	Ankita	10/29/2024 10:01:31	Peak Integrated by Software
PEM	PL092674.D	4,4"-DDE #2	Abdul	10/29/2024 9:08:21 AM	Ankita	10/29/2024 10:01:31	Peak Integrated by Software
PEM	PL092674.D	Endrin ketone #2	Abdul	10/29/2024 9:08:21 AM	Ankita	10/29/2024 10:01:31	Peak Integrated by Software
PSTDCCC050	PL092675.D	Aldrin	Abdul	10/29/2024 9:08:25 AM	Ankita	10/29/2024 10:01:33	Peak Integrated by Software
PSTDCCC050	PL092675.D	Dieldrin #2	Abdul	10/29/2024 9:08:25 AM	Ankita	10/29/2024 10:01:33	Peak Integrated by Software
PSTDCCC050	PL092675.D	gamma-BHC (Lindane)	Abdul	10/29/2024 9:08:25 AM	Ankita	10/29/2024 10:01:33	Peak Integrated by Software
PSTDCCC050	PL092675.D	Tetrachloro-m-xylene #2	Abdul	10/29/2024 9:08:25 AM	Ankita	10/29/2024 10:01:33	Peak Integrated by Software
I.BLK	PL092690.D	Tetrachloro-m-xylene #2	Abdul	10/29/2024 9:09:28 AM	Ankita	10/29/2024 10:02:09	Peak Integrated by Software

Manual Integration Report

Sequence:	PL102824	Instrument	ECD_I
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
PSTDCCC050	PL092691.D	Endosulfan II #2	Abdul	10/29/2024 9:09:32 AM	Ankita	10/29/2024 10:02:10	Peak Integrated by Software
PSTDCCC050	PL092691.D	gamma-Chlordane	Abdul	10/29/2024 9:09:32 AM	Ankita	10/29/2024 10:02:10	Peak Integrated by Software
PSTDCCC050	PL092691.D	Heptachlor epoxide	Abdul	10/29/2024 9:09:32 AM	Ankita	10/29/2024 10:02:10	Peak Integrated by Software
PSTDCCC050	PL092691.D	Mirex #2	Abdul	10/29/2024 9:09:32 AM	Ankita	10/29/2024 10:02:10	Peak Integrated by Software

Manual Integration Report

Sequence:	PL102924	Instrument	ECD_I
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
PB164445BS	PL092698.D	Endrin	Abdul	10/30/2024 3:35:03 PM	Ankita	11/4/2024 9:19:18	Peak Integrated by Software
P4578-06	PL092700.D	alpha-BHC	Abdul	10/30/2024 3:35:08 PM	Ankita	11/4/2024 9:19:19	Peak Integrated by Software
P4578-06MS	PL092701.D	Aldrin	Abdul	10/30/2024 3:35:12 PM	Ankita	11/4/2024 9:19:21	Peak Integrated by Software
P4578-06MS	PL092701.D	delta-BHC #2	Abdul	10/30/2024 3:35:12 PM	Ankita	11/4/2024 9:19:21	Peak Integrated by Software
P4578-06MS	PL092701.D	Endrin	Abdul	10/30/2024 3:35:12 PM	Ankita	11/4/2024 9:19:21	Peak Integrated by Software
P4578-06MS	PL092701.D	gamma-BHC (Lindane)	Abdul	10/30/2024 3:35:12 PM	Ankita	11/4/2024 9:19:21	Peak Integrated by Software
P4578-06MS	PL092701.D	gamma-Chlordane	Abdul	10/30/2024 3:35:12 PM	Ankita	11/4/2024 9:19:21	Peak Integrated by Software
P4578-06MS	PL092701.D	Methoxychlor	Abdul	10/30/2024 3:35:12 PM	Ankita	11/4/2024 9:19:21	Peak Integrated by Software
P4578-06MS	PL092701.D	Mirex #2	Abdul	10/30/2024 3:35:12 PM	Ankita	11/4/2024 9:19:21	Peak Integrated by Software
P4578-06MS	PL092701.D	Tetrachloro-m-xylene	Abdul	10/30/2024 3:35:12 PM	Ankita	11/4/2024 9:19:21	Peak Integrated by Software
P4578-06MSD	PL092702.D	Aldrin	Abdul	10/30/2024 3:35:16 PM	Ankita	11/4/2024 9:19:23	Peak Integrated by Software
P4578-06MSD	PL092702.D	Endrin	Abdul	10/30/2024 3:35:16 PM	Ankita	11/4/2024 9:19:23	Peak Integrated by Software
P4578-06MSD	PL092702.D	gamma-BHC (Lindane)	Abdul	10/30/2024 3:35:16 PM	Ankita	11/4/2024 9:19:23	Peak Integrated by Software

Manual Integration Report

Sequence:

PL102924

Instrument

ECD_I

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
P4578-06MSD	PL092702.D	gamma-Chlordane	Abdul	10/30/2024 3:35:16 PM	Ankita	11/4/2024 9:19:23	Peak Integrated by Software
P4578-06MSD	PL092702.D	Mirex #2	Abdul	10/30/2024 3:35:16 PM	Ankita	11/4/2024 9:19:23	Peak Integrated by Software
P4578-06MSD	PL092702.D	Tetrachloro-m-xylene	Abdul	10/30/2024 3:35:16 PM	Ankita	11/4/2024 9:19:23	Peak Integrated by Software
P4578-08	PL092703.D	Tetrachloro-m-xylene	Abdul	10/30/2024 3:35:21 PM	Ankita	11/4/2024 9:19:25	Peak Integrated by Software
I.BLK	PL092710.D	Tetrachloro-m-xylene #2	Abdul	10/30/2024 3:35:50 PM	Ankita	11/4/2024 9:19:34	Peak Integrated by Software
PSTDCCC050	PL092711.D	Aldrin	Abdul	10/30/2024 3:35:54 PM	Ankita	11/4/2024 9:19:35	Peak Integrated by Software
PSTDCCC050	PL092711.D	Endosulfan II #2	Abdul	10/30/2024 3:35:54 PM	Ankita	11/4/2024 9:19:35	Peak Integrated by Software
PSTDCCC050	PL092711.D	Mirex #2	Abdul	10/30/2024 3:35:54 PM	Ankita	11/4/2024 9:19:35	Peak Integrated by Software
I.BLK	PL092722.D	Decachlorobiphenyl	Abdul	10/30/2024 3:37:14 PM	Ankita	11/4/2024 9:20:12	Peak Integrated by Software
I.BLK	PL092722.D	Tetrachloro-m-xylene #2	Abdul	10/30/2024 3:37:14 PM	Ankita	11/4/2024 9:20:12	Peak Integrated by Software
PSTDCCC050	PL092723.D	4,4"-DDE #2	Abdul	10/30/2024 3:37:17 PM	Ankita	11/4/2024 9:20:13	Peak Integrated by Software
PSTDCCC050	PL092723.D	Aldrin	Abdul	10/30/2024 3:37:17 PM	Ankita	11/4/2024 9:20:13	Peak Integrated by Software
PSTDCCC050	PL092723.D	Endosulfan II #2	Abdul	10/30/2024 3:37:17 PM	Ankita	11/4/2024 9:20:13	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

PL102924

Instrument

ECD_I

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
PSTDCCC050	PL092723.D	Heptachlor	Abdul	10/30/2024 3:37:17 PM	Ankita	11/4/2024 9:20:13	Peak Integrated by Software
PSTDCCC050	PL092723.D	Heptachlor epoxide	Abdul	10/30/2024 3:37:17 PM	Ankita	11/4/2024 9:20:13	Peak Integrated by Software

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102824

Review By	Abdul	Review On	10/29/2024 9:09:59 AM
Supervise By	Ankita	Supervise On	10/29/2024 10:02:30 AM
SubDirectory	PL102824	HP Acquire Method	HP Processing Method pl102824 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP23793,PP23517		
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683		
CCC	PP23686,PP23690,PP23695		
Internal Standard/PEM			
ICV/I.BLK	PP23687,PP23693,PP23698		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PL092651.D	28 Oct 2024 13:41	AR\AJ	Ok
2	I.BLK	PL092652.D	28 Oct 2024 13:55	AR\AJ	Ok
3	PEM	PL092653.D	28 Oct 2024 14:16	AR\AJ	Ok,M
4	RESCHK	PL092654.D	28 Oct 2024 14:29	AR\AJ	Ok
5	PSTDICC100	PL092655.D	28 Oct 2024 14:43	AR\AJ	Ok
6	PSTDICC075	PL092656.D	28 Oct 2024 14:56	AR\AJ	Ok
7	PSTDICC050	PL092657.D	28 Oct 2024 15:09	AR\AJ	Ok
8	PSTDICC025	PL092658.D	28 Oct 2024 15:23	AR\AJ	Ok
9	PSTDICC005	PL092659.D	28 Oct 2024 15:36	AR\AJ	Ok,M
10	PCHLORICC1000	PL092660.D	28 Oct 2024 15:49	AR\AJ	Ok
11	PCHLORICC750	PL092661.D	28 Oct 2024 16:03	AR\AJ	Ok
12	PCHLORICC500	PL092662.D	28 Oct 2024 16:16	AR\AJ	Ok
13	PCHLORICC250	PL092663.D	28 Oct 2024 16:30	AR\AJ	Ok
14	PCHLORICC050	PL092664.D	28 Oct 2024 16:43	AR\AJ	Ok
15	PTOXICC1000	PL092665.D	28 Oct 2024 16:56	AR\AJ	Ok
16	PTOXICC750	PL092666.D	28 Oct 2024 17:10	AR\AJ	Ok
17	PTOXICC500	PL092667.D	28 Oct 2024 17:23	AR\AJ	Ok
18	PTOXICC250	PL092668.D	28 Oct 2024 17:37	AR\AJ	Ok
19	PTOXICC100	PL092669.D	28 Oct 2024 17:50	AR\AJ	Ok,M
20	PSTDICV050	PL092670.D	28 Oct 2024 18:03	AR\AJ	Ok
21	PCHLORICV500	PL092671.D	28 Oct 2024 18:30	AR\AJ	Ok

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102824

Review By	Abdul	Review On	10/29/2024 9:09:59 AM
Supervise By	Ankita	Supervise On	10/29/2024 10:02:30 AM
SubDirectory	PL102824	HP Acquire Method	HP Processing Method pl102824 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP23793,PP23517		
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683		
CCC	PP23686,PP23690,PP23695		
Internal Standard/PEM			
ICV/I.BLK	PP23687,PP23693,PP23698		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	PTOXICV500	PL092672.D	28 Oct 2024 18:57	AR\AJ	Ok
23	I.BLK	PL092673.D	28 Oct 2024 19:24	AR\AJ	Ok
24	PEM	PL092674.D	28 Oct 2024 19:37	AR\AJ	Ok,M
25	PSTDCCC050	PL092675.D	28 Oct 2024 19:51	AR\AJ	Ok,M
26	PB164460BL	PL092676.D	28 Oct 2024 20:04	AR\AJ	Ok,M
27	PB164460BS	PL092677.D	28 Oct 2024 20:17	AR\AJ	Ok,M
28	P4575-01	PL092678.D	28 Oct 2024 20:31	AR\AJ	Ok,M
29	P4566-01	PL092679.D	28 Oct 2024 20:44	AR\AJ	Ok,M
30	P4567-01	PL092680.D	28 Oct 2024 20:57	AR\AJ	Ok,M
31	P4567-05	PL092681.D	28 Oct 2024 21:11	AR\AJ	Ok
32	P4567-09	PL092682.D	28 Oct 2024 21:24	AR\AJ	Ok,M
33	P4574-01	PL092683.D	28 Oct 2024 21:38	AR\AJ	Ok,M
34	P4574-04	PL092684.D	28 Oct 2024 21:51	AR\AJ	Ok,M
35	P4577-01	PL092685.D	28 Oct 2024 22:04	AR\AJ	Ok,M
36	P4561-01	PL092686.D	28 Oct 2024 22:18	AR\AJ	Ok,M
37	P4561-01MS	PL092687.D	28 Oct 2024 22:31	AR\AJ	Ok,M
38	P4561-01MSD	PL092688.D	28 Oct 2024 22:44	AR\AJ	Ok,M
39	P4561-05	PL092689.D	28 Oct 2024 22:58	AR\AJ	Ok,M
40	I.BLK	PL092690.D	28 Oct 2024 23:11	AR\AJ	Ok,M
41	PSTDCCC050	PL092691.D	29 Oct 2024 00:32	AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102924

Review By	Abdul	Review On	10/30/2024 3:38:50 PM
Supervise By	Ankita	Supervise On	11/4/2024 9:20:27 AM
SubDirectory	PL102924	HP Acquire Method	HP Processing Method pl102824 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP23793,PP23517		
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683		
CCC	PP23686,PP23690,PP23695		
Internal Standard/PEM			
ICV/I.BLK	PP23687,PP23693,PP23698		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PL092692.D	29 Oct 2024 09:35	AR\AJ	Ok
2	I.BLK	PL092693.D	29 Oct 2024 09:48	AR\AJ	Ok
3	PEM	PL092694.D	29 Oct 2024 10:02	AR\AJ	Ok
4	PSTDCCC050	PL092695.D	29 Oct 2024 10:15	AR\AJ	Ok
5	P4545-01RE	PL092696.D	29 Oct 2024 10:30	AR\AJ	Confirms
6	PB164445BL	PL092697.D	29 Oct 2024 10:43	AR\AJ	Ok
7	PB164445BS	PL092698.D	29 Oct 2024 10:57	AR\AJ	Ok,M
8	PB164393TB	PL092699.D	29 Oct 2024 11:10	AR\AJ	Ok
9	P4578-06	PL092700.D	29 Oct 2024 11:23	AR\AJ	Ok,M
10	P4578-06MS	PL092701.D	29 Oct 2024 11:37	AR\AJ	Ok,M
11	P4578-06MSD	PL092702.D	29 Oct 2024 11:50	AR\AJ	Ok,M
12	P4578-08	PL092703.D	29 Oct 2024 12:04	AR\AJ	Ok,M
13	PB164496BL	PL092704.D	29 Oct 2024 12:17	AR\AJ	Ok
14	PB164496BS	PL092705.D	29 Oct 2024 12:30	AR\AJ	Ok,M
15	P4597-01	PL092706.D	29 Oct 2024 12:58	AR\AJ	Ok,M
16	P4597-04	PL092707.D	29 Oct 2024 13:12	AR\AJ	Ok,M
17	P4597-07	PL092708.D	29 Oct 2024 13:26	AR\AJ	Ok,M
18	P4597-10	PL092709.D	29 Oct 2024 13:39	AR\AJ	Ok,M
19	I.BLK	PL092710.D	29 Oct 2024 13:53	AR\AJ	Ok,M
20	PSTDCCC050	PL092711.D	29 Oct 2024 14:07	AR\AJ	Ok,M
21	P4594-01	PL092712.D	29 Oct 2024 14:21	AR\AJ	Ok,M

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102924

Review By	Abdul	Review On	10/30/2024 3:38:50 PM
Supervise By	Ankita	Supervise On	11/4/2024 9:20:27 AM
SubDirectory	PL102924	HP Acquire Method	HP Processing Method pl102824 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP23793,PP23517		
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683		
CCC	PP23686,PP23690,PP23695		
Internal Standard/PEM			
ICV/I.BLK	PP23687,PP23693,PP23698		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	P4594-01MS	PL092713.D	29 Oct 2024 14:35	AR\AJ	Ok,M
23	P4594-01MSD	PL092714.D	29 Oct 2024 14:49	AR\AJ	Ok,M
24	P4594-05	PL092715.D	29 Oct 2024 15:02	AR\AJ	Ok,M
25	P4594-09	PL092716.D	29 Oct 2024 15:16	AR\AJ	Ok,M
26	P4594-13	PL092717.D	29 Oct 2024 15:30	AR\AJ	Ok,M
27	P4594-17	PL092718.D	29 Oct 2024 15:44	AR\AJ	Ok,M
28	P4598-01	PL092719.D	29 Oct 2024 15:58	AR\AJ	Ok,M
29	P4598-05	PL092720.D	29 Oct 2024 16:11	AR\AJ	Ok,M
30	P4598-09	PL092721.D	29 Oct 2024 16:25	AR\AJ	Ok,M
31	I.BLK	PL092722.D	29 Oct 2024 16:39	AR\AJ	Ok,M
32	PSTDCCC050	PL092723.D	29 Oct 2024 16:53	AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102824

Review By	Abdul	Review On	10/29/2024 9:09:59 AM
Supervise By	Ankita	Supervise On	10/29/2024 10:02:30 AM
SubDirectory	PL102824	HP Acquire Method	HP Processing Method pl102824 8081

STD. NAME	STD REF.#
Tune/Reschk	PP23793,PP23517
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683
CCC	PP23686,PP23690,PP23695
Internal Standard/PEM	
ICV/I.BLK	PP23687,PP23693,PP23698
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PL092651.D	28 Oct 2024 13:41		AR\AJ	Ok
2	I.BLK	I.BLK	PL092652.D	28 Oct 2024 13:55		AR\AJ	Ok
3	PEM	PEM	PL092653.D	28 Oct 2024 14:16		AR\AJ	Ok,M
4	RESCHK	RESCHK	PL092654.D	28 Oct 2024 14:29		AR\AJ	Ok
5	PSTDICC100	PSTDICC100	PL092655.D	28 Oct 2024 14:43		AR\AJ	Ok
6	PSTDICC075	PSTDICC075	PL092656.D	28 Oct 2024 14:56		AR\AJ	Ok
7	PSTDICC050	PSTDICC050	PL092657.D	28 Oct 2024 15:09		AR\AJ	Ok
8	PSTDICC025	PSTDICC025	PL092658.D	28 Oct 2024 15:23		AR\AJ	Ok
9	PSTDICC005	PSTDICC005	PL092659.D	28 Oct 2024 15:36		AR\AJ	Ok,M
10	PCHLORICC1000	PCHLORICC1000	PL092660.D	28 Oct 2024 15:49		AR\AJ	Ok
11	PCHLORICC750	PCHLORICC750	PL092661.D	28 Oct 2024 16:03		AR\AJ	Ok
12	PCHLORICC500	PCHLORICC500	PL092662.D	28 Oct 2024 16:16		AR\AJ	Ok
13	PCHLORICC250	PCHLORICC250	PL092663.D	28 Oct 2024 16:30		AR\AJ	Ok
14	PCHLORICC050	PCHLORICC050	PL092664.D	28 Oct 2024 16:43		AR\AJ	Ok
15	PTOXICC1000	PTOXICC1000	PL092665.D	28 Oct 2024 16:56		AR\AJ	Ok
16	PTOXICC750	PTOXICC750	PL092666.D	28 Oct 2024 17:10		AR\AJ	Ok
17	PTOXICC500	PTOXICC500	PL092667.D	28 Oct 2024 17:23		AR\AJ	Ok
18	PTOXICC250	PTOXICC250	PL092668.D	28 Oct 2024 17:37		AR\AJ	Ok

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102824

Review By	Abdul	Review On	10/29/2024 9:09:59 AM
Supervise By	Ankita	Supervise On	10/29/2024 10:02:30 AM
SubDirectory	PL102824	HP Acquire Method	HP Processing Method
			pl102824 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP23793,PP23517		
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683		
CCC	PP23686,PP23690,PP23695		
Internal Standard/PEM			
ICV/I.BLK	PP23687,PP23693,PP23698		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	PTOXICC100	PTOXICC100	PL092669.D	28 Oct 2024 17:50		AR\AJ	Ok,M
20	PSTDICV050	ICVPL102824	PL092670.D	28 Oct 2024 18:03		AR\AJ	Ok
21	PCHLORICV500	ICVPL102824CHLOR	PL092671.D	28 Oct 2024 18:30		AR\AJ	Ok
22	PTOXICV500	ICVPL102824TOX	PL092672.D	28 Oct 2024 18:57		AR\AJ	Ok
23	I.BLK	I.BLK	PL092673.D	28 Oct 2024 19:24		AR\AJ	Ok
24	PEM	PEM	PL092674.D	28 Oct 2024 19:37		AR\AJ	Ok,M
25	PSTDCCC050	PSTDCCC050	PL092675.D	28 Oct 2024 19:51		AR\AJ	Ok,M
26	PB164460BL	PB164460BL	PL092676.D	28 Oct 2024 20:04		AR\AJ	Ok,M
27	PB164460BS	PB164460BS	PL092677.D	28 Oct 2024 20:17		AR\AJ	Ok,M
28	P4575-01	PL-02-102424	PL092678.D	28 Oct 2024 20:31		AR\AJ	Ok,M
29	P4566-01	HD-01-102524	PL092679.D	28 Oct 2024 20:44		AR\AJ	Ok,M
30	P4567-01	WC-1	PL092680.D	28 Oct 2024 20:57		AR\AJ	Ok,M
31	P4567-05	WC-2	PL092681.D	28 Oct 2024 21:11		AR\AJ	Ok
32	P4567-09	WC-3	PL092682.D	28 Oct 2024 21:24		AR\AJ	Ok,M
33	P4574-01	GRAVEL-1	PL092683.D	28 Oct 2024 21:38		AR\AJ	Ok,M
34	P4574-04	GRAVEL-2	PL092684.D	28 Oct 2024 21:51		AR\AJ	Ok,M
35	P4577-01	TR-05-102524	PL092685.D	28 Oct 2024 22:04		AR\AJ	Ok,M
36	P4561-01	BP-F-19	PL092686.D	28 Oct 2024 22:18		AR\AJ	Ok,M
37	P4561-01MS	BP-F-19MS	PL092687.D	28 Oct 2024 22:31		AR\AJ	Ok,M

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102824

Review By	Abdul	Review On	10/29/2024 9:09:59 AM
Supervise By	Ankita	Supervise On	10/29/2024 10:02:30 AM
SubDirectory	PL102824	HP Acquire Method	HP Processing Method pl102824 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP23793,PP23517		
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683		
CCC	PP23686,PP23690,PP23695		
Internal Standard/PEM			
ICV/I.BLK	PP23687,PP23693,PP23698		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	P4561-01MSD	BP-F-19MSD	PL092688.D	28 Oct 2024 22:44		AR\AJ	Ok,M
39	P4561-05	BP-F-18	PL092689.D	28 Oct 2024 22:58		AR\AJ	Ok,M
40	I.BLK	I.BLK	PL092690.D	28 Oct 2024 23:11		AR\AJ	Ok,M
41	PSTDCCC050	PSTDCCC050	PL092691.D	29 Oct 2024 00:32		AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102924

Review By	Abdul	Review On	10/30/2024 3:38:50 PM
Supervise By	Ankita	Supervise On	11/4/2024 9:20:27 AM
SubDirectory	PL102924	HP Acquire Method	HP Processing Method pl102824 8081

STD. NAME	STD REF.#
Tune/Reschk	PP23793,PP23517
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683
CCC	PP23686,PP23690,PP23695
Internal Standard/PEM	
ICV/I.BLK	PP23687,PP23693,PP23698
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PL092692.D	29 Oct 2024 09:35		AR\AJ	Ok
2	I.BLK	I.BLK	PL092693.D	29 Oct 2024 09:48		AR\AJ	Ok
3	PEM	PEM	PL092694.D	29 Oct 2024 10:02		AR\AJ	Ok
4	PSTDCCC050	PSTDCCC050	PL092695.D	29 Oct 2024 10:15		AR\AJ	Ok
5	P4545-01RE	VNJ-215RE	PL092696.D	29 Oct 2024 10:30	DCB low in both column	AR\AJ	Confirms
6	PB164445BL	PB164445BL	PL092697.D	29 Oct 2024 10:43		AR\AJ	Ok
7	PB164445BS	PB164445BS	PL092698.D	29 Oct 2024 10:57		AR\AJ	Ok,M
8	PB164393TB	PB164393TB	PL092699.D	29 Oct 2024 11:10		AR\AJ	Ok
9	P4578-06	WB-305-BOT	PL092700.D	29 Oct 2024 11:23		AR\AJ	Ok,M
10	P4578-06MS	WB-305-BOTMS	PL092701.D	29 Oct 2024 11:37		AR\AJ	Ok,M
11	P4578-06MSD	WB-305-BOTMSD	PL092702.D	29 Oct 2024 11:50		AR\AJ	Ok,M
12	P4578-08	WB-305-BOT-1	PL092703.D	29 Oct 2024 12:04		AR\AJ	Ok,M
13	PB164496BL	PB164496BL	PL092704.D	29 Oct 2024 12:17		AR\AJ	Ok
14	PB164496BS	PB164496BS	PL092705.D	29 Oct 2024 12:30		AR\AJ	Ok,M
15	P4597-01	RED-1-1	PL092706.D	29 Oct 2024 12:58		AR\AJ	Ok,M
16	P4597-04	RED-1-2	PL092707.D	29 Oct 2024 13:12		AR\AJ	Ok,M
17	P4597-07	BLUE-2-1	PL092708.D	29 Oct 2024 13:26		AR\AJ	Ok,M
18	P4597-10	BLUE-2-2	PL092709.D	29 Oct 2024 13:39		AR\AJ	Ok,M

Instrument ID: ECD_L

Daily Analysis Runlog For Sequence/QC Batch ID # PL102924

Review By	Abdul	Review On	10/30/2024 3:38:50 PM
Supervise By	Ankita	Supervise On	11/4/2024 9:20:27 AM
SubDirectory	PL102924	HP Acquire Method	HP Processing Method pl102824 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP23793,PP23517		
Initial Calibration Stds	PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,PP23680,PP23681,PP23682,PP23683		
CCC	PP23686,PP23690,PP23695		
Internal Standard/PEM			
ICV/I.BLK	PP23687,PP23693,PP23698		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	I.BLK	I.BLK	PL092710.D	29 Oct 2024 13:53		AR\AJ	Ok,M
20	PSTDCCC050	PSTDCCC050	PL092711.D	29 Oct 2024 14:07		AR\AJ	Ok,M
21	P4594-01	TP-4	PL092712.D	29 Oct 2024 14:21		AR\AJ	Ok,M
22	P4594-01MS	TP-4MS	PL092713.D	29 Oct 2024 14:35		AR\AJ	Ok,M
23	P4594-01MSD	TP-4MSD	PL092714.D	29 Oct 2024 14:49		AR\AJ	Ok,M
24	P4594-05	BP-F17	PL092715.D	29 Oct 2024 15:02		AR\AJ	Ok,M
25	P4594-09	BP-F16	PL092716.D	29 Oct 2024 15:16		AR\AJ	Ok,M
26	P4594-13	TP-5	PL092717.D	29 Oct 2024 15:30		AR\AJ	Ok,M
27	P4594-17	BP-F15	PL092718.D	29 Oct 2024 15:44		AR\AJ	Ok,M
28	P4598-01	BP-F12	PL092719.D	29 Oct 2024 15:58		AR\AJ	Ok,M
29	P4598-05	BP-F11	PL092720.D	29 Oct 2024 16:11		AR\AJ	Ok,M
30	P4598-09	TP-8	PL092721.D	29 Oct 2024 16:25		AR\AJ	Ok,M
31	I.BLK	I.BLK	PL092722.D	29 Oct 2024 16:39		AR\AJ	Ok,M
32	PSTDCCC050	PSTDCCC050	PL092723.D	29 Oct 2024 16:53		AR\AJ	Ok,M

M : Manual Integration

SOP ID :	M1311-TCLP-15	
SDG No :	N/A	Start Prep Date : 10/25/2024 Time : 17:40
Weight By :	JP	End Prep Date : 10/26/2024 Time : 10:37
Balance ID :	WC SC-4	Combination Ratio : 20
pH Meter ID :	WC PH METER-1	ZHE Cleaning Batch : N/A
Extraction By :	JP	Initial Room Temperature: 23 °C
Filter By :	JP	Final Room Temperature: 22 °C
Pipette ID :	WC	TCLP Technician Signature : JP
Tumbler ID :	T-1 / T-2	Supervisor By : 12
TCLP Filter ID :	114771	

Standardized Name	MLS USED	STD REF. # FROM LOG
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Chemical Used	ML/SAMPLE U	Lot Number
TCLP-FLUID-1	N/A	WP108622
HCL-TCLP,1N	N/A	WP108584
HNO3-TCLP,1N	N/A	WP108585
pH Strips	N/A	W1931,W1934,W2350,W2755
pH Strips	N/A	W1937,W1938,W1939,W1940,W1941,W1942
1 Liter Amber	N/A	23091
120ml Plastic bottle	N/A	21029
1:1 HNO3	MP81119	N/A

Extraction Conformance/Non-Conformance Comments:

Matrix spikes are added after filtration and before preservation. Tumbler T-1 / T-2 CHECKED,30 RPM. Particle size reduction is not required. p4578-08 is used for MS-MSD.

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
10/26/24 11:45	JP 1st Room	JP 1st Room
	Preparation Group	Analysis Group

Sample ID	ClientID	TCLP Vessel ID	Sample Wt (g)	Volume Extraction Fluid #1 (mL)	Multi phasic	Phase Miscible	Phases Combined	Final Leachate PH	Metals Leachate Adj. PH	Prep Pos
P4452-03	ETGI-285	01	100.03	2000	N/A	N/A	N/A	11.0	1.5	T-1
P4545-02	VNJ-215	02	100.02	2000	N/A	N/A	N/A	5.8	1.5	T-1
P4547-04	BP-F-21	03	100.01	2000	N/A	N/A	N/A	4.5	1.0	T-1
P4547-08	BP-F-20	04	100.02	2000	N/A	N/A	N/A	6.0	1.0	T-1
P4561-04	BP-F-19	05	100.03	2000	N/A	N/A	N/A	5.6	1.5	T-1
P4561-08	BP-F-18	06	100.04	2000	N/A	N/A	N/A	4.0	1.0	T-1
P4567-04	WC-1	07	100.02	2000	N/A	N/A	N/A	7.2	1.5	T-1
P4567-08	WC-2	08	100.03	2000	N/A	N/A	N/A	7.6	1.0	T-1
P4567-12	WC-3	09	100.04	2000	N/A	N/A	N/A	7.6	1.5	T-1
P4574-03	GRAVEL-1	10	100.02	2000	N/A	N/A	N/A	4.5	1.0	T-1
P4574-06	GRAVEL-2	11	100.03	2000	N/A	N/A	N/A	3.5	1.5	T-2
P4574-08	CONCRETE-1	12	100.02	2000	N/A	N/A	N/A	10.5	1.0	T-2
P4574-10	CONCRETE-2	13	100.02	2000	N/A	N/A	N/A	10.5	1.5	T-2
P4574-12	CONCRETE-3	14	100.03	2000	N/A	N/A	N/A	11.0	1.0	T-2
P4578-06	WB-305-BOT	15	100.04	2000	N/A	N/A	N/A	5.8	1.5	T-2
P4578-08	WB-305-BOT-1	16	100.02	2000	N/A	N/A	N/A	6.0	1.5	T-2
PB164393TB	LEB393	17	N/A	2000	N/A	N/A	N/A	4.93	1.5	T-2

SampleID	ClientID	Sample Weight (g)	Filter Weight (g)	Filtrate (mL)	Filter + Solid (After 100°C)	% solids	% Dry Solids
P4452-03	ETGI-285	N/A	N/A	N/A	N/A	100	N/A
P4545-02	VNJ-215	N/A	N/A	N/A	N/A	100	N/A
P4547-04	BP-F-21	N/A	N/A	N/A	N/A	100	N/A
P4547-08	BP-F-20	N/A	N/A	N/A	N/A	100	N/A
P4561-04	BP-F-19	N/A	N/A	N/A	N/A	100	N/A
P4561-08	BP-F-18	N/A	N/A	N/A	N/A	100	N/A
P4567-04	WC-1	N/A	N/A	N/A	N/A	100	N/A
P4567-08	WC-2	N/A	N/A	N/A	N/A	100	N/A
P4567-12	WC-3	N/A	N/A	N/A	N/A	100	N/A
P4574-03	GRAVEL-1	N/A	N/A	N/A	N/A	100	N/A
P4574-06	GRAVEL-2	N/A	N/A	N/A	N/A	100	N/A
P4574-08	CONCRETE-1	N/A	N/A	N/A	N/A	100	N/A
P4574-10	CONCRETE-2	N/A	N/A	N/A	N/A	100	N/A
P4574-12	CONCRETE-3	N/A	N/A	N/A	N/A	100	N/A
P4578-06	WB-305-BOT	N/A	N/A	N/A	N/A	100	N/A
P4578-08	WB-305-BOT-1	N/A	N/A	N/A	N/A	100	N/A
PB164393TB	LEB393	N/A	N/A	N/A	N/A	N/A	N/A

Hot Block ID : WC S-1 /WC S-2
Thermometer ID : FLASHPOINT

SampleID	ClientID	Sample Weight (g)	Volume DI Water (mL)	PH after 5 min stir	PH after 10 min stir	Extraction Fluid 1 or 2	pH Extraction Fluid
P4452-03	ETGI-285	5.02	96.5	11.0	4.0	#1	4.93
P4545-02	VNJ-215	5.02	96.5	7.6	2.5	#1	4.93
P4547-04	BP-F-21	5.00	96.5	6.2	2.0	#1	4.93
P4547-08	BP-F-20	5.03	96.5	8.2	3.0	#1	4.93
P4561-04	BP-F-19	5.02	96.5	7.6	2.5	#1	4.93
P4561-08	BP-F-18	5.02	96.5	7.0	2.5	#1	4.93
P4567-04	WC-1	5.03	96.5	9.1	4.0	#1	4.93
P4567-08	WC-2	5.02	96.5	9.5	4.0	#1	4.93
P4567-12	WC-3	5.02	96.5	7.2	3.0	#1	4.93
P4574-03	GRAVEL-1	5.02	96.5	6.0	2.0	#1	4.93
P4574-06	GRAVEL-2	5.03	96.5	5.6	1.5	#1	4.93
P4574-08	CONCRETE-1	5.02	96.5	11.0	4.0	#1	4.93
P4574-10	CONCRETE-2	5.03	96.5	11.0	4.0	#1	4.93
P4574-12	CONCRETE-3	5.02	96.5	11.5	4.5	#1	4.93
P4578-06	WB-305-BOT	5.03	96.5	7.6	2.5	#1	4.93
P4578-08	WB-305-BOT-1	5.02	96.5	8.2	3.0	#1	4.93
PB164393TB	LEB393	N/A	N/A	N/A	N/A	#1	4.93

WORKLIST(Hardcopy Internal Chain)

WorkList Name : tcip p4545

WorkList ID : 184760

Department : TCLP Extraction

Date : 10-25-2024 07:58:53

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P4542-03	ETGI-285	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K51	10/18/2024	1311
P4545-02	VNJ-215	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K61	10/24/2024	1311
P4547-04	BP-F-21	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K51	10/24/2024	1311
P4547-08	BP-F-20	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K51	10/24/2024	1311
P4561-04	BP-F-19	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K63	10/25/2024	1311
P4561-08	BP-F-18	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K63	10/25/2024	1311
P4567-04	WC-1	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K61	10/25/2024	1311
P4567-08	WC-2	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K61	10/25/2024	1311
P4567-12	WC-3	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K61	10/25/2024	1311
P4574-03	GRAVEL-1	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K63	10/25/2024	1311
P4574-06	GRAVEL-2	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K63	10/25/2024	1311
P4574-08	CONCRETE-1	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K63	10/25/2024	1311
P4574-10	CONCRETE-2	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K63	10/25/2024	1311
P4574-12	CONCRETE-3	Solid	TCLP Extraction	Cool 4 deg C	PSEG03	K63	10/25/2024	1311
P4578-06	WB-305-BOT	Solid	TCLP Extraction	Cool 4 deg C	PORT06	K63	10/25/2024	1311
P4578-08	WB-305-BOT-1	Solid	TCLP Extraction	Cool 4 deg C	PORT06	K63	10/25/2024	1311

Date/Time 10/25/24 17:25
 Raw Sample Received by: SO WOC
 Raw Sample Relinquished by: J.C (sm)

Date/Time 10/23/24 19:30
 Raw Sample Received by: J.C (sm)
 Raw Sample Relinquished by: SO WOC

SOP ID:	M3541-ASE Extraction-14		
Clean Up SOP #:	N/A	Extraction Start Date :	10/26/2024
Matrix :	Water	Extraction Start Time :	12:50
Weigh By:	N/A	Extraction By:	RS
Balance check:	N/A	Filter By:	RS
Balance ID:	N/A	pH Meter ID:	N/A
pH Strip Lot#:	N/A	Hood ID:	4,6,7
Extraction Method:	☒ Separatory Funnel	☐ Continous Liquid/Liquid	☐ Sonication
		☐ Waste Dilution	☐ Soxhlet
		Extraction End Date :	10/26/2024
		Extraction End Time :	17:45
		Concentration By:	EH
		Supervisor By :	rajesh

Standardized Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	500 PPB	PP23638
Surrogate	1.0ML	200 PPB	PP23858
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3822
Baked Na2SO4	N/A	EP2551
Hexane	N/A	E3819
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40 BTS721.

KD Bath ID:	Water bath -01	Envap ID:	NEVAP-02
KD Bath Temperature:	60 °C	Envap Temperature:	40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
10/28/24	RP (Est. 206)	Y-P-PRSTHPS.
3:00	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-14

Concentration Date: 10/26/2024

Sample ID	Client Sample ID	Test	g / (mL)	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB164393TB	PB164393TB	TCLP Pesticide	100	6	RUPESH	rajesh	1			SEP-01
PB164445BL	PBLK445	TCLP Pesticide	1000	6	RUPESH	rajesh	1			2
PB164445BS	PLCS445	TCLP Pesticide	1000	6	RUPESH	rajesh	1			3
P4578-06	WB-305-BOT	TCLP Pesticide	100	6	RUPESH	rajesh	1	A		4
P4578-06MS	WB-305-BOTMS	TCLP Pesticide	100	6	RUPESH	rajesh	1	A		5
P4578-06MS D	WB-305-BOTMSD	TCLP Pesticide	100	6	RUPESH	rajesh	1	A		6
P4578-08	WB-305-BOT-1	TCLP Pesticide	100	6	RUPESH	rajesh	1	A		7

* Extracts relinquished on the same date as received.

2
10/26/24

SOP ID:	M3541-ASE Extraction-14		
Clean Up SOP #:	N/A	Extraction Start Date :	10/26/2024
Matrix :	Water	Extraction Start Time :	12:50
Weigh By:	N/A	Extraction By:	RS
Balance check:	N/A	Filter By:	RS
Balance ID:	N/A	Extraction End Date :	10/26/2024
pH Strip Lot#:	N/A	Extraction End Time :	17:45
		Concentration By:	EH
		Supervisor By :	rajesh
Extraction Method:	☒ Separatory Funnel ☐ Continous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☐ Soxhlet		

Standardized Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	500 PPB	PP23638
Surrogate	1.0ML	200 PPB	PP23858
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3822
Baked Na2SO4	N/A	EP2551
Hexane	N/A	E3819
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40 BTS721.

KD Bath ID:	Water bath -01	Envap ID:	NEVAP-02
KD Bath Temperature:	60 °C	Envap Temperature:	40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
10/28/24	RP (Est. 206)	Y-P-PRSTHPS.
3:00	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-14

Concentration Date: 10/26/2024

Sample ID	Client Sample ID	Test	g / (mL)	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB164393TB	PB164393TB	TCLP Pesticide	100	6	RUPESH	rajesh	1			SEP-01
PB164445BL	PBLK445	TCLP Pesticide	1000	6	RUPESH	rajesh	1			2
PB164445BS	PLCS445	TCLP Pesticide	1000	6	RUPESH	rajesh	1			3
P4578-06	WB-305-BOT	TCLP Pesticide	100	6	RUPESH	rajesh	1	A		4
P4578-06MS	WB-305-BOTMS	TCLP Pesticide	100	6	RUPESH	rajesh	1	A		5
P4578-06MS D	WB-305-BOTMSD	TCLP Pesticide	100	6	RUPESH	rajesh	1	A		6
P4578-08	WB-305-BOT-1	TCLP Pesticide	100	6	RUPESH	rajesh	1	A		7

* Extracts relinquished on the same date as received.

2
10/26/24

Prep Standard - Chemical Standard Summary

Order ID : P4578

Test : TCLP Pesticide

Prepbatch ID : PB164445,

Sequence ID/Qc Batch ID: PL102924,

Standard ID :

EP2551,PP23474,PP23476,PP23517,PP23638,PP23673,PP23674,PP23675,PP23676,PP23677,PP23678,PP23679,P
P23680,PP23681,PP23682,PP23683,PP23686,PP23687,PP23690,PP23693,PP23695,PP23698,PP23733,PP23793,P
P23858,

Chemical ID :

E3551,E3762,E3770,E3788,E3792,E3805,E3815,E3819,E3822,P11145,P11146,P11896,P13035,P13036,P13039,P132
44,P13349,P13350,P13351,P13359,P13402,



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2551	10/18/2024	01/03/2025	Rajesh Parikh	Extraction_SCALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 10/18/2024
<u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1472	20 PPM Pest Stock Solution 2nd Source	PP23474	06/20/2024	12/18/2024	Abdul Mirza	None	None	Ankita Jodhani 06/21/2024
<u>FROM</u>	1.00000ml of P13035 + 9.00000ml of E3762 = Final Quantity: 10.000 ml							

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3663	20 PPM MIREX Stock STD (Secondary source)	PP23476	06/20/2024	12/18/2024	Abdul Mirza	None	None	Ankita Jodhani
								06/21/2024

FROM 0.20000ml of P11145 + 9.80000ml of E3762 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4027	Pesticide resolution Check Mixture 8081	PP23517	07/12/2024	01/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								07/16/2024

FROM 1.00000ml of E3770 + 99.00000ml of P13244 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
79	500 PPB Pesticide Spike Solution	PP23638	09/05/2024	12/18/2024	Abdul Mirza	None	None	Ankita Jodhani
								09/10/2024

FROM 95.00000ml of E3788 + 2.50000ml of PP23474 + 2.50000ml of PP23476 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP23673	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 1.00000ml of P13349 + 9.00000ml of E3792 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3629	20 PPM PEST stock Solution 1st source(RESTEK)	PP23674	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 1.00000ml of P13036 + 9.00000ml of E3792 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1472	20 PPM Pest Stock Solution 2nd Source	PP23675	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 1.00000ml of P13039 + 9.00000ml of E3792 = Final Quantity: 10.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1273	20 PPM Mirex Stock (Primary Source)	PP23676	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani 10/01/2024
<u>FROM</u> 0.20000ml of P11146 + 9.80000ml of E3792 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3663	20 PPM MIREX Stock STD (Secondary source)	PP23677	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani 10/01/2024
<u>FROM</u> 0.20000ml of P11146 + 9.80000ml of E3792 = Final Quantity: 10.000 ml								



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
386	1000/100 PPB Chlordane STD (Restek)	PP23680	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.10000ml of P11896 + 99.40000ml of E3792 + 0.50000ml of PP23673 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3746	1000/100 ppb Chlordane STD-RESTEK 2ND SOURCE	PP23681	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.10000ml of P11896 + 99.40000ml of E3792 + 0.50000ml of PP23673 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
383	1000/100 PPB Toxaphene STD (Restek)	PP23682	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.10000ml of P13359 + 99.40000ml of E3792 + 0.50000ml of PP23673 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3669	1000/100 PPB TOXAPHENE STD 2nd source (RESTEK)	PP23683	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.10000ml of P13402 + 99.40000ml of E3792 + 0.50000ml of PP23673 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3632	50 PPB ICAL PEST STD(RESTEK)	PP23686	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.50000ml of E3792 + 0.50000ml of PP23678 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3988	50 PPB PEST ICV STD(RESTEK)	PP23687	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.50000ml of E3792 + 0.50000ml of PP23679 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
529	CHLOR 500 PPB STD	PP23690	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.50000ml of E3792 + 0.50000ml of PP23680 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
532	CHLOR 500 PPB ICV STD	PP23693	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.50000ml of E3792 + 0.50000ml of PP23681 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
534	TOX 500 PPB STD	PP23695	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.50000ml of E3792 + 0.50000ml of PP23682 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3670	TOX 500 PPB ICV std (RESTEK)	PP23698	09/21/2024	03/11/2025	Abdul Mirza	None	None	Ankita Jodhani
								10/01/2024

FROM 0.50000ml of E3792 + 0.50000ml of PP23683 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP23733	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13350 + 9.00000ml of E3805 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
518	Pest/PCB I.BLK 20 PPB	PP23793	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 99.90000ml of E3805 + 0.10000ml of PP23733 = Final Quantity: 100.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP23858	10/14/2024	04/04/2025	Abdul Mirza	None	None	Ankita Jodhani 10/14/2024
<u>FROM</u> 1.00000ml of P13351 + 999.00000ml of E3815 = Final Quantity: 1000.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	01/03/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	12/18/2024	06/18/2024 / Rajesh	06/17/2024 / Rajesh	E3762

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	04/15/2025	07/12/2024 / Rajesh	07/02/2024 / Rajesh	E3770

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	23H1462005	04/23/2025	08/13/2024 / Rajesh	08/13/2024 / Rajesh	E3788

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/11/2025	09/12/2024 / Rajesh	09/11/2024 / Rajesh	E3792

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/30/2025	09/30/2024 / Rajesh	09/25/2024 / Rajesh	E3805

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	04/04/2025	10/04/2024 / Rajesh	10/04/2024 / Rajesh	E3815

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	04/15/2025	10/15/2024 / Rajesh	10/09/2024 / Rajesh	E3819

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24I2662006	04/23/2025	10/24/2024 / Rajesh	10/24/2024 / Rajesh	E3822

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	102821	12/20/2024	06/20/2024 / Abdul	10/29/2021 / Abdul	P11145

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	102821	03/21/2025	09/21/2024 / Abdul	10/29/2021 / Abdul	P11146

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32021 / Chlordane Std.	A0181737	03/21/2025	09/21/2024 / Abdul	06/17/2022 / Abdul	P11896

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0200423	12/20/2024	06/20/2024 / Abdul	12/26/2023 / Abdul	P13035

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0200423	03/21/2025	09/21/2024 / Abdul	12/26/2023 / Abdul	P13036

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0199099	03/21/2025	09/21/2024 / Abdul	12/26/2023 / Abdul	P13039

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	19161 / 8081 pesticide resolution check mixture	013124	01/12/2025	07/12/2024 / Abdul	02/09/2024 / Abdul	P13244

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	03/21/2025	09/21/2024 / Abdul	04/22/2024 / Abdul	P13349

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/03/2025	10/03/2024 / Ankita	04/22/2024 / Abdul	P13350

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/14/2025	10/14/2024 / Abdul	04/22/2024 / Abdul	P13351

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0203830	03/21/2025	09/21/2024 / Abdul	05/03/2024 / Abdul	P13359

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0203038	03/21/2025	09/21/2024 / Abdul	05/15/2024 / Abdul	P13402



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 6/11/24

E 3762

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 23H1462005

Manufactured Date: 2023-07-26

Expiration Date: 2026-07-25

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 7/21/24

E 3769

Ken Koehnlein
Sr. Manager, Quality Assurance

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03
Batch No.: 23H1462005
Manufactured Date: 2023-07-26
Expiration Date: 2026-07-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 8/13/24

E 3788

Ken Koehnlein
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 09/11/24

E 3192

Jamie Croak
Director Quality Operations, Bioscience Production

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 9/25/24

E 3805

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 24H1462005
Manufactured Date: 2024-05-24
Expiration Date: 2027-05-24
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3815

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087 U.S.A. Phone 610.386.1700

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis

 **avantors**



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 10/09/24

E 3819



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700
Page 1 of 1

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)

 **avantors**



Material No.: 9266-A4

Batch No.: 24I2662006

Manufactured Date: 2024-08-29

Expiration Date: 2025-11-28

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	3
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	99.9%
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3822



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32021 Lot No.: A0181737
Description: Chlordane Standard
Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul
Container Size: 2 mL Pkg Amt: > 1 mL
Expiration Date: May 31, 2028 Storage: 10°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Chlordane CAS # 57-74-9 (Lot 978545) Purity ----%	1,006.0 µg/mL	+/- 5.9753 µg/mL Gravimetric +/- 31.8975 µg/mL Unstressed +/- 41.6615 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

P 11892
↓
P 11896
5

06/17/2022

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

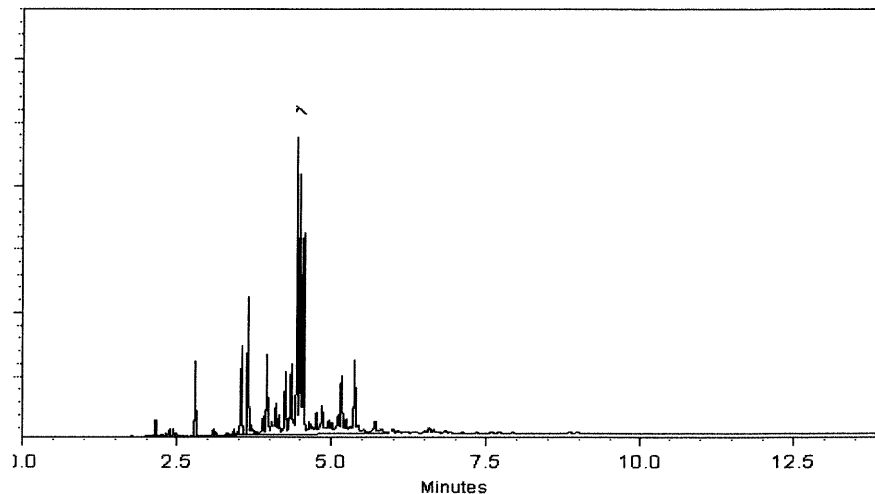


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Josh McCloskey - Operations Technician I

Date Mixed: 11-Feb-2022

Balance: B442140311


Marlene Cowan - Operations Tech I

Date Passed: 24-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 11892 / (5)
↓
P 11896 / 1


06/17/2022



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 Lot No.: A0199099

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : June 30, 2027 Storage: 10°C or colder

Ship: Ambient

P130397 5
↓
P13043 1
✓
12-26-2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	alpha-BHC	319-84-6	14434500	99%	200.0 µg/mL	+/- 8.9732
2	gamma-BHC (Lindane)	58-89-9	14184400	98%	200.1 µg/mL	+/- 8.9762
3	beta-BHC	319-85-7	BCCC6425	99%	200.3 µg/mL	+/- 8.9844
4	delta-BHC	319-86-8	14450800	98%	200.0 µg/mL	+/- 8.9740
5	Heptachlor	76-44-8	813251	99%	200.1 µg/mL	+/- 8.9754
6	Aldrin	309-00-2	14389400	98%	200.0 µg/mL	+/- 8.9718
7	Heptachlor epoxide (isomer B)	1024-57-3	14448800	99%	200.1 µg/mL	+/- 8.9754
8	trans-Chlordane	5103-74-2	32943	98%	199.9 µg/mL	+/- 8.9696
9	cis-Chlordane	5103-71-9	31766	98%	200.1 µg/mL	+/- 8.9762
10	Endosulfan I	959-98-8	BCCF4060	99%	200.1 µg/mL	+/- 8.9754
11	4,4'-DDE	72-55-9	GHYQG	99%	200.1 µg/mL	+/- 8.9777
12	Dieldrin	60-57-1	11129900	98%	200.0 µg/mL	+/- 8.9718
13	Endrin	72-20-8	14123200	98%	199.9 µg/mL	+/- 8.9696
14	4,4'-DDD	72-54-8	HAN02	99%	200.1 µg/mL	+/- 8.9777
15	Endosulfan II	33213-65-9	14374700	99%	200.0 µg/mL	+/- 8.9732
16	4,4'-DDT	50-29-3	230410JLMA	98%	200.0 µg/mL	+/- 8.9718

17	Endrin aldehyde	7421-93-4	30720	98%	200.1	µg/mL	+/- 8.9784
18	Endosulfan sulfate	1031-07-8	BCCH9010	99%	200.0	µg/mL	+/- 8.9732
19	Methoxychlor	72-43-5	13668200	99%	200.1	µg/mL	+/- 8.9777
20	Endrin ketone	53494-70-5	1-ABS-16-7	98%	200.0	µg/mL	+/- 8.9740

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane/Toluene (50:50)
CAS # 110-54-3/108-88-3
Purity 99%

P13039
 ↓
 P13043
 5
 1
 JAW
 12/26/23

Quality Confirmation Test

Column:
 30m x .25mm x .2um
 Rtx-CLP II (cat.# 11323)

Carrier Gas:
 helium-constant pressure 20 psi.

Temp. Program:
 150°C to 300°C
 @ 4°C/min. (hold 5 min.)


Inj. Temp:
 200°C

Det. Temp:
 300°C

Det. Type:
 ECD

Split Vent:
 Split ratio 50:1

Inj. Vol
 1µl

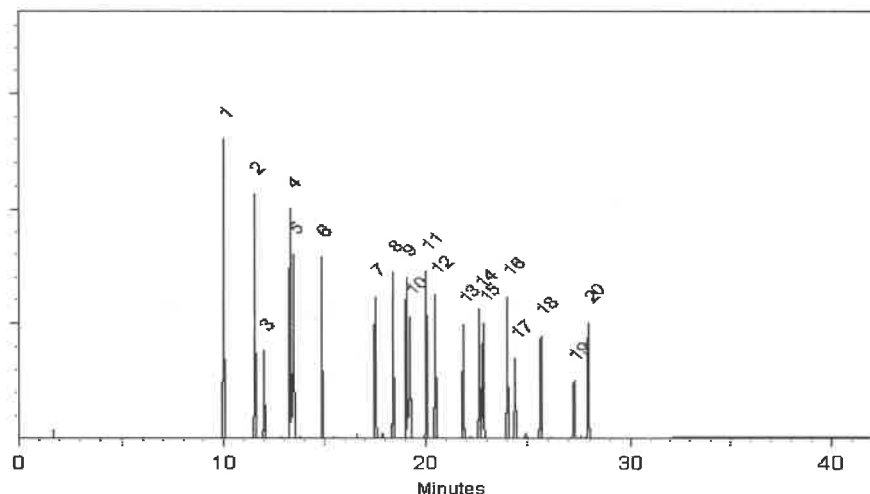

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Josh McCloskey
 Josh McCloskey - Operations Technician I

Date Mixed: 19-Jun-2023

Balance Serial # 1128360905


Jennifer Pollino
 Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 23-Jun-2023

Manufactured under Restek's ISO 9001:2015
 Registered Quality System
 Certificate #FM 80397



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

79136
102821
Mirex

Solvent(s):
Lot#
Acetone **81025**

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

102826
Refrigerate (4 °C)
1000
6UTB

5E-05 **Balance Uncertainty**
0.006 **Flask Uncertainty**


Weight(s) shown below were combined and diluted to (mL):

50.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded SDS Information		
									Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	(SHA PEL (TWA) LD50)

1. Mirex	437	9492400	1000	99.4	0.5	0.05034	0.05039	1000.9	10.3	2385-85-5	N/A	orl-rat 306mg/kg
----------	-----	---------	------	------	-----	---------	---------	--------	------	-----------	-----	------------------


Method GC7MSD-1.M: Column: SPB-608 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (4min.), Temp 2 = 290°C (13.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C. Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Candice Warren.

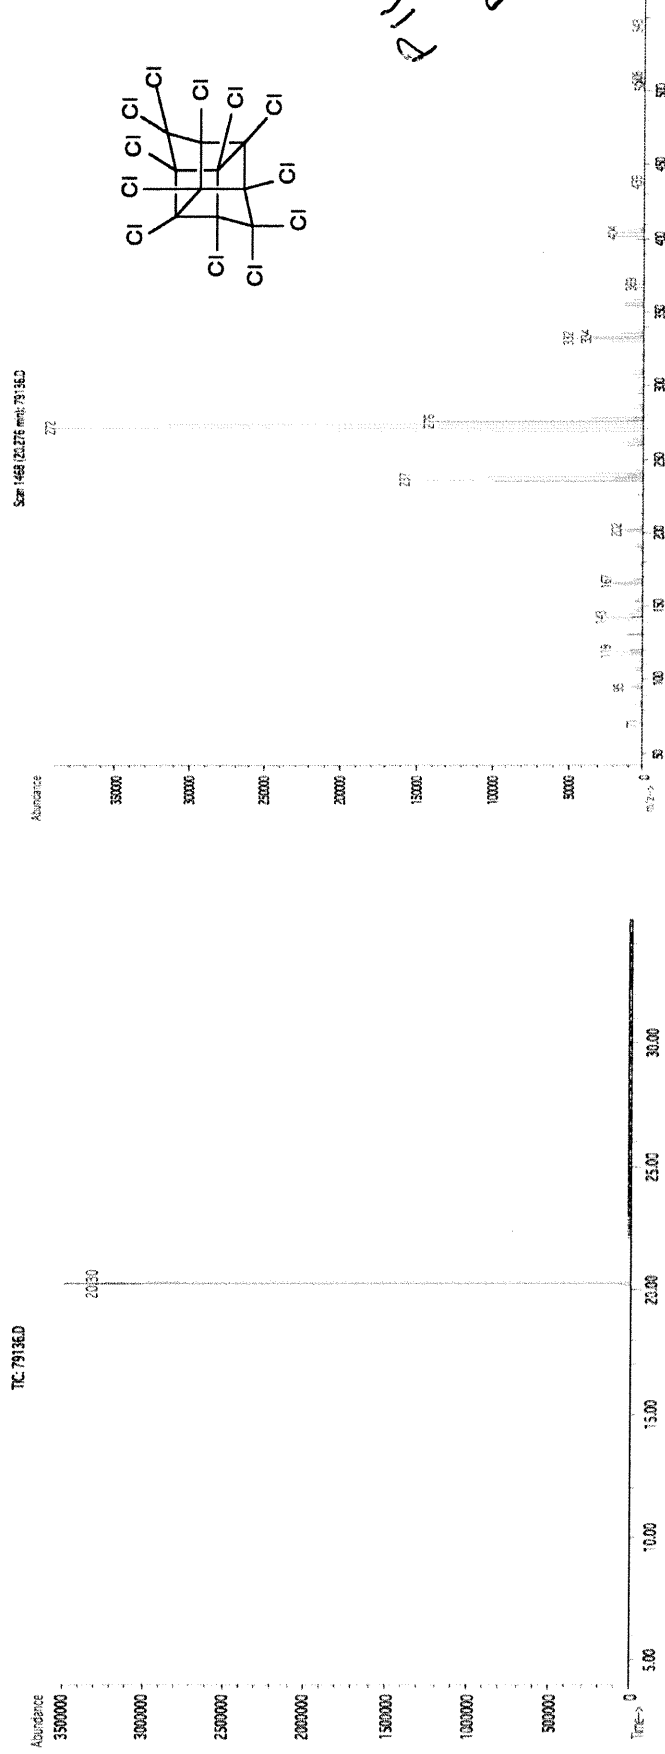

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

79136
102821
Mirex

Solvent(s):
Lot#
Acetone **81025**

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

102826
Refrigerate (4 °C)
1000
6UTB

5E-05 **Balance Uncertainty**
0.006 **Flask Uncertainty**


Weight(s) shown below were combined and diluted to (mL):

50.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded SDS Information		
									Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	(SHA PEL (TWA) LD50)

1. Mirex	437	9492400	1000	99.4	0.5	0.05034	0.05039	1000.9	10.3	2385-85-5	N/A	orl-rat 306mg/kg
----------	-----	---------	------	------	-----	---------	---------	--------	------	-----------	-----	------------------

Method GC7MSD-1.M: Column: SPB-608 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (4min.), Temp 2 = 290°C (13.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C. Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Candice Warren.

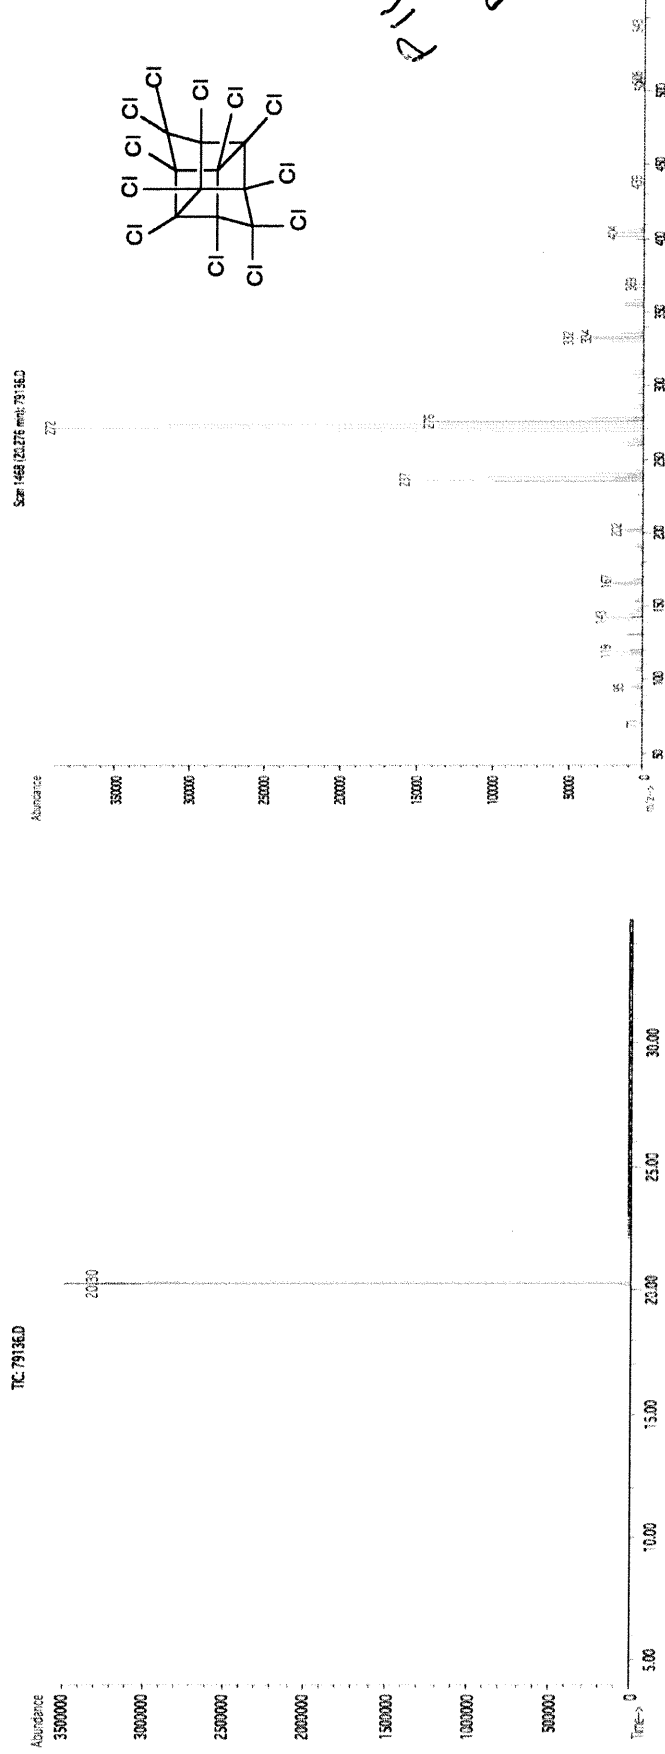

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 **Lot No.:** A0200423

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2027 **Storage:** 10°C or colder

Ship: Ambient

P 13034
↓
P 13038
✓
12.26.2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	alpha-BHC	319-84-6	14434500	99%	200.5 µg/mL	+/- 8.9956
2	gamma-BHC (Lindane)	58-89-9	14184400	98%	199.9 µg/mL	+/- 8.9696
3	beta-BHC	319-85-7	BCCC6425	99%	200.0 µg/mL	+/- 8.9732
4	delta-BHC	319-86-8	14450800	98%	199.9 µg/mL	+/- 8.9696
5	Heptachlor	76-44-8	813251	99%	202.0 µg/mL	+/- 9.0629
6	Aldrin	309-00-2	14389400	98%	200.9 µg/mL	+/- 9.0136
7	Heptachlor epoxide (isomer B)	1024-57-3	14448800	99%	200.0 µg/mL	+/- 8.9732
8	trans-Chlordane	5103-74-2	34616	99%	200.5 µg/mL	+/- 8.9956
9	cis-Chlordane	5103-71-9	31766	98%	201.4 µg/mL	+/- 9.0356
10	Endosulfan I	959-98-8	BCCF4060	99%	200.0 µg/mL	+/- 8.9732
11	4,4'-DDE	72-55-9	GHYQG	99%	201.5 µg/mL	+/- 9.0405
12	Dieldrin	60-57-1	14515000	98%	199.9 µg/mL	+/- 8.9696
13	Endrin	72-20-8	14485300	98%	200.4 µg/mL	+/- 8.9916
14	4,4'-DDD	72-54-8	HAN02	99%	200.5 µg/mL	+/- 8.9956
15	Endosulfan II	33213-65-9	14374700	99%	200.0 µg/mL	+/- 8.9732
16	4,4'-DDT	50-29-3	230410JLMA	98%	201.9 µg/mL	+/- 9.0575

17	Endrin aldehyde	7421-93-4	30720	98%	201.4 µg/mL	+/- 9.0356
18	Endosulfan sulfate	1031-07-8	BCCH9010	99%	200.5 µg/mL	+/- 8.9956
19	Methoxychlor	72-43-5	14563200	98%	200.9 µg/mL	+/- 9.0136
20	Endrin ketone	53494-70-5	14537700	98%	199.9 µg/mL	+/- 8.9696

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane/Toluene (50:50)
CAS # 110-54-3/108-88-3
Purity 99%

P13034
P13038
1
5
12/26/2023

Quality Confirmation Test

Column:
30m x .25mm x .2µm
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
150°C to 300°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
200°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
Split ratio 50:1

Inj. Vol
1µl

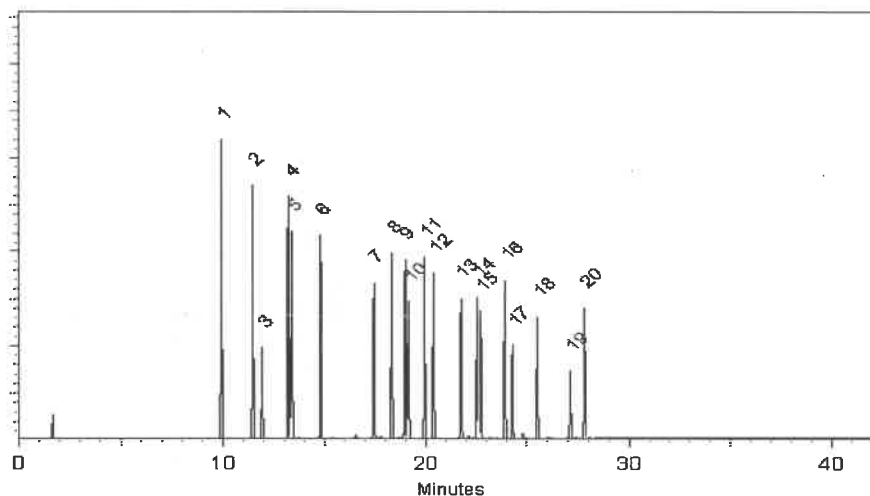

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 31-Jul-2023

Balance Serial # B442140311

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 03-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 **Lot No.:** A0200423

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2027 **Storage:** 10°C or colder

Ship: Ambient

P 13034
↓
P 13038
12.26.2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	alpha-BHC	319-84-6	14434500	99%	200.5 µg/mL	+/- 8.9956
2	gamma-BHC (Lindane)	58-89-9	14184400	98%	199.9 µg/mL	+/- 8.9696
3	beta-BHC	319-85-7	BCCC6425	99%	200.0 µg/mL	+/- 8.9732
4	delta-BHC	319-86-8	14450800	98%	199.9 µg/mL	+/- 8.9696
5	Heptachlor	76-44-8	813251	99%	202.0 µg/mL	+/- 9.0629
6	Aldrin	309-00-2	14389400	98%	200.9 µg/mL	+/- 9.0136
7	Heptachlor epoxide (isomer B)	1024-57-3	14448800	99%	200.0 µg/mL	+/- 8.9732
8	trans-Chlordane	5103-74-2	34616	99%	200.5 µg/mL	+/- 8.9956
9	cis-Chlordane	5103-71-9	31766	98%	201.4 µg/mL	+/- 9.0356
10	Endosulfan I	959-98-8	BCCF4060	99%	200.0 µg/mL	+/- 8.9732
11	4,4'-DDE	72-55-9	GHYQG	99%	201.5 µg/mL	+/- 9.0405
12	Dieldrin	60-57-1	14515000	98%	199.9 µg/mL	+/- 8.9696
13	Endrin	72-20-8	14485300	98%	200.4 µg/mL	+/- 8.9916
14	4,4'-DDD	72-54-8	HAN02	99%	200.5 µg/mL	+/- 8.9956
15	Endosulfan II	33213-65-9	14374700	99%	200.0 µg/mL	+/- 8.9732
16	4,4'-DDT	50-29-3	230410JLMA	98%	201.9 µg/mL	+/- 9.0575

17	Endrin aldehyde	7421-93-4	30720	98%	201.4 µg/mL	+/- 9.0356
18	Endosulfan sulfate	1031-07-8	BCCH9010	99%	200.5 µg/mL	+/- 8.9956
19	Methoxychlor	72-43-5	14563200	98%	200.9 µg/mL	+/- 9.0136
20	Endrin ketone	53494-70-5	14537700	98%	199.9 µg/mL	+/- 8.9696

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane/Toluene (50:50)
CAS # 110-54-3/108-88-3
Purity 99%

P13034
P13038
1
5
12/26/2023

Quality Confirmation Test

Column:
30m x .25mm x .2µm
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
150°C to 300°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
200°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
Split ratio 50:1

Inj. Vol
1µl

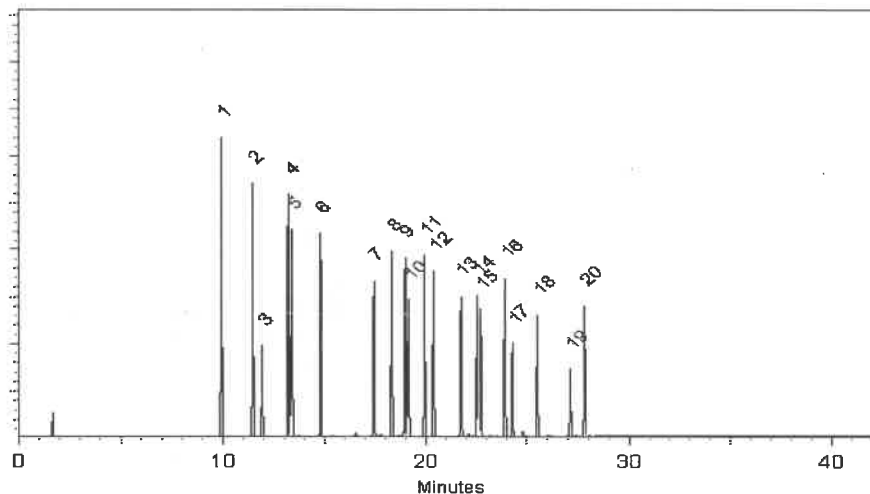

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 31-Jul-2023

Balance Serial # B442140311

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 03-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

19161
013124
CLP Pesticides & PCBs Resolution Check Standard

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):

9 components
013129
Refrigerate (4 °C)
Varied

Solvent(s):
Hexane
Toluene
Lot#
273615
28508
(50%)
(50%)

NIST Test ID#:

6UTB

Volume(s) shown below were combined and diluted to (mL):

5E-05
Balance Uncertainty
0.021
Pipet Uncertainty

<i>Lawrence Barry</i>	
Formulated By:	Lawrence Barry
DATE	013124
<i>Pedro L. Rentes</i>	
Reviewed By:	Pedro L. Rentes
DATE	013124

Compound

1. trans-Chlordane	19361	013124	0.010	1.00	0.004	101.3	1.0	0.02	5103-74-2	0.5mg/m3 (skin)	or-rat 500mg/kg
2. Endosulfan I	19361	013124	0.010	1.00	0.004	101.3	1.0	0.02	959-98-8	0.1mg/m3 (skin)	or-rat 18mg/kg
3. 4,4'-DDE	19361	013124	0.010	1.00	0.004	201.6	2.0	0.03	72-55-9	N/A	or-rat 880mg/kg
4. Dieldrin	19361	013124	0.010	1.00	0.004	202.8	2.0	0.03	60-57-1	0.25mg/m3 (skin)	or-rat 36300ug/kg
5. Endosulfan sulfate	19361	013124	0.010	1.00	0.004	204.2	2.0	0.03	1031-07-8	N/A	or-rat 18mg/kg
6. Endrin ketone	19361	013124	0.010	1.00	0.004	202.6	2.0	0.03	53494-70-5	N/A	N/A
7. 4,4-Methoxychlor	19361	013124	0.010	1.00	0.004	1000.7	10.0	0.09	72-43-5	10mg/m3	or-rat 6000mg/kg
8. 2,4,5,6-Tetrachloro-m-xylene	19361	013124	0.010	1.00	0.004	202.6	2.0	0.03	877-09-8	N/A	N/A
9. Decachlorobiphenyl (209)	19361	013124	0.010	1.00	0.004	202.0	2.0	0.03	2051-24-3	N/A	N/A

P13243
P13244
P13245
P13246
P13247
P13248
P13249
P13250
P13251
P13252
P13253
P13254
P13255
P13256
P13257
P13258
P13259
P13260
P13261
P13262
P13263
P13264
P13265
P13266
P13267
P13268
P13269
P13270
P13271
P13272
P13273
P13274
P13275
P13276
P13277
P13278
P13279
P13280
P13281
P13282
P13283
P13284
P13285
P13286
P13287
P13288
P13289
P13290
P13291
P13292
P13293
P13294
P13295
P13296
P13297
P13298
P13299
P13300
P13301
P13302
P13303
P13304
P13305
P13306
P13307
P13308
P13309
P13310
P13311
P13312
P13313
P13314
P13315
P13316
P13317
P13318
P13319
P13320
P13321
P13322
P13323
P13324
P13325
P13326
P13327
P13328
P13329
P13330
P13331
P13332
P13333
P13334
P13335
P13336
P13337
P13338
P13339
P13340
P13341
P13342
P13343
P13344
P13345
P13346
P13347
P13348
P13349
P13350
P13351
P13352
P13353
P13354
P13355
P13356
P13357
P13358
P13359
P13360
P13361
P13362
P13363
P13364
P13365
P13366
P13367
P13368
P13369
P13370
P13371
P13372
P13373
P13374
P13375
P13376
P13377
P13378
P13379
P13380
P13381
P13382
P13383
P13384
P13385
P13386
P13387
P13388
P13389
P13390
P13391
P13392
P13393
P13394
P13395
P13396
P13397
P13398
P13399
P13400
P13401
P13402
P13403
P13404
P13405
P13406
P13407
P13408
P13409
P13410
P13411
P13412
P13413
P13414
P13415
P13416
P13417
P13418
P13419
P13420
P13421
P13422
P13423
P13424
P13425
P13426
P13427
P13428
P13429
P13430
P13431
P13432
P13433
P13434
P13435
P13436
P13437
P13438
P13439
P13440
P13441
P13442
P13443
P13444
P13445
P13446
P13447
P13448
P13449
P13450
P13451
P13452
P13453
P13454
P13455
P13456
P13457
P13458
P13459
P13460
P13461
P13462
P13463
P13464
P13465
P13466
P13467
P13468
P13469
P13470
P13471
P13472
P13473
P13474
P13475
P13476
P13477
P13478
P13479
P13480
P13481
P13482
P13483
P13484
P13485
P13486
P13487
P13488
P13489
P13490
P13491
P13492
P13493
P13494
P13495
P13496
P13497
P13498
P13499
P13500
P13501
P13502
P13503
P13504
P13505
P13506
P13507
P13508
P13509
P13510
P13511
P13512
P13513
P13514
P13515
P13516
P13517
P13518
P13519
P13520
P13521
P13522
P13523
P13524
P13525
P13526
P13527
P13528
P13529
P13530
P13531
P13532
P13533
P13534
P13535
P13536
P13537
P13538
P13539
P13540
P13541
P13542
P13543
P13544
P13545
P13546
P13547
P13548
P13549
P13550
P13551
P13552
P13553
P13554
P13555
P13556
P13557
P13558
P13559
P13560
P13561
P13562
P13563
P13564
P13565
P13566
P13567
P13568
P13569
P13570
P13571
P13572
P13573
P13574
P13575
P13576
P13577
P13578
P13579
P13580
P13581
P13582
P13583
P13584
P13585
P13586
P13587
P13588
P13589
P13590
P13591
P13592
P13593
P13594
P13595
P13596
P13597
P13598
P13599
P13600
P13601
P13602
P13603
P13604
P13605
P13606
P13607
P13608
P13609
P13610
P13611
P13612
P13613
P13614
P13615
P13616
P13617
P13618
P13619
P13620
P13621
P13622
P13623
P13624
P13625
P13626
P13627
P13628
P13629
P13630
P13631
P13632
P13633
P13634
P13635
P13636
P13637
P13638
P13639
P13640
P13641
P13642
P13643
P13644
P13645
P13646
P13647
P13648
P13649
P13650
P13651
P13652
P13653
P13654
P13655
P13656
P13657
P13658
P13659
P13660
P13661
P13662
P13663
P13664
P13665
P13666
P13667
P13668
P13669
P13670
P13671
P13672
P13673
P13674
P13675
P13676
P13677
P13678
P13679
P13680
P13681
P13682
P13683
P13684
P13685
P13686
P13687
P13688
P13689
P13690
P13691
P13692
P13693
P13694
P13695
P13696
P13697
P13698
P13699
P13700
P13701
P13702
P13703
P13704
P13705
P13706
P13707
P13708
P13709
P13710
P13711
P13712
P13713
P13714
P13715
P13716
P13717
P13718
P13719
P13720
P13721
P13722
P13723
P13724
P13725
P13726
P13727
P13728
P13729
P13730
P13731
P13732
P13733
P13734
P13735
P13736
P13737
P13738
P13739
P13740
P13741
P13742
P13743
P13744
P13745
P13746
P13747
P13748
P13749
P13750
P13751
P13752
P13753
P13754
P13755
P13756
P13757
P13758
P13759
P13760
P13761
P13762
P13763
P13764
P13765
P13766
P13767
P13768
P13769
P13770
P13771
P13772
P13773
P13774
P13775
P13776
P13777
P13778
P13779
P13780
P13781
P13782
P13783
P13784
P13785
P13786
P13787
P13788
P13789
P13790
P13791
P13792
P13793
P13794
P13795
P13796
P13797
P13798
P13799
P13800
P13801
P13802
P13803
P13804
P13805
P13806
P13807
P13808
P13809
P13810
P13811
P13812
P13813
P13814
P13815
P13816
P13817
P13818
P13819
P13820
P13821
P13822
P13823
P13824
P13825
P13826
P13827
P13828
P13829
P13830
P13831
P13832
P13833
P13834
P13835
P13836
P13837
P13838
P13839
P13840
P13841
P13842
P13843
P13844
P13845
P13846
P13847
P13848
P13849
P13850
P13851
P13852
P13853
P13854
P13855
P13856
P13857
P13858
P13859
P13860
P13861
P13862
P13863
P13864
P13865
P13866
P13867
P13868
P13869
P13870
P13871
P13872
P13873
P13874
P13875
P13876
P13877
P13878
P13879
P13880
P13881
P13882
P13883
P13884
P13885
P13886
P13887
P13888
P13889
P13890
P13891
P13892
P13893
P13894
P13895
P13896
P13897
P13898
P13899
P13900
P13901
P13902
P13903
P13904
P13905
P13906
P13907
P13908
P13909
P13910
P13911
P13912
P13913
P13914
P13915
P13916
P13917
P13918
P13919
P13920
P13921
P13922
P13923
P13924
P13925
P13926
P13927
P13928
P13929
P13930
P13931
P13932
P13933
P13934
P13935
P13936
P13937
P13938
P13939
P13940
P13941
P13942
P13943
P13944
P13945
P13946
P13947
P13948
P13949
P13950
P13951
P13952
P13953
P13954
P13955
P13956
P13957
P13958
P13959
P13960
P13961
P13962
P13963
P13964
P13965
P13966
P13967
P13968
P13969
P13970
P13971
P13972
P13973
P13974
P13975
P13976
P13977
P13978
P13979
P13980
P13981
P13982
P13983
P13984
P13985
P13986
P13987
P13988
P13989
P13990
P13991
P13992
P13993
P13994
P13995
P13996
P13997
P13998
P13999
P14000
P14001
P14002
P14003
P14004
P14005
P14006
P14007
P14008
P14009
P14010
P14011
P14012
P14013
P14014
P14015
P14016
P14017
P14018
P14019
P14020
P14021
P14022
P14023
P14024
P14025
P14026
P14027
P14028
P14029
P14030
P14031
P14032
P14033
P14034
P14035
P14036
P14037
P14038
P14039
P14040
P14041
P14042
P14043
P14044
P14045
P14046
P14047
P14048
P14049
P14050
P14051
P14052
P14053
P14054
P14055
P14056
P14057
P14058
P14059
P14060
P14061
P14062
P14063
P14064
P14065
P14066
P14067
P14068
P14069
P14070
P14071
P14072
P14073
P14074
P14075
P14076
P14077
P14078
P14079
P14080
P14081
P14082
P14083
P14084
P14085
P14086
P14087
P14088
P14089
P14090
P14091
P14092
P14093
P14094
P14095
P14096
P14097
P14098
P14099
P14100
P14101
P14102
P14103
P14104
P14105
P14106
P14107
P14108
P14109
P14110
P14111
P14112
P14113
P14114
P14115
P14116
P14117
P14118
P14119
P14120
P14121
P14122
P14123
P14124
P14125
P14126
P14127
P14128
P14129
P14130
P14131
P14132
P14133
P14134
P14135
P14136
P14137
P14138
P14139
P14140
P14141
P14142
P14143
P14144
P14145
P14146
P14147
P14148
P14149
P14150
P14151
P14152
P14153
P14154
P14155
P14156
P14157
P14158
P14159
P14160
P14161
P14162
P14163
P14164
P14165
P14166
P14167
P14168
P14169
P14170
P14171
P14172
P14173
P14174
P14175
P14176
P14177
P14178
P14179
P14180
P14181
P14182
P14183
P14184
P14185
P14186
P14187
P14188
P14189
P14190
P14191
P14192
P14193
P14194
P14195
P14196
P14197
P14198
P14199
P14200
P14201
P14202
P14203
P14204
P14205
P14206
P14207
P14208
P14209
P14210
P14211
P14212
P14213
P14214
P14215
P14216
P14217
P14218
P14219
P14220
P14221
P14222
P14223
P14224
P14225
P14226
P14227
P14228
P14229
P14230
P14231
P14232
P14233
P14234
P14235
P14236
P14237
P14238
P14239
P14240
P14241
P14242
P14243
P14244
P14245
P14246
P14247
P14248
P14249
P14250
P14251
P14252
P14253
P14254
P14255
P14256
P14257
P14258
P14259
P14260
P14261
P14262
P14263
P14264
P14265
P14266
P14267
P14268
P14269
P14270
P14271
P14272
P14273
P14274
P14275
P14276
P14277
P14278
P14279
P14280
P14281
P14282
P14283
P14284
P14285
P14286
P14287
P14288
P14289
P14290
P14291
P14292
P14293
P14294
P14295
P14296
P14297
P14298
P14299
P14300
P14301
P14302
P14303
P14304
P14305
P14306
P14307
P14308
P14309
P14310
P14311
P14312
P14313
P14314
P14315
P14316
P14317
P14318
P14319
P14320
P14321
P14322
P14323
P14324
P14325
P14326
P14327
P14328
P14329
P14330
P14331
P14332
P14333
P14334
P14335
P14336
P14337
P14338
P14339
P14340
P14341
P14342
P14343
P14344
P14345
P14346
P14347
P14348
P14349
P14350
P14351
P14352
P14353
P14354
P14355
P14356
P14357
P14358
P14359
P14360
P14361
P14362
P14363
P14364
P14365
P14366
P14367
P14368
P14369
P14370
P14371
P14372
P14373
P14374
P14375
P14376
P14377
P14378
P14379
P14380
P14381
P14382
P14383
P14384
P14385
P14386
P14387
P14388
P14389
P14390
P14391
P14392
P14393
P14394
P14395
P14396
P14397
P14398
P14399
P14400
P14401
P14402
P14403
P14404
P14405
P14406
P14407
P14408
P14409
P14410
P14411
P14412
P14413
P14414
P14415
P14416
P14417
P14418
P14419
P14420
P14421
P14422
P14423
P14424
P14425
P14426
P14427
P14428
P14429
P14430
P14431
P14432
P14433
P14434
P14435
P14436
P14437
P14438
P14439
P14440
P14441
P14442
P14443
P14444
P14445
P14446
P14447
P14448
P14449
P14450
P14451
P14452
P14453
P14454
P14455
P14456
P14457
P14458
P14459
P14460
P14461
P14462
P14463
P14464
P14465
P14466
P14467
P14468
P14469
P14470
P14471
P14472
P14473
P14474



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

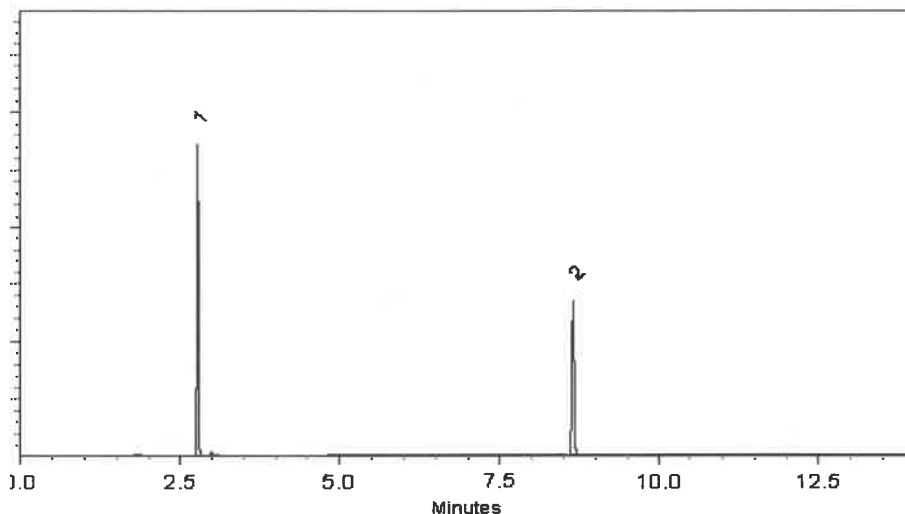


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024

Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

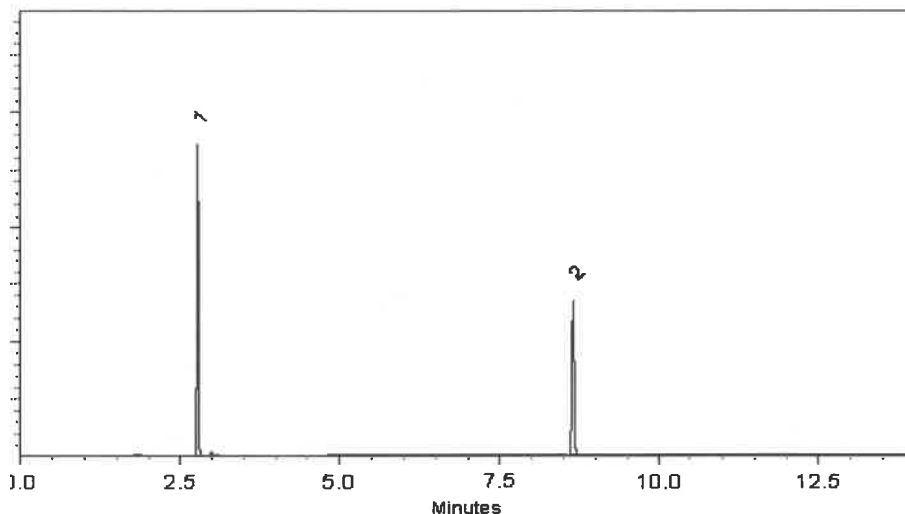


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

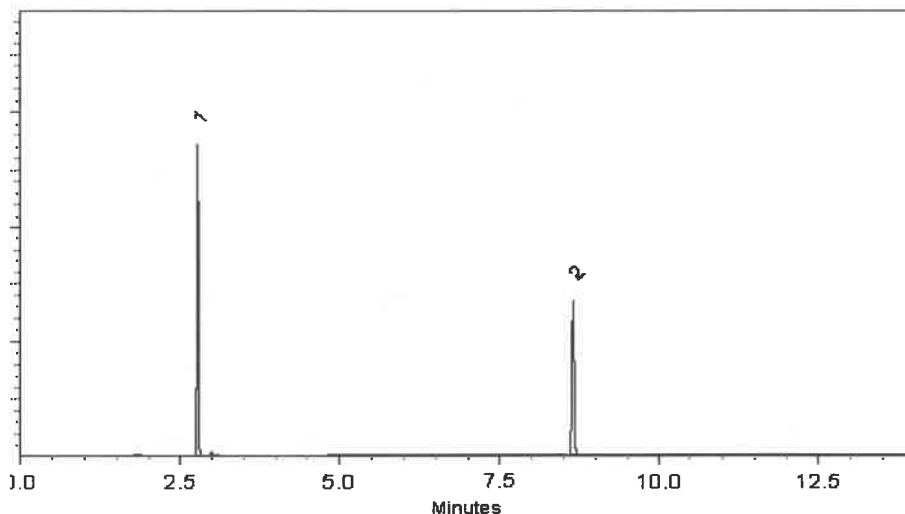


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32005 **Lot No.:** A0203038

Description : Toxaphene Standard

Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2028 **Storage:** 10°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Toxaphene	8001-35-2	1051817	----%	1,009.0 µg/mL	+/- 55.9920

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 13358
↓
P 13369
(12)

✓
05-06-2024

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

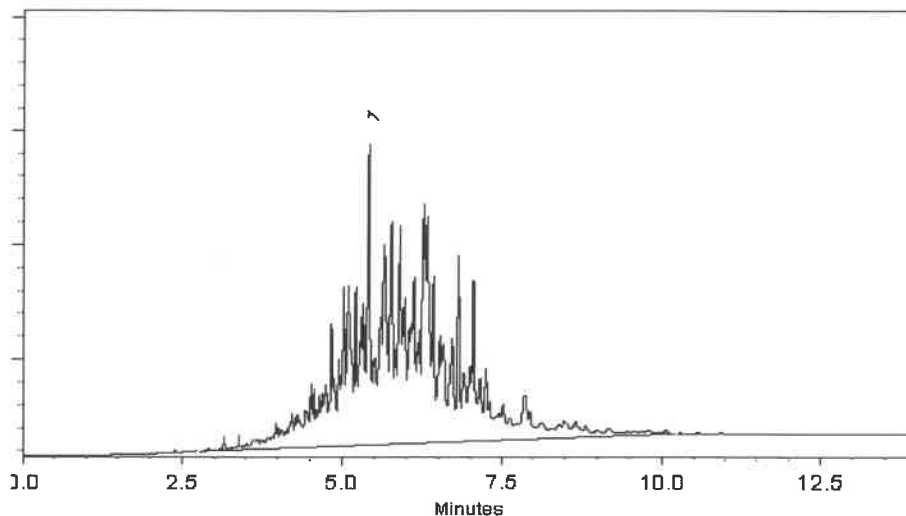

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 10-Oct-2023

Balance Serial # 1128353505


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P13358
↓
P13369
↓
(12)


05-06-2024



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32005 **Lot No.:** A0203038

Description : Toxaphene Standard
Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2028 **Storage:** 10°C or colder
Ship: Ambient

P13402
P13406
5/22/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Toxaphene	8001-35-2	1051817	---%	1,009.0 µg/mL	+/- 55.9920

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

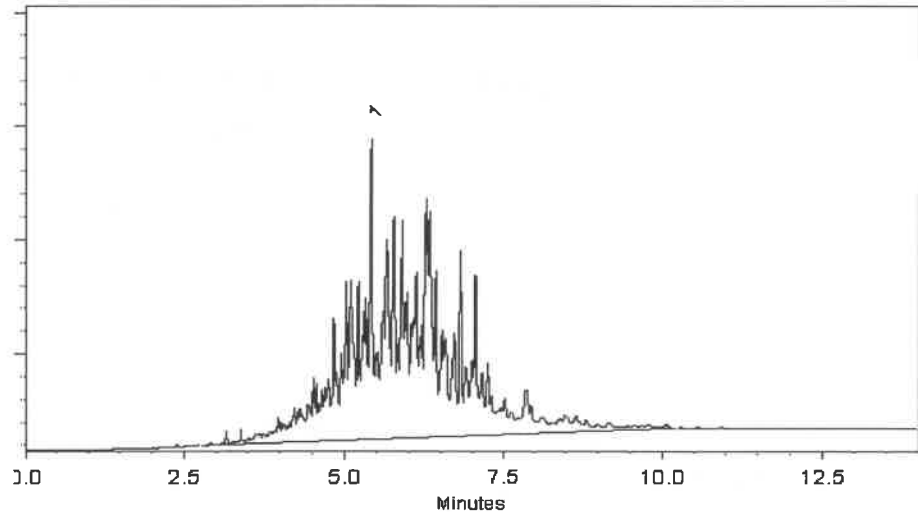


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 10-Oct-2023

Balance Serial # 1128353505


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P13402
↓
P13406 } (5)

5/22/2024



SHIPPING DOCUMENTS

CHEMTECH

CHAIN OF CUSTODY RECORD

284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 • Fax (908) 789-8922
www.chemtech.net

CHEMTECH PROJECT NO.

QUOTE NO.

COC Number

2042038

P4578/79

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: GANNETT FLEMING
ADDRESS: 1010 Adams Avenue
CITY: Audubon STATE: PA ZIP: 19408
ATTENTION: JOE Krupansky
PHONE: 610-301-8342 FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Amtrak's rep. of SB
PROJECT NO.: 95000088 LOCATION: Kearny, NJ
PROJECT MANAGER: JOE Krupansky
e-mail: QAQC@bomys.com
PHONE: 610-301-8342 FAX:

CLIENT BILLING INFORMATION

BILL TO: chemtech PO#:
ADDRESS: 284 Sheffield St.
CITY: Mountainside STATE: NJ ZIP: 07092
ATTENTION: Samantha PHONE: 908-789-298

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) _____ DAYS*
HARDCOPY (DATA PACKAGE): 10 DAYS*
EDD: 10 DAYS*

*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☒ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other
☐ EDD FORMAT BEN EDD

TECH VOC TO
TECH PAH
PCB'S
CHLORINATED
TAA Metals
EPH
TCLP-FULL
PCRA Parameters
TOX

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS		
			COMP	GRAB	DATE	TIME		A			F	B							← Specify Preservatives
1	2	3	4	5	6	7	8	9	A-HCl	D-NaOH									
																	B-HNO3	E-ICE	
																	C-H2SO4	F-OTHER	
1.	NB-305-SW	GW	X		10/25	8:20	7	X	X	X	X	X	X						
2.	NB-305-SW-1	GW	X		10/25	8:30	7	X	X	X	X	X	X						
3.	NB-305-Top	S	X		10/25	9:20	11	X	X	X	X	X	X						
4.	NB-305-Top-1	S	X		10/25	9:30	11	X	X	X	X	X	X						
5.	NB-305-Bot	S	X		10/25	11:15	11	X	X	X	X	X	X	X	X	X			
6.	NB-305-Bot-1.	S	X		10/25	11:20	11	X	X	X	X	X	X	X	X	X			
7.	FB-10252024.	DIW.			10/25		2	X											
8.																			
9.																			
10.																			

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. Yvonda Pujara	DATE/TIME: 10/25/24-3:11	RECEIVED BY: 1. [Signature]	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☒ COOLER TEMP 3.1°C Comments:
RELINQUISHED BY SAMPLER: 2. [Signature]	DATE/TIME: 10.25.2024	RECEIVED BY: 2. [Signature]	
RELINQUISHED BY SAMPLER: 3. [Signature]	DATE/TIME: 10.25.2024	RECEIVED BY: 3. [Signature]	

Page ____ of ____

CLIENT: ☐ Hand Delivered ☐ Other
CHEMTECH: ☐ Picked Up ☐ Field Sampling

Shipment Complete
☐ YES ☐ NO



284 Sheffield Street, Mountainside NJ 07092 (908)-789-8900 Fax : 908 789 8922

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

LOGIN REPORT/SAMPLE TRANSFER

Order ID : P4578	PORT06	Order Date : 10/25/2024 3:58:00 PM	Project Mgr :
Client Name : Portal Partners Tri-Venture		Project Name : Amtrak Sawtooth Bridges 2	Report Type : NJ Reduced
Client Contact : Joseph Krupansky		Receive DateTime : 10/25/2024 4:04:00 PM	EDD Type : EXCEL NJCLEANUP
Invoice Name : Portal Partners Tri-Venture		Purchase Order :	Hard Copy Date :
Invoice Contact : Joseph Krupansky			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
P4578-01	WB-305-SW	Water	10/25/2024	08:20	VOC-TCLVOA-10		8260-Low		10 Bus. Days
P4578-02	WB-305-SW-1	Water	10/25/2024	08:30	VOC-TCLVOA-10		8260-Low		10 Bus. Days
P4578-03	WB-305-TOP	Solid	10/25/2024	09:20	VOC-TCLVOA-10		8260D		10 Bus. Days
P4578-04	WB-305-TOP-1	Solid	10/25/2024	09:30	VOC-TCLVOA-10		8260D		10 Bus. Days
P4578-05	WB-305-BOT	Solid	10/25/2024	11:15	VOC-TCLVOA-10		8260D		10 Bus. Days
P4578-07	WB-305-BOT-1	Solid	10/25/2024	11:20	VOC-TCLVOA-10		8260D		10 Bus. Days
P4578-09	TB-10252024	Water	10/25/2024	00:00	VOC-TCLVOA-10		8260-Low		10 Bus. Days

LOGIN REPORT/SAMPLE TRANSFER

Order ID : P4578	PORT06	Order Date : 10/25/2024 3:58:00 PM	Project Mgr :
Client Name : Portal Partners Tri-Venture		Project Name : Amtrak Sawtooth Bridges 2	Report Type : NJ Reduced
Client Contact : Joseph Krupansky		Receive DateTime : 10/25/2024 4:04:00 PM	EDD Type : EXCEL NJCLEANUP
Invoice Name : Portal Partners Tri-Venture		Purchase Order :	Hard Copy Date :
Invoice Contact : Joseph Krupansky			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
--------	-----------	--------	-------------	-------------	------	------------	--------	----------	-----------

* J.C samples are in sm Refrigerator *

Relinquished By :

J.C.

Date / Time :

10-25-2024 1710

Received By :

Sam
10/25/2024 17:10

Date / Time :

Sam

Storage Area : VOA Refridgerator Room

Rg 6
122
Rg 45