

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
 Data File : BE101397.D
 Acq On : 28 Oct 2024 16:37
 Operator : RC/JU
 Sample : SSTDICV040
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 ICVBE102824

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/29/2024
 Supervised By :mohammad ahmed 10/30/2024

Quant Time: Oct 29 01:28:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 29 01:26:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.570	152	135975	20.000	ng	0.00
21) Naphthalene-d8	10.343	136	689556	20.000	ng	0.00
39) Acenaphthene-d10	14.186	164	494390	20.000	ng	0.00
64) Phenanthrene-d10	16.918	188	1118107	20.000	ng	0.00
76) Chrysene-d12	21.077	240	1178888	20.000	ng	0.00
86) Perylene-d12	23.369	264	1506294	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.319	112	642682	82.839	ng	0.00
7) Phenol-d6	6.953	99	943928	87.746	ng	0.00
23) Nitrobenzene-d5	8.786	82	931158	84.816	ng	0.00
42) 2,4,6-Tribromophenol	15.690	330	730631	84.319	ng	0.00
45) 2-Fluorobiphenyl	12.805	172	2410105	82.558	ng	0.00
79) Terphenyl-d14	19.515	244	4018242	78.448	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.204	88	112859	39.003	ng	99
3) Pyridine	3.639	79	342567m	41.845	ng	
4) n-Nitrosodimethylamine	3.557	42	131547	41.530	ng	99
6) Aniline	7.012	93	381702m	46.299	ng	
8) 2-Chlorophenol	7.217	128	394111	42.354	ng	99
9) Benzaldehyde	6.782	77	243959	46.978	ng	98
10) Phenol	6.976	94	524973	44.977	ng	99
11) bis(2-Chloroethyl)ether	7.041	93	352789	36.844	ng	99
12) 1,3-Dichlorobenzene	7.458	146	407554	40.619	ng	99
13) 1,4-Dichlorobenzene	7.605	146	416170	40.617	ng	99
14) 1,2-Dichlorobenzene	7.934	146	416666	41.544	ng	99
15) Benzyl Alcohol	7.916	79	280441	43.735	ng	100
16) 2,2'-oxybis(1-Chloropr...	8.075	45	504614	41.877	ng	96
17) 2-Methylphenol	8.157	107	338367	42.832	ng	100
18) Hexachloroethane	8.627	117	140124	41.877	ng	97
19) n-Nitroso-di-n-propyla...	8.375	70	334804	46.901	ng	98
20) 3+4-Methylphenols	8.492	107	482425	44.240	ng	96
22) Acetophenone	8.422	105	658880	42.082	ng	99
24) Nitrobenzene	8.827	77	486233	41.612	ng	98
25) Isophorone	9.280	82	923963	43.128	ng	99
26) 2-Nitrophenol	9.509	139	247215	43.773	ng	99
27) 2,4-Dimethylphenol	9.632	122	296382	41.704	ng	99
28) bis(2-Chloroethoxy)met...	9.779	93	543065	41.799	ng	99
29) 2,4-Dichlorophenol	10.061	162	413366	42.044	ng	100
30) 1,2,4-Trichlorobenzene	10.184	180	432858	40.415	ng	99
31) Naphthalene	10.390	128	1427648	40.628	ng	100
32) Benzoic acid	9.896	122	280040	39.965	ng	99
33) 4-Chloroaniline	10.613	127	560356	45.859	ng	99
34) Hexachlorobutadiene	10.637	225	255945	40.372	ng	99
35) Caprolactam	11.395	113	166215	44.104	ng	98
36) 4-Chloro-3-methylphenol	11.788	107	479680	42.850	ng	99
37) 2-Methylnaphthalene	11.976	142	1040801	41.112	ng	99
38) 1-Methylnaphthalene	12.206	142	1039012	41.122	ng	99
40) 1,2,4,5-Tetrachloroben...	12.335	216	508563	40.977	ng	100
41) Hexachlorocyclopentadiene	12.317	237	169665	41.393	ng	99
43) 2,4,6-Trichlorophenol	12.658	196	369991	43.244	ng	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
 Data File : BE101397.D
 Acq On : 28 Oct 2024 16:37
 Operator : RC/JU
 Sample : SSTDICV040
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 ICVBE102824

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/29/2024
 Supervised By :mohammad ahmed 10/30/2024

Quant Time: Oct 29 01:28:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 29 01:26:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 2,4,5-Trichlorophenol	12.758	196	417164	42.577	ng	100
46) 1,1'-Biphenyl	13.010	154	1390011	41.038	ng	99
47) 2-Chloronaphthalene	13.057	162	1102426	41.196	ng	99
48) 2-Nitroaniline	13.386	65	326383	45.320	ng	99
49) Acenaphthylene	13.915	152	1651908	41.742	ng	99
50) Dimethylphthalate	13.692	163	1435201	41.126	ng	100
51) 2,6-Dinitrotoluene	13.827	165	339386	42.124	ng	97
52) Acenaphthene	14.244	154	1064171	41.182	ng	99
53) 3-Nitroaniline	14.233	138	354038	44.191	ng	99
54) 2,4-Dinitrophenol	14.368	184	204189	38.780	ng	98
55) Dibenzofuran	14.591	168	1676523	40.705	ng	99
56) 4-Nitrophenol	14.650	139	305994	41.707	ng	99
57) 2,4-Dinitrotoluene	14.609	165	480487	43.318	ng	99
58) Fluorene	15.225	166	1418626	41.173	ng	99
59) 2,3,4,6-Tetrachlorophenol	14.855	232	384198	42.441	ng	99
60) Diethylphthalate	15.014	149	1493405	40.913	ng	100
61) 4-Chlorophenyl-phenyle...	15.214	204	701783	41.046	ng	99
62) 4-Nitroaniline	15.419	138	385584	43.251	ng	99
63) Azobenzene	15.508	77	1304082	41.563	ng	99
65) 4,6-Dinitro-2-methylph...	15.349	198	274306	41.750	ng	99
66) n-Nitrosodiphenylamine	15.466	169	1234319	41.628	ng	99
67) 4-Bromophenyl-phenylether	16.101	248	491891	41.822	ng	96
68) Hexachlorobenzene	16.207	284	643314	41.729	ng	97
69) Atrazine	16.395	200	406439	44.711	ng	100
70) Pentachlorophenol	16.612	266	397449	44.788	ng	98
71) Phenanthrene	16.959	178	2206489	41.217	ng	100
72) Anthracene	17.047	178	2193019	41.954	ng	99
73) Carbazole	17.376	167	2216213	41.436	ng	100
74) Di-n-butylphthalate	17.822	149	2524597	42.876	ng	100
75) Fluoranthene	18.962	202	2654890	40.831	ng	99
77) Benzidine	19.221	184	902385	60.311	ng	100
78) Pyrene	19.332	202	2798951	43.174	ng	100
80) Butylbenzylphthalate	20.184	149	1229626	43.265	ng	99
81) Benzo(a)anthracene	21.060	228	2796518	42.205	ng	100
82) 3,3'-Dichlorobenzidine	21.036	252	1140565	43.941	ng	100
83) Chrysene	21.113	228	2666843	41.627	ng	99
84) Bis(2-ethylhexyl)phtha...	20.889	149	1683088	44.579	ng	99
85) Di-n-octyl phthalate	21.736	149	2752236	44.414	ng	100
87) Indeno(1,2,3-cd)pyrene	25.696	276	4140658	41.075	ng	100
88) Benzo(b)fluoranthene	22.658	252	3307474	42.134	ng	99
89) Benzo(k)fluoranthene	22.705	252	3044393	41.512	ng	99
90) Benzo(a)pyrene	23.257	252	2880588	41.960	ng	100
91) Dibenzo(a,h)anthracene	25.684	278	3469403	41.651	ng	99
92) Benzo(g,h,i)perylene	26.442	276	3517606	40.986	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
Data File : BE101397.D
Acq On : 28 Oct 2024 16:37
Operator : RC/JU
Sample : SSTDICV040
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

ICVBE102824


Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 10/29/2024

Supervised By :mohammad ahmed 10/30/2024

Quant Time: Oct 29 01:28:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

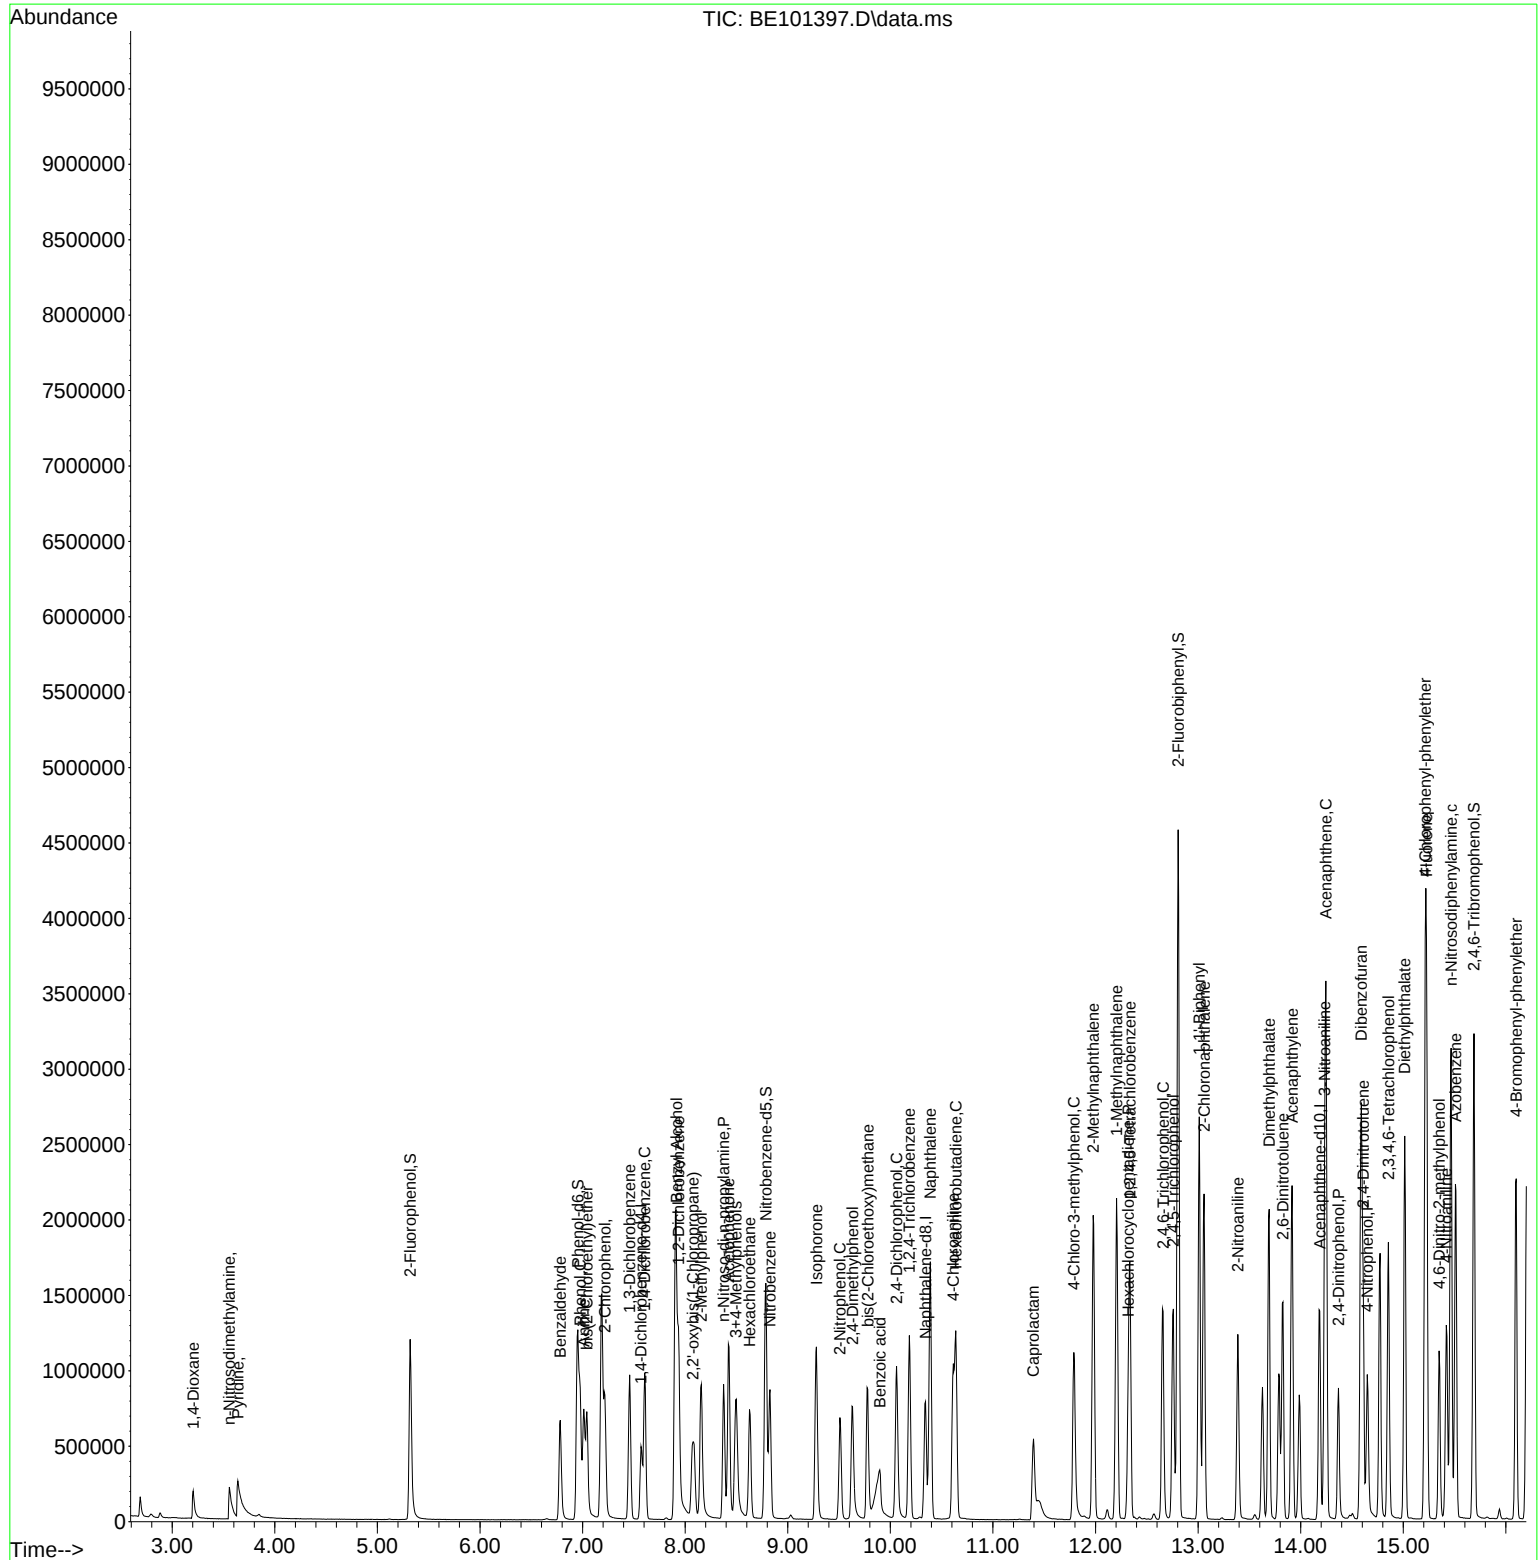

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
Data File : BE101397.D
Acq On : 28 Oct 2024 16:37
Operator : RC/JU
Sample : SSTDICV040
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
ICVBE102824

Quant Time: Oct 29 01:28:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2024
Supervised By :mohammad ahmed 10/30/2024

