
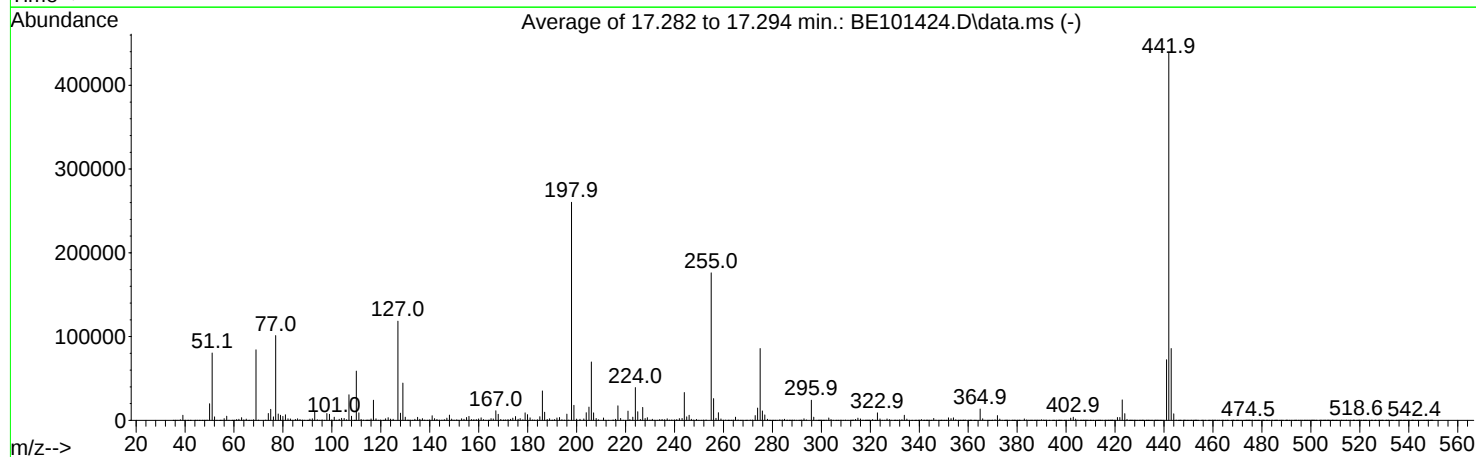


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101424.D
Acq On : 31 Oct 2024 9:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 29 01:26:30 2024

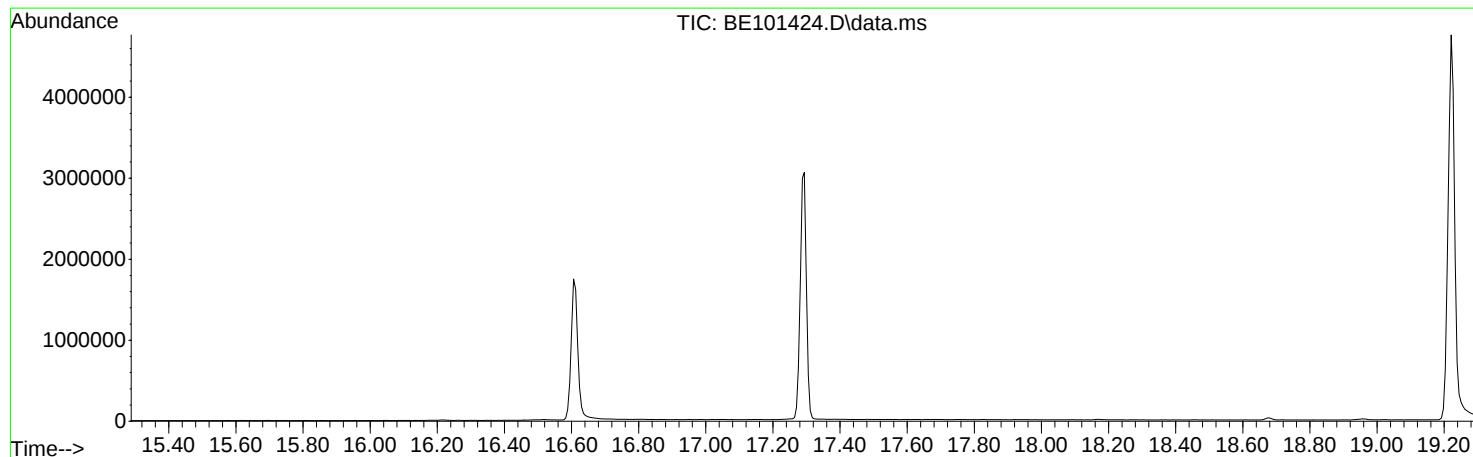




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	80401	PASS
68	69	0.00	2	0.8	691	PASS
69	198	0.00	100	32.4	84267	PASS
70	69	0.00	2	0.5	389	PASS
127	198	10	80	45.5	118439	PASS
197	198	0.00	2	0.2	400	PASS
198	198	100	100	100.0	260309	PASS
199	198	5	9	6.9	17941	PASS
275	198	10	60	32.9	85684	PASS
365	198	1	100	5.2	13582	PASS
441	198	0.01	100	27.8	72413	PASS
442	442	50	100	100.0	439142	PASS
443	442	15	24	19.6	85860	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101424.D
Acq On : 31 Oct 2024 9:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Oct 31 18:55:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

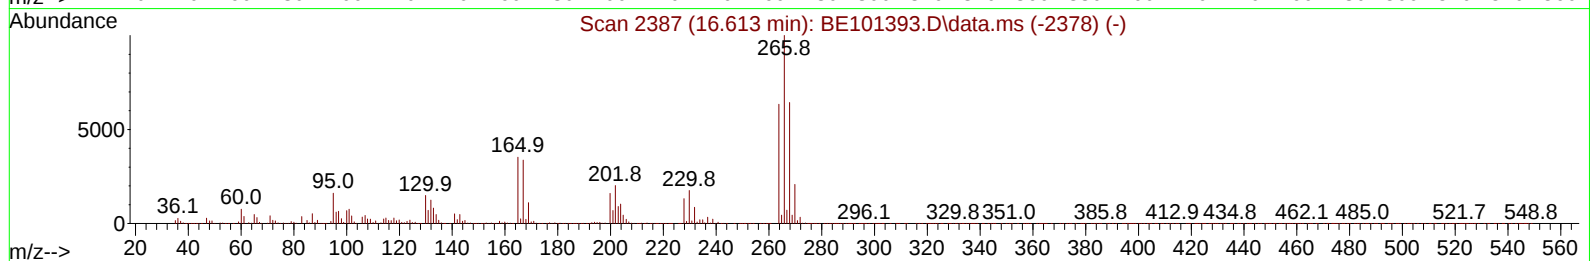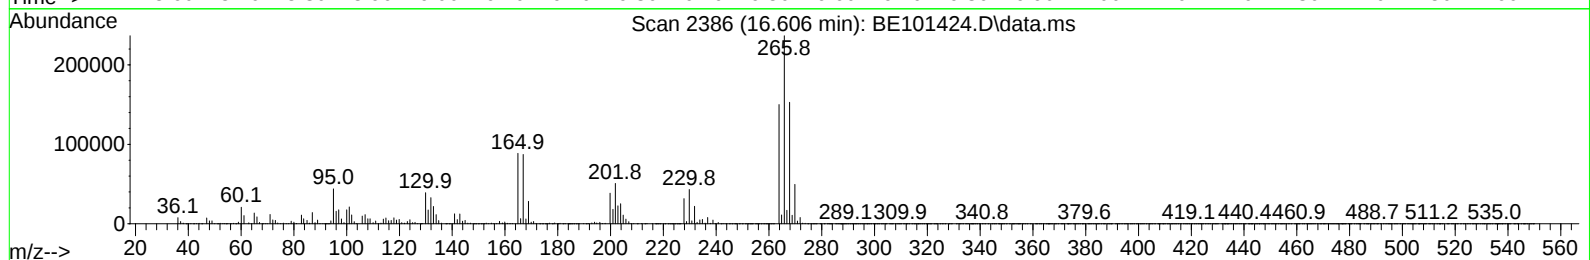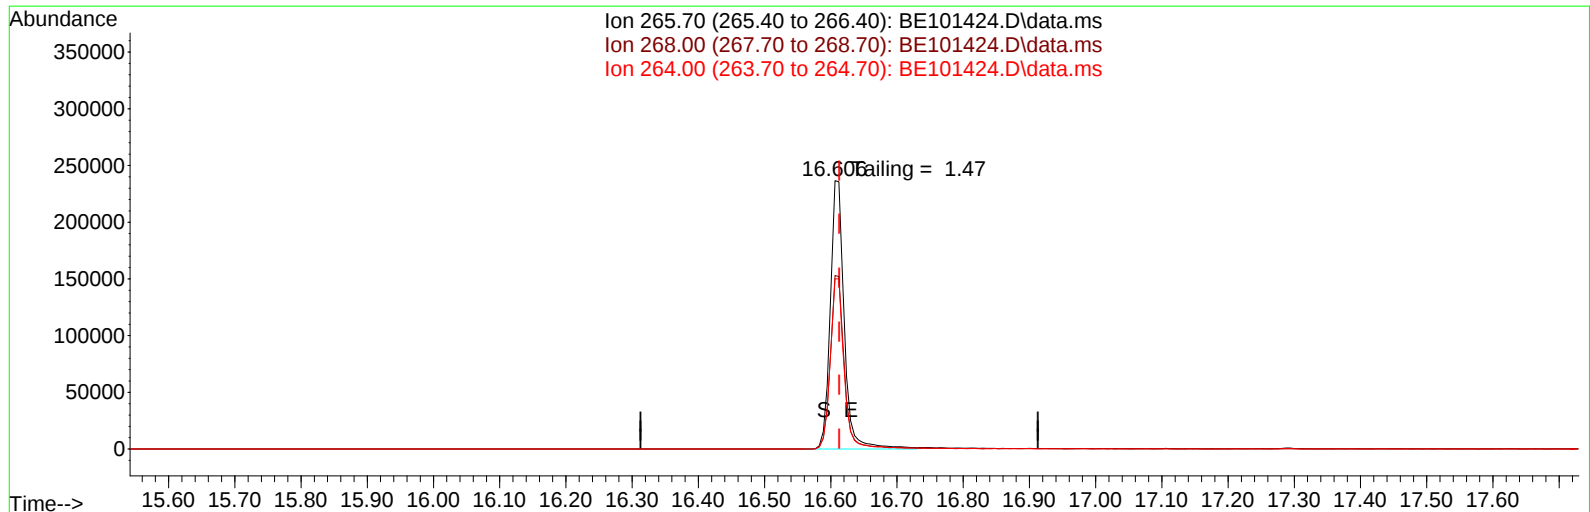

TIC: BE101424.D\data.ms

(70) Pentachlorophenol (C)

16.606min (-0.007) 35129.78 ng




response 348516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.63
264.00	63.40	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
 Data File : BE101424.D
 Acq On : 31 Oct 2024 9:40
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Oct 31 18:55:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 29 01:26:30 2024
 Response via : Initial Calibration

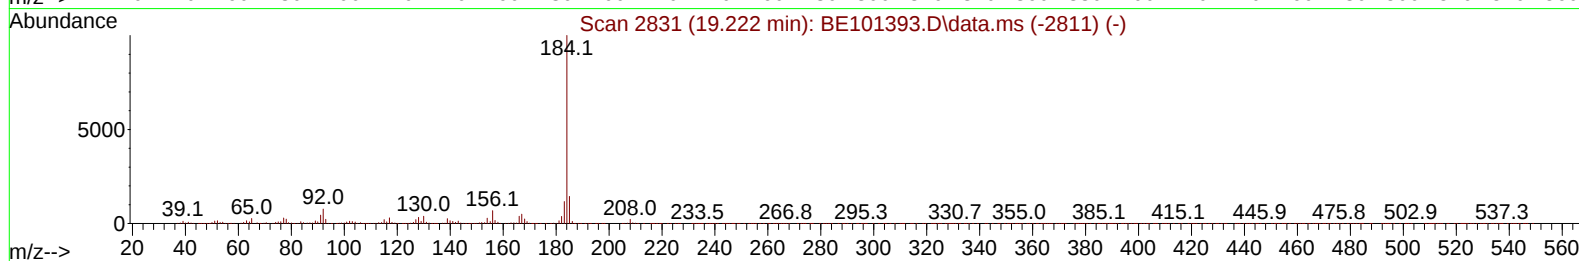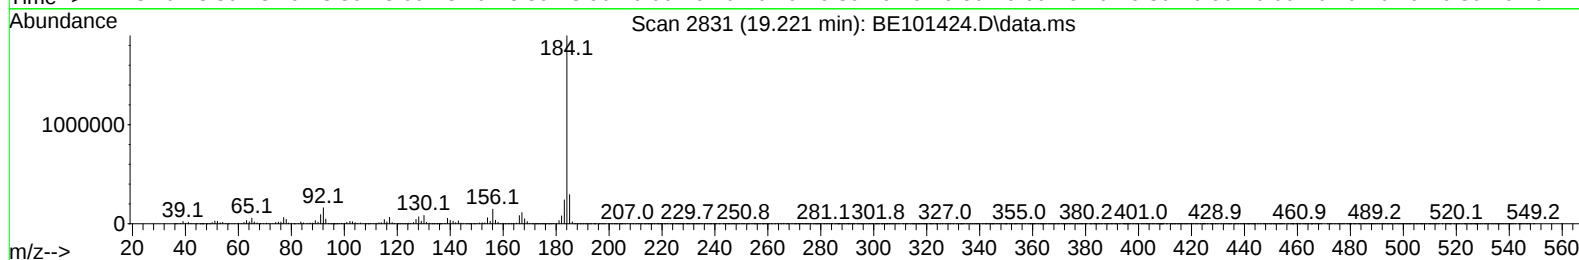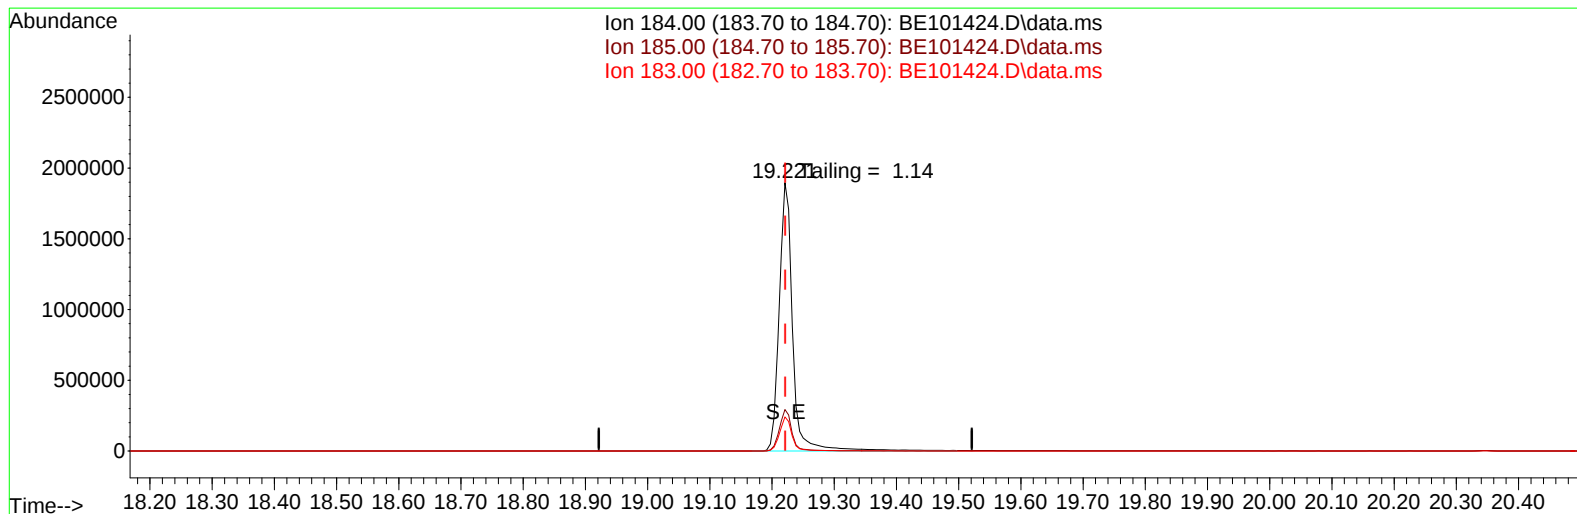

TIC: BE101424.D\data.ms

(77) Benzidine

19.221min (-0.001) 20555.57 ng

response 2867124

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.47
183.00	11.60	12.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/31/2024	BNA_E	<u>BE101424.D</u>
Compound Name	Response	Retention Time
DDT	1107960	20.349
DDD	32485	19.914
DDE	1234	19.403
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33719	1141679	2.95

Instrument :
BNA_E
ClientSampleId :
DFTPP