
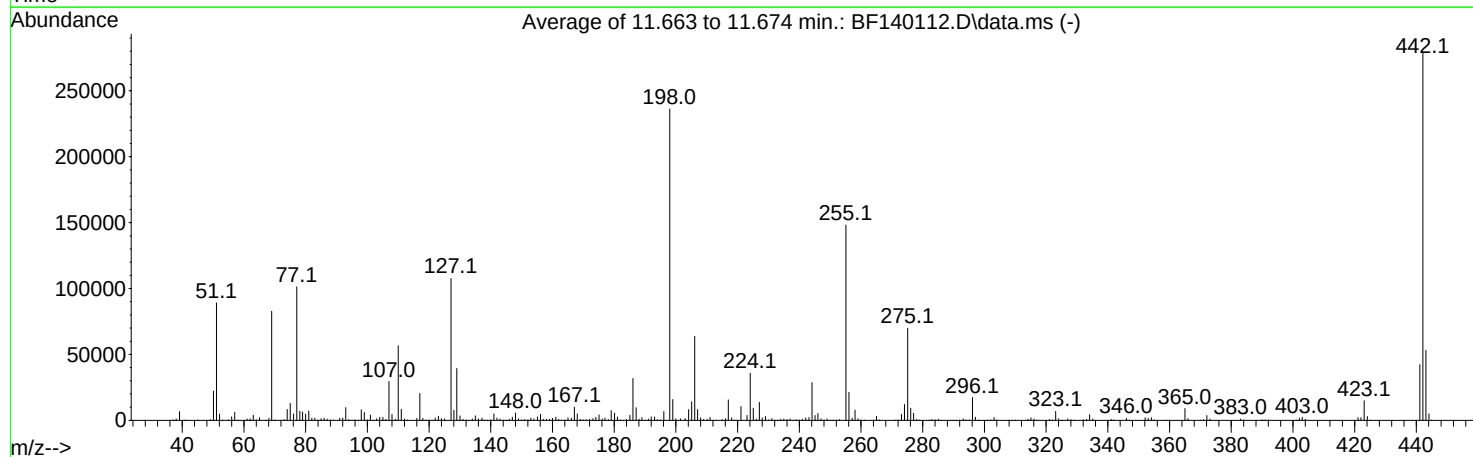


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140112.D
Acq On : 29 Oct 2024 15:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

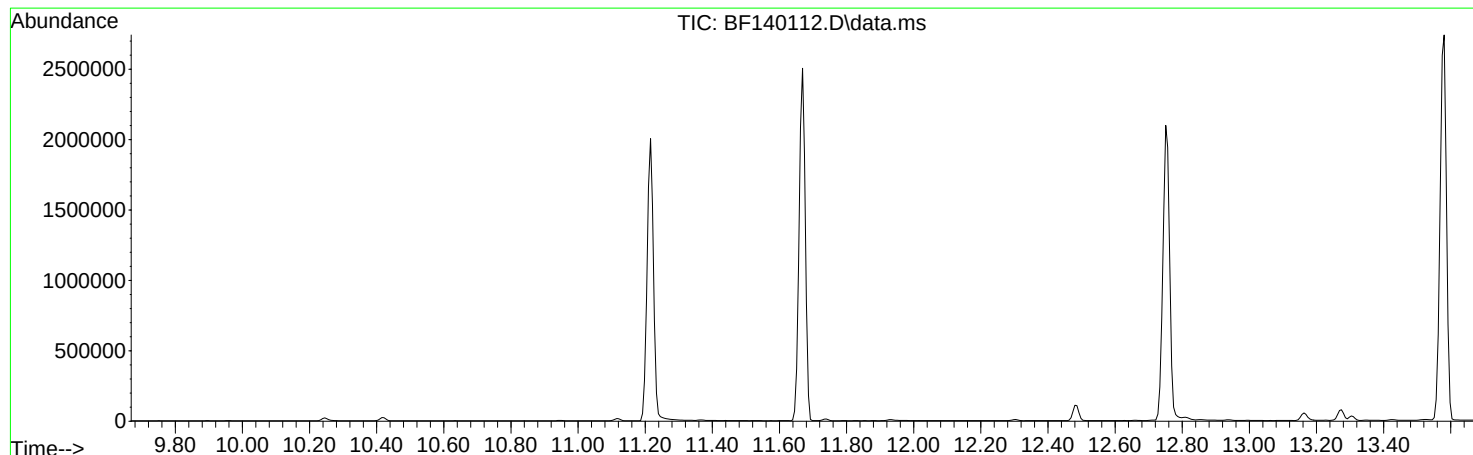




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	89133	PASS
68	69	0.00	2	1.9	1537	PASS
69	198	0.00	100	35.1	82843	PASS
70	69	0.00	2	0.5	379	PASS
127	198	10	80	45.6	107720	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	236160	PASS
199	198	5	9	6.7	15805	PASS
275	198	10	60	29.6	69907	PASS
365	198	1	100	3.8	8929	PASS
441	198	0.01	100	17.9	42256	PASS
442	442	50	100	100.0	279061	PASS
443	442	15	24	19.1	53197	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140112.D
Acq On : 29 Oct 2024 15:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 29 16:07:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

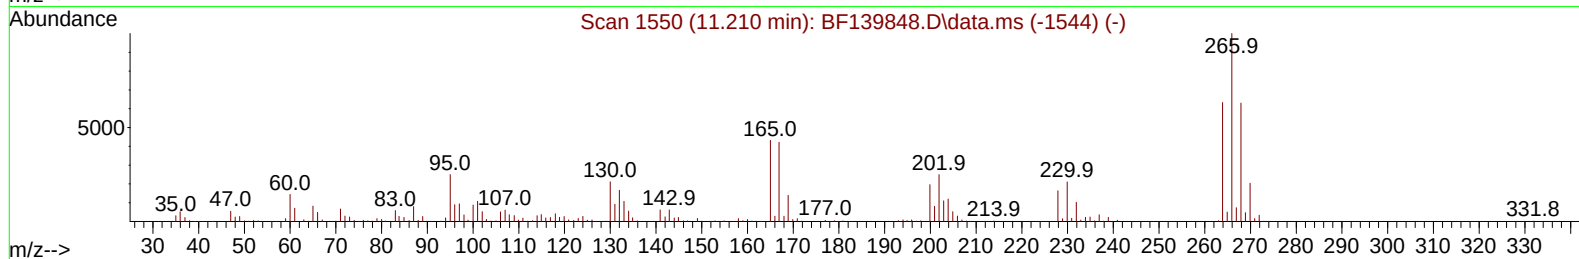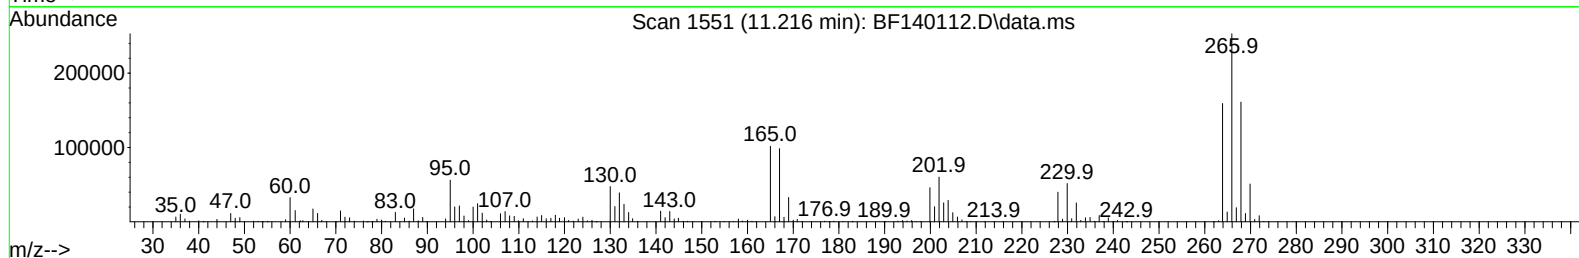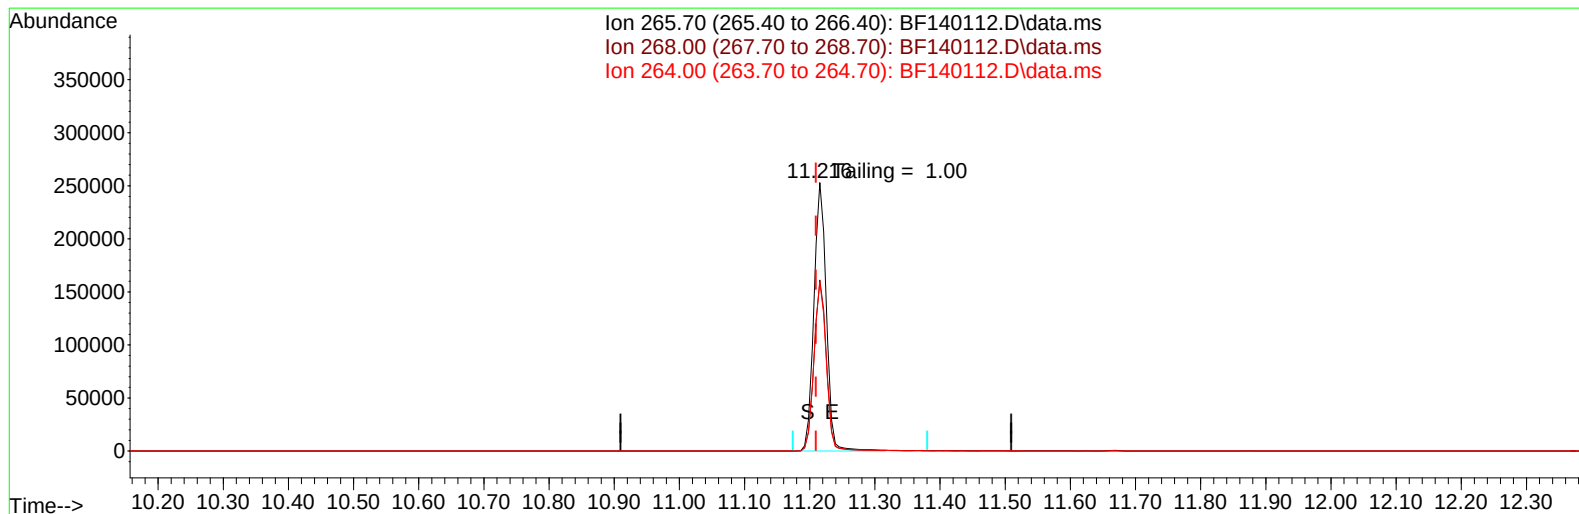

TIC: BF140112.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 107927.56 ng




response 336959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.70
264.00	63.20	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102924\
Data File : BF140112.D
Acq On : 29 Oct 2024 15:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 29 16:07:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

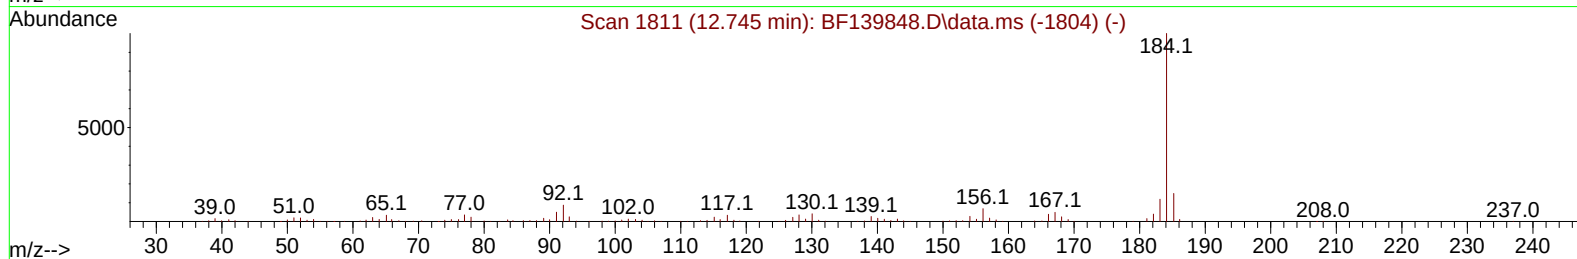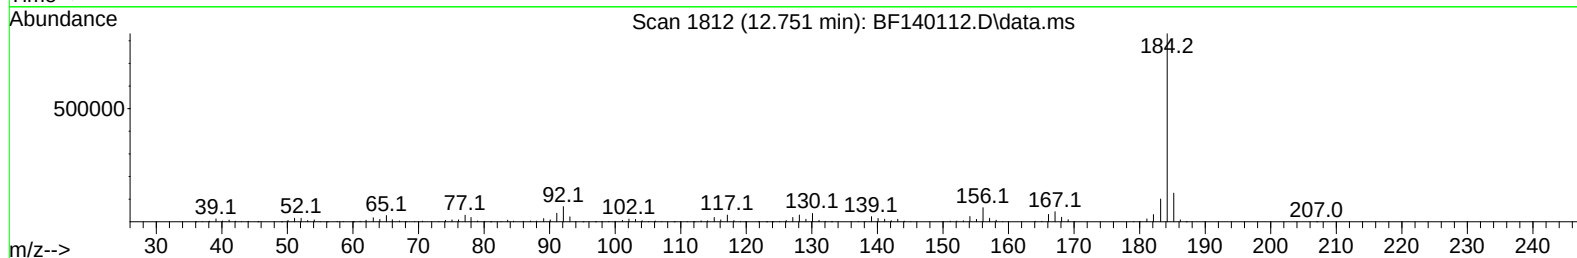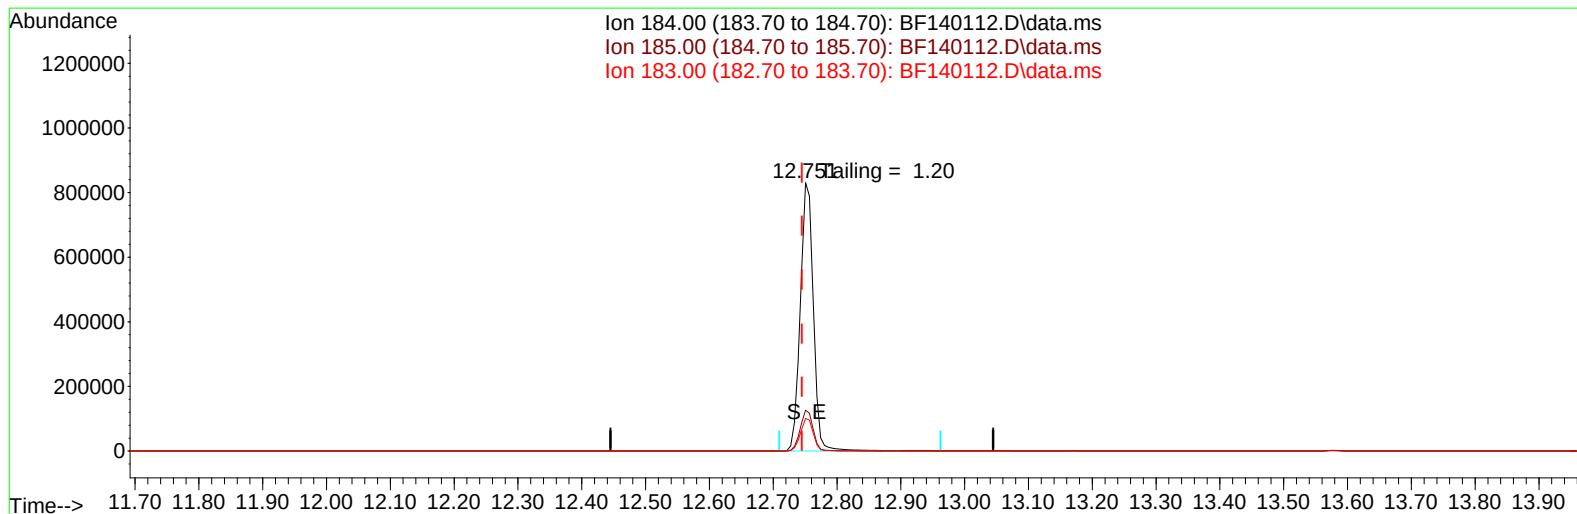

TIC: BF140112.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 174264.48 ng

response 1186317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.23
183.00	11.80	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/29/2024	BNA_F	<u>BF140112.D</u>
Compound Name	Response	Retention Time
DDT	730796	13.58
DDD	10774	13.304
DDE	1439	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12213	743009	1.64

Instrument :
BNA_F
ClientSampleId :
DFTPP