
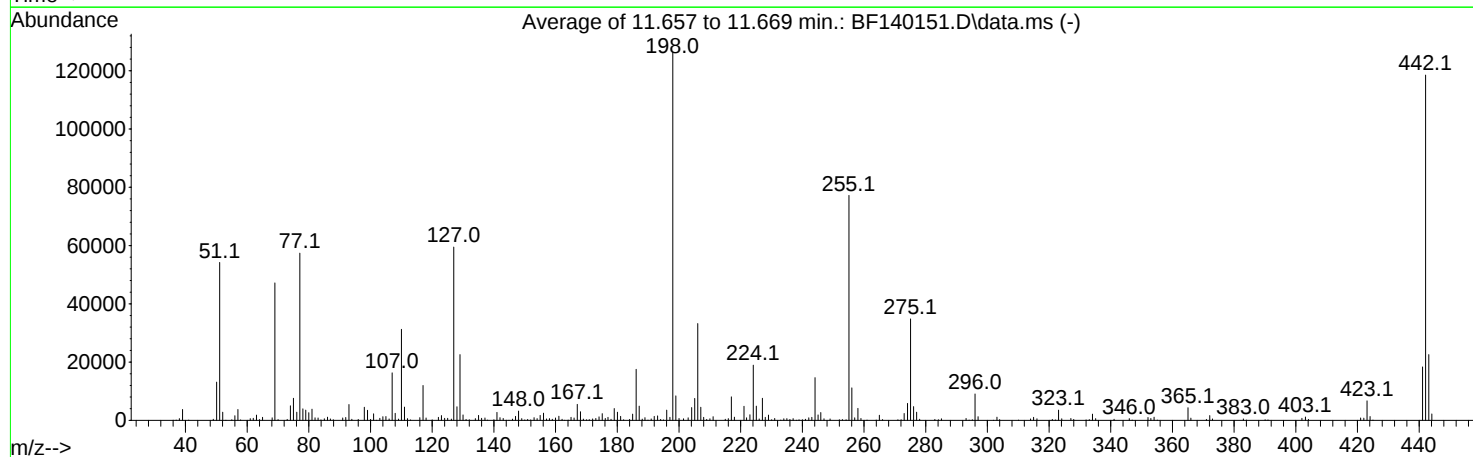


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103024\
Data File : BF140151.D
Acq On : 30 Oct 2024 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

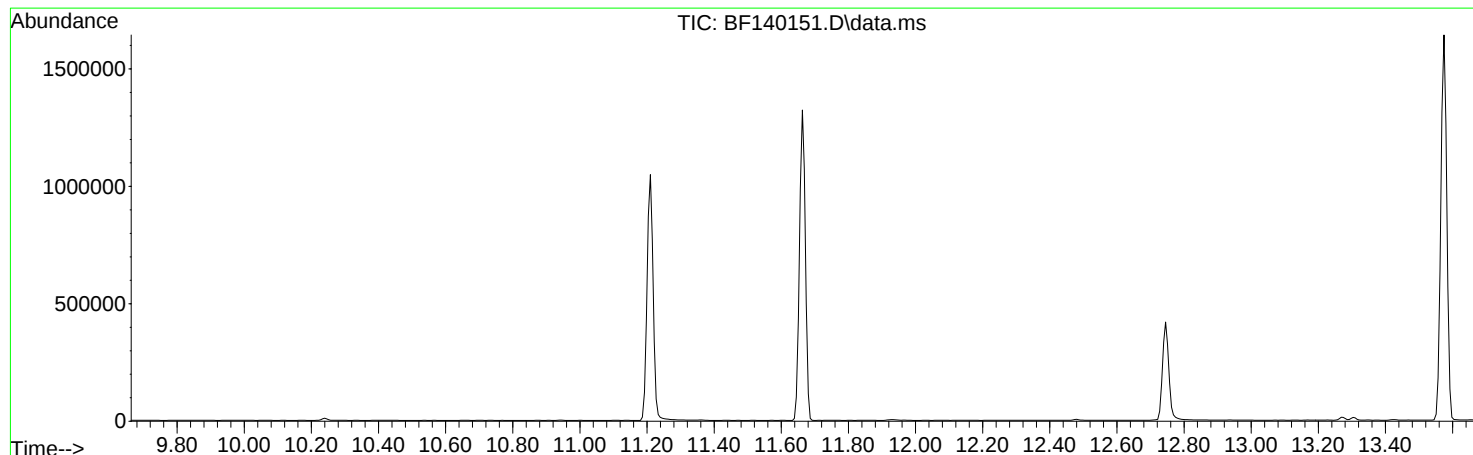


AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	54205	PASS
68	69	0.00	2	1.9	911	PASS
69	198	0.00	100	37.4	47179	PASS
70	69	0.00	2	0.6	260	PASS
127	198	10	80	47.1	59464	PASS
197	198	0.00	2	0.8	1062	PASS
198	198	100	100	100.0	126277	PASS
199	198	5	9	6.7	8423	PASS
275	198	10	60	27.6	34829	PASS
365	198	1	100	3.4	4328	PASS
441	198	0.01	100	14.5	18370	PASS
442	442	50	100	100.0	118523	PASS
443	442	15	24	19.1	22598	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103024\
Data File : BF140151.D
Acq On : 30 Oct 2024 11:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 30 13:37:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

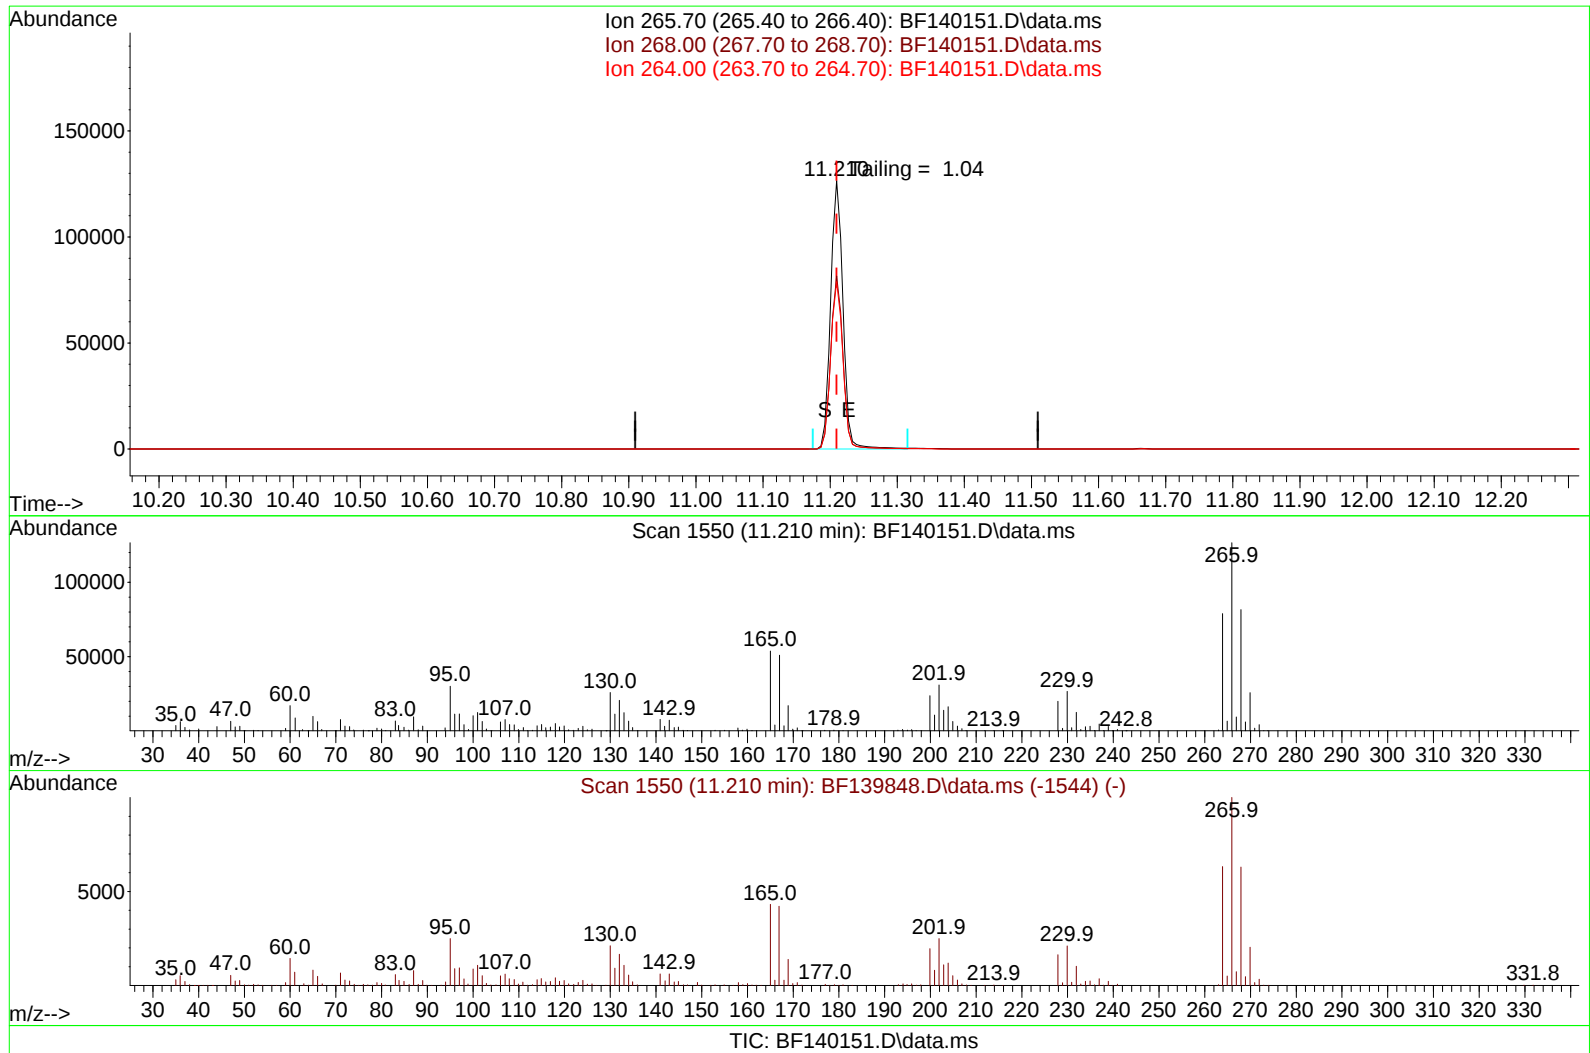

(70) Pentachlorophenol (C)

11.210min (+ 0.000) 36507.12 ng




response 161726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.47
264.00	63.20	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103024\
 Data File : BF140151.D
 Acq On : 30 Oct 2024 11:56
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 30 13:37:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 15:07:50 2024
 Response via : Initial Calibration

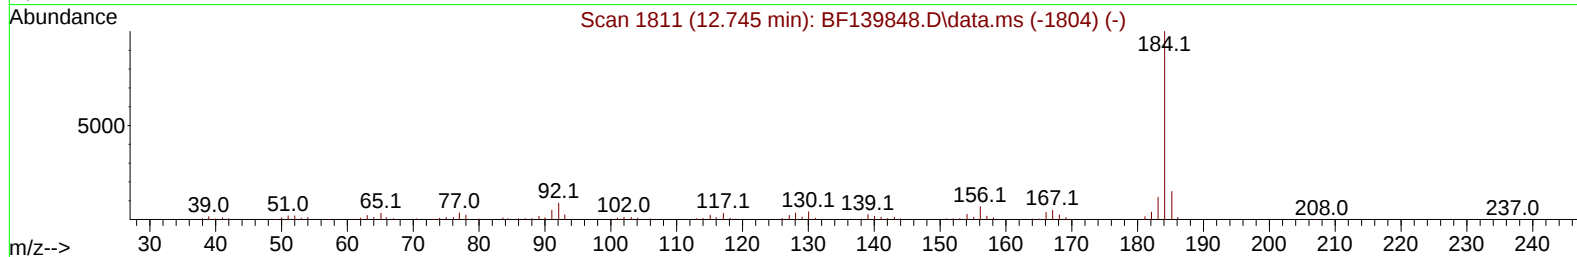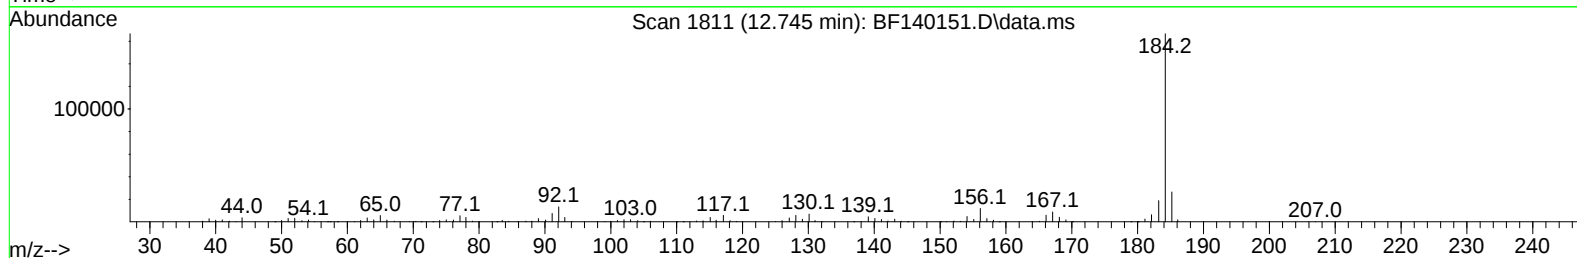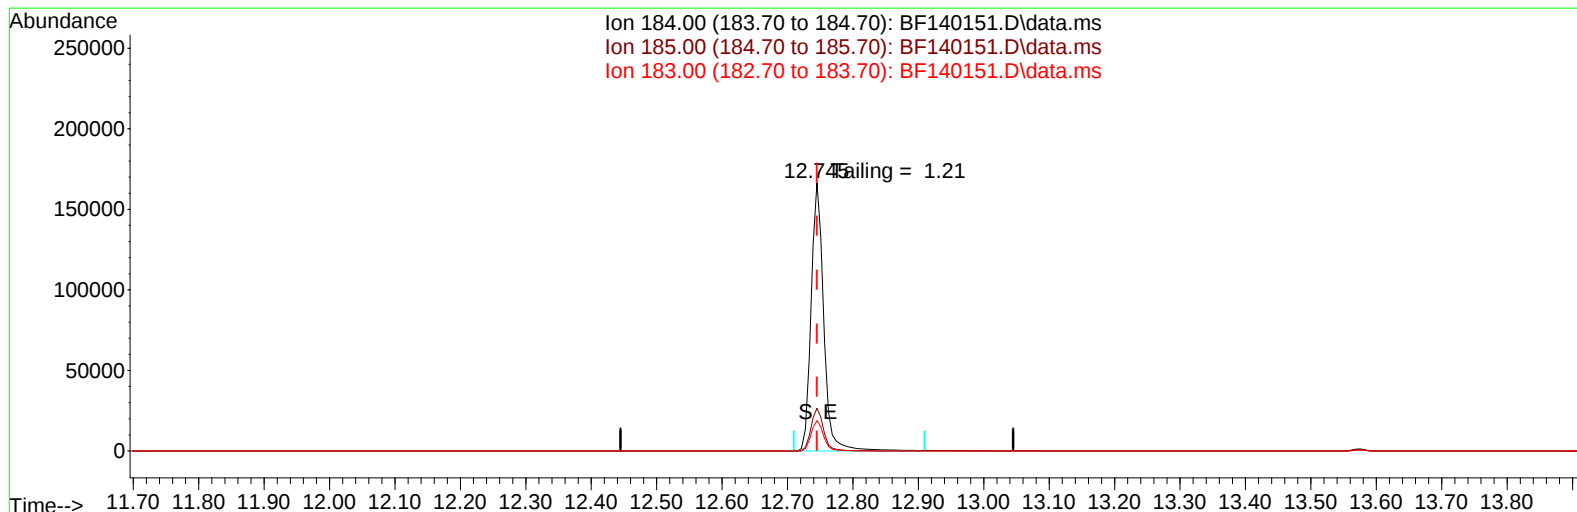

TIC: BF140151.D\data.ms

(77) Benzidine

12.745min (-0.000) 0.00 ng

response 224304

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.92
183.00	11.80	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/30/2024	BNA_F	<u>BF140151.D</u>
Compound Name	Response	Retention Time
DDT	401063	13.574
DDD	7330	13.274
DDE	529	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7859	408922	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP