
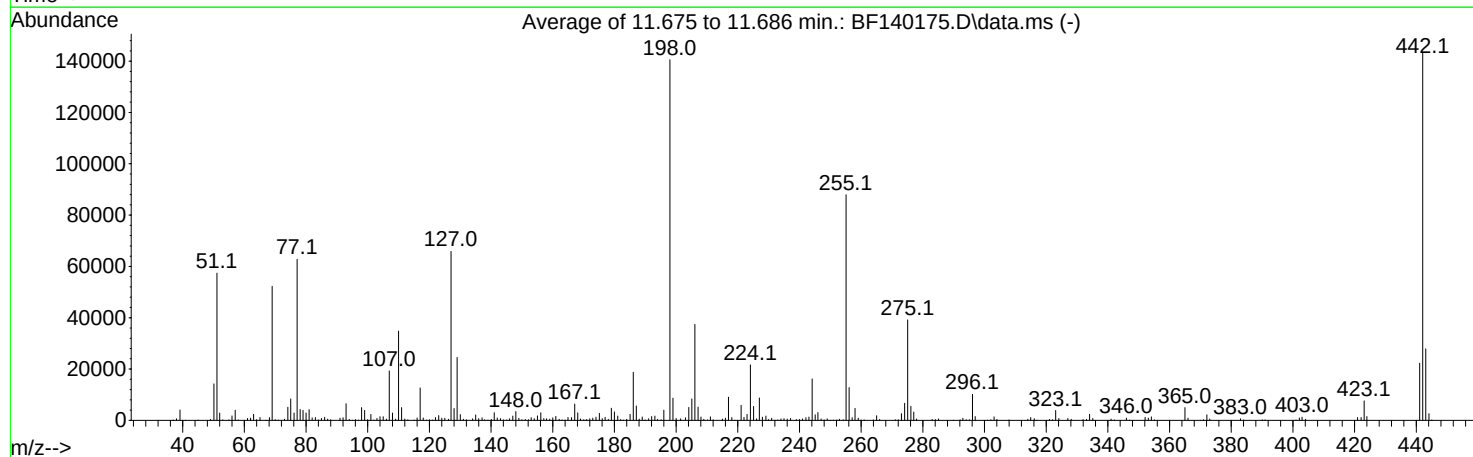


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140175.D
Acq On : 31 Oct 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

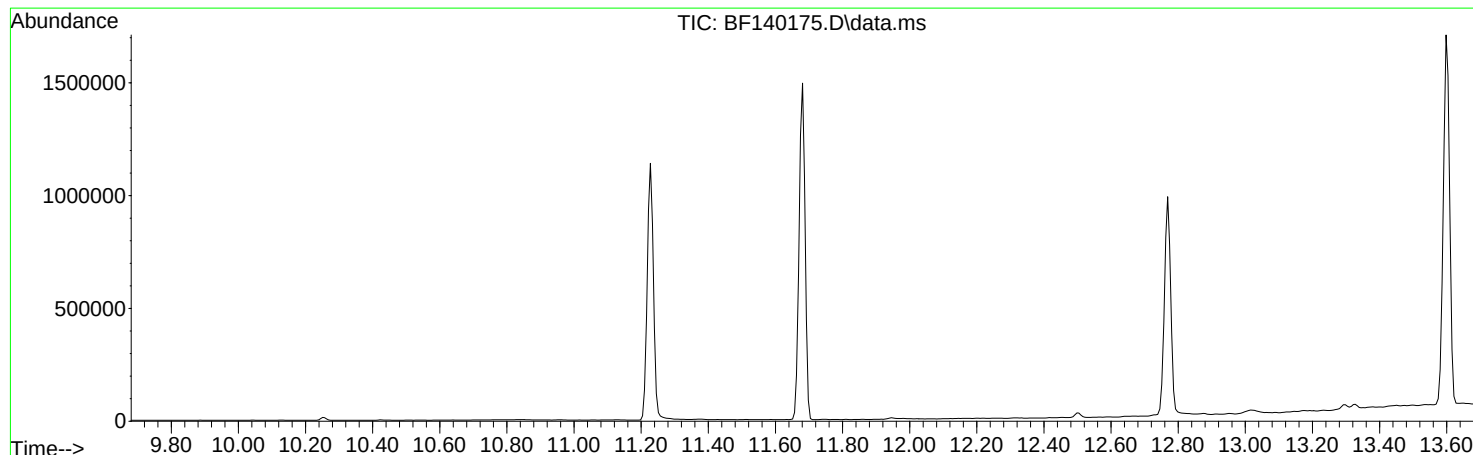




AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	57381	PASS
68	69	0.00	2	2.0	1036	PASS
69	198	0.00	100	37.2	52250	PASS
70	69	0.00	2	0.7	348	PASS
127	198	10	80	46.9	65869	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140544	PASS
199	198	5	9	6.2	8676	PASS
275	198	10	60	27.9	39160	PASS
365	198	1	100	3.6	4993	PASS
441	198	0.01	100	15.8	22235	PASS
442	442	50	100	100.0	143365	PASS
443	442	15	24	19.4	27880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140175.D
Acq On : 31 Oct 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 31 19:50:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

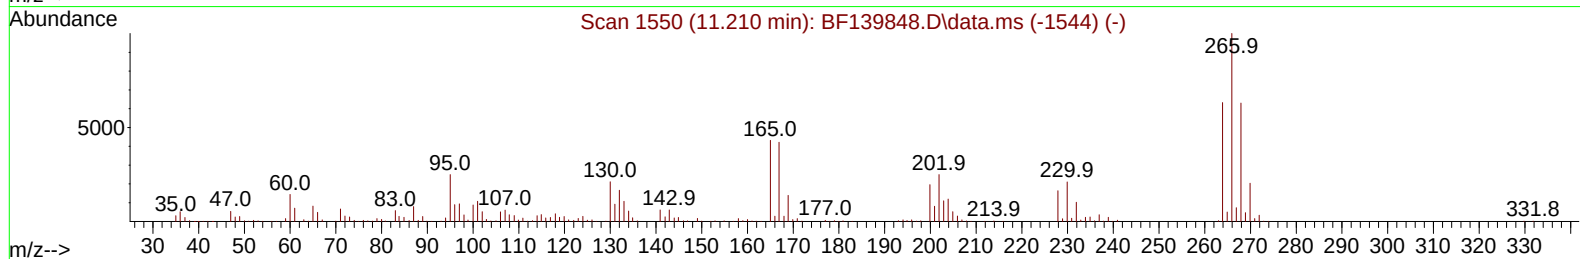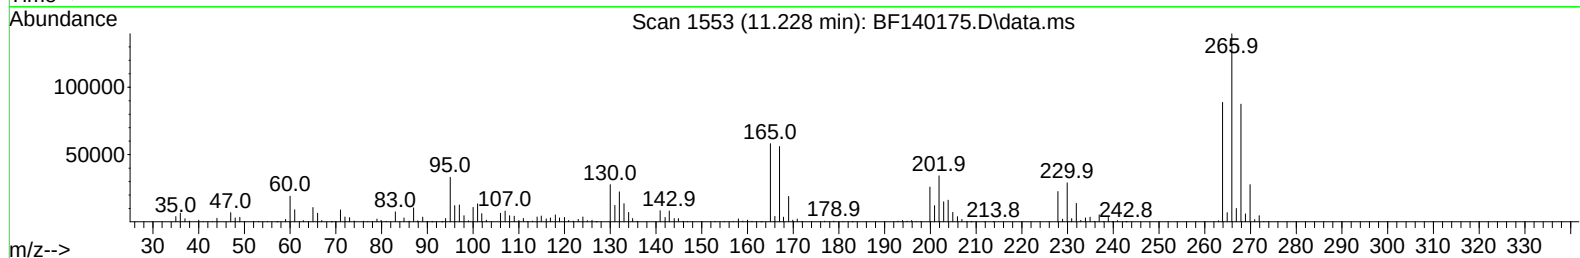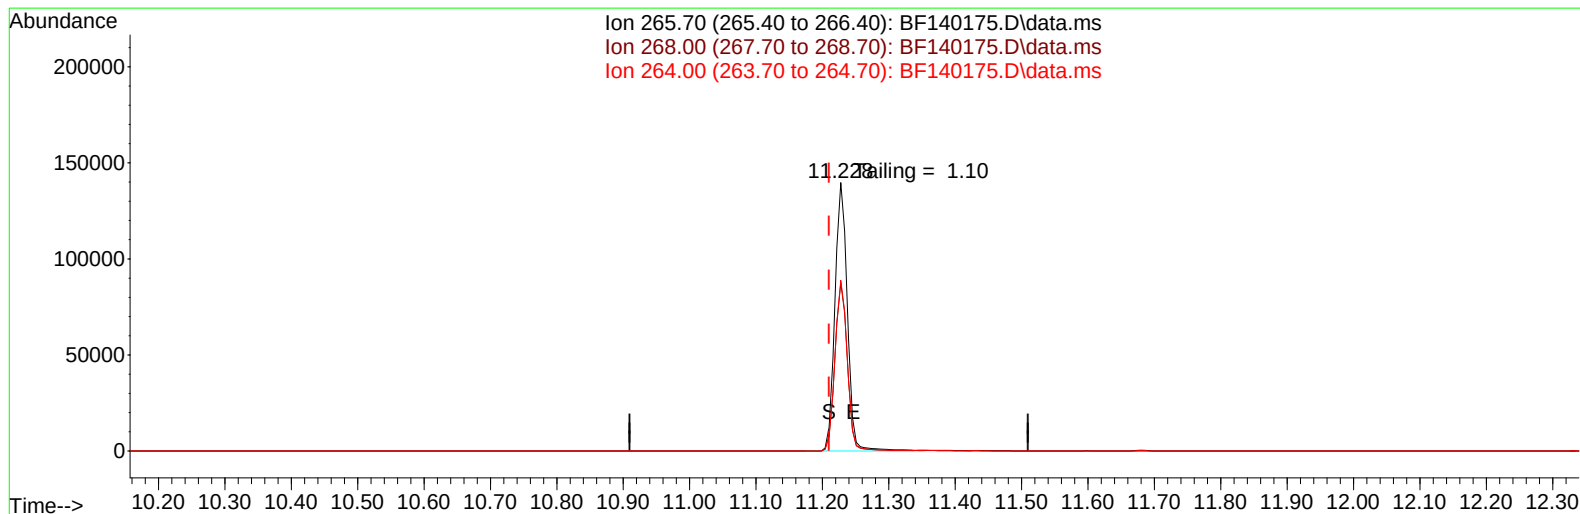

TIC: BF140175.D\data.ms

(70) Pentachlorophenol (C)

11.228min (+ 0.018) 96214.53 ng




response 181993

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.62
264.00	63.20	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103124\
Data File : BF140175.D
Acq On : 31 Oct 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 31 19:50:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

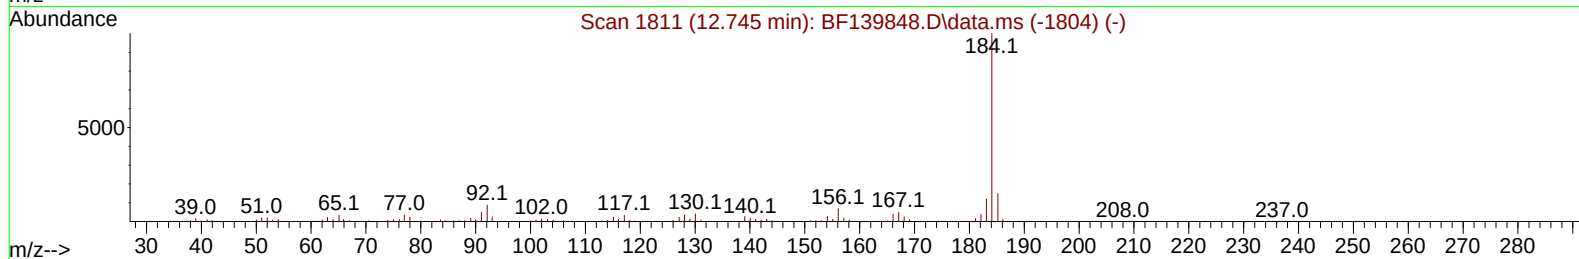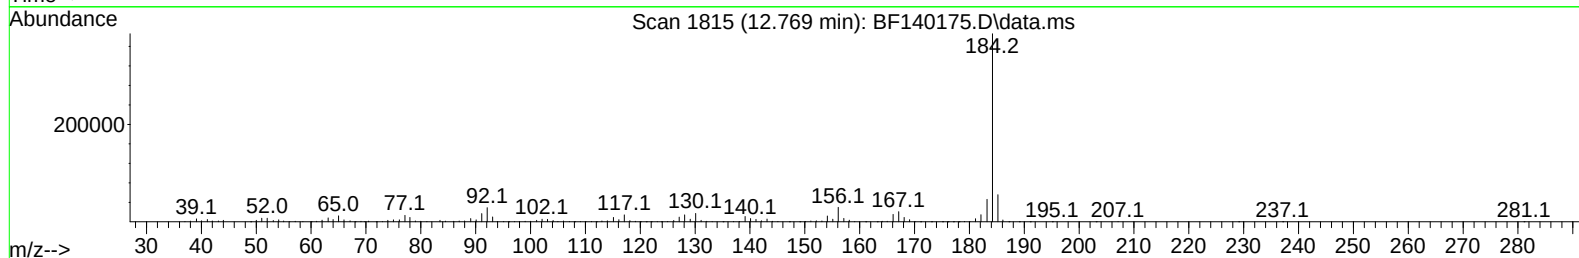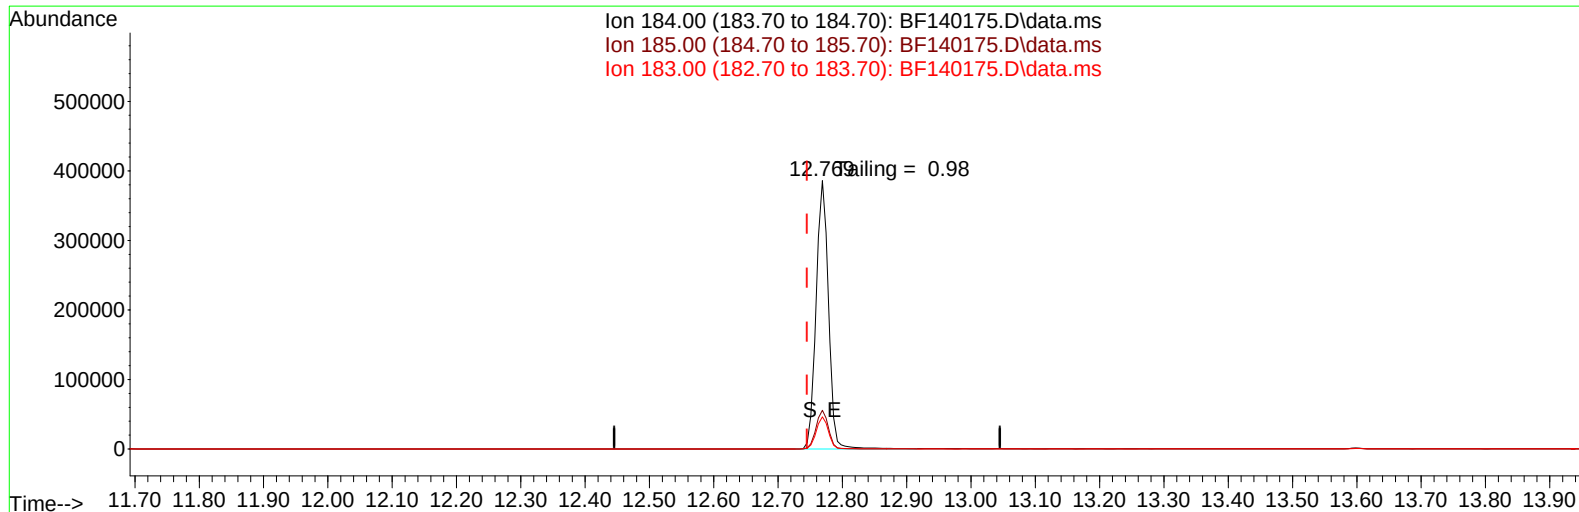

TIC: BF140175.D\data.ms

(77) Benzidine

12.769min (+ 0.024) 28582.51 ng

response 516523

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.45
183.00	11.80	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/31/2024	BNA_F	<u>BF140175.D</u>
Compound Name	Response	Retention Time
DDT	423753	13.598
DDD	10560	13.292
DDE	411	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10971	434724	2.52

Instrument :
BNA_F
ClientSampleId :
DFTPP