
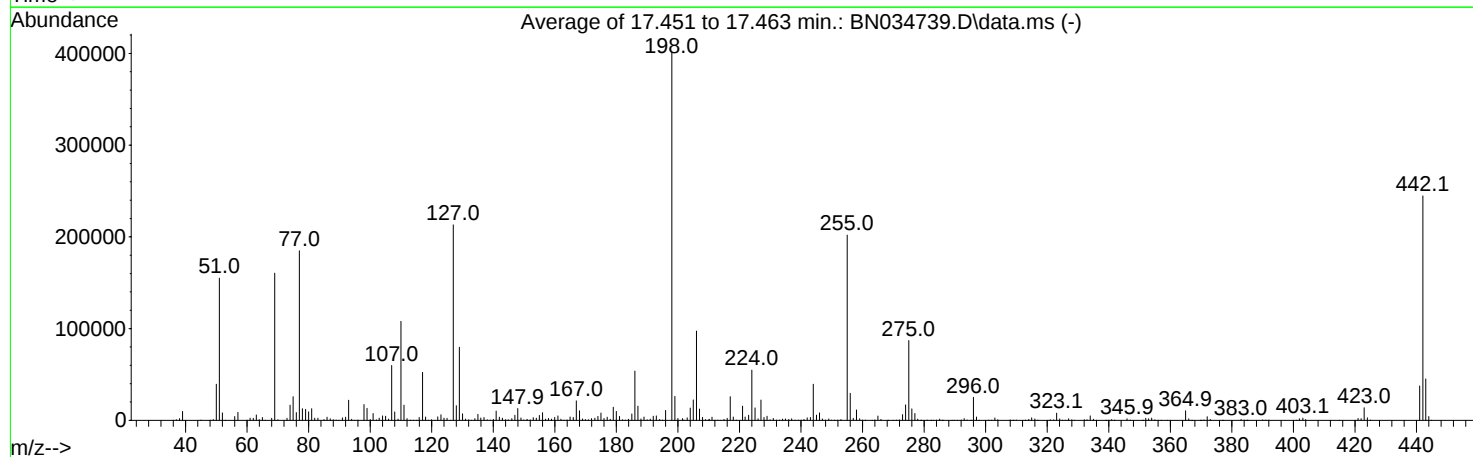


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103024\
Data File : BN034739.D
Acq On : 30 Oct 2024 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN103024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 30 13:28:24 2024

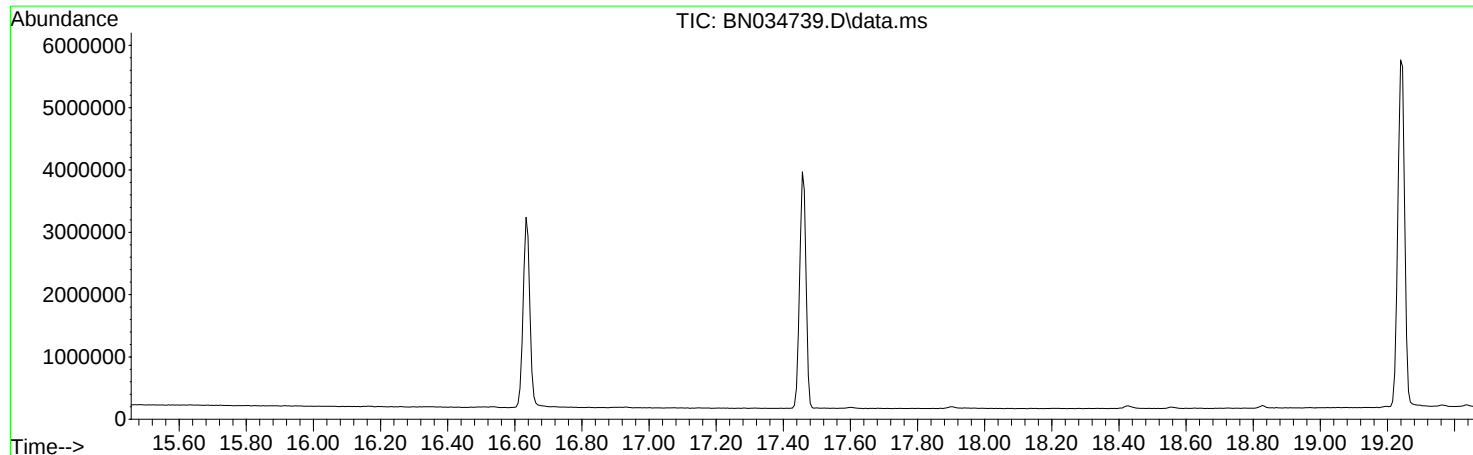




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	155112	PASS
68	69	0.00	2	1.4	2270	PASS
69	198	0.00	100	40.0	160508	PASS
70	69	0.00	2	0.4	626	PASS
127	198	10	80	53.2	213181	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	401024	PASS
199	198	5	9	6.5	26222	PASS
275	198	10	60	21.7	87027	PASS
365	198	1	100	2.6	10522	PASS
441	198	0.01	100	9.4	37536	PASS
442	442	50	100	100.0	244821	PASS
443	442	15	24	18.5	45208	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103024\
Data File : BN034739.D
Acq On : 30 Oct 2024 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 06:42:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 06:42:45 2024
Response via : Initial Calibration

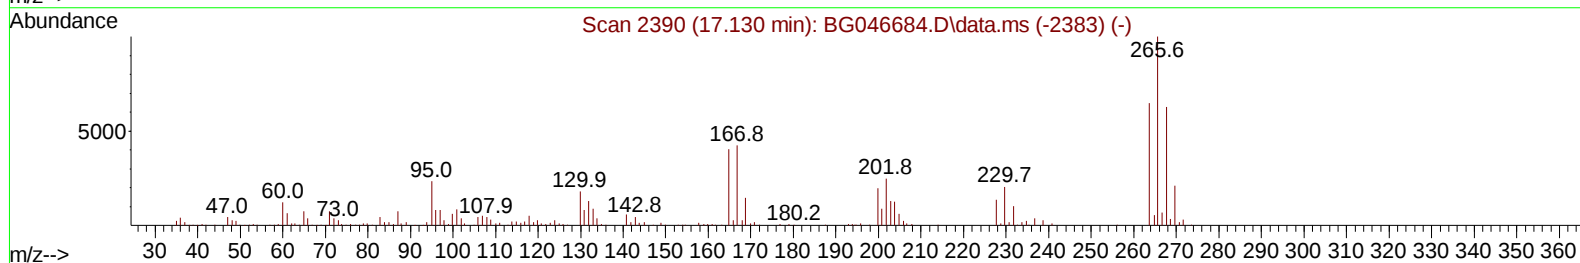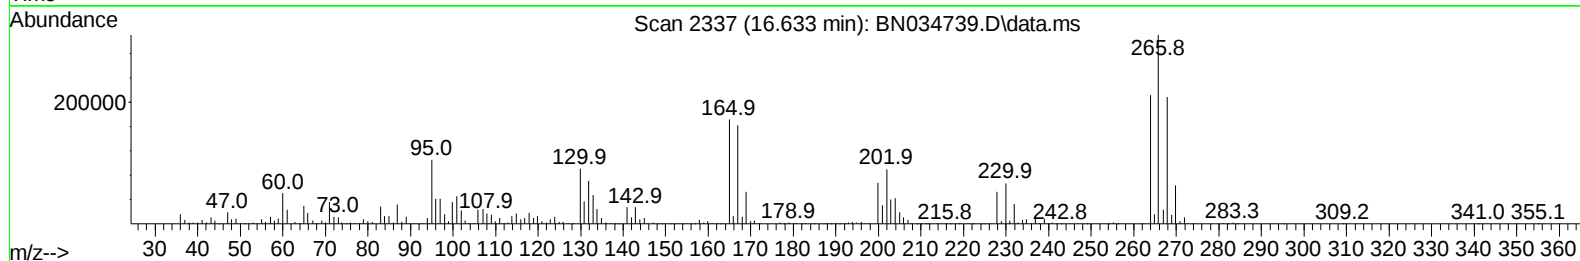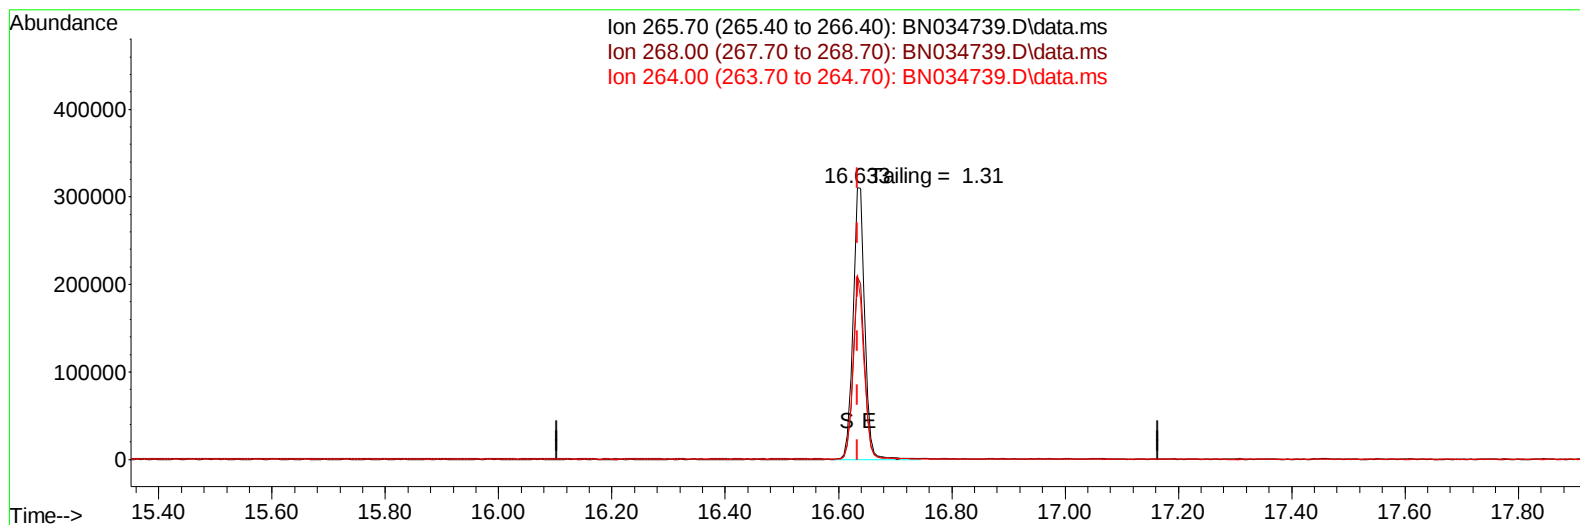

TIC: BN034739.D\data.ms

(70) Pentachlorophenol (C)

16.633min (0.000) 23615.75 ng




response 445905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.99
264.00	61.60	68.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103024\
Data File : BN034739.D
Acq On : 30 Oct 2024 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 06:42:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 06:42:45 2024
Response via : Initial Calibration

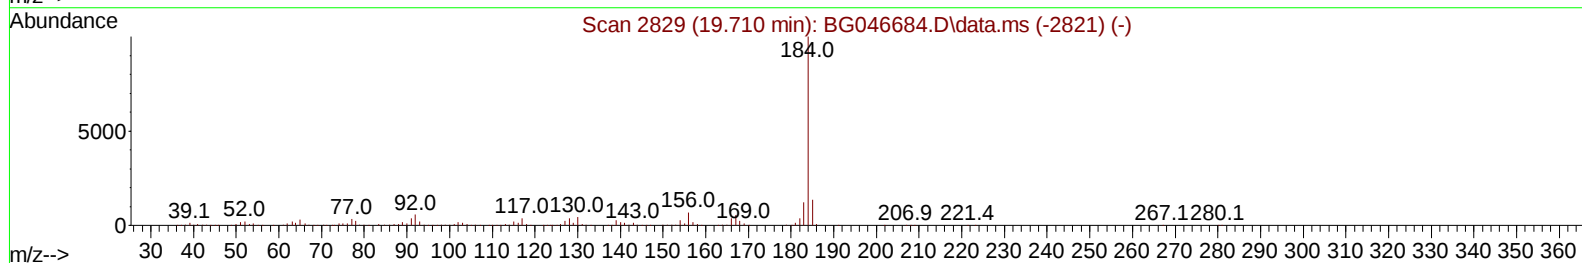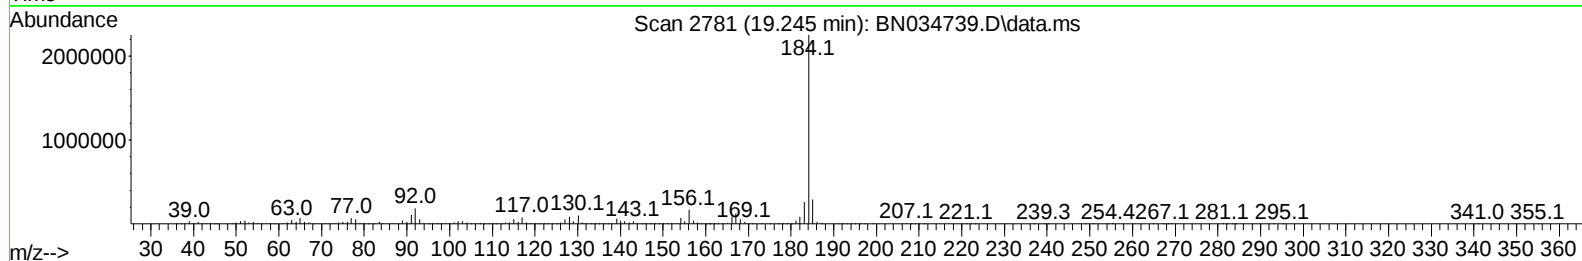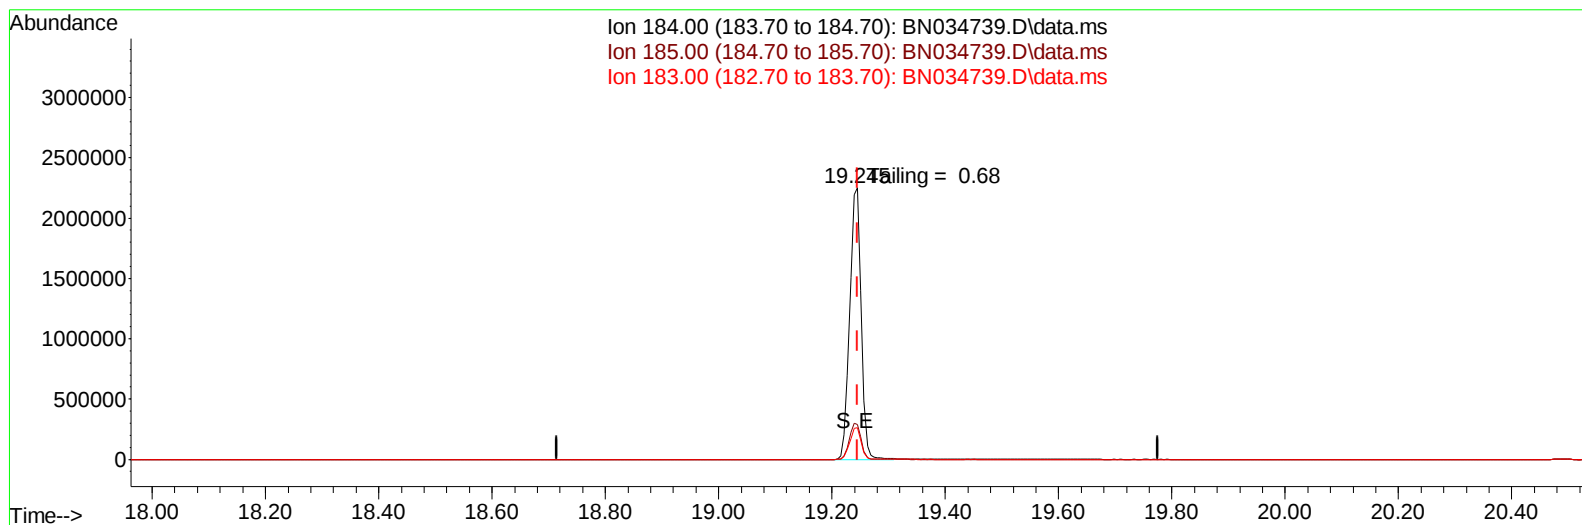

TIC: BN034739.D\data.ms

(77) Benzidine

19.245min (0.000) 766500.86 ng

response 3189736

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.97
183.00	13.20	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/30/2024	BNA_N	<u>BN034739.D</u>
Compound Name	Response	Retention Time
DDT	1360651	20.492
DDD	28684	20.098
DDE	0	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28684	1389335	2.06

Instrument :
BNA_N
ClientSampleId :
DFTPP