

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103124\
 Data File : P0107569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2024 18:31
 Operator : YP/AJ
 Sample : P4620-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P001-CF13-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/01/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 23:11:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.644	153.5E6	69524096	16.842m	21.601m#
2) SA Decachlor...	10.068	8.641	42240503	44611459	17.217	16.272

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103124\
Data File : PO107569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2024 18:31
Operator : YP/AJ
Sample : P4620-16
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P001-CF13-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/01/2024
Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 23:11:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

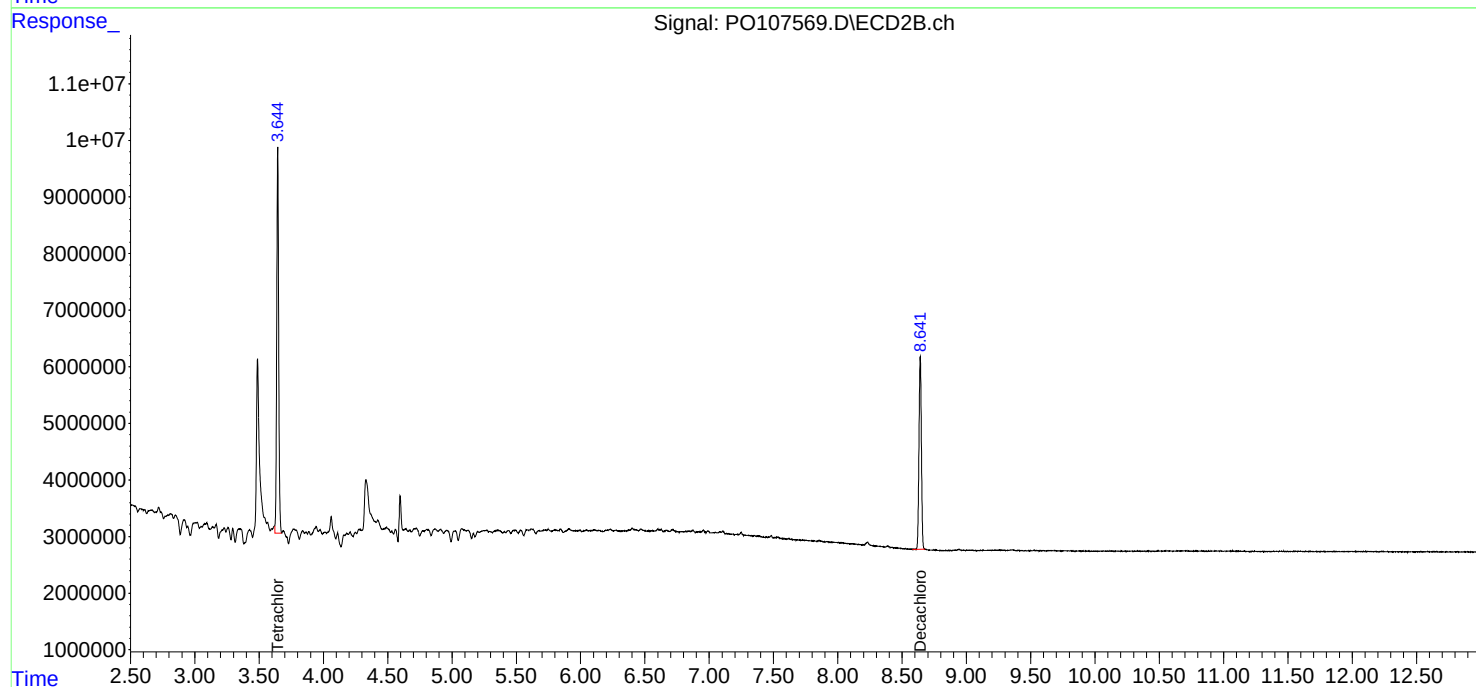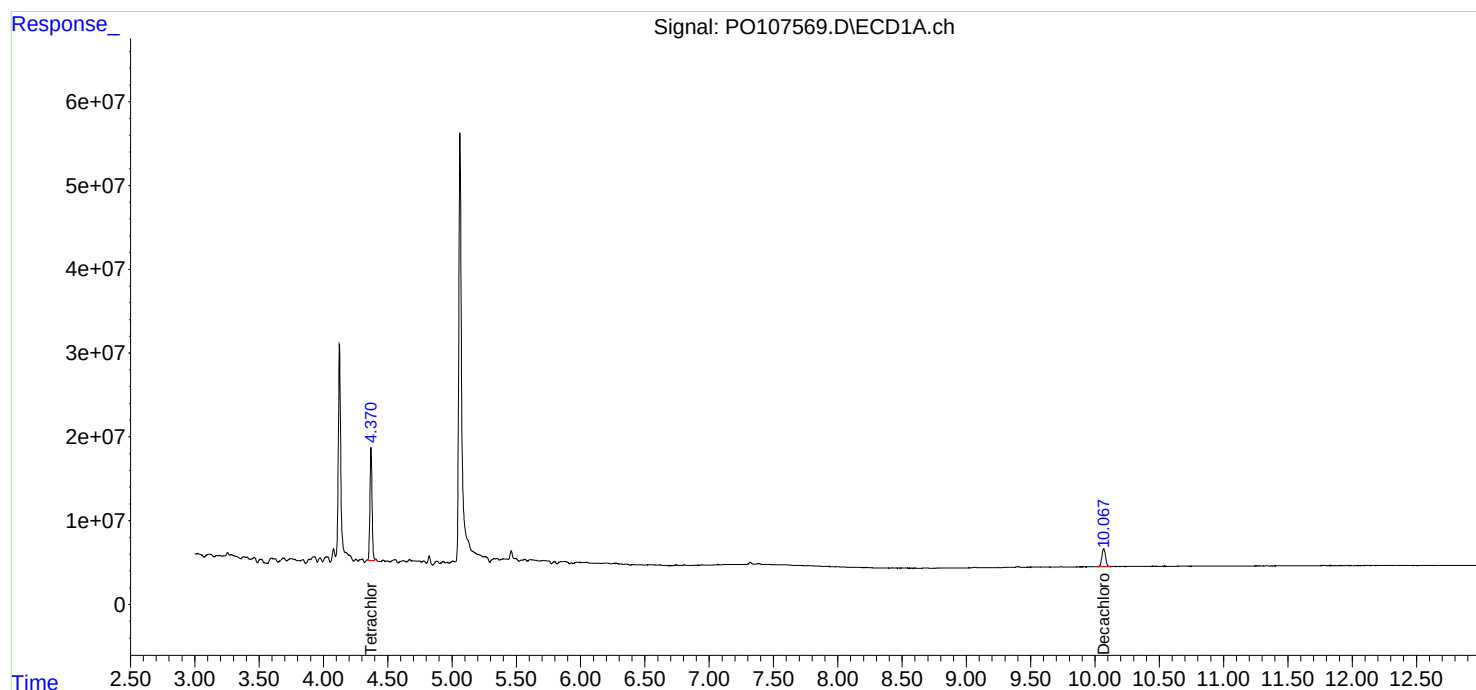

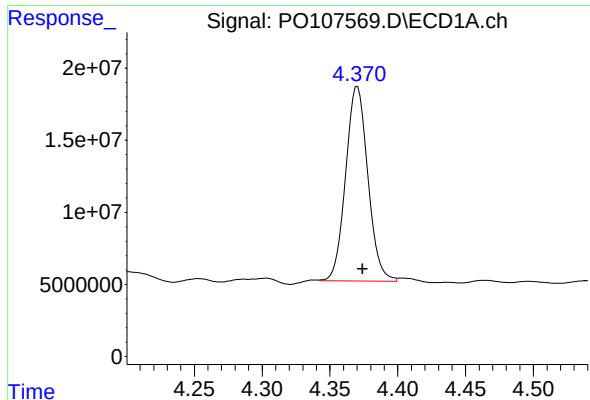


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: -0.004 min
Response: 153496973
Conc: 16.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
P001-CF13-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/01/2024
Supervised By :Ankita Jodhani 11/04/2024

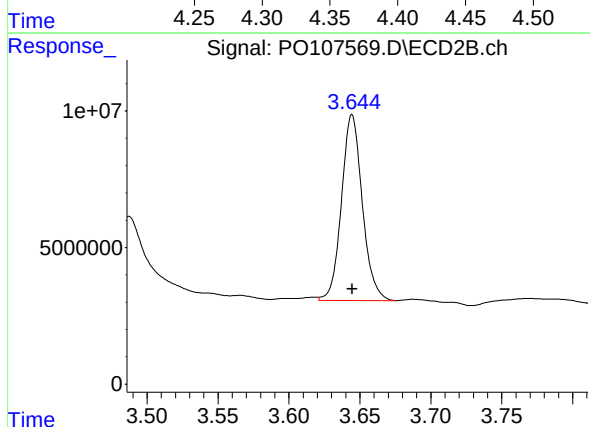


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.000 min
Response: 69524096
Conc: 21.60 ng/ml m

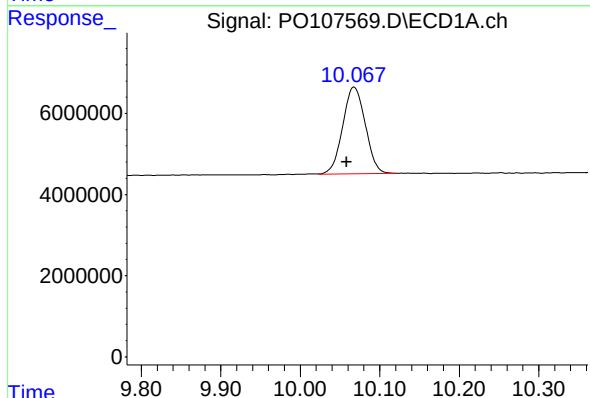

#2 Decachlorobiphenyl

R.T.: 10.068 min
Delta R.T.: 0.009 min
Response: 42240503
Conc: 17.22 ng/ml

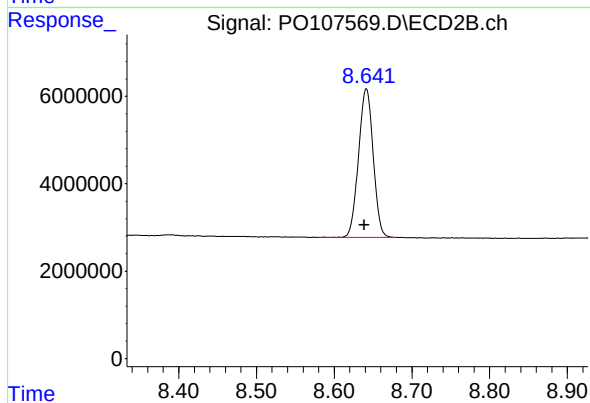

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.003 min
Response: 44611459
Conc: 16.27 ng/ml