

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103124\
 Data File : PP068330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2024 17:33
 Operator : YP\AJ
 Sample : P4620-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P001-CF10-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/01/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 00:45:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.759	4.053	20034939	20181904	21.644m	19.974
2) SA Decachlor...	10.673	9.208	28559517	26795721	24.806	23.894

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP103124\
Data File : PP068330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2024 17:33
Operator : YP\AJ
Sample : P4620-10
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
P001-CF10-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/01/2024
Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 00:45:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

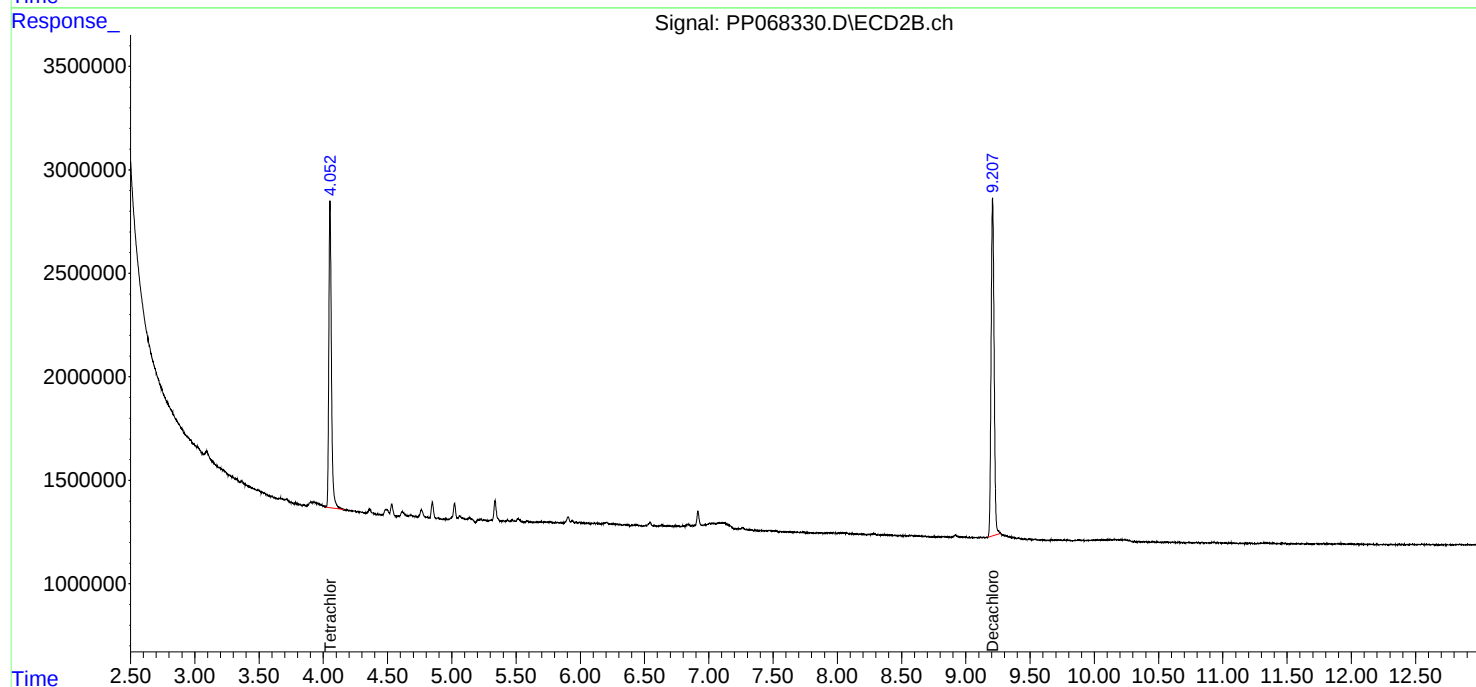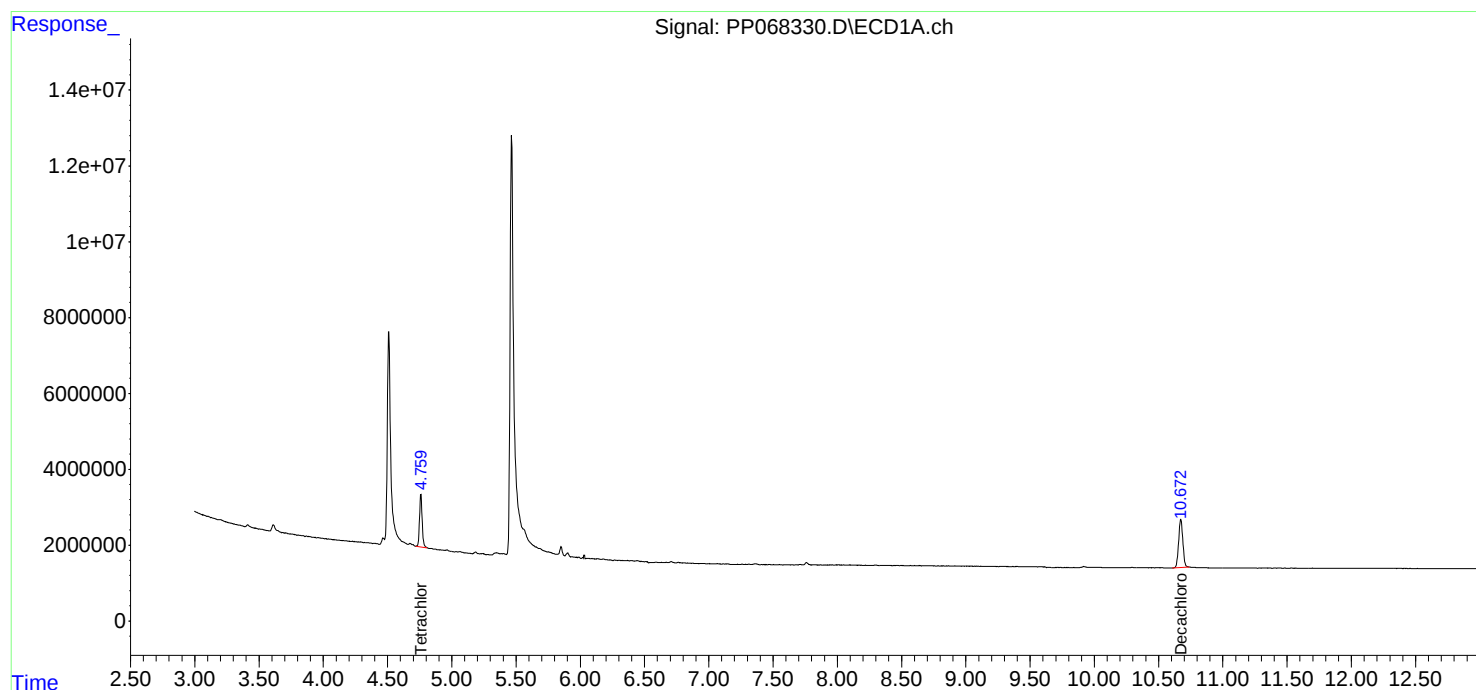

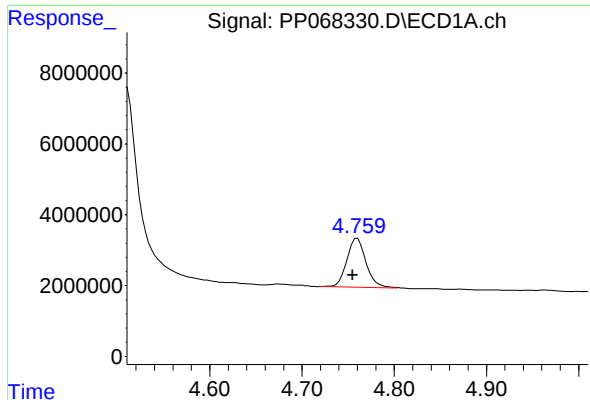


#1 Tetrachloro-m-xylene

R.T.: 4.759 min
Delta R.T.: 0.004 min
Response: 20034939
Conc: 21.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
P001-CF10-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/01/2024
Supervised By :Ankita Jodhani 11/04/2024

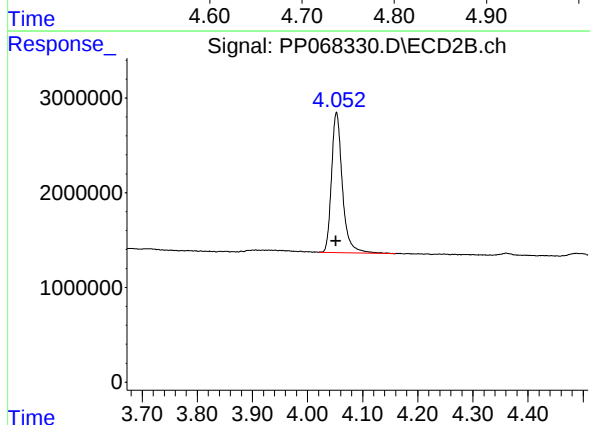


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: 0.000 min
Response: 20181904
Conc: 19.97 ng/ml

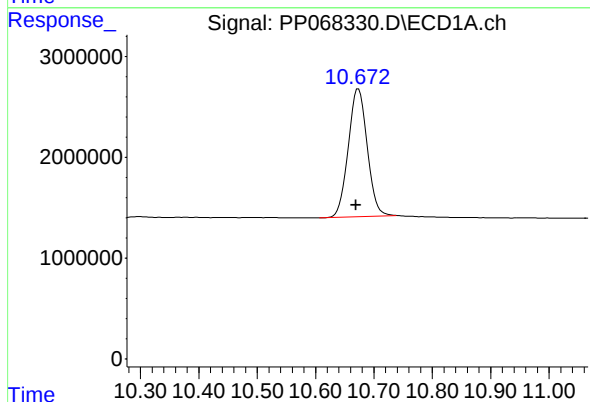

#2 Decachlorobiphenyl

R.T.: 10.673 min
Delta R.T.: 0.005 min
Response: 28559517
Conc: 24.81 ng/ml

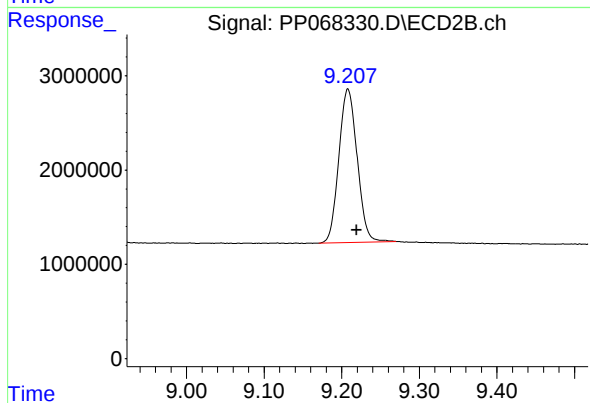

#2 Decachlorobiphenyl

R.T.: 9.208 min
Delta R.T.: -0.011 min
Response: 26795721
Conc: 23.89 ng/ml