


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110424\
Data File : BN034849.D
Acq On : 04 Nov 2024 20:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN103024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 05 00:03:28 2024

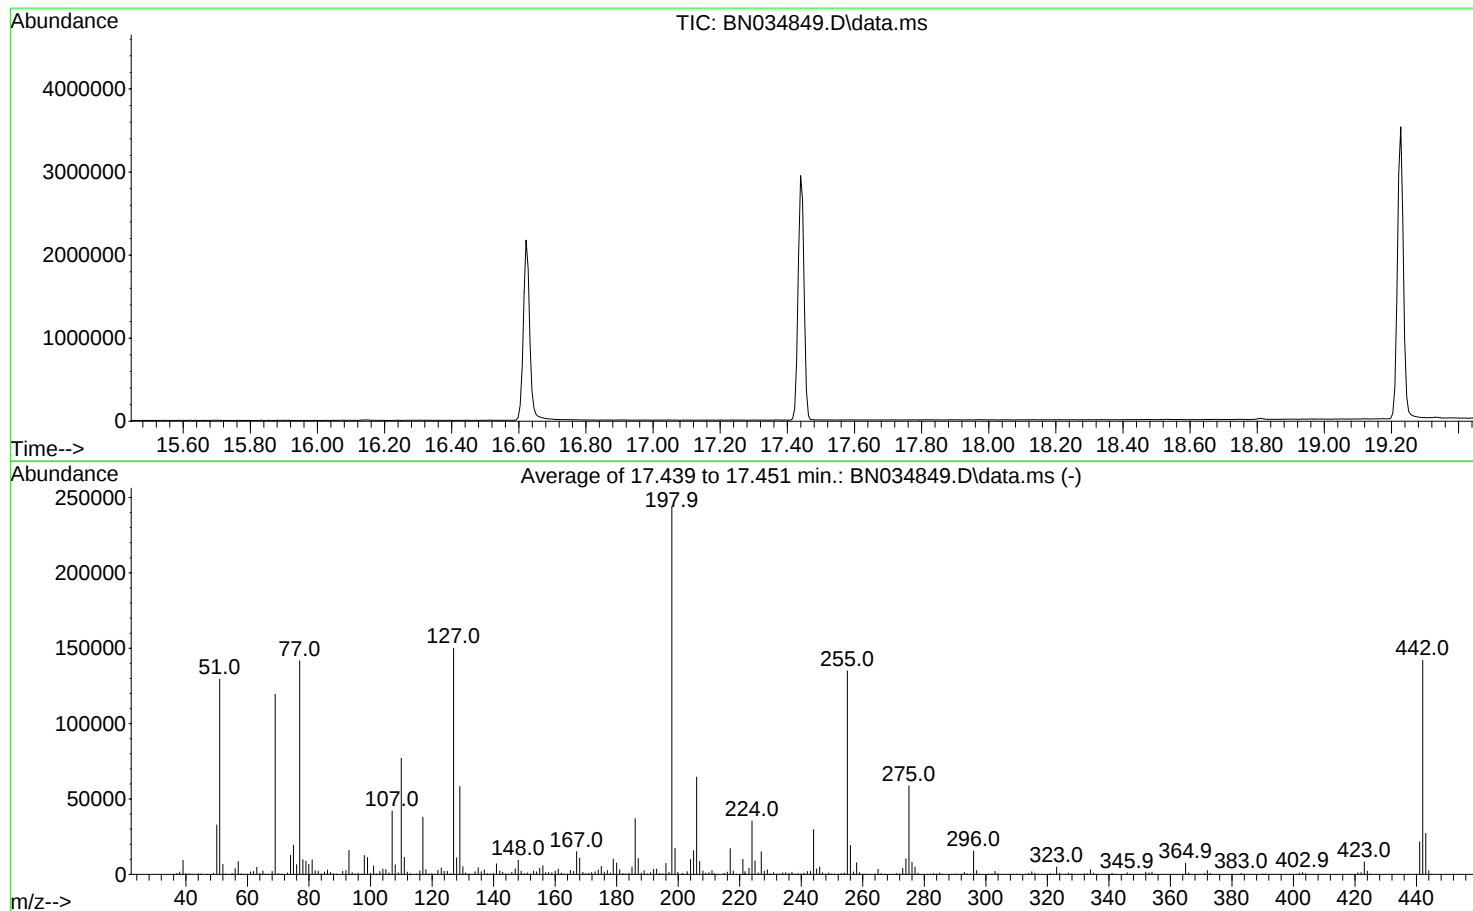




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	129505	PASS
68	69	0.00	2	1.6	1938	PASS
69	198	0.00	100	49.0	119523	PASS
70	69	0.00	2	0.6	686	PASS
127	198	10	80	61.5	149968	PASS
197	198	0.00	2	0.6	1346	PASS
198	198	100	100	100.0	244032	PASS
199	198	5	9	7.1	17358	PASS
275	198	10	60	24.1	58707	PASS
365	198	1	100	3.0	7442	PASS
441	198	0.01	100	8.8	21576	PASS
442	442	50	100	100.0	142067	PASS
443	442	15	24	19.1	27149	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110424\
Data File : BN034849.D
Acq On : 04 Nov 2024 20:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 23:56:03 2024
Response via : Initial Calibration

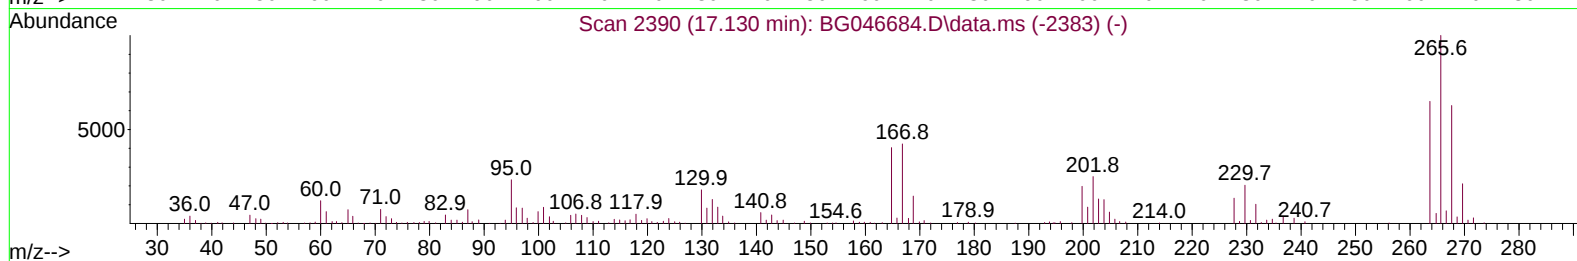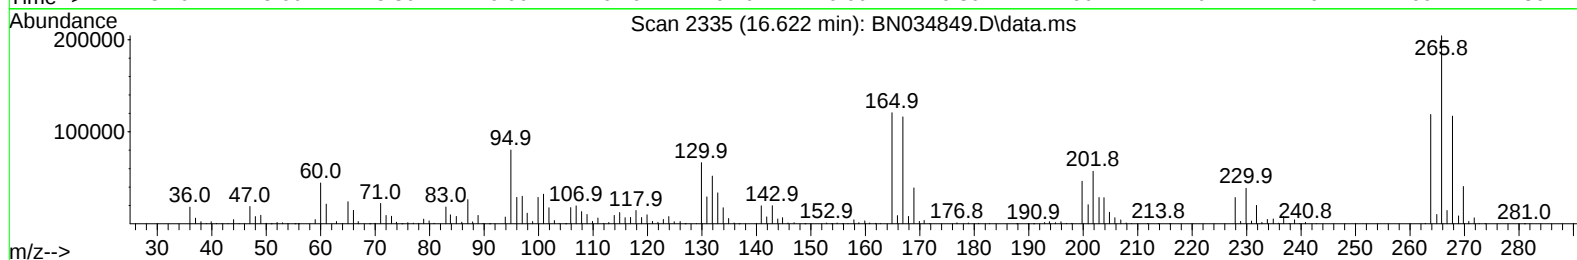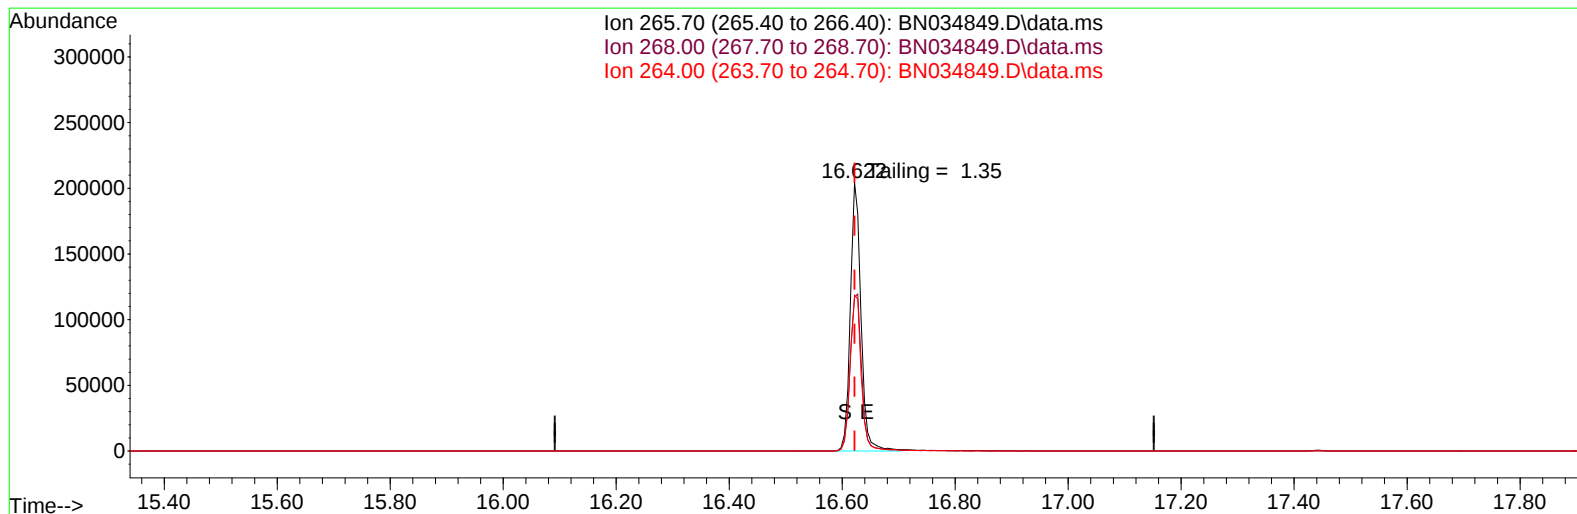

TIC: BN034849.D\data.ms

(70) Pentachlorophenol (C)

16.622min (0.000) 21272.94 ng




response 271619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.32
264.00	61.60	58.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110424\
Data File : BN034849.D
Acq On : 04 Nov 2024 20:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 23:56:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 23:56:03 2024
Response via : Initial Calibration

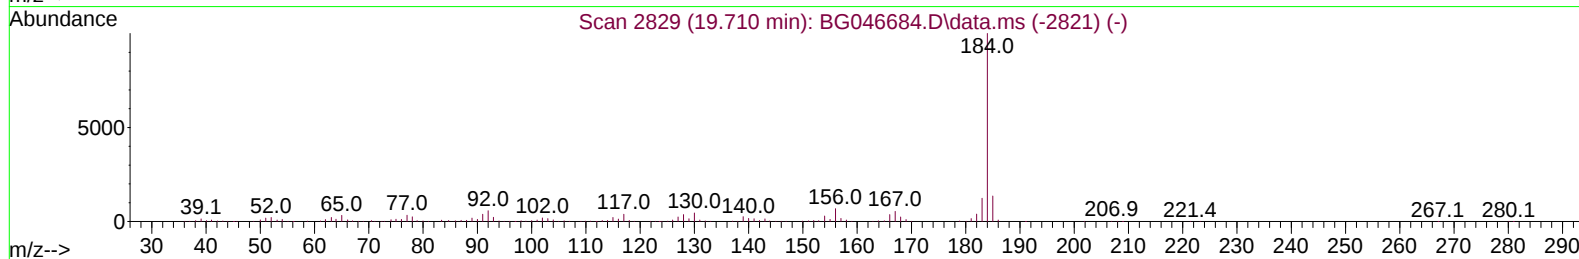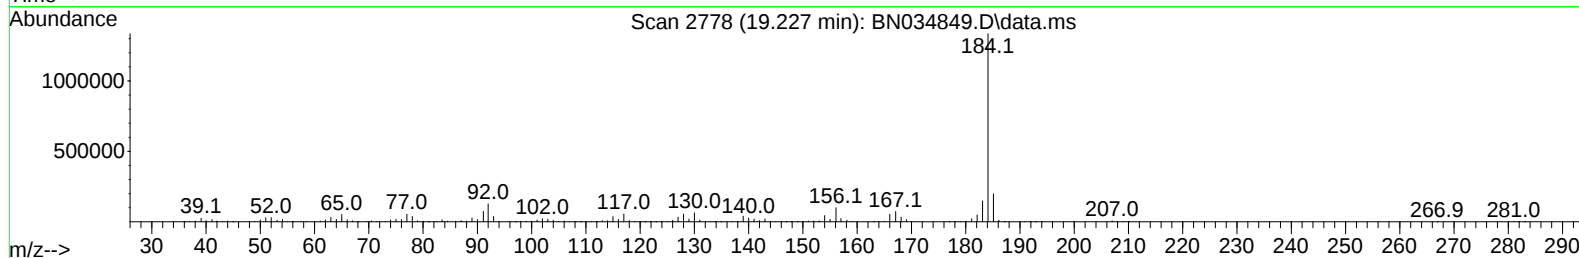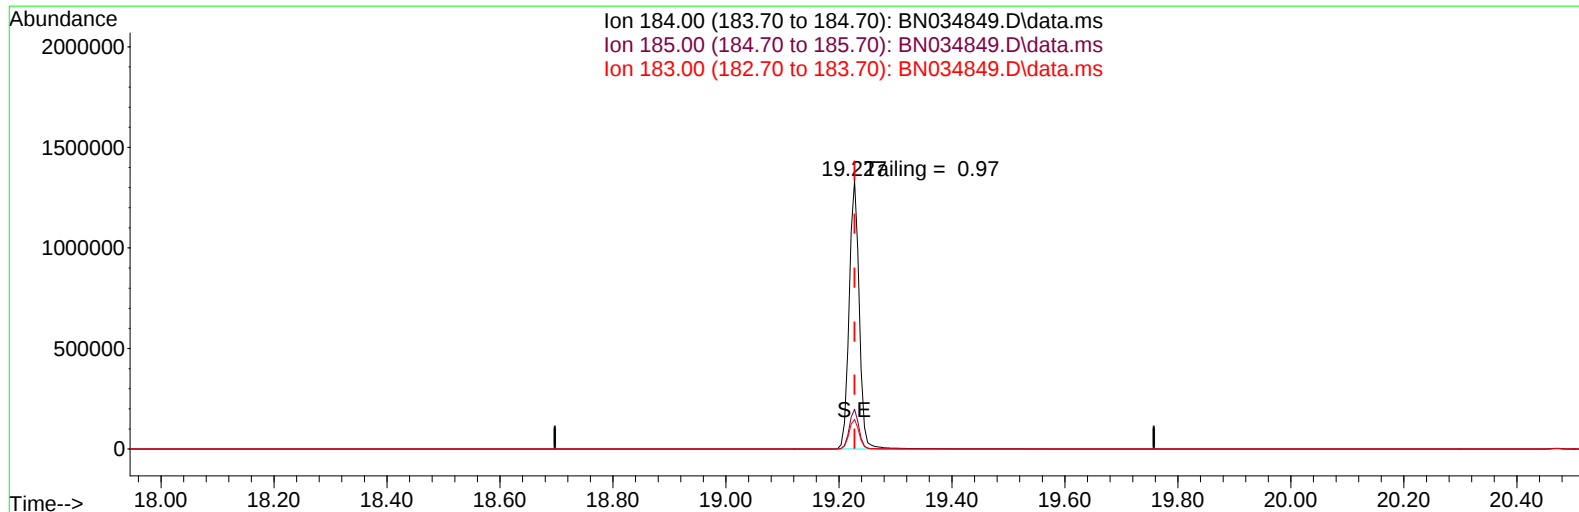

TIC: BN034849.D\data.ms

(77) Benzidine

19.227min (0.000) 0.00 ng

response 1662756

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.88
183.00	13.20	11.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2024	BNA_N	<u>BN034849.D</u>
Compound Name	Response	Retention Time
DDT	864034	20.469
DDD	21444	20.027
DDE	934	19.522
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22378	886412	2.52

Instrument :
BNA_N
ClientSampleId :
DFTPP