
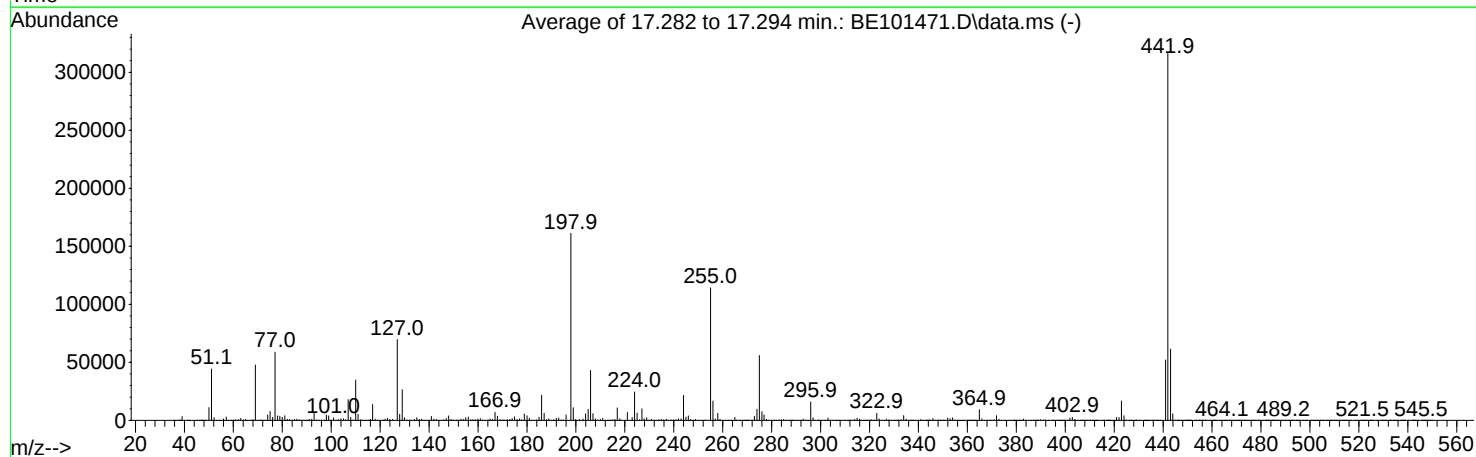


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101471.D
Acq On : 5 Nov 2024 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 29 01:26:30 2024

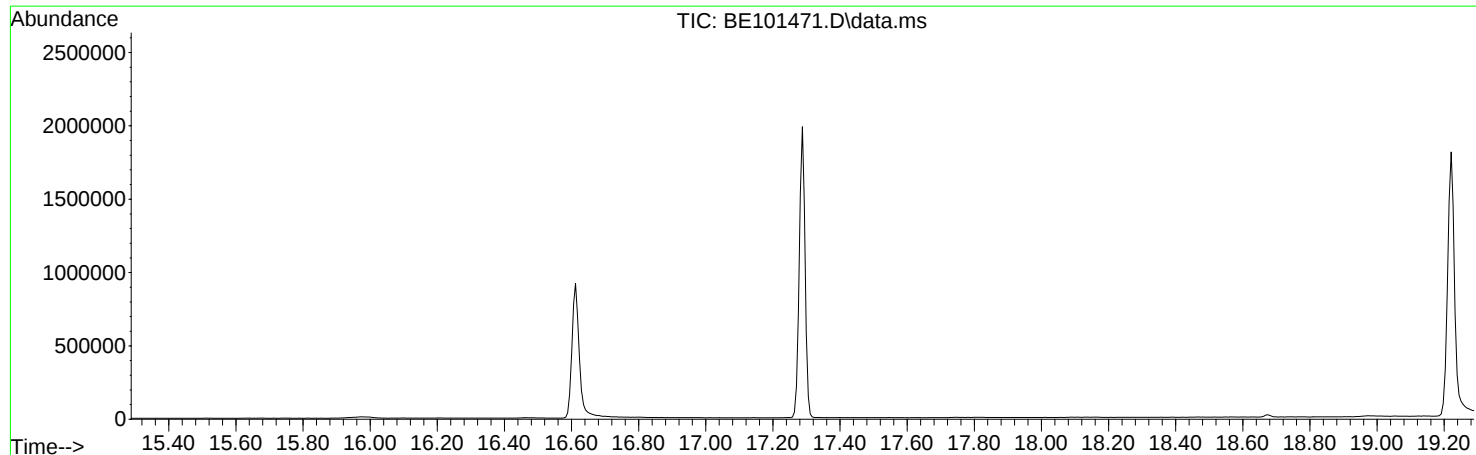




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	44346	PASS
68	69	0.00	2	1.5	722	PASS
69	198	0.00	100	29.6	47763	PASS
70	69	0.00	2	0.5	219	PASS
127	198	10	80	43.2	69694	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	161185	PASS
199	198	5	9	6.8	10923	PASS
275	198	10	60	34.7	55934	PASS
365	198	1	100	5.7	9265	PASS
441	198	0.01	100	32.3	51997	PASS
442	442	50	100	100.0	317053	PASS
443	442	15	24	19.3	61341	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101471.D
Acq On : 5 Nov 2024 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 05 10:41:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

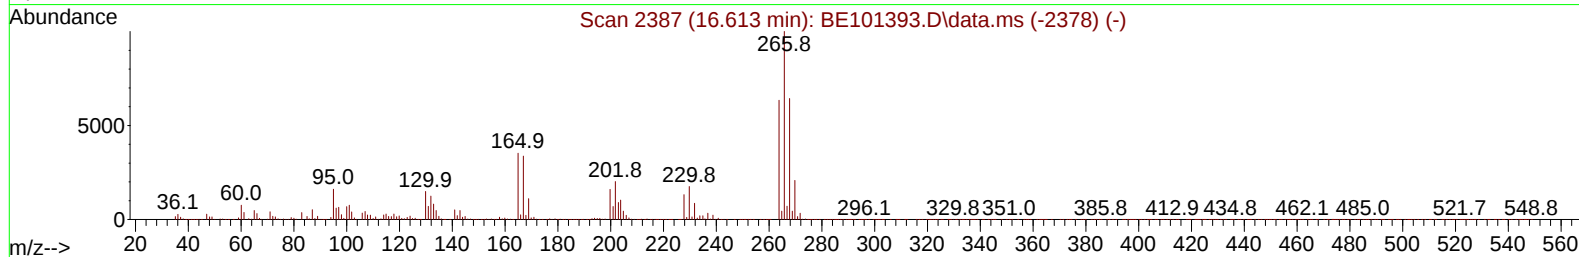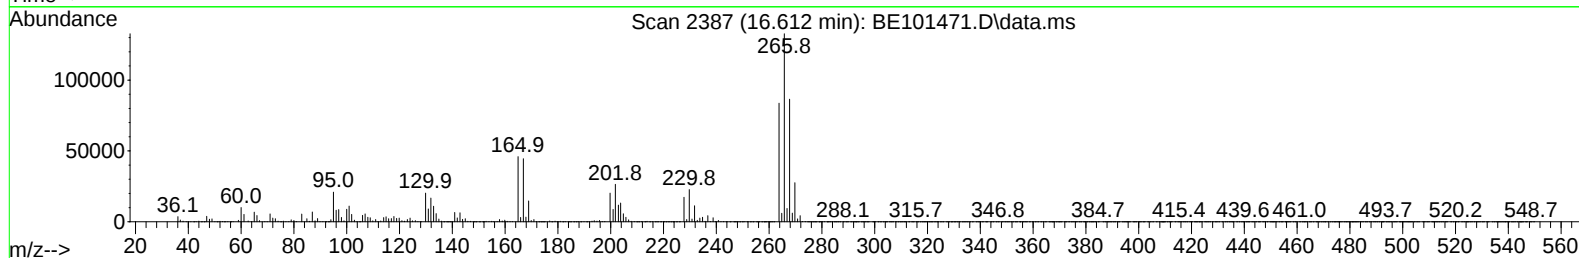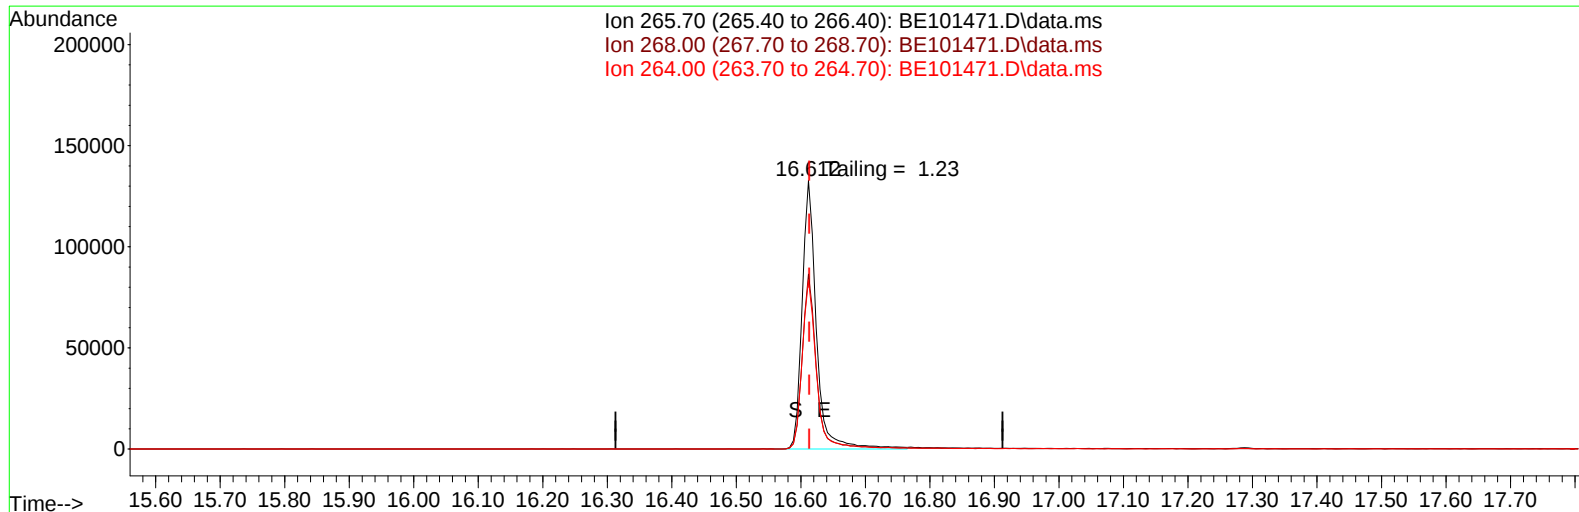

TIC: BE101471.D\data.ms

(70) Pentachlorophenol (C)

16.612min (-0.001) 1236265.89 ng




response 206048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.18
264.00	63.40	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101471.D
Acq On : 5 Nov 2024 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 05 10:41:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

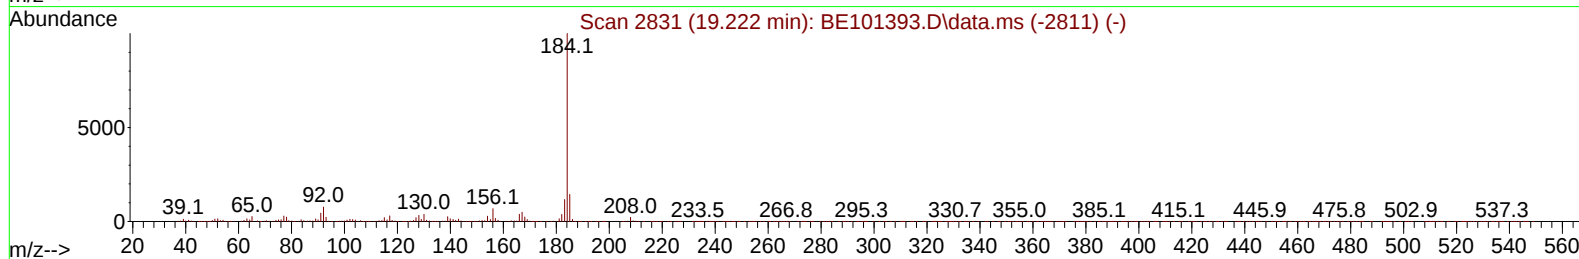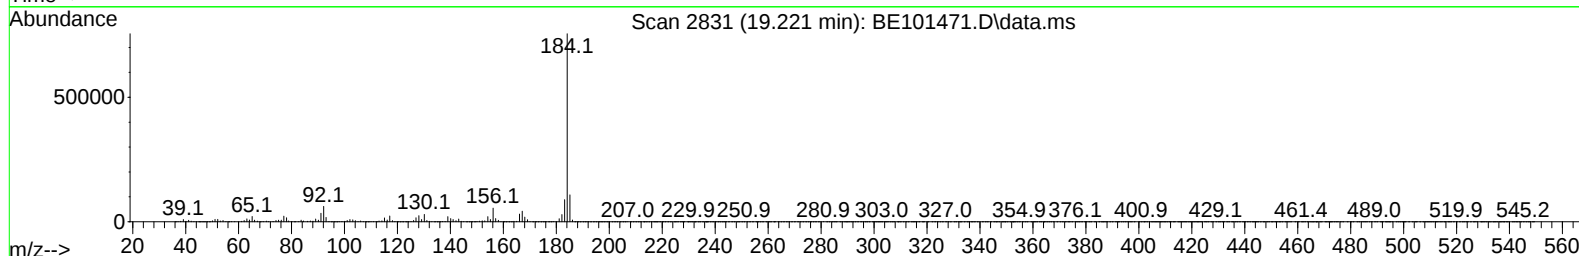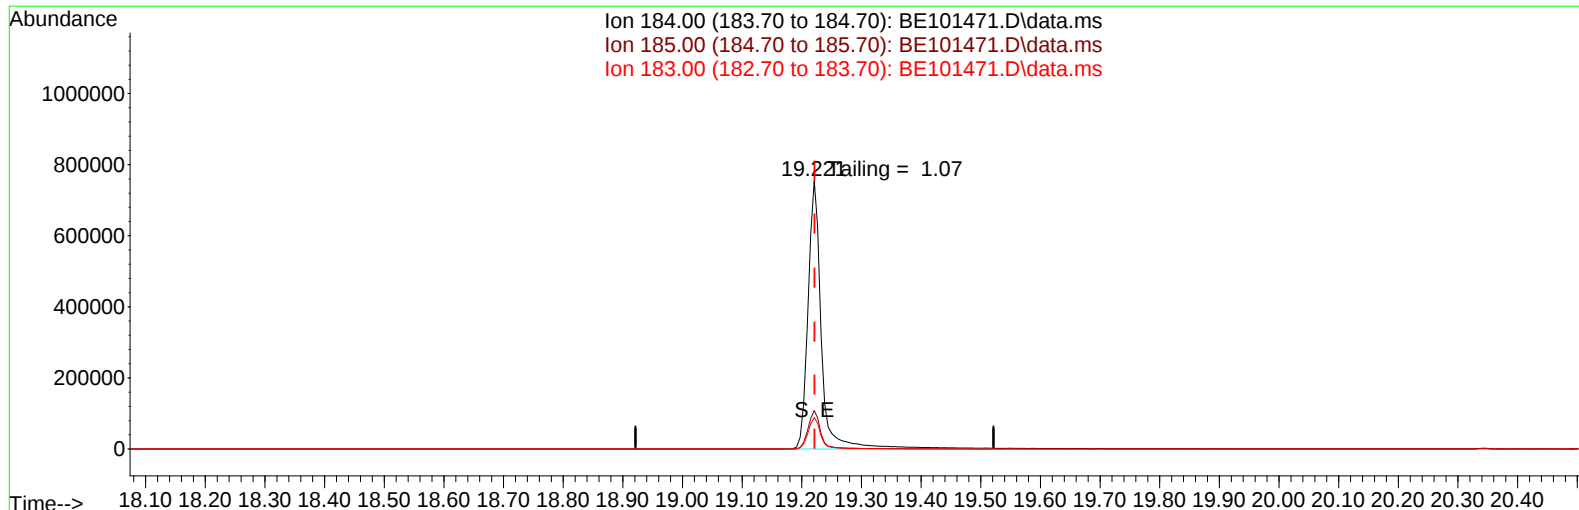

TIC: BE101471.D\data.ms

(77) Benzidine

19.221min (-0.001) 1366074.03 ng

response 1196307

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.33
183.00	11.60	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/5/2024	BNA_E	<u>BE101471.D</u>
Compound Name	Response	Retention Time
DDT	654338	20.343
DDD	17823	19.914
DDE	932	19.403
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18755	673093	2.79

Instrument :
BNA_E
ClientSampleId :
DFTPP