
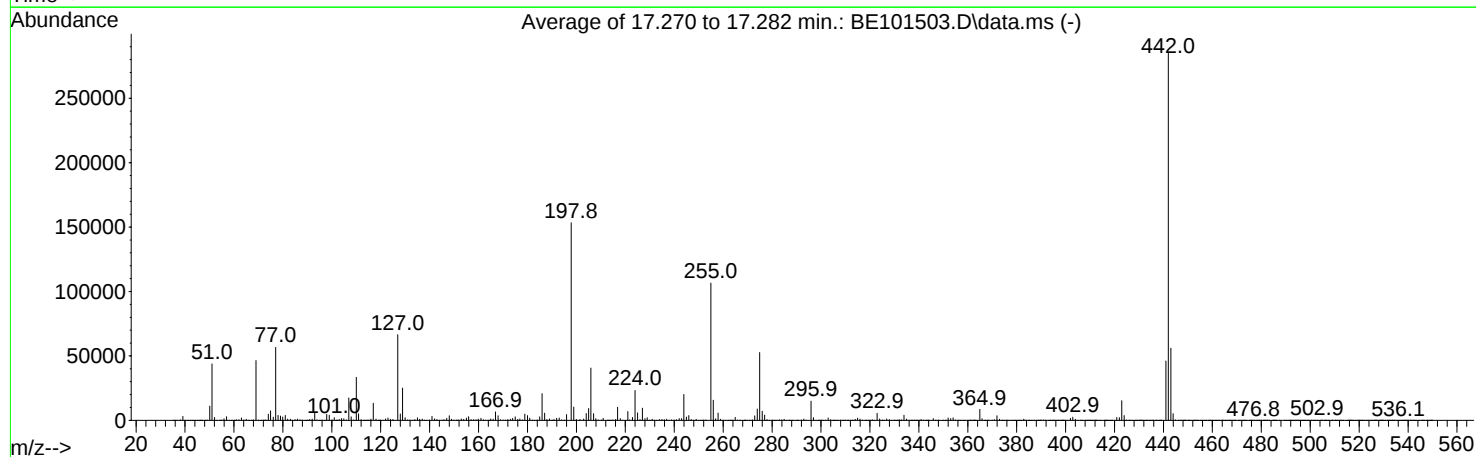


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101503.D
Acq On : 6 Nov 2024 19:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 00:01:20 2024

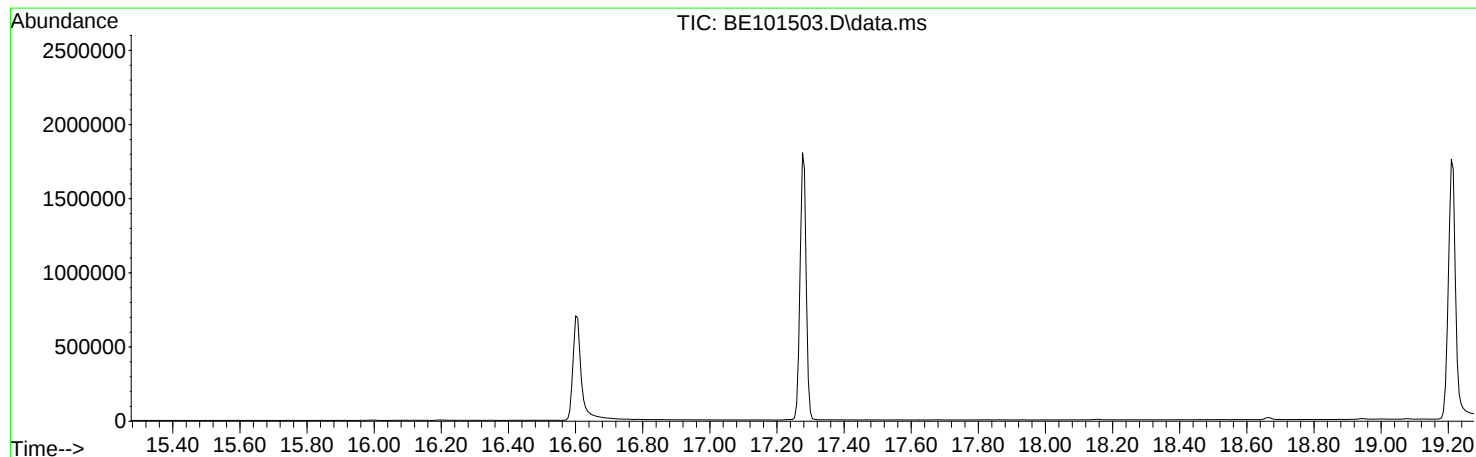




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	43910	PASS
68	69	0.00	2	0.9	413	PASS
69	198	0.00	100	30.3	46502	PASS
70	69	0.00	2	0.4	201	PASS
127	198	10	80	43.3	66441	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153415	PASS
199	198	5	9	6.7	10338	PASS
275	198	10	60	34.3	52667	PASS
365	198	1	100	5.5	8512	PASS
441	198	0.01	100	30.0	46040	PASS
442	442	50	100	100.0	285525	PASS
443	442	15	24	19.6	56020	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101503.D
Acq On : 6 Nov 2024 19:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 07 00:16:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

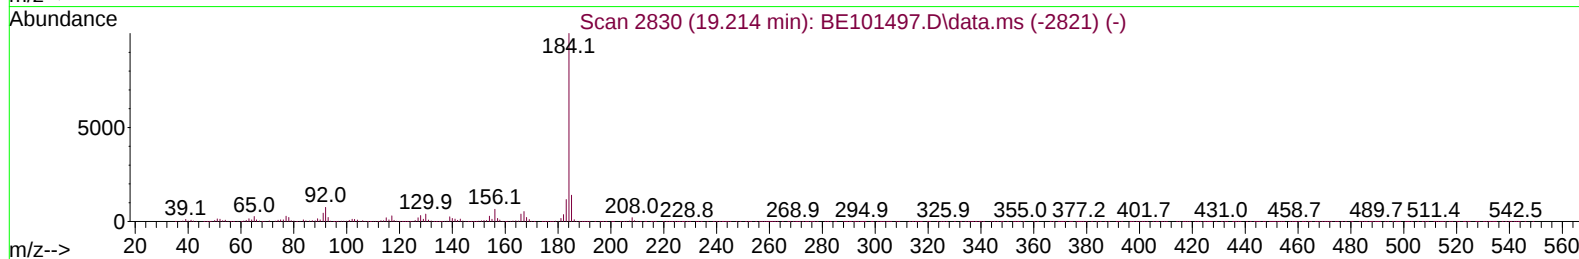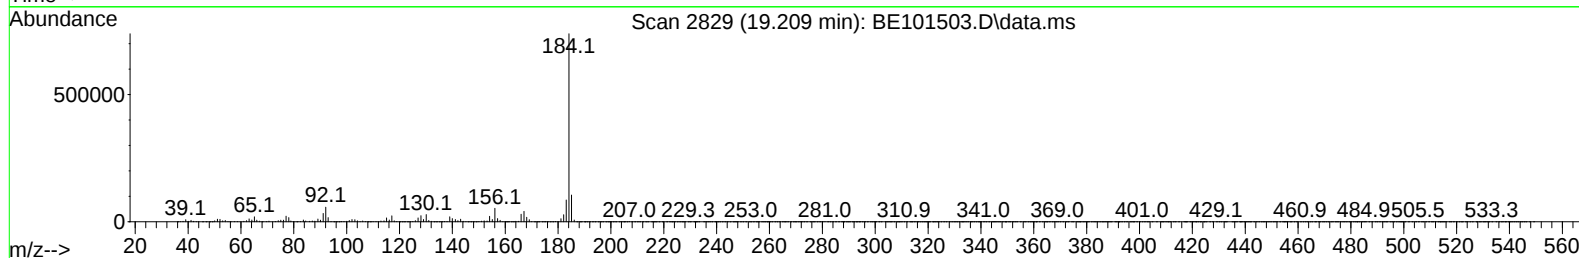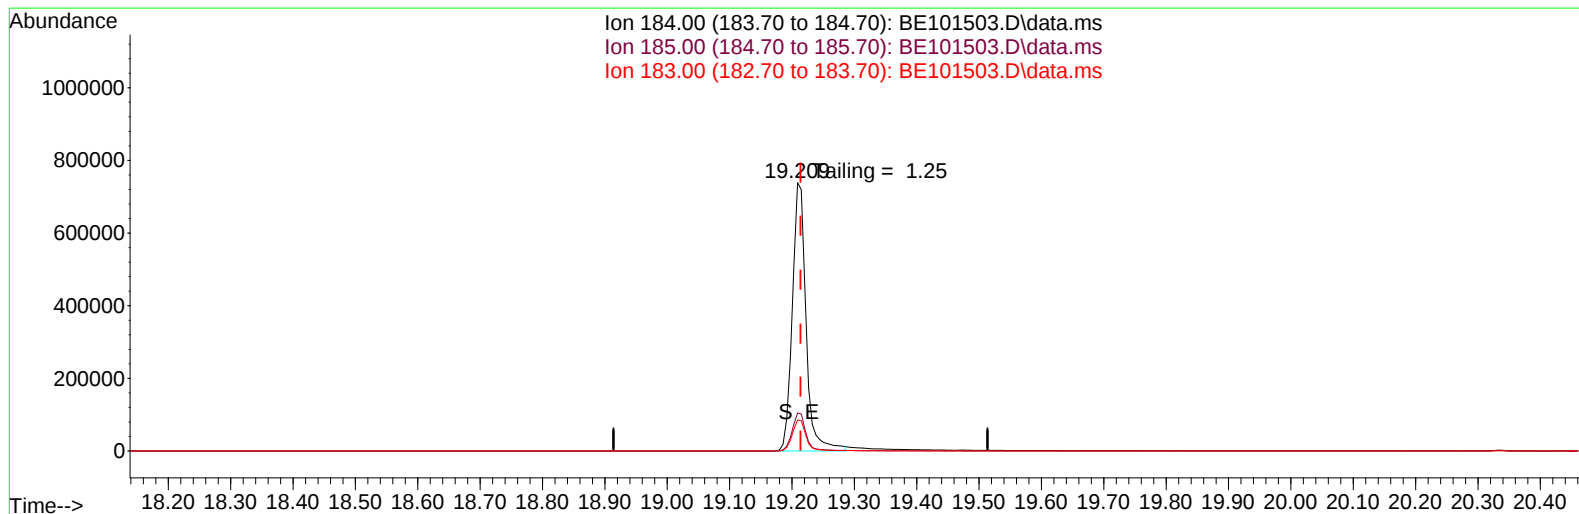

TIC: BE101503.D\data.ms

(77) Benzidine

19.209min (-0.005) 546347.88 ng

response 1185344

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.21
183.00	11.70	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/6/2024	BNA_E	<u>BE101503.D</u>
Compound Name	Response	Retention Time
DDT	652477	20.337
DDD	22005	19.902
DDE	898	19.391
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22903	675380	3.39

Instrument :
BNA_E
ClientSampleId :
DFTPP