

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
 Data File : BE101505.D
 Acq On : 6 Nov 2024 21:04
 Operator : RC/JU
 Sample : PB164561TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB164561TB

Quant Time: Nov 07 01:04:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.565	152	53927	20.000	ng	0.00
21) Naphthalene-d8	10.326	136	223555	20.000	ng	0.00
39) Acenaphthene-d10	14.169	164	146954	20.000	ng	0.00
64) Phenanthrene-d10	16.907	188	335497	20.000	ng	0.00
76) Chrysene-d12	21.067	240	420702	20.000	ng	-0.01
86) Perylene-d12	23.352	264	609595	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.314	112	477509	156.567	ng	0.00
7) Phenol-d6	6.942	99	592785	141.760	ng	0.00
23) Nitrobenzene-d5	8.769	82	345256	97.551	ng	0.00
42) 2,4,6-Tribromophenol	15.679	330	389579	140.885	ng	0.00
45) 2-Fluorobiphenyl	12.794	172	908654	100.960	ng	0.00
79) Terphenyl-d14	19.504	244	1855262	97.616	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101505.D
Acq On : 6 Nov 2024 21:04
Operator : RC/JU
Sample : PB164561TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164561TB


Quant Time: Nov 07 01:04:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

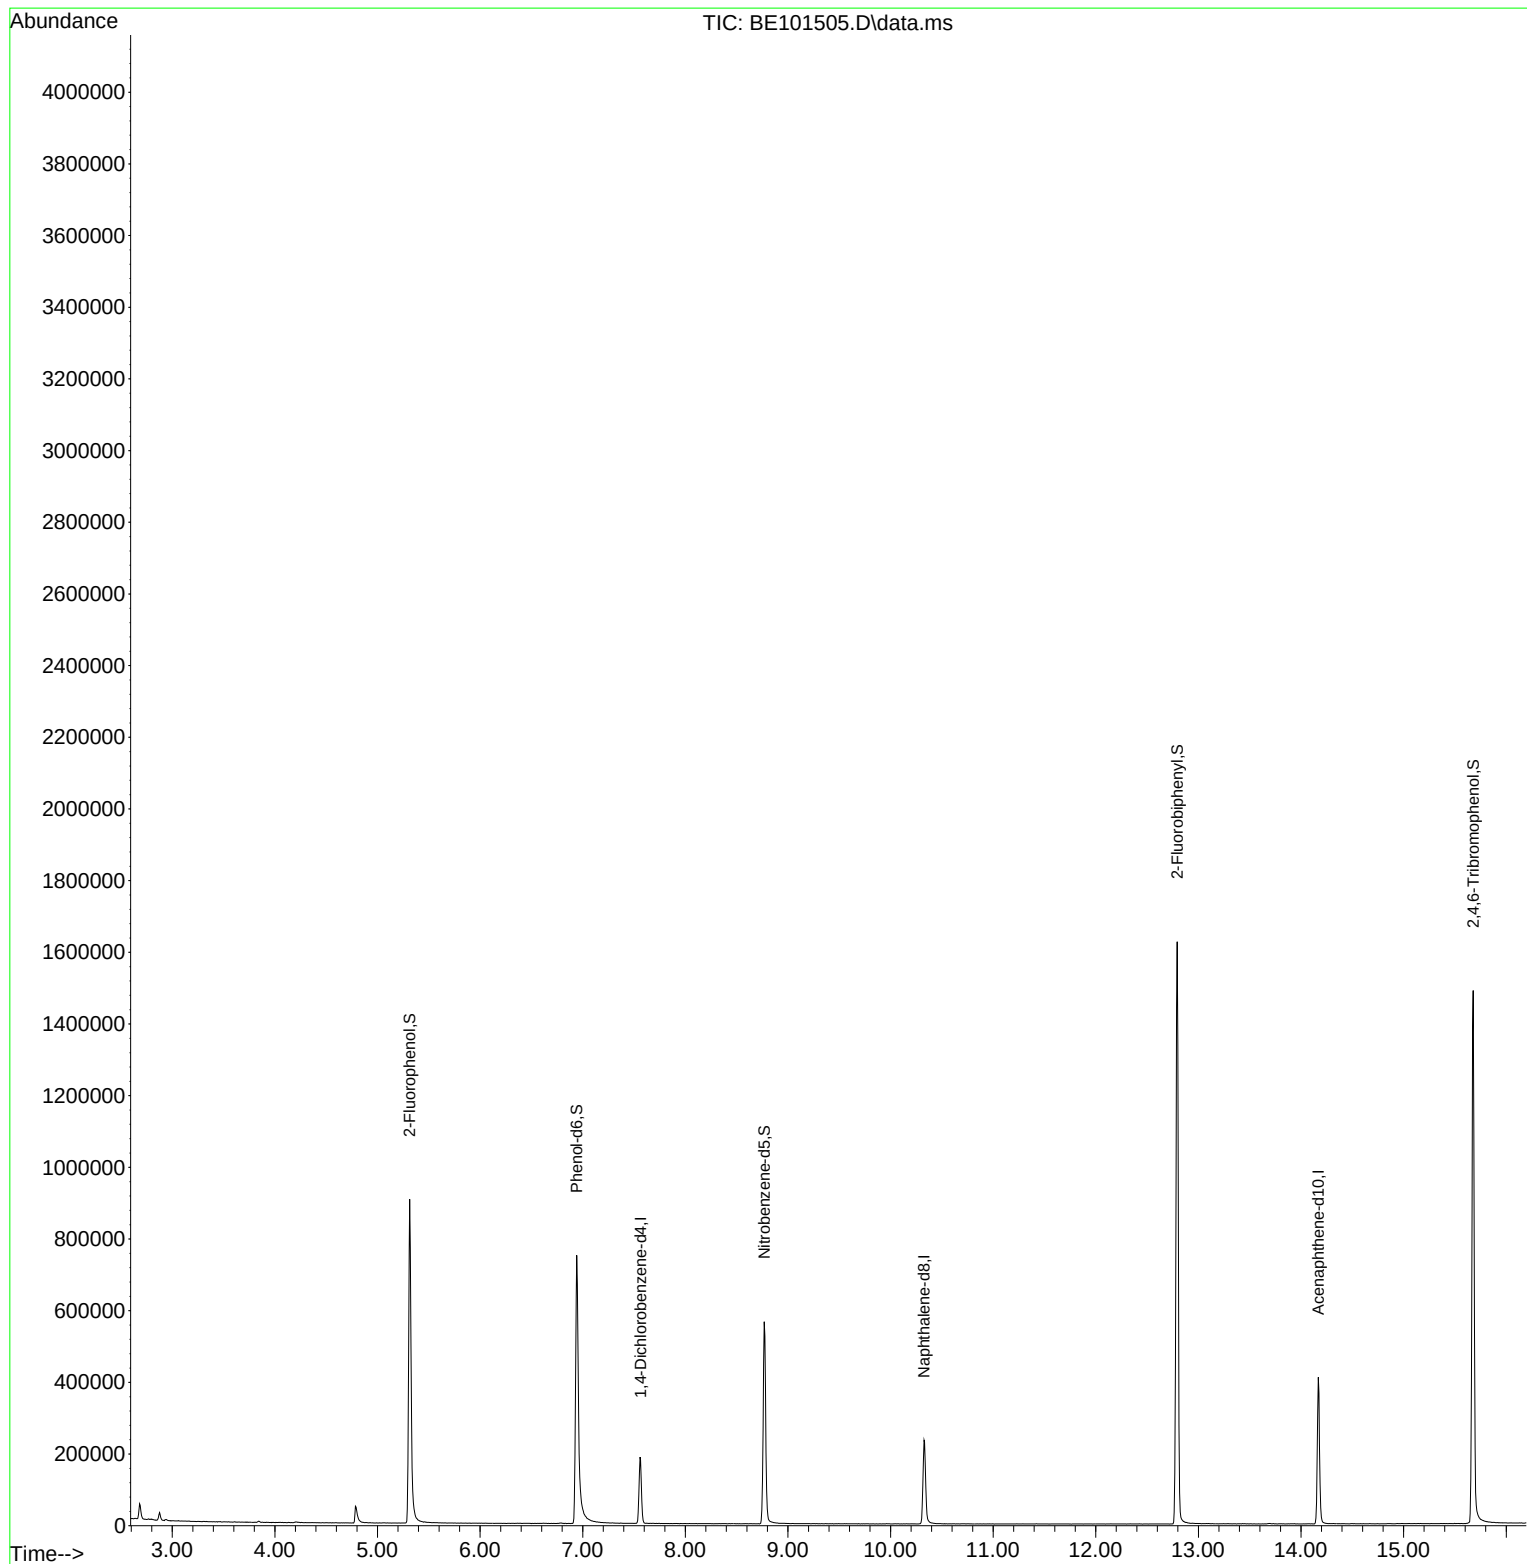


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110624\
Data File : BE101505.D
Acq On : 6 Nov 2024 21:04
Operator : RC/JU
Sample : PB164561TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164561TB

Quant Time: Nov 07 01:04:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration




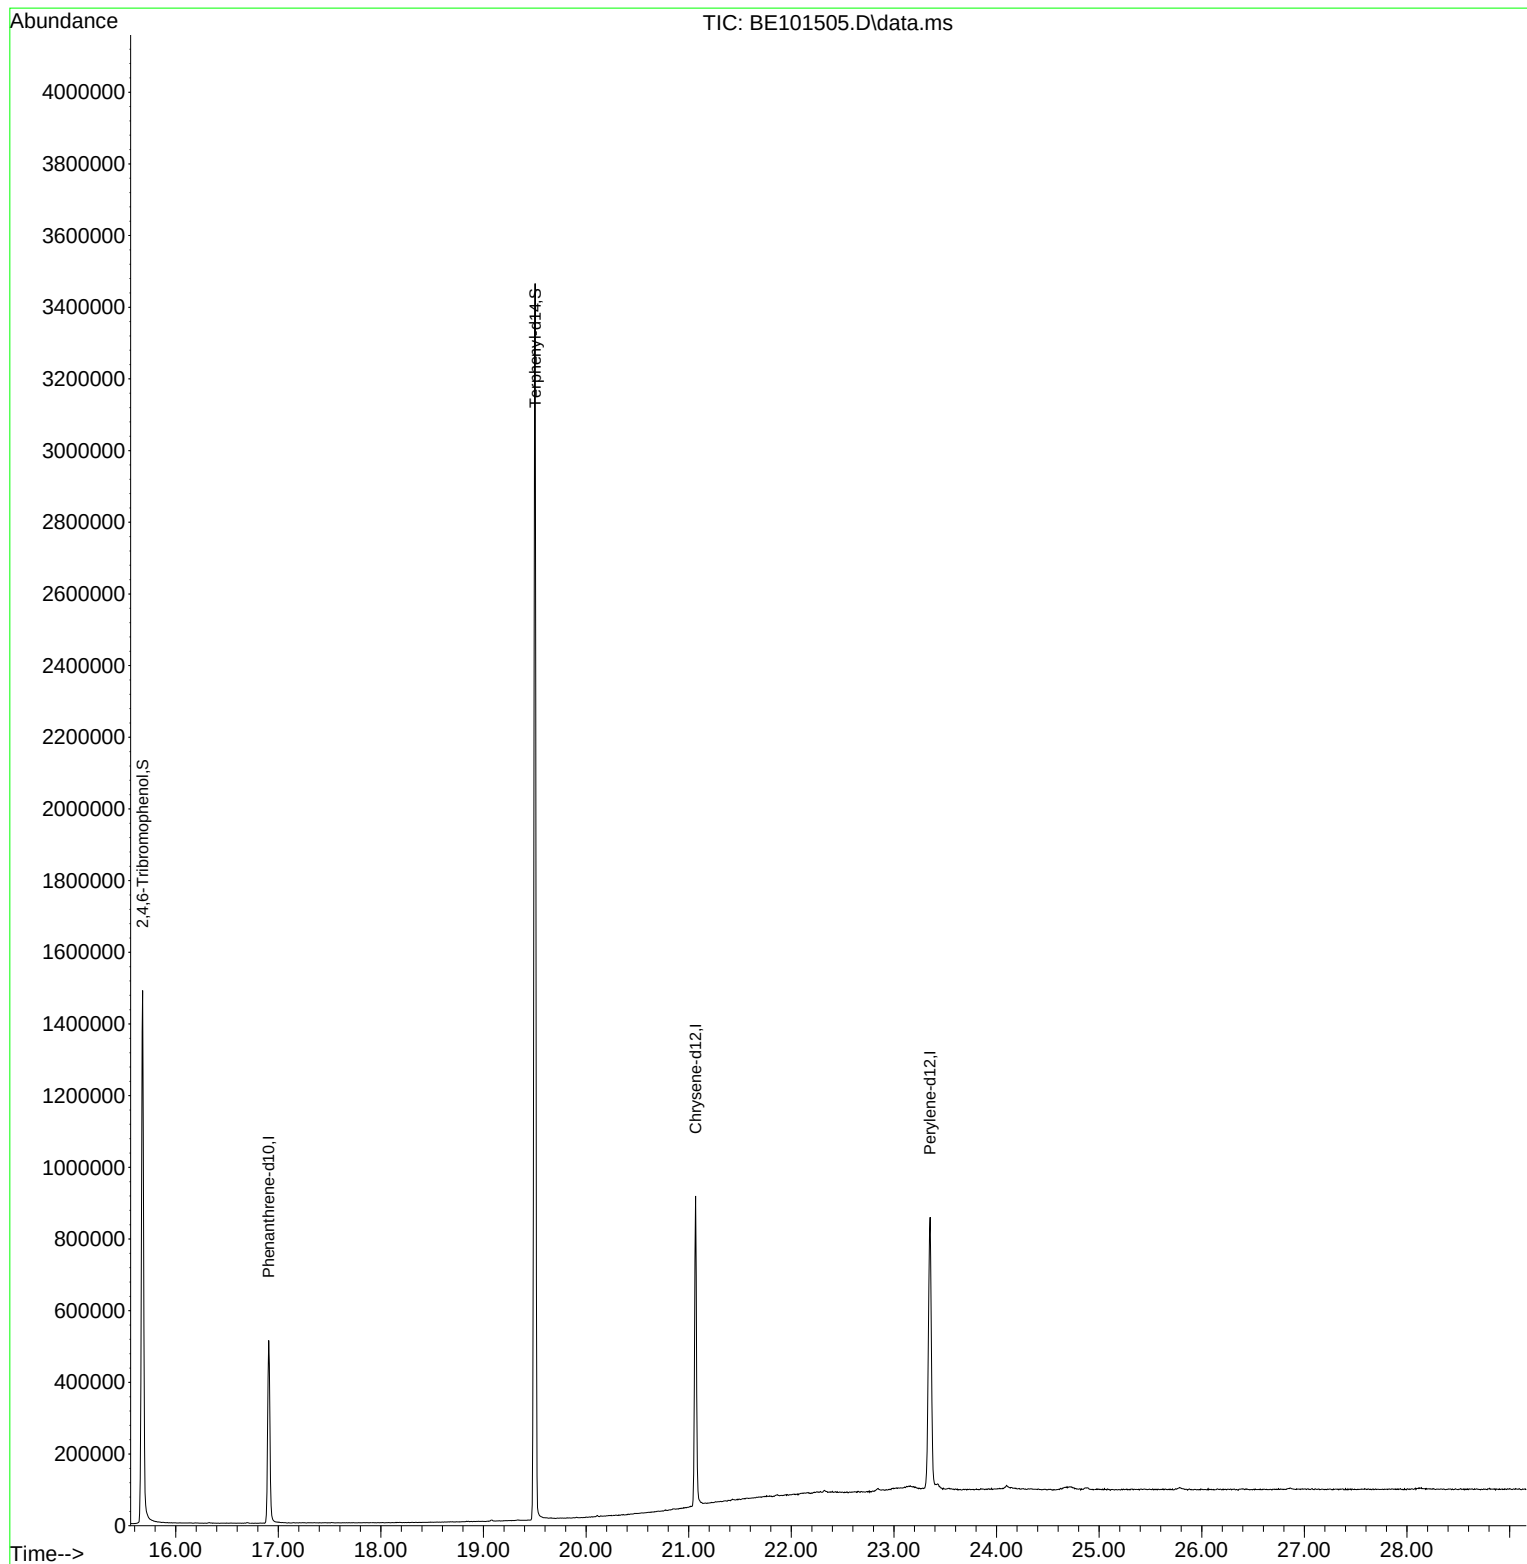




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.565 min Scan# 847
Delta R.T. 0.002 min
Lab File: BE101505.D
Acq: 6 Nov 2024 21:04




Instrument :
BNA_E
ClientSampleId :
PB164561TB


Tgt Ion:152 Resp: 53927
Ion Ratio Lower Upper
152 100
150 150.3 126.3 189.5
115 55.8 45.0 67.4

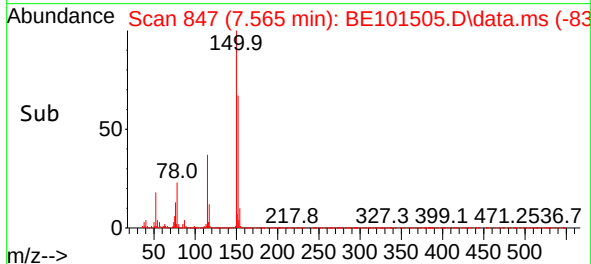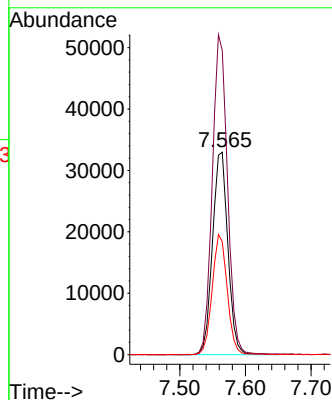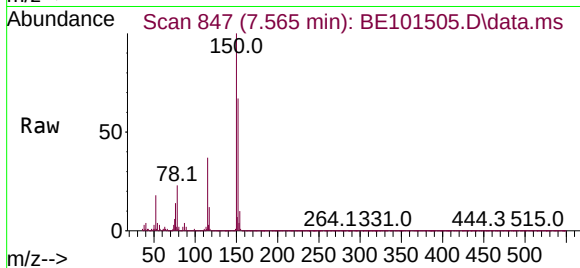

#5
2-Fluorophenol
Concen: 156.567 ng
RT: 5.314 min Scan# 464
Delta R.T. 0.001 min
Lab File: BE101505.D
Acq: 6 Nov 2024 21:04

Tgt Ion:112 Resp: 477509
Ion Ratio Lower Upper
112 100
64 53.5 43.2 64.8
63 26.9 21.8 32.6


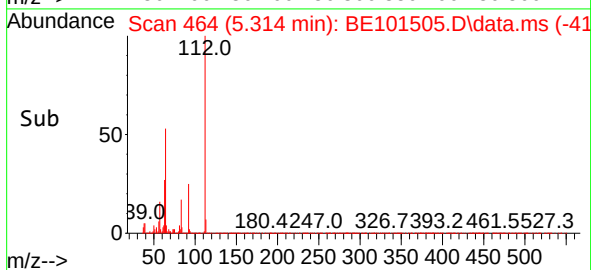
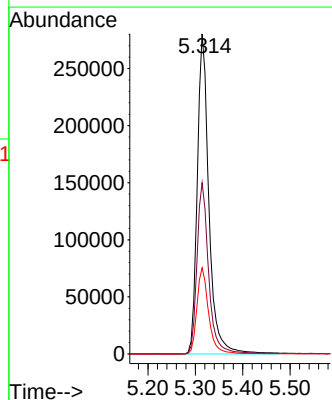
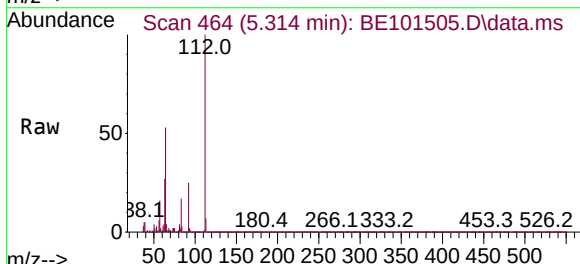




#7
Phenol-d6
Concen: 141.760 ng
RT: 6.942 min Scan# 741
Delta R.T. -0.004 min
Lab File: BE101505.D
Acq: 6 Nov 2024 21:04




Instrument :
BNA_E
ClientSampleId :
PB164561TB


Tgt Ion: 99 Resp: 592785
Ion Ratio Lower Upper
99 100
42 15.8 12.5 18.7
71 31.0 24.2 36.2

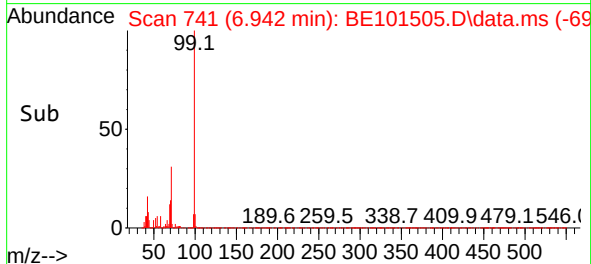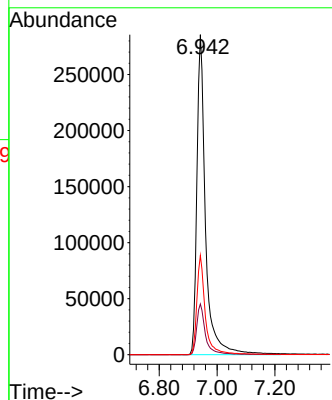

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.326 min Scan# 1317
Delta R.T. -0.004 min
Lab File: BE101505.D
Acq: 6 Nov 2024 21:04

Tgt Ion: 136 Resp: 223555
Ion Ratio Lower Upper
136 100
137 11.1 8.6 13.0
54 7.0 5.6 8.4
68 6.2 4.8 7.2


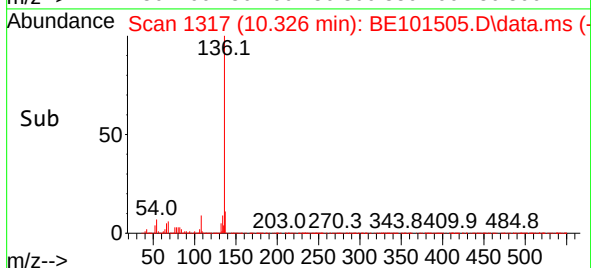
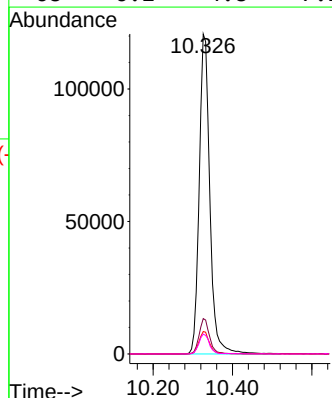
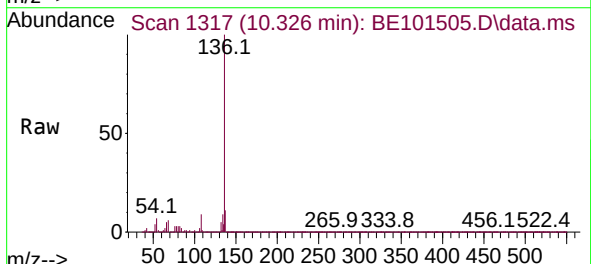




#23
Nitrobenzene-d5
Concen: 97.551 ng
RT: 8.769 min Scan# 1052
Delta R.T. -0.004 min
Lab File: BE101505.D
Acq: 6 Nov 2024 21:04




Instrument :
BNA_E
ClientSampleId :
PB164561TB


Tgt Ion: 82 Resp: 345256
Ion Ratio Lower Upper
82 100
128 46.9 38.6 58.0
54 45.3 36.3 54.5

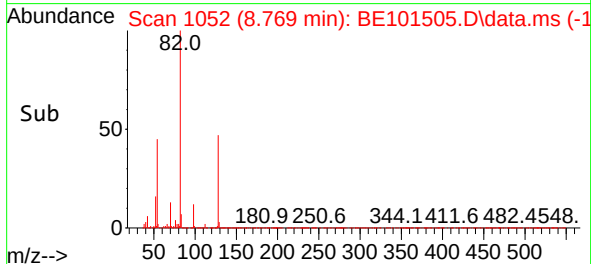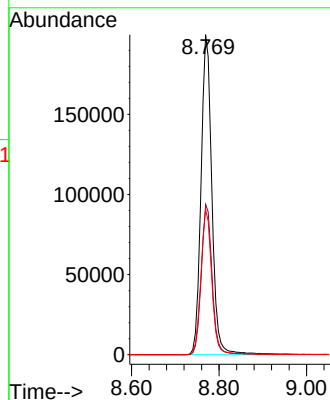

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.169 min Scan# 1971
Delta R.T. -0.004 min
Lab File: BE101505.D
Acq: 6 Nov 2024 21:04

Tgt Ion:164 Resp: 146954
Ion Ratio Lower Upper
164 100
162 105.9 83.7 125.5
160 45.8 37.1 55.7

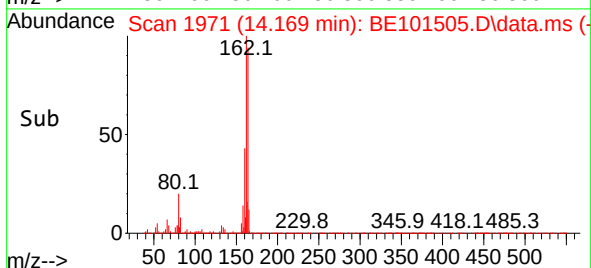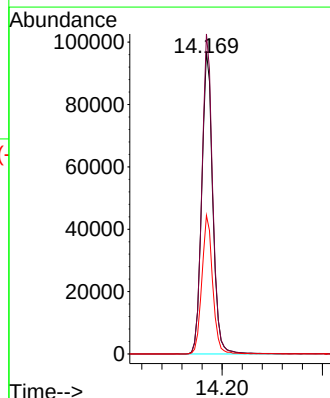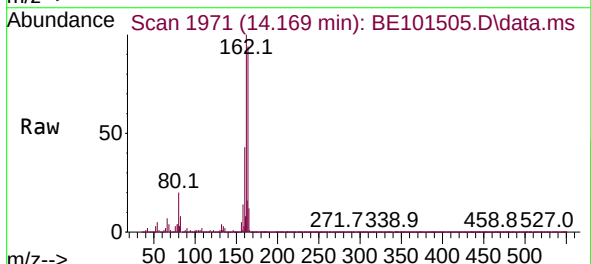

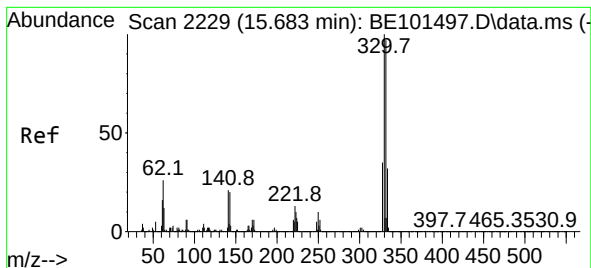

#42

2,4,6-Tribromophenol

Concen: 140.885 ng

RT: 15.679 min Scan# 21

Delta R.T. -0.004 min

Lab File: BE101505.D

Acq: 6 Nov 2024 21:04

Instrument :

BNA_E

ClientSampleId :

PB164561TB





Tgt Ion:330 Resp: 389579

Ion Ratio Lower Upper

330 100

332 97.2 77.7 116.5

141 21.3 17.0 25.4

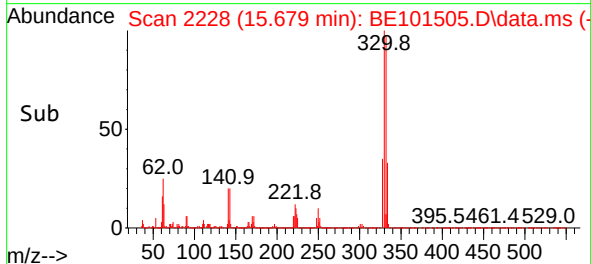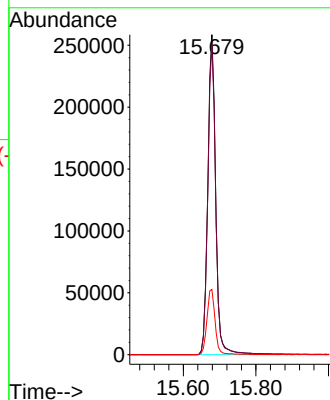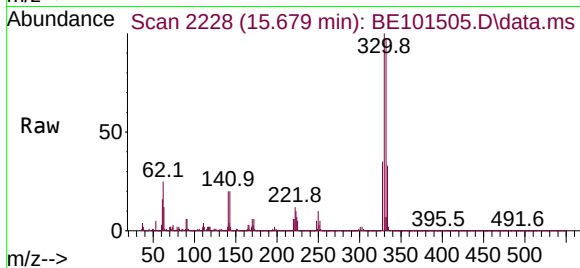

#45

2-Fluorobiphenyl

Concen: 100.960 ng

RT: 12.794 min Scan# 1737

Delta R.T. -0.004 min

Lab File: BE101505.D

Acq: 6 Nov 2024 21:04




Tgt Ion:172 Resp: 908654


Ion Ratio Lower Upper

172 100

171 35.0 28.6 43.0

170 23.5 18.9 28.3


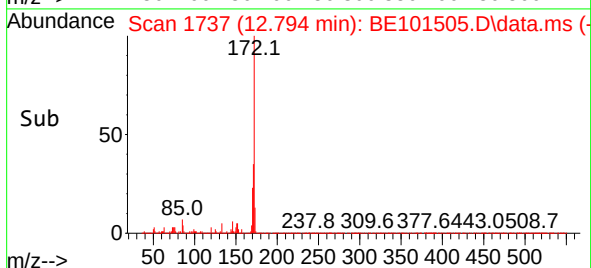
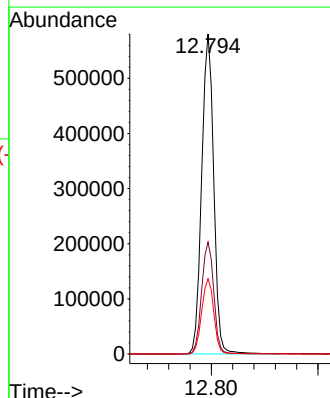
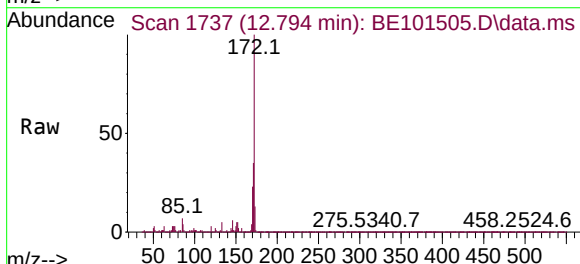


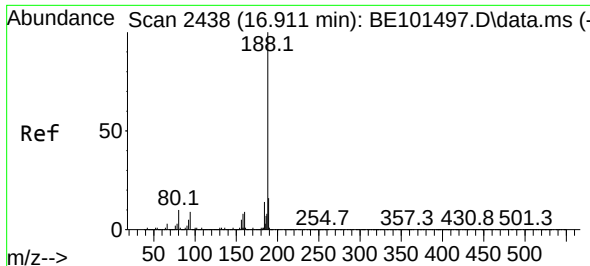

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.907 min Scan# 2438
Delta R.T. -0.004 min
Lab File: BE101505.D
Acq: 6 Nov 2024 21:04




Instrument :
BNA_E
ClientSampleId :
PB164561TB


Tgt Ion:188 Resp: 335497
Ion Ratio Lower Upper
188 100
94 9.7 7.4 11.2
80 10.3 8.0 12.0

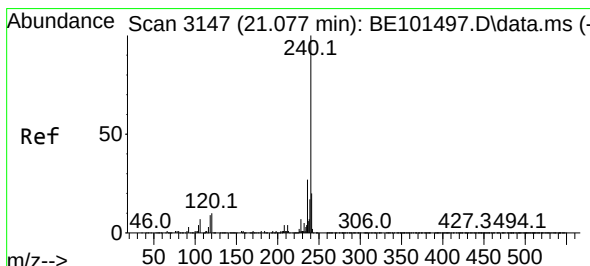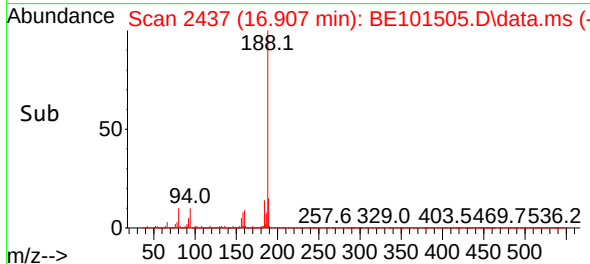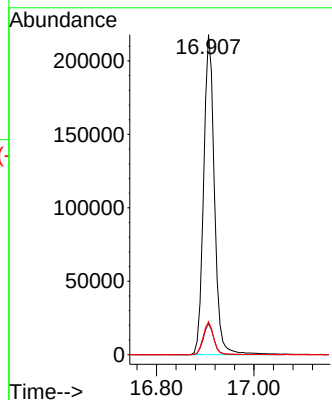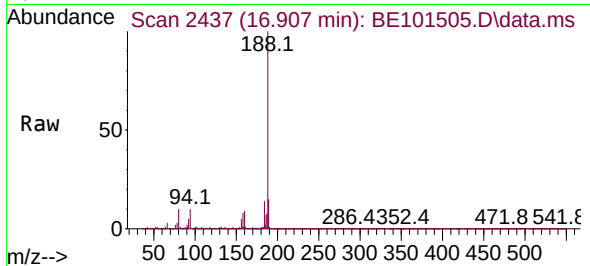

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.067 min Scan# 3145
Delta R.T. -0.010 min
Lab File: BE101505.D
Acq: 6 Nov 2024 21:04

Tgt Ion:240 Resp: 420702
Ion Ratio Lower Upper
240 100
120 10.6 8.2 12.4
236 26.1 21.4 32.2

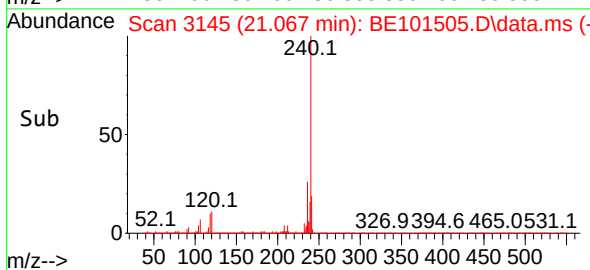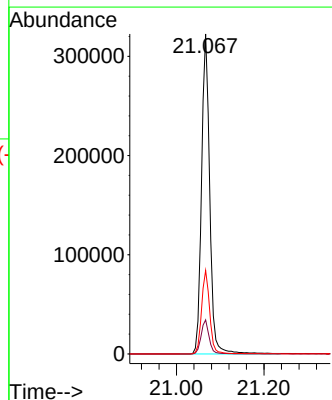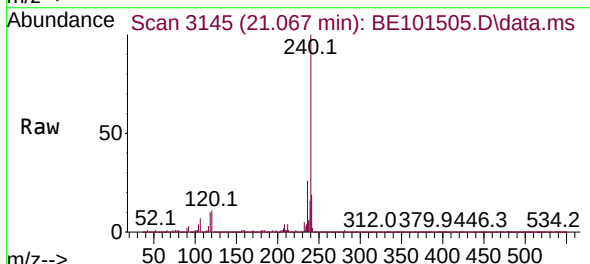

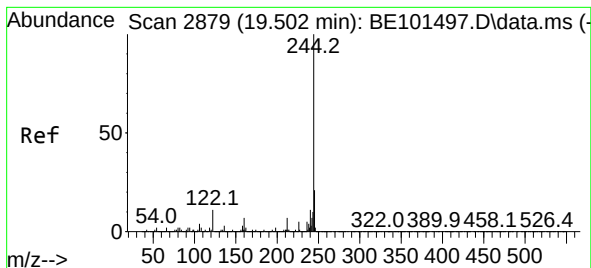

#79

Terphenyl-d14

Concen: 97.616 ng

RT: 19.504 min Scan# 21

Delta R.T. 0.001 min

Lab File: BE101505.D

Acq: 6 Nov 2024 21:04

Instrument :

BNA_E

ClientSampleId :

PB164561TB





Tgt Ion:244 Resp: 1855262

Ion Ratio Lower Upper

244 100

212 6.8 5.8 8.8

122 10.0 8.4 12.6

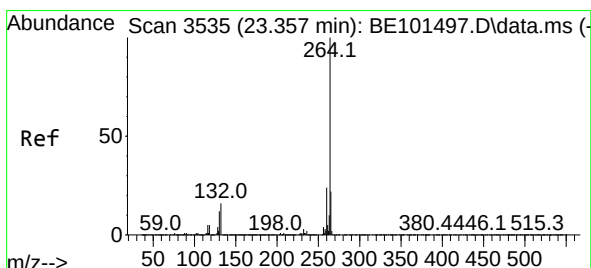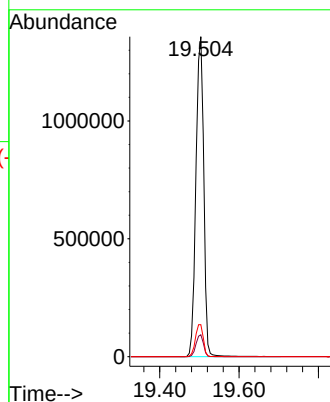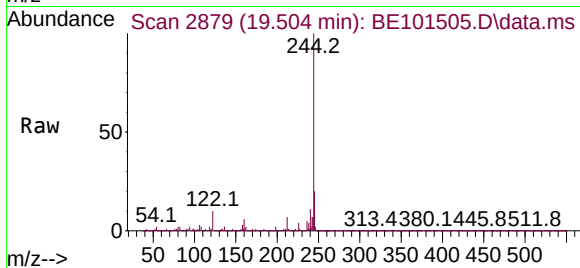

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.352 min Scan# 3534

Delta R.T. -0.004 min

Lab File: BE101505.D

Acq: 6 Nov 2024 21:04

Tgt Ion:264 Resp: 609595

Ion Ratio Lower Upper

264 100

260 24.0 19.4 29.2

265 21.5 17.4 26.2

