


LA133275

7471B

INSTRUMENT ID: CV1

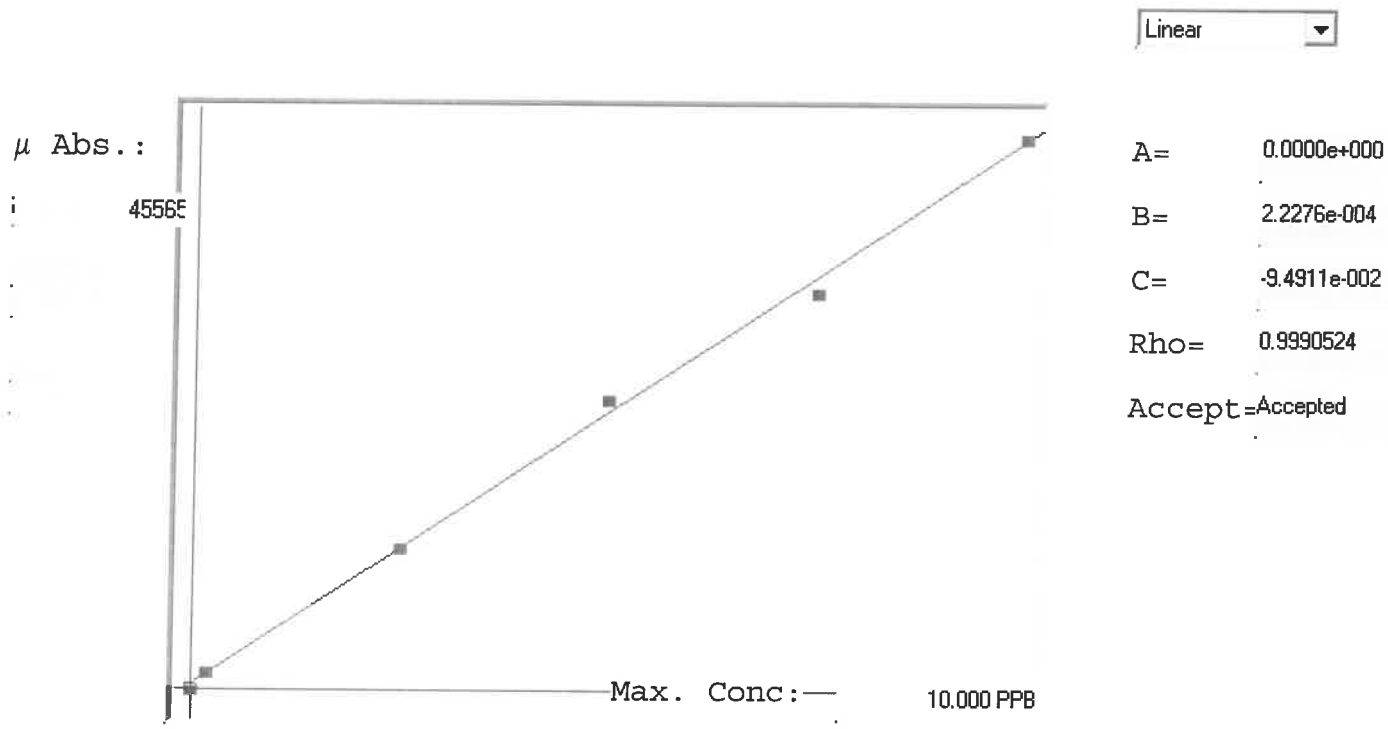

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	O/b)
0.0	0.000	-0.087	-0.087	36	0.000	36					0/0)
0.2	0.200	0.234	0.034	1476	0.0 %	1476					17
2.5	2.500	2.509	0.009	11687	0.0 %	11687					0
5.0	5.000	5.262	0.262	24047	0.0 %	24047					5
7.5	7.500	7.227	-0.273	32870	0.0 %	32870					-4
10.0	10.000	10.055	0.055	45565	0.0 %	45565					1

LB133275 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 04 Nov 2024 13:44:04

Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	36	-	0.0000	7471B	PPB	04 Nov 2024 13:47:07	S	Std
0.2 - 1	56.2	1476	-	0.2000	7471B	PPB	04 Nov 2024 13:49:24	S	Std
2.5 - 1	52.5	11687	-	2.5000	7471B	PPB	04 Nov 2024 13:51:40	S	Std
5.0 - 1	55	24047	-	5.0000	7471B	PPB	04 Nov 2024 13:53:57	S	Std
7.5 - 1	57.5	32870	-	7.5000	7471B	PPB	04 Nov 2024 13:56:16	S	Std
10.0 - 1	510	45565	-	10.0000	7471B	PPB	04 Nov 2024 14:08:28	S	Std
ICV68 - 1	ICV68	18935	4.1231	-	7471B	PPB	04 Nov 2024 14:11:13	U	SMPL
ICB68 - 1	ICB68	78	-0.0775	-	7471B	PPB	04 Nov 2024 14:16:05	U	SMPL
CCV22 - 1	CCV22	24181	5.2917	-	7471B	PPB	04 Nov 2024 14:18:20	U	SMPL
CCB22 - 1	CCB22	139	-0.0639	-	7471B	PPB	04 Nov 2024 14:23:16	U	SMPL
CRA - 1	CRA	1368	0.2098	-	7471B	PPB	04 Nov 2024 14:25:31	U	SMPL
HighStd - 1	HighStd	45263	9.9880	-	7471B	PPB	04 Nov 2024 14:27:45	U	SMPL
ChkStd - 1	ChkStd	30897	6.7878	-	7471B	PPB	04 Nov 2024 14:30:00	U	SMPL
PB164668BL - 1	PBS	81	-0.0769	-	7471B	PPB	04 Nov 2024 14:32:24	U	SMPL
PB164668BS - 1	LCSS	16266	3.5286	-	7471B	PPB	04 Nov 2024 14:34:45	U	SMPL
P4663-02MS - 1	TENNANT-PAD-2-3-STOCKPILEMS	22366	4.8874	-	7471B	PPB	04 Nov 2024 14:41:40	U	SMPL
P4663-02MSD - 1	TENNANT-PAD-2-3-STOCKPILEMSD	21594	4.7154	-	7471B	PPB	04 Nov 2024 14:43:58	U	SMPL
P4663-04 - 1	RES-BUILDING-PAD-NO-11	1576	0.2562	-	7471B	PPB	04 Nov 2024 14:46:16	U	SMPL
CCV23 - 1	CCV23	24377	5.3354	-	7471B	PPB	04 Nov 2024 14:48:34	U	SMPL
CCB23 - 1	CCB23	132	-0.0655	-	7471B	PPB	04 Nov 2024 14:53:22	U	SMPL
P4663-06 - 1	RES-BUILDING-PAD-NO-3	1510	0.2415	-	7471B	PPB	04 Nov 2024 14:55:37	U	SMPL
P4663-08 - 1	RES-BUILDING-PAD-NO-2	462	0.0080	-	7471B	PPB	04 Nov 2024 14:57:53	U	SMPL
P4667-01 - 1	BP-F-6	198	-0.0508	-	7471B	PPB	04 Nov 2024 15:00:08	U	SMPL
P4667-05 - 1	BP-F-5	639	0.0474	-	7471B	PPB	04 Nov 2024 15:02:24	U	SMPL
P4667-09 - 1	BP-F-10	822	0.0882	-	7471B	PPB	04 Nov 2024 15:04:39	U	SMPL
P4667-13 - 1	BP-F-7	198	-0.0508	-	7471B	PPB	04 Nov 2024 15:06:55	U	SMPL
P4675-01 - 1	COMP-1	3264	0.6322	-	7471B	PPB	04 Nov 2024 15:09:11	U	SMPL
P4675-02 - 1	COMP-2	1771	0.2996	-	7471B	PPB	04 Nov 2024 15:11:28	U	SMPL
P4675-03 - 1	COMP-3	1218	0.1764	-	7471B	PPB	04 Nov 2024 15:13:46	U	SMPL
P4675-04 - 1	COMP-4	2011	0.3531	-	7471B	PPB	04 Nov 2024 15:16:01	U	SMPL
CCV24 - 1	CCV24	24513	5.3657	-	7471B	PPB	04 Nov 2024 15:18:17	U	SMPL
CCB24 - 1	CCB24	10	-0.0927	-	7471B	PPB	04 Nov 2024 15:20:33	U	SMPL
P4675-05 - 1	COMP-5	4610	0.9320	-	7471B	PPB	04 Nov 2024 15:22:51	U	SMPL
P4675-06 - 1	COMP-6	1650	0.2726	-	7471B	PPB	04 Nov 2024 15:25:06	U	SMPL
P4679-01 - 1	MH-1	5373	1.1020	-	7471B	PPB	04 Nov 2024 15:27:23	U	SMPL
P4680-01 - 1	BP-F26	90	-0.0749	-	7471B	PPB	04 Nov 2024 15:29:38	U	SMPL
P4680-05 - 1	BP-F25	269	-0.0350	-	7471B	PPB	04 Nov 2024 15:31:56	U	SMPL
P4663-02 - 1		1146	0.1604	-	7471B	PPB	04 Nov 2024 15:34:12	U	SMPL
P4663-02DUP - 1		1119	0.1544	-	7471B	PPB	04 Nov 2024 15:36:27	U	SMPL
P4663-02LX5 - 1		137	-0.0644	-	7471B	PPB	04 Nov 2024 15:38:44	U	SMPL
P4663-02A - 1		21838	4.7698	-	7471B	PPB	04 Nov 2024 15:41:01	U	SMPL
CCV25 - 1	CCV25	24728	5.4136	-	7471B	PPB	04 Nov 2024 15:43:16	U	SMPL
CCB25 - 1	CCB25	233	-0.0430	-	7471B	PPB	04 Nov 2024 15:45:34	U	SMPL