

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
 Data File : PS028236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 01:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 01:15:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 00:14:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.265	7.767	1031.4E6	841.3E6	572.049	537.947
Target Compounds							
1) T	Dalapon	2.643	0.000	810108	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.415	0.000	605770	0	<MDL	N.D. #
3) T	4-Nitroph...	7.055	0.000	4806175	0	4.055	N.D. #
6) T	MCP	0.000	8.116f	0	30264919	N.D.	5.849
7) T	MCPA	0.000	8.286f	0	12642513	N.D.	1.763
8) T	DICHLORPROP	8.179	0.000	221402	0	<MDL	N.D. #
10) T	Pentachlo...	8.746f	0.000	1240124	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.944	0	20828784	N.D.	1.937
12) T	2,4,5-T	0.000	10.342	0	3465338	N.D.	<MDL
13) T	2,4-DB	10.143	0.000	110288	0	<MDL	N.D. #
15) T	Picloram	11.152	12.397	7122510	2706095	<MDL	<MDL #
16) T	DCPA	11.659	0.000	1899272	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110524\
Data File : PS028236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 01:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 01:15:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110524.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 00:14:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

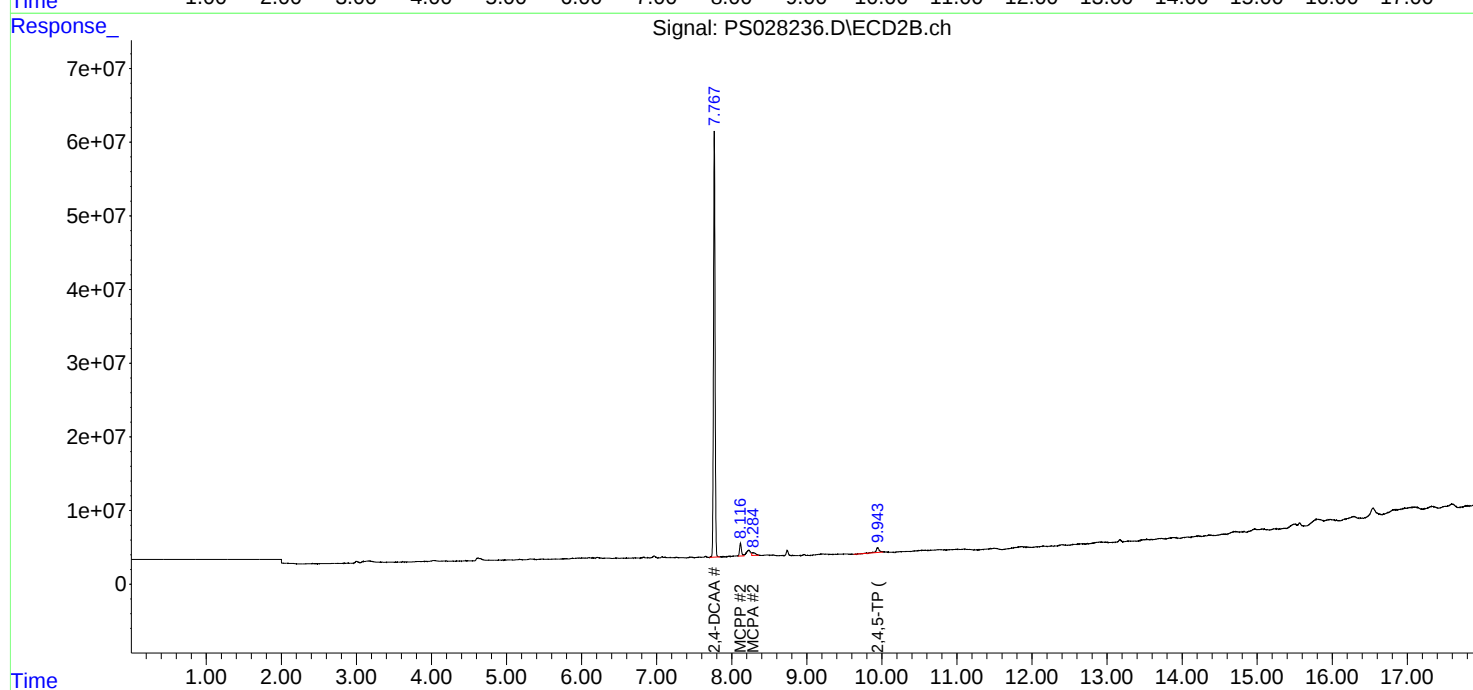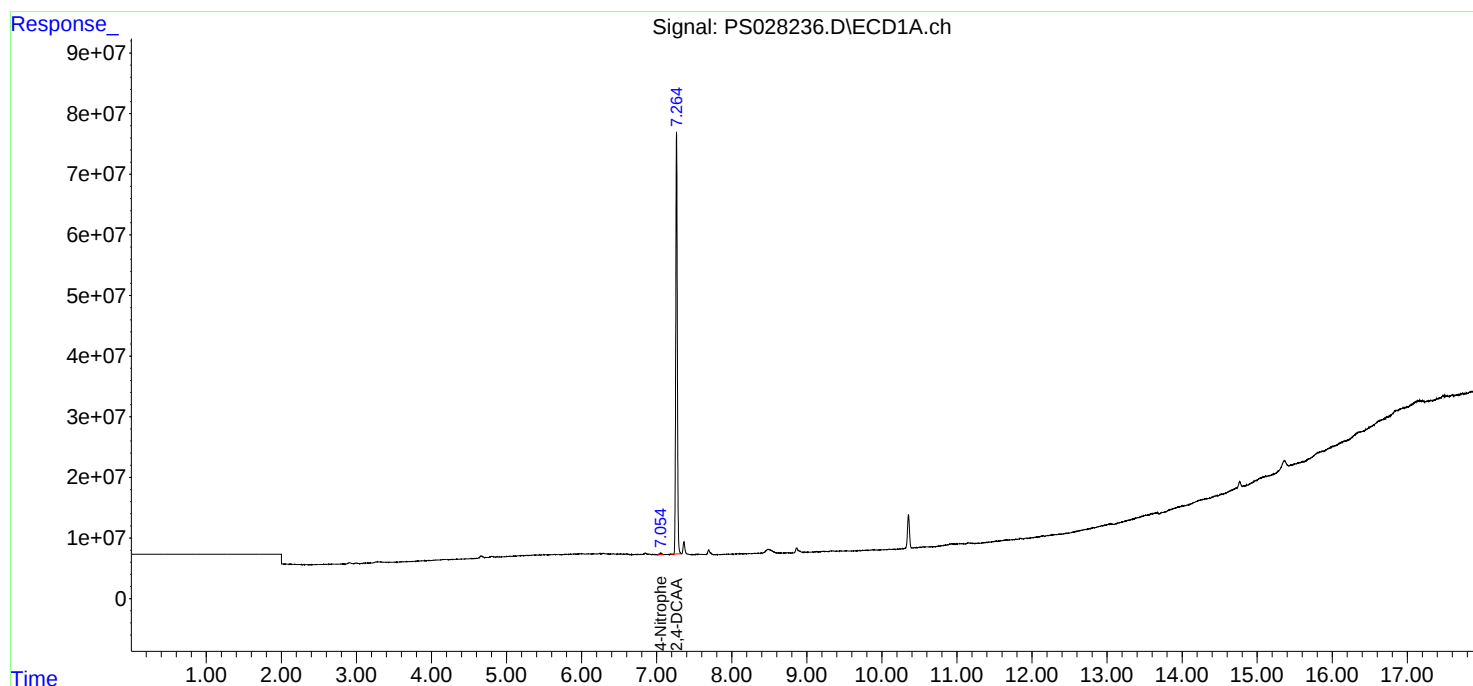


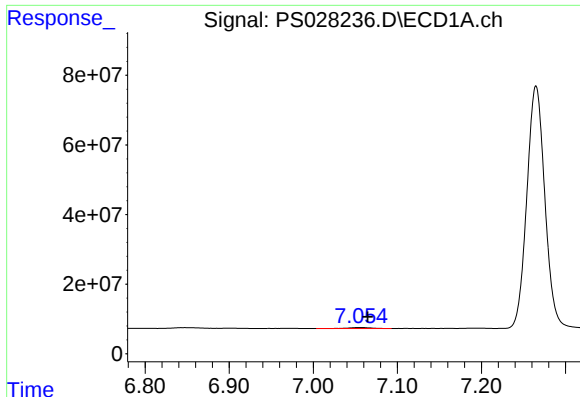

#3 4-Nitrophenol


R.T.: 7.055 min
Delta R.T.: -0.010 min
Response: 4806175
Conc: 4.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

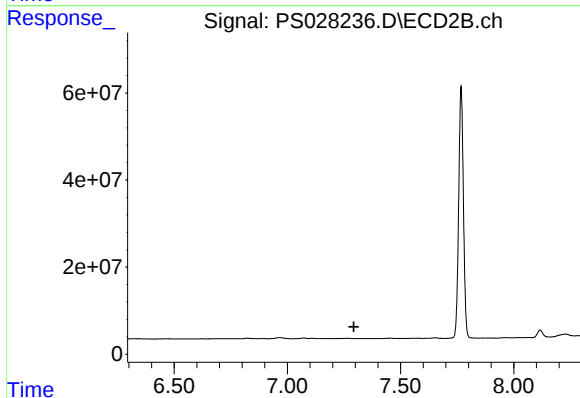


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.293 min
Response: 0
Conc: N.D.

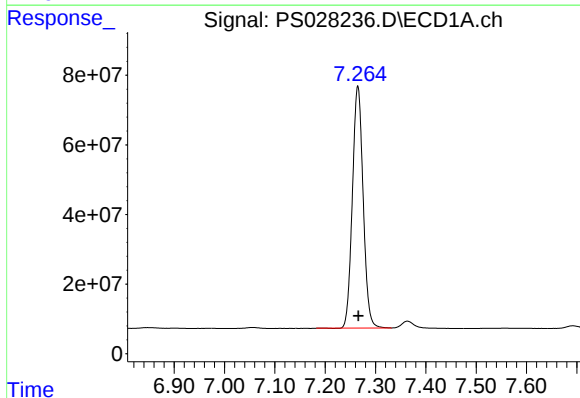


#4 2,4-DCAA

R.T.: 7.265 min
Delta R.T.: -0.001 min
Response: 1031423117
Conc: 572.05 ng/ml

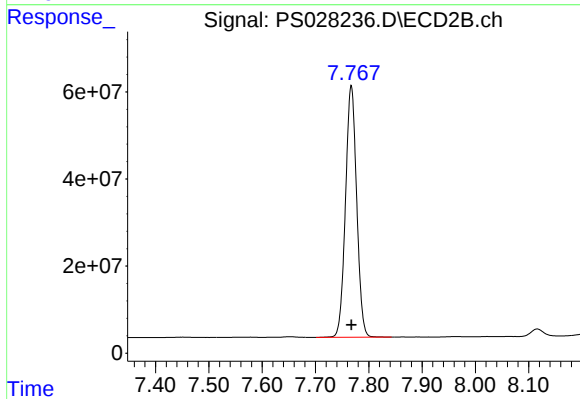

#4 2,4-DCAA


R.T.: 7.767 min
Delta R.T.: 0.000 min
Response: 841289422
Conc: 537.95 ng/ml

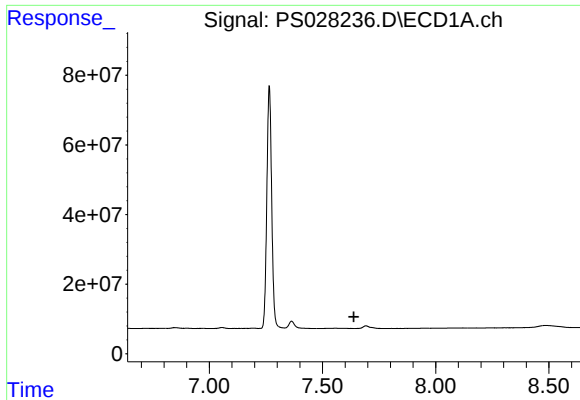

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.639 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

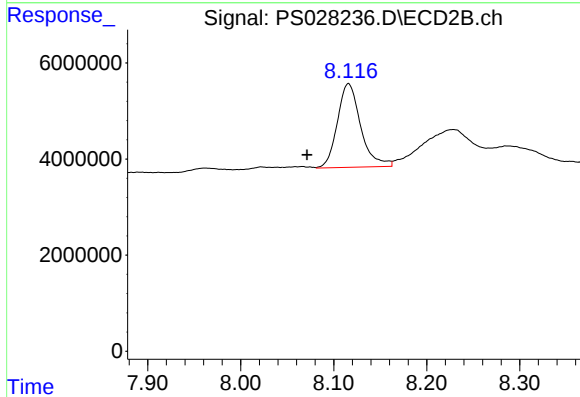


#6 MCPP

R.T.: 8.116 min
Delta R.T.: 0.044 min
Response: 30264919
Conc: 5.85 ug/ml

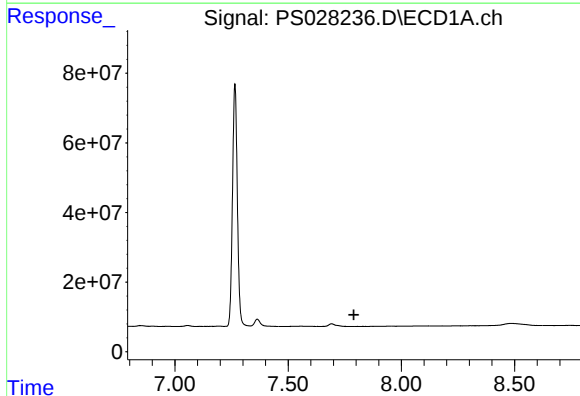


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.790 min
Response: 0
Conc: N.D.

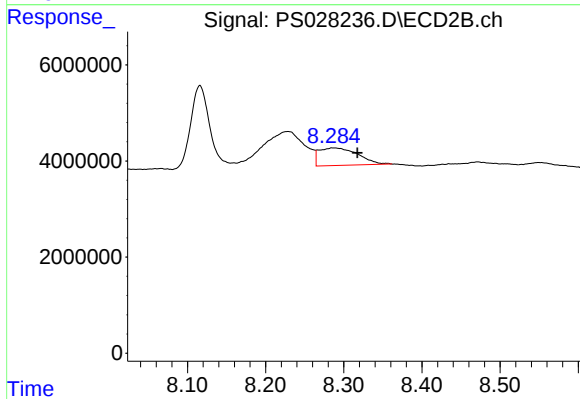

#7 MCPA


R.T.: 8.286 min
Delta R.T.: -0.031 min
Response: 12642513
Conc: 1.76 ug/ml

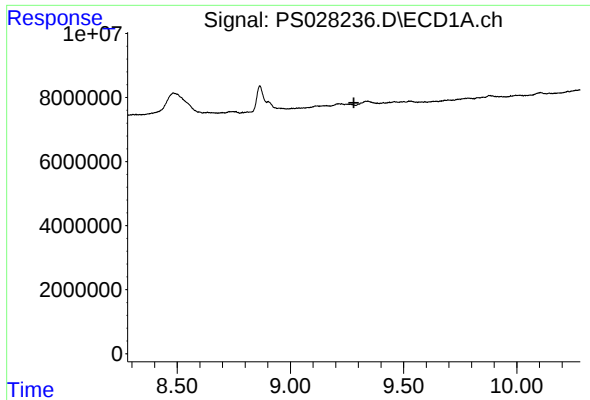

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

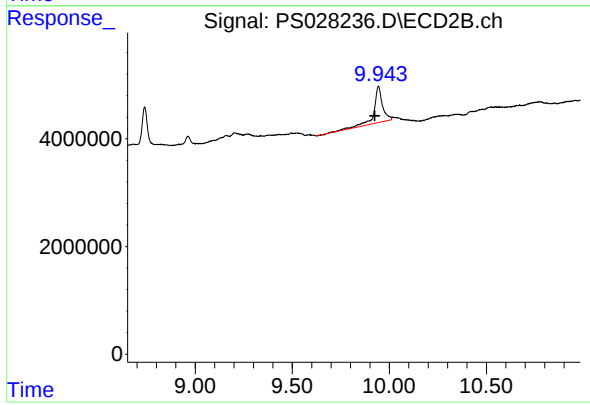

#11 2,4,5-TP (SILVEX)

R.T.: 9.944 min
Delta R.T.: 0.018 min
Response: 20828784
Conc: 1.94 ng/ml