

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110124\
 Data File : PP068353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 17:22
 Operator : YP\AJ
 Sample : P4663-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RES-BUILDING-PAD-NO-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:49:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.762	4.051	17086856	17374001	18.459	17.195
2) SA Decachlor...	10.677	9.209	19475197	17428494	16.916	15.541

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP110124\
Data File : PP068353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 17:22
Operator : YP\AJ
Sample : P4663-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RES-BUILDING-PAD-NO-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:49:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

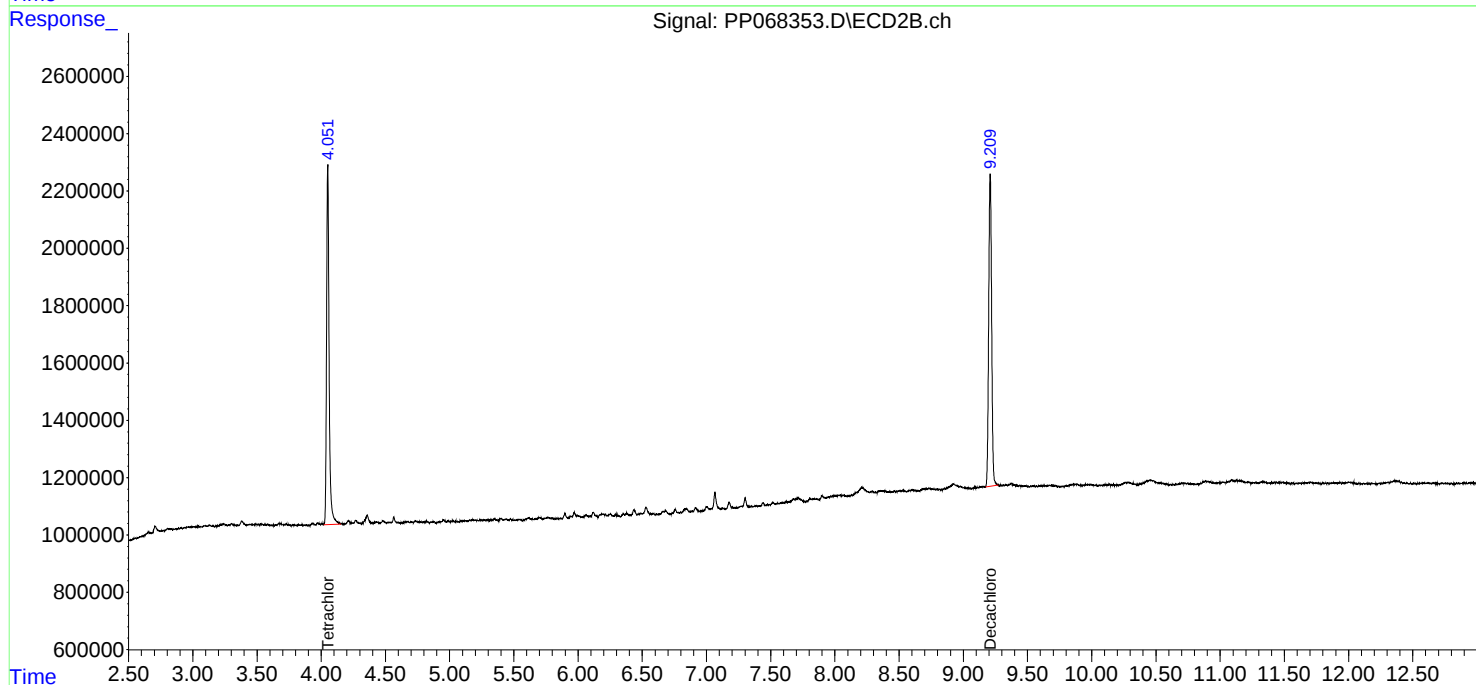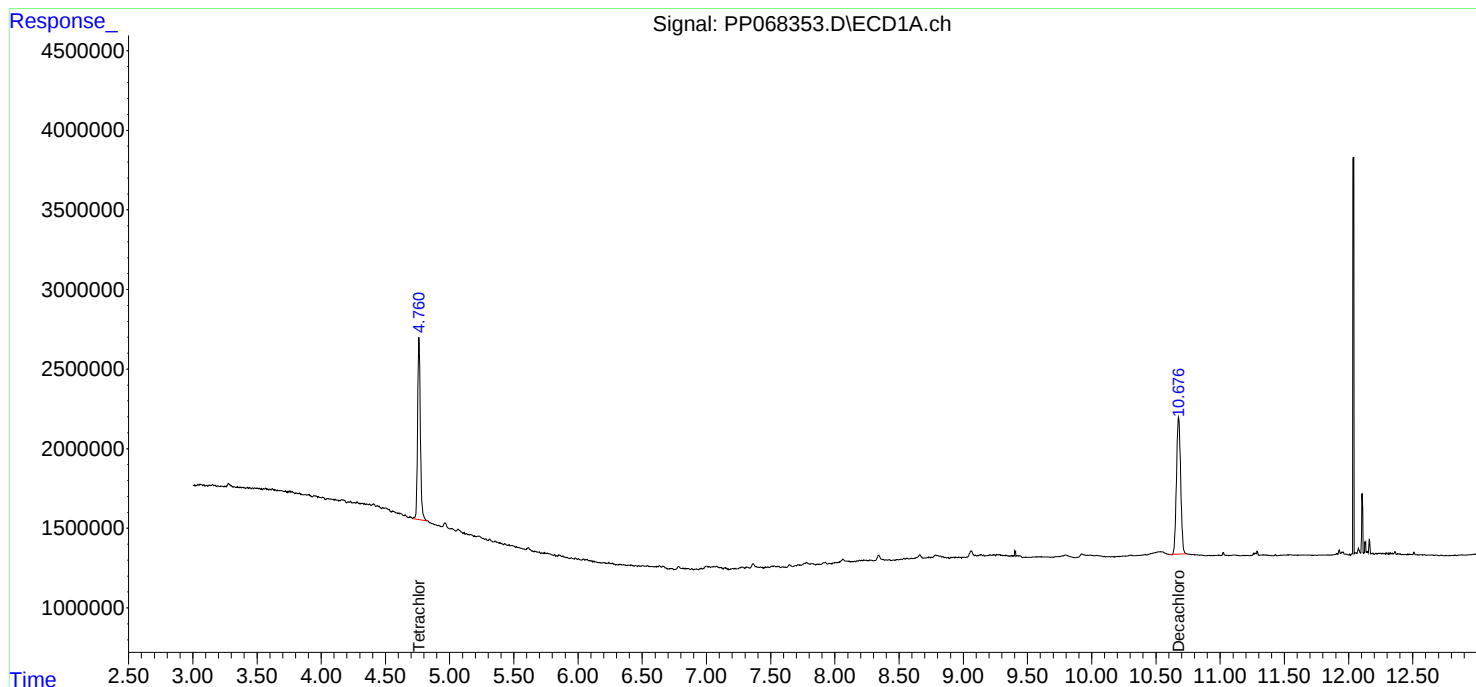


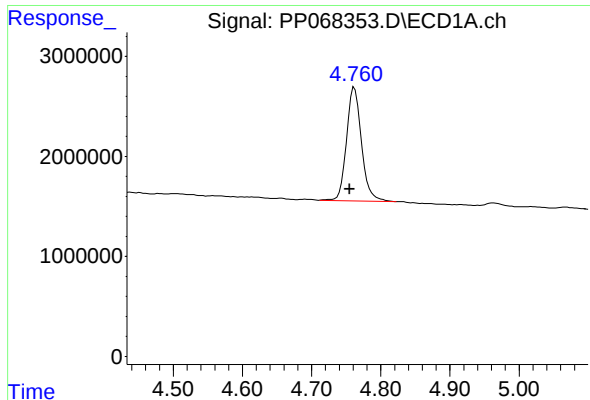

#1 Tetrachloro-m-xylene


R.T.: 4.762 min
Delta R.T.: 0.007 min
Response: 17086856
Conc: 18.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
RES-BUILDING-PAD-NO-2

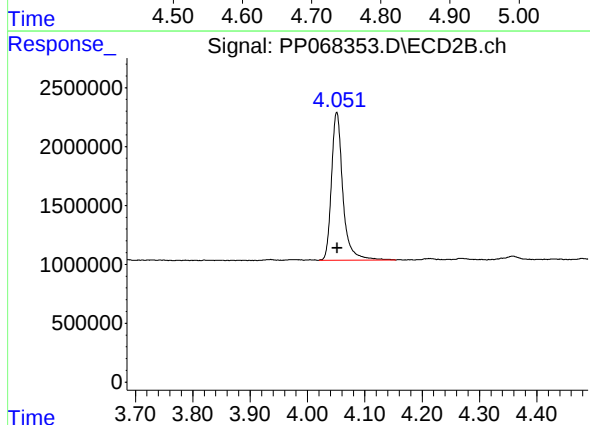


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 17374001
Conc: 17.20 ng/ml

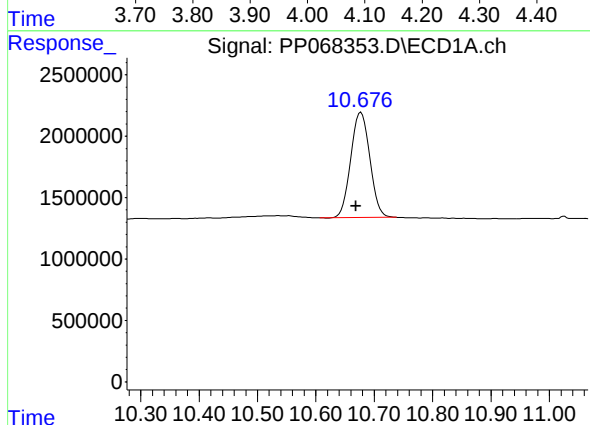

#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: 0.008 min
Response: 19475197
Conc: 16.92 ng/ml

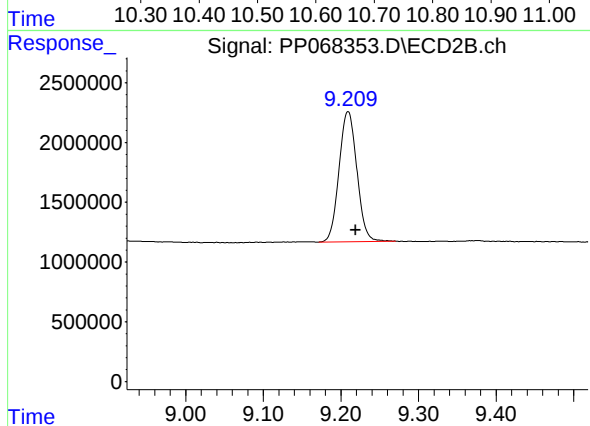

#2 Decachlorobiphenyl

R.T.: 9.209 min
Delta R.T.: -0.010 min
Response: 17428494
Conc: 15.54 ng/ml