
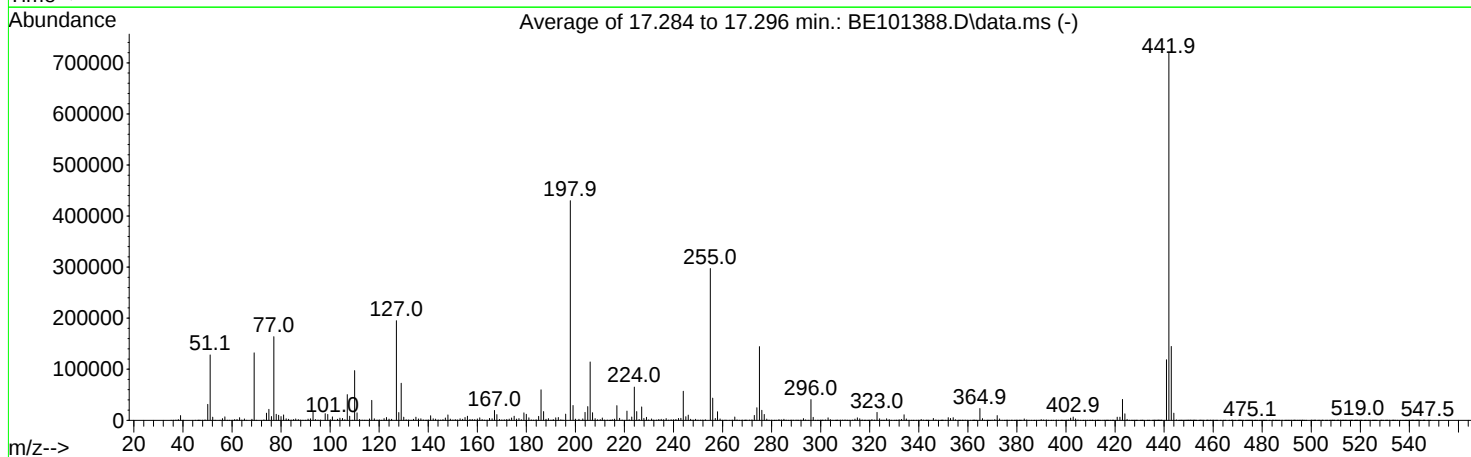


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
Data File : BE101388.D
Acq On : 28 Oct 2024 10:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 29 01:26:30 2024

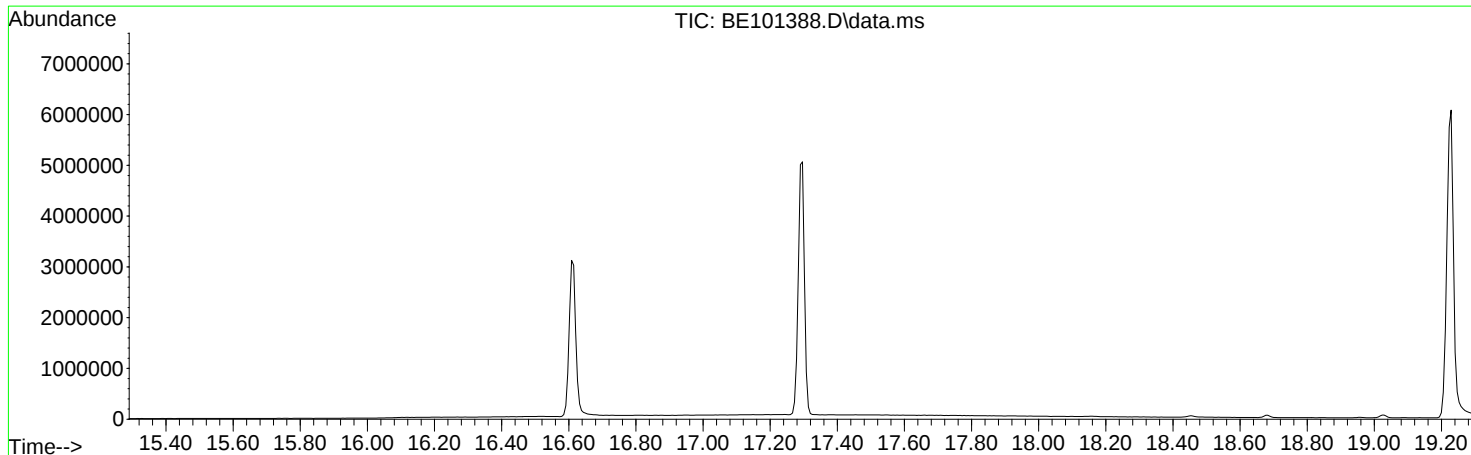

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	128023	PASS
68	69	0.00	2	1.5	1984	PASS
69	198	0.00	100	30.7	132146	PASS
70	69	0.00	2	0.1	198	PASS
127	198	10	80	45.4	195155	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	430187	PASS
199	198	5	9	6.7	28884	PASS
275	198	10	60	33.5	144206	PASS
365	198	1	100	5.4	23020	PASS
441	198	0.01	100	27.6	118563	PASS
442	442	50	100	100.0	720425	PASS
443	442	15	24	20.1	144667	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/28/2024	BNA_E	<u>BE101388.D</u>
Compound Name	Response	Retention Time
DDT	1836699	20.351
DDD	25787	19.916
DDE	1987	19.405
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27774	1864473	1.49

Instrument :
BNA_E
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
Data File : BE101388.D
Acq On : 28 Oct 2024 10:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Oct 29 01:32:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

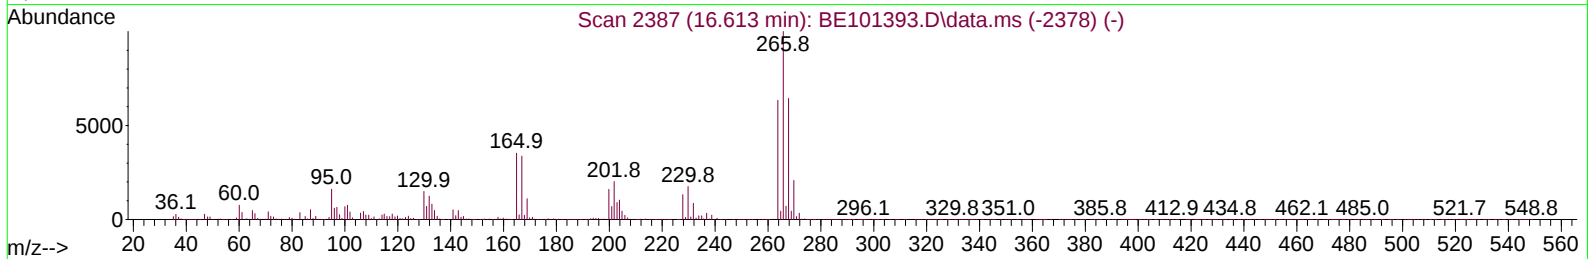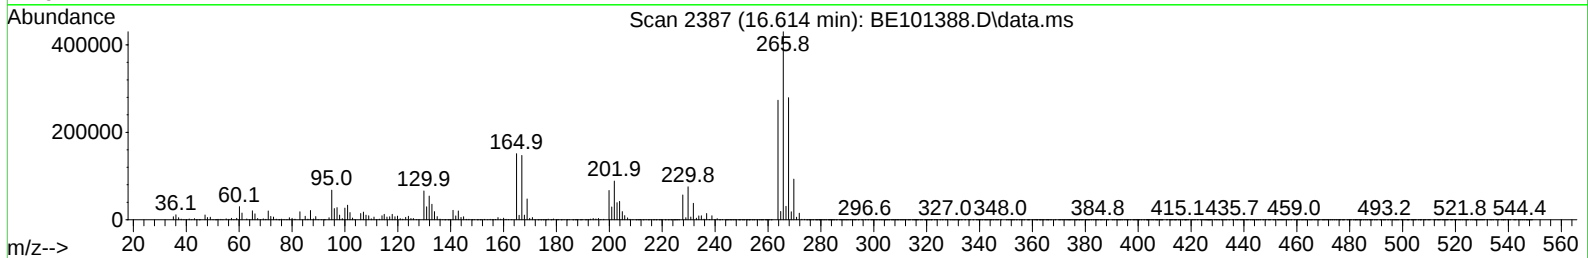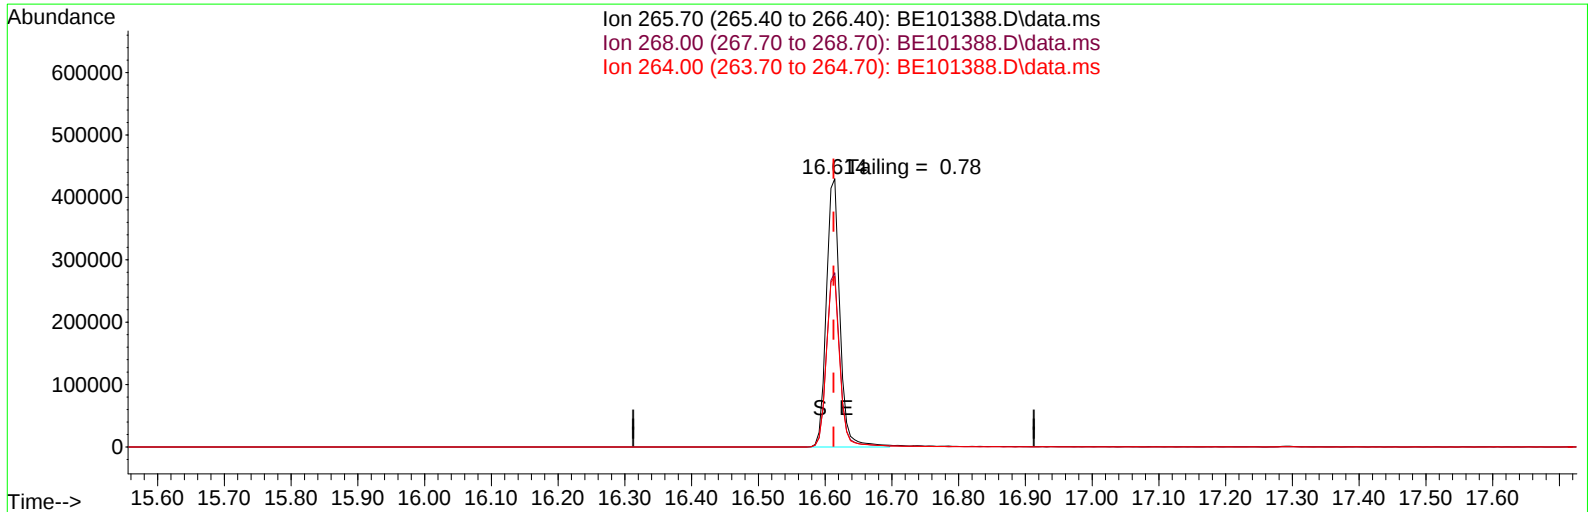

TIC: BE101388.D\data.ms

(70) Pentachlorophenol (C)

16.614min (+ 0.002) 1241130.64 ng




response 610726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.96
264.00	63.40	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
Data File : BE101388.D
Acq On : 28 Oct 2024 10:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Oct 29 01:32:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

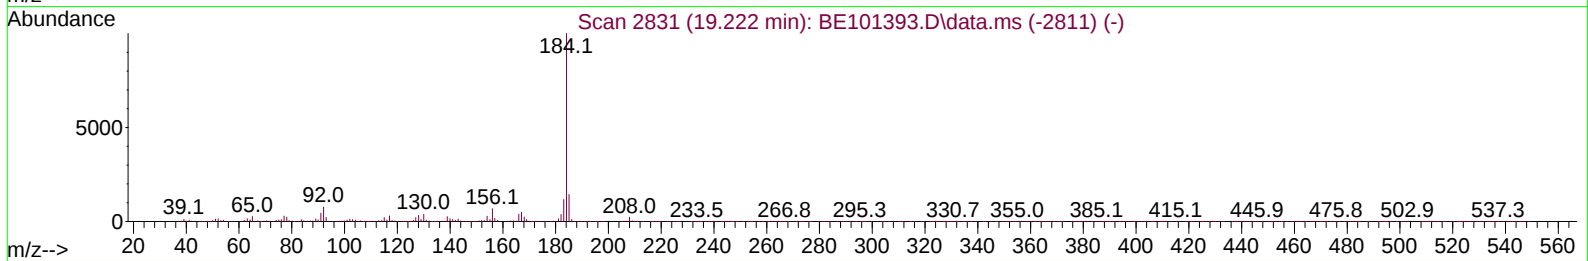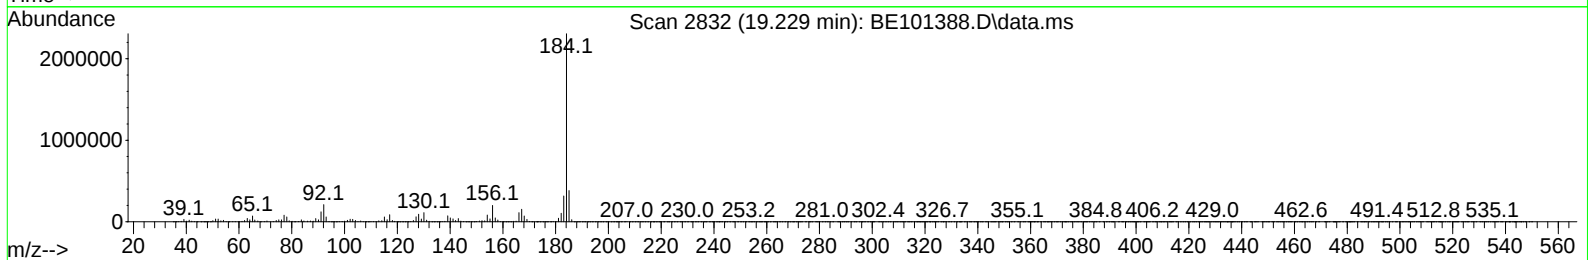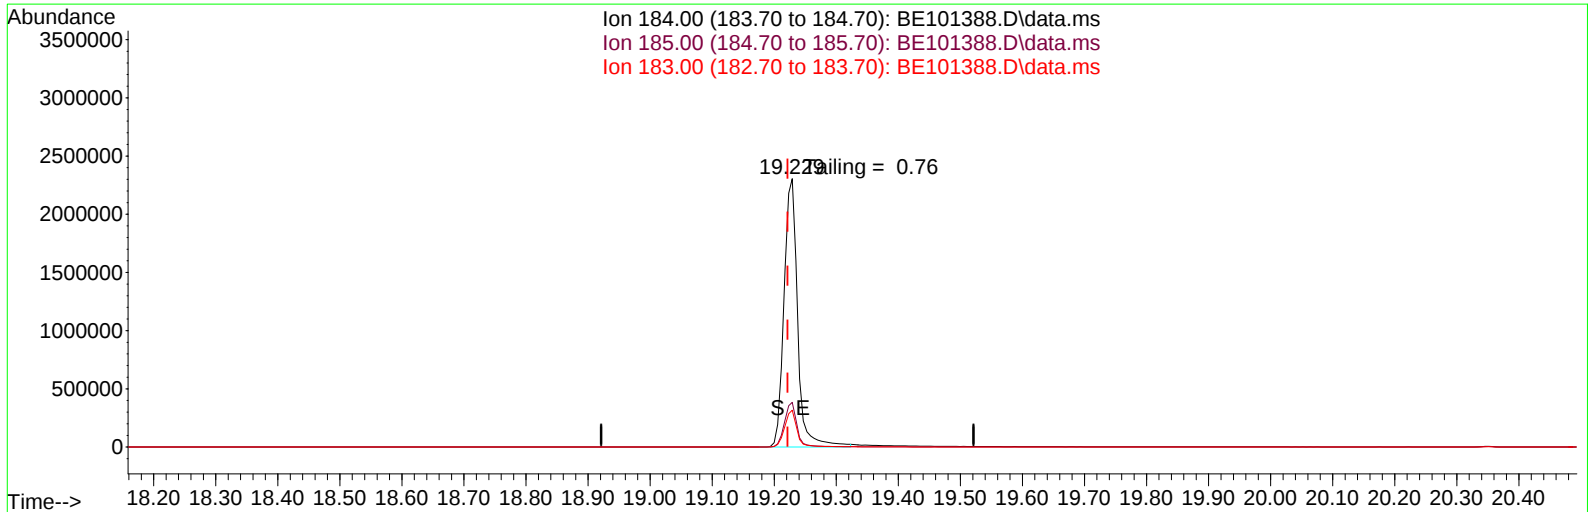

TIC: BE101388.D\data.ms

(77) Benzidine

19.229min (+ 0.008) 277076.80 ng

response 3629102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	16.64
183.00	11.60	13.72
0.00	0.00	0.00