
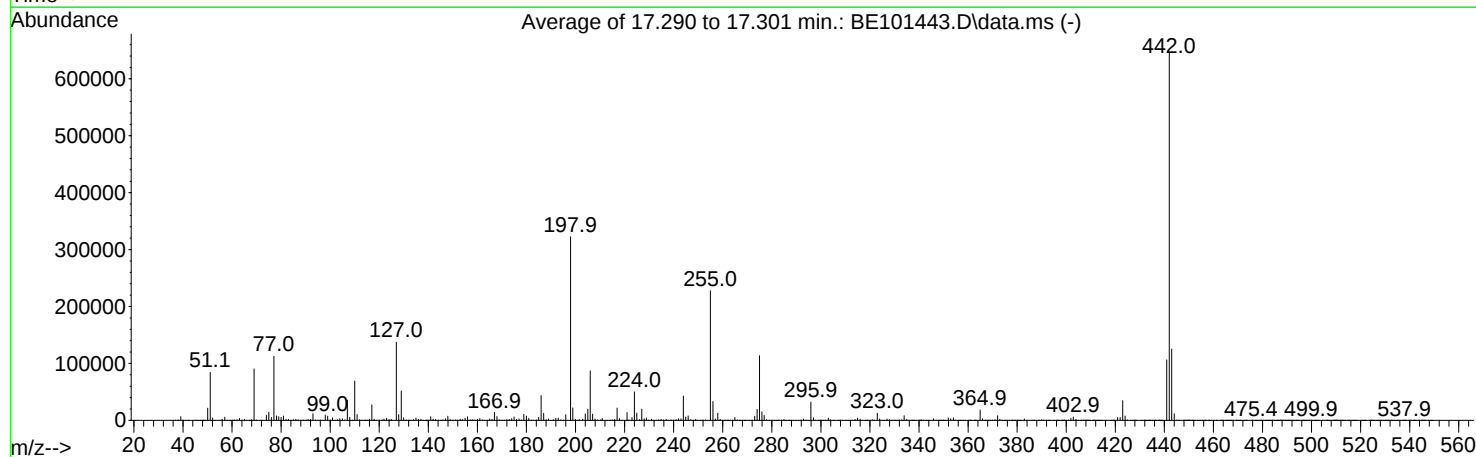


Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110124\  
Data File : BE101443.D  
Acq On : 1 Nov 2024 9:05  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE102824.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Oct 29 01:26:30 2024

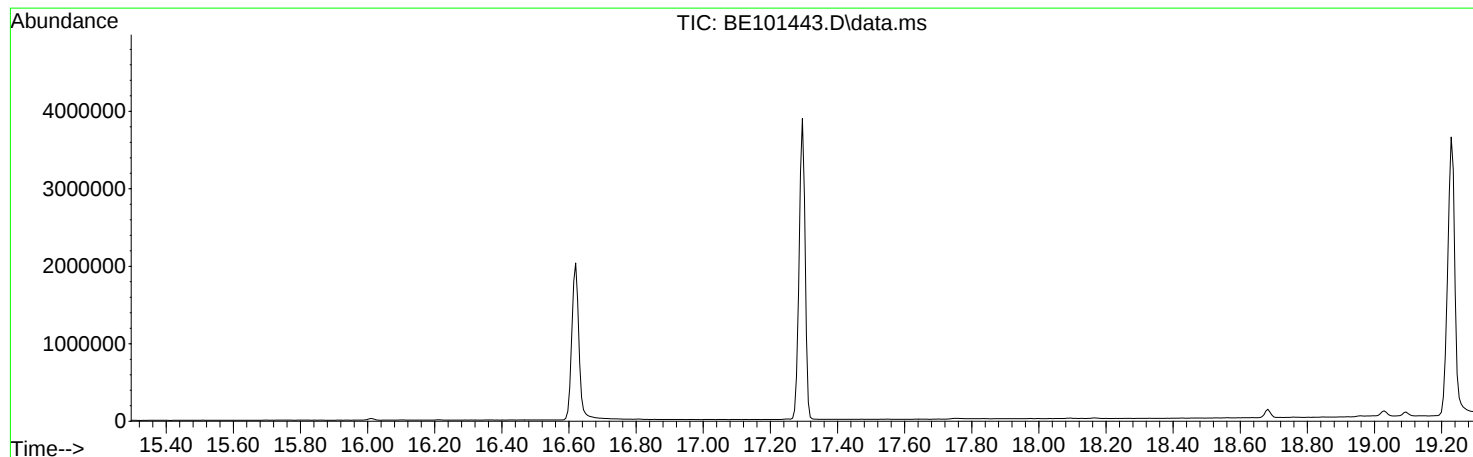




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2494

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 26.1         | 84334      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 1427       | PASS                |
| 69             | 198             | 0.00            | 100             | 28.1         | 90651      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 469        | PASS                |
| 127            | 198             | 10              | 80              | 42.5         | 137052     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 322581     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 22027      | PASS                |
| 275            | 198             | 10              | 60              | 35.2         | 113664     | PASS                |
| 365            | 198             | 1               | 100             | 5.7          | 18318      | PASS                |
| 441            | 198             | 0.01            | 100             | 32.9         | 106170     | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 646101     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 125248     | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN103024\  
Data File : BN034739.D  
Acq On : 30 Oct 2024 08:41  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Quant Time: Nov 04 06:42:49 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 04 06:42:45 2024  
Response via : Initial Calibration

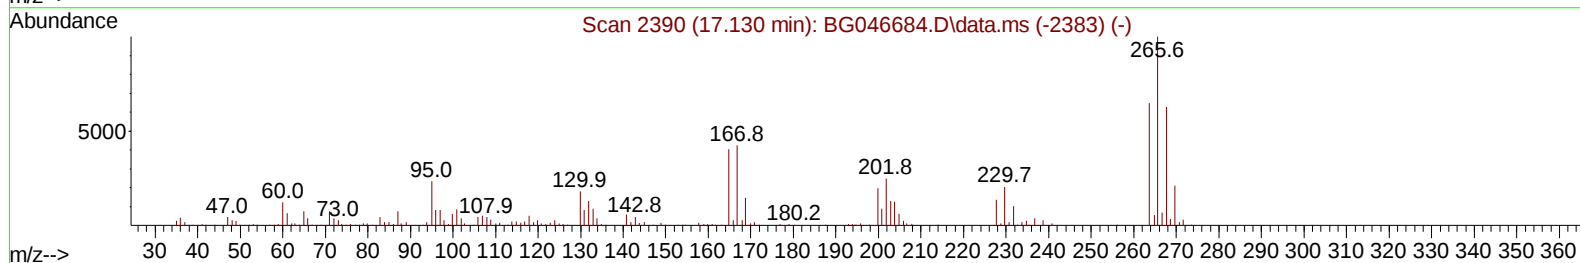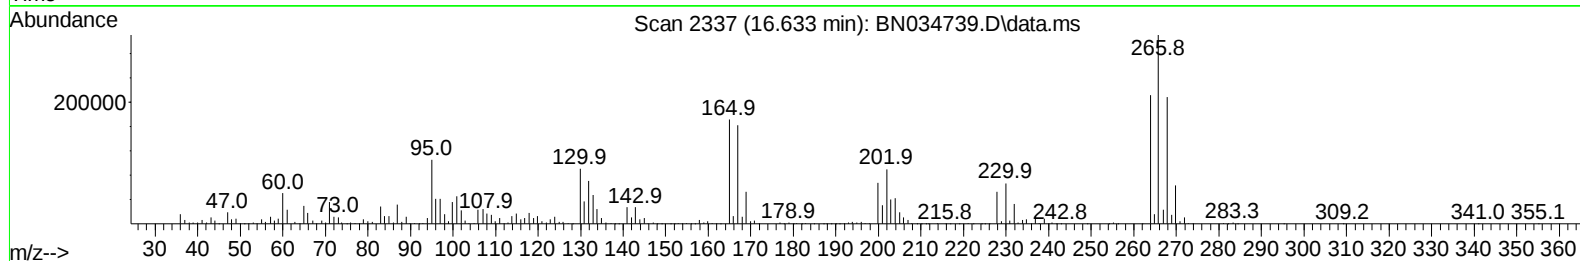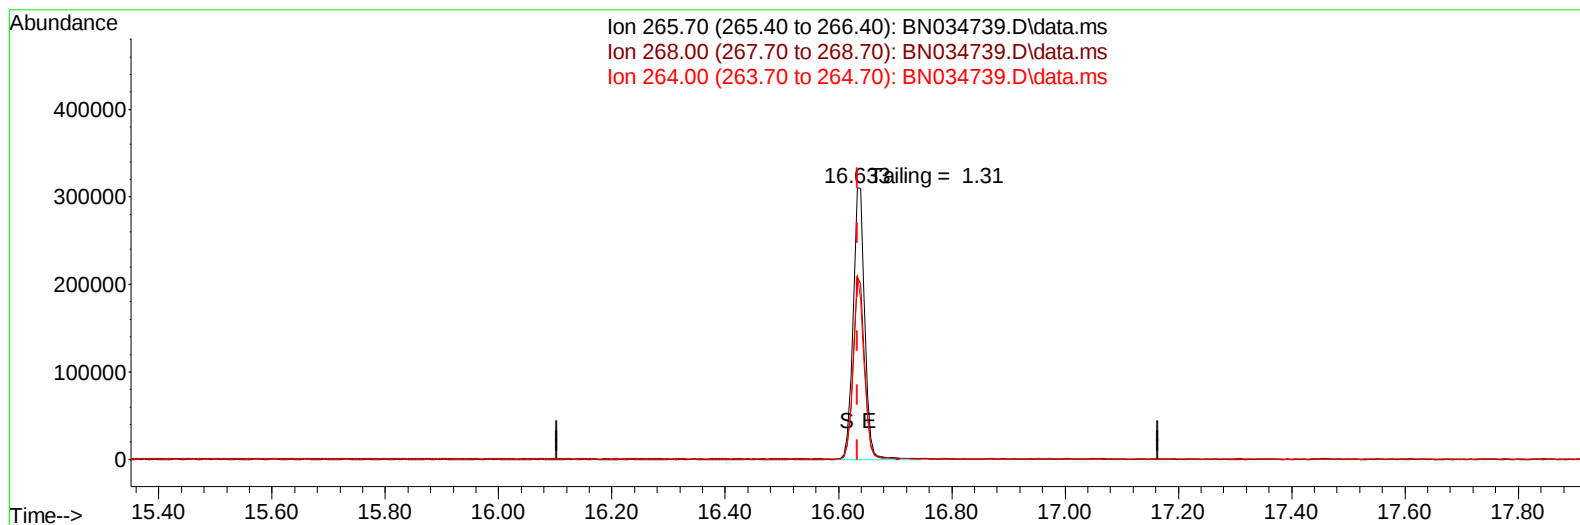

TIC: BN034739.D\data.ms

**(70) Pentachlorophenol (C)**

**16.633min ( 0.000) 23615.75 ng**




**response 445905**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 66.99  |
| 264.00 | 61.60  | 68.12  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN103024\  
Data File : BN034739.D  
Acq On : 30 Oct 2024 08:41  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Quant Time: Nov 04 06:42:49 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 04 06:42:45 2024  
Response via : Initial Calibration

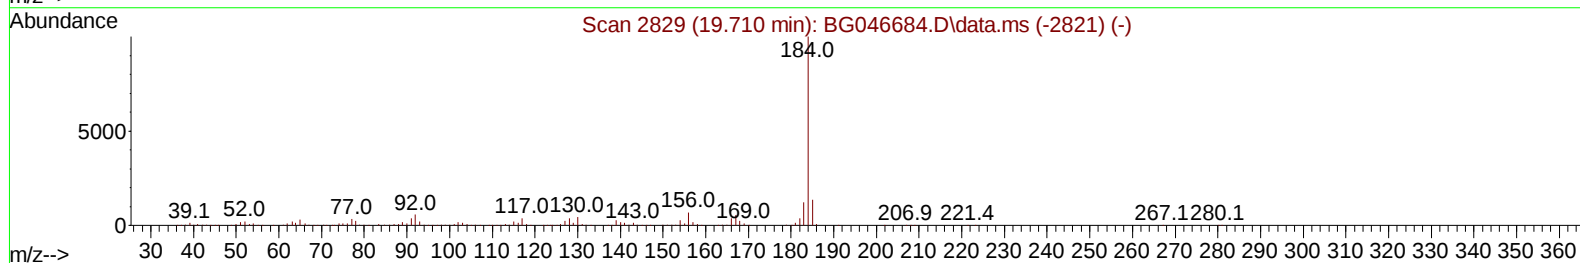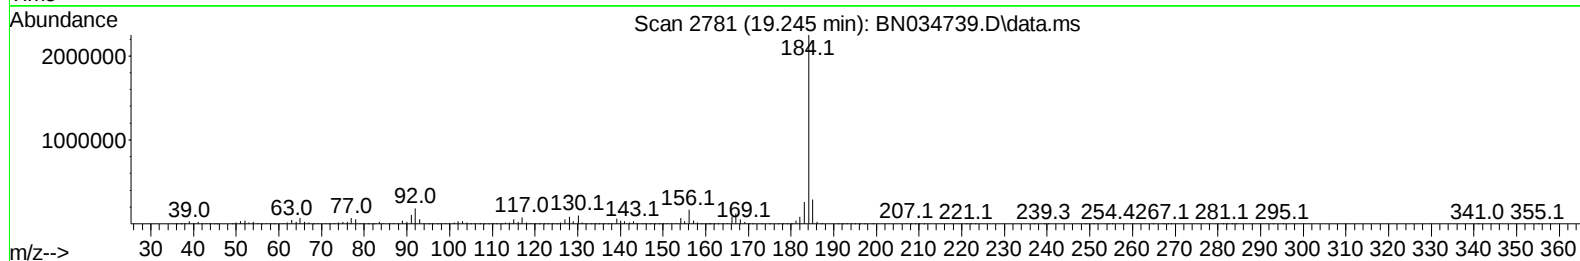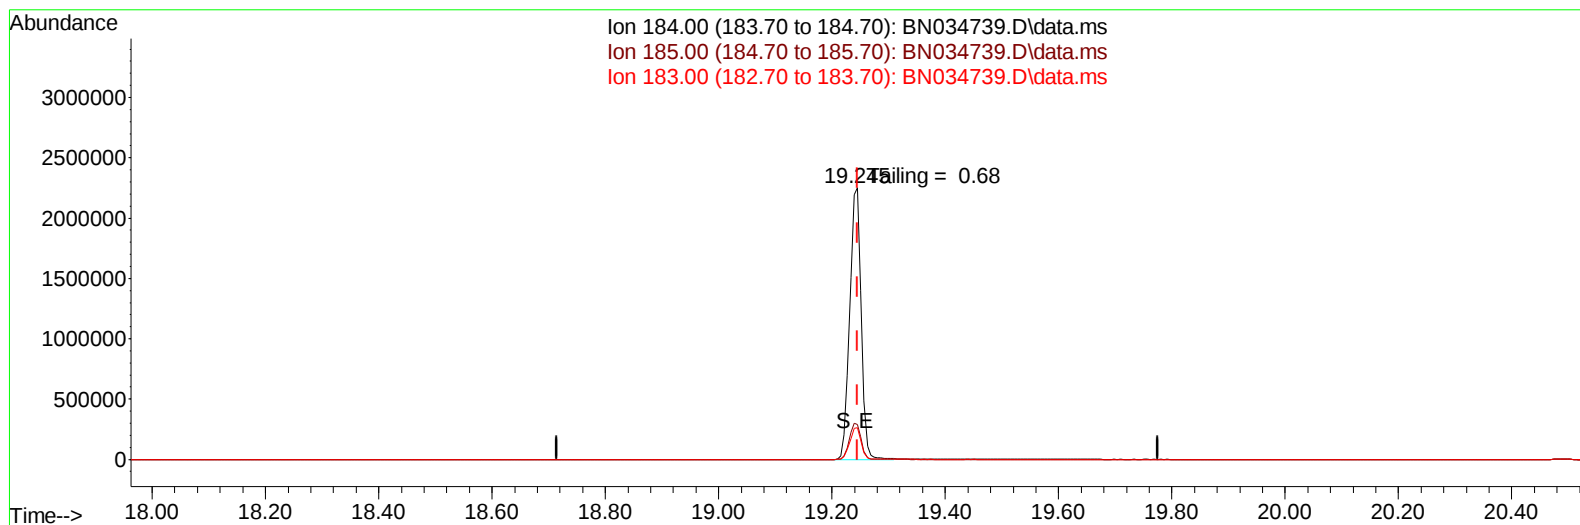

TIC: BN034739.D\data.ms

(77) Benzidine

19.245min ( 0.000) 766500.86 ng

response 3189736

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 12.97  |
| 183.00 | 13.20  | 11.61  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/30/2024    | BNA_N            | <u>BN034739.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1360651          | 20.492             |
| DDD           | 28684            | 20.098             |
| DDE           | 0                | 19.569             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 28684         | 1389335          | 2.06               |
|               |                  |                    |

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP