


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110124\
Data File : BF140199.D
Acq On : 01 Nov 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

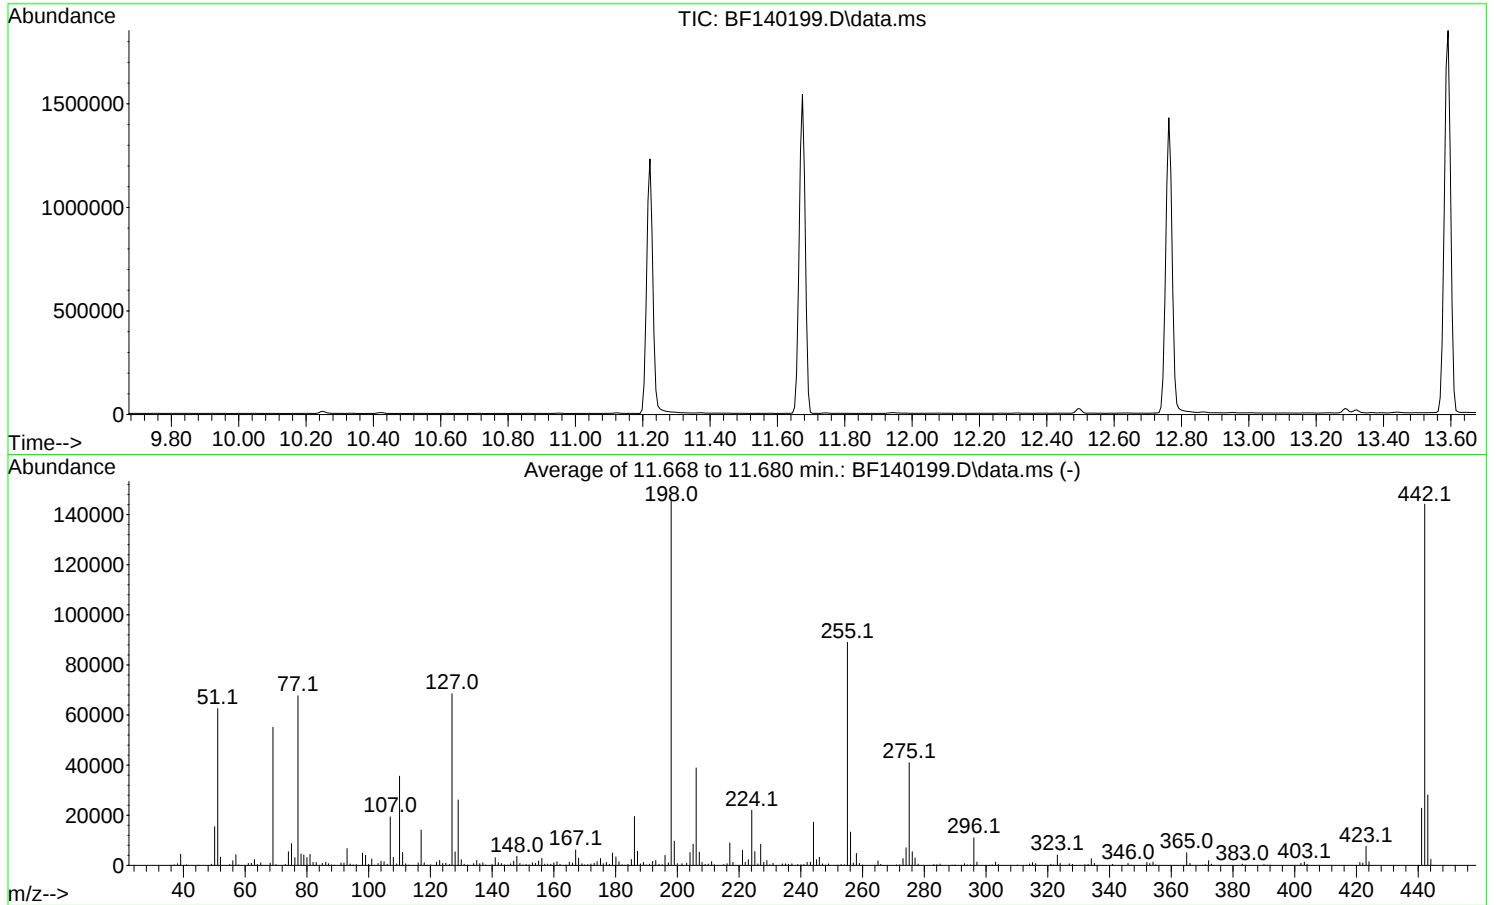




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	62603	PASS
68	69	0.00	2	1.7	956	PASS
69	198	0.00	100	37.8	55155	PASS
70	69	0.00	2	0.6	315	PASS
127	198	10	80	47.0	68533	PASS
197	198	0.00	2	0.7	1013	PASS
198	198	100	100	100.0	145960	PASS
199	198	5	9	6.6	9704	PASS
275	198	10	60	28.1	40979	PASS
365	198	1	100	3.5	5070	PASS
441	198	0.01	100	15.6	22800	PASS
442	442	50	100	100.0	144173	PASS
443	442	15	24	19.5	28141	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110124\
Data File : BF140199.D
Acq On : 01 Nov 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 01 11:17:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

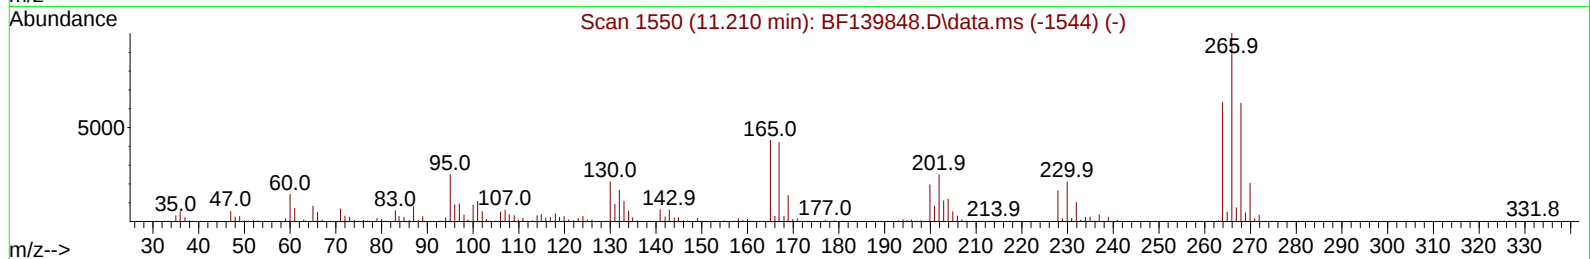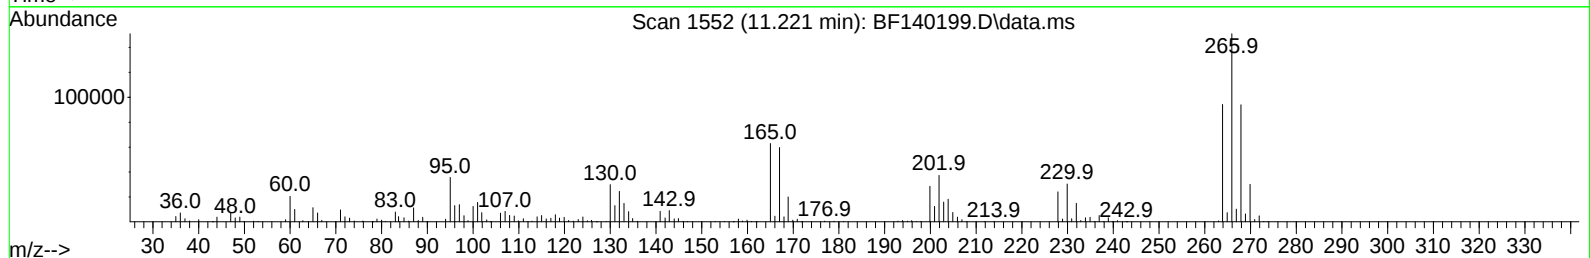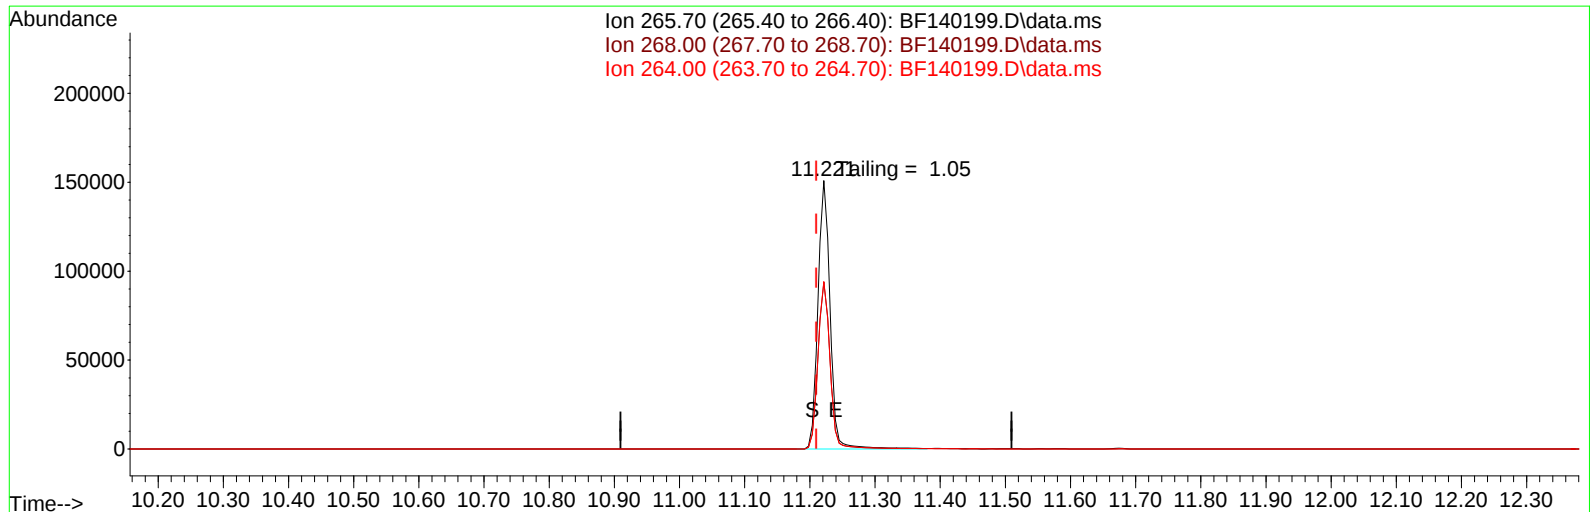

TIC: BF140199.D\data.ms

(70) Pentachlorophenol (C)

11.221min (+ 0.012) 111304.73 ng




response 195666

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.21
264.00	63.20	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110124\
Data File : BF140199.D
Acq On : 01 Nov 2024 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 01 11:17:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

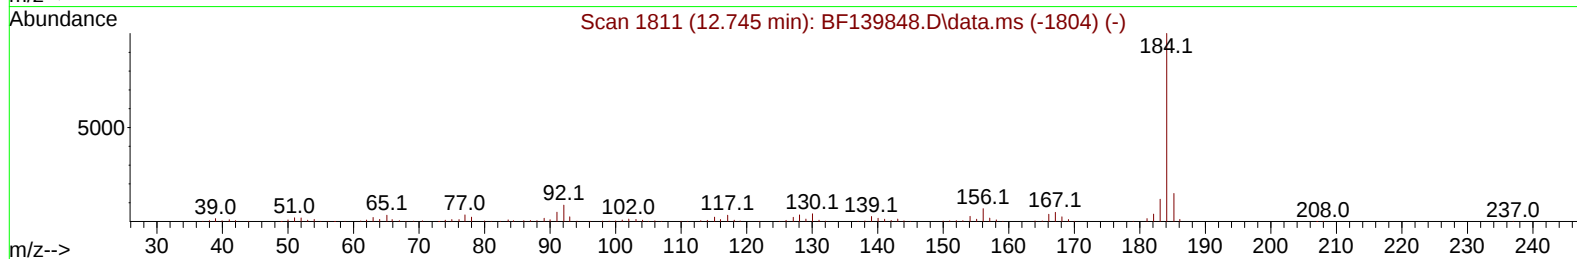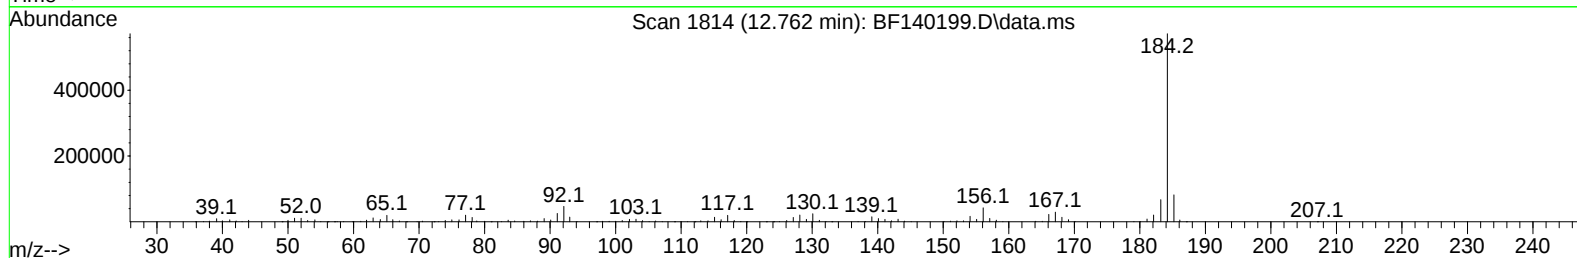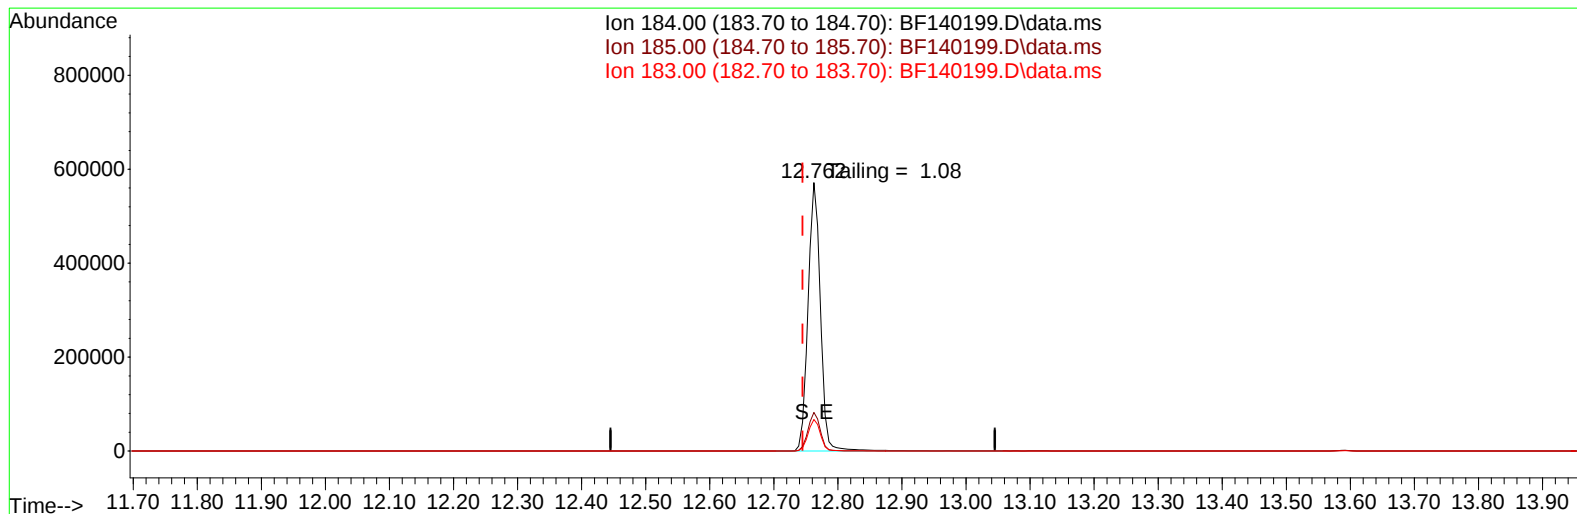

TIC: BF140199.D\data.ms

(77) Benzidine

12.762min (+ 0.017) 118399.71 ng

response 767076

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.36
183.00	11.80	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2024	BNA_F	<u>BF140199.D</u>
Compound Name	Response	Retention Time
DDT	471343	13.592
DDD	9865	13.286
DDE	718	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10583	481926	2.20

Instrument :
BNA_F
ClientSampleId :
DFTPP