
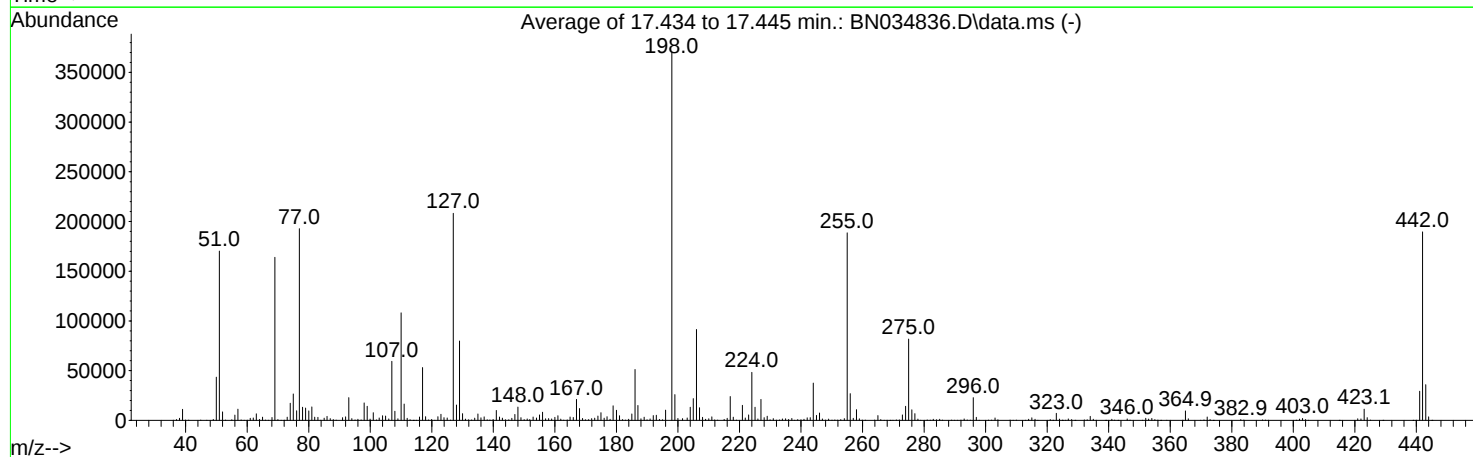


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110424\
Data File : BN034836.D
Acq On : 04 Nov 2024 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN103024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 05 00:03:28 2024

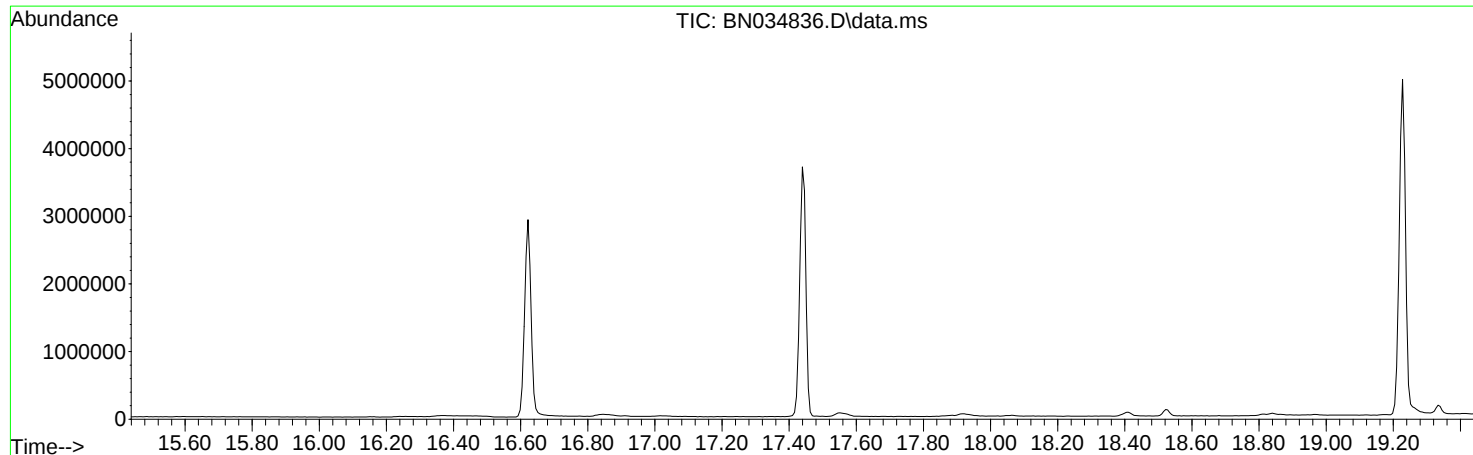




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	170208	PASS
68	69	0.00	2	1.8	2889	PASS
69	198	0.00	100	44.3	163998	PASS
70	69	0.00	2	0.5	771	PASS
127	198	10	80	56.3	208256	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	369963	PASS
199	198	5	9	7.0	25955	PASS
275	198	10	60	22.1	81781	PASS
365	198	1	100	2.6	9567	PASS
441	198	0.01	100	7.9	29307	PASS
442	442	50	100	100.0	189643	PASS
443	442	15	24	18.9	35912	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110424\
Data File : BN034836.D
Acq On : 04 Nov 2024 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 14:30:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 06:42:45 2024
Response via : Initial Calibration

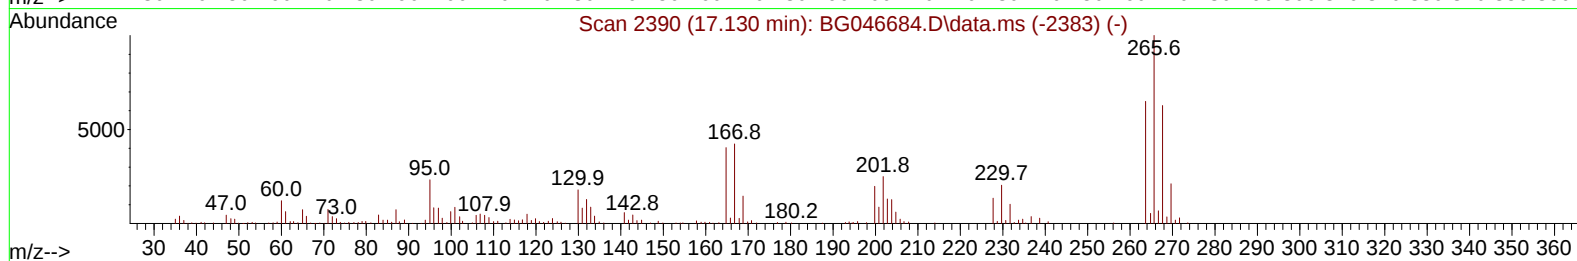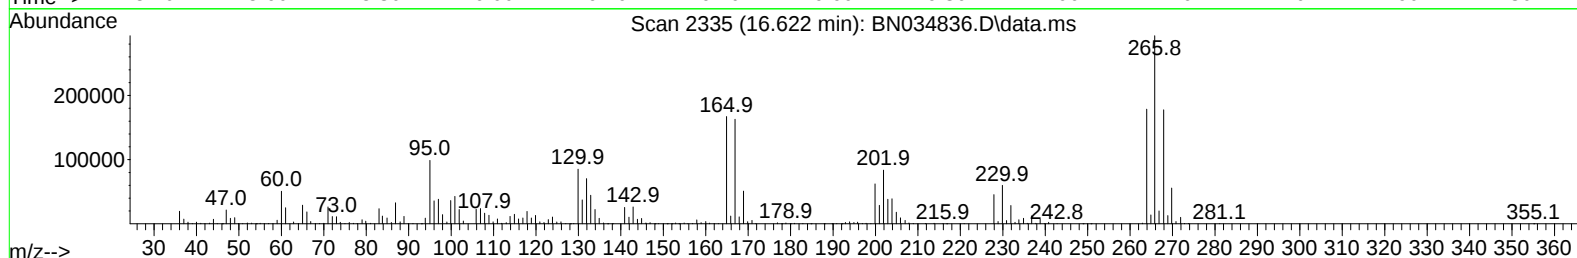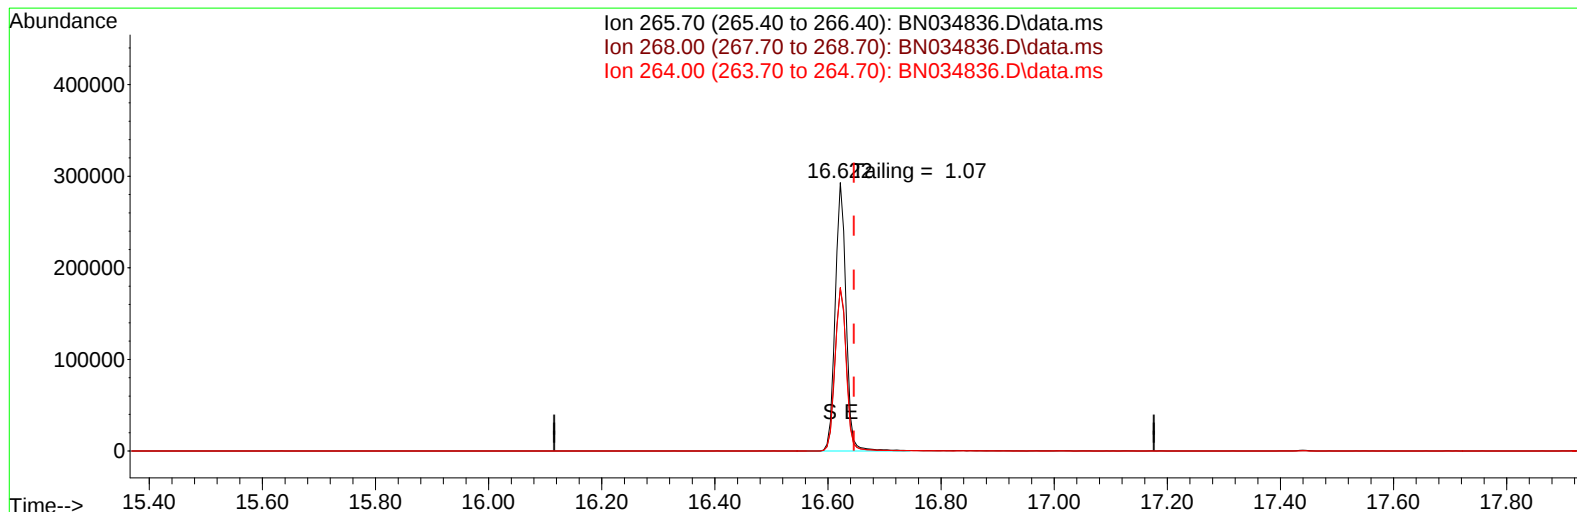

TIC: BN034836.D\data.ms

(70) Pentachlorophenol (C)

16.622min (-0.024) 22261.66 ng




response 390638

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.64
264.00	61.60	60.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110424\
Data File : BN034836.D
Acq On : 04 Nov 2024 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 14:30:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 06:42:45 2024
Response via : Initial Calibration

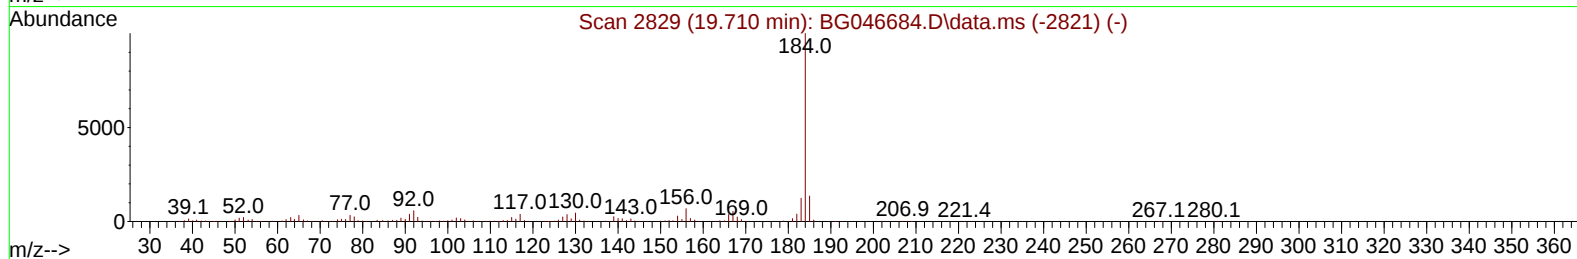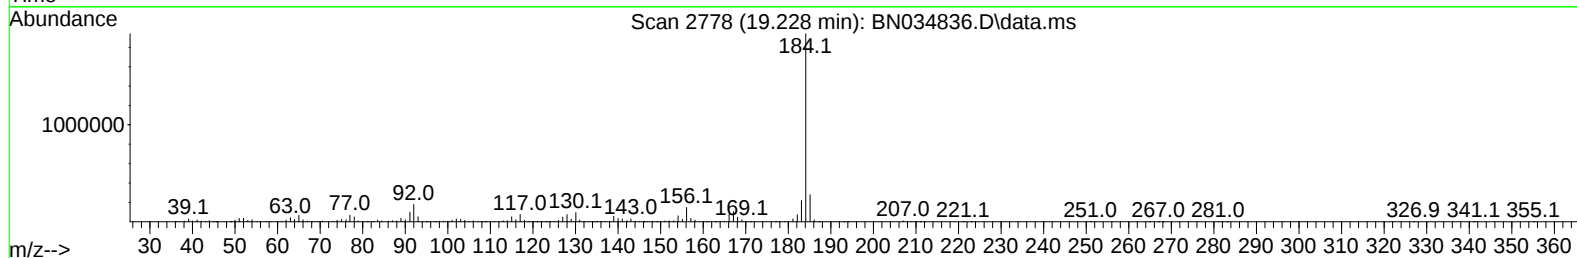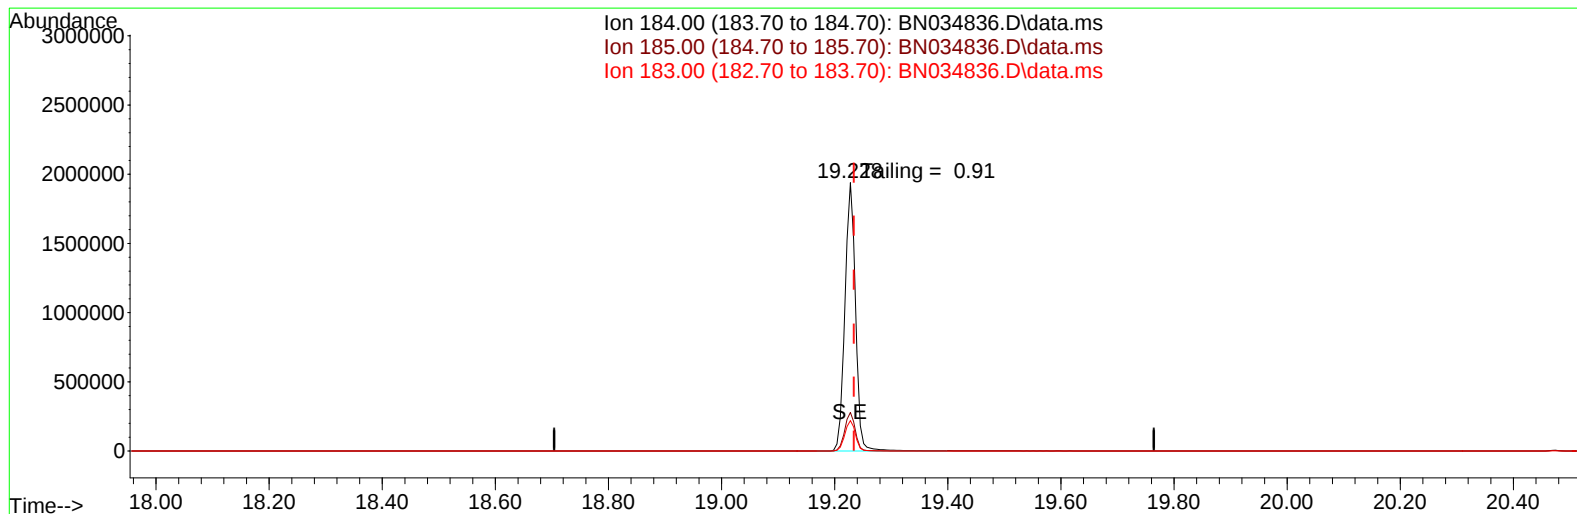

TIC: BN034836.D\data.ms

(77) Benzdine

19.228min (-0.006) 0.00 ng

response 2538235

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.38
183.00	13.20	11.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2024	BNA_N	<u>BN034836.D</u>
Compound Name	Response	Retention Time
DDT	1131699	20.475
DDD	36181	20.028
DDE	1756	19.522
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37937	1169636	3.24

Instrument :
BNA_N
ClientSampleId :
DFTPP