
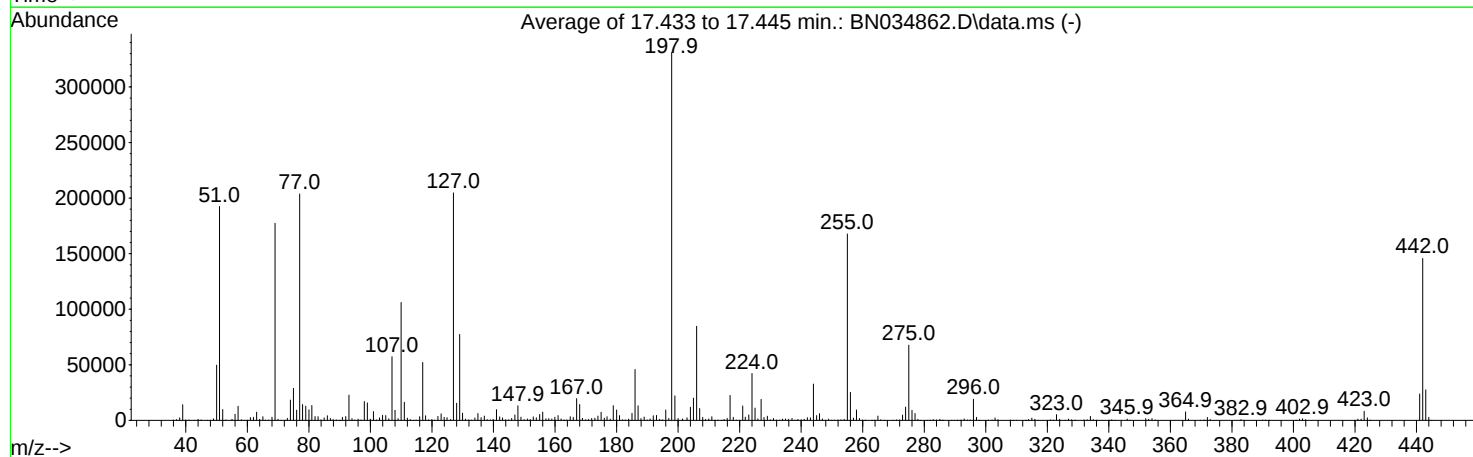


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110524\
Data File : BN034862.D
Acq On : 05 Nov 2024 08:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN103024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 05 00:03:28 2024

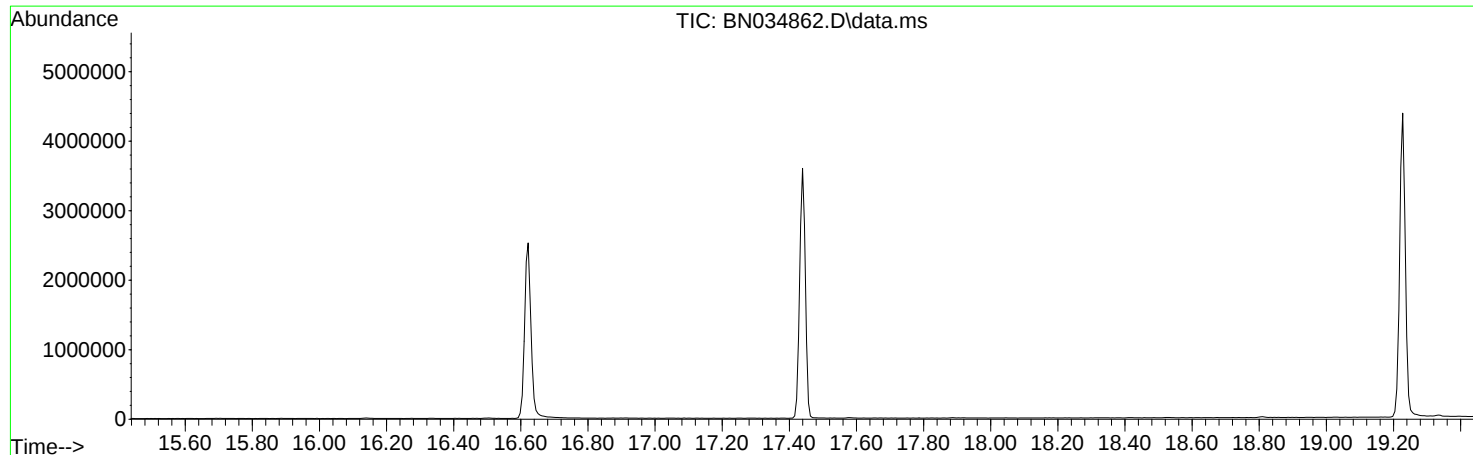

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.2	192477	PASS
68	69	0.00	2	1.6	2874	PASS
69	198	0.00	100	53.6	177323	PASS
70	69	0.00	2	0.5	975	PASS
127	198	10	80	61.8	204715	PASS
197	198	0.00	2	0.5	1729	PASS
198	198	100	100	100.0	330987	PASS
199	198	5	9	6.6	22003	PASS
275	198	10	60	20.4	67669	PASS
365	198	1	100	2.3	7667	PASS
441	198	0.01	100	7.2	23705	PASS
442	442	50	100	100.0	145749	PASS
443	442	15	24	18.9	27560	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/5/2024	BNA_N	<u>BN034862.D</u>
Compound Name	Response	Retention Time
DDT	1019765	20.474
DDD	23573	20.027
DDE	1293	19.527
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24866	1044631	2.38

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110524\
Data File : BN034862.D
Acq On : 05 Nov 2024 08:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 05 14:17:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:55:25 2022
Response via : Initial Calibration

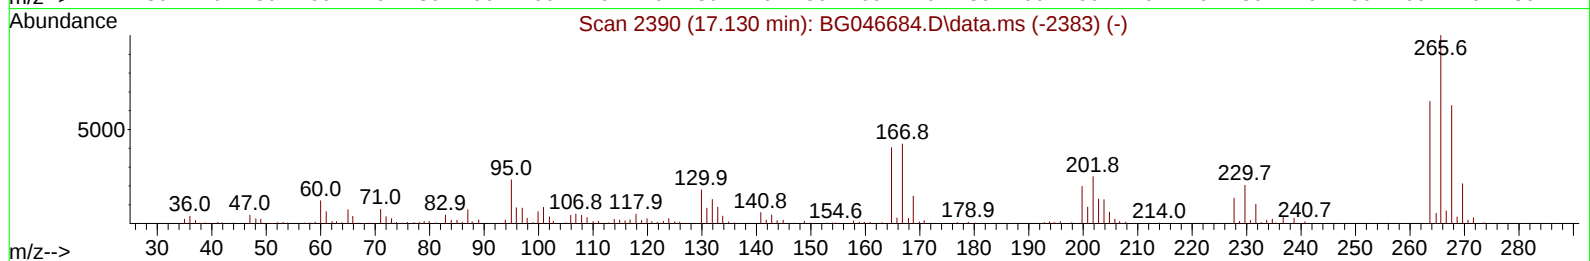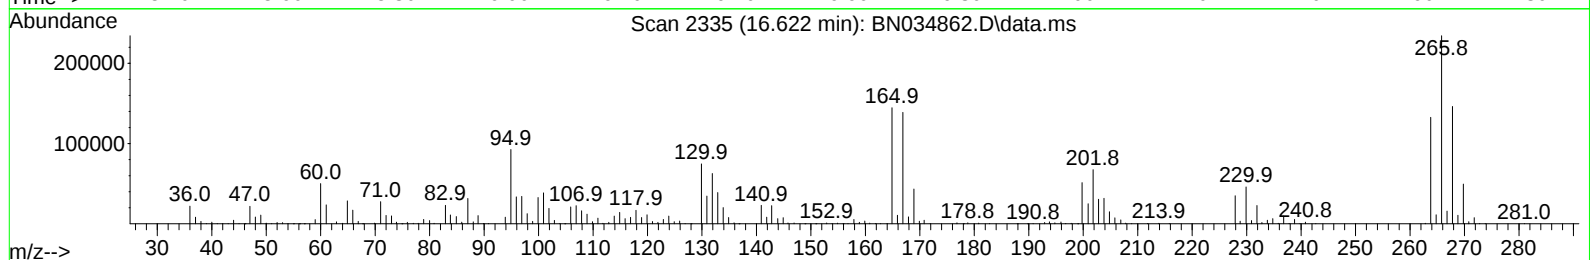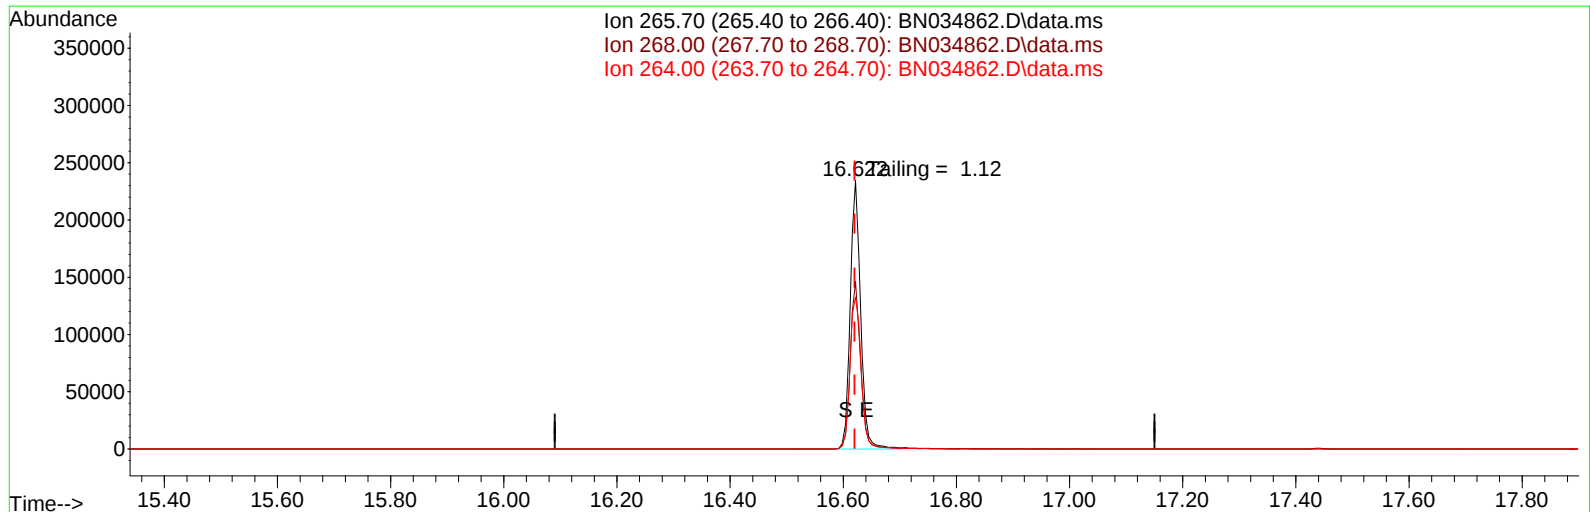

TIC: BN034862.D\data.ms

(70) Pentachlorophenol (C)

16.622min (+ 0.002) 130230.19 ng




response 297406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.42
264.00	61.60	56.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110524\
Data File : BN034862.D
Acq On : 05 Nov 2024 08:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 05 14:17:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:55:25 2022
Response via : Initial Calibration

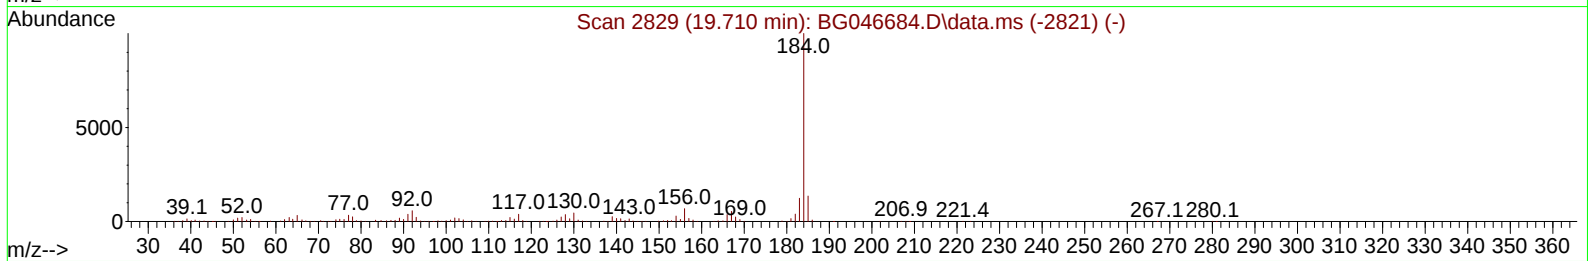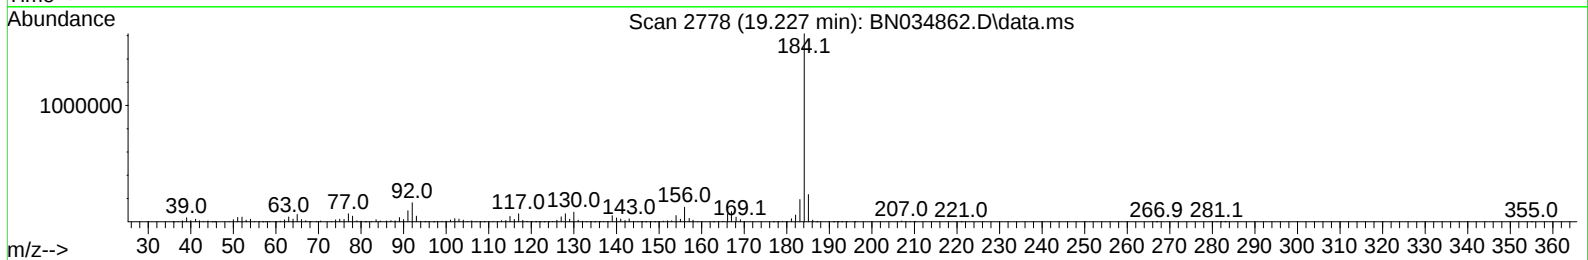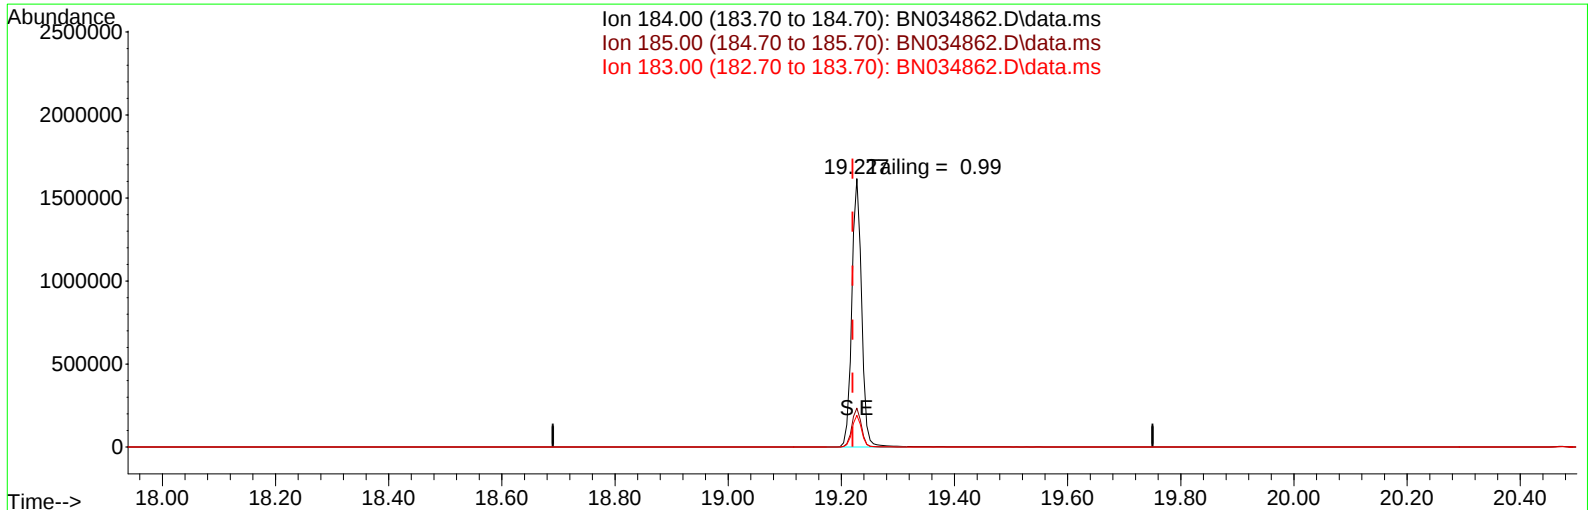

TIC: BN034862.D\data.ms

(77) Benzidine

19.227min (+ 0.008) 239356.43 ng m

response 1940480

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.50
183.00	13.20	11.83
0.00	0.00	0.00