

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110524\
 Data File : BN034866.D
 Acq On : 05 Nov 2024 11:49
 Operator : RC/JU
 Sample : P4665-02RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 VPB190-HYD-20241030RE

Quant Time: Nov 05 12:24:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN103024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 05 00:03:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.589	152	7601	0.400	ng	0.00
7) Naphthalene-d8	10.351	136	22735	0.400	ng	# 0.00
13) Acenaphthene-d10	14.222	164	10621	0.400	ng	0.00
19) Phenanthrene-d10	16.970	188	21100	0.400	ng	# 0.00
29) Chrysene-d12	21.160	240	12441	0.400	ng	# 0.00
35) Perylene-d12	23.335	264	8745	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.199	112	9	0.000	ng	-0.01
5) Phenol-d6	6.744	99	38	0.001	ng	-0.02
8) Nitrobenzene-d5	8.728	82	7085	0.397	ng	0.00
11) 2-Methylnaphthalene-d10	11.943	152	12	0.000	ng	0.00
14) 2,4,6-Tribromophenol	15.716	330	760	0.145	ng	0.00
15) 2-Fluorobiphenyl	12.843	172	17176	0.411	ng	0.00
27) Fluoranthene-d10	19.001	212	1148	0.023	ng	0.00
31) Terphenyl-d14	19.610	244	11240	0.421	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.107	149	1982	0.048	ng	# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110524\
Data File : BN034866.D
Acq On : 05 Nov 2024 11:49
Operator : RC/JU
Sample : P4665-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
VPB190-HYD-20241030RE


Quant Time: Nov 05 12:24:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN103024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 05 00:03:28 2024
Response via : Initial Calibration

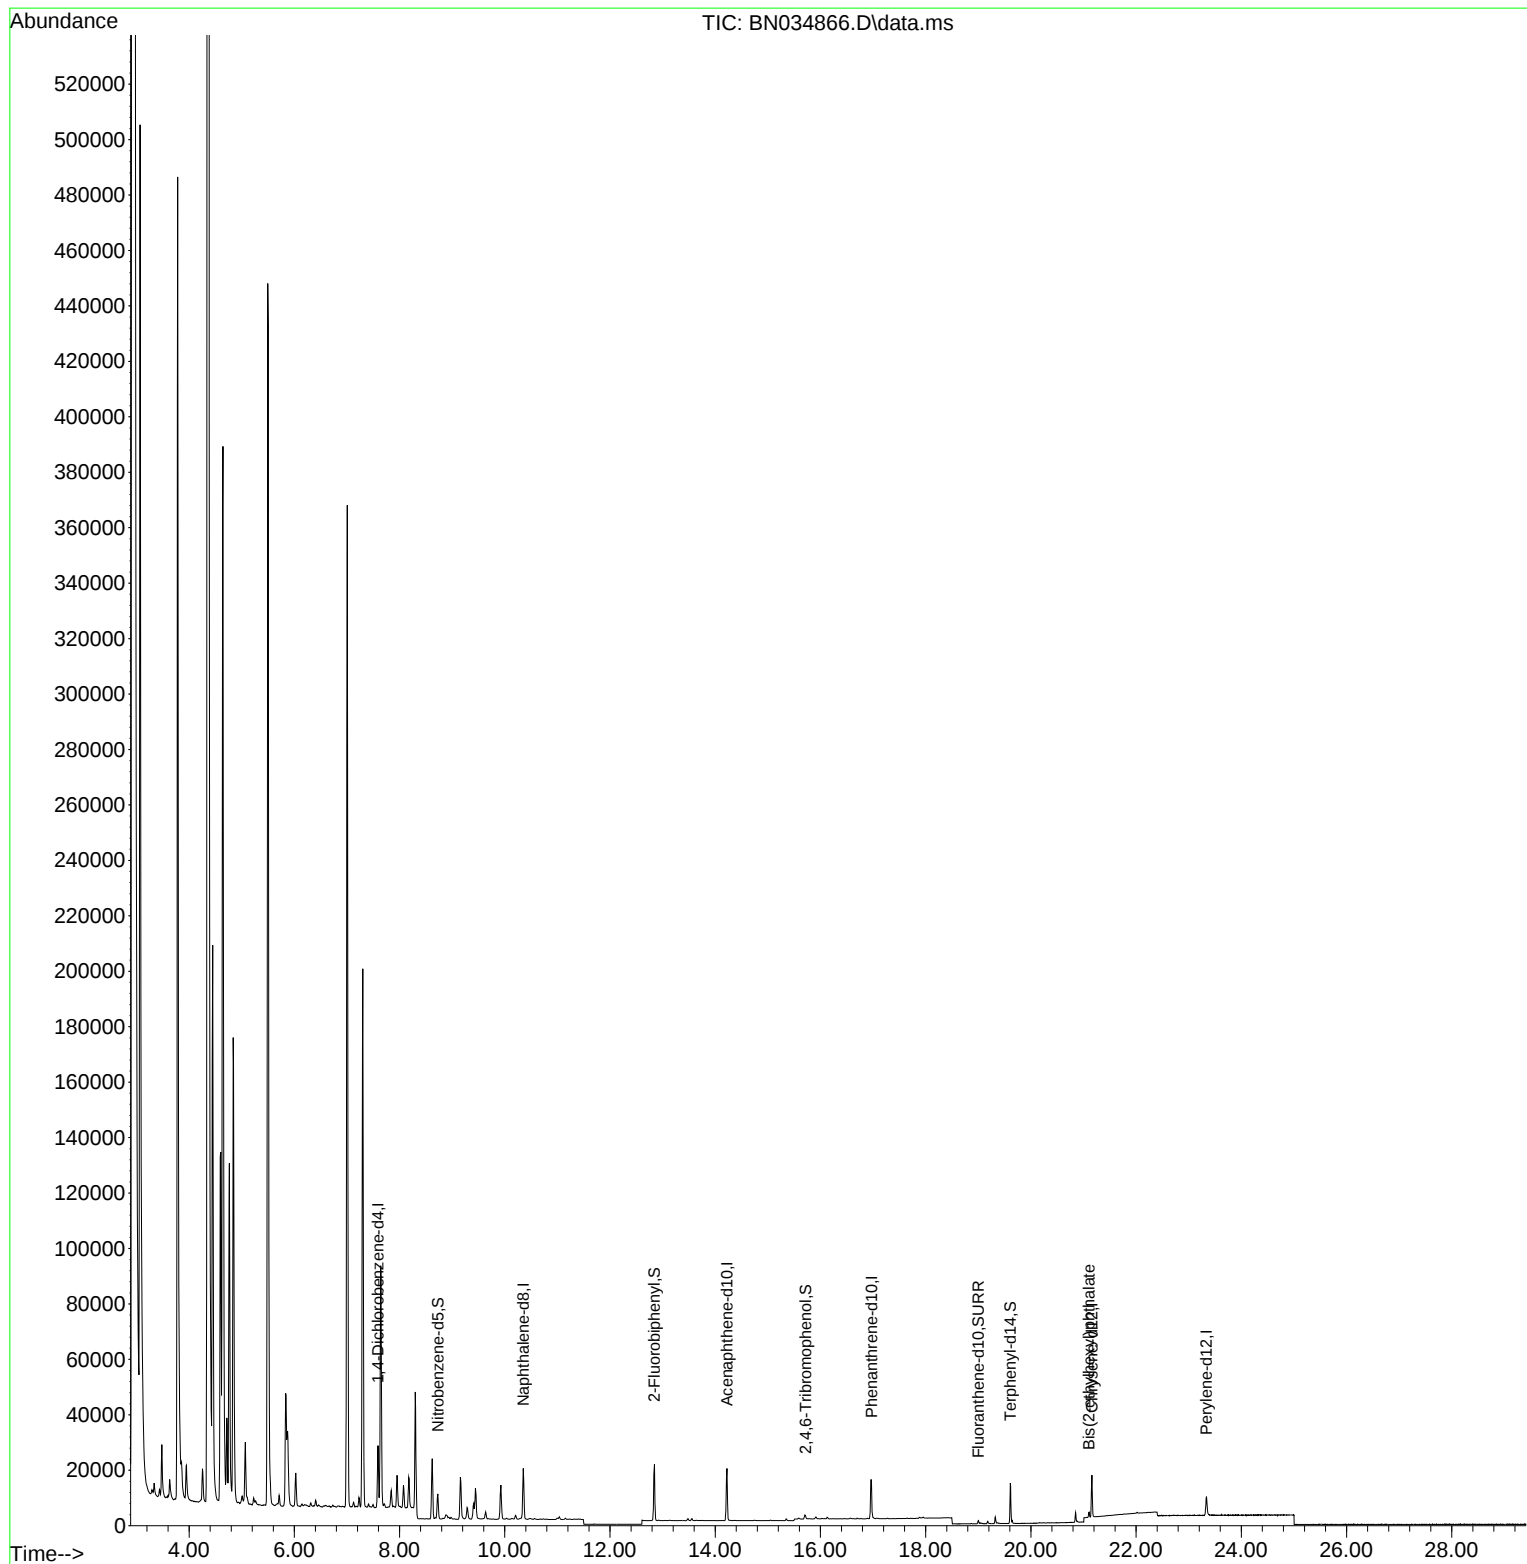






#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.589 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49

Instrument :
BNA_N
ClientSampleId :
VPB190-HYD-20241030RE



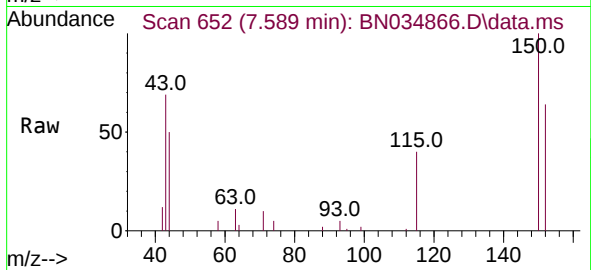



Tgt Ion:152 Resp: 7601
Ion Ratio Lower Upper
152 100
150 155.6 124.9 187.3
115 62.2 50.2 75.2

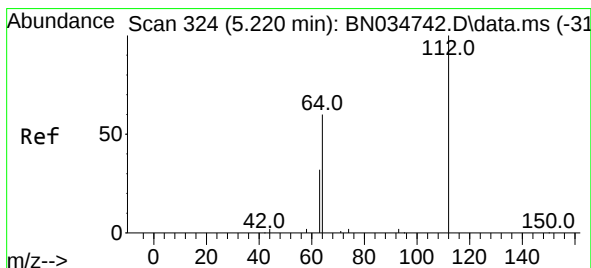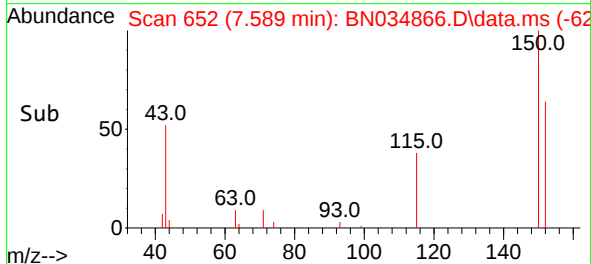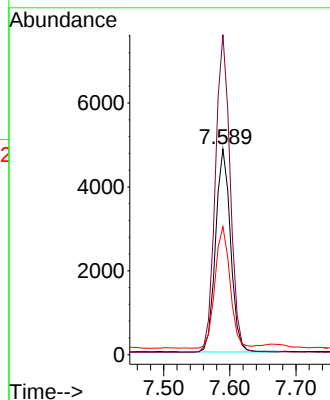

#4
2-Fluorophenol
Concen: 0.000 ng
RT: 5.199 min Scan# 321
Delta R.T. -0.014 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49

Tgt Ion:112 Resp: 9
Ion Ratio Lower Upper
112 100
64 0.0 44.9 67.3#
63 0.0 23.5 35.3#


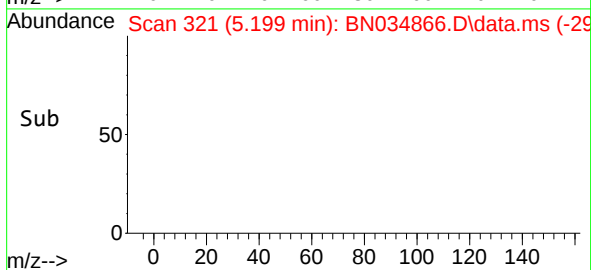
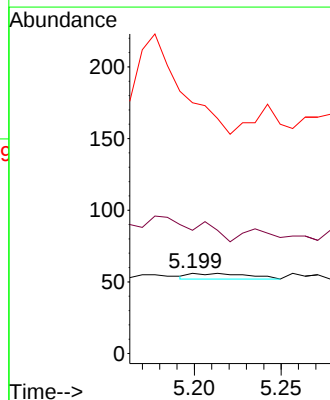
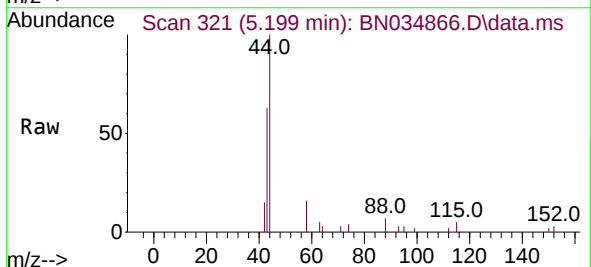


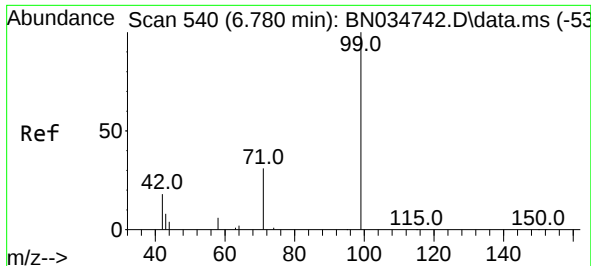

#5
Phenol-d6
Concen: 0.001 ng
RT: 6.744 min Scan# 51
Delta R.T. -0.022 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49




Instrument :
BNA_N
ClientSampleId :
VPB190-HYD-20241030RE


Tgt Ion: 99 Resp: 38
Ion Ratio Lower Upper
99 100
42 326.3 15.9 23.9#
71 0.0 24.3 36.5#

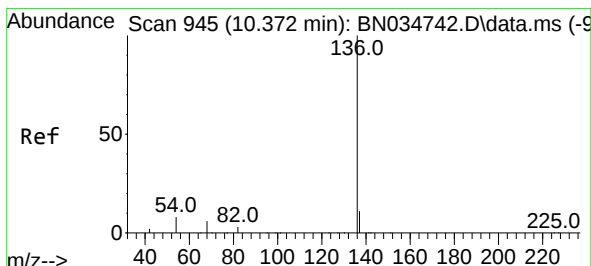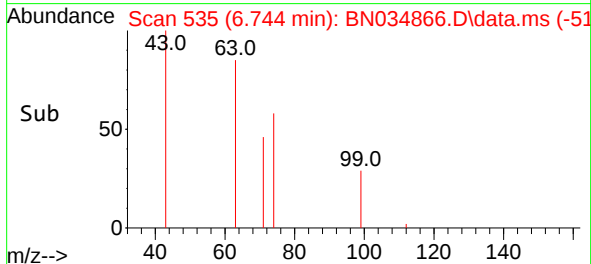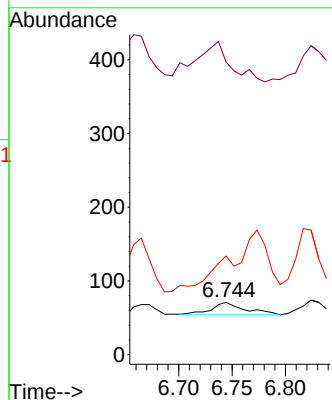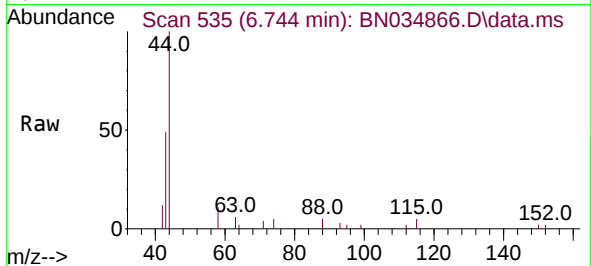

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.351 min Scan# 943
Delta R.T. 0.000 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49

Tgt Ion:136 Resp: 22735
Ion Ratio Lower Upper
136 100
137 11.3 9.2 13.8
54 10.6 7.0 10.4#
68 7.6 5.6 8.4

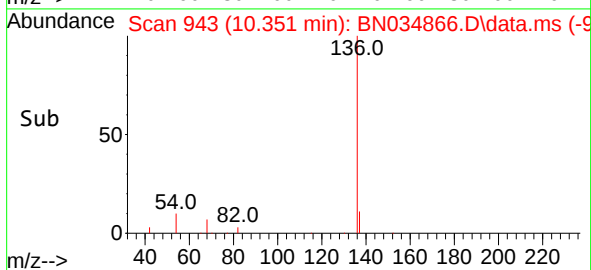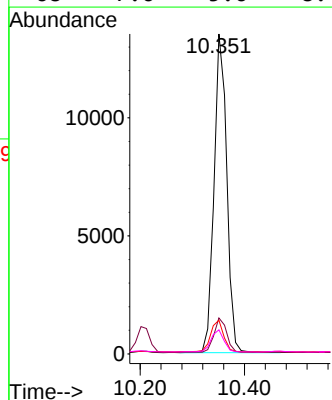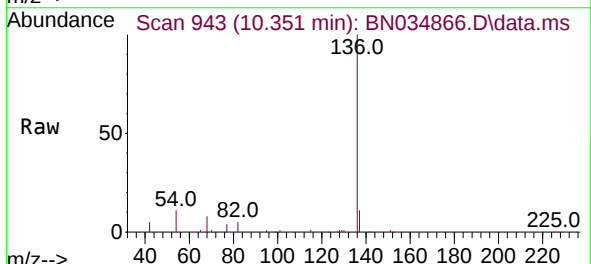

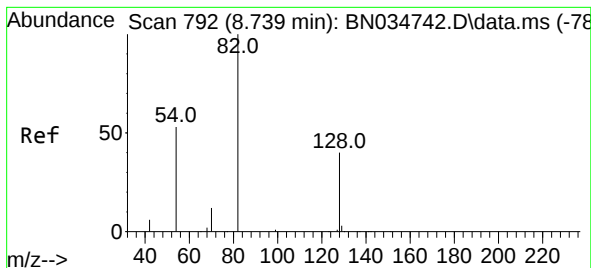

#8

Nitrobenzene-d5

Concen: 0.397 ng

RT: 8.728 min Scan# 791

Delta R.T. 0.000 min

Lab File: BN034866.D


Acq: 05 Nov 2024 11:49

Instrument :

BNA_N

ClientSampleId :

VPB190-HYD-20241030RE

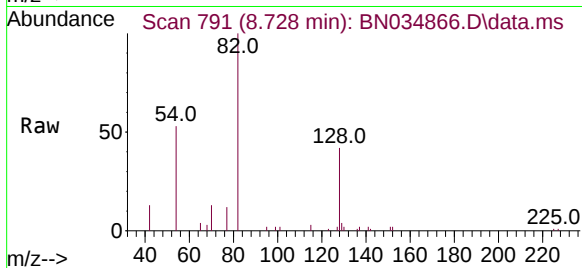




Tgt Ion: 82 Resp: 7085

Ion Ratio Lower Upper

82 100

128 41.8 33.7 50.5

54 53.3 44.4 66.6

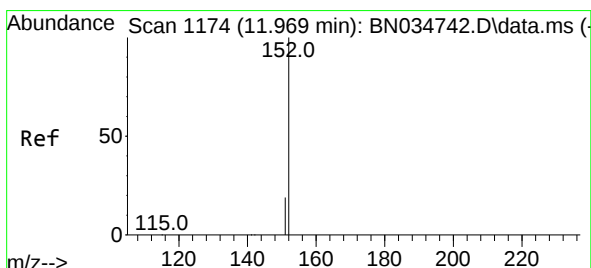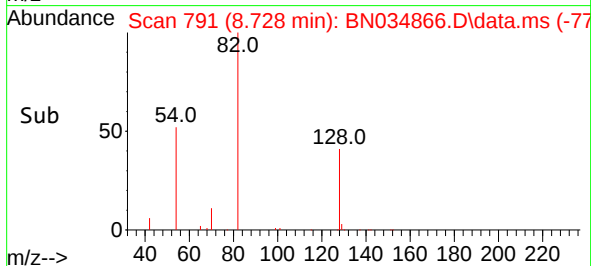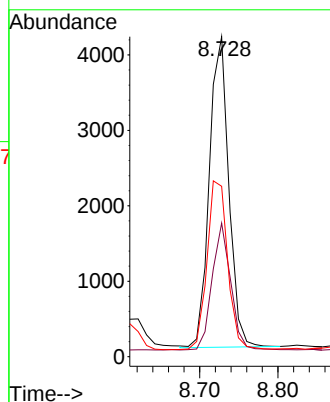

#11

2-Methylnaphthalene-d10

Concen: 0.000 ng

RT: 11.943 min Scan# 1167

Delta R.T. -0.008 min

Lab File: BN034866.D




Acq: 05 Nov 2024 11:49


Tgt Ion:152 Resp: 12

Ion Ratio Lower Upper

152 100

151 16.7 16.6 24.8

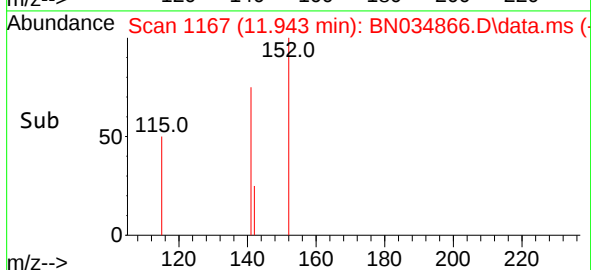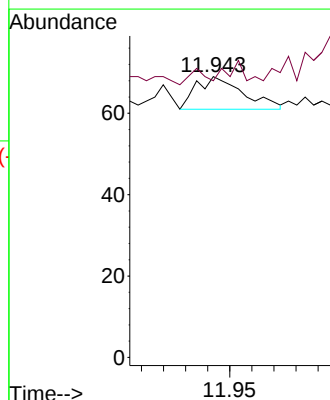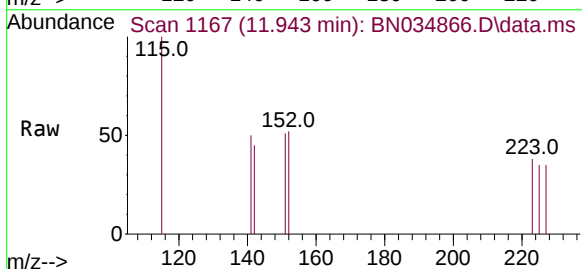

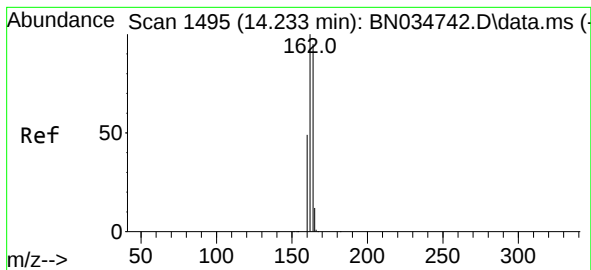

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.222 min Scan# 1494

Delta R.T. 0.000 min

Lab File: BN034866.D

Acq: 05 Nov 2024 11:49

Instrument :

BNA_N

ClientSampleId :

VPB190-HYD-20241030RE





Tgt Ion:164 Resp: 10621

Ion Ratio Lower Upper

164 100

162 103.2 84.3 126.5

160 54.0 41.7 62.5

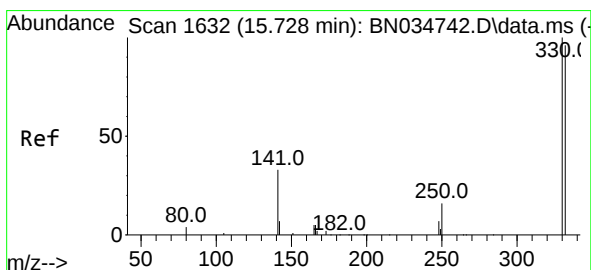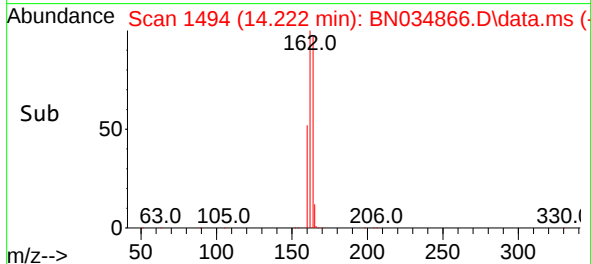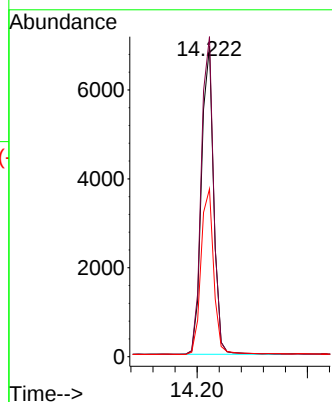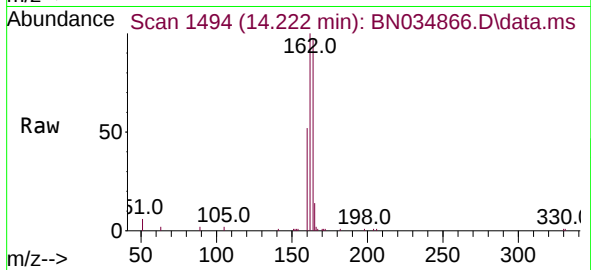

#14

2,4,6-Tribromophenol

Concen: 0.145 ng

RT: 15.716 min Scan# 1631

Delta R.T. 0.000 min

Lab File: BN034866.D

Acq: 05 Nov 2024 11:49




Tgt Ion:330 Resp: 760


Ion Ratio Lower Upper

330 100

332 141.1 77.8 116.6#

141 53.9 41.0 61.4


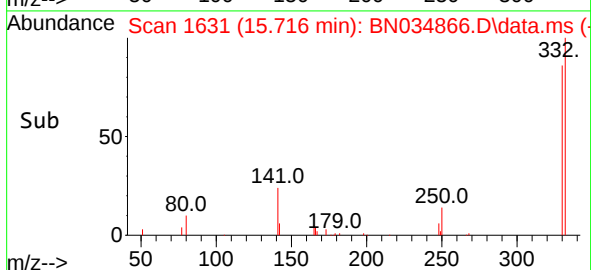
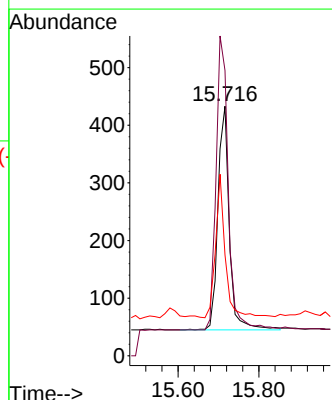
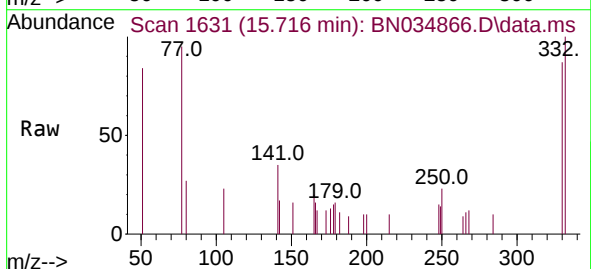


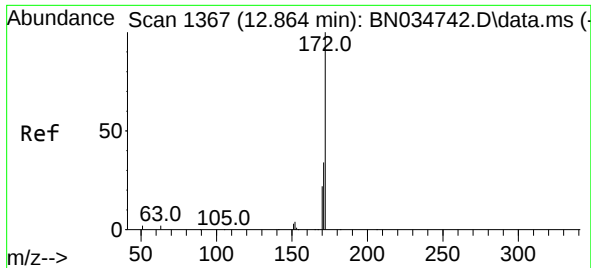

#15
2-Fluorobiphenyl
Concen: 0.411 ng
RT: 12.843 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49




Instrument :
BNA_N
ClientSampleId :
VPB190-HYD-20241030RE


Tgt Ion:	172	Resp:	17176
Ion	Ratio	Lower	Upper
172	100		
171	33.7	27.2	40.8
170	23.3	18.0	27.0

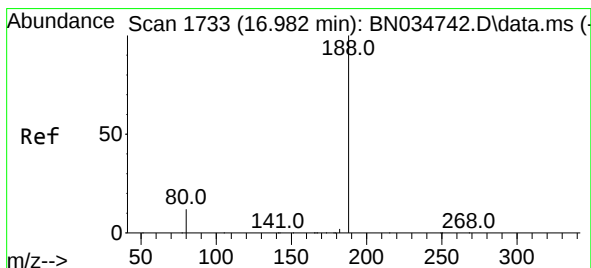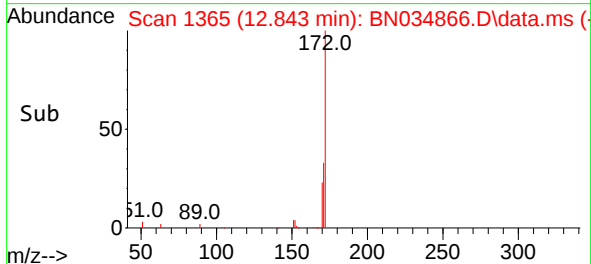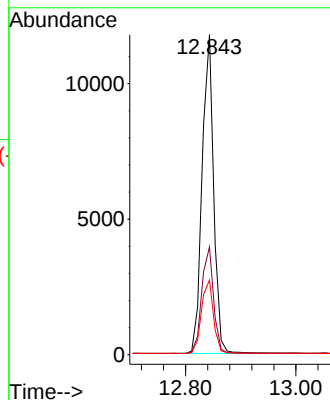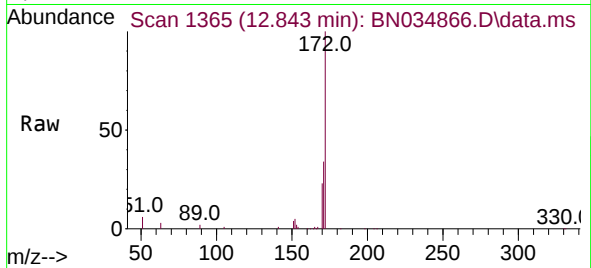

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.970 min Scan# 1732
Delta R.T. 0.000 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49

Tgt Ion:	188	Resp:	21100
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	9.6	9.8	14.6


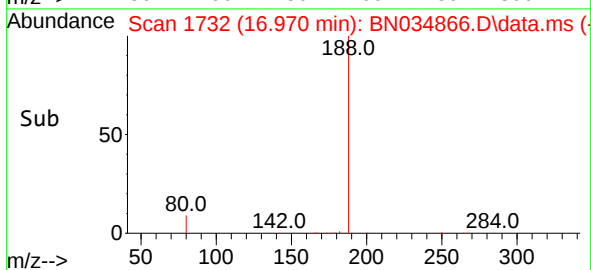
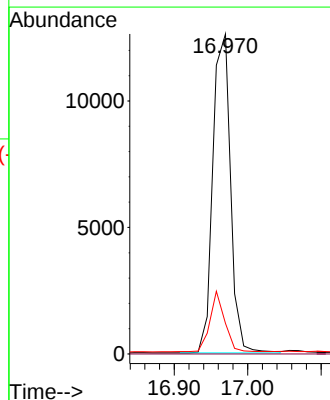
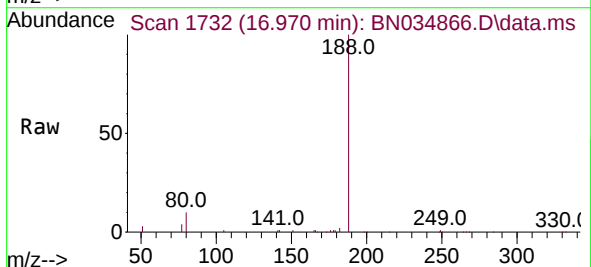


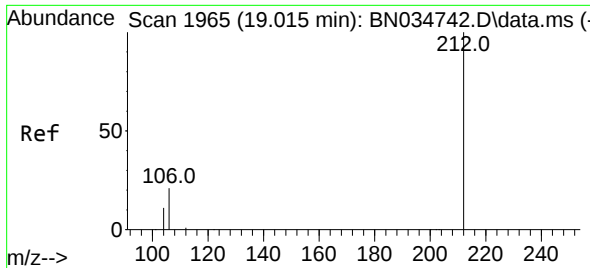

#27
Fluoranthene-d10
Concen: 0.023 ng
RT: 19.001 min Scan# 1962
Delta R.T. 0.000 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49




Instrument :
BNA_N
ClientSampleId :
VPB190-HYD-20241030RE


Tgt Ion	Ratio	Lower	Upper
212	100		
106	21.8	16.1	24.1
104	15.1	9.2	13.8

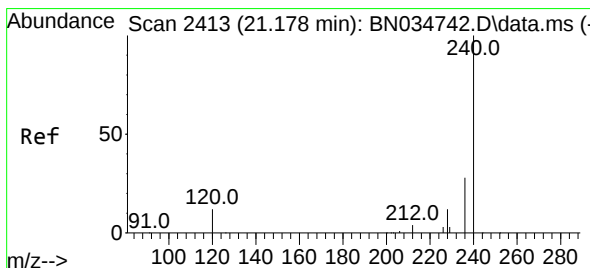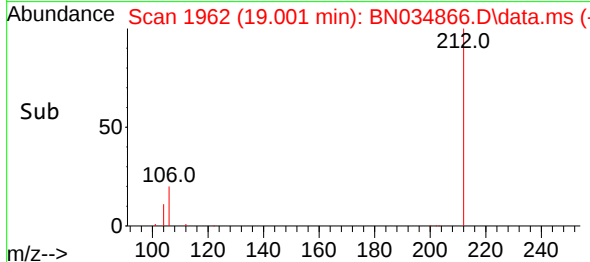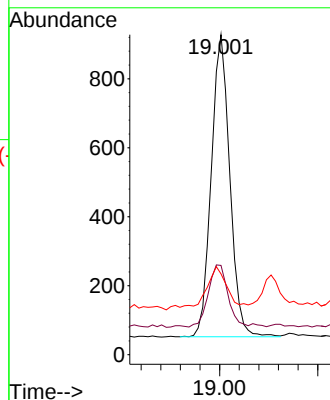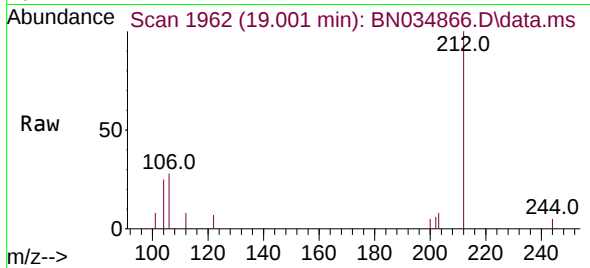

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.160 min Scan# 2411
Delta R.T. 0.000 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49

Tgt Ion	Ratio	Lower	Upper
240	100		
120	20.1	11.5	17.3
236	29.6	23.2	34.8


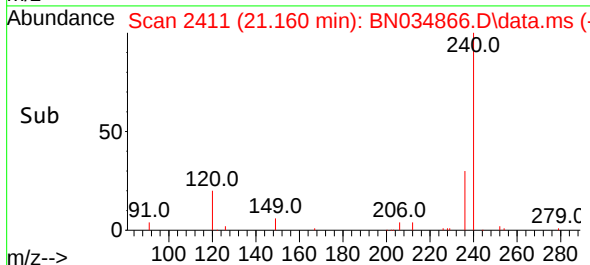
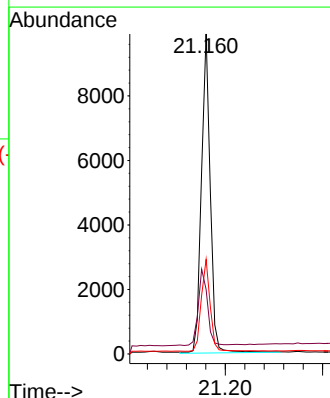
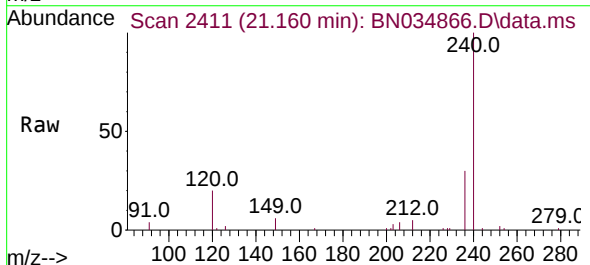


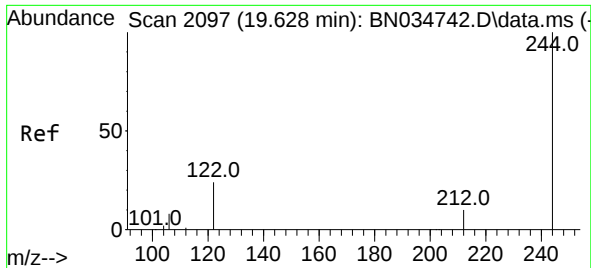

#31
 Terphenyl-d14
 Concen: 0.421 ng
 RT: 19.610 min Scan# 2093
 Delta R.T. -0.005 min
 Lab File: BN034866.D
 Acq: 05 Nov 2024 11:49




Instrument :
 BNA_N
 ClientSampleId :
 VPB190-HYD-20241030RE


Tgt Ion:244 Resp: 11240
 Ion Ratio Lower Upper
 244 100
 212 11.5 8.2 12.4
 122 30.2 19.8 29.6#

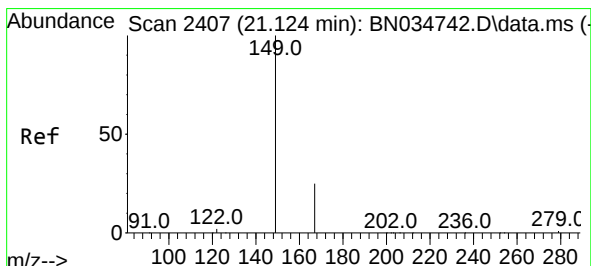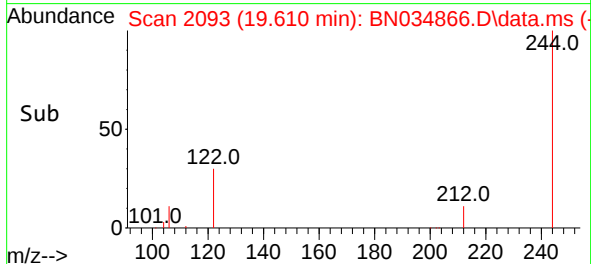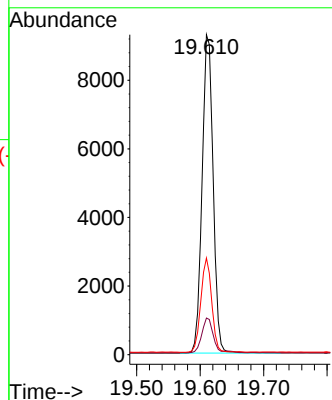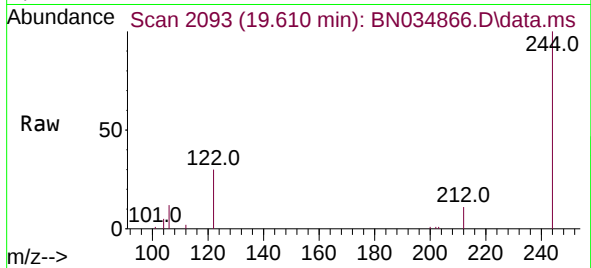

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.048 ng
 RT: 21.107 min Scan# 2405
 Delta R.T. 0.000 min
 Lab File: BN034866.D
 Acq: 05 Nov 2024 11:49

Tgt Ion:149 Resp: 1982
 Ion Ratio Lower Upper
 149 100
 167 22.6 20.6 30.8
 279 2.9 1.5 2.3#

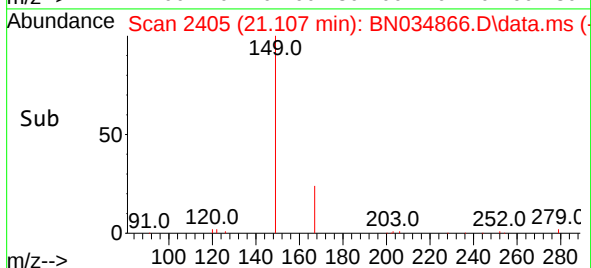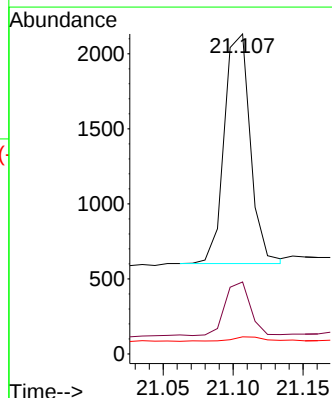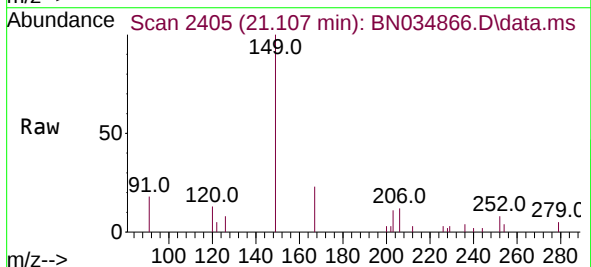

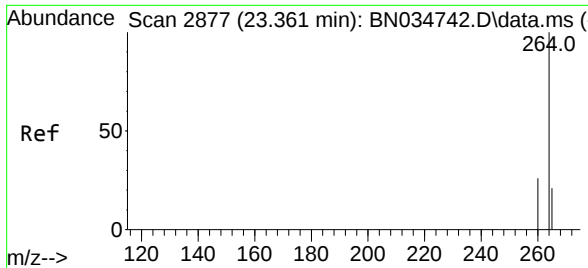

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.335 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN034866.D
Acq: 05 Nov 2024 11:49

Instrument :
BNA_N
ClientSampleId :
VPB190-HYD-20241030RE

Tgt Ion:264	Resp:	8745
Ion	Ratio	Lower Upper
264	100	
260	28.0	21.5 32.3
265	68.0	47.5 71.3

