
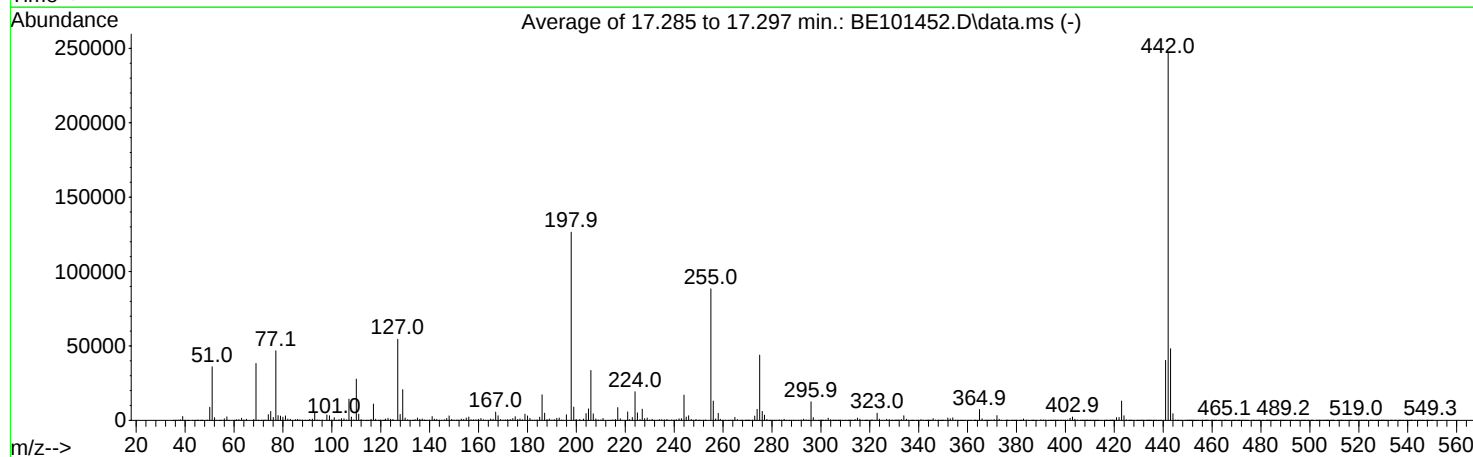


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101452.D
Acq On : 4 Nov 2024 12:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 29 01:26:30 2024

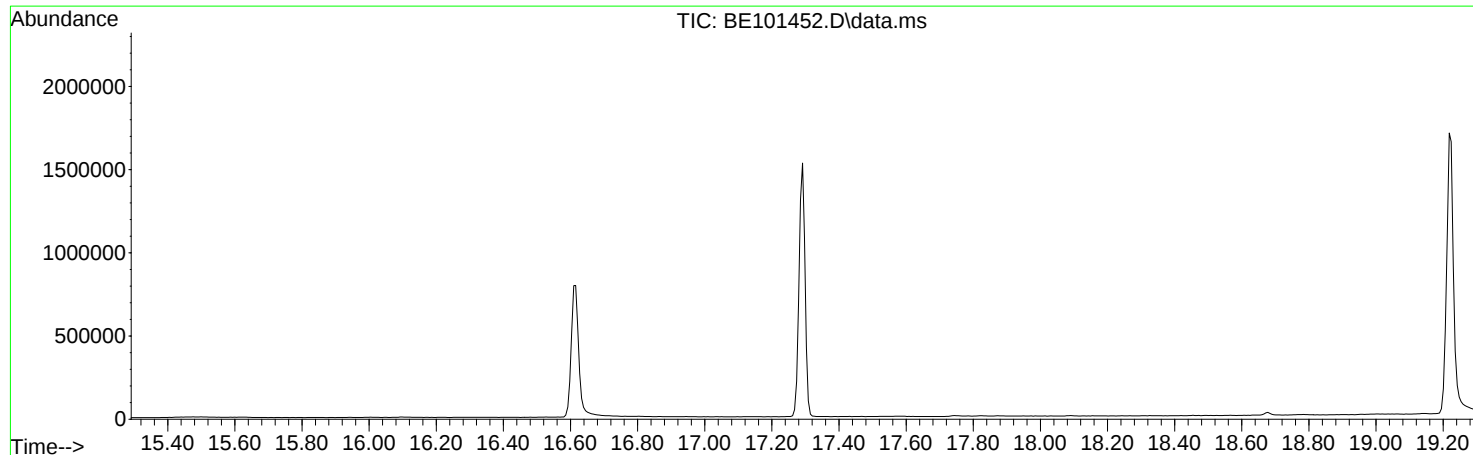




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	36066	PASS
68	69	0.00	2	1.6	597	PASS
69	198	0.00	100	30.3	38281	PASS
70	69	0.00	2	0.5	179	PASS
127	198	10	80	43.1	54497	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	126472	PASS
199	198	5	9	7.1	8926	PASS
275	198	10	60	34.6	43822	PASS
365	198	1	100	5.8	7315	PASS
441	198	0.01	100	31.9	40331	PASS
442	442	50	100	100.0	247168	PASS
443	442	15	24	19.5	48143	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101452.D
Acq On : 4 Nov 2024 12:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 04 19:28:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

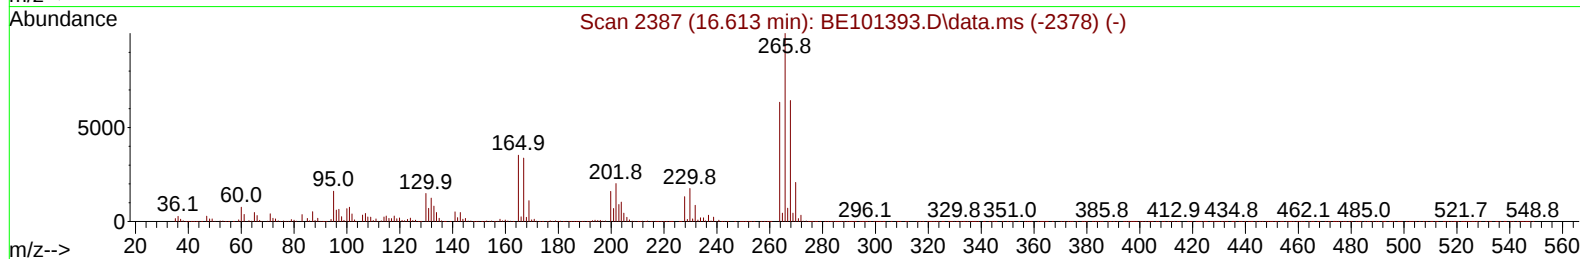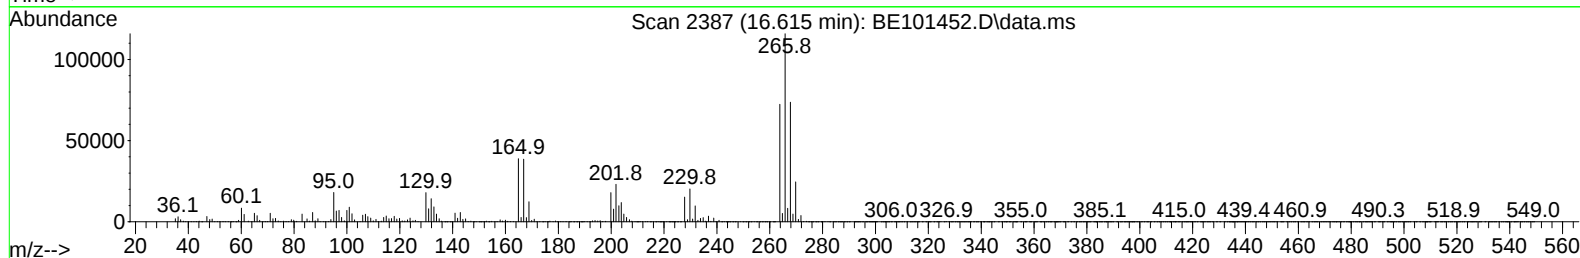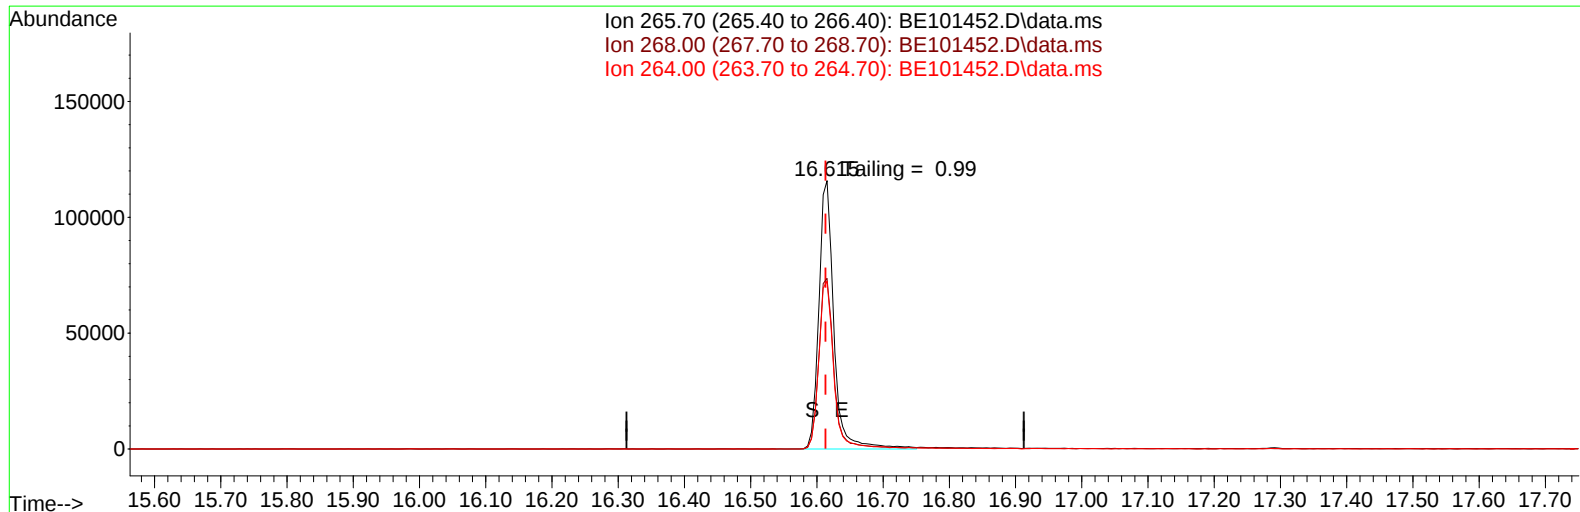

TIC: BE101452.D\data.ms

(70) Pentachlorophenol (C)

16.615min (+ 0.003) 502373.06 ng




response 175435

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	63.57
264.00	63.40	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101452.D
Acq On : 4 Nov 2024 12:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 04 19:28:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

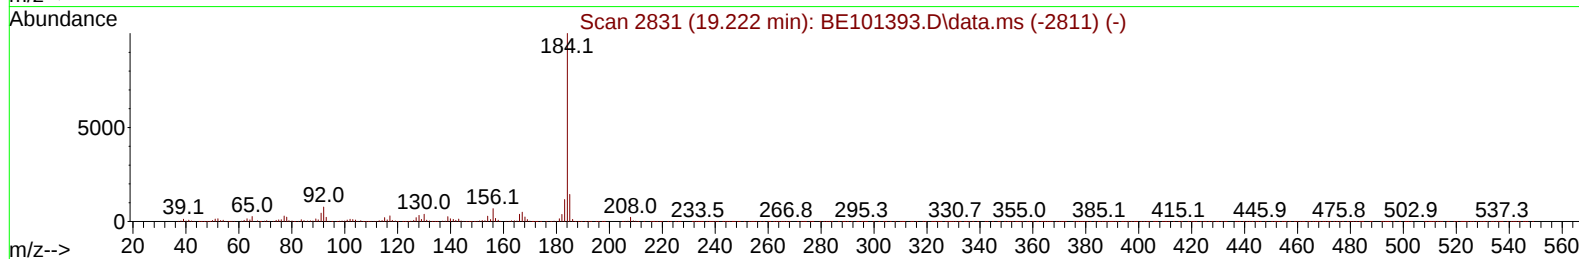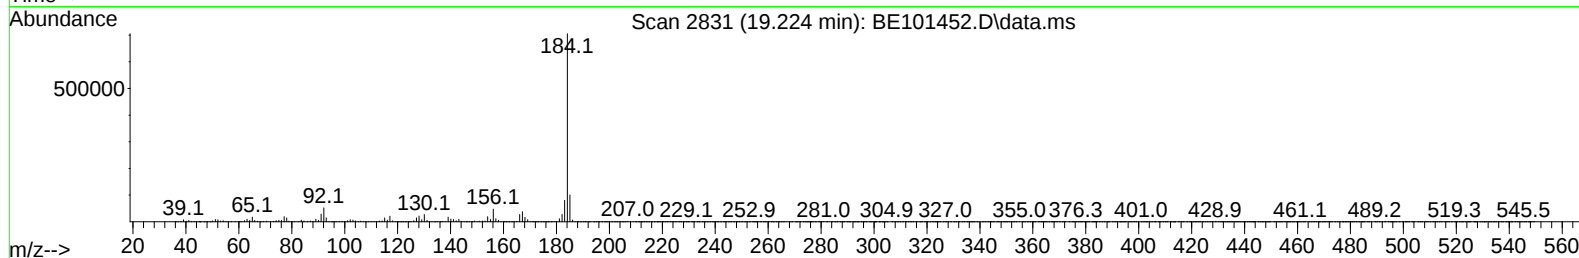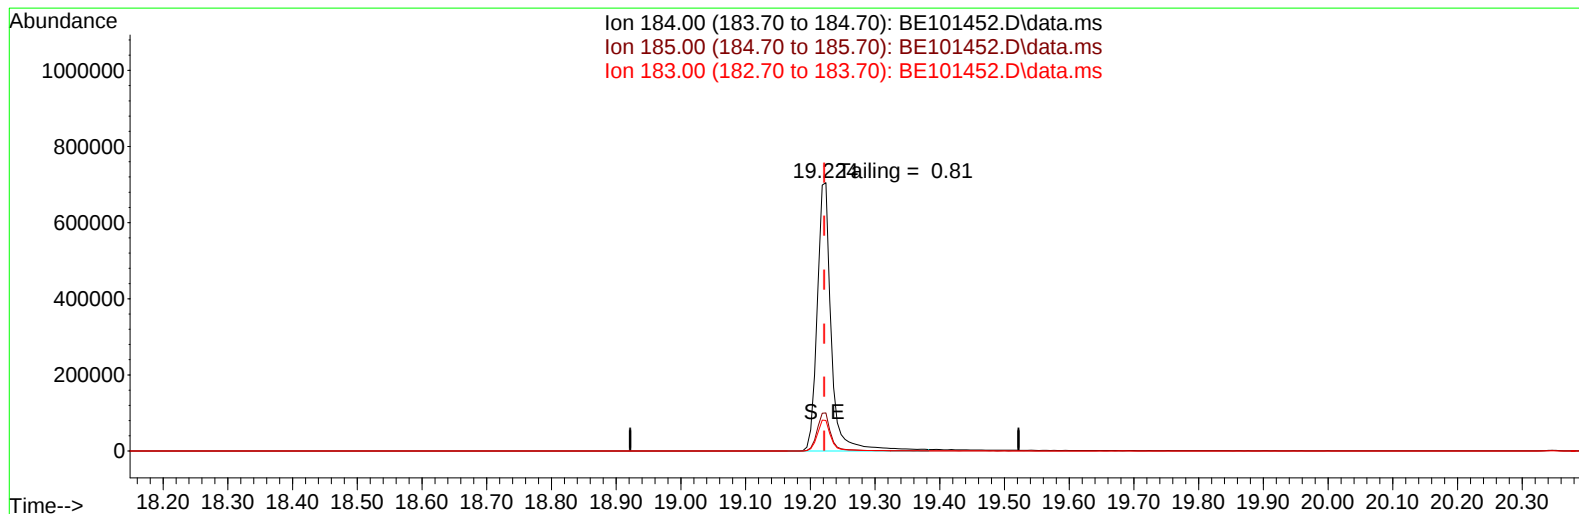

TIC: BE101452.D\data.ms

(77) Benzidine

19.224min (+ 0.003) 969740.64 ng m

response 1070765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.19
183.00	11.60	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2024	BNA_E	<u>BE101452.D</u>
Compound Name	Response	Retention Time
DDT	539338	20.346
DDD	21084	19.917
DDE	981	19.406
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22065	561403	3.93

Instrument :
BNA_E
ClientSampleId :
DFTPP